

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060222\
 Data File : PL075413.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2022 22:21
 Operator : AR\AJ
 Sample : N2951-09
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 06:11:04 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 01 10:19:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	5.643	4.642	9541381	25918026	16.234	16.361
28)	SA Decachlor...	11.641	10.388	6870401	16793098	12.814	12.237
Target Compounds							
5)	MB Aldrin	0.000	6.494	0	320930	N.D.	0.166 #
7)	B delta-BHC	0.000	6.412	0	235645	N.D.	0.110 #
9)	A Endosulfan I	0.000	7.470	0	159392	N.D.	0.094 #
11)	B alpha-Chl...	0.000	7.396f	0	313794	N.D.	0.172 #
13)	MA Dieldrin	0.000	7.751	0	401983	N.D.	0.232 #
14)	MA Endrin	0.000	8.071f	0	109879	N.D.	0.071 #
15)	B Endosulfa...	9.306	0.000	267494	0	0.474	N.D. #
19)	B Endosulfa...	9.670	0.000	108402	0	0.195	N.D. #
21)	B Endrin ke...	10.188f	0.000	83593	0	0.136	N.D. #
22)	Mirex	0.000	9.489	0	48525	N.D.	0.038 #
26)	Chlordane-4	0.000	7.396f	0	313794	N.D.	1.661 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060222\
Data File : PL075413.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2022 22:21
Operator : AR\AJ
Sample : N2951-09
Misc :
ALS Vial : 44 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 06:11:04 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
Quant Title : GC Extractables
QLast Update : Wed Jun 01 10:19:11 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

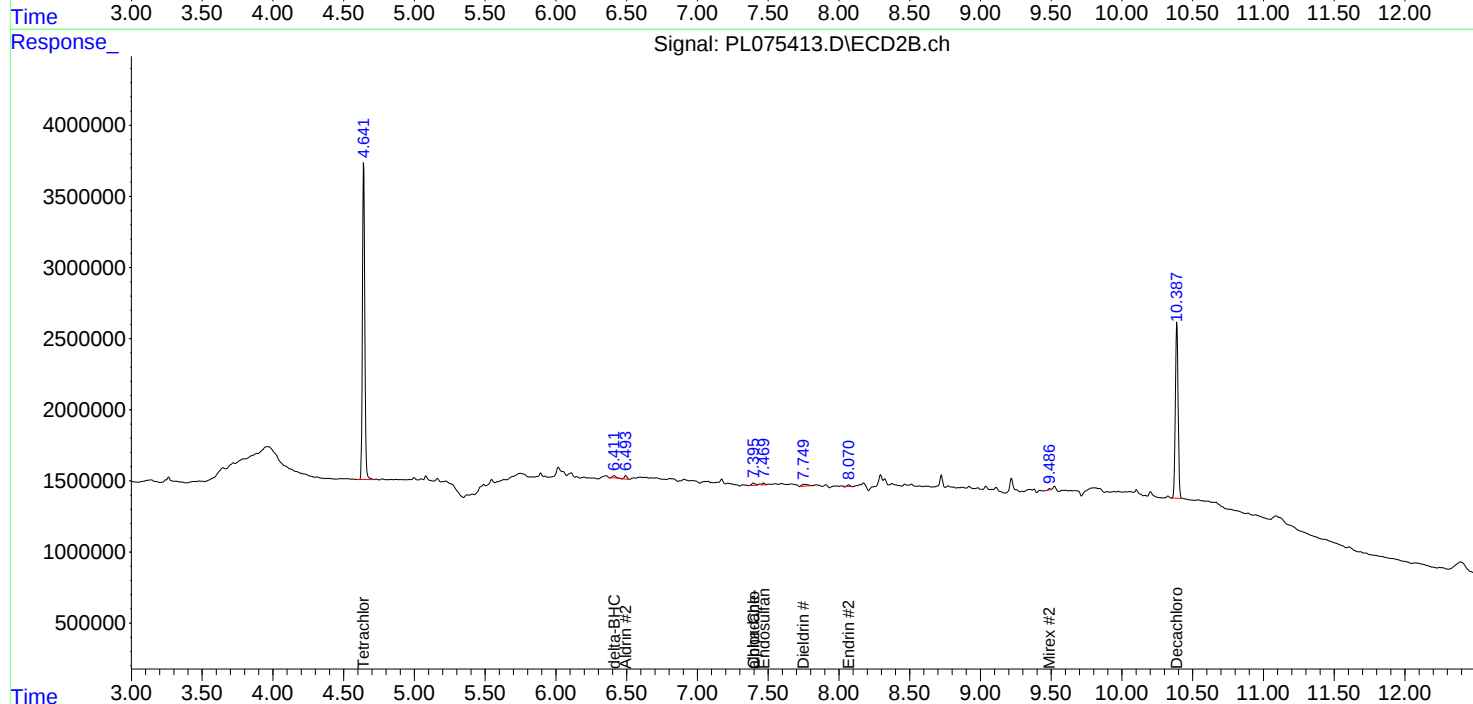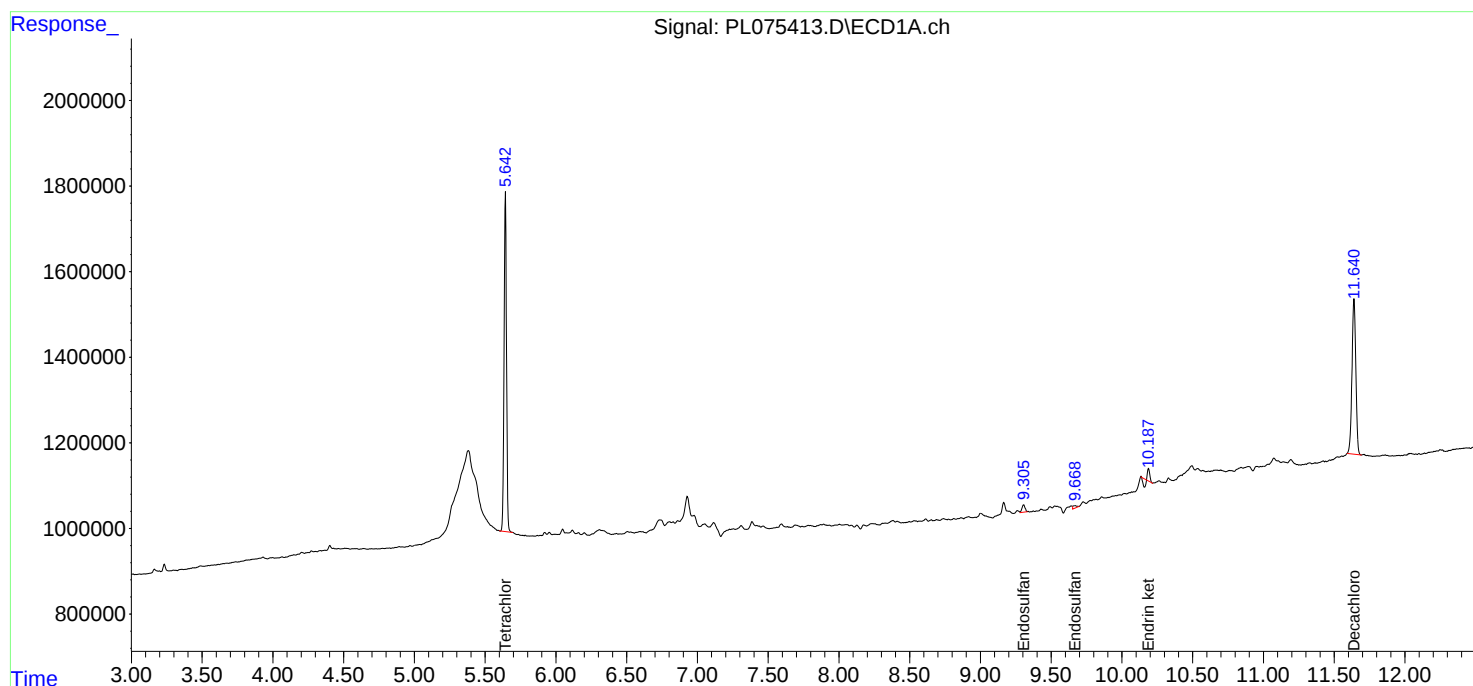

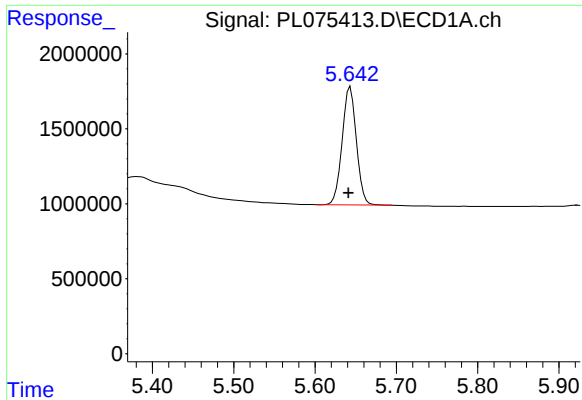


#1 Tetrachloro-m-xylene

R.T.: 5.643 min
Delta R.T.: 0.002 min
Response: 9541381
Conc: 16.23 ng/ml

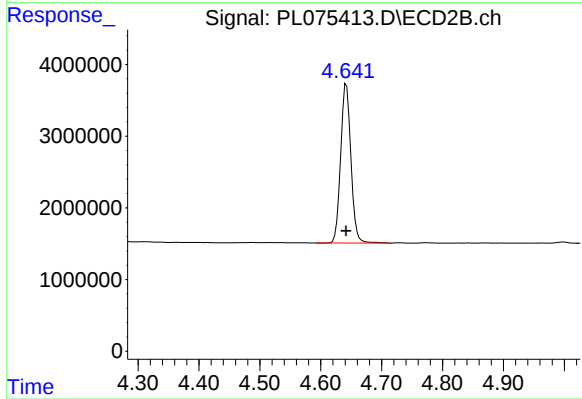


#1 Tetrachloro-m-xylene

R.T.: 4.642 min
Delta R.T.: 0.000 min
Response: 25918026
Conc: 16.36 ng/ml

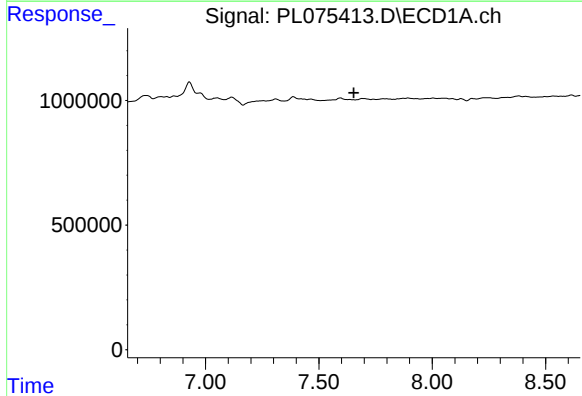


#5 Aldrin

R.T.: 0.000 min
Exp R.T.: 7.654 min
Response: 0
Conc: N.D.

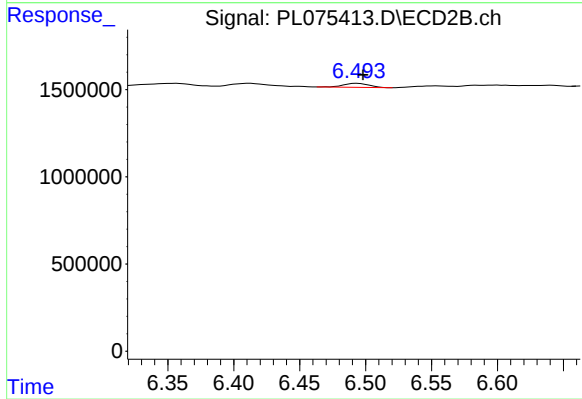


#5 Aldrin

R.T.: 6.494 min
Delta R.T.: -0.004 min
Response: 320930
Conc: 0.17 ng/ml

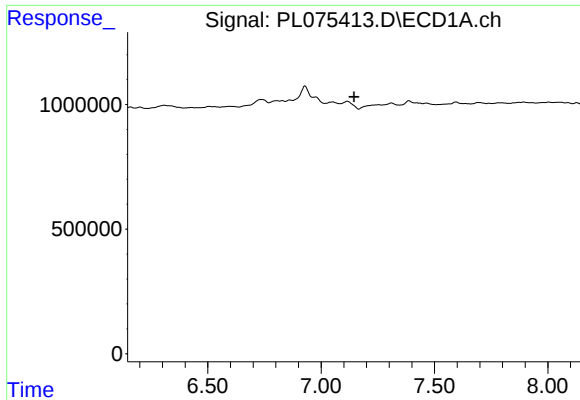


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.146 min
Response: 0
Conc: N.D.

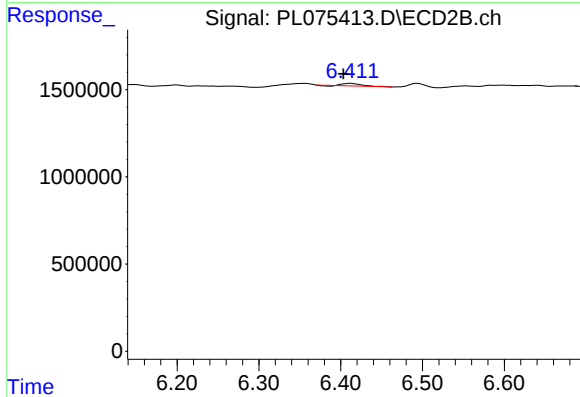


#7 delta-BHC

R.T.: 6.412 min
Delta R.T.: 0.009 min
Response: 235645
Conc: 0.11 ng/ml

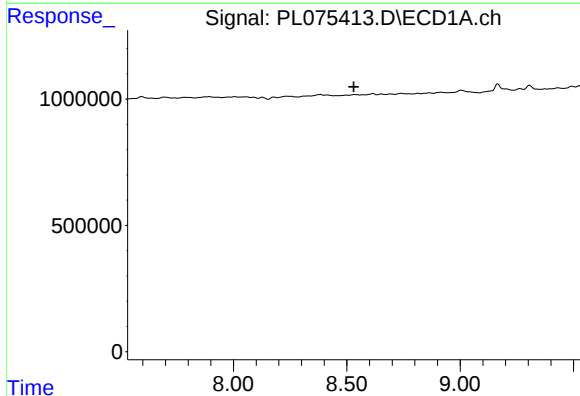


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 8.530 min
Response: 0
Conc: N.D.

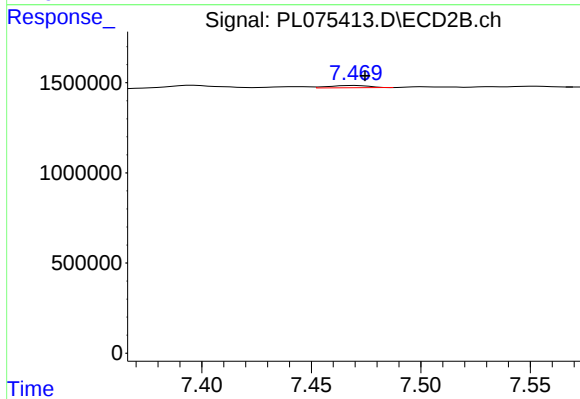


#9 Endosulfan I

R.T.: 7.470 min
Delta R.T.: -0.004 min
Response: 159392
Conc: 0.09 ng/ml

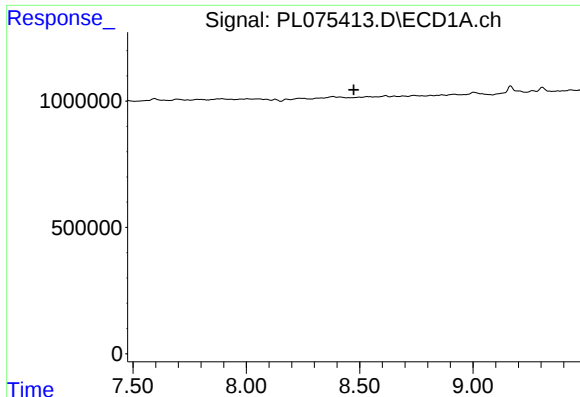


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.474 min
Response: 0
Conc: N.D.

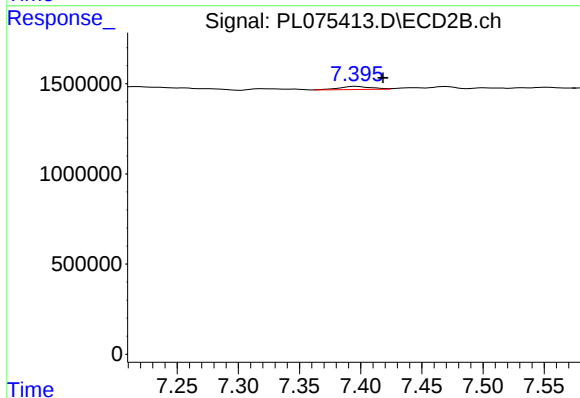


#11 alpha-Chlordane

R.T.: 7.396 min
Delta R.T.: -0.022 min
Response: 313794
Conc: 0.17 ng/ml

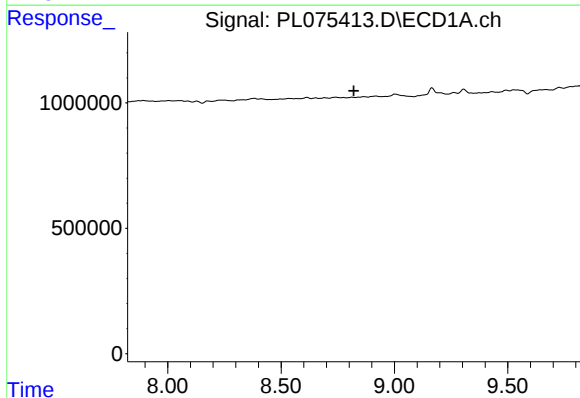


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 8.821 min
Response: 0
Conc: N.D.

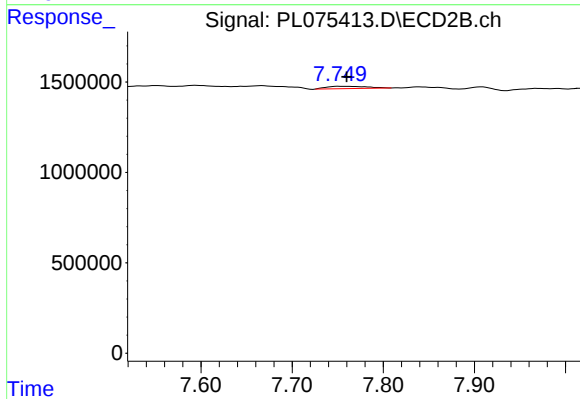


#13 Dieldrin

R.T.: 7.751 min
Delta R.T.: -0.009 min
Response: 401983
Conc: 0.23 ng/ml

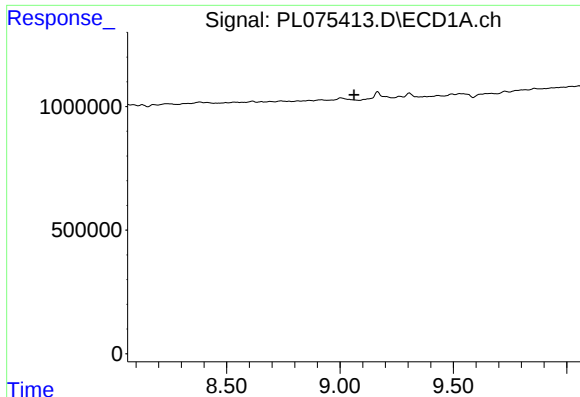


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 9.062 min
Response: 0
Conc: N.D.

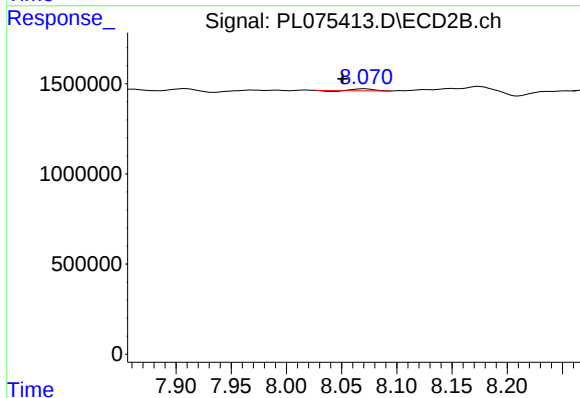


#14 Endrin

R.T.: 8.071 min
Delta R.T.: 0.020 min
Response: 109879
Conc: 0.07 ng/ml

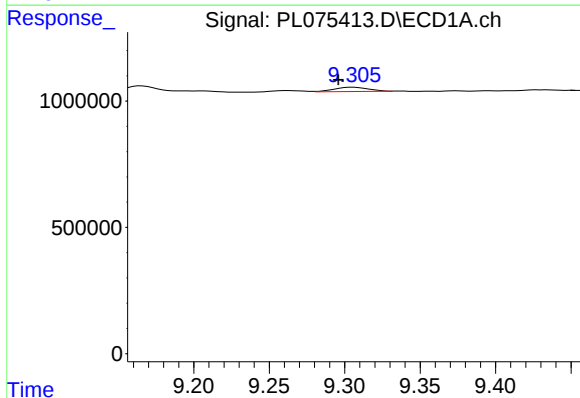


#15 Endosulfan II

R.T.: 9.306 min
Delta R.T.: 0.010 min
Response: 267494
Conc: 0.47 ng/ml

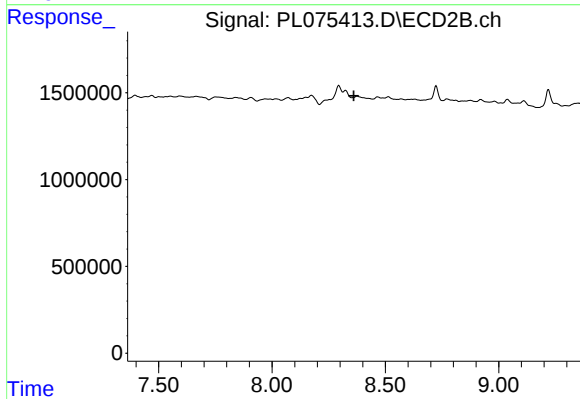


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.361 min
Response: 0
Conc: N.D.

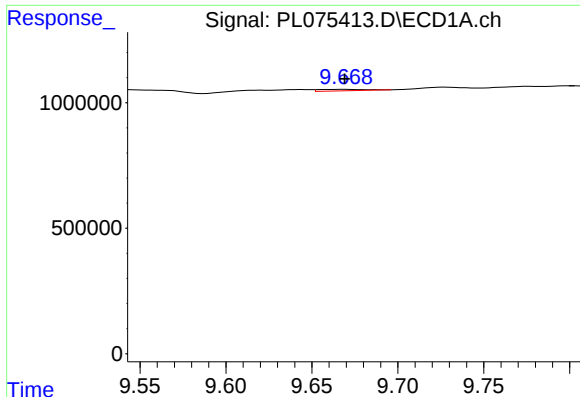


#19 Endosulfan Sulfate

R.T.: 9.670 min
Delta R.T.: 0.000 min
Response: 108402
Conc: 0.19 ng/ml

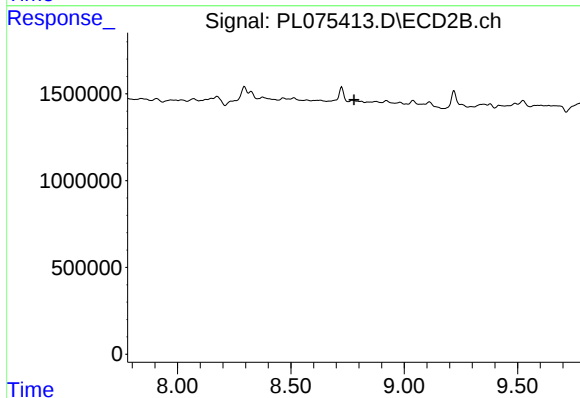


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 8.779 min
Response: 0
Conc: N.D.

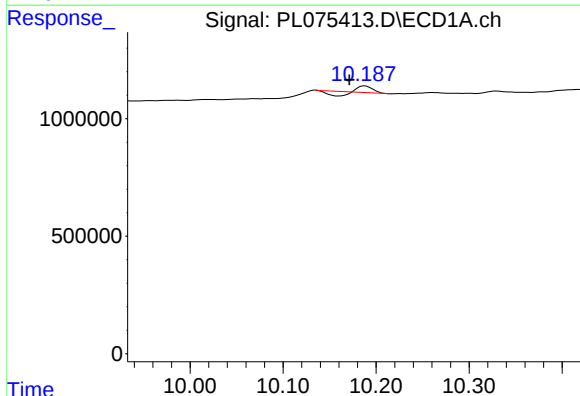


#21 Endrin ketone

R.T.: 10.188 min
Delta R.T.: 0.017 min
Response: 83593
Conc: 0.14 ng/ml

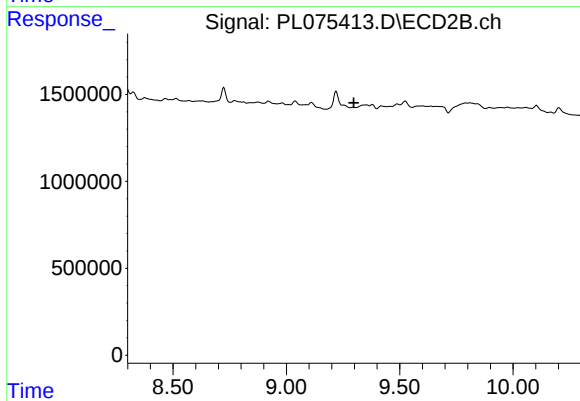


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 9.298 min
Response: 0
Conc: N.D.

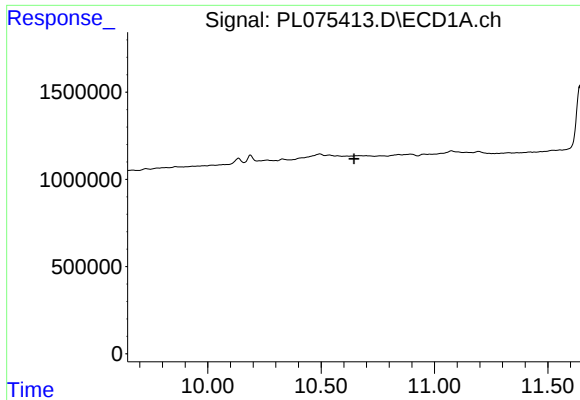


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 10.645 min
Response: 0
Conc: N.D.

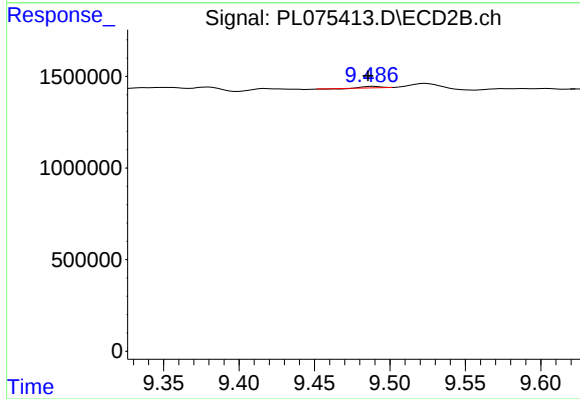


#22 Mirex

R.T.: 9.489 min
Delta R.T.: 0.003 min
Response: 48525
Conc: 0.04 ng/ml

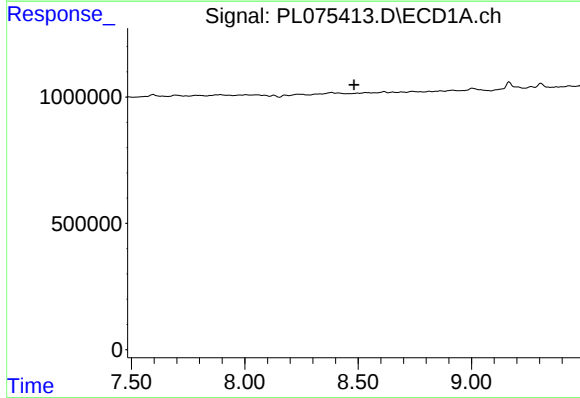


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 8.482 min
Response: 0
Conc: N.D.

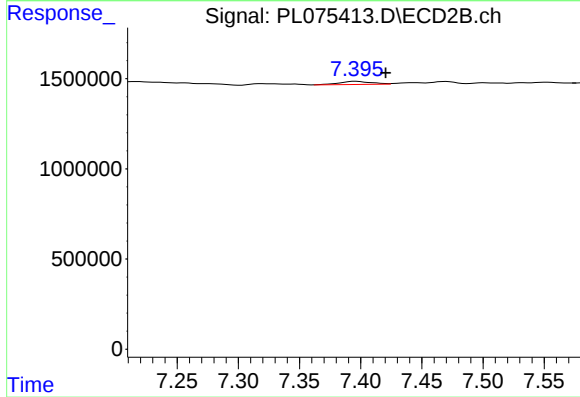


#26 Chlordane-4

R.T.: 7.396 min
Delta R.T.: -0.024 min
Response: 313794
Conc: 1.66 ng/ml

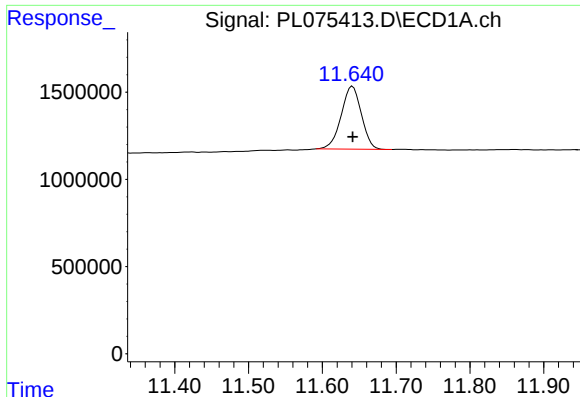

#28 Decachlorobiphenyl

R.T.: 11.641 min
Delta R.T.: 0.000 min
Response: 6870401
Conc: 12.81 ng/ml

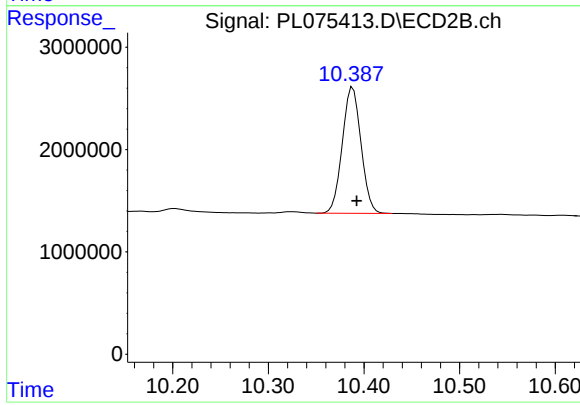

#28 Decachlorobiphenyl

R.T.: 10.388 min
Delta R.T.: -0.004 min
Response: 16793098
Conc: 12.24 ng/ml