

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060222\
 Data File : PL075417.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2022 00:51
 Operator : AR\AJ
 Sample : N2951-10
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 06:12:12 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 01 10:19:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	5.644	4.643	11348012	30341144	19.308	19.153
28)	SA Decachlor...	11.641	10.389	7037545	17249498	13.125	12.570
Target Compounds							
7)	B delta-BHC	0.000	6.410	0	365582	N.D.	0.170 #
11)	B alpha-Chl...	0.000	7.396f	0	253982	N.D.	0.139 #
13)	MA Dieldrin	0.000	7.764	0	329405	N.D.	0.190 #
14)	MA Endrin	0.000	8.071f	0	432753	N.D.	0.278 #
15)	B Endosulfa...	9.307	0.000	277791	0	0.492	N.D. #
16)	A 4,4'-DDD	9.201	8.214	333520	169335	0.674	0.127 #
17)	MA 4,4'-DDT	0.000	8.471	0	324057	N.D.	0.227 #
21)	B Endrin ke...	10.188f	0.000	441615	0	0.719	N.D. #
26)	Chlordane-4	0.000	7.396f	0	253982	N.D.	1.345 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060222\
Data File : PL075417.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2022 00:51
Operator : AR\AJ
Sample : N2951-10
Misc :
ALS Vial : 45 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 06:12:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
Quant Title : GC Extractables
QLast Update : Wed Jun 01 10:19:11 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

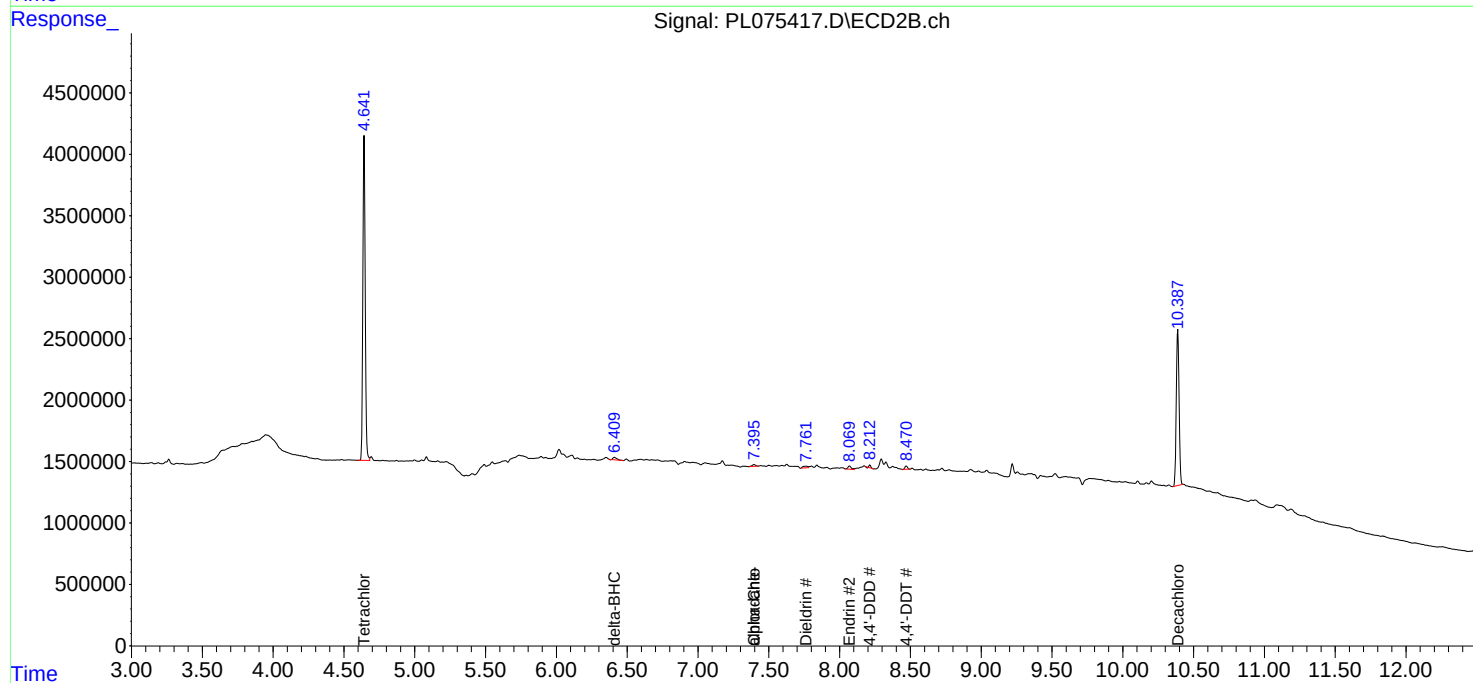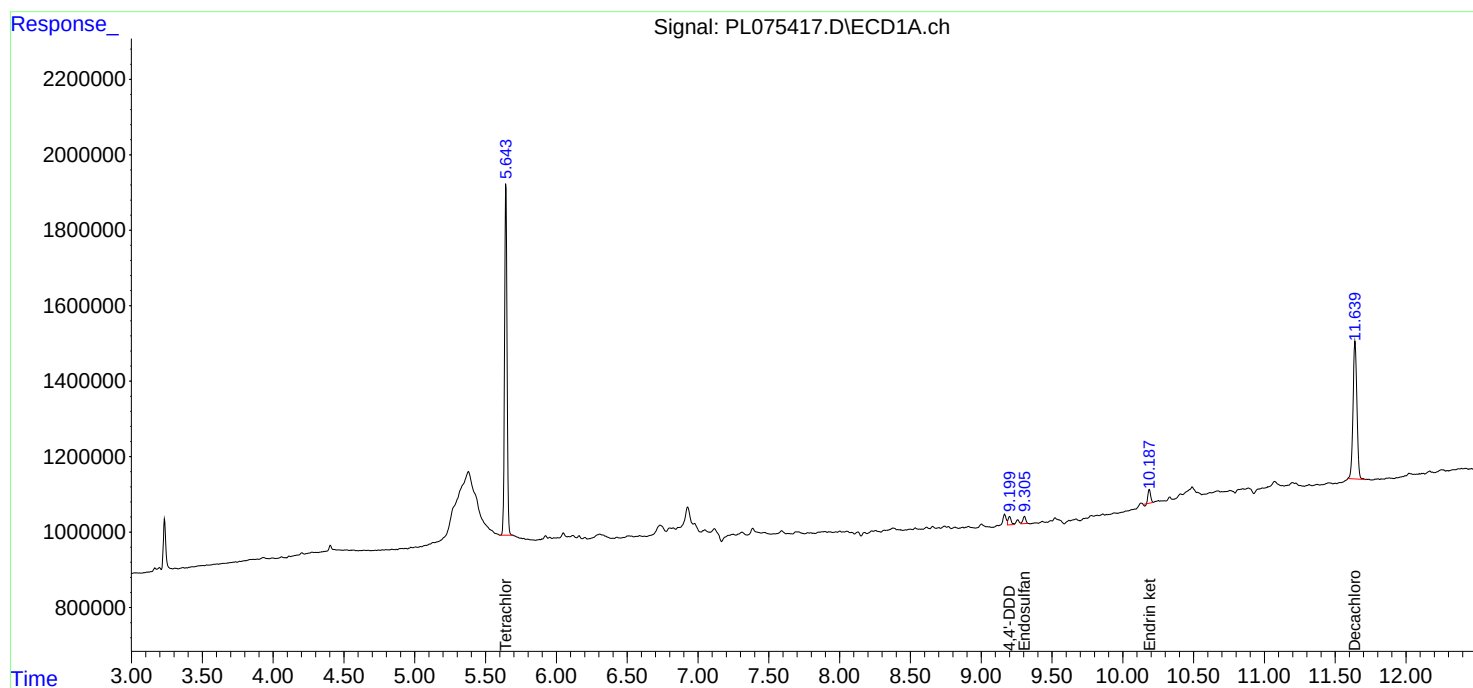

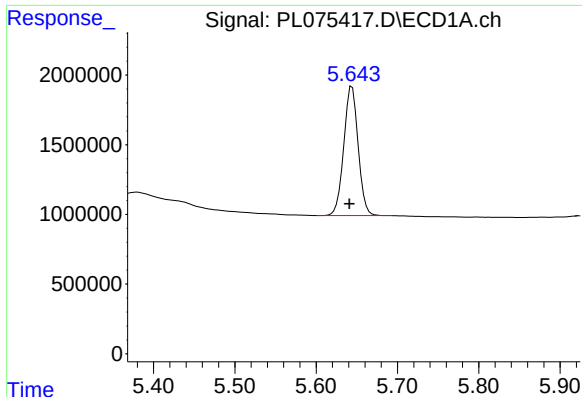


#1 Tetrachloro-m-xylene

R.T.: 5.644 min
Delta R.T.: 0.003 min
Response: 11348012
Conc: 19.31 ng/ml

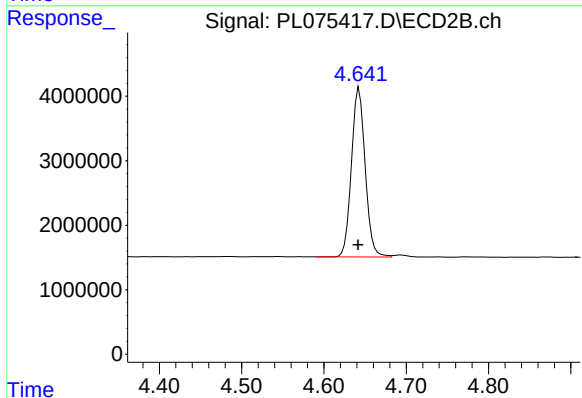


#1 Tetrachloro-m-xylene

R.T.: 4.643 min
Delta R.T.: 0.001 min
Response: 30341144
Conc: 19.15 ng/ml

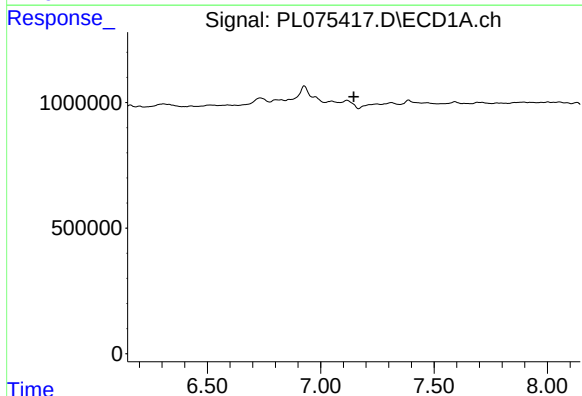


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.146 min
Response: 0
Conc: N.D.

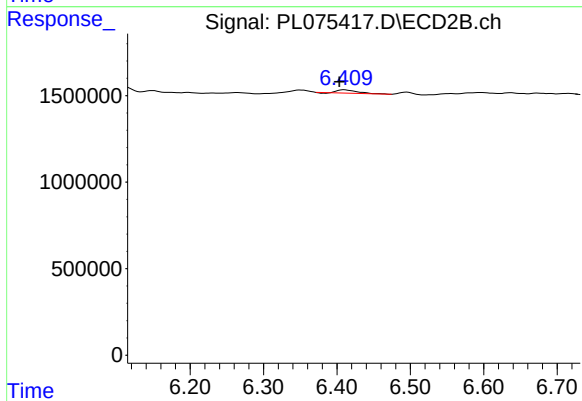


#7 delta-BHC

R.T.: 6.410 min
Delta R.T.: 0.007 min
Response: 365582
Conc: 0.17 ng/ml

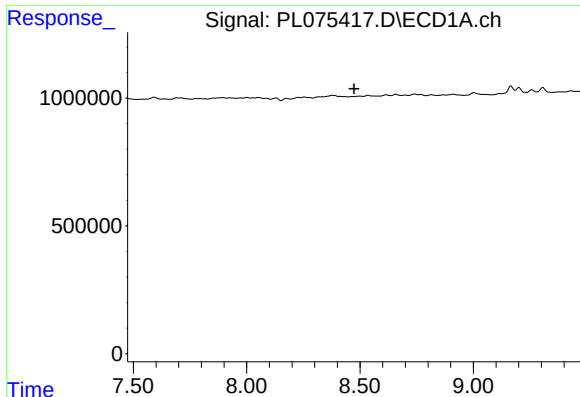


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.474 min
Response: 0
Conc: N.D.

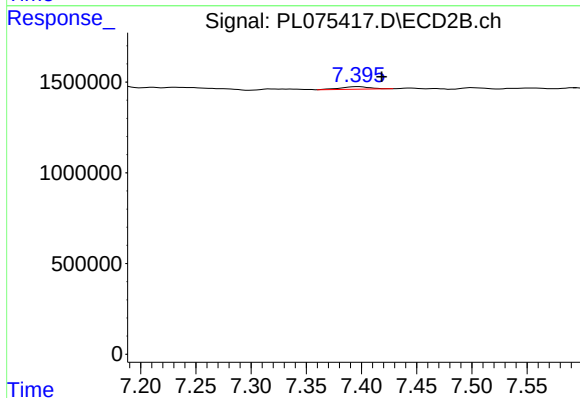


#11 alpha-Chlordane

R.T.: 7.396 min
Delta R.T.: -0.022 min
Response: 253982
Conc: 0.14 ng/ml

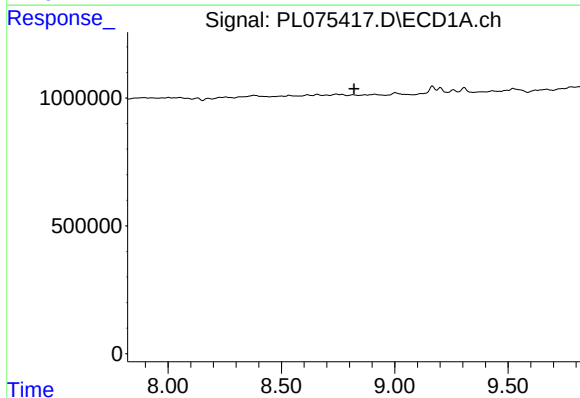


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 8.821 min
Response: 0
Conc: N.D.

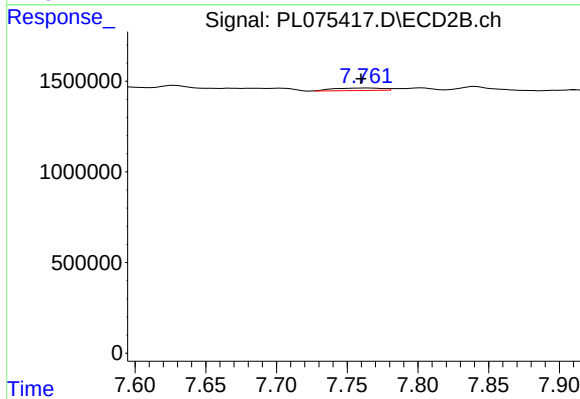


#13 Dieldrin

R.T.: 7.764 min
Delta R.T.: 0.004 min
Response: 329405
Conc: 0.19 ng/ml

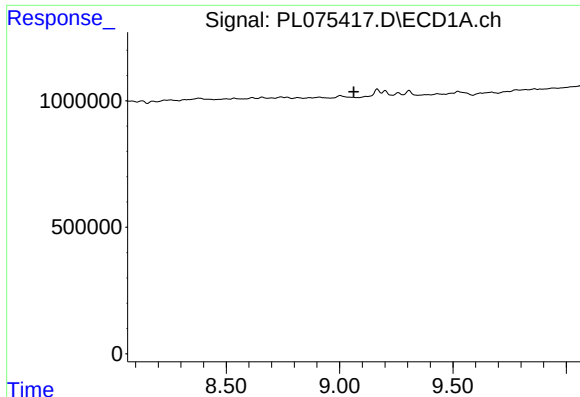


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 9.062 min
Response: 0
Conc: N.D.

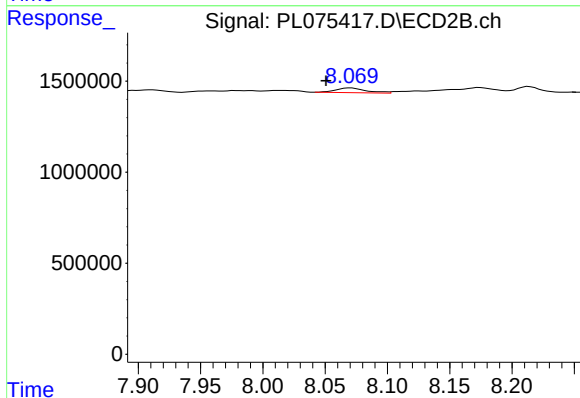


#14 Endrin

R.T.: 8.071 min
Delta R.T.: 0.020 min
Response: 432753
Conc: 0.28 ng/ml

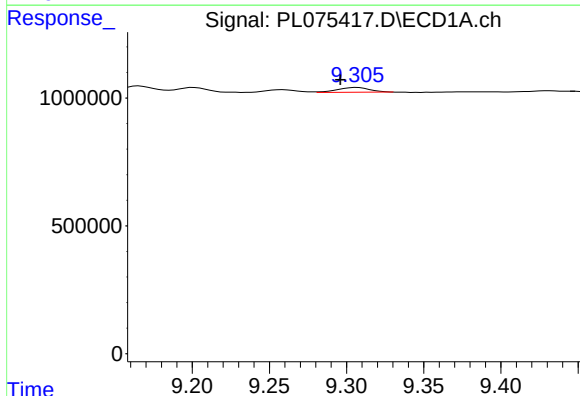


#15 Endosulfan II

R.T.: 9.307 min
Delta R.T.: 0.011 min
Response: 277791
Conc: 0.49 ng/ml

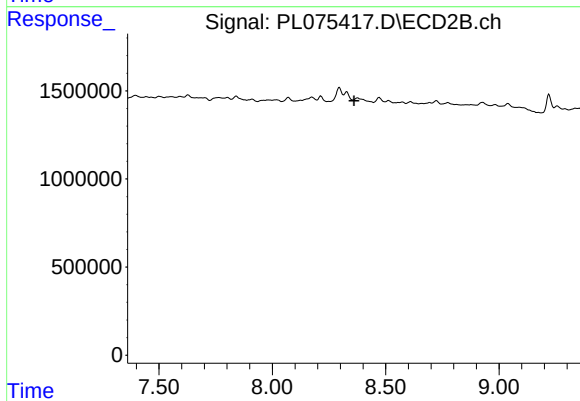


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.361 min
Response: 0
Conc: N.D.

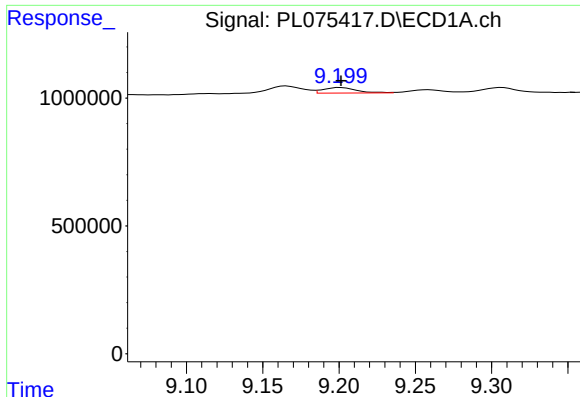


#16 4,4'-DDD

R.T.: 9.201 min
Delta R.T.: 0.000 min
Response: 333520
Conc: 0.67 ng/ml

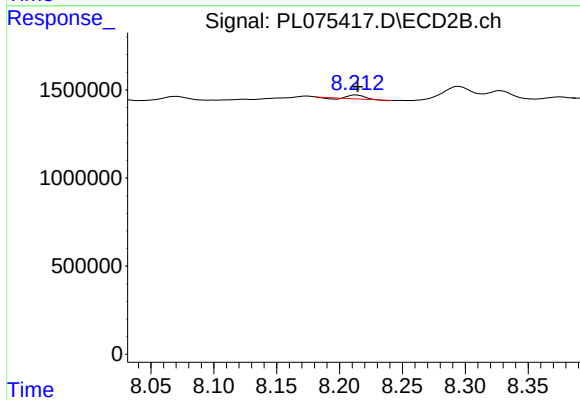


#16 4,4'-DDD

R.T.: 8.214 min
Delta R.T.: 0.000 min
Response: 169335
Conc: 0.13 ng/ml

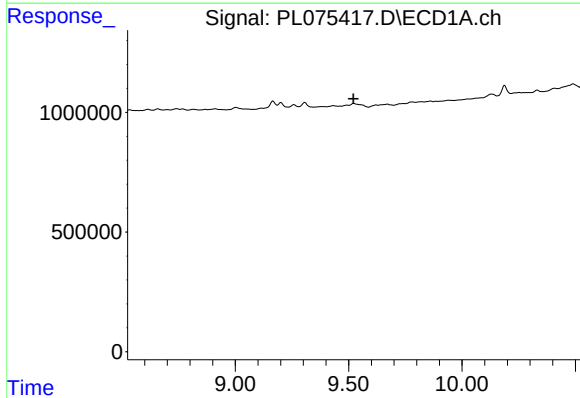


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 9.522 min
Response: 0
Conc: N.D.

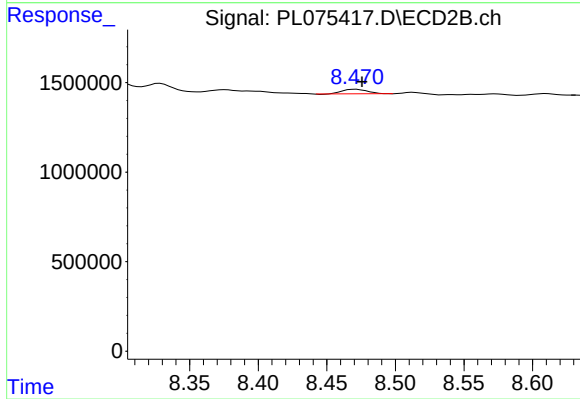


#17 4,4'-DDT

R.T.: 8.471 min
Delta R.T.: -0.004 min
Response: 324057
Conc: 0.23 ng/ml

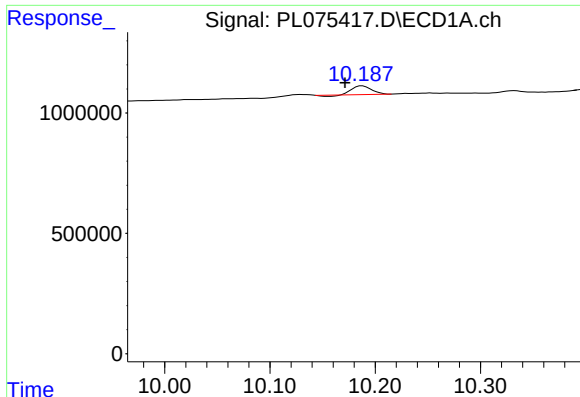


#21 Endrin ketone

R.T.: 10.188 min
Delta R.T.: 0.017 min
Response: 441615
Conc: 0.72 ng/ml

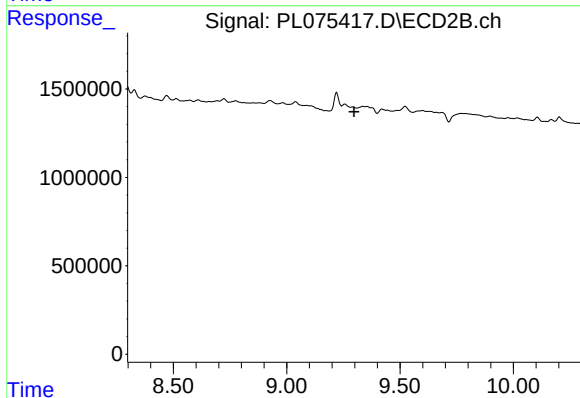


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.298 min
Response: 0
Conc: N.D.

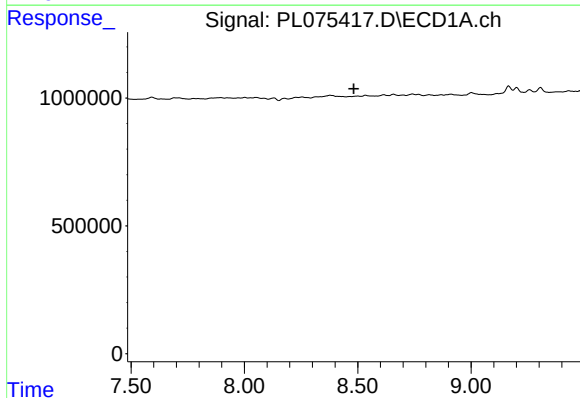


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 8.482 min
Response: 0
Conc: N.D.

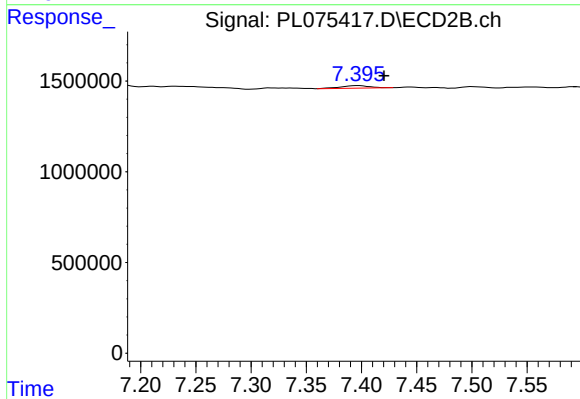


#26 Chlordane-4

R.T.: 7.396 min
Delta R.T.: -0.024 min
Response: 253982
Conc: 1.34 ng/ml

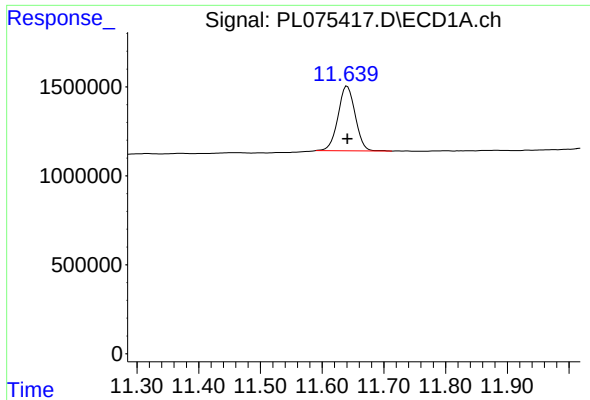

#28 Decachlorobiphenyl

R.T.: 11.641 min
Delta R.T.: 0.000 min
Response: 7037545
Conc: 13.13 ng/ml

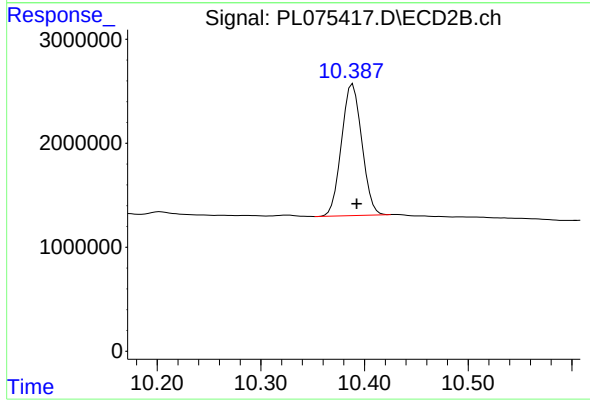

#28 Decachlorobiphenyl

R.T.: 10.389 min
Delta R.T.: -0.004 min
Response: 17249498
Conc: 12.57 ng/ml