

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060222\
 Data File : PL075419.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2022 01:24
 Operator : AR\AJ
 Sample : N2951-12
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 06:12:38 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 01 10:19:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	5.644	4.642	11739562	31480750	19.974	19.872
28)	SA Decachlor...	11.639	10.388	9430073	23287289	17.587	16.970
Target Compounds							
7)	B delta-BHC	0.000	6.414	0	513219	N.D.	0.239 #
9)	A Endosulfan I	8.539	7.461	153391	242583	0.244	0.144 #
11)	B alpha-Chl...	0.000	7.396f	0	328828	N.D.	0.180 #
12)	B 4,4'-DDE	0.000	7.627	0	208440	N.D.	0.128 #
13)	MA Dieldrin	0.000	7.764	0	232629	N.D.	0.134 #
14)	MA Endrin	0.000	8.066f	0	549748	N.D.	0.353 #
15)	B Endosulfa...	9.308	0.000	218653	0	0.387	N.D. #
16)	A 4,4'-DDD	9.203	8.232f	854563	-134311	1.728	N.D. #
17)	MA 4,4'-DDT	0.000	8.465	0	2128726	N.D.	1.488 #
18)	B Endrin al...	0.000	8.568f	0	368438	N.D.	0.306 #
19)	B Endosulfa...	0.000	8.776	0	1309035	N.D.	0.875 #
21)	B Endrin ke...	10.187f	0.000	110255	0	0.180	N.D. #
26)	Chlordane-4	0.000	7.396f	0	328828	N.D.	1.741 #
27)	Chlordane-5	0.000	8.128	0	2033271	N.D.	40.746 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060222\
Data File : PL075419.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2022 01:24
Operator : AR\AJ
Sample : N2951-12
Misc :
ALS Vial : 47 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 06:12:38 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
Quant Title : GC Extractables
QLast Update : Wed Jun 01 10:19:11 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

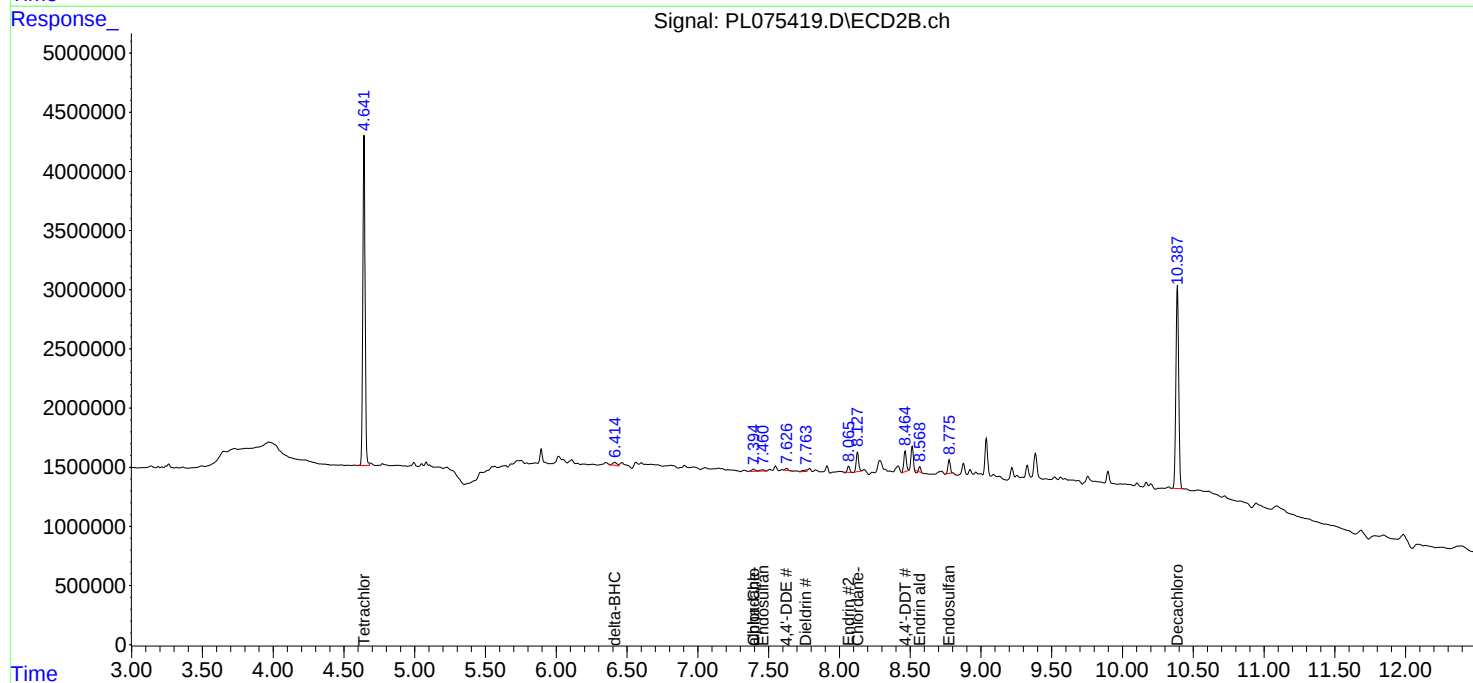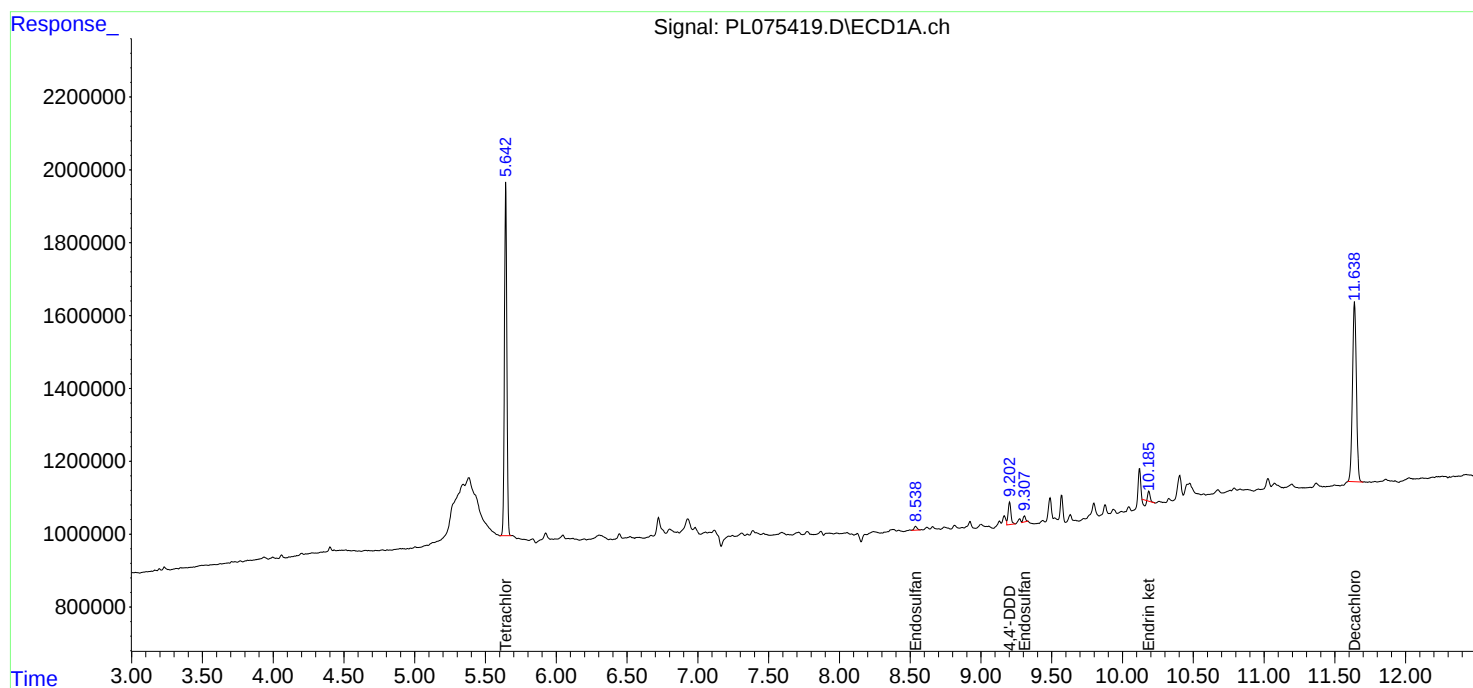

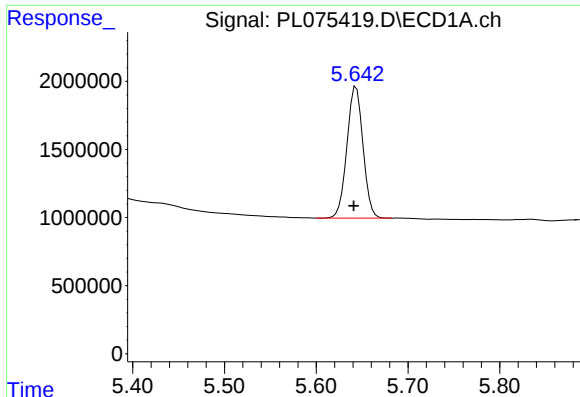


#1 Tetrachloro-m-xylene

R.T.: 5.644 min
Delta R.T.: 0.003 min
Response: 11739562
Conc: 19.97 ng/ml

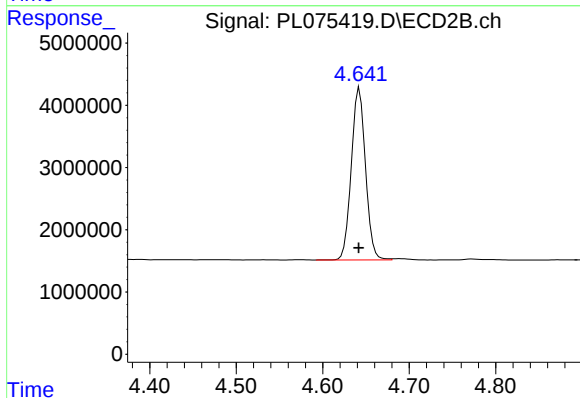


#1 Tetrachloro-m-xylene

R.T.: 4.642 min
Delta R.T.: 0.000 min
Response: 31480750
Conc: 19.87 ng/ml

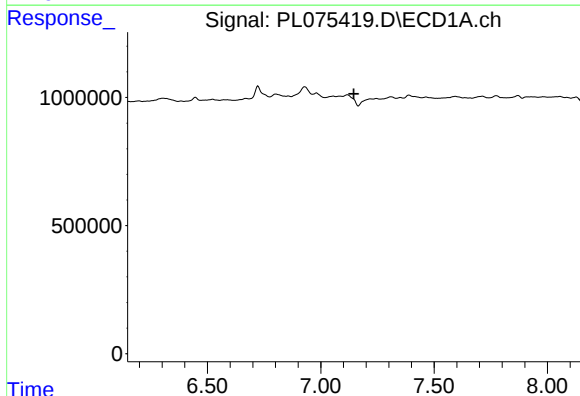


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.146 min
Response: 0
Conc: N.D.

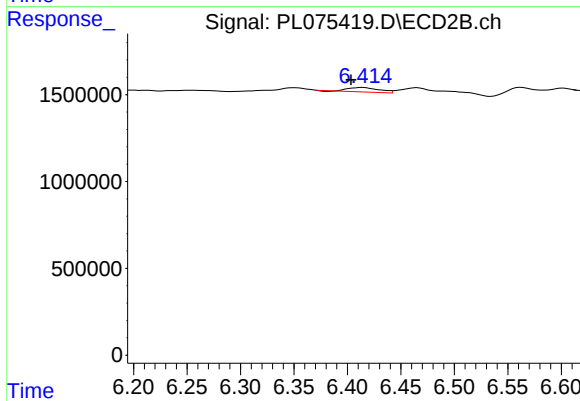


#7 delta-BHC

R.T.: 6.414 min
Delta R.T.: 0.011 min
Response: 513219
Conc: 0.24 ng/ml

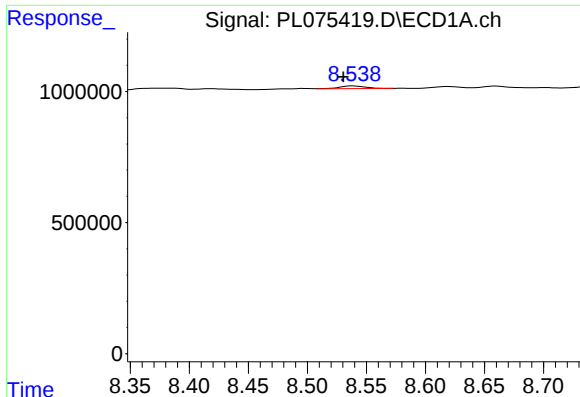


#9 Endosulfan I

R.T.: 8.539 min
Delta R.T.: 0.009 min
Response: 153391
Conc: 0.24 ng/ml

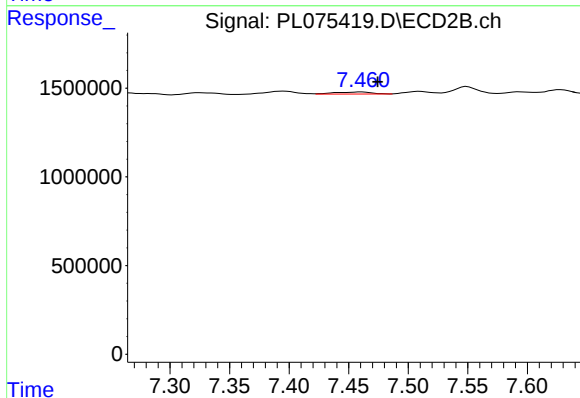


#9 Endosulfan I

R.T.: 7.461 min
Delta R.T.: -0.013 min
Response: 242583
Conc: 0.14 ng/ml

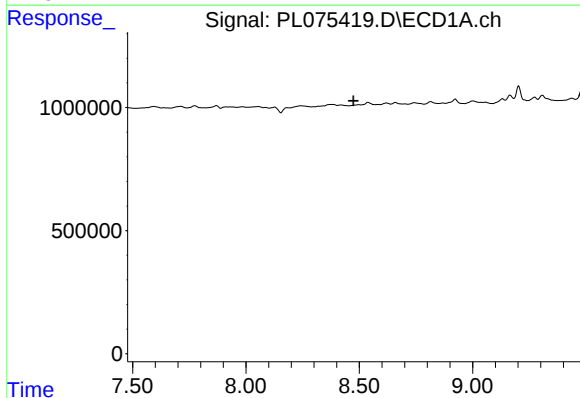


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 8.474 min
Response: 0
Conc: N.D.

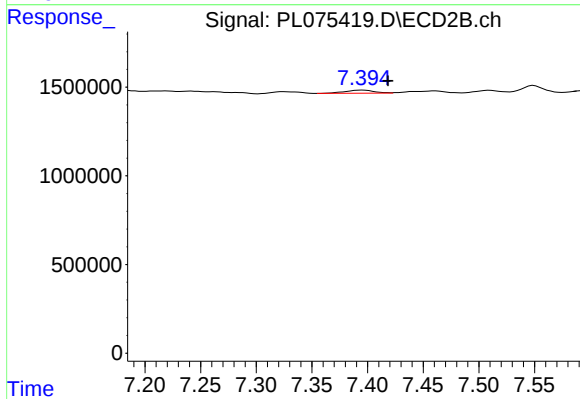


#11 alpha-Chlordane

R.T.: 7.396 min
Delta R.T.: -0.022 min
Response: 328828
Conc: 0.18 ng/ml

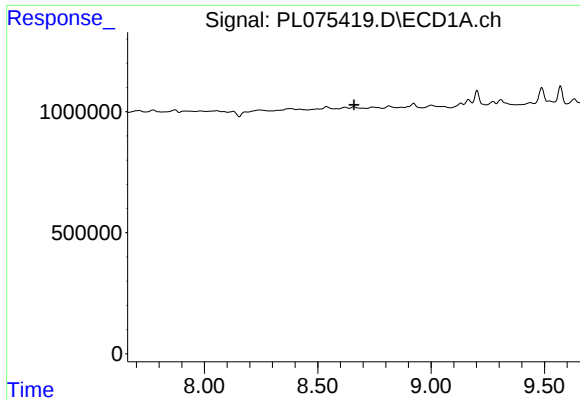


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 8.660 min
Response: 0
Conc: N.D.

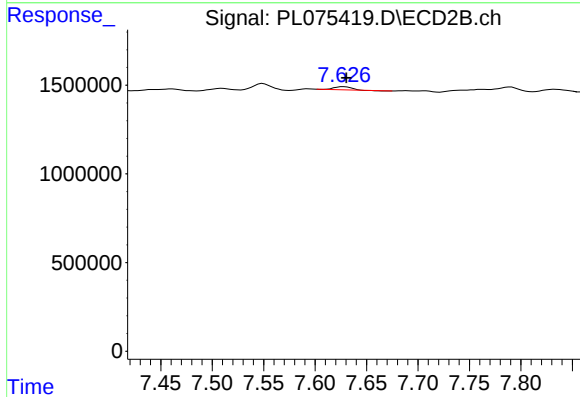


#12 4,4'-DDE

R.T.: 7.627 min
Delta R.T.: -0.003 min
Response: 208440
Conc: 0.13 ng/ml

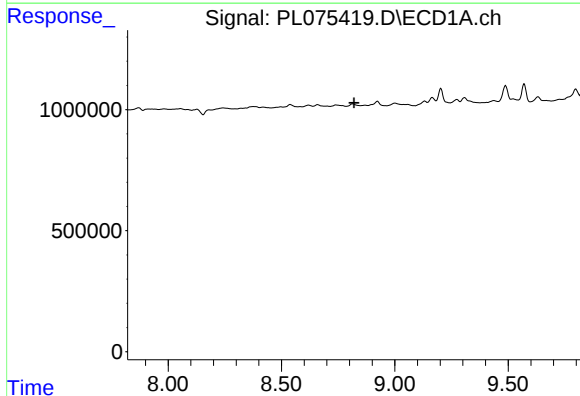


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 8.821 min
Response: 0
Conc: N.D.

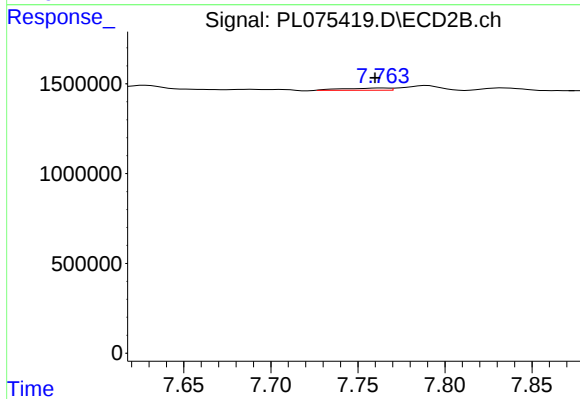


#13 Dieldrin

R.T.: 7.764 min
Delta R.T.: 0.004 min
Response: 232629
Conc: 0.13 ng/ml

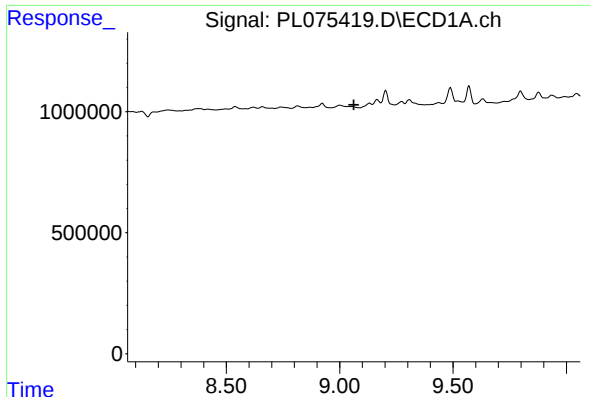


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 9.062 min
Response: 0
Conc: N.D.

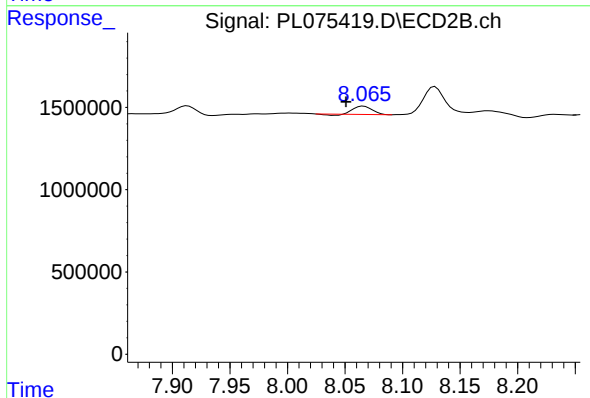


#14 Endrin

R.T.: 8.066 min
Delta R.T.: 0.015 min
Response: 549748
Conc: 0.35 ng/ml

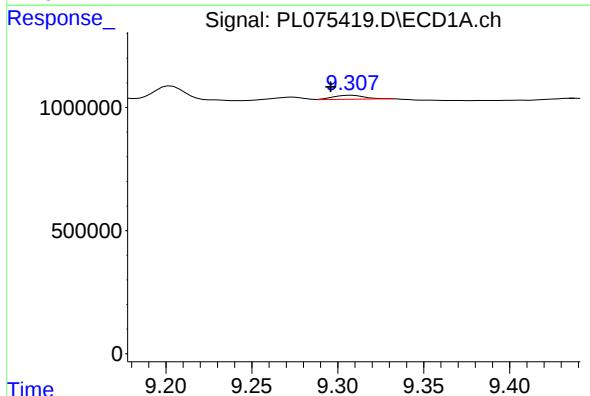


#15 Endosulfan II

R.T.: 9.308 min
Delta R.T.: 0.012 min
Response: 218653
Conc: 0.39 ng/ml

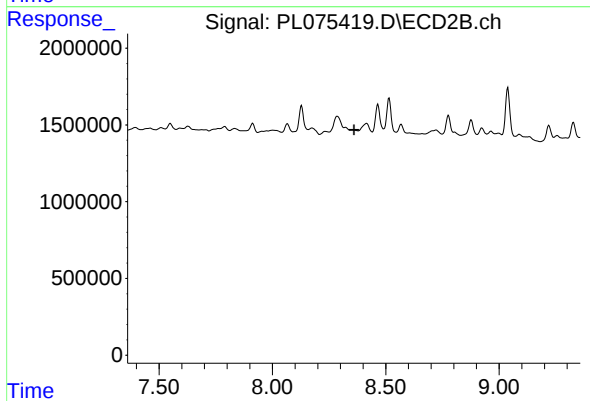


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.361 min
Response: 0
Conc: N.D.

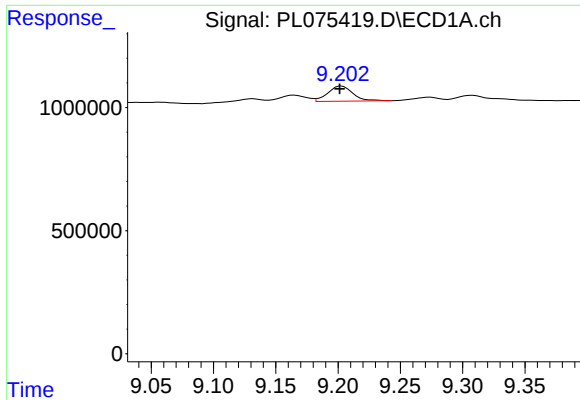


#16 4,4'-DDD

R.T.: 9.203 min
Delta R.T.: 0.002 min
Response: 854563
Conc: 1.73 ng/ml

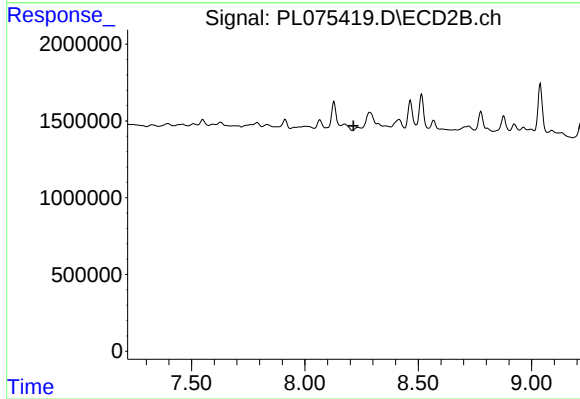


#16 4,4'-DDD

R.T.: 8.232 min
Delta R.T.: 0.017 min
Response: -134311
Conc: N.D.

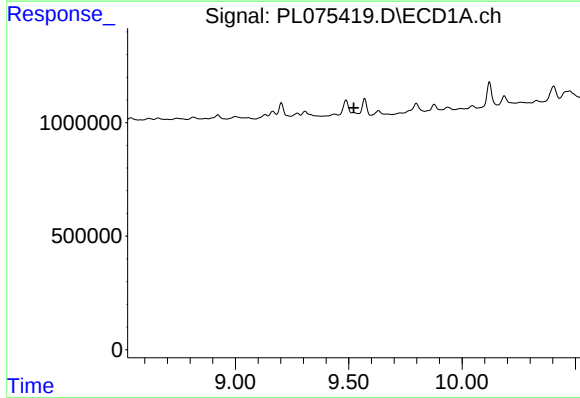


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 9.522 min
Response: 0
Conc: N.D.

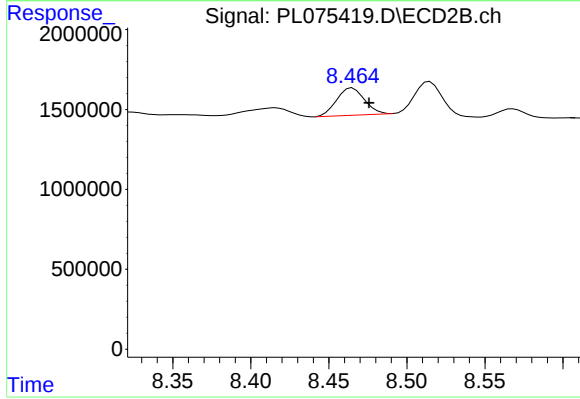


#17 4,4'-DDT

R.T.: 8.465 min
Delta R.T.: -0.011 min
Response: 2128726
Conc: 1.49 ng/ml

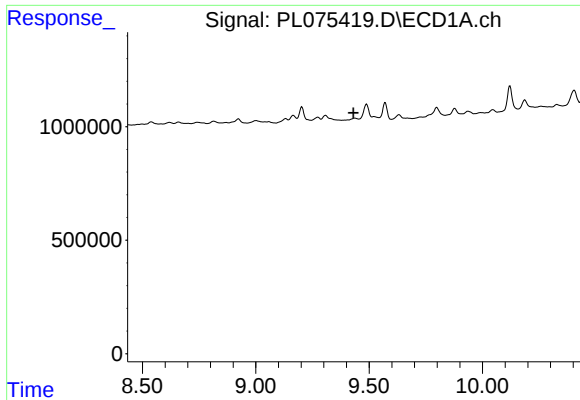


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 9.431 min
Response: 0
Conc: N.D.

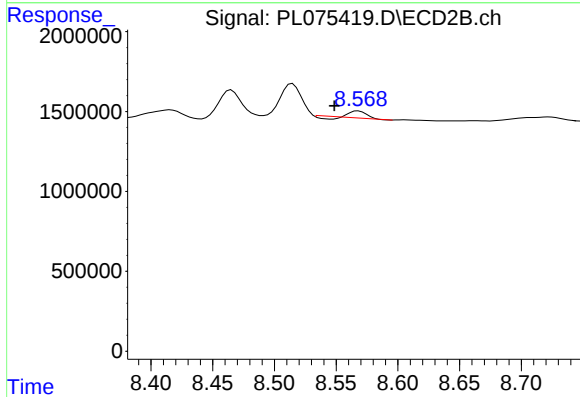


#18 Endrin aldehyde

R.T.: 8.568 min
Delta R.T.: 0.019 min
Response: 368438
Conc: 0.31 ng/ml

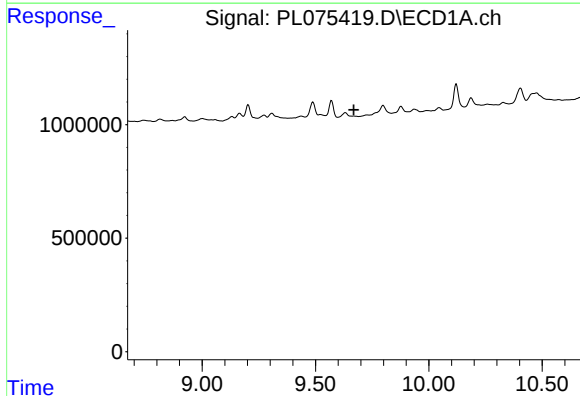


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 9.669 min
Response: 0
Conc: N.D.

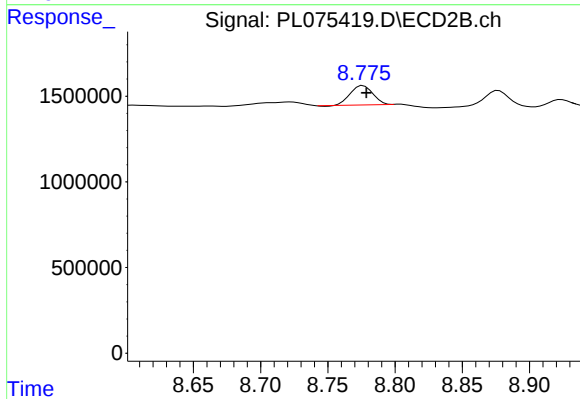


#19 Endosulfan Sulfate

R.T.: 8.776 min
Delta R.T.: -0.002 min
Response: 1309035
Conc: 0.87 ng/ml

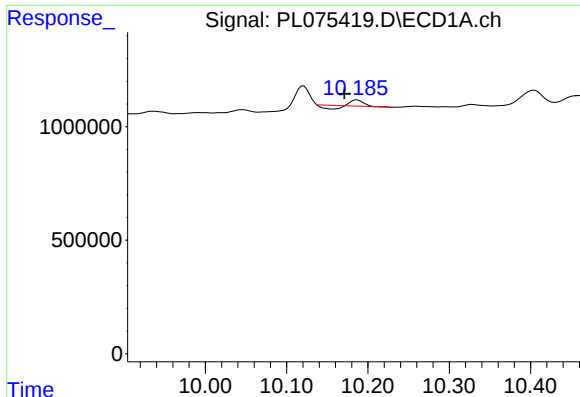


#21 Endrin ketone

R.T.: 10.187 min
Delta R.T.: 0.015 min
Response: 110255
Conc: 0.18 ng/ml

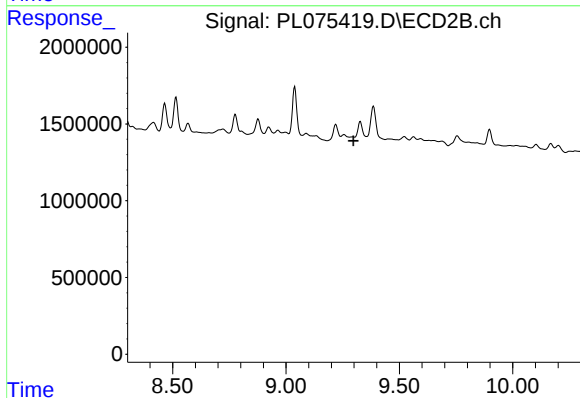


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.298 min
Response: 0
Conc: N.D.

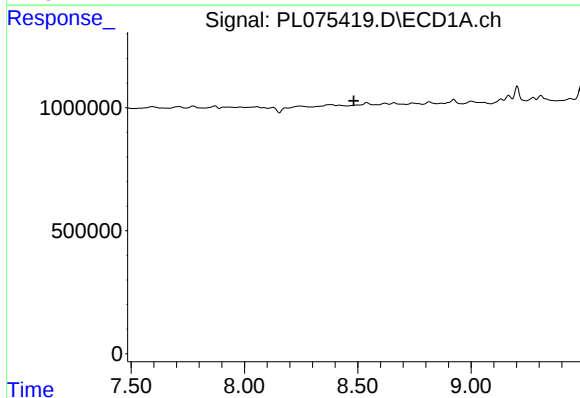


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 8.482 min
Response: 0
Conc: N.D.

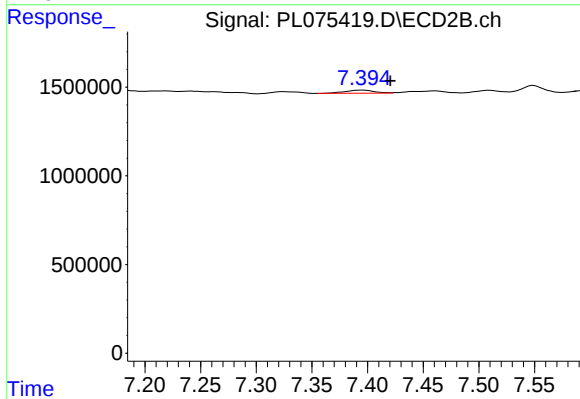


#26 Chlordane-4

R.T.: 7.396 min
Delta R.T.: -0.025 min
Response: 328828
Conc: 1.74 ng/ml

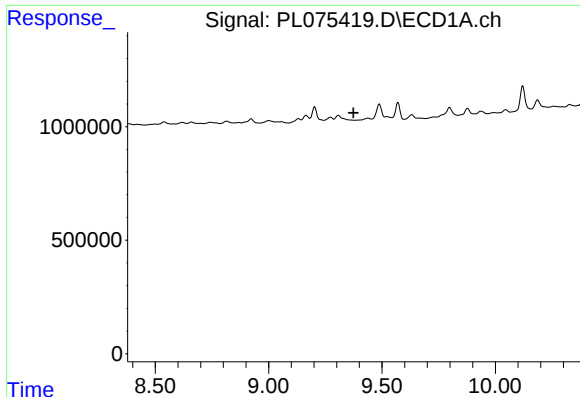


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 9.375 min
Response: 0
Conc: N.D.

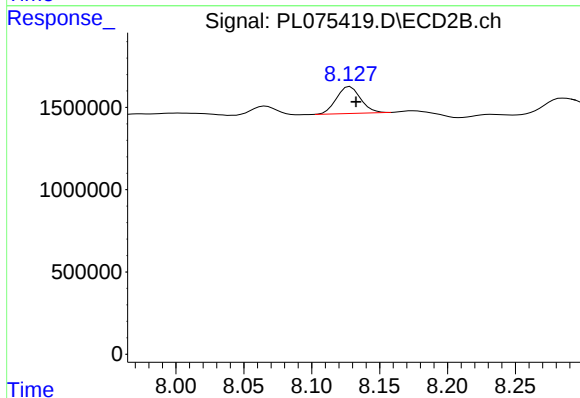


#27 Chlordane-5

R.T.: 8.128 min
Delta R.T.: -0.004 min
Response: 2033271
Conc: 40.75 ng/ml

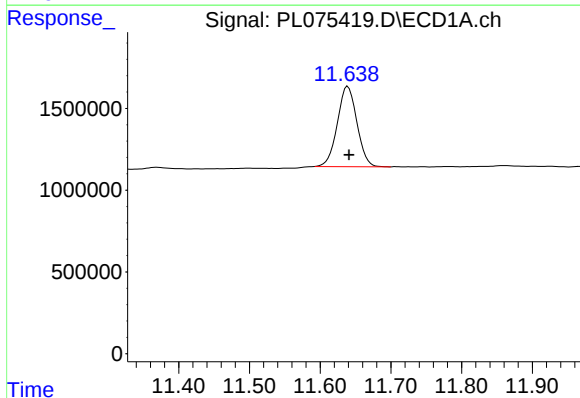

#28 Decachlorobiphenyl

R.T.: 11.639 min
Delta R.T.: -0.002 min
Response: 9430073
Conc: 17.59 ng/ml

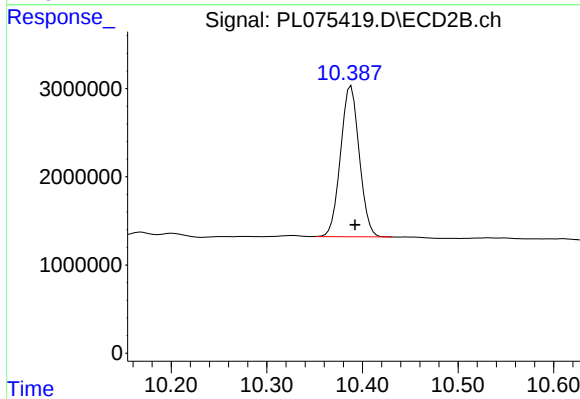

#28 Decachlorobiphenyl

R.T.: 10.388 min
Delta R.T.: -0.004 min
Response: 23287289
Conc: 16.97 ng/ml