

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060222\
 Data File : PL075421.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2022 01:57
 Operator : AR\AJ
 Sample : N2951-01 10X
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 06:13:08 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 01 10:19:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	5.643	4.642	877710	2612772	1.493	1.649
28)	SA Decachlor...	11.640	10.388	1066587	2218865	1.989	1.617
Target Compounds							
7)	B delta-BHC	0.000	6.412	0	525711	N.D.	0.245 #
11)	B alpha-Chl...	0.000	7.395f	0	253884	N.D.	0.139 #
13)	MA Dieldrin	0.000	7.755	0	186271	N.D.	0.107 #
14)	MA Endrin	0.000	8.068f	0	182478	N.D.	0.117 #
15)	B Endosulfa...	9.307	0.000	254704	0	0.451	N.D. #
16)	A 4,4'-DDD	9.204	0.000	283642	0	0.574	N.D. #
17)	MA 4,4'-DDT	0.000	8.465	0	519237	N.D.	0.363 #
19)	B Endosulfa...	0.000	8.775	0	297418	N.D.	0.199 #
21)	B Endrin ke...	10.188f	0.000	900834	0	1.467	N.D. #
26)	Chlordane-4	0.000	7.395f	0	253884	N.D.	1.344 #
27)	Chlordane-5	0.000	8.128	0	503039	N.D.	10.081 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060222\
Data File : PL075421.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2022 01:57
Operator : AR\AJ
Sample : N2951-01 10X
Misc :
ALS Vial : 49 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 06:13:08 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
Quant Title : GC Extractables
QLast Update : Wed Jun 01 10:19:11 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

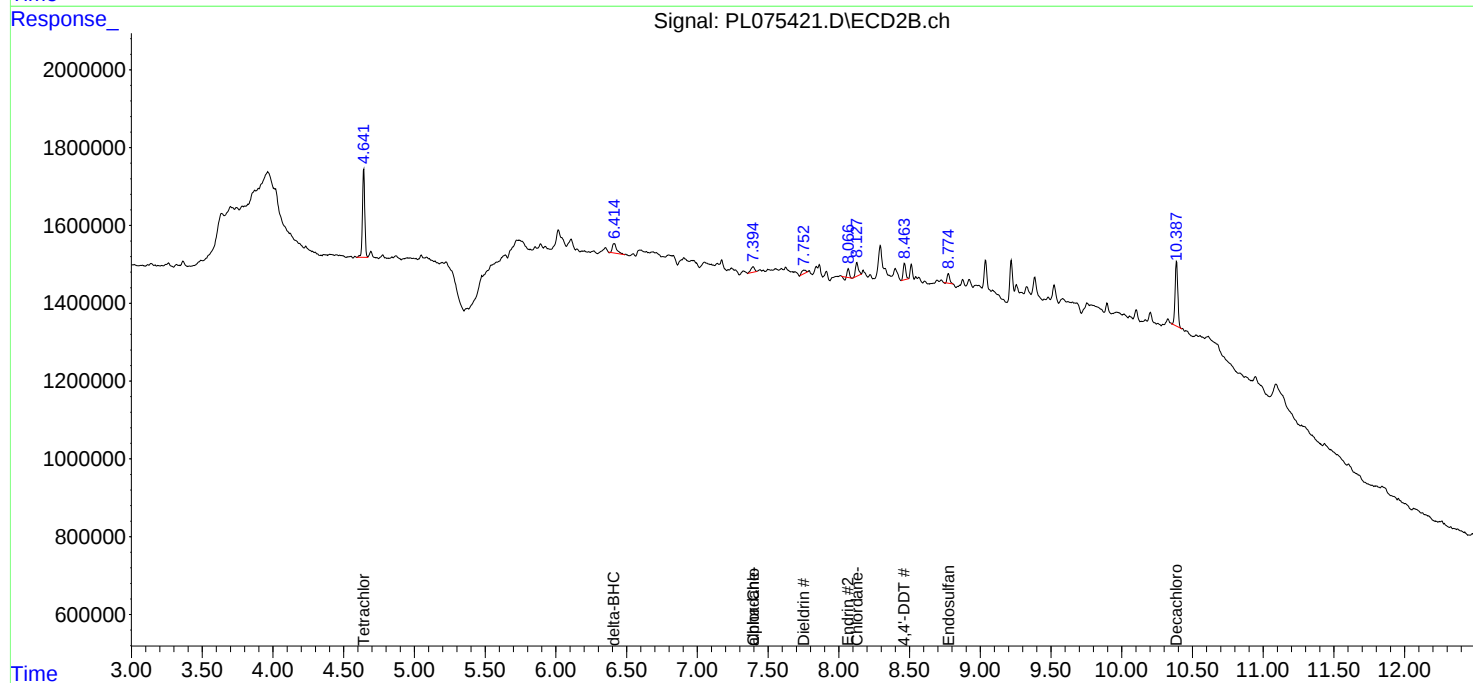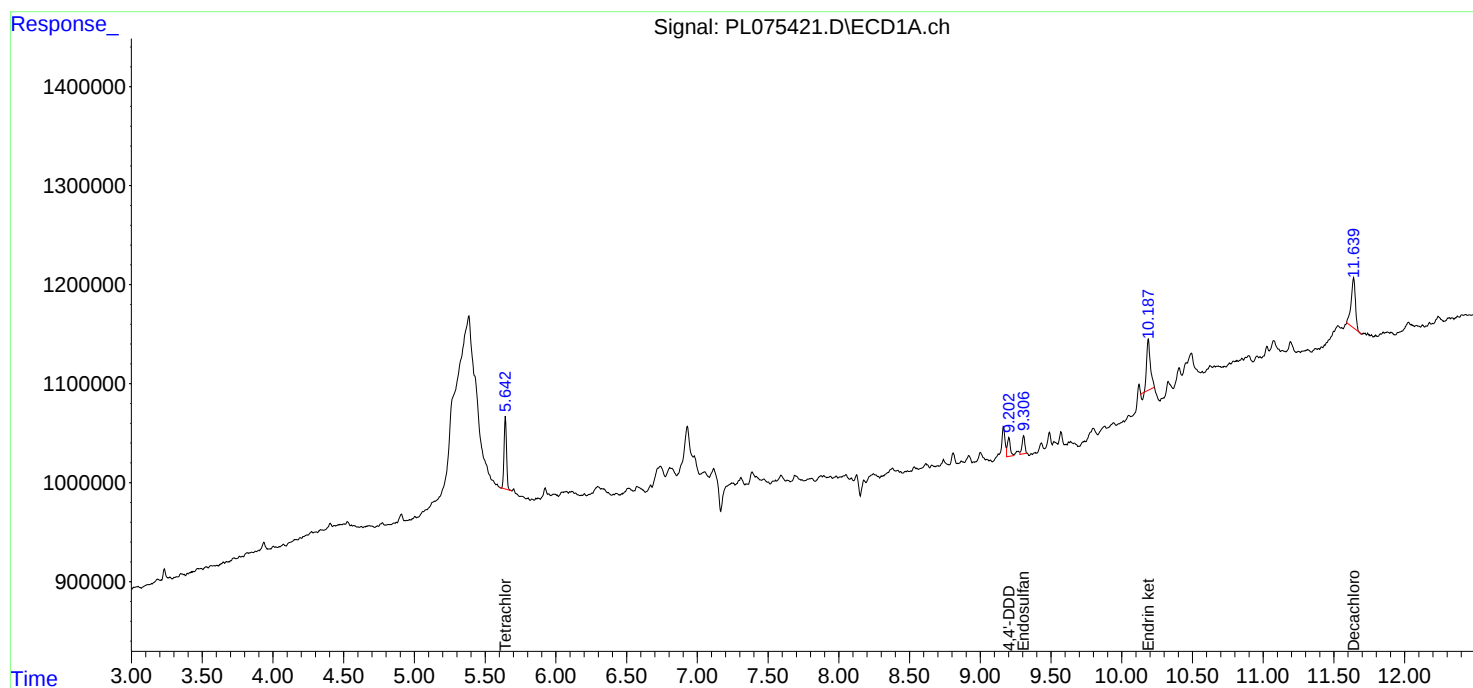

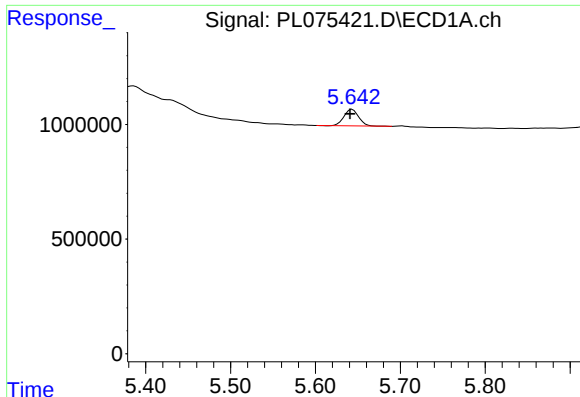


#1 Tetrachloro-m-xylene

R.T.: 5.643 min
Delta R.T.: 0.002 min
Response: 877710
Conc: 1.49 ng/ml

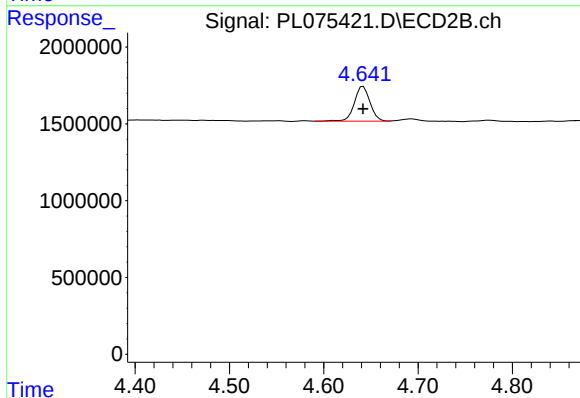


#1 Tetrachloro-m-xylene

R.T.: 4.642 min
Delta R.T.: 0.000 min
Response: 2612772
Conc: 1.65 ng/ml

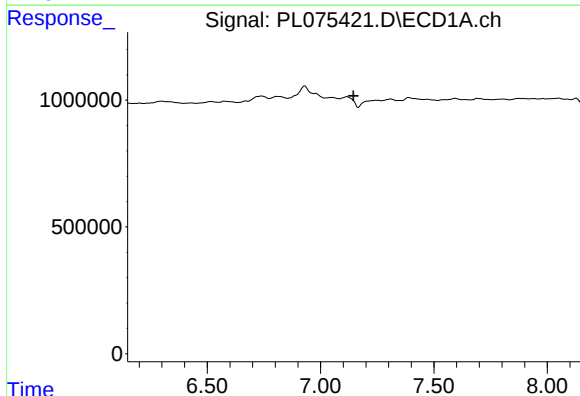


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.146 min
Response: 0
Conc: N.D.

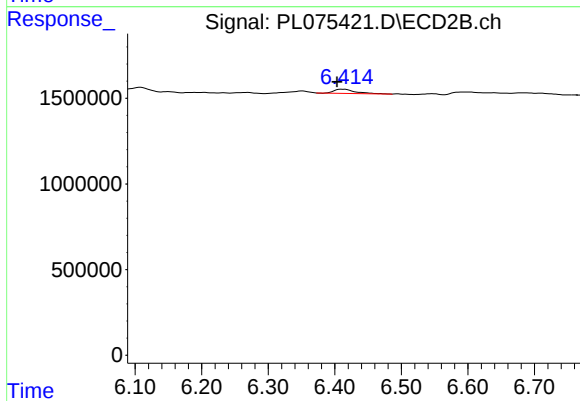


#7 delta-BHC

R.T.: 6.412 min
Delta R.T.: 0.008 min
Response: 525711
Conc: 0.25 ng/ml

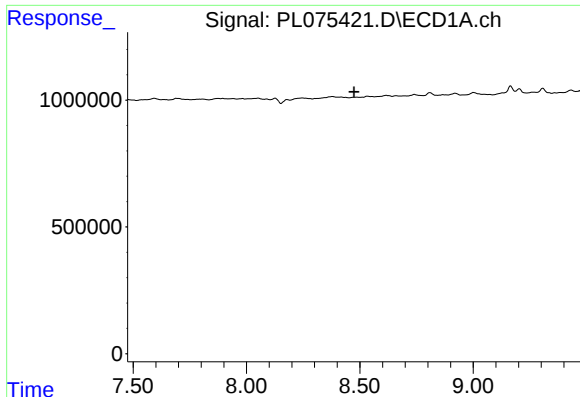


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.474 min
Response: 0
Conc: N.D.

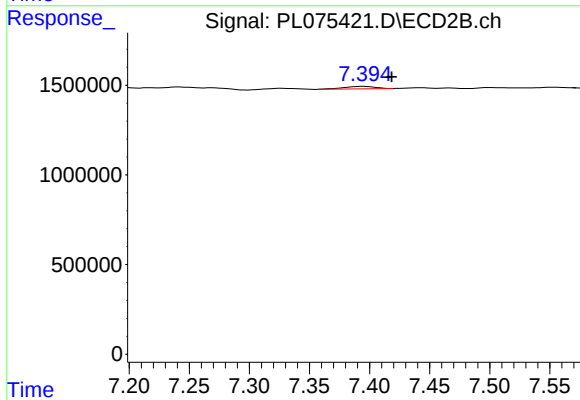


#11 alpha-Chlordane

R.T.: 7.395 min
Delta R.T.: -0.023 min
Response: 253884
Conc: 0.14 ng/ml

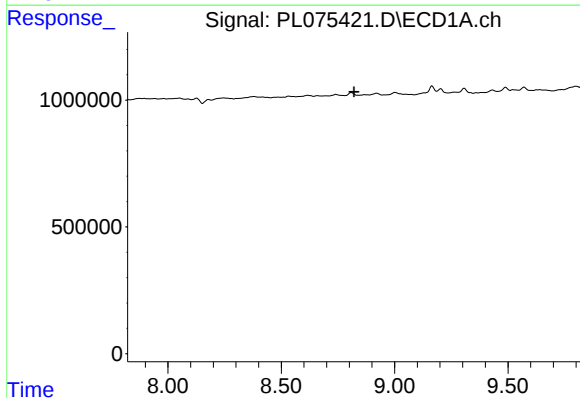


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 8.821 min
Response: 0
Conc: N.D.

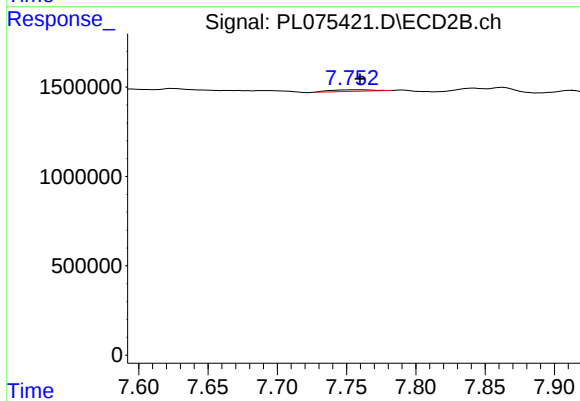


#13 Dieldrin

R.T.: 7.755 min
Delta R.T.: -0.005 min
Response: 186271
Conc: 0.11 ng/ml

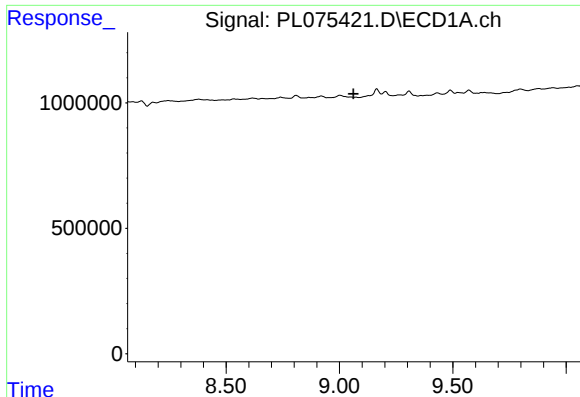


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 9.062 min
Response: 0
Conc: N.D.

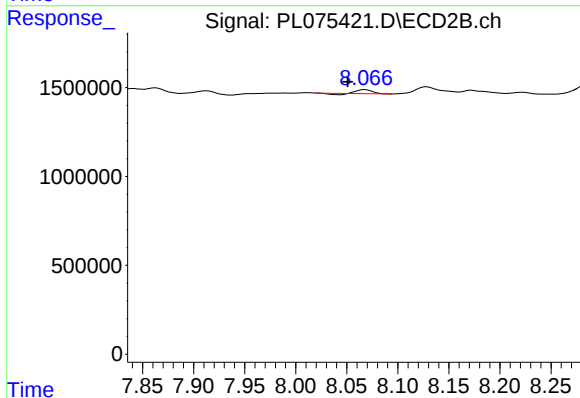


#14 Endrin

R.T.: 8.068 min
Delta R.T.: 0.017 min
Response: 182478
Conc: 0.12 ng/ml

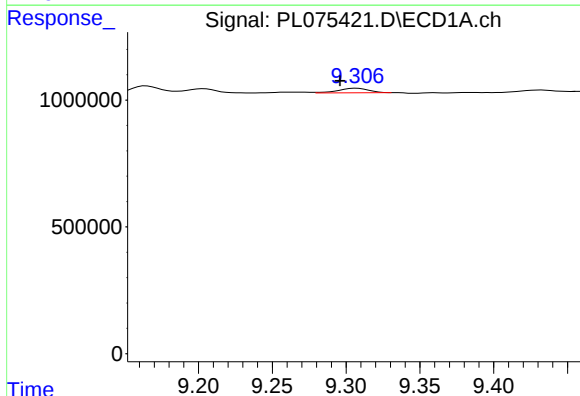


#15 Endosulfan II

R.T.: 9.307 min
Delta R.T.: 0.011 min
Response: 254704
Conc: 0.45 ng/ml

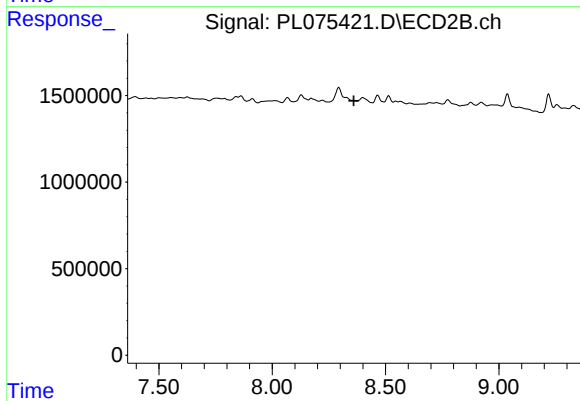


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.361 min
Response: 0
Conc: N.D.

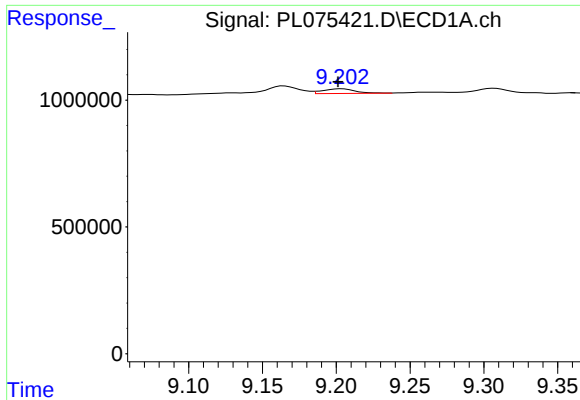


#16 4,4'-DDD

R.T.: 9.204 min
Delta R.T.: 0.002 min
Response: 283642
Conc: 0.57 ng/ml

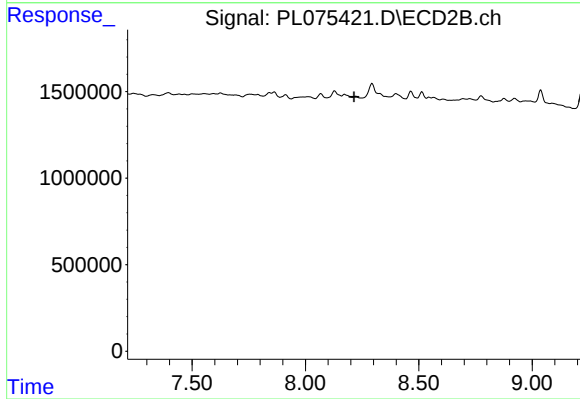


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 8.215 min
Response: 0
Conc: N.D.

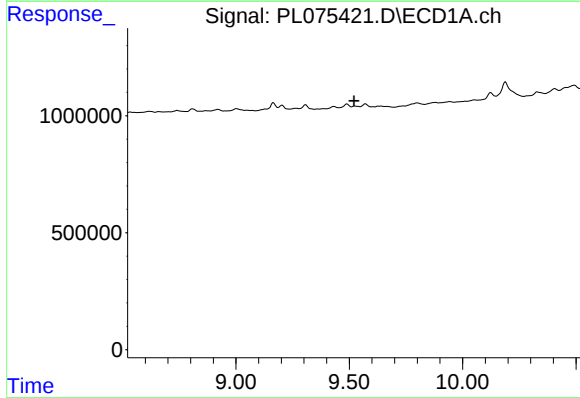


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 9.522 min
Response: 0
Conc: N.D.

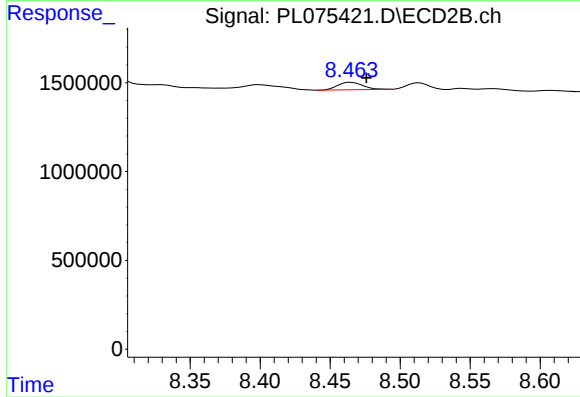


#17 4,4'-DDT

R.T.: 8.465 min
Delta R.T.: -0.011 min
Response: 519237
Conc: 0.36 ng/ml

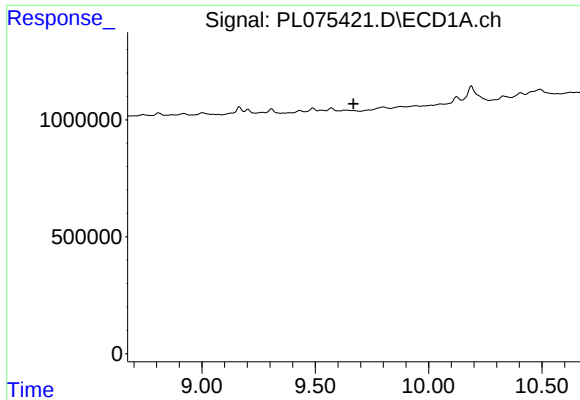


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 9.669 min
Response: 0
Conc: N.D.

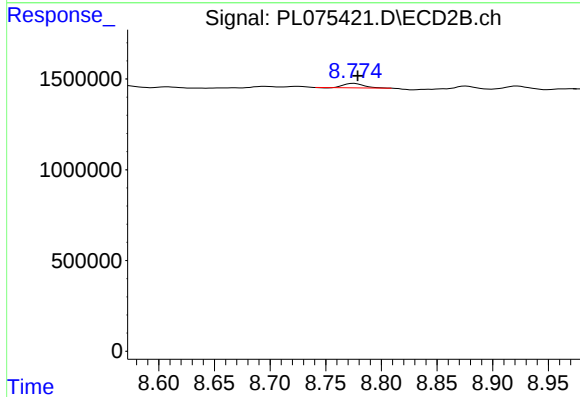


#19 Endosulfan Sulfate

R.T.: 8.775 min
Delta R.T.: -0.003 min
Response: 297418
Conc: 0.20 ng/ml

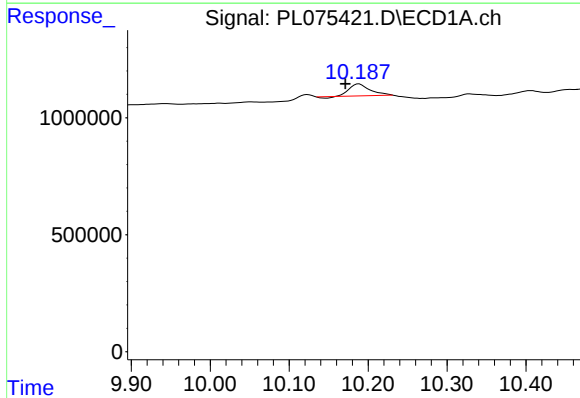


#21 Endrin ketone

R.T.: 10.188 min
Delta R.T.: 0.017 min
Response: 900834
Conc: 1.47 ng/ml

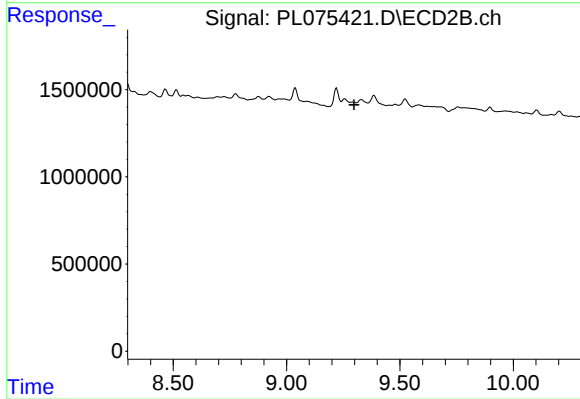


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.298 min
Response: 0
Conc: N.D.

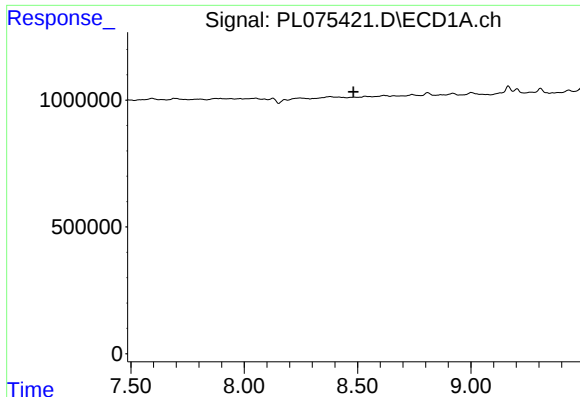


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 8.482 min
Response: 0
Conc: N.D.

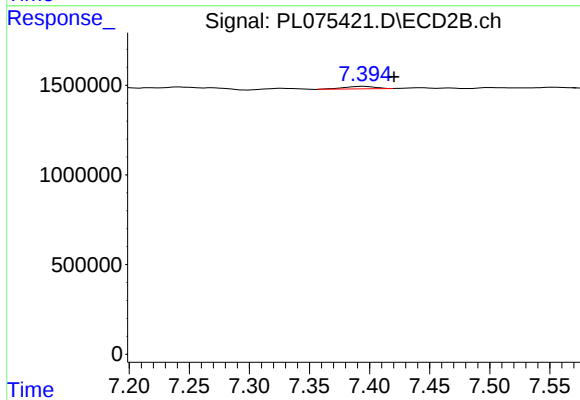


#26 Chlordane-4

R.T.: 7.395 min
Delta R.T.: -0.025 min
Response: 253884
Conc: 1.34 ng/ml

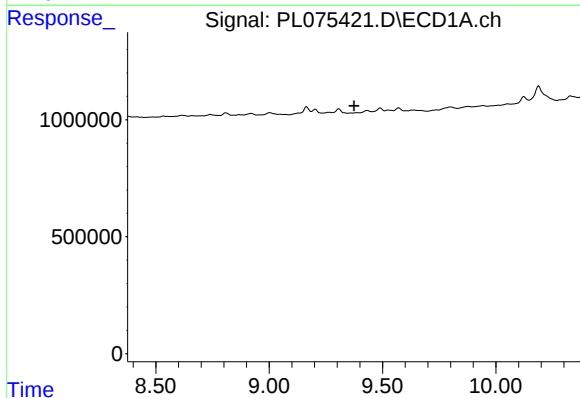


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 9.375 min
Response: 0
Conc: N.D.

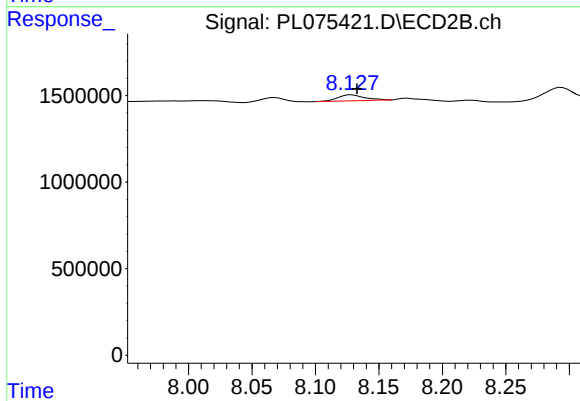


#27 Chlordane-5

R.T.: 8.128 min
Delta R.T.: -0.004 min
Response: 503039
Conc: 10.08 ng/ml

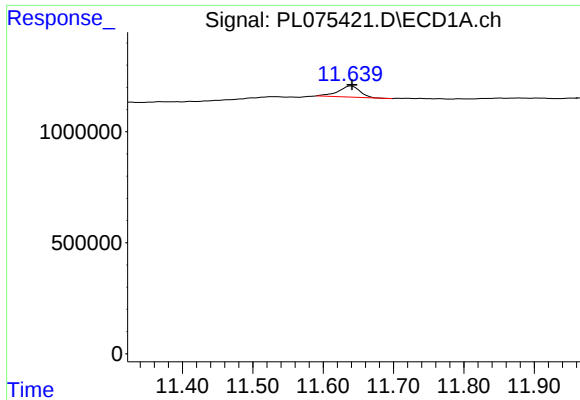

#28 Decachlorobiphenyl

R.T.: 11.640 min
Delta R.T.: -0.001 min
Response: 1066587
Conc: 1.99 ng/ml

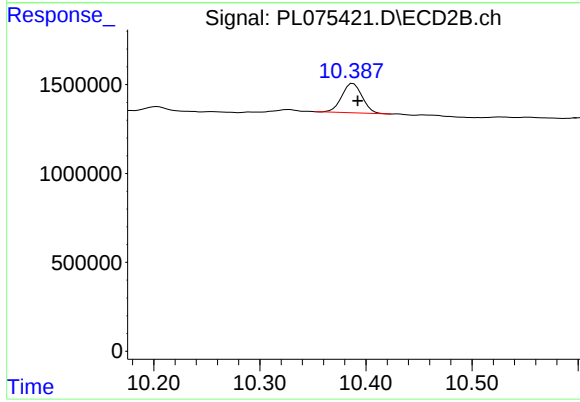

#28 Decachlorobiphenyl

R.T.: 10.388 min
Delta R.T.: -0.004 min
Response: 2218865
Conc: 1.62 ng/ml