

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060222\
 Data File : PL075430.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2022 04:26
 Operator : AR\AJ
 Sample : PB145193BL
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 06:16:27 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 01 10:19:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	5.643	4.642	11705917	30681902	19.917	19.368
28)	SA Decachlor...	11.641	10.388	11485559	26461073	21.421	19.283
Target Compounds							
7)	B delta-BHC	0.000	6.415	0	180419	N.D.	0.084 #
9)	A Endosulfan I	0.000	7.484	0	132345	N.D.	0.078 #
11)	B alpha-Chl...	0.000	7.395f	0	71265	N.D.	0.039 #
14)	MA Endrin	0.000	8.070f	0	63402	N.D.	0.041 #
15)	B Endosulfa...	9.307	0.000	269390	0	0.477	N.D. #
18)	B Endrin al...	0.000	8.552	0	1106056	N.D.	0.917 #
19)	B Endosulfa...	9.679	8.773	183009	1137834	0.329	0.760 #
21)	B Endrin ke...	10.190f	0.000	315080	0	0.513	N.D. #
26)	Chlordane-4	0.000	7.395f	0	71265	N.D.	0.377 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060222\
Data File : PL075430.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2022 04:26
Operator : AR\AJ
Sample : PB145193BL
Misc :
ALS Vial : 58 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 06:16:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
Quant Title : GC Extractables
QLast Update : Wed Jun 01 10:19:11 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

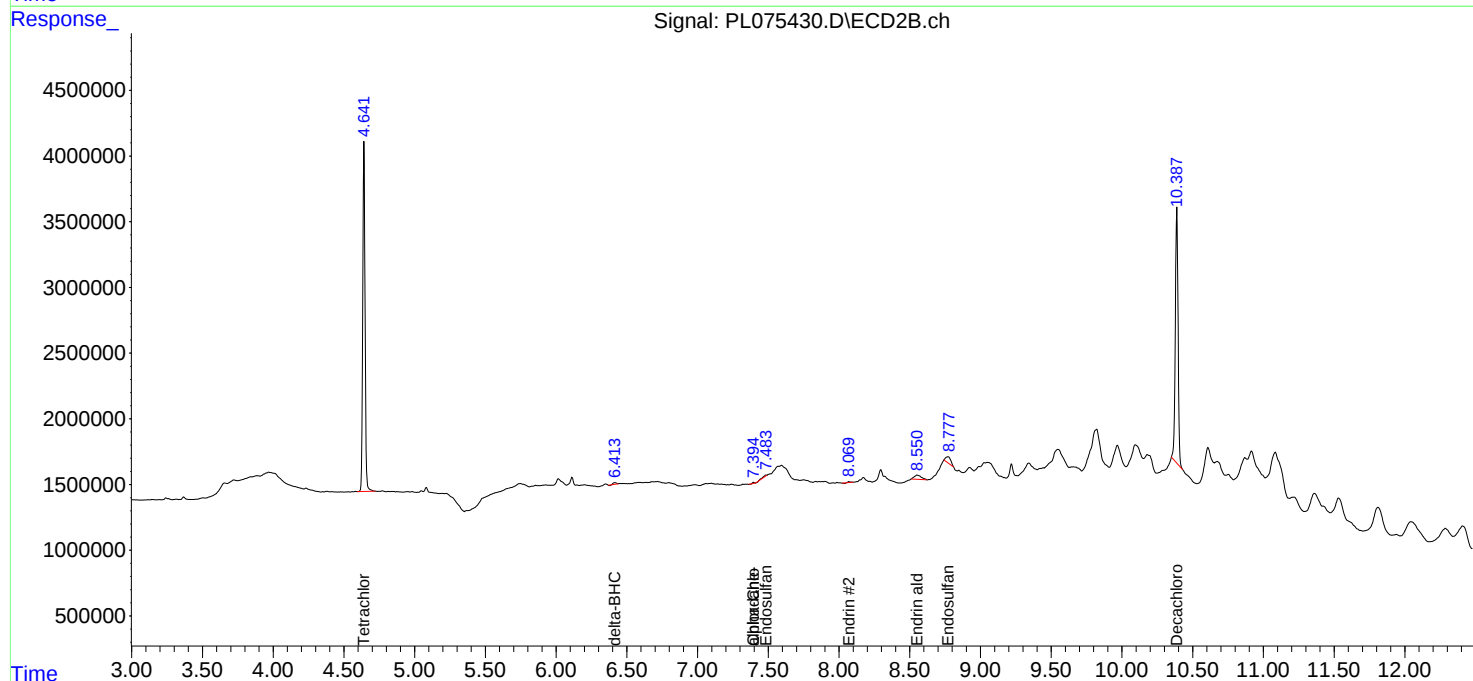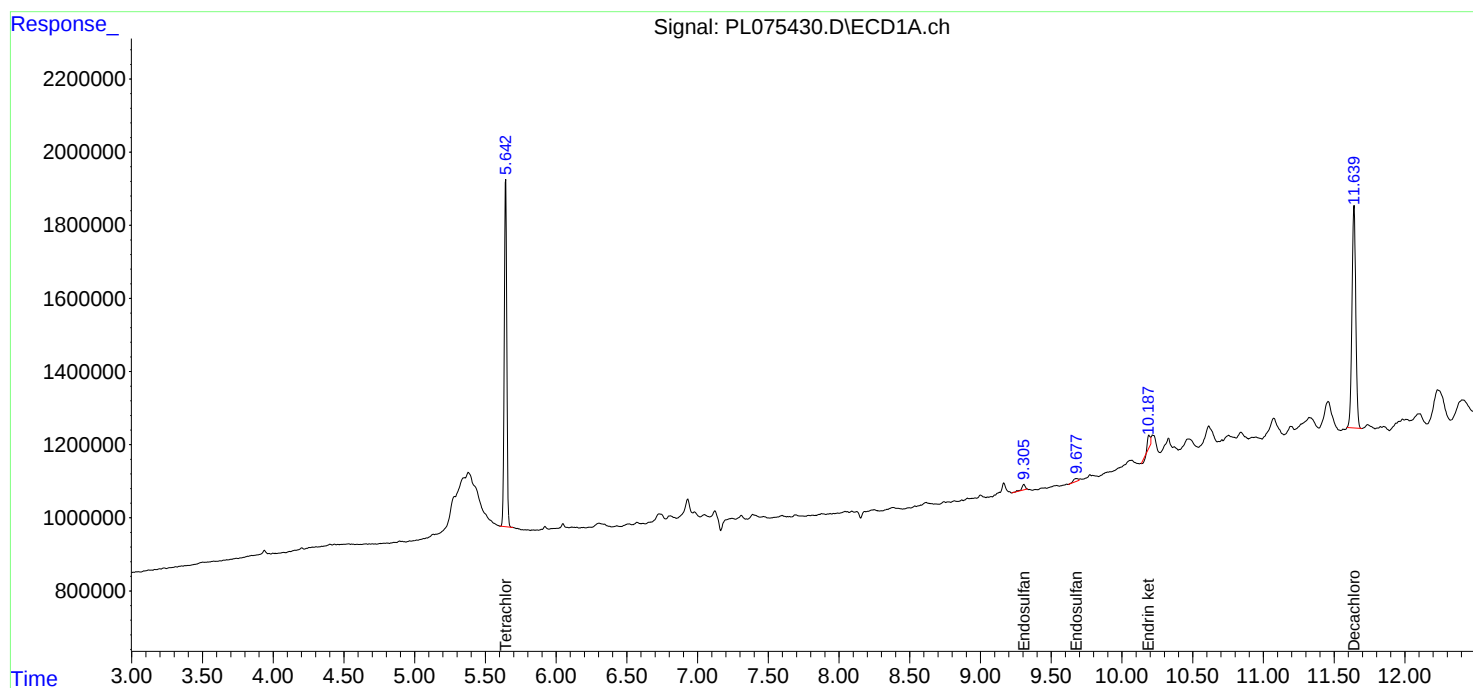

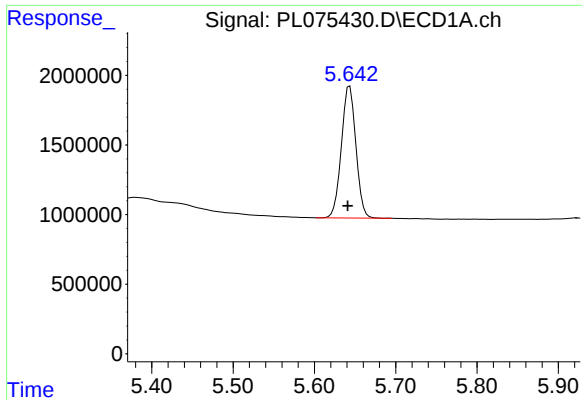


#1 Tetrachloro-m-xylene

R.T.: 5.643 min
Delta R.T.: 0.002 min
Response: 11705917
Conc: 19.92 ng/ml

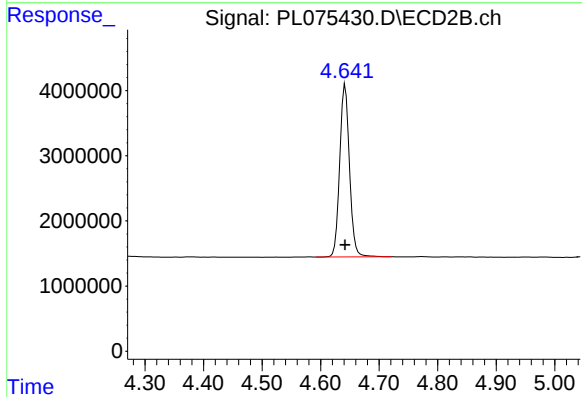


#1 Tetrachloro-m-xylene

R.T.: 4.642 min
Delta R.T.: 0.000 min
Response: 30681902
Conc: 19.37 ng/ml

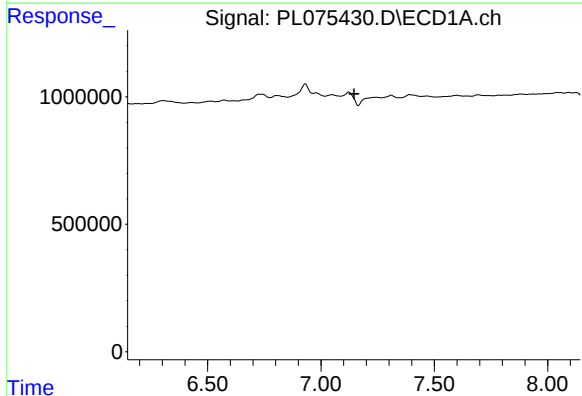


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.146 min
Response: 0
Conc: N.D.

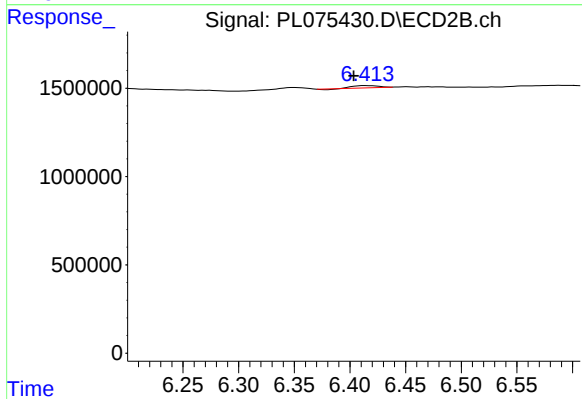


#7 delta-BHC

R.T.: 6.415 min
Delta R.T.: 0.012 min
Response: 180419
Conc: 0.08 ng/ml

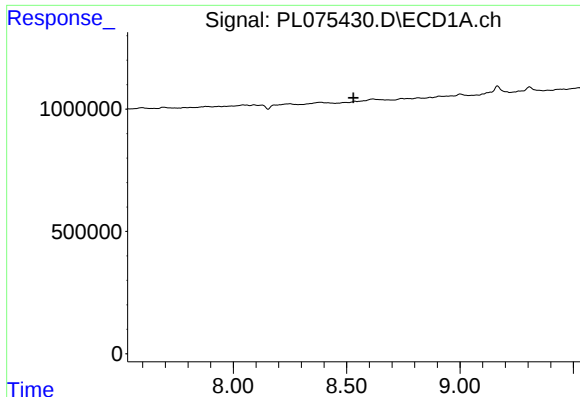


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 8.530 min
Response: 0
Conc: N.D.

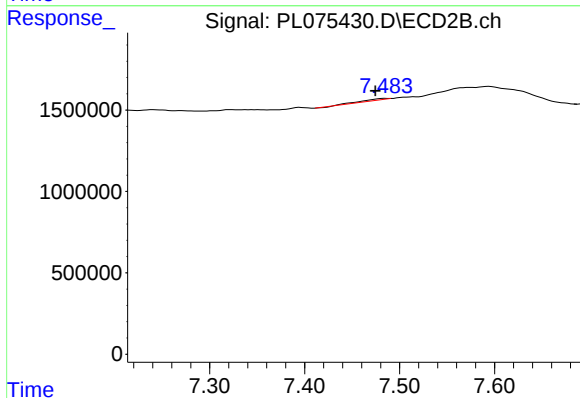


#9 Endosulfan I

R.T.: 7.484 min
Delta R.T.: 0.010 min
Response: 132345
Conc: 0.08 ng/ml

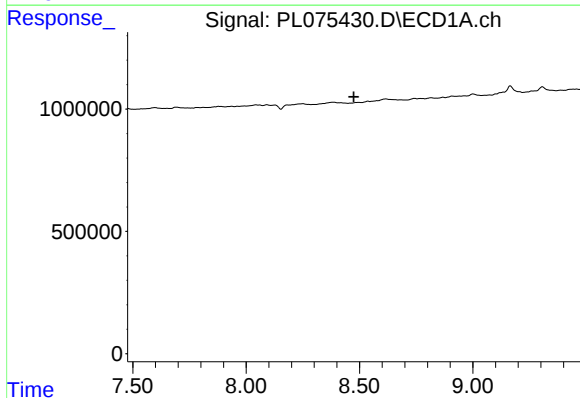


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.474 min
Response: 0
Conc: N.D.

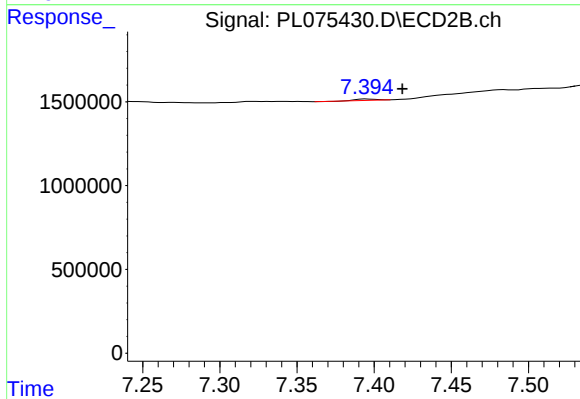


#11 alpha-Chlordane

R.T.: 7.395 min
Delta R.T.: -0.023 min
Response: 71265
Conc: 0.04 ng/ml

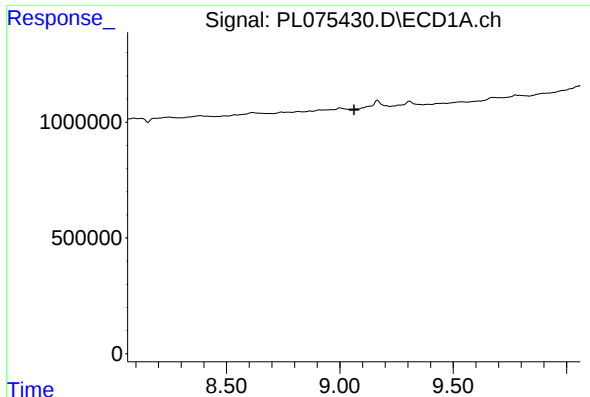


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 9.062 min
Response: 0
Conc: N.D.

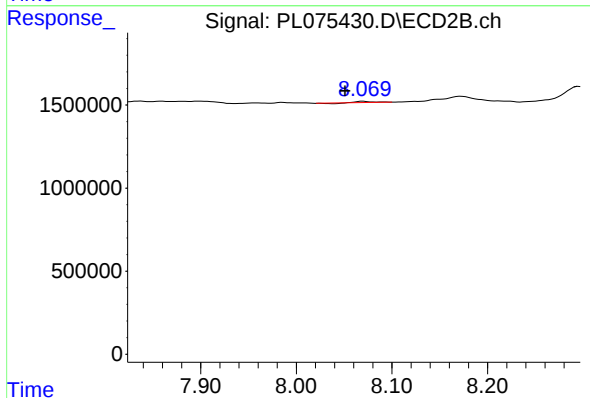


#14 Endrin

R.T.: 8.070 min
Delta R.T.: 0.019 min
Response: 63402
Conc: 0.04 ng/ml

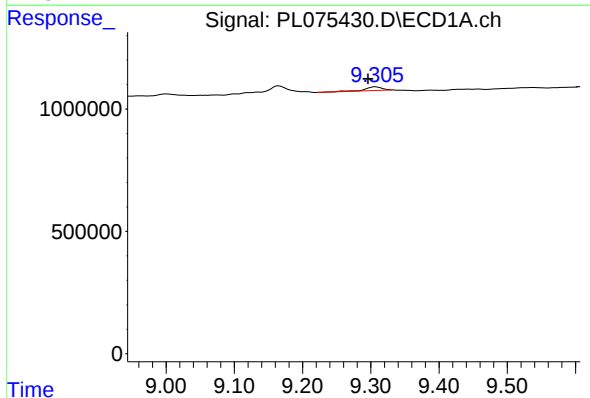


#15 Endosulfan II

R.T.: 9.307 min
Delta R.T.: 0.011 min
Response: 269390
Conc: 0.48 ng/ml

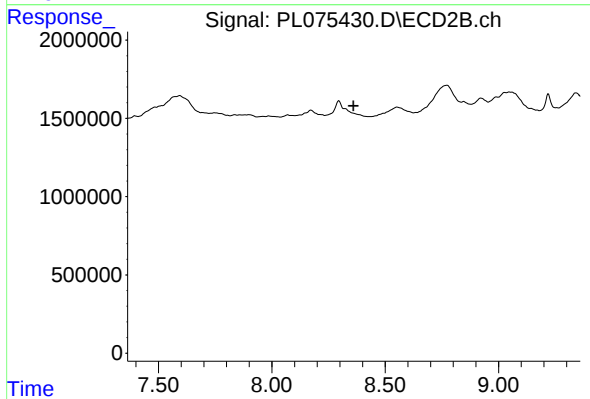


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.361 min
Response: 0
Conc: N.D.

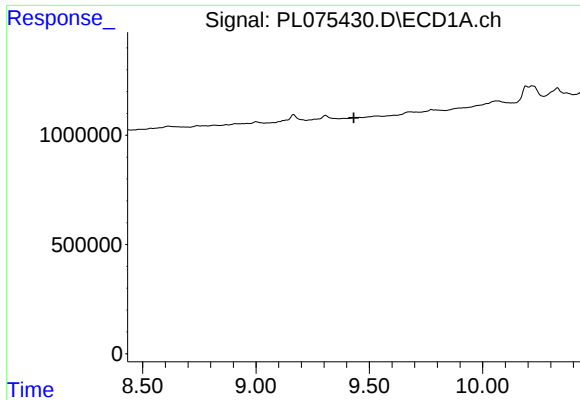


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 9.431 min
Response: 0
Conc: N.D.

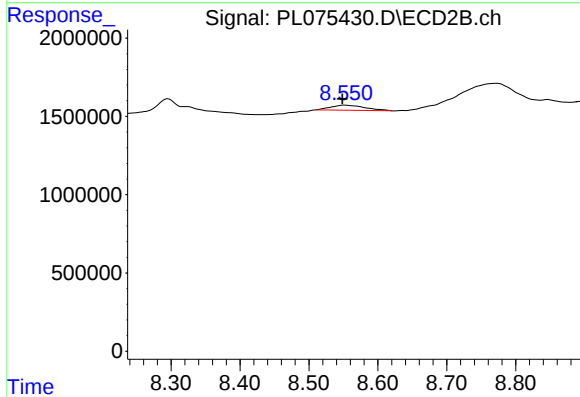


#18 Endrin aldehyde

R.T.: 8.552 min
Delta R.T.: 0.003 min
Response: 1106056
Conc: 0.92 ng/ml

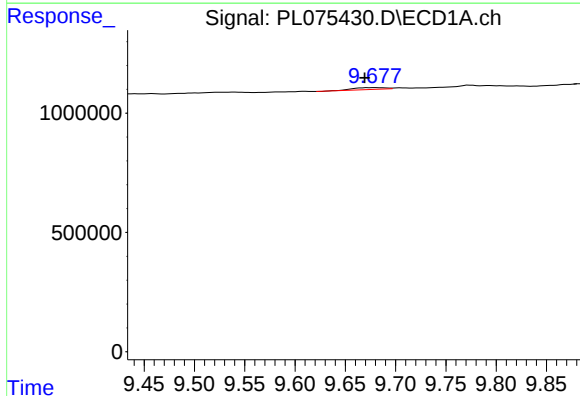


#19 Endosulfan Sulfate

R.T.: 9.679 min
Delta R.T.: 0.010 min
Response: 183009
Conc: 0.33 ng/ml

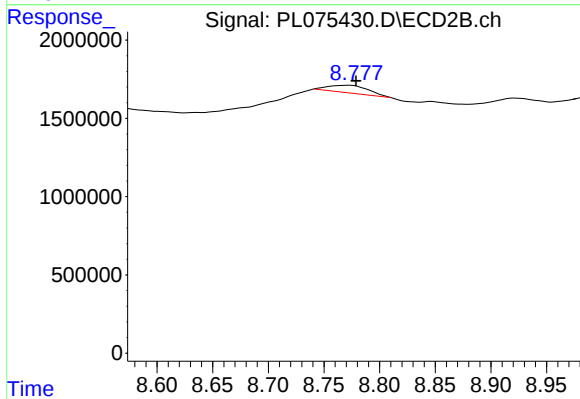


#19 Endosulfan Sulfate

R.T.: 8.773 min
Delta R.T.: -0.006 min
Response: 1137834
Conc: 0.76 ng/ml

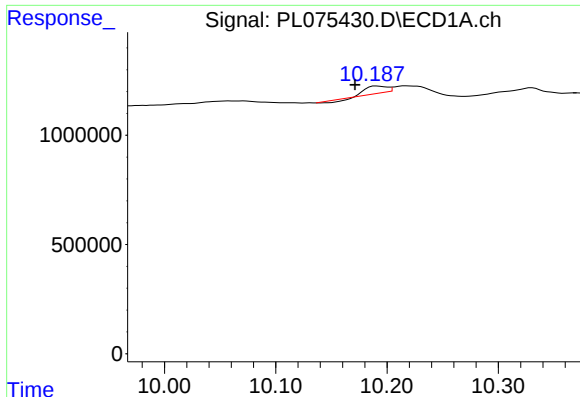


#21 Endrin ketone

R.T.: 10.190 min
Delta R.T.: 0.019 min
Response: 315080
Conc: 0.51 ng/ml

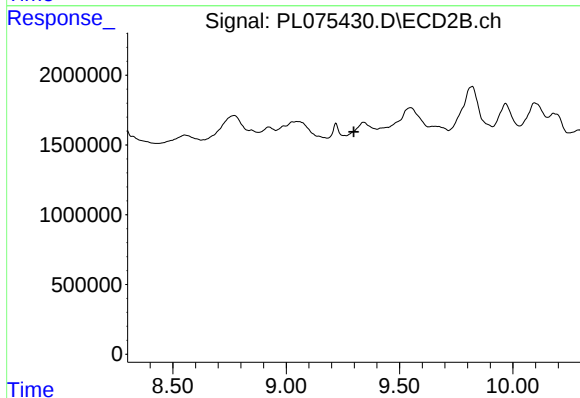


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.298 min
Response: 0
Conc: N.D.

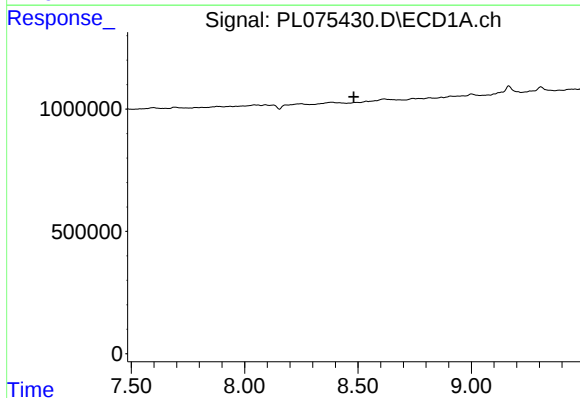


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 8.482 min
Response: 0
Conc: N.D.

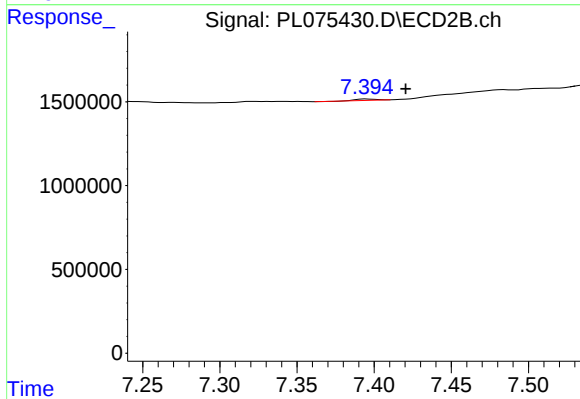

#26 Chlordane-4

R.T.: 7.395 min
Delta R.T.: -0.026 min
Response: 71265
Conc: 0.38 ng/ml

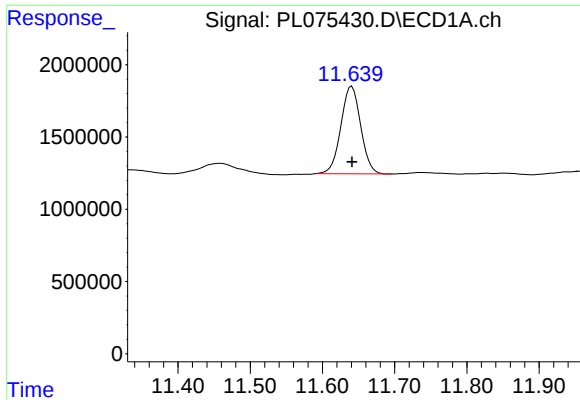


#28 Decachlorobiphenyl

R.T.: 11.641 min

Delta R.T.: 0.000 min

Response: 11485559

Conc: 21.42 ng/ml

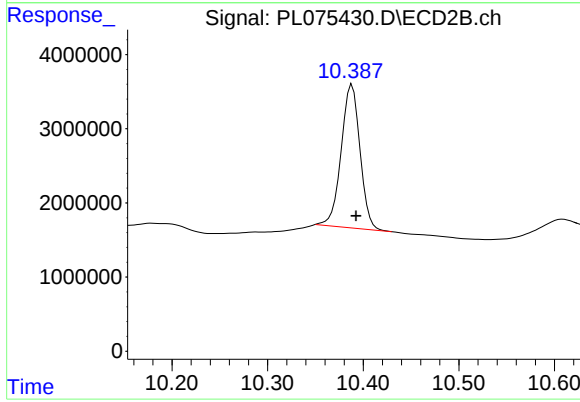

#28 Decachlorobiphenyl

R.T.: 10.388 min

Delta R.T.: -0.004 min

Response: 26461073

Conc: 19.28 ng/ml