

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060222\
 Data File : PL075432.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2022 04:59
 Operator : AR\AJ
 Sample : PB145262BL
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 06:17:05 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 01 10:19:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	5.644	4.643	11231835	29222043	19.110	18.447
28)	SA Decachlor...	11.641	10.388	10667235	24963485	19.895	18.191
Target Compounds							
7)	B delta-BHC	0.000	6.413	0	251296	N.D.	0.117 #
9)	A Endosulfan I	0.000	7.445f	0	155329	N.D.	0.092 #
11)	B alpha-Chl...	0.000	7.397f	0	358011	N.D.	0.196 #
14)	MA Endrin	0.000	8.068f	0	70193	N.D.	0.045 #
15)	B Endosulfa...	9.305	0.000	184073	0	0.326	N.D. #
21)	B Endrin ke...	10.189f	0.000	591086	0	0.963	N.D. #
26)	Chlordane-4	0.000	7.397f	0	358011	N.D.	1.895 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060222\
Data File : PL075432.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2022 04:59
Operator : AR\AJ
Sample : PB145262BL
Misc :
ALS Vial : 60 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 06:17:05 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
Quant Title : GC Extractables
QLast Update : Wed Jun 01 10:19:11 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

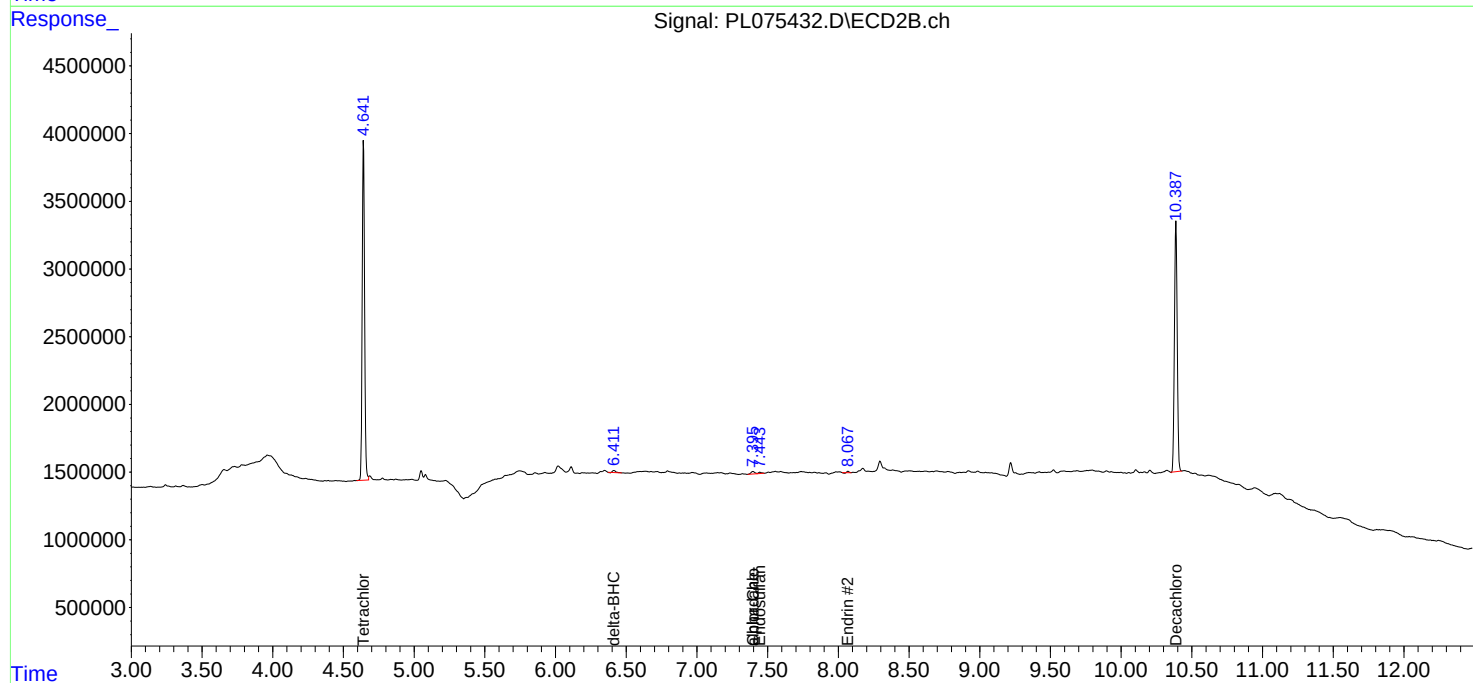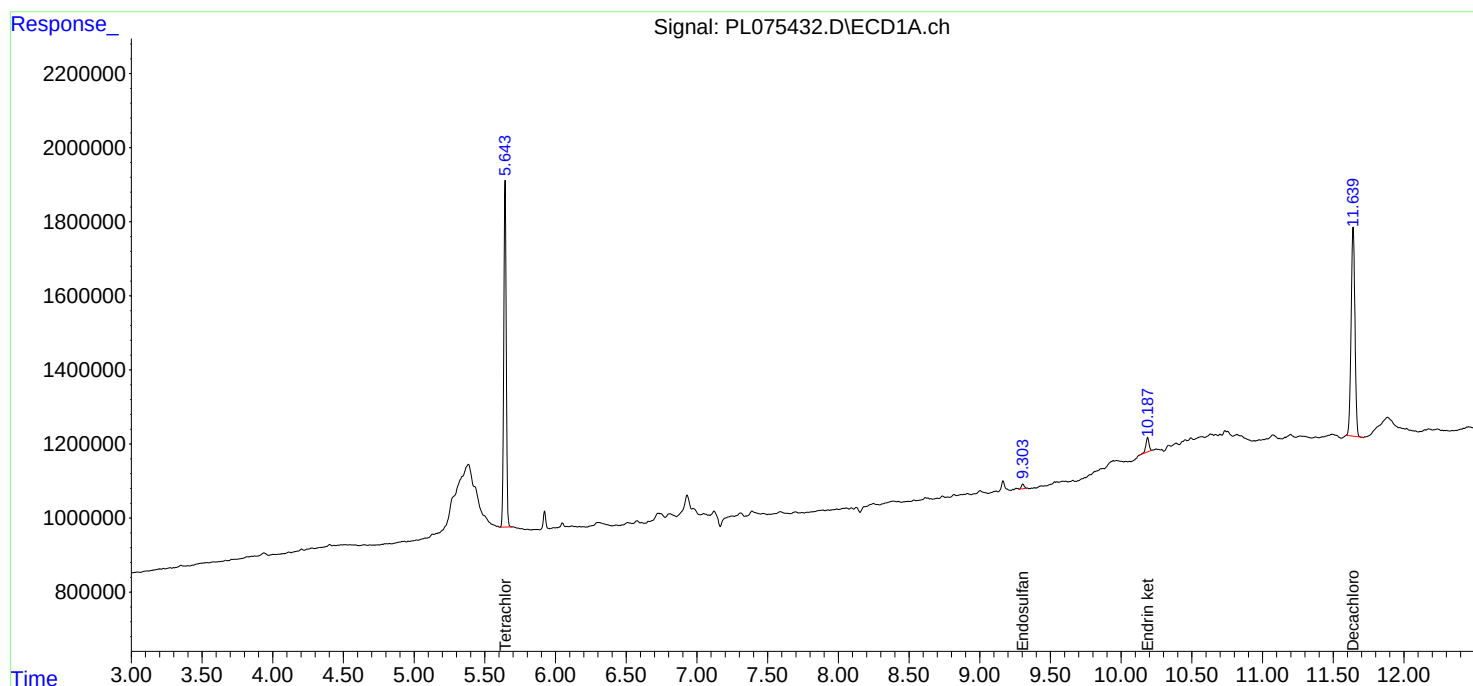

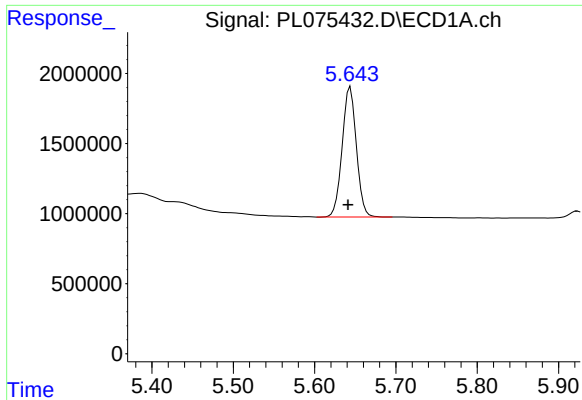


#1 Tetrachloro-m-xylene

R.T.: 5.644 min
Delta R.T.: 0.003 min
Response: 11231835
Conc: 19.11 ng/ml

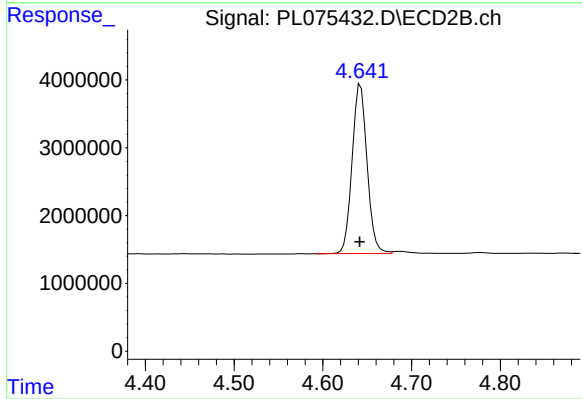


#1 Tetrachloro-m-xylene

R.T.: 4.643 min
Delta R.T.: 0.000 min
Response: 29222043
Conc: 18.45 ng/ml

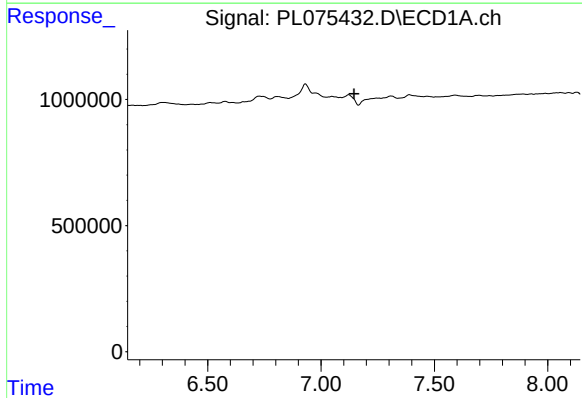


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.146 min
Response: 0
Conc: N.D.

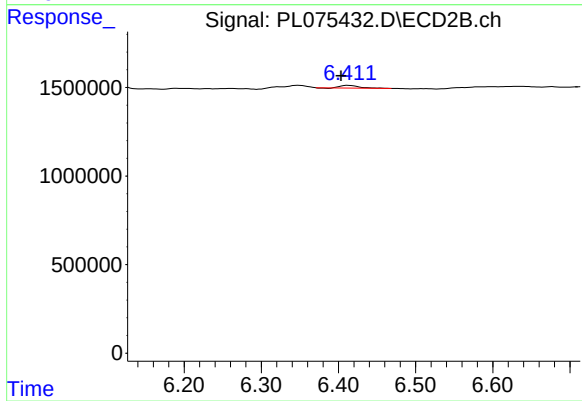


#7 delta-BHC

R.T.: 6.413 min
Delta R.T.: 0.010 min
Response: 251296
Conc: 0.12 ng/ml

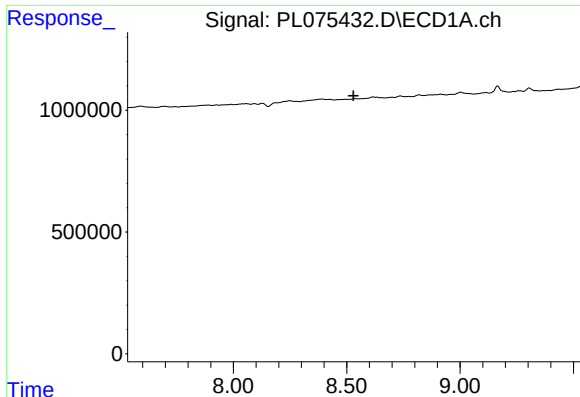


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 8.530 min
Response: 0
Conc: N.D.

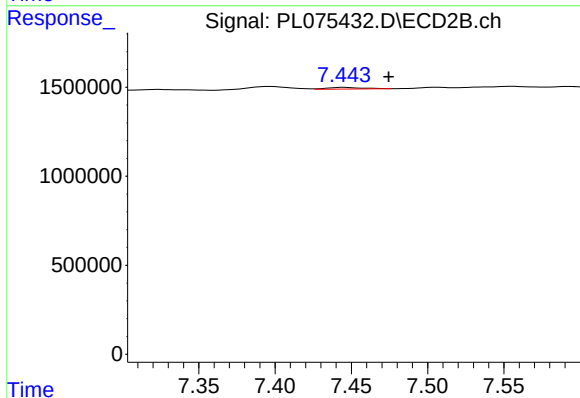


#9 Endosulfan I

R.T.: 7.445 min
Delta R.T.: -0.029 min
Response: 155329
Conc: 0.09 ng/ml

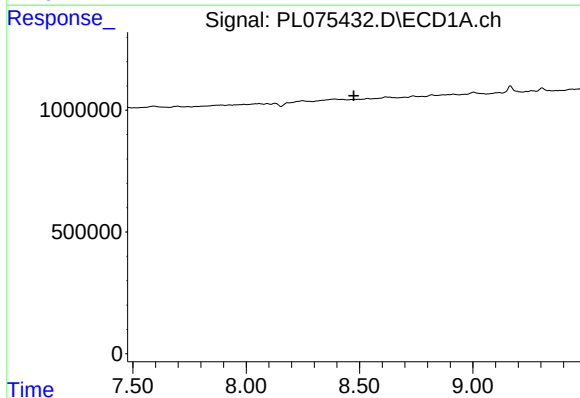


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.474 min
Response: 0
Conc: N.D.

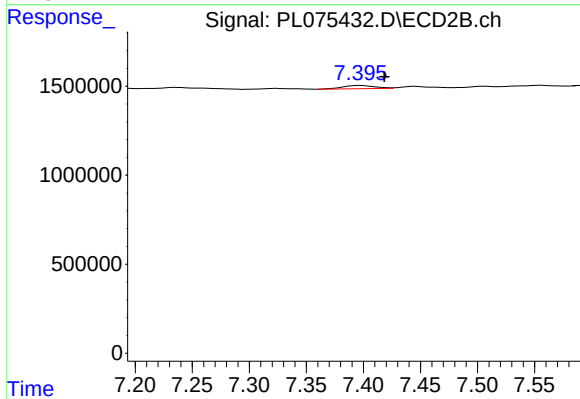


#11 alpha-Chlordane

R.T.: 7.397 min
Delta R.T.: -0.022 min
Response: 358011
Conc: 0.20 ng/ml

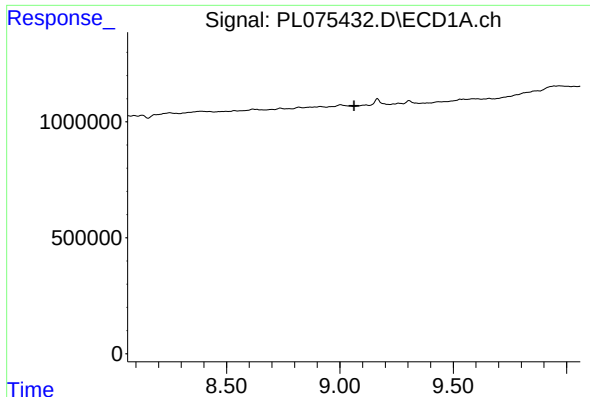


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 9.062 min
Response: 0
Conc: N.D.

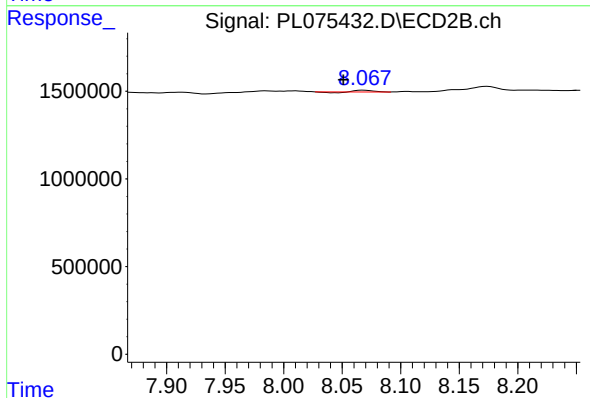


#14 Endrin

R.T.: 8.068 min
Delta R.T.: 0.018 min
Response: 70193
Conc: 0.05 ng/ml

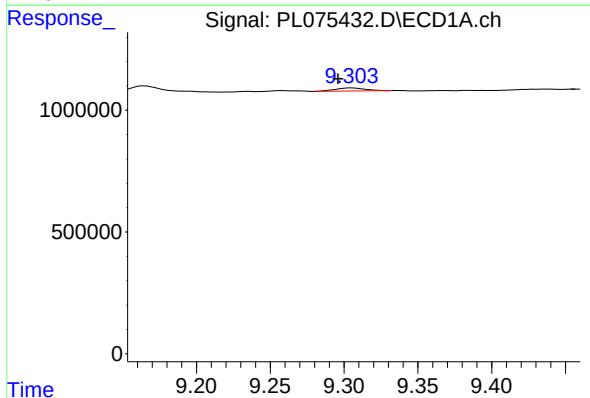


#15 Endosulfan II

R.T.: 9.305 min
Delta R.T.: 0.009 min
Response: 184073
Conc: 0.33 ng/ml

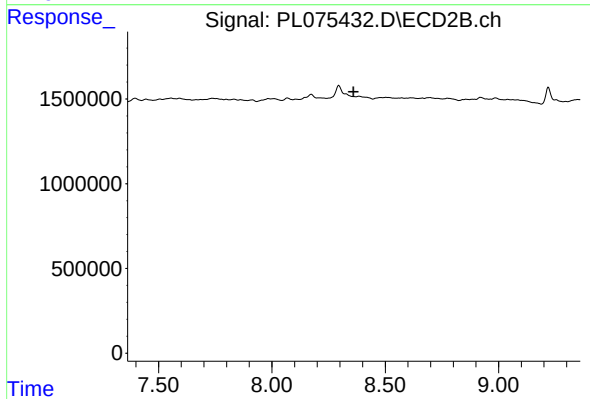


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.361 min
Response: 0
Conc: N.D.

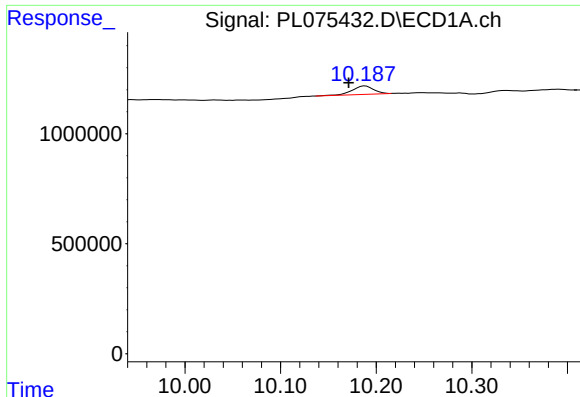


#21 Endrin ketone

R.T.: 10.189 min
Delta R.T.: 0.017 min
Response: 591086
Conc: 0.96 ng/ml

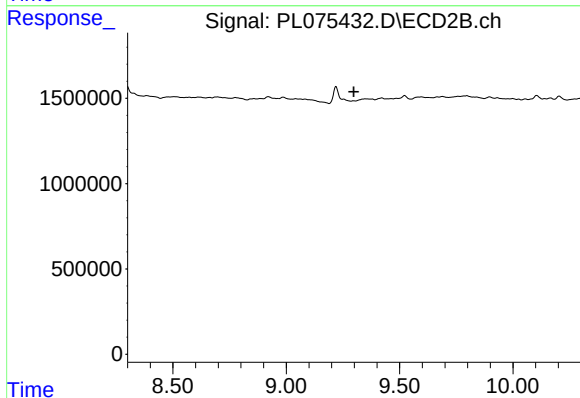


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.298 min
Response: 0
Conc: N.D.

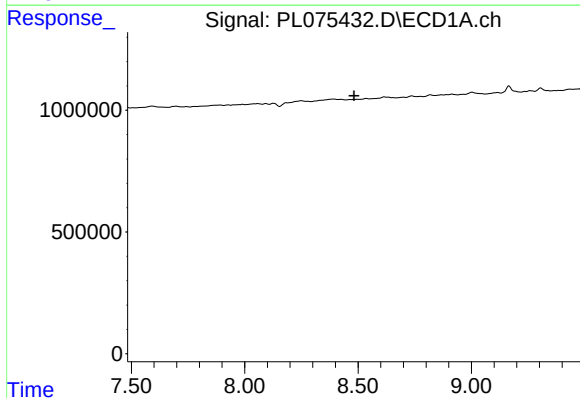


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 8.482 min
Response: 0
Conc: N.D.

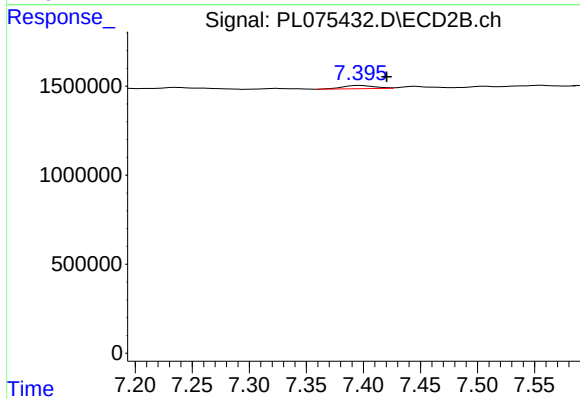


#26 Chlordane-4

R.T.: 7.397 min
Delta R.T.: -0.024 min
Response: 358011
Conc: 1.90 ng/ml

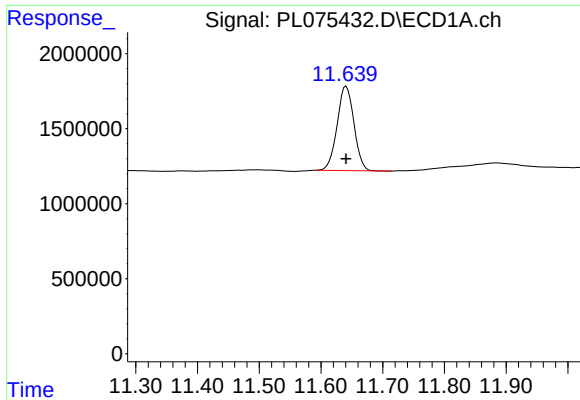

#28 Decachlorobiphenyl

R.T.: 11.641 min
Delta R.T.: 0.000 min
Response: 10667235
Conc: 19.89 ng/ml

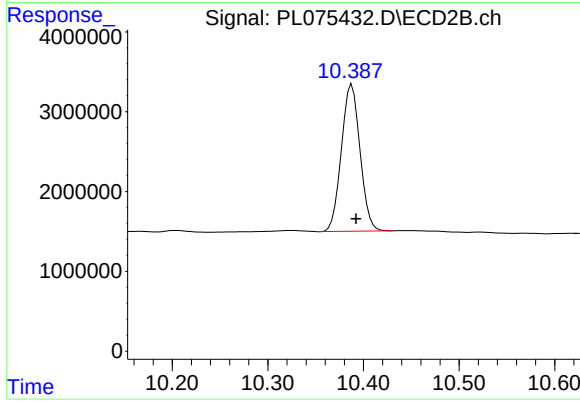

#28 Decachlorobiphenyl

R.T.: 10.388 min
Delta R.T.: -0.005 min
Response: 24963485
Conc: 18.19 ng/ml