

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060225\
 Data File : PL095833.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2025 09:06
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 21:51:34 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052125.M
 Quant Title : GC Extractables
 QLast Update : Thu May 22 06:29:30 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
8) B	Heptachlo...	5.714	0.000	115.2E6	0	30.170	N.D. #
13) MA	Dieldrin	0.000	5.492	0	26351013	N.D.	4.972 #
14) MA	Endrin	0.000	5.783	0	13315671	N.D.	2.731 #
15) B	Endosulfa...	0.000	6.069	0	9842638	N.D.	2.071 #
16) A	4,4'-DDD	6.757f	0.000	20396600	0	6.960	N.D. #
24)	Chlordane-2	0.000	4.475	0	29069395	N.D.	130.501 #
27)	Chlordane-5	0.000	6.069	0	9842638	N.D.	38.609 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060225\
Data File : PL095833.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2025 09:06
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 21:51:34 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052125.M
Quant Title : GC Extractables
QLast Update : Thu May 22 06:29:30 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

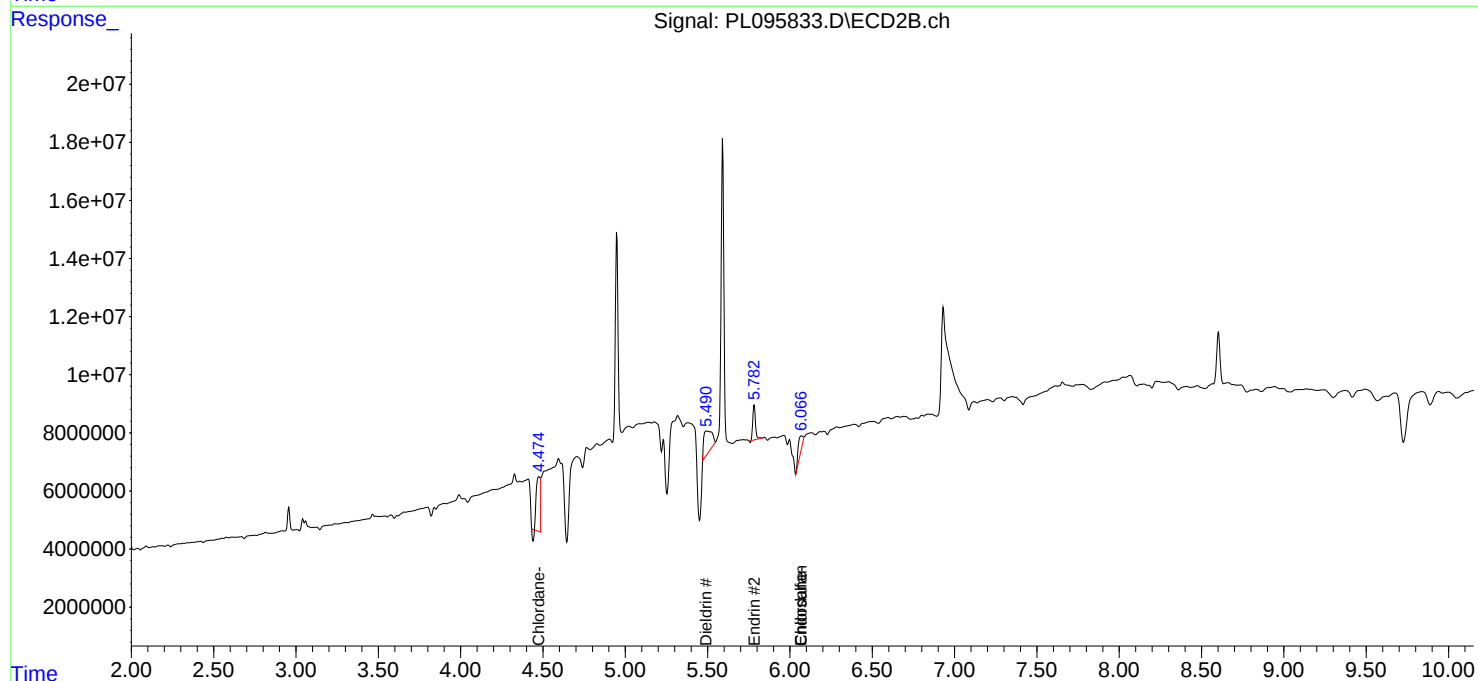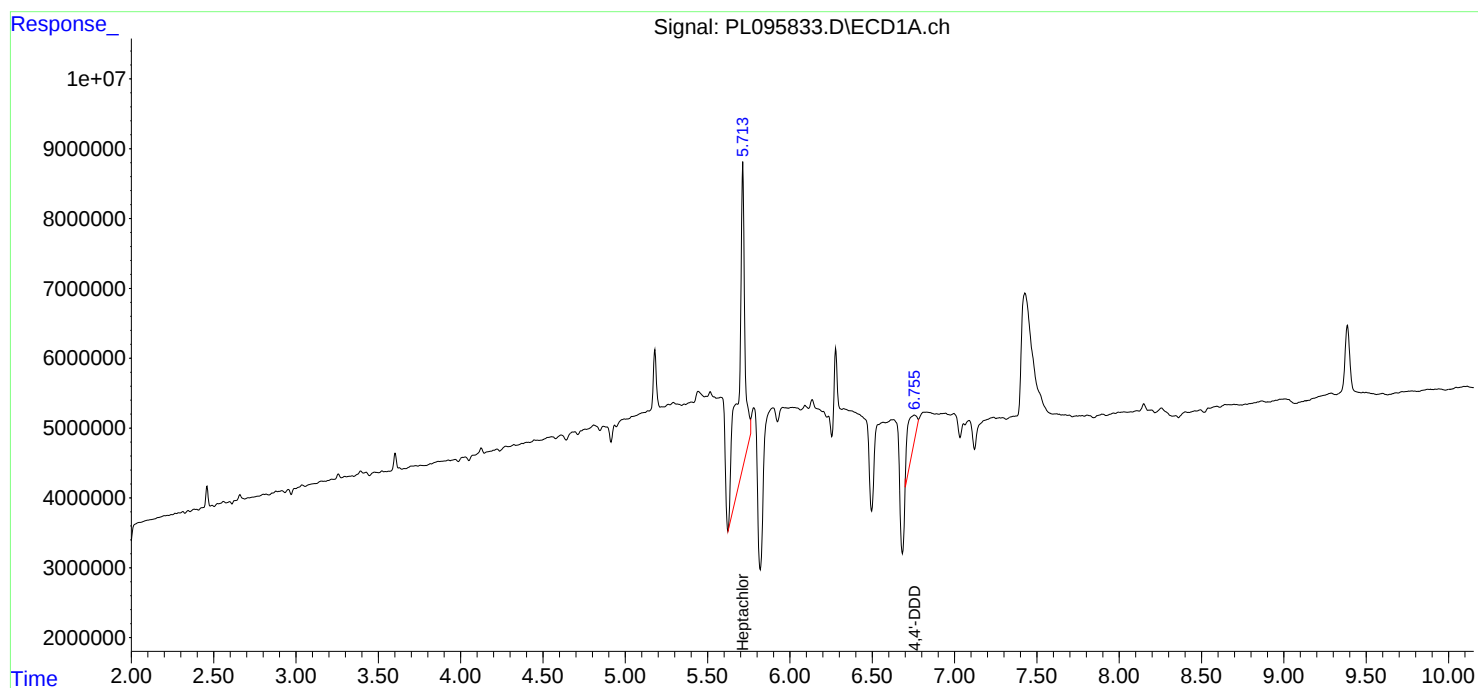


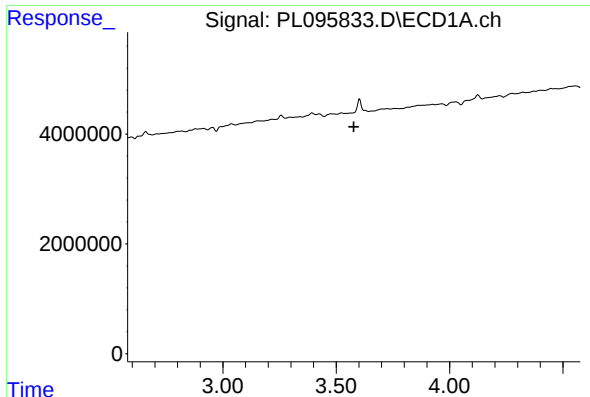

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.577 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

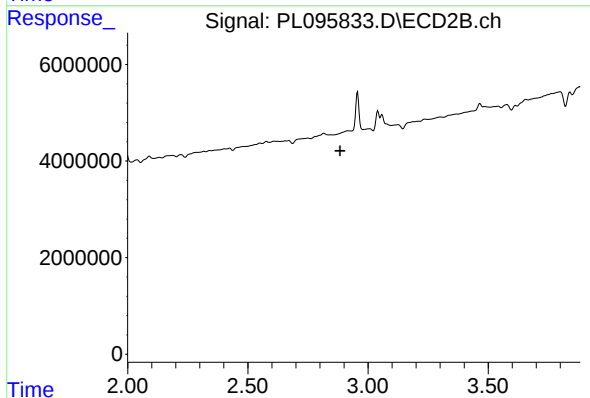


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 2.883 min
Response: 0
Conc: N.D.

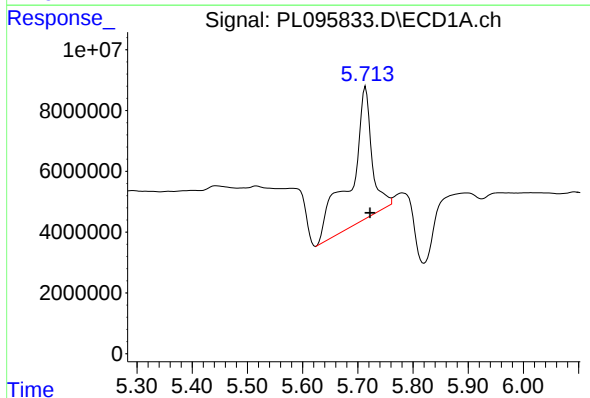


#8 Heptachlor epoxide

R.T.: 5.714 min
Delta R.T.: -0.008 min
Response: 115155099
Conc: 30.17 ng/ml

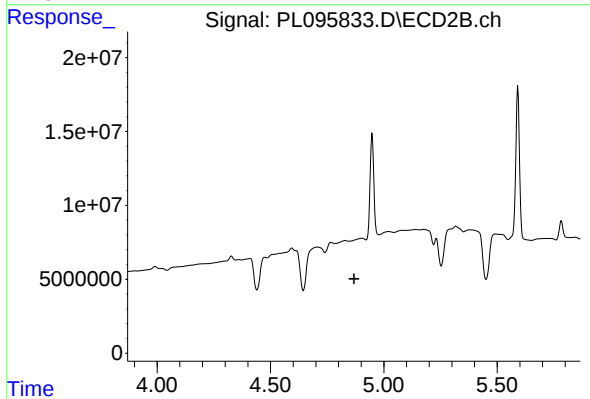

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.869 min
Response: 0
Conc: N.D.

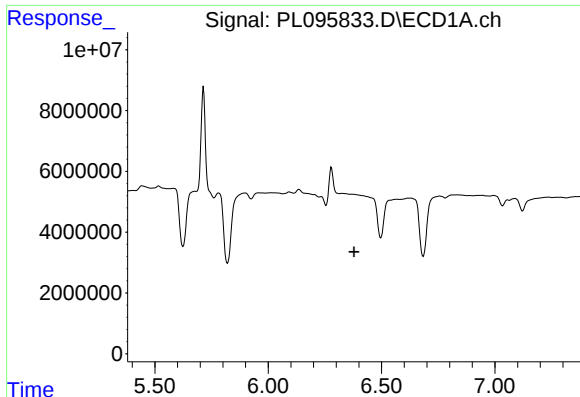

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.379 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

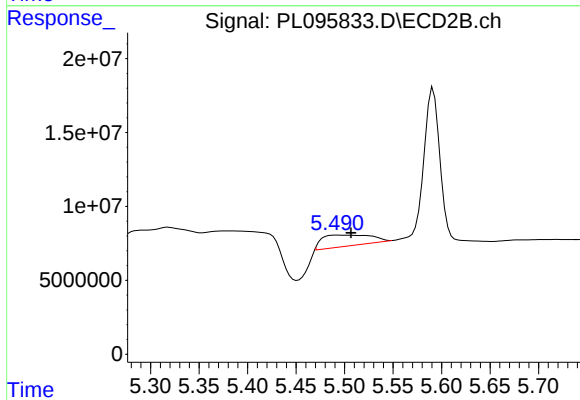


#13 Dieldrin

R.T.: 5.492 min
Delta R.T.: -0.015 min
Response: 26351013
Conc: 4.97 ng/ml

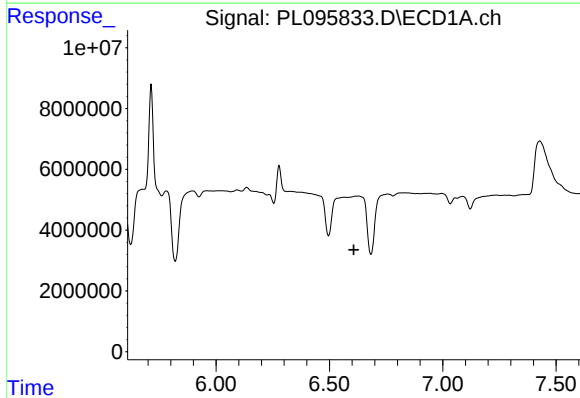


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.607 min
Response: 0
Conc: N.D.

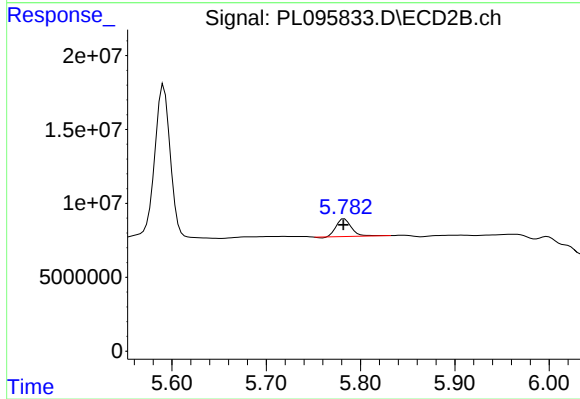

#14 Endrin


R.T.: 5.783 min
Delta R.T.: 0.001 min
Response: 13315671
Conc: 2.73 ng/ml

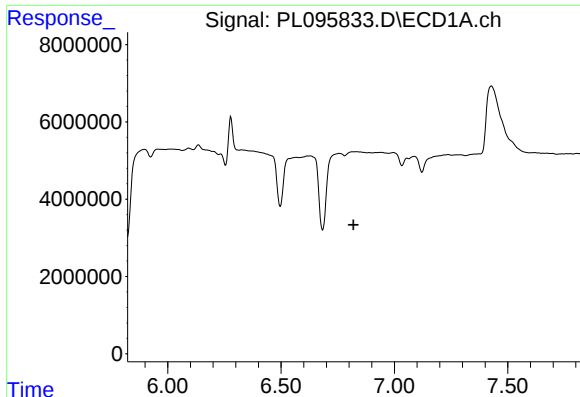

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.820 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

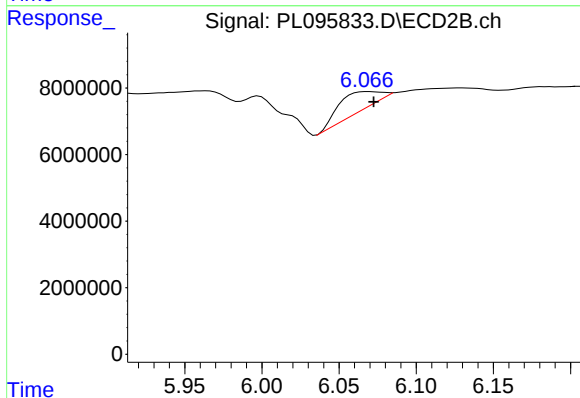


#15 Endosulfan II

R.T.: 6.069 min
Delta R.T.: -0.003 min
Response: 9842638
Conc: 2.07 ng/ml

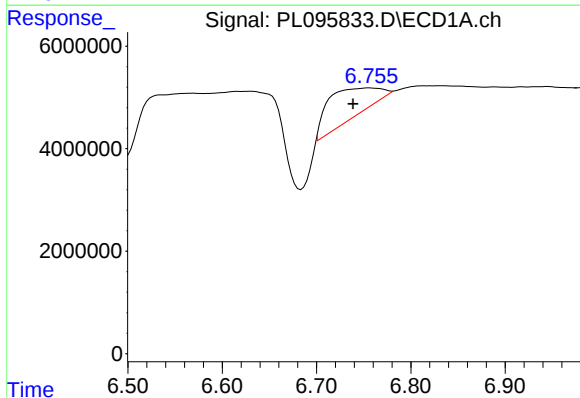


#16 4,4'-DDD

R.T.: 6.757 min
Delta R.T.: 0.018 min
Response: 20396600
Conc: 6.96 ng/ml

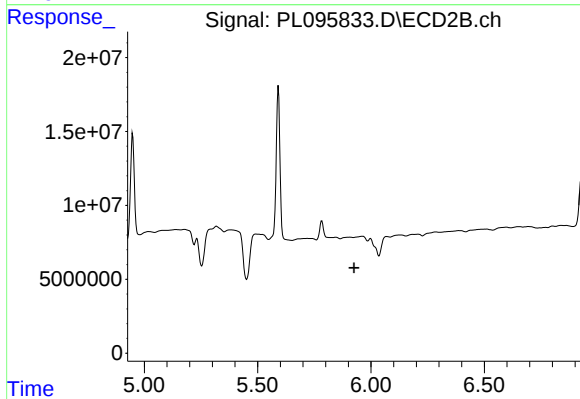

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.926 min
Response: 0
Conc: N.D.

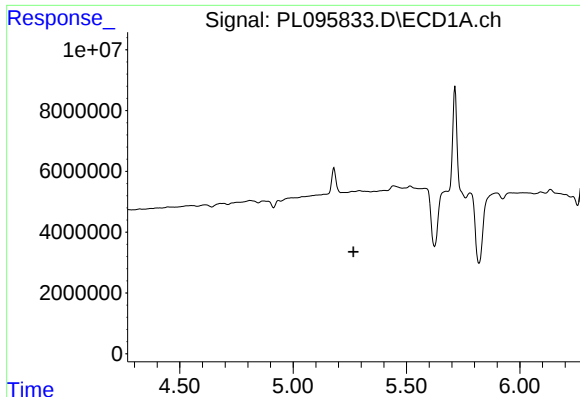

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.267 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

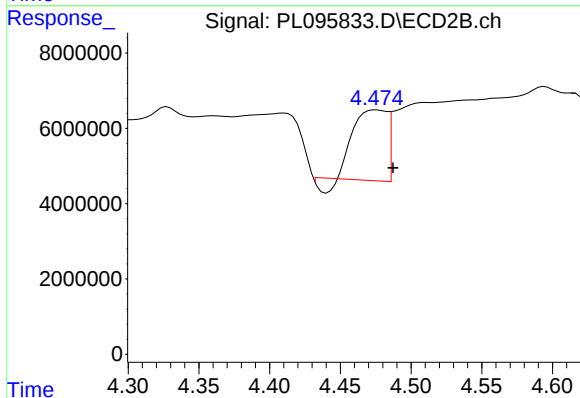


#24 Chlordane-2

R.T.: 4.475 min
Delta R.T.: -0.012 min
Response: 29069395
Conc: 130.50 ng/ml

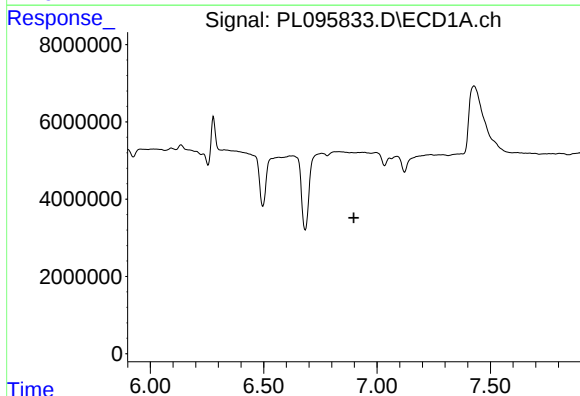


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.897 min
Response: 0
Conc: N.D.

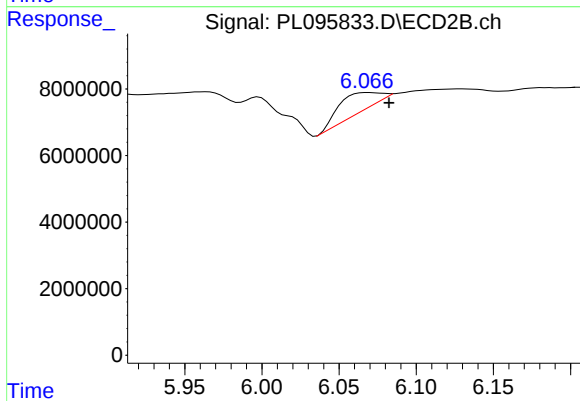

#27 Chlordane-5


R.T.: 6.069 min
Delta R.T.: -0.013 min
Response: 9842638
Conc: 38.61 ng/ml

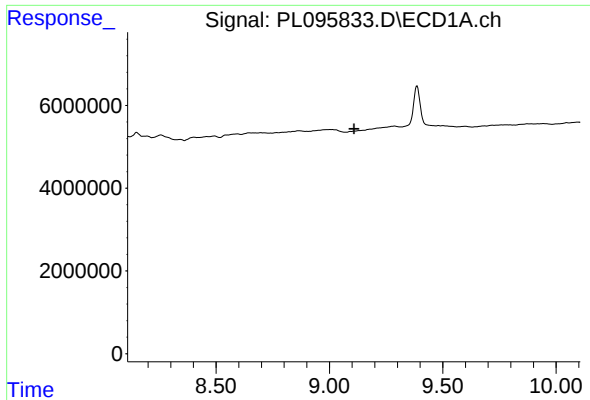

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.109 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

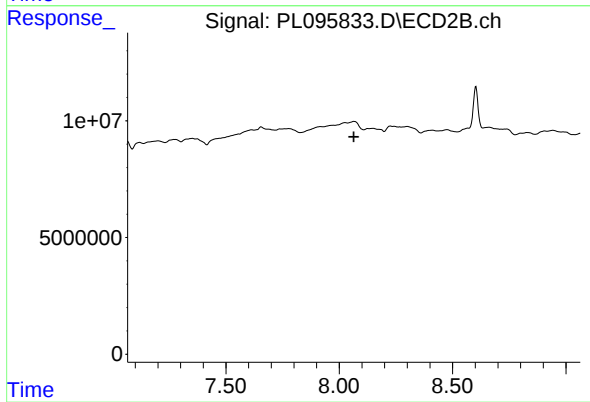

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.064 min
Response: 0
Conc: N.D.