

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060225\
 Data File : PL095834.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2025 09:20
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 21:51:42 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052125.M
 Quant Title : GC Extractables
 QLast Update : Thu May 22 06:29:30 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.572	2.884	72566125	84988745	22.998	21.714
28)	SA Decachlor...	9.102	8.060	52124158	87863976	22.121	20.086
Target Compounds							
8)	B Heptachlo...	5.708	0.000	18435811	0	4.830	N.D. #
10)	B gamma-Chl...	5.967	0.000	3429385	0	0.881	N.D. #
24)	Chlordane-2	0.000	4.473	0	5679851	N.D.	25.498 #
25)	Chlordane-3	5.967	0.000	3429385	0	4.640	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060225\
Data File : PL095834.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2025 09:20
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 21:51:42 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052125.M
Quant Title : GC Extractables
QLast Update : Thu May 22 06:29:30 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

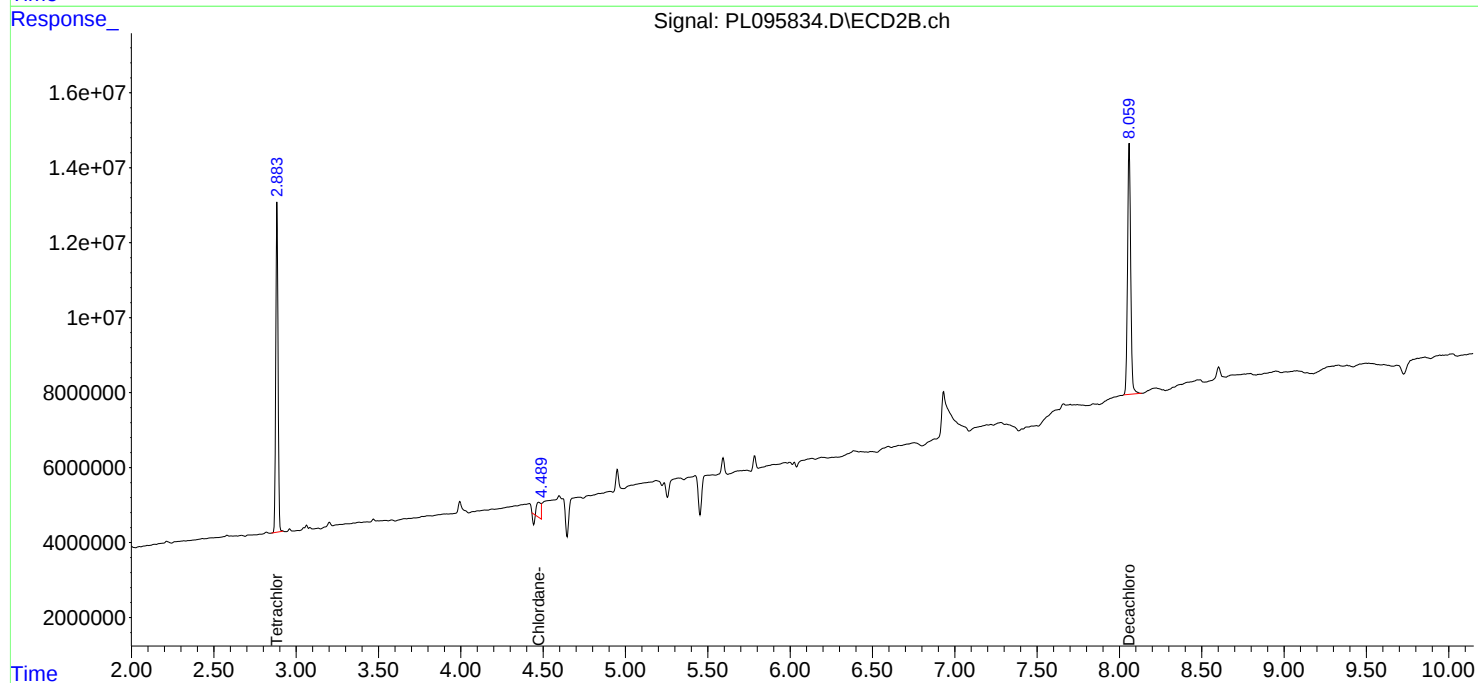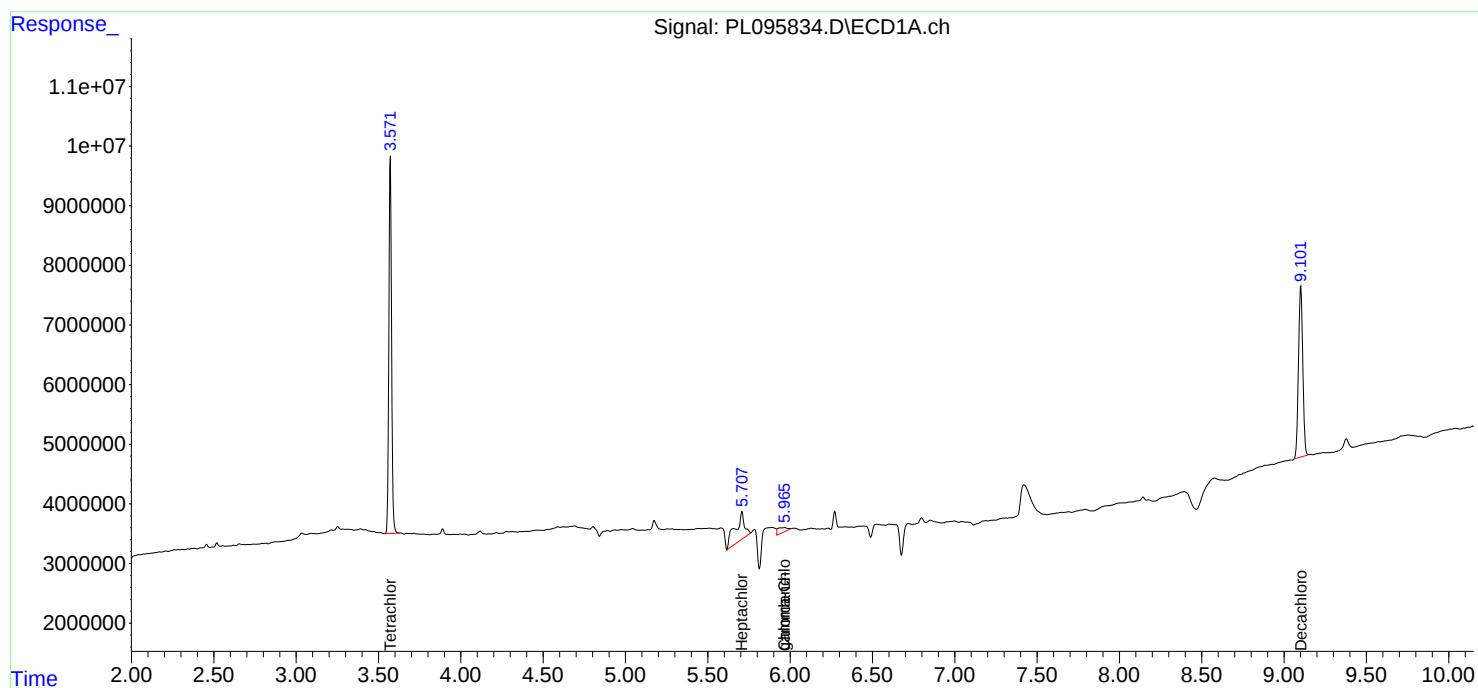


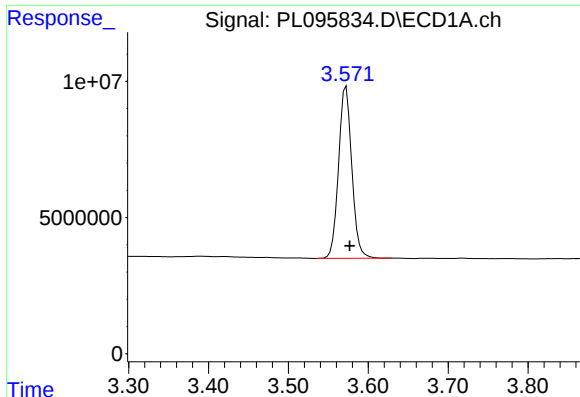

#1 Tetrachloro-m-xylene


R.T.: 3.572 min
Delta R.T.: -0.005 min
Response: 72566125
Conc: 23.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

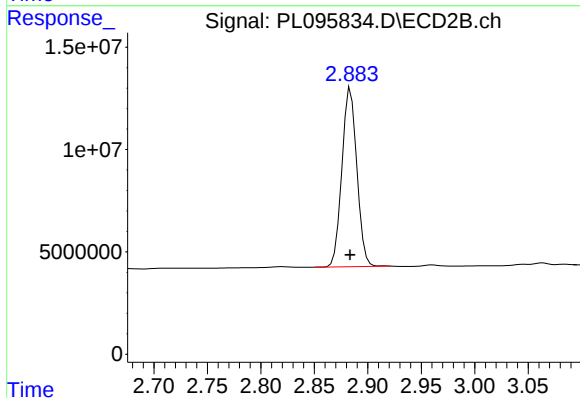


#1 Tetrachloro-m-xylene

R.T.: 2.884 min
Delta R.T.: 0.000 min
Response: 84988745
Conc: 21.71 ng/ml

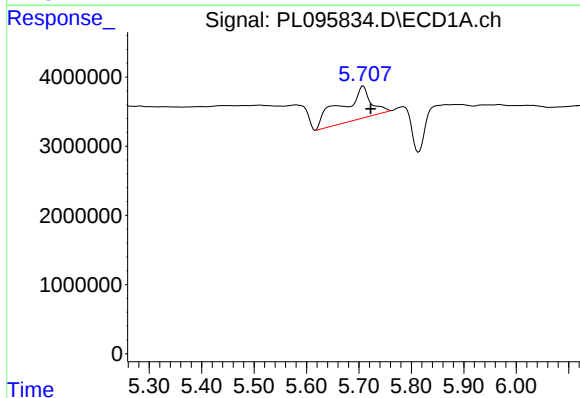


#8 Heptachlor epoxide

R.T.: 5.708 min
Delta R.T.: -0.014 min
Response: 18435811
Conc: 4.83 ng/ml

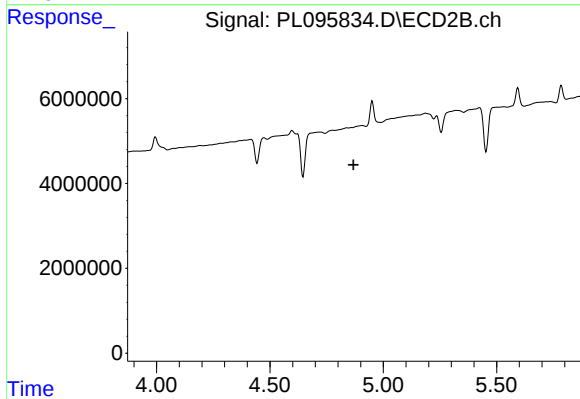

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.869 min
Response: 0
Conc: N.D.

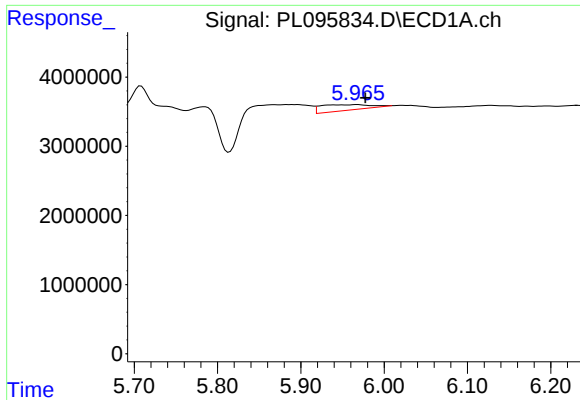

#10 gamma-Chlordane


R.T.: 5.967 min
Delta R.T.: -0.010 min
Response: 3429385
Conc: 0.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

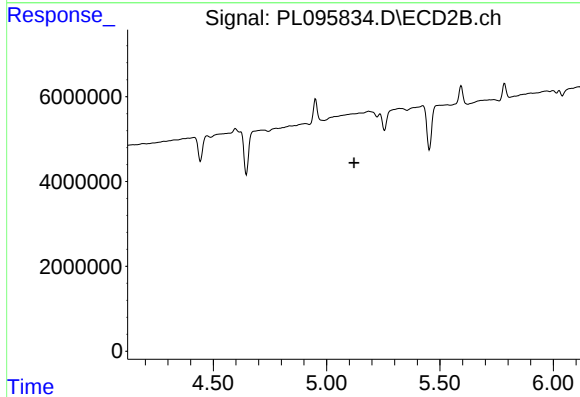


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.122 min
Response: 0
Conc: N.D.

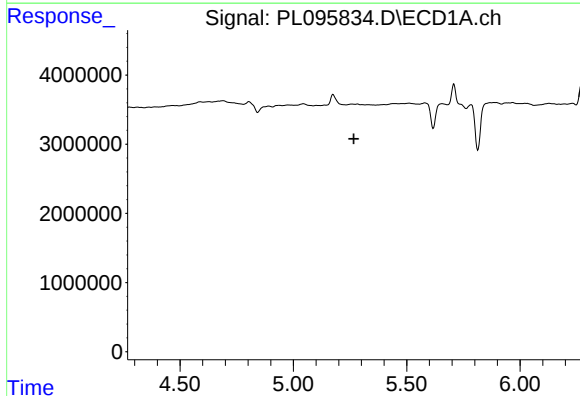


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.267 min
Response: 0
Conc: N.D.

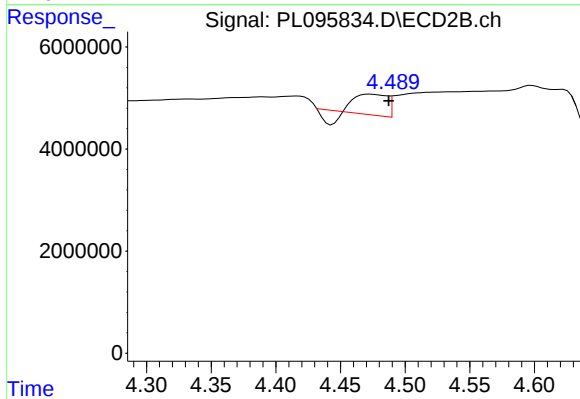

#24 Chlordane-2


R.T.: 4.473 min
Delta R.T.: -0.014 min
Response: 5679851
Conc: 25.50 ng/ml

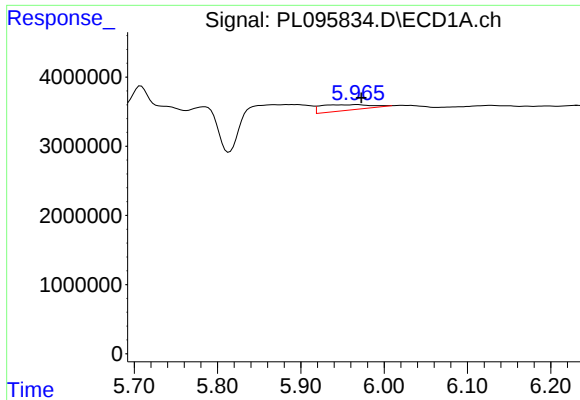

#25 Chlordane-3


R.T.: 5.967 min
Delta R.T.: -0.005 min
Response: 3429385
Conc: 4.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

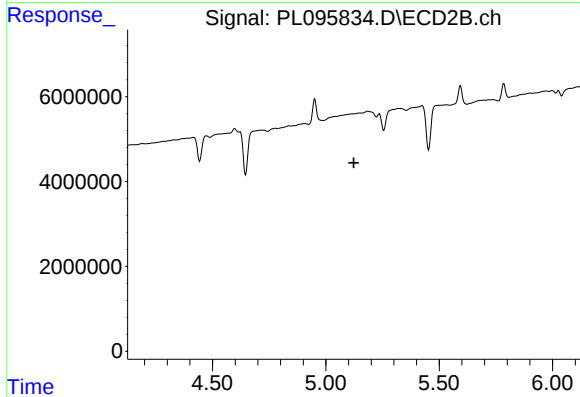


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.123 min
Response: 0
Conc: N.D.

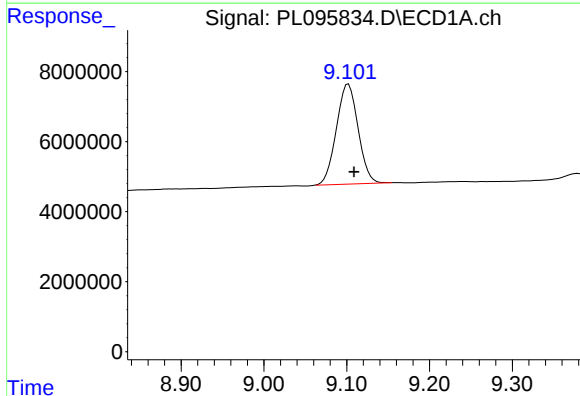

#28 Decachlorobiphenyl

R.T.: 9.102 min
Delta R.T.: -0.007 min
Response: 52124158
Conc: 22.12 ng/ml

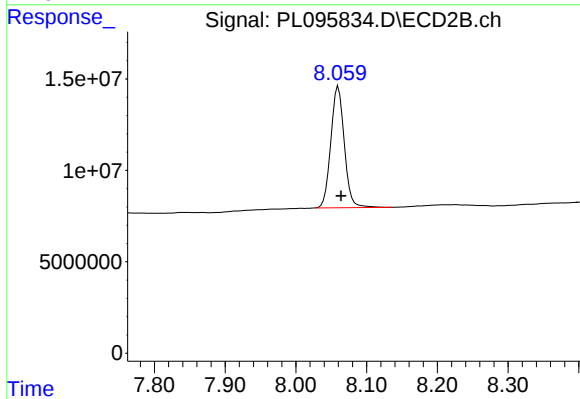

#28 Decachlorobiphenyl

R.T.: 8.060 min
Delta R.T.: -0.004 min
Response: 87863976
Conc: 20.09 ng/ml