

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060225\
 Data File : PL095847.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2025 16:52
 Operator : AR\AJ
 Sample : Q2173-13
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-50

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 21:54:01 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052125.M
 Quant Title : GC Extractables
 QLast Update : Thu May 22 06:29:30 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.573	2.885	27652688	31987019	8.764	8.173
28)	SA Decachlor...	9.100	8.060	11936303	24579127	5.066	5.619
Target Compounds							
10)	B gamma-Chl...	0.000	5.147f	0	4477507	N.D.	0.852 #
11)	B alpha-Chl...	6.059	0.000	6147441	0	1.557	N.D. #
12)	B 4,4'-DDE	6.223	5.371	9381212	15338381	2.558	2.860
17)	MA 4,4'-DDT	0.000	6.174	0	7593936	N.D.	1.588 #
22)	Mirex	8.145	0.000	19469313	0	8.415	N.D. #
25)	Chlordane-3	0.000	5.147f	0	4477507	N.D.	6.795 #
26)	Chlordane-4	6.059	0.000	6147441	0	6.840	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060225\
Data File : PL095847.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2025 16:52
Operator : AR\AJ
Sample : Q2173-13
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-50

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 21:54:01 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052125.M
Quant Title : GC Extractables
QLast Update : Thu May 22 06:29:30 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

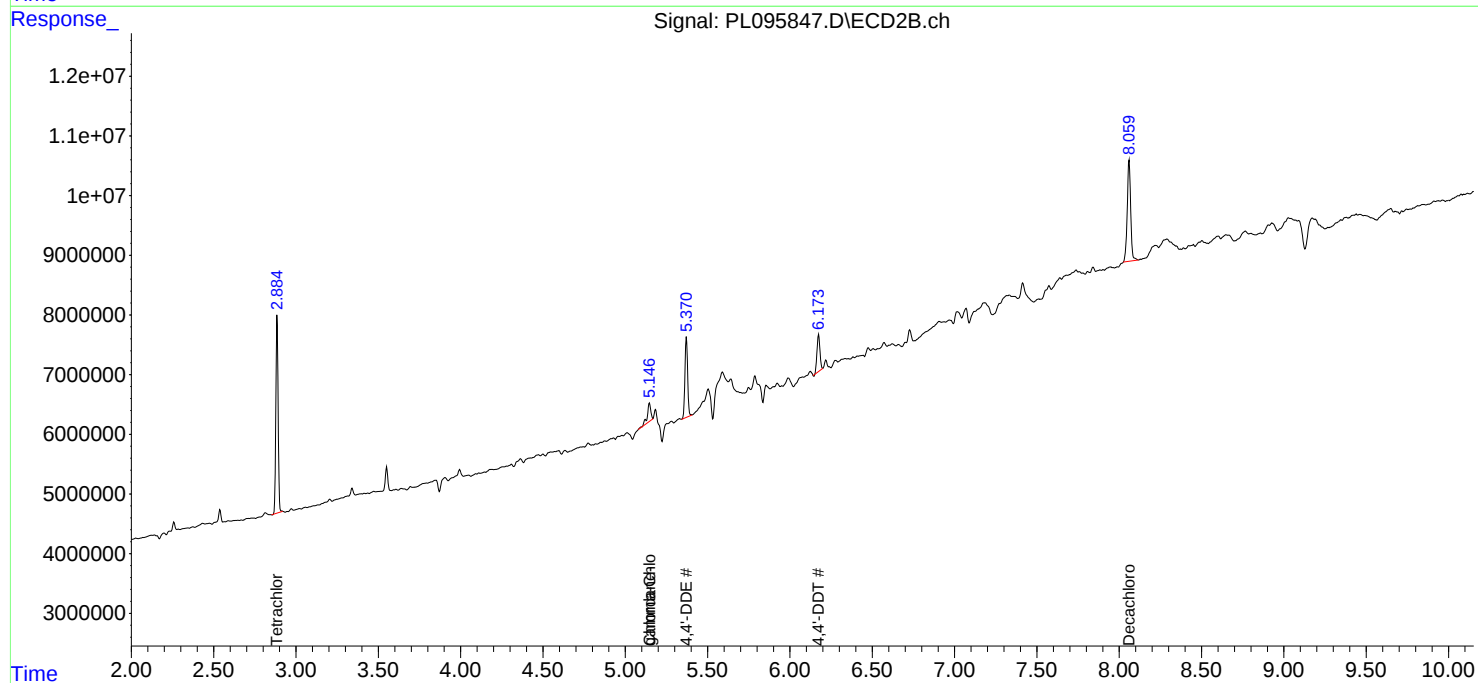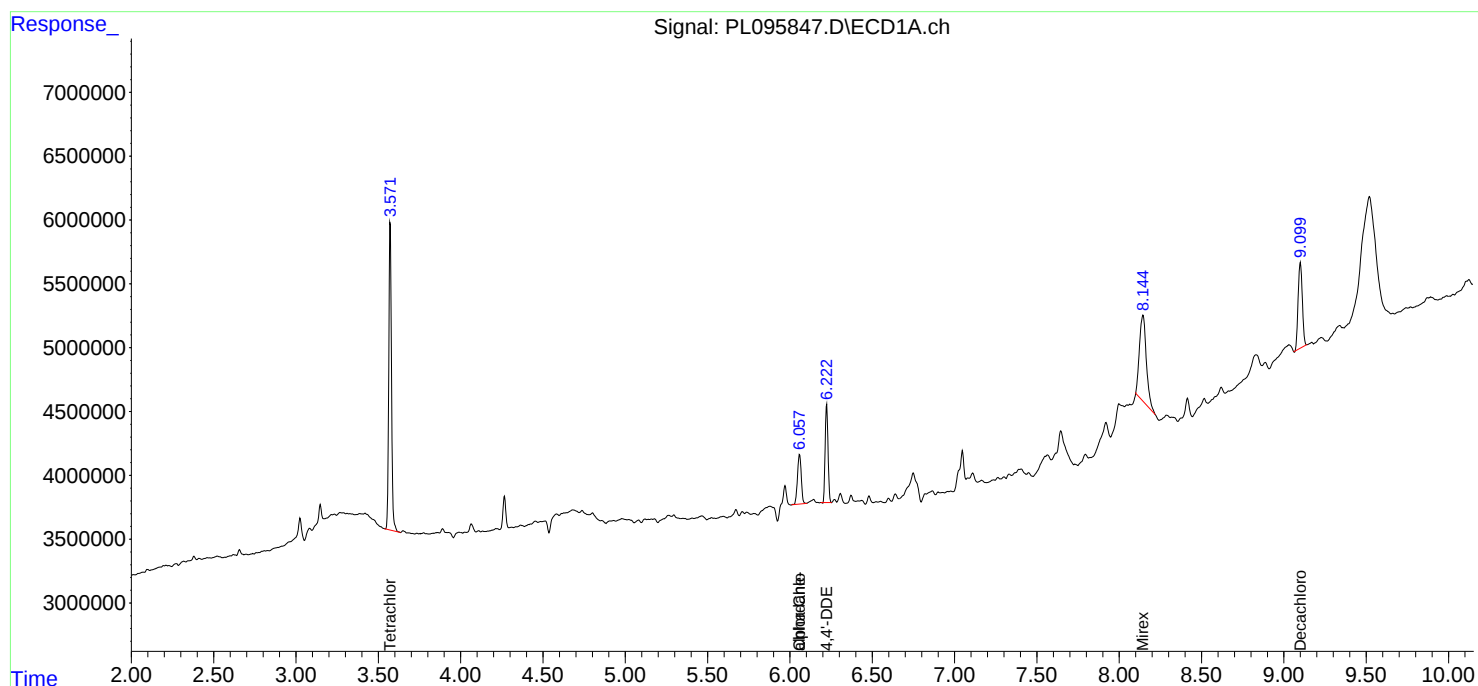


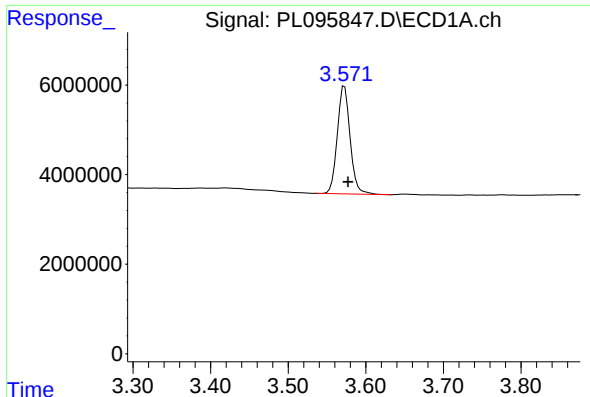

#1 Tetrachloro-m-xylene


R.T.: 3.573 min
Delta R.T.: -0.004 min
Response: 27652688
Conc: 8.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-50

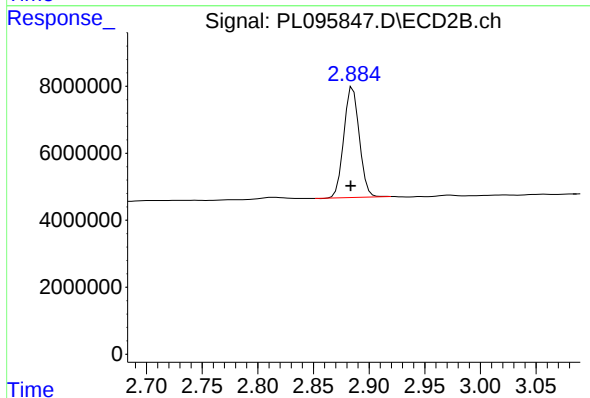


#1 Tetrachloro-m-xylene

R.T.: 2.885 min
Delta R.T.: 0.002 min
Response: 31987019
Conc: 8.17 ng/ml

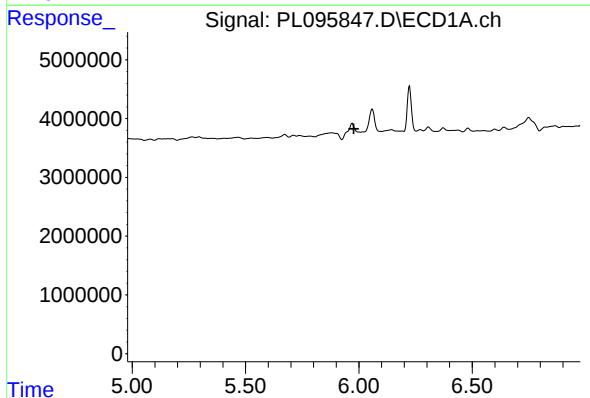


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.977 min
Response: 0
Conc: N.D.

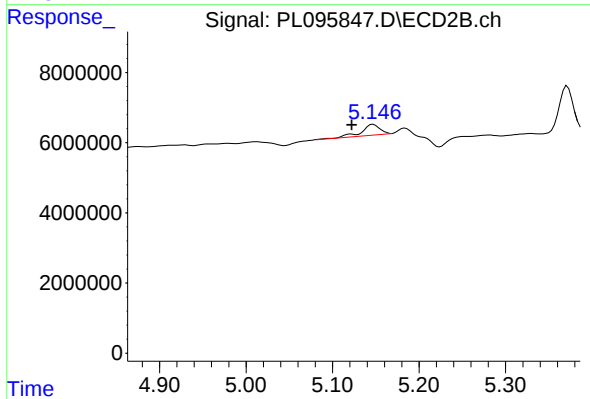

#10 gamma-Chlordane


R.T.: 5.147 min
Delta R.T.: 0.025 min
Response: 4477507
Conc: 0.85 ng/ml

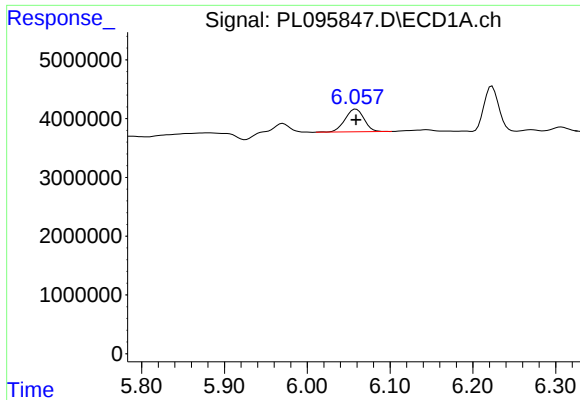

#11 alpha-Chlordane


R.T.: 6.059 min
Delta R.T.: 0.000 min
Response: 6147441
Conc: 1.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-50

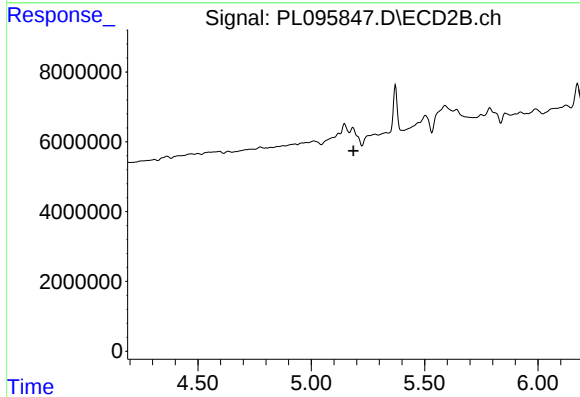


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.186 min
Response: 0
Conc: N.D.

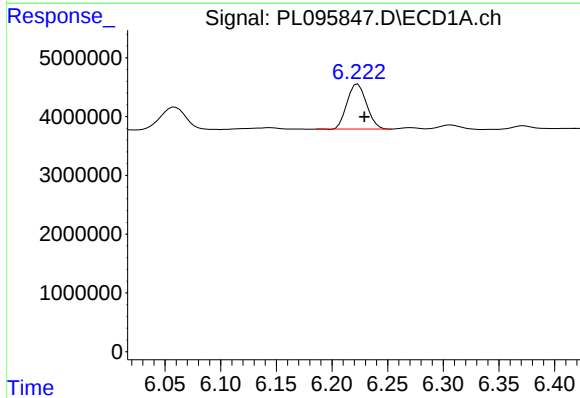


#12 4,4'-DDE

R.T.: 6.223 min
Delta R.T.: -0.006 min
Response: 9381212
Conc: 2.56 ng/ml

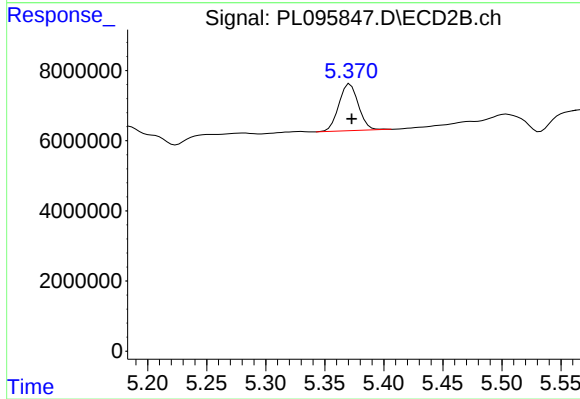

#12 4,4'-DDE


R.T.: 5.371 min
Delta R.T.: -0.002 min
Response: 15338381
Conc: 2.86 ng/ml

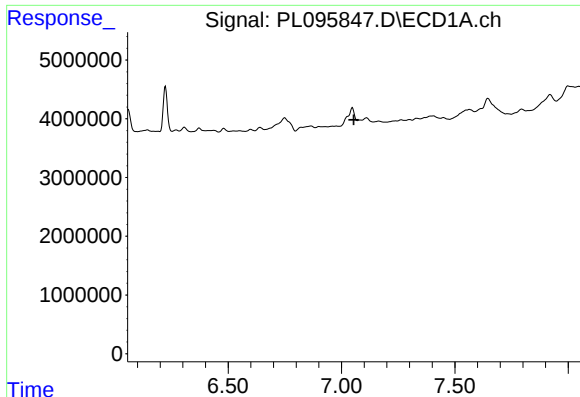

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 7.054 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-50

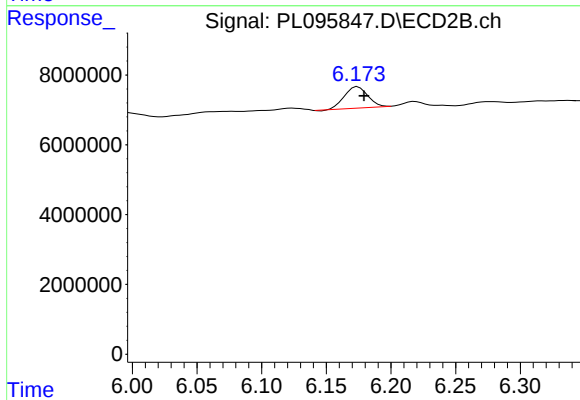


#17 4,4'-DDT

R.T.: 6.174 min
Delta R.T.: -0.005 min
Response: 7593936
Conc: 1.59 ng/ml

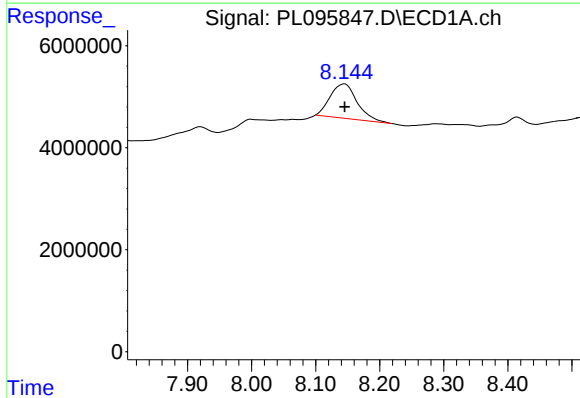


#22 Mirex

R.T.: 8.145 min
Delta R.T.: 0.000 min
Response: 19469313
Conc: 8.41 ng/ml

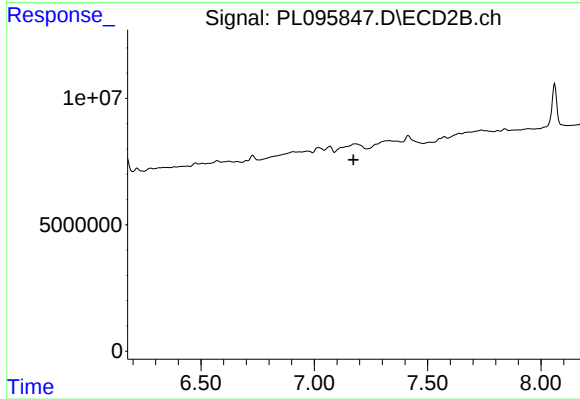

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 7.173 min
Response: 0
Conc: N.D.

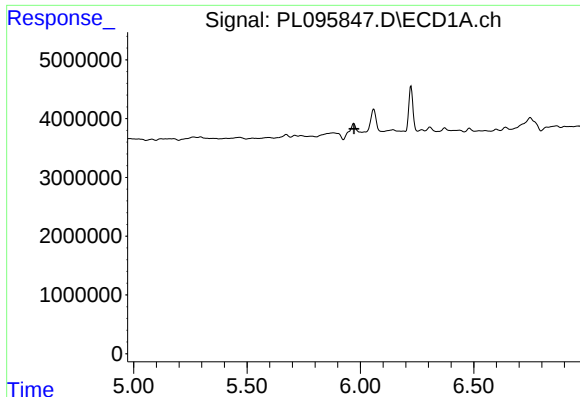

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.973 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-50

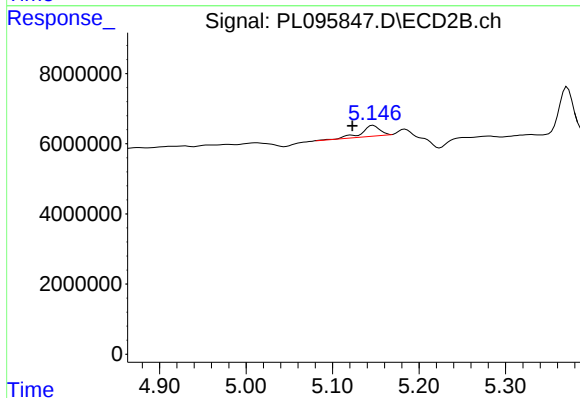


#25 Chlordane-3

R.T.: 5.147 min
Delta R.T.: 0.024 min
Response: 4477507
Conc: 6.80 ng/ml

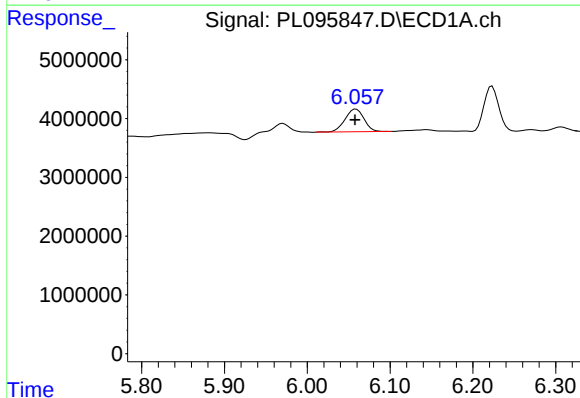


#26 Chlordane-4

R.T.: 6.059 min
Delta R.T.: 0.001 min
Response: 6147441
Conc: 6.84 ng/ml

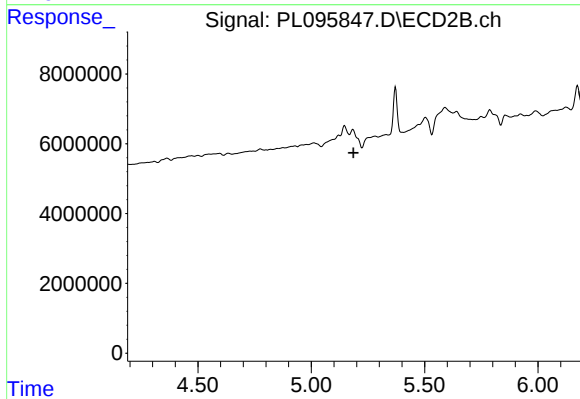

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.187 min
Response: 0
Conc: N.D.

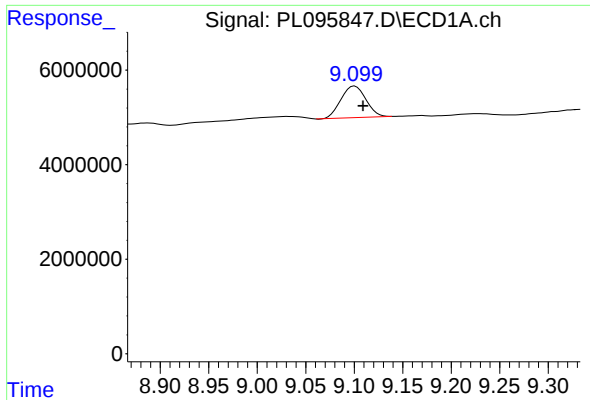

#28 Decachlorobiphenyl

R.T.: 9.100 min
Delta R.T.: -0.009 min
Response: 11936303
Conc: 5.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-50

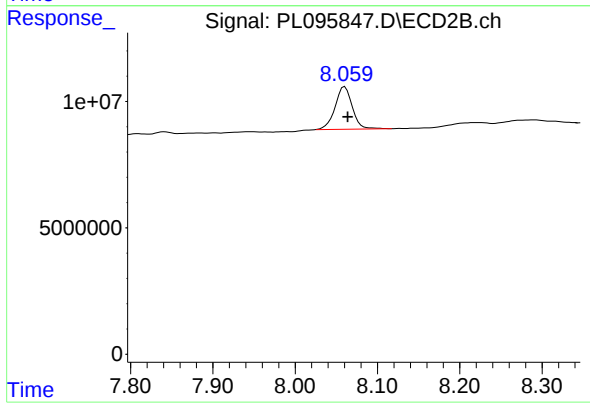

#28 Decachlorobiphenyl

R.T.: 8.060 min
Delta R.T.: -0.003 min
Response: 24579127
Conc: 5.62 ng/ml