

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060319\
 Data File : PL049211.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2019 10:35
 Operator : SM\AJ
 Sample : K3124-09
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-25-D

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 01:47:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
 Quant Title : GC Extractables
 QLast Update : Fri May 31 01:35:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.325	3.937	238.5E6	62257824	21.641	21.550
28)	SA Decachlor...	7.994	8.974	222.6E6	63144327	17.507	18.907
Target Compounds							
15)	B Endosulfa...	0.000	6.860f	0	425026	N.D.	0.140 #
22)	Mirex	7.127	0.000	2136523	0	0.203	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060319\
Data File : PL049211.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2019 10:35
Operator : SM\AJ
Sample : K3124-09
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
TP-25-D

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 01:47:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
Quant Title : GC Extractables
QLast Update : Fri May 31 01:35:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

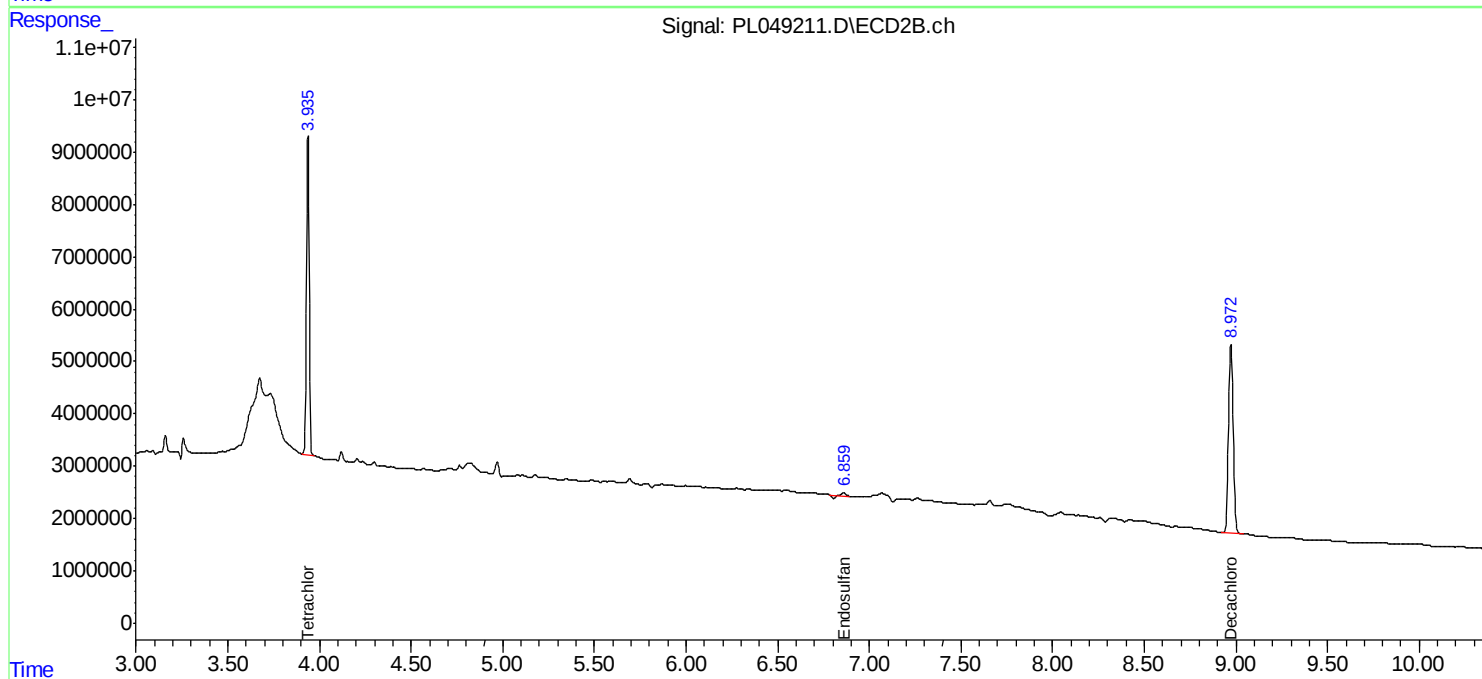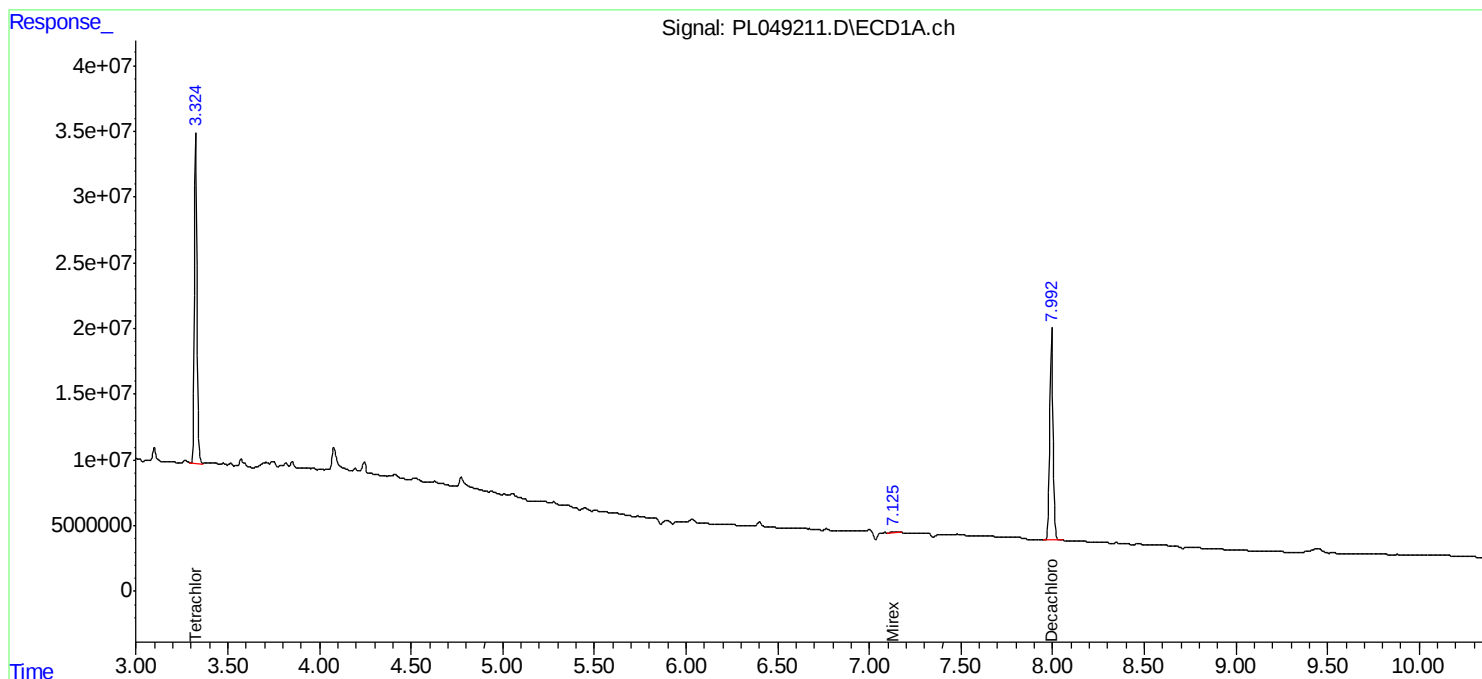


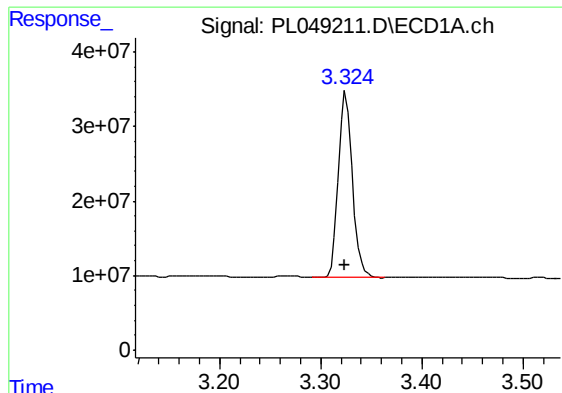

#1 Tetrachloro-m-xylene


R.T.: 3.325 min
Delta R.T.: 0.001 min
Response: 238459612
Conc: 21.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-25-D

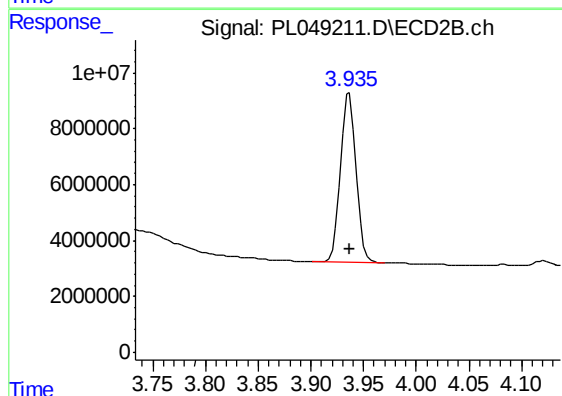


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: 0.000 min
Response: 62257824
Conc: 21.55 ng/ml

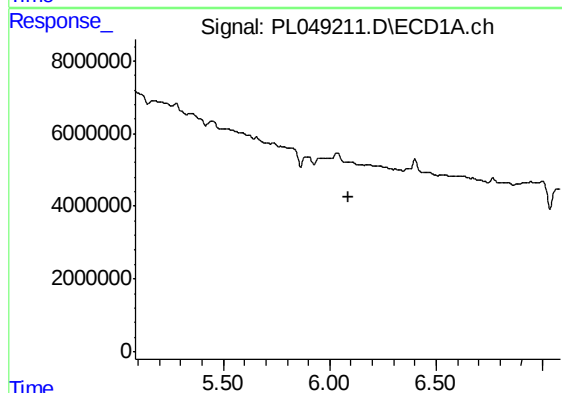


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.085 min
Response: 0
Conc: N.D.

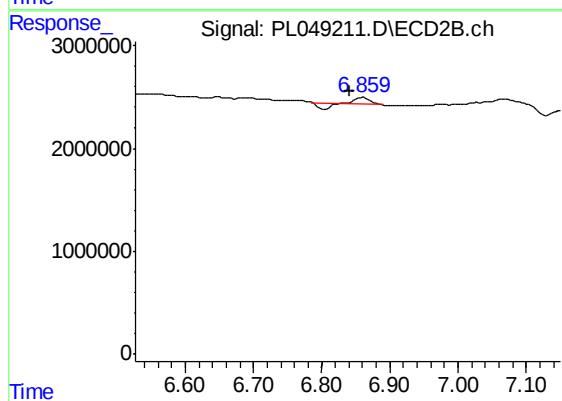

#15 Endosulfan II


R.T.: 6.860 min
Delta R.T.: 0.020 min
Response: 425026
Conc: 0.14 ng/ml

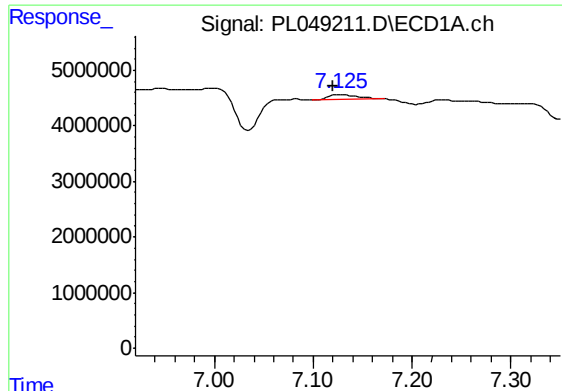

#22 Mirex


R.T.: 7.127 min
Delta R.T.: 0.007 min
Response: 2136523
Conc: 0.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-25-D

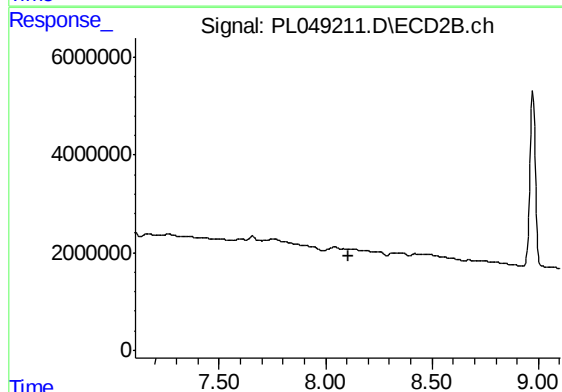


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 8.107 min
Response: 0
Conc: N.D.

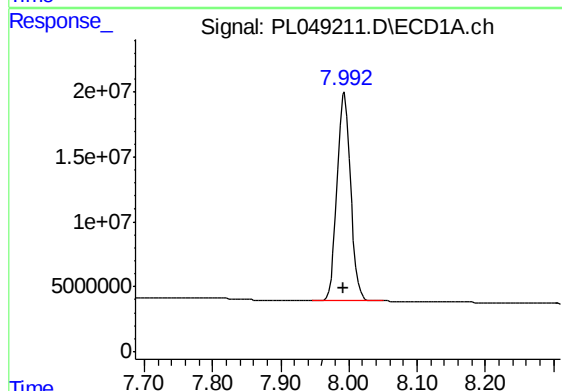

#28 Decachlorobiphenyl

R.T.: 7.994 min
Delta R.T.: 0.001 min
Response: 222610035
Conc: 17.51 ng/ml

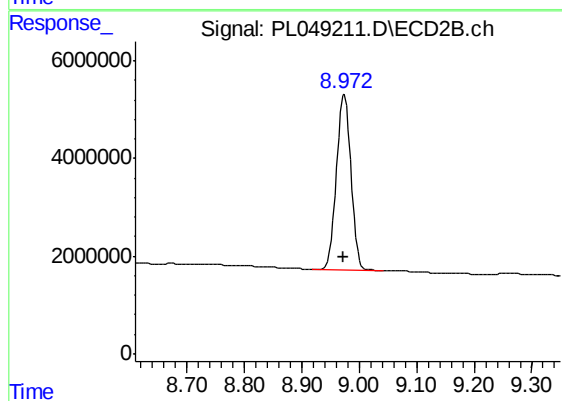

#28 Decachlorobiphenyl

R.T.: 8.974 min
Delta R.T.: 0.001 min
Response: 63144327
Conc: 18.91 ng/ml