

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060319\
 Data File : PL049257.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2019 22:03
 Operator : SM\AJ
 Sample : K3135-01
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PSTDCCC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 02:01:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
 Quant Title : GC Extractables
 QLast Update : Fri May 31 01:35:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.323	3.936	151.9E6	42679078	13.784	14.773
28)	SA Decachlor...	7.990	8.971	151.0E6	51227746	11.873	15.339 #
Target Compounds							
10)	B gamma-Chl...	5.229f	0.000	24899875	0	1.560	N.D. #
11)	B alpha-Chl...	0.000	6.108	0	6957879	N.D.	2.006 #
25)	Chlordane-3	5.229f	0.000	24899875	0	13.954	N.D. #
26)	Chlordane-4	0.000	6.108	0	6957879	N.D.	12.279 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060319\
Data File : PL049257.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2019 22:03
Operator : SM\AJ
Sample : K3135-01
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 02:01:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
Quant Title : GC Extractables
QLast Update : Fri May 31 01:35:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

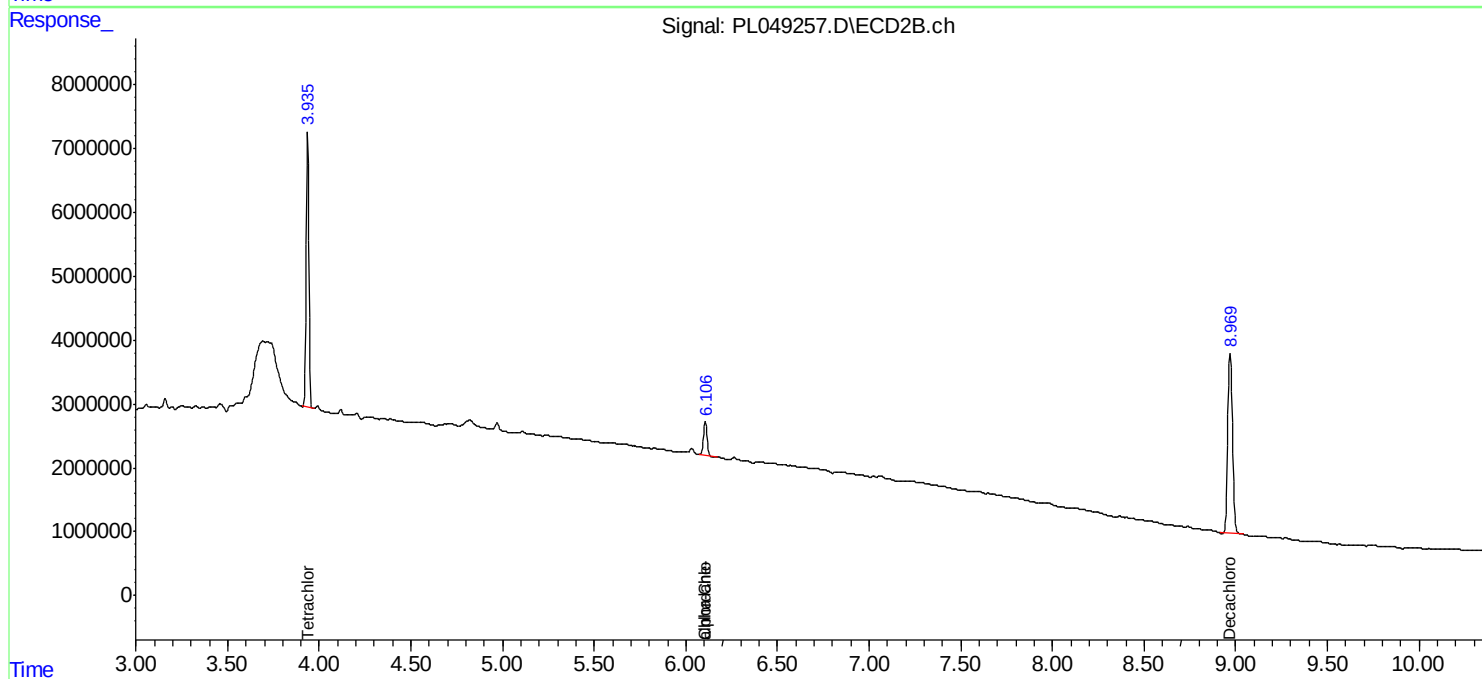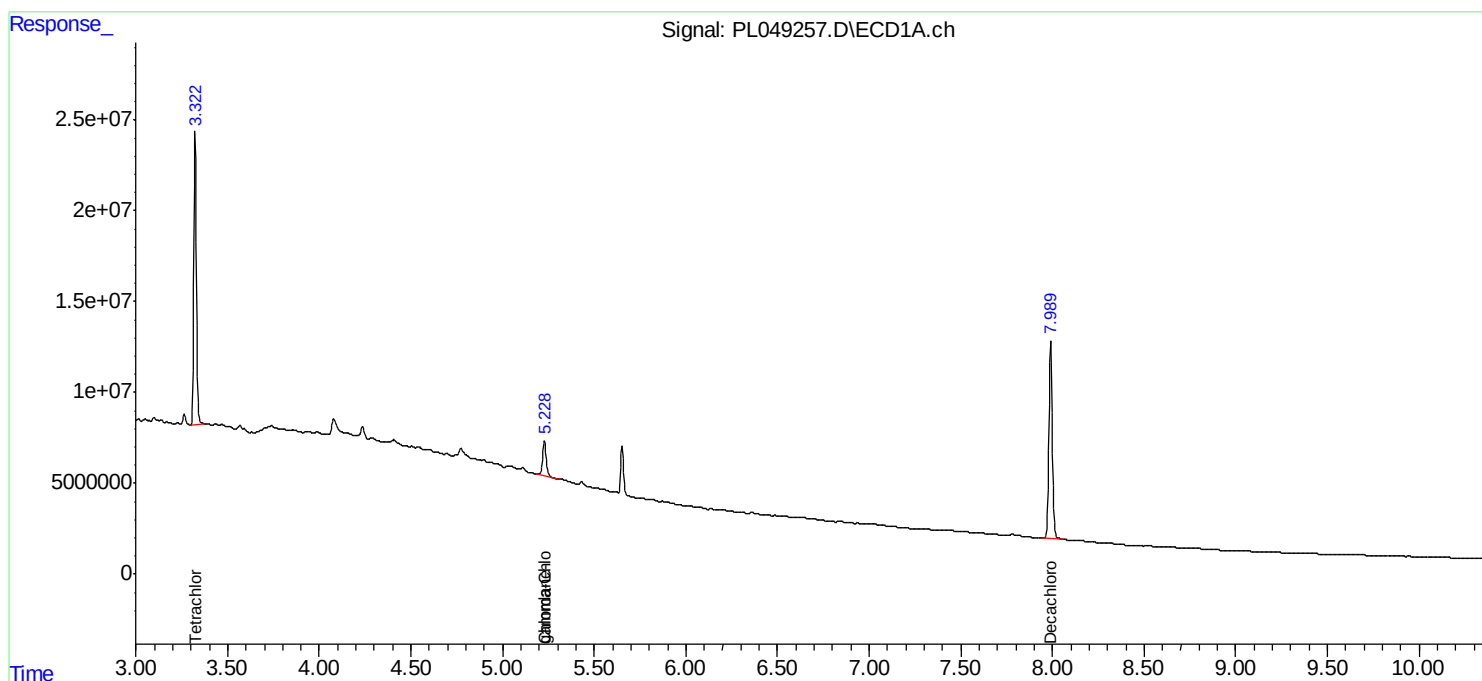


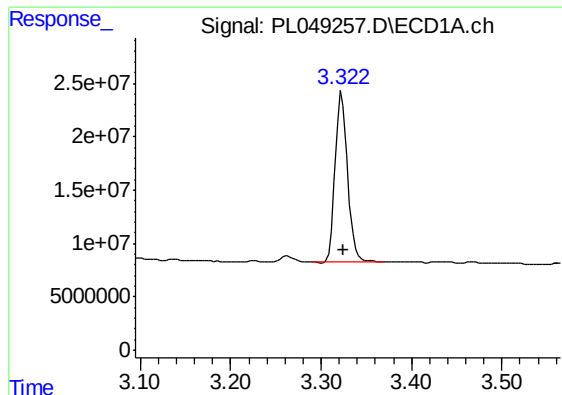

#1 Tetrachloro-m-xylene


R.T.: 3.323 min
Delta R.T.: 0.000 min
Response: 151880410
Conc: 13.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

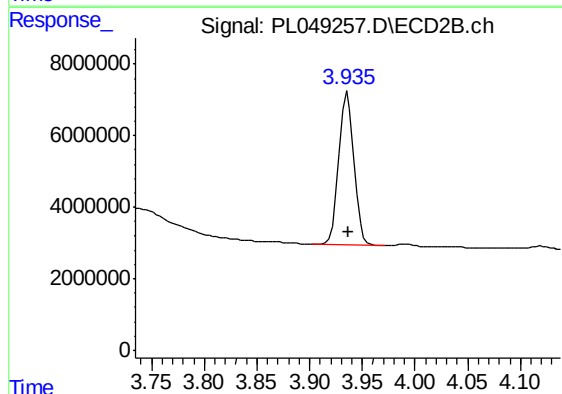


#1 Tetrachloro-m-xylene

R.T.: 3.936 min
Delta R.T.: 0.000 min
Response: 42679078
Conc: 14.77 ng/ml

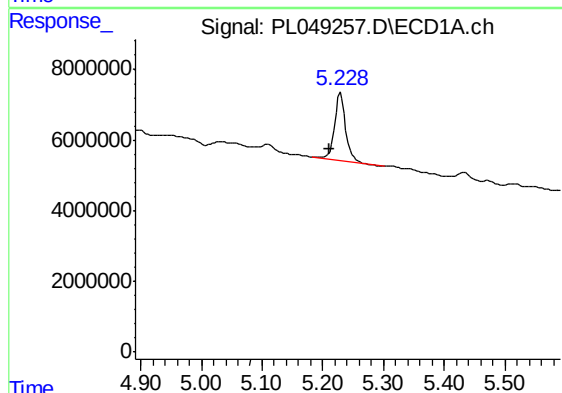


#10 gamma-Chlordane

R.T.: 5.229 min
Delta R.T.: 0.019 min
Response: 24899875
Conc: 1.56 ng/ml

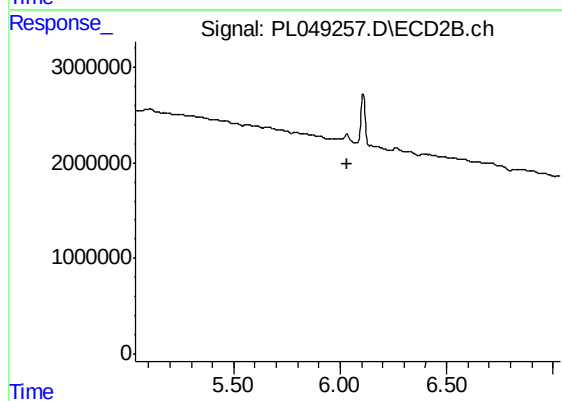

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.035 min
Response: 0
Conc: N.D.

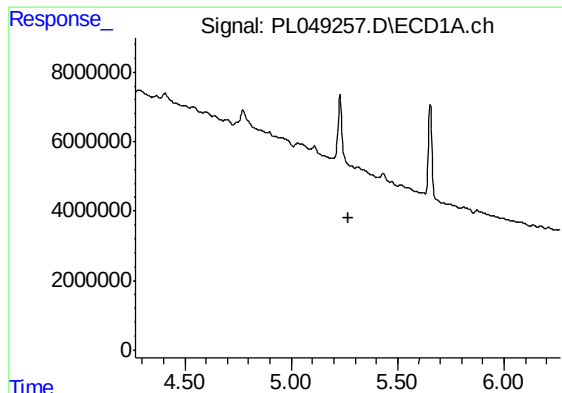

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.267 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

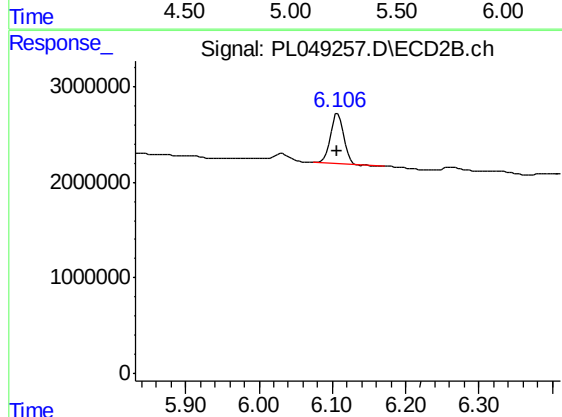


#11 alpha-Chlordane

R.T.: 6.108 min
Delta R.T.: 0.000 min
Response: 6957879
Conc: 2.01 ng/ml

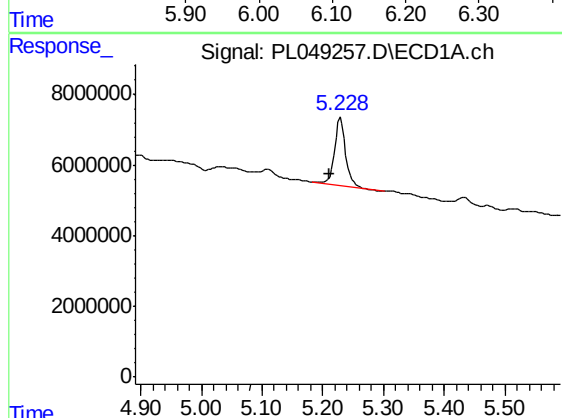


#25 Chlordane-3

R.T.: 5.229 min
Delta R.T.: 0.018 min
Response: 24899875
Conc: 13.95 ng/ml

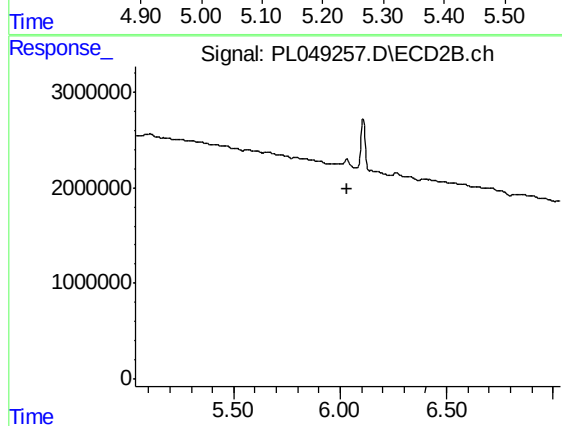

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.035 min
Response: 0
Conc: N.D.

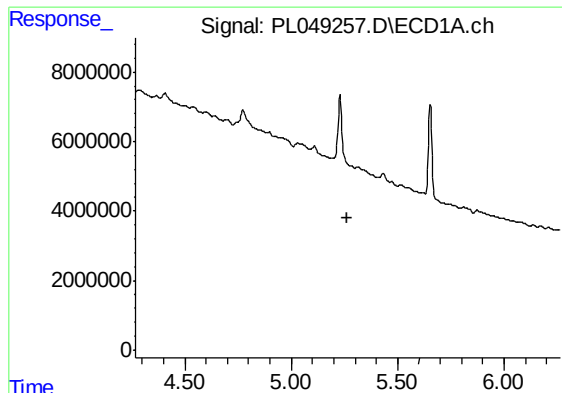

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.266 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

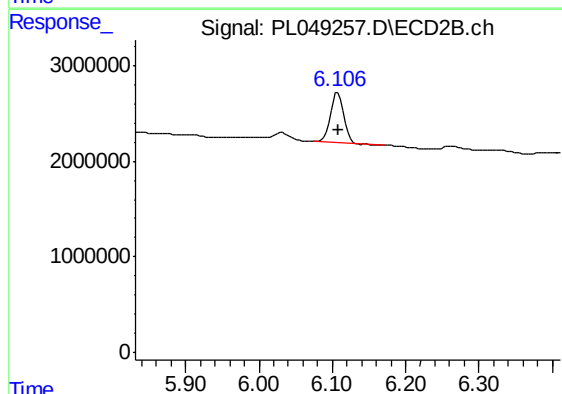


#26 Chlordane-4

R.T.: 6.108 min
Delta R.T.: 0.000 min
Response: 6957879
Conc: 12.28 ng/ml

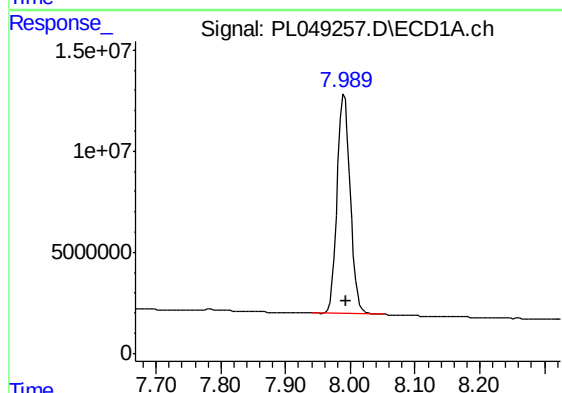

#28 Decachlorobiphenyl

R.T.: 7.990 min
Delta R.T.: -0.002 min
Response: 150973367
Conc: 11.87 ng/ml

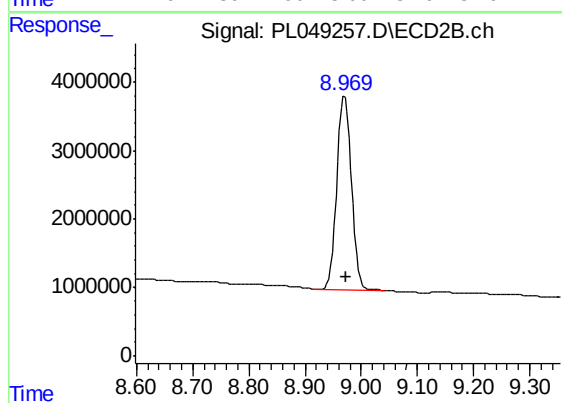

#28 Decachlorobiphenyl

R.T.: 8.971 min
Delta R.T.: -0.002 min
Response: 51227746
Conc: 15.34 ng/ml