

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060320\
 Data File : PL059094.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2020 12:22
 Operator : AJ\MA
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 13:07:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060320.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 03 13:07:22 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.520	4.072	91913746	123.8E6	50.000	50.000
28)	SA Decachlor...	8.297	9.184	76842063	109.1E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.401	5.077	25150935	50516357	500.000	500.000
24)	Chlordane-2	4.904	5.547	26090176	47704985	500.000	500.000
25)	Chlordane-3	5.477	6.197	73884035	187.5E6	500.000	500.000
26)	Chlordane-4	5.535	6.272	59981072	227.5E6	500.000	500.000
27)	Chlordane-5	6.374	7.080	24881589	39571078	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060320\
Data File : PL059094.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2020 12:22
Operator : AJ\MA
Sample : PCHLORICC500
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 13:07:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060320.M
Quant Title : GC Extractables
QLast Update : Wed Jun 03 13:07:22 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

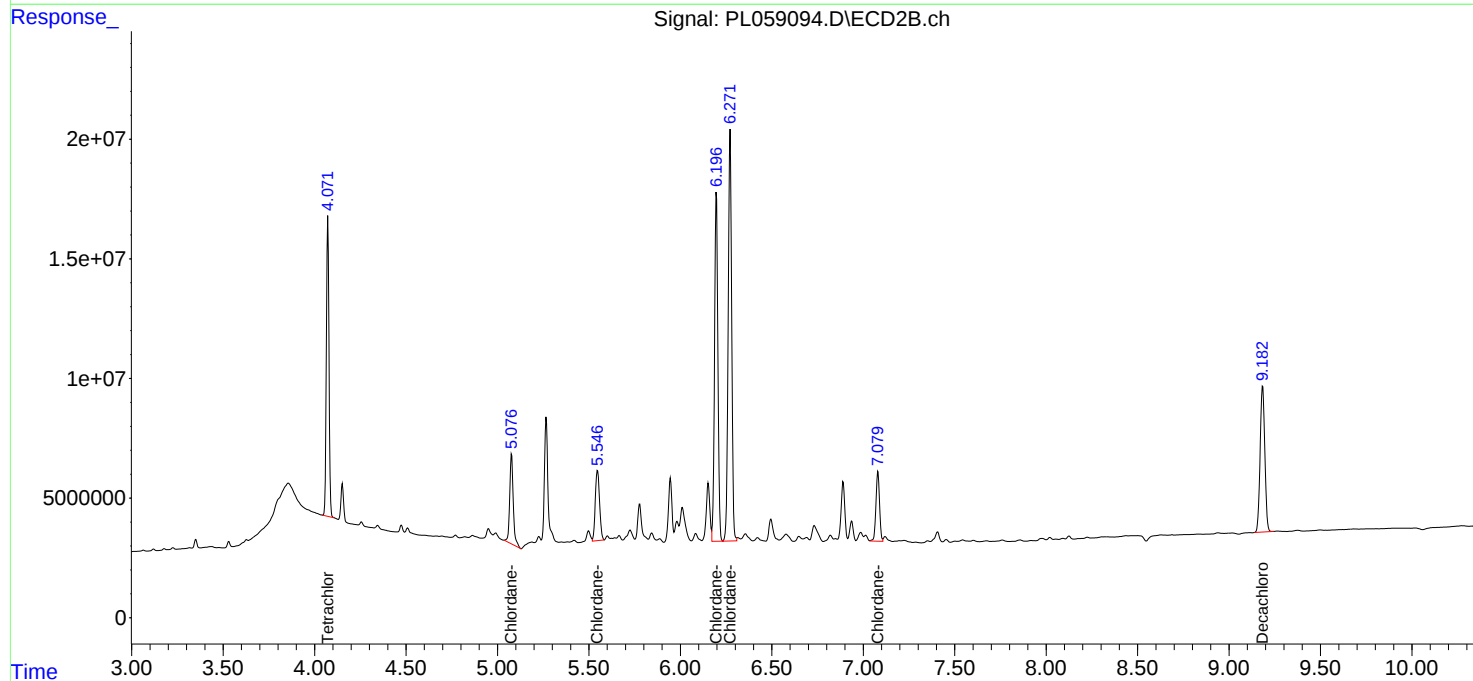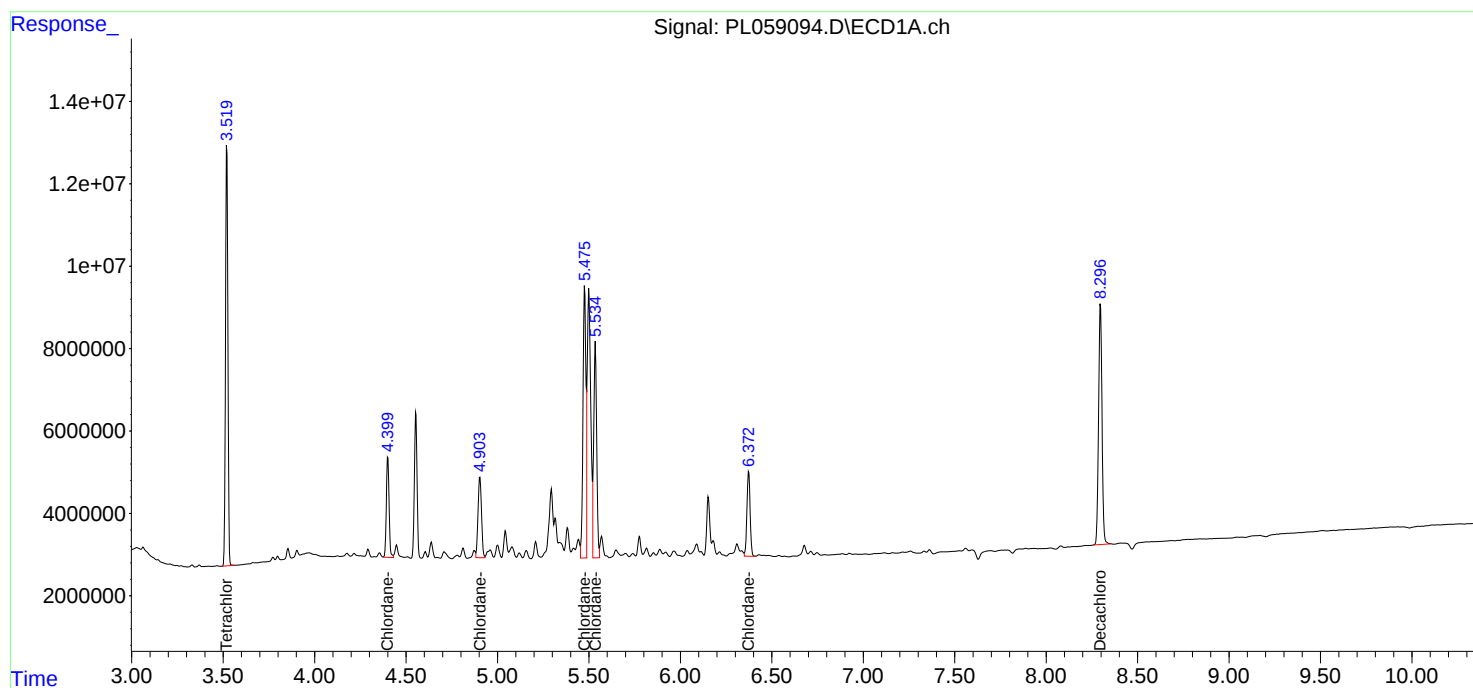


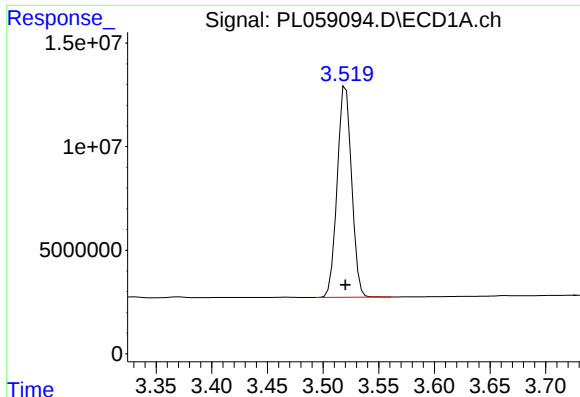

#1 Tetrachloro-m-xylene


R.T.: 3.520 min
Delta R.T.: 0.000 min
Response: 91913746
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

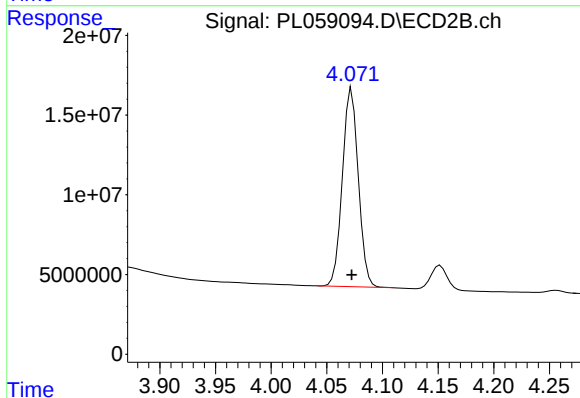


#1 Tetrachloro-m-xylene

R.T.: 4.072 min
Delta R.T.: 0.000 min
Response: 123805093
Conc: 50.00 ng/ml

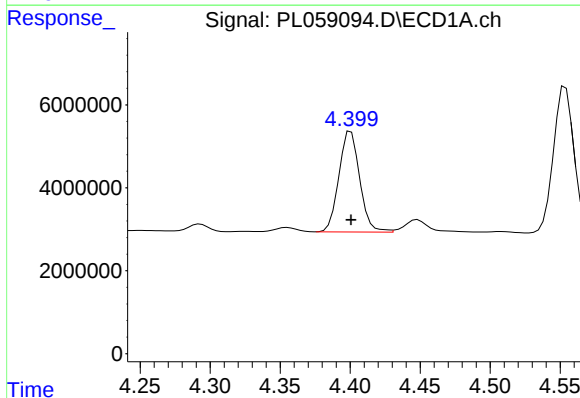


#23 Chlordane-1

R.T.: 4.401 min
Delta R.T.: 0.000 min
Response: 25150935
Conc: 500.00 ng/ml

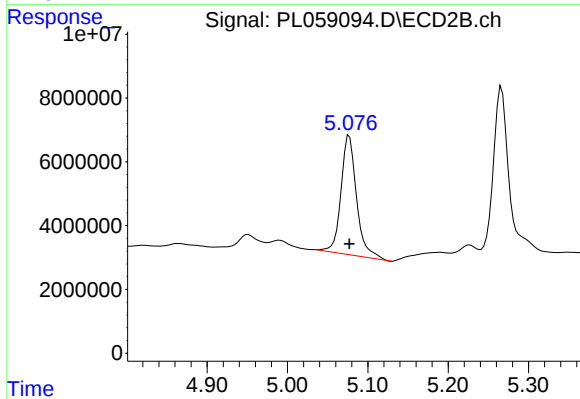

#23 Chlordane-1


R.T.: 5.077 min
Delta R.T.: 0.000 min
Response: 50516357
Conc: 500.00 ng/ml

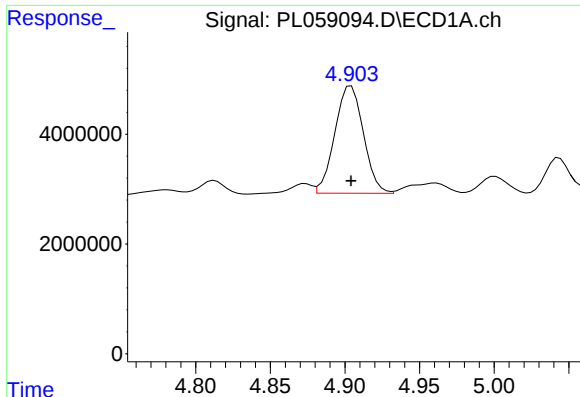

#24 Chlordane-2


R.T.: 4.904 min
Delta R.T.: 0.000 min
Response: 26090176
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

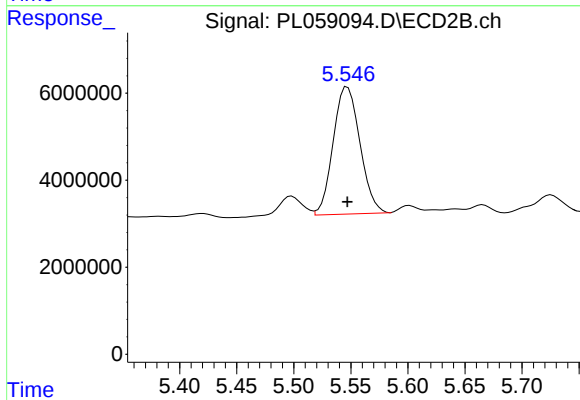


#24 Chlordane-2

R.T.: 5.547 min
Delta R.T.: 0.000 min
Response: 47704985
Conc: 500.00 ng/ml

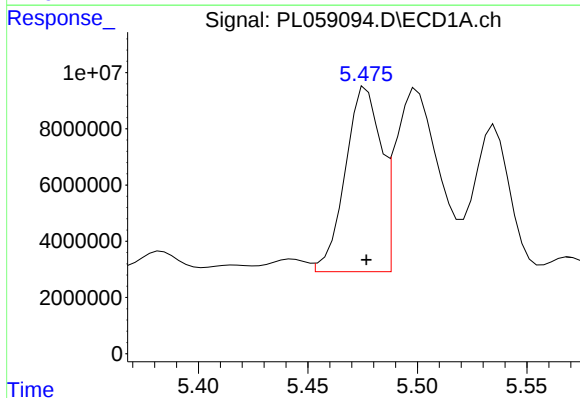


#25 Chlordane-3

R.T.: 5.477 min
Delta R.T.: 0.000 min
Response: 73884035
Conc: 500.00 ng/ml

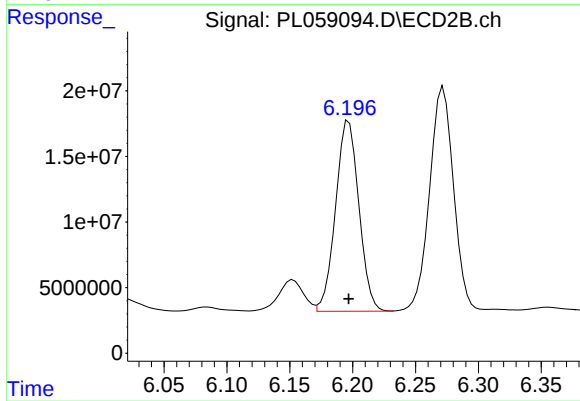

#25 Chlordane-3


R.T.: 6.197 min
Delta R.T.: 0.000 min
Response: 187495080
Conc: 500.00 ng/ml

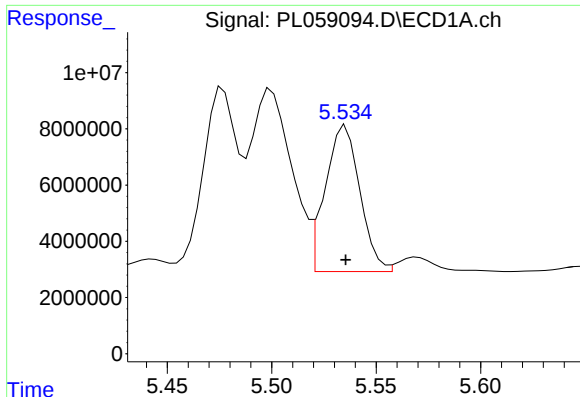

#26 Chlordane-4


R.T.: 5.535 min
Delta R.T.: 0.000 min
Response: 59981072
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

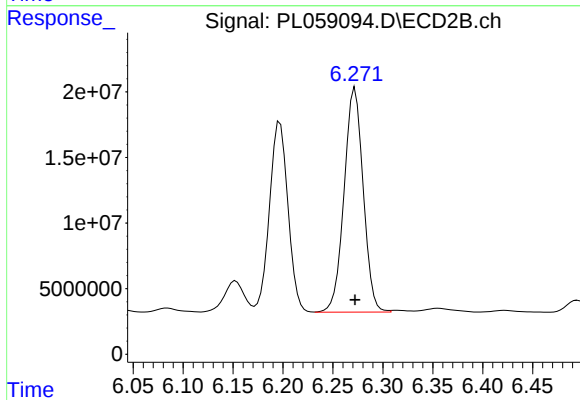


#26 Chlordane-4

R.T.: 6.272 min
Delta R.T.: 0.000 min
Response: 227523070
Conc: 500.00 ng/ml

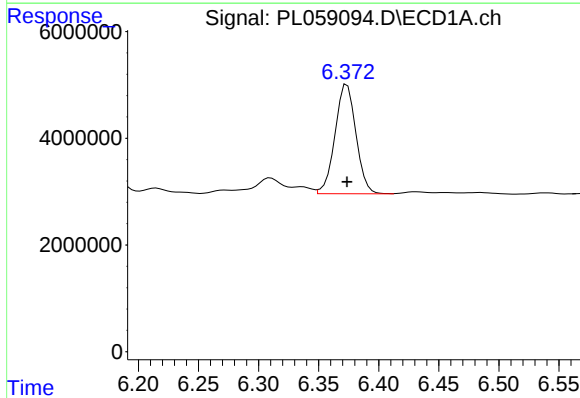


#27 Chlordane-5

R.T.: 6.374 min
Delta R.T.: 0.000 min
Response: 24881589
Conc: 500.00 ng/ml

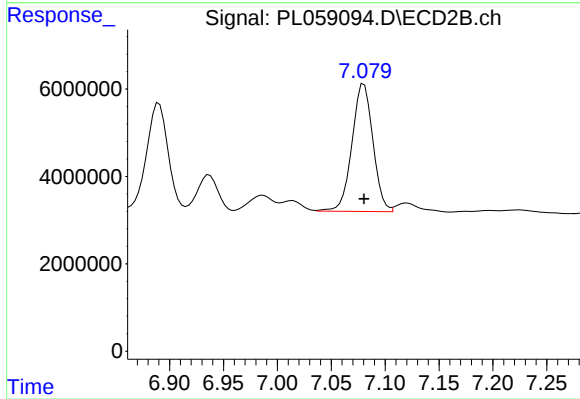

#27 Chlordane-5


R.T.: 7.080 min
Delta R.T.: 0.000 min
Response: 39571078
Conc: 500.00 ng/ml

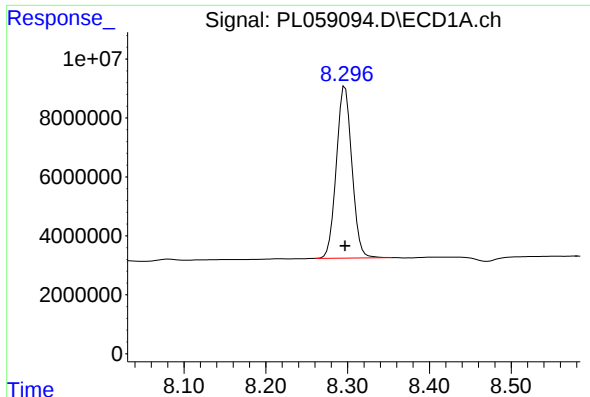

#28 Decachlorobiphenyl

R.T.: 8.297 min
Delta R.T.: 0.000 min
Response: 76842063
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

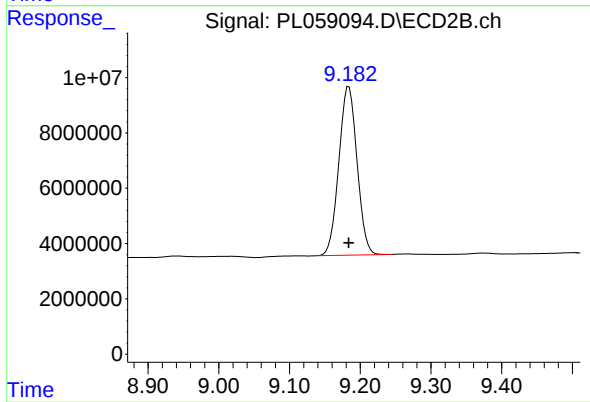

#28 Decachlorobiphenyl

R.T.: 9.184 min
Delta R.T.: 0.000 min
Response: 109094002
Conc: 50.00 ng/ml