

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060320\
 Data File : PL059110.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2020 16:21
 Operator : AJ\MA
 Sample : L2832-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 20200383-DI-WATER

Manual Integrations
 APPROVED

mohammad
 6/4/2020 12:46:42 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 09:09:07 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060320.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 04 08:16:22 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.522	4.071	58429014	58397866	33.836	22.444m#
28)	SA Decachlor...	8.296	9.184	25094274	37204673	15.261	15.695

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060320\
Data File : PL059110.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2020 16:21
Operator : AJ\MA
Sample : L2832-01
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
20200383-DI-WATER


Manual Integrations
APPROVED

mohammad
6/4/2020 12:46:42 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 09:09:07 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060320.M
Quant Title : GC Extractables
QLast Update : Thu Jun 04 08:16:22 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

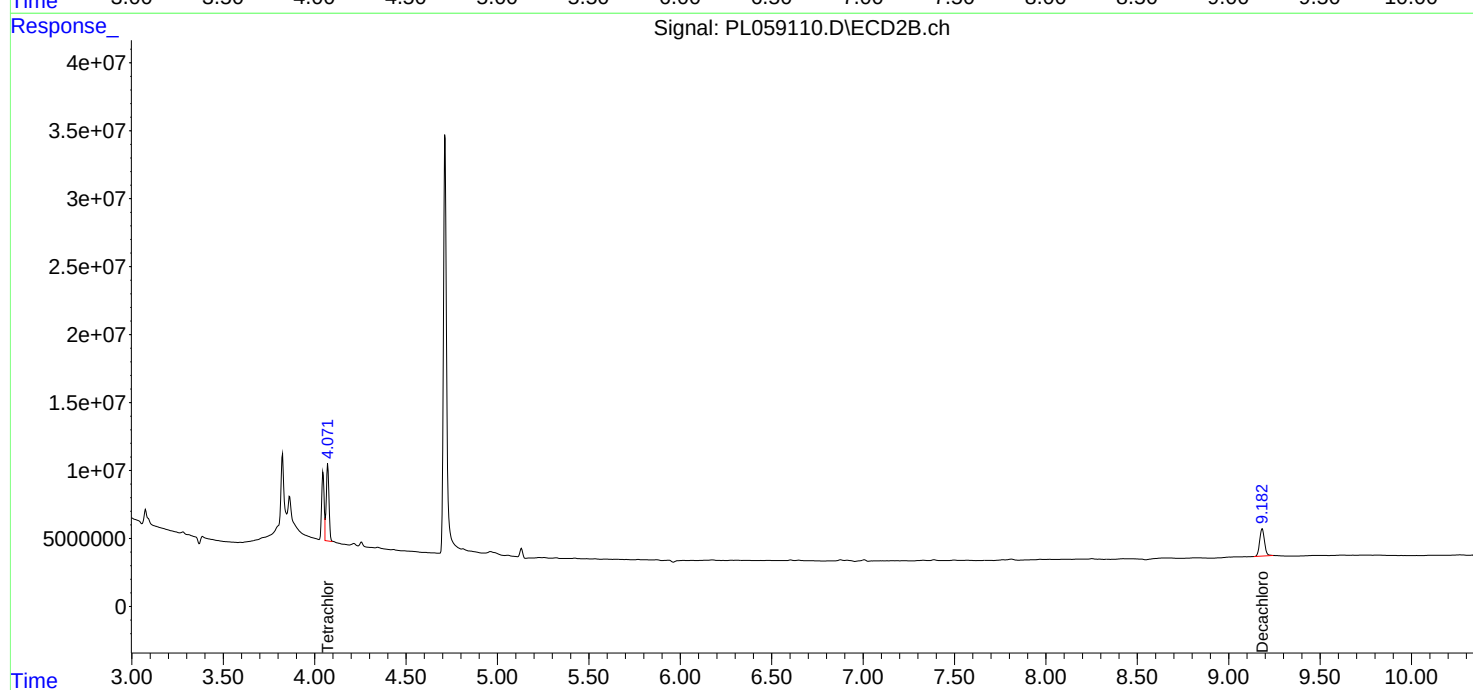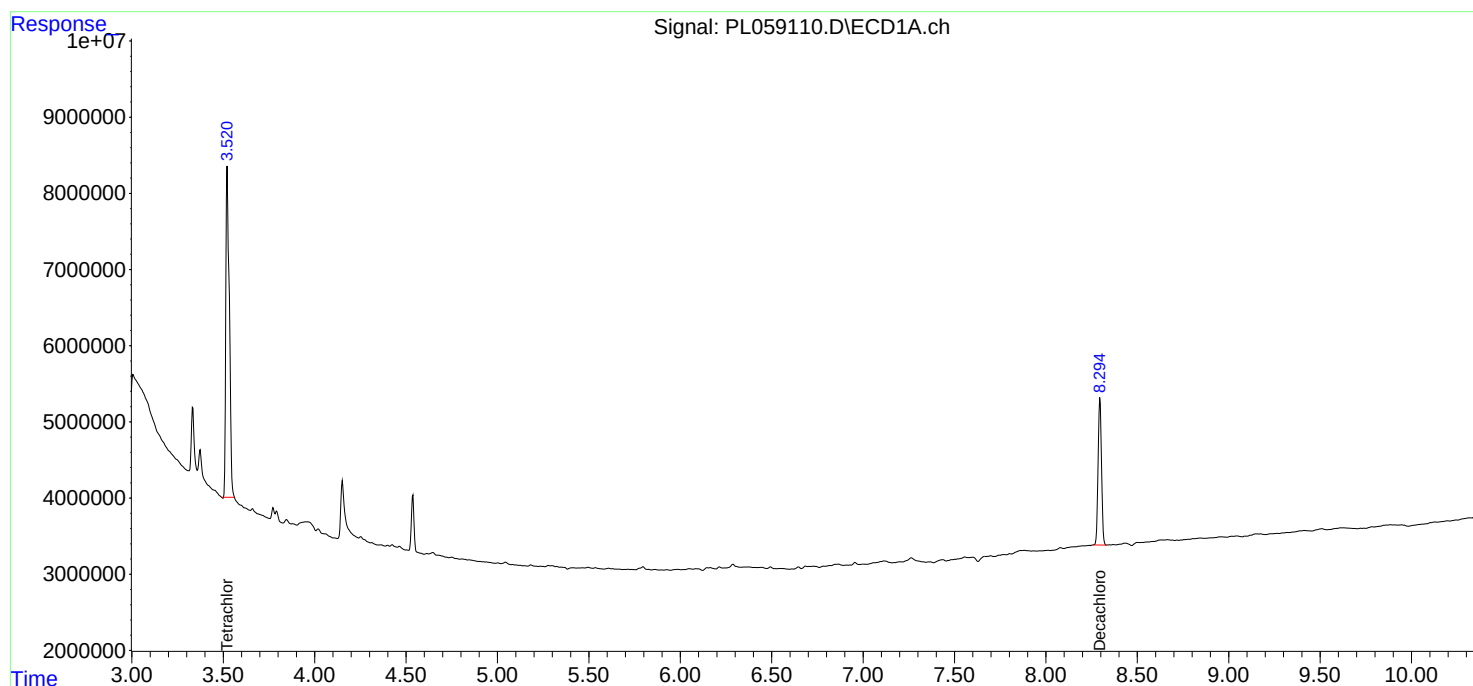

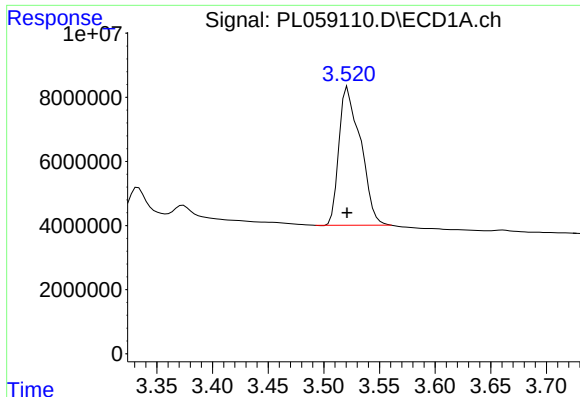


#1 Tetrachloro-m-xylene

R.T.: 3.522 min
Delta R.T.: 0.000 min
Response: 58429014
Conc: 33.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
20200383-DI-WATER


Manual Integrations
APPROVED

mohammad
6/4/2020 12:46:42 PM

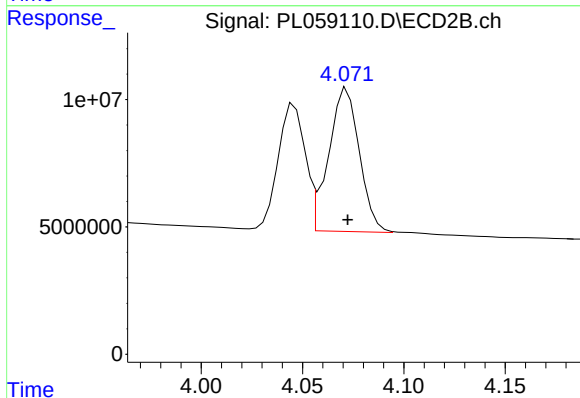


#1 Tetrachloro-m-xylene

R.T.: 4.071 min
Delta R.T.: -0.002 min
Response: 58397866
Conc: 22.44 ng/ml m

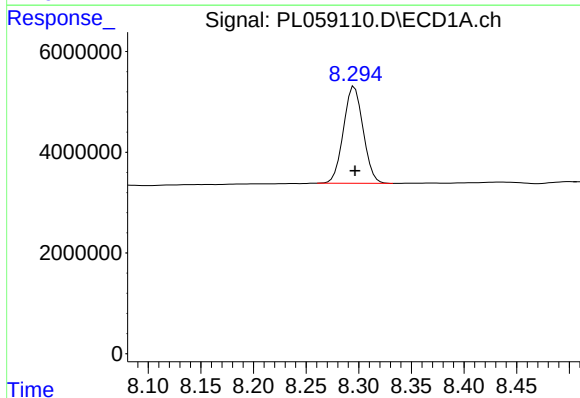

#28 Decachlorobiphenyl

R.T.: 8.296 min
Delta R.T.: 0.000 min
Response: 25094274
Conc: 15.26 ng/ml

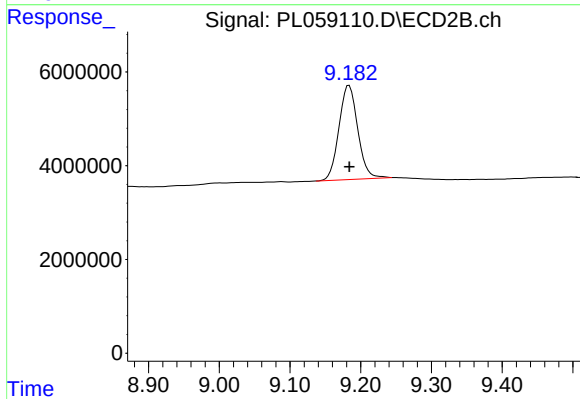

#28 Decachlorobiphenyl

R.T.: 9.184 min
Delta R.T.: 0.000 min
Response: 37204673
Conc: 15.69 ng/ml