

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060320\
 Data File : PL059122.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2020 19:38
 Operator : AJ\MA
 Sample : L2494-02 5X
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 20200382-MANASQUAN-WATER

Manual Integrations
 APPROVED

mohammad
 6/4/2020 12:47:04 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 08:47:15 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060320.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 04 08:16:22 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.522	4.072	10856563	11961443	6.287	4.597m#
2) SA Decachlor...	8.298	9.185	8039254	11717977	4.889	4.943
Target Compounds						
16) A 4,4'-DDD	6.215	6.914	654127	1481448	0.495	0.638m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060320\
Data File : PL059122.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2020 19:38
Operator : AJ\MA
Sample : L2494-02 5X
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
20200382-MANASQUAN-WATER


Manual Integrations
APPROVED

mohammad
6/4/2020 12:47:04 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 08:47:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060320.M
Quant Title : GC Extractables
QLast Update : Thu Jun 04 08:16:22 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

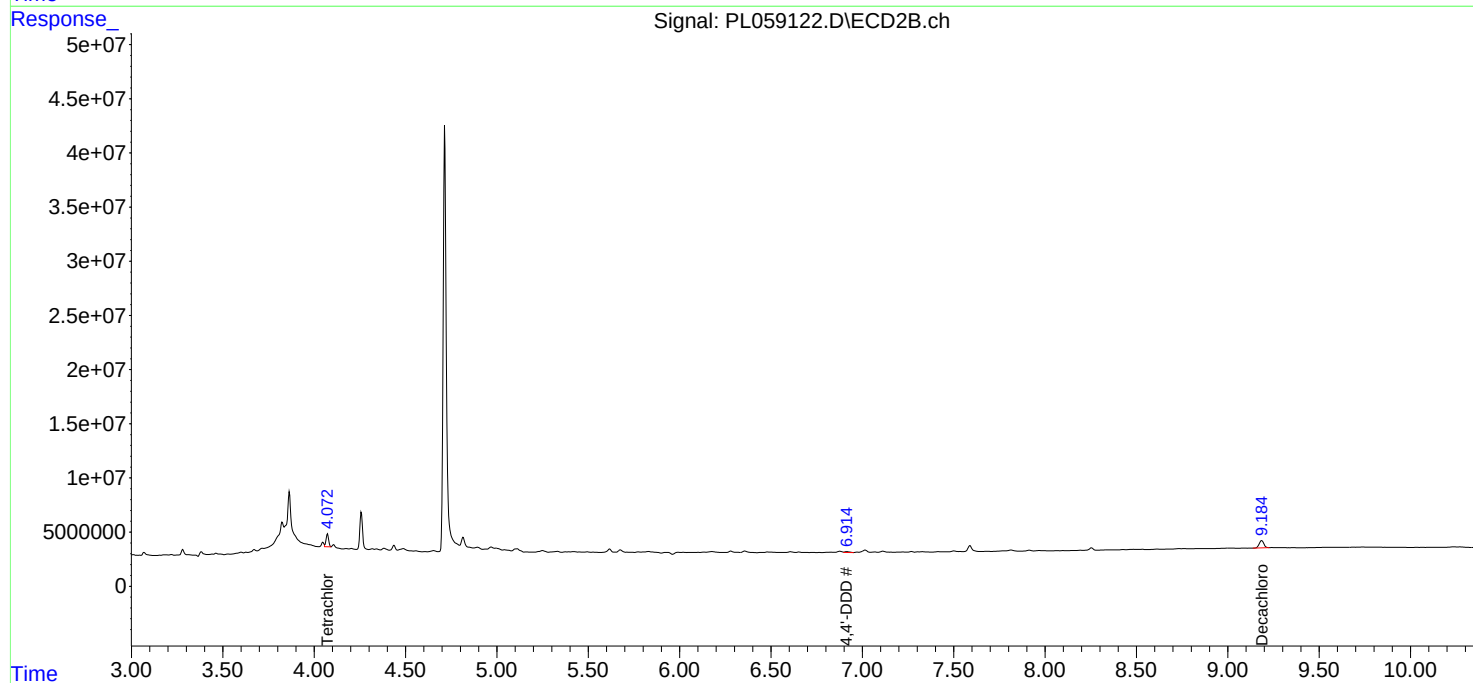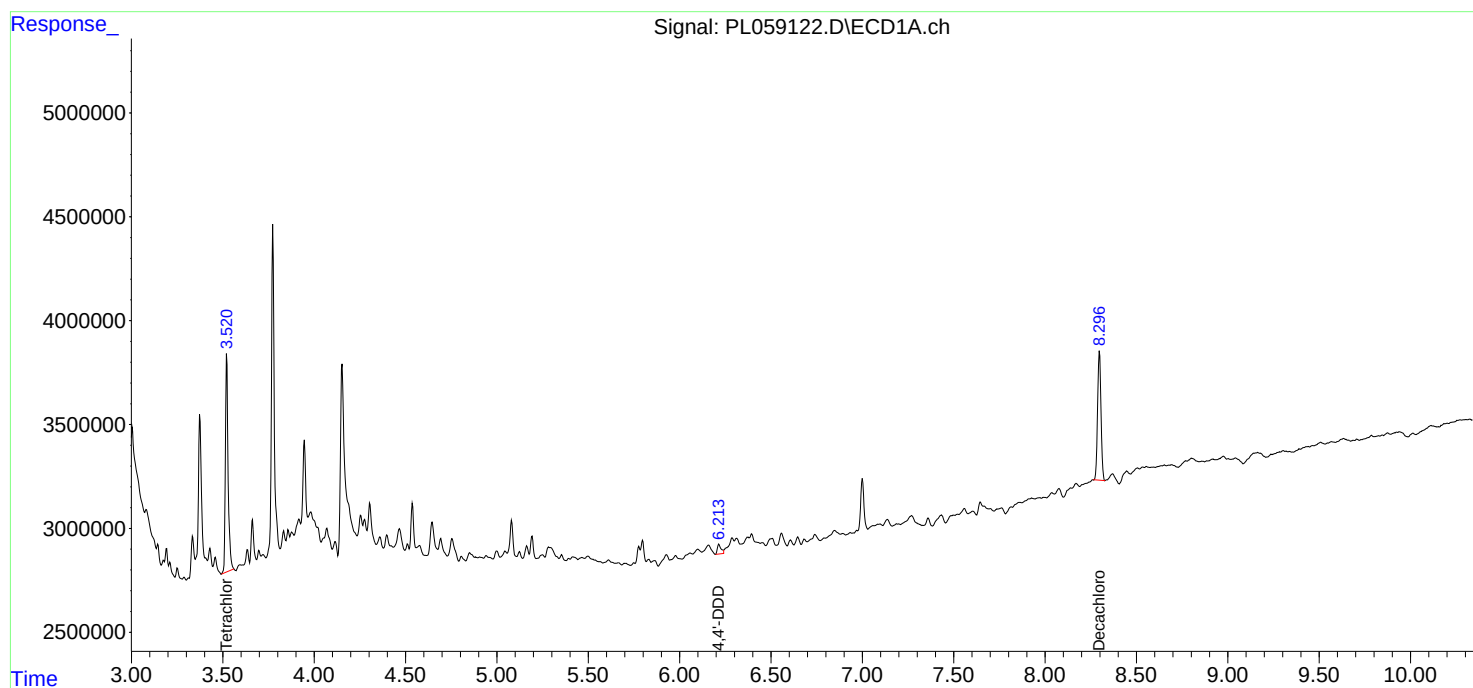

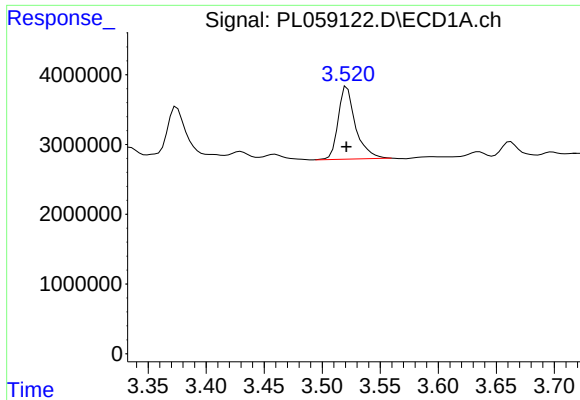


#1 Tetrachloro-m-xylene

R.T.: 3.522 min
Delta R.T.: 0.000 min
Response: 10856563
Conc: 6.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
20200382-MANASQUAN-WATER


Manual Integrations
APPROVED

mohammad
6/4/2020 12:47:04 PM

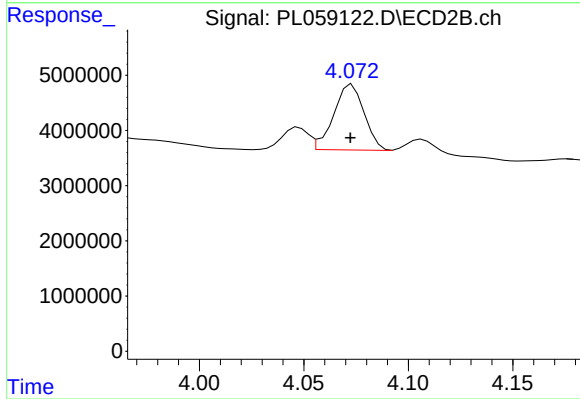


#1 Tetrachloro-m-xylene

R.T.: 4.072 min
Delta R.T.: 0.000 min
Response: 11961443
Conc: 4.60 ng/ml m

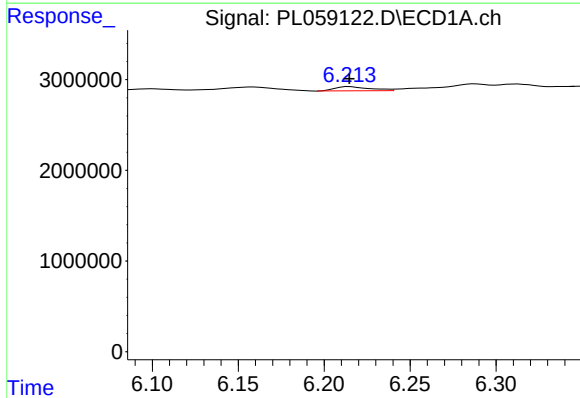


#16 4,4'-DDD

R.T.: 6.215 min
Delta R.T.: 0.000 min
Response: 654127
Conc: 0.49 ng/ml

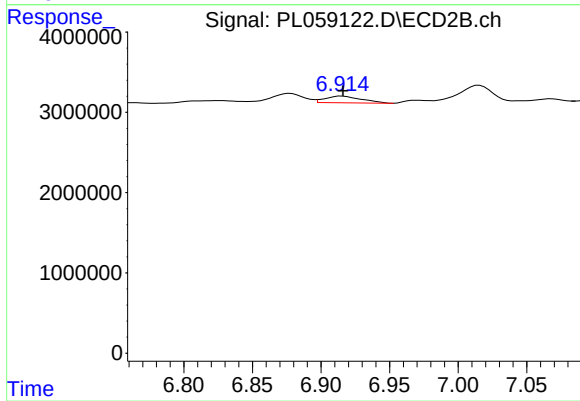

#16 4,4'-DDD

R.T.: 6.914 min
Delta R.T.: -0.003 min
Response: 1481448
Conc: 0.64 ng/ml m

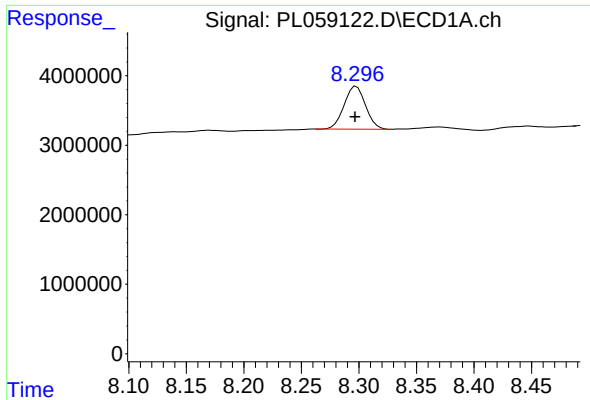


#28 Decachlorobiphenyl

R.T.: 8.298 min
Delta R.T.: 0.001 min
Response: 8039254
Conc: 4.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
20200382-MANASQUAN-WATER

Manual Integrations
APPROVED

mohammad
6/4/2020 12:47:04 PM

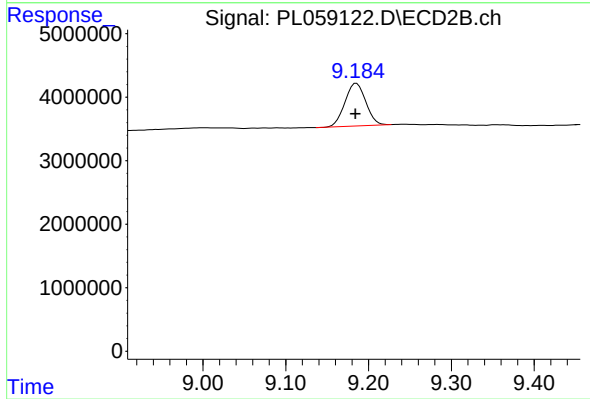

#28 Decachlorobiphenyl

R.T.: 9.185 min
Delta R.T.: 0.001 min
Response: 11717977
Conc: 4.94 ng/ml