

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060321\
 Data File : PL067047.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2021 15:42
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 02:36:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060121.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 02 14:20:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.480	5.531	9404504	14571784	22.966	22.526
28)	SA Decachlor...	10.223	11.430	12080868	16419440	18.683	19.679
Target Compounds							
3)	MA gamma-BHC...	5.597	0.000	853776	0	1.533	N.D. #
6)	B beta-BHC	5.964f	0.000	153428	0	0.576	N.D. #
7)	B delta-BHC	0.000	7.003f	0	1752269	N.D.	2.308 #
14)	MA Endrin	7.897f	0.000	1934455	0	3.735	N.D. #
23)	Chlordane-1	0.000	6.940f	0	732894	N.D.	35.761 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060321\
Data File : PL067047.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2021 15:42
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 02:36:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060121.M
Quant Title : GC Extractables
QLast Update : Wed Jun 02 14:20:39 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

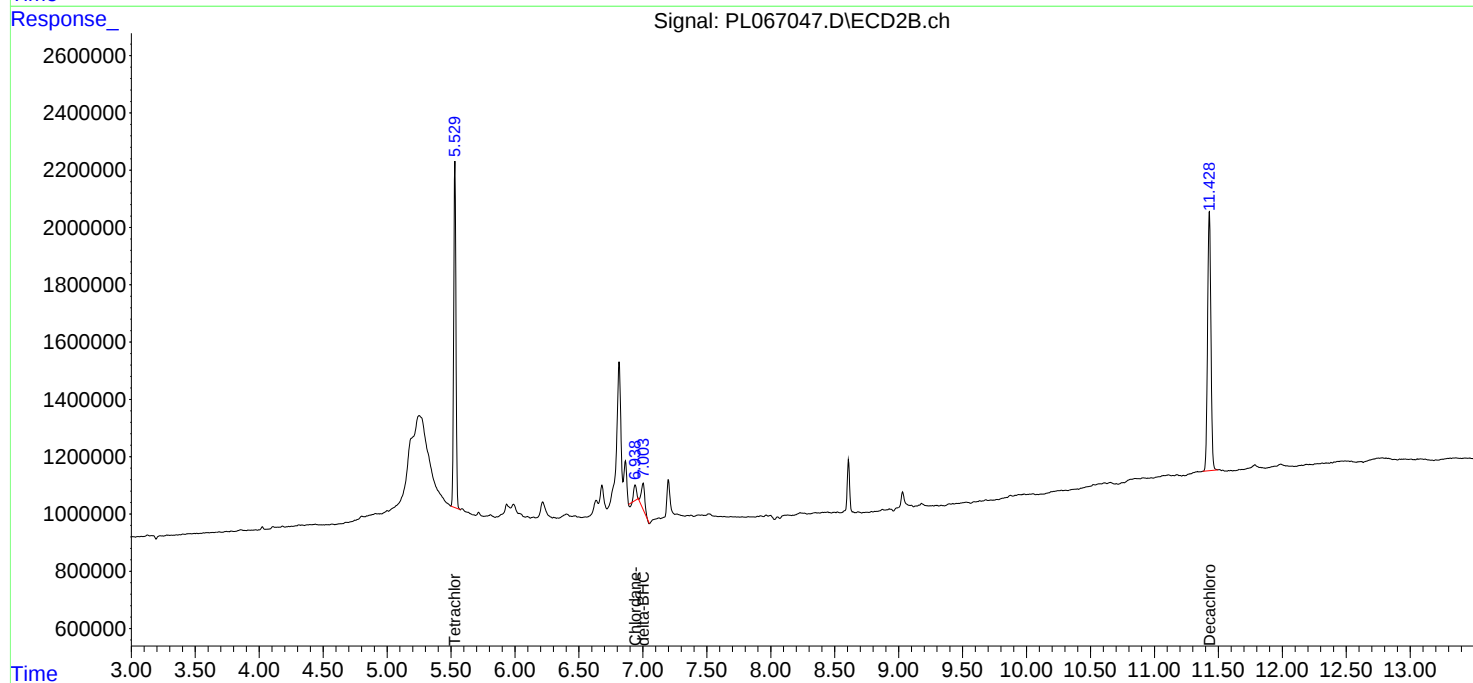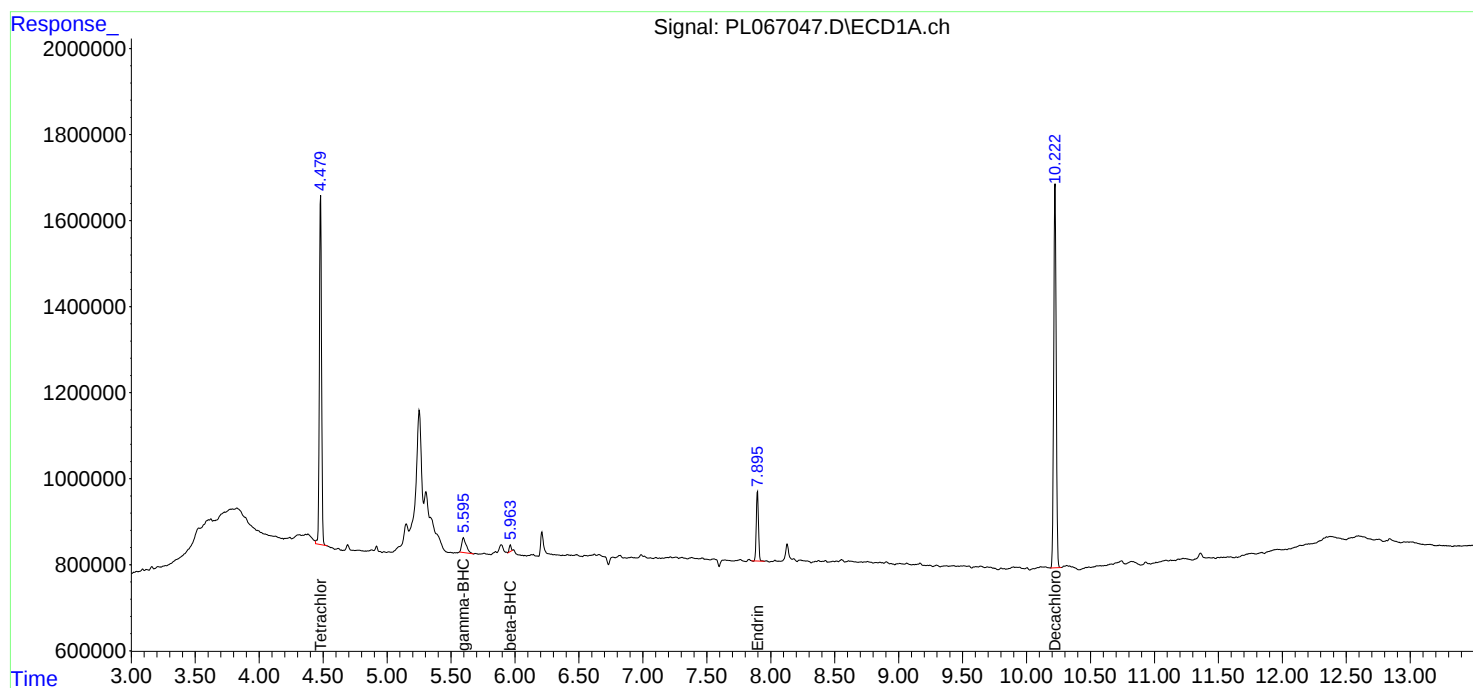


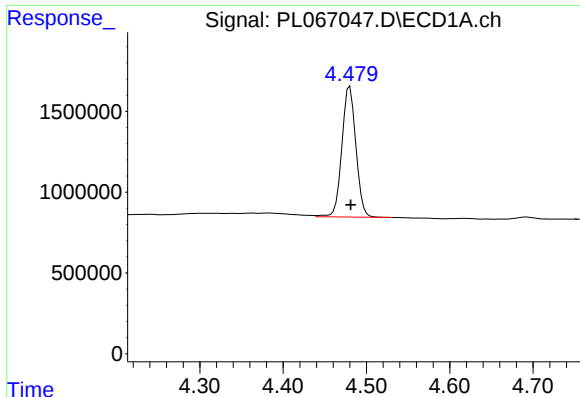

#1 Tetrachloro-m-xylene


R.T.: 4.480 min
Delta R.T.: 0.000 min
Response: 9404504
Conc: 22.97 ng/ml

Instrument :
ECD_L
ClientSampleId :

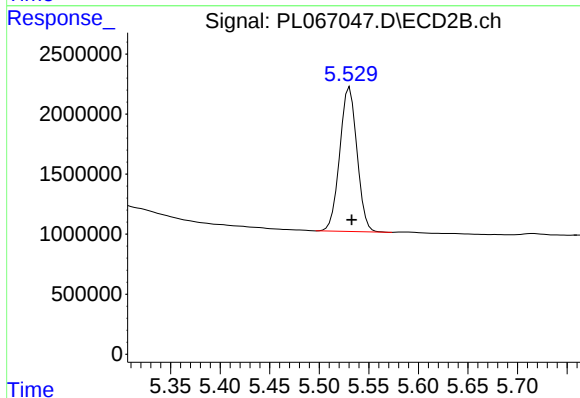


#1 Tetrachloro-m-xylene

R.T.: 5.531 min
Delta R.T.: -0.002 min
Response: 14571784
Conc: 22.53 ng/ml

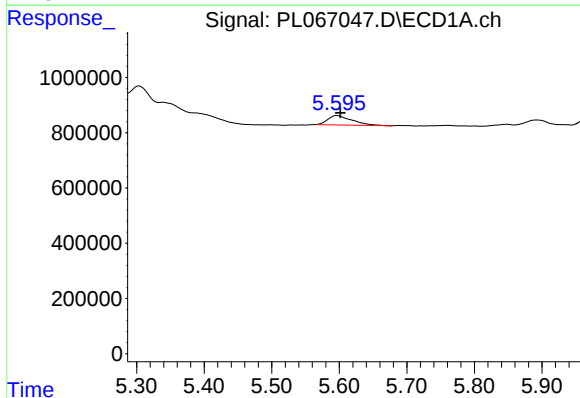


#3 gamma-BHC (Lindane)

R.T.: 5.597 min
Delta R.T.: -0.005 min
Response: 853776
Conc: 1.53 ng/ml

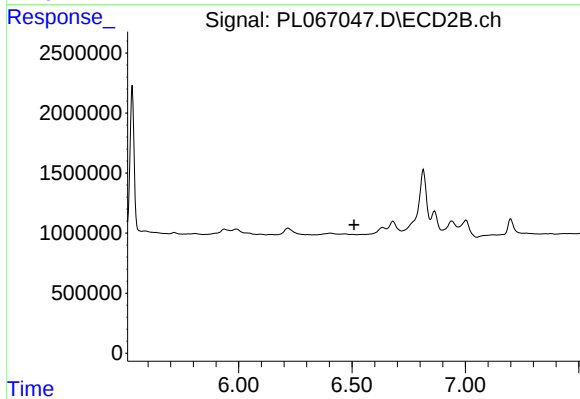

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 6.509 min
Response: 0
Conc: N.D.

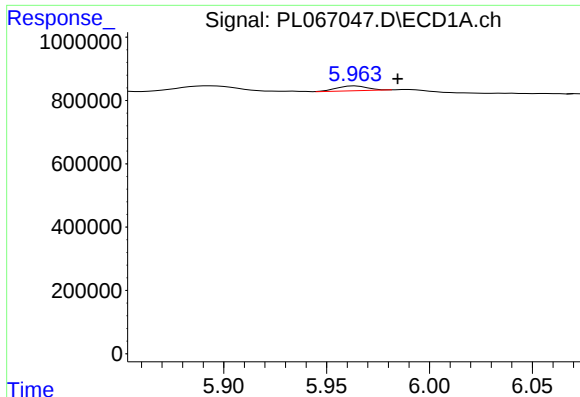

#6 beta-BHC


R.T.: 5.964 min
Delta R.T.: -0.021 min
Response: 153428
Conc: 0.58 ng/ml

Instrument :
ECD_L
ClientSampleId :

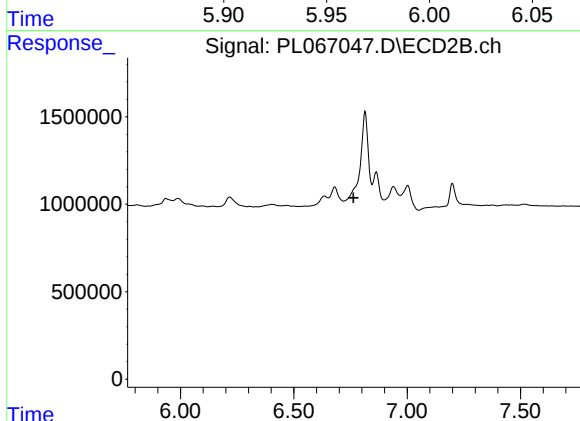


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.763 min
Response: 0
Conc: N.D.

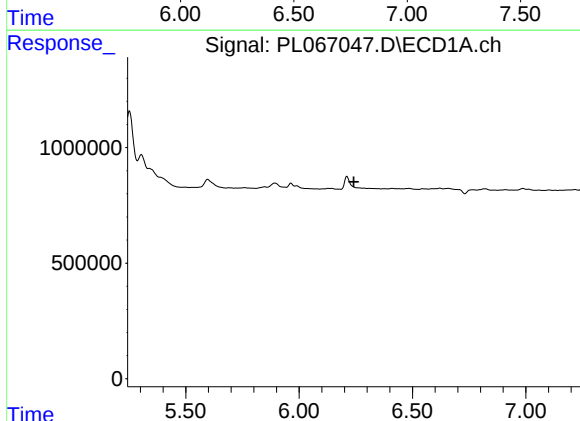


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.241 min
Response: 0
Conc: N.D.

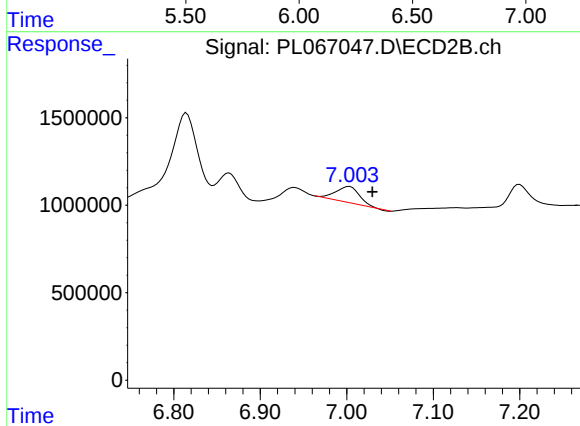

#7 delta-BHC


R.T.: 7.003 min
Delta R.T.: -0.026 min
Response: 1752269
Conc: 2.31 ng/ml

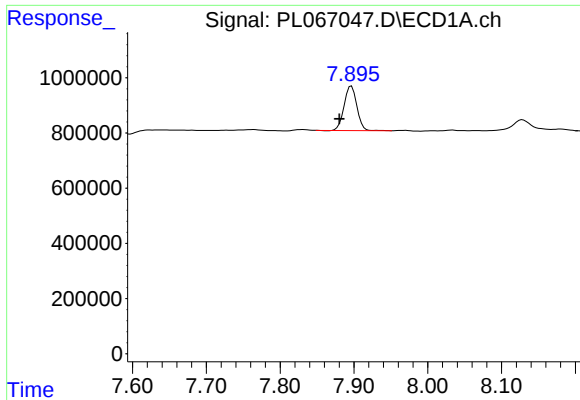

#14 Endrin


R.T.: 7.897 min
Delta R.T.: 0.016 min
Response: 1934455
Conc: 3.74 ng/ml

Instrument :
ECD_L
ClientSampleId :

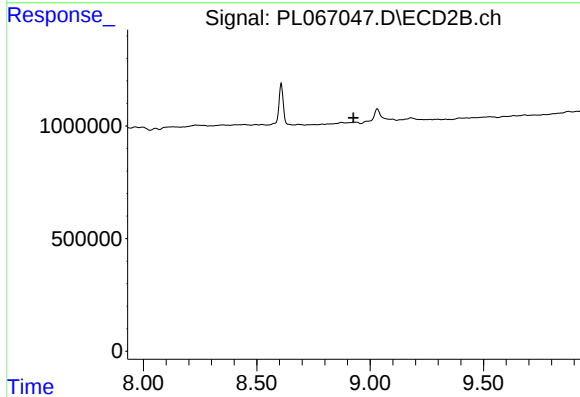


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.927 min
Response: 0
Conc: N.D.

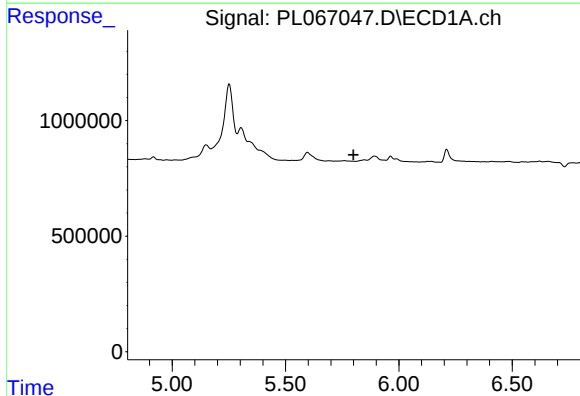


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.800 min
Response: 0
Conc: N.D.

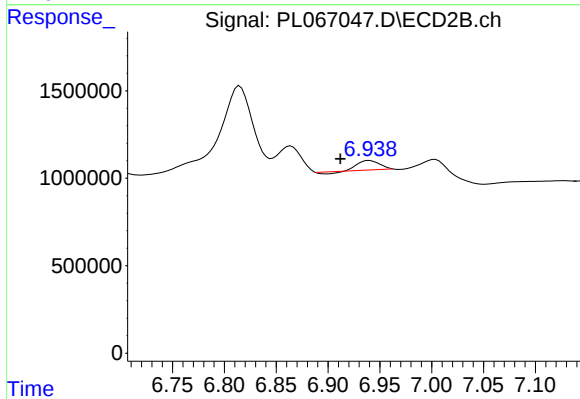

#23 Chlordane-1


R.T.: 6.940 min
Delta R.T.: 0.028 min
Response: 732894
Conc: 35.76 ng/ml

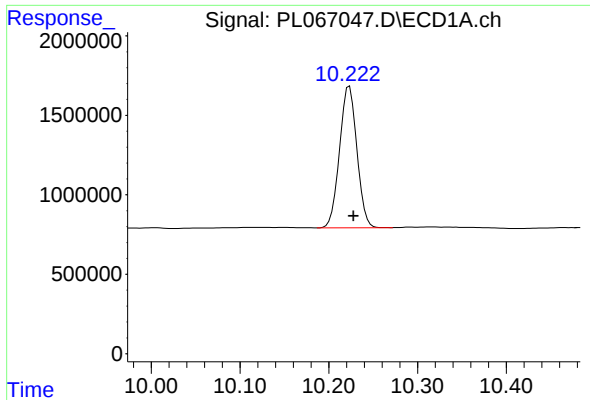

#28 Decachlorobiphenyl

R.T.: 10.223 min
Delta R.T.: -0.005 min
Response: 12080868
Conc: 18.68 ng/ml

Instrument :
ECD_L
ClientSampleId :

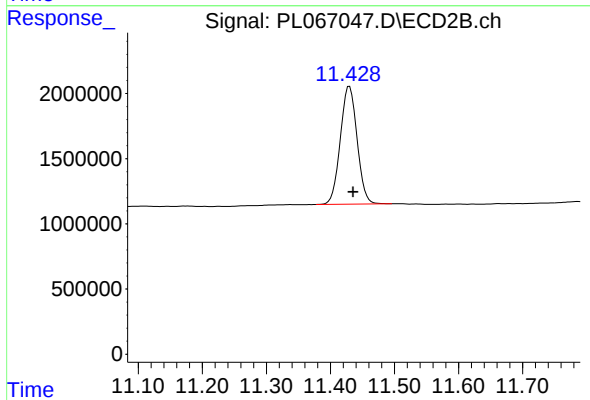

#28 Decachlorobiphenyl

R.T.: 11.430 min
Delta R.T.: -0.005 min
Response: 16419440
Conc: 19.68 ng/ml