

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060321\
 Data File : PL067054.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2021 18:00
 Operator : AR\AJ
 Sample : M2580-07
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 18-B3(0-2)

Manual Integrations
 APPROVED

Ankita
 6/4/2021 2:09:04 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 02:38:08 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060121.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 02 14:20:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.478	5.531	4958473	6244172	12.109m	9.652
28)	SA Decachlor...	10.224	11.431	5975645	8586050	9.241	10.291
Target Compounds							
7)	B delta-BHC	6.249	7.034	1514430	2256641	2.854	2.972
12)	B 4,4'-DDE	7.471	8.528	6531866	15243678	12.234	23.319 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060321\
Data File : PL067054.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2021 18:00
Operator : AR\AJ
Sample : M2580-07
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
18-B3(0-2)


Manual Integrations
APPROVED

Ankita
6/4/2021 2:09:04 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 02:38:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060121.M
Quant Title : GC Extractables
QLast Update : Wed Jun 02 14:20:39 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

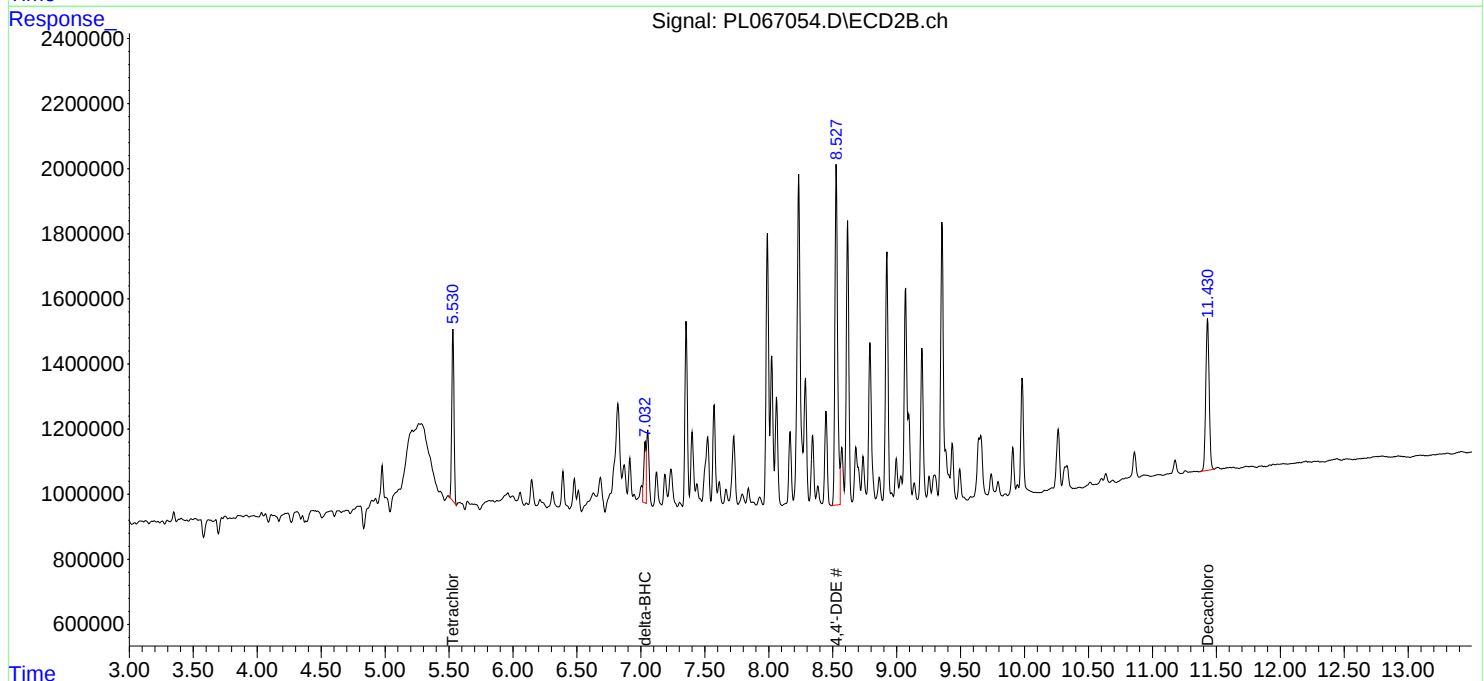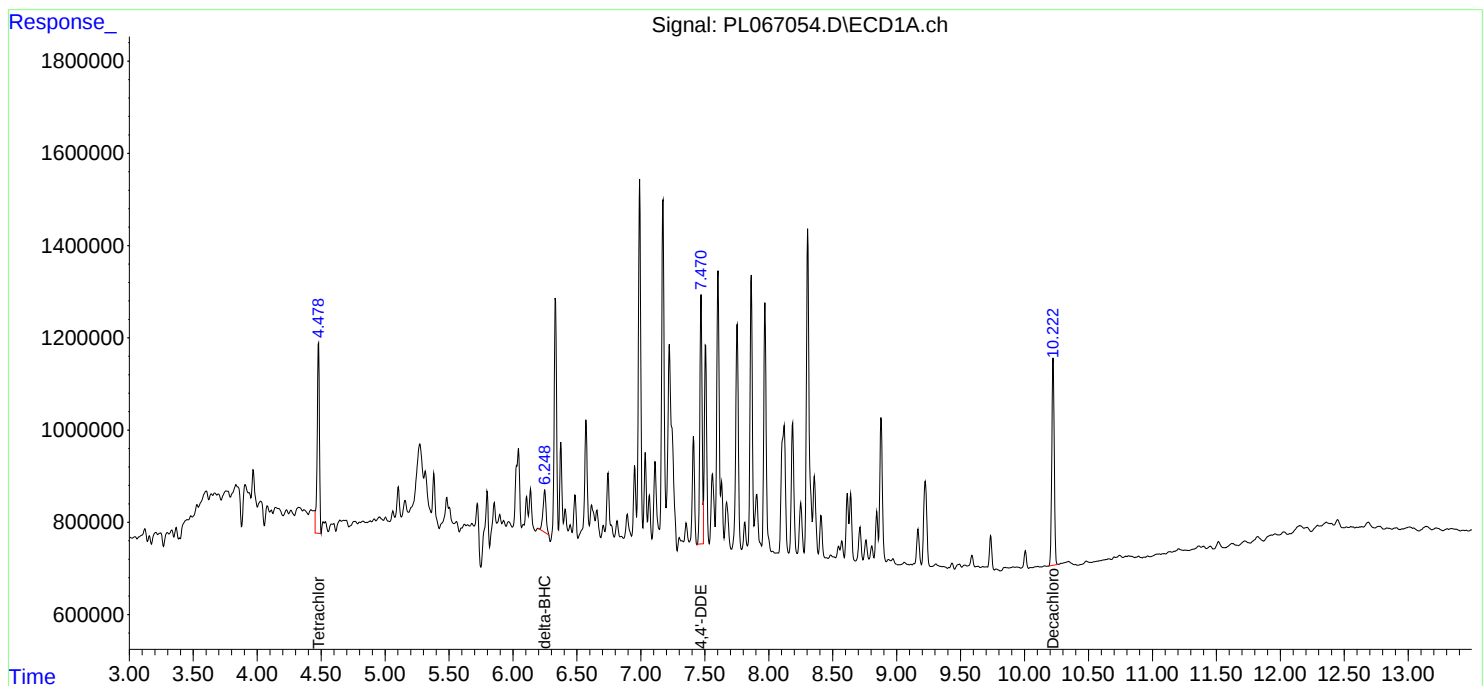

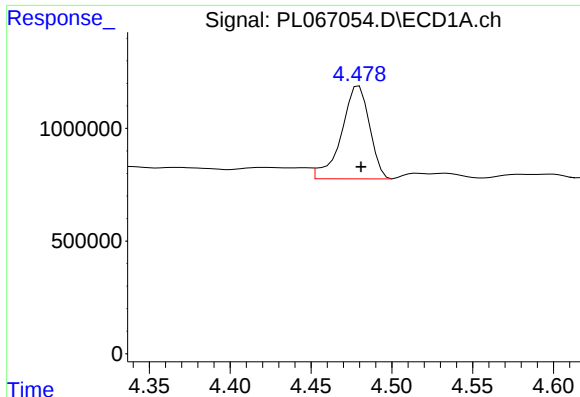


#1 Tetrachloro-m-xylene

R.T.: 4.478 min
Delta R.T.: -0.003 min
Response: 4958473
Conc: 12.11 ng/ml m

Instrument :
ECD_L
ClientSampleId :
18-B3(0-2)


Manual Integrations
APPROVED

Ankita
6/4/2021 2:09:04 PM

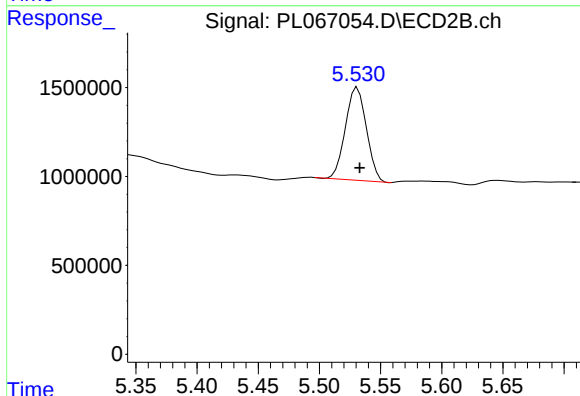


#1 Tetrachloro-m-xylene

R.T.: 5.531 min
Delta R.T.: -0.002 min
Response: 6244172
Conc: 9.65 ng/ml

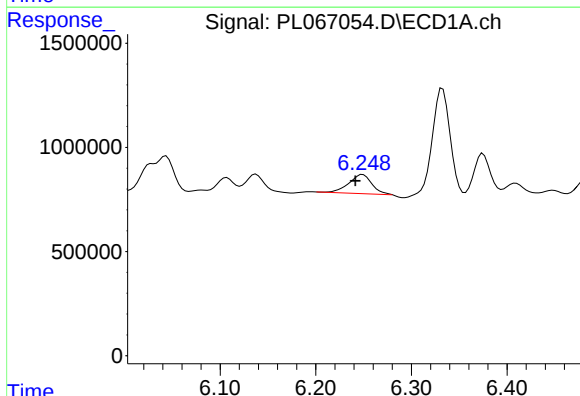


#7 delta-BHC

R.T.: 6.249 min
Delta R.T.: 0.008 min
Response: 1514430
Conc: 2.85 ng/ml

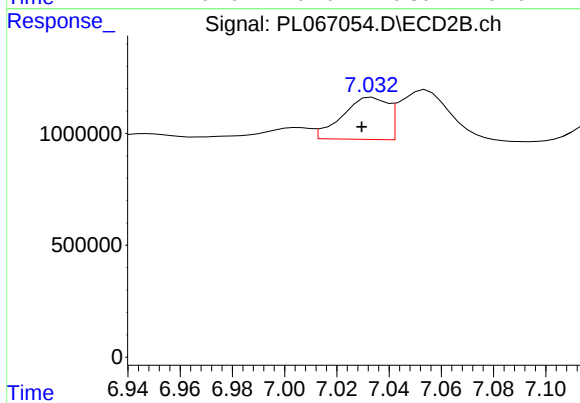

#7 delta-BHC

R.T.: 7.034 min
Delta R.T.: 0.004 min
Response: 2256641
Conc: 2.97 ng/ml

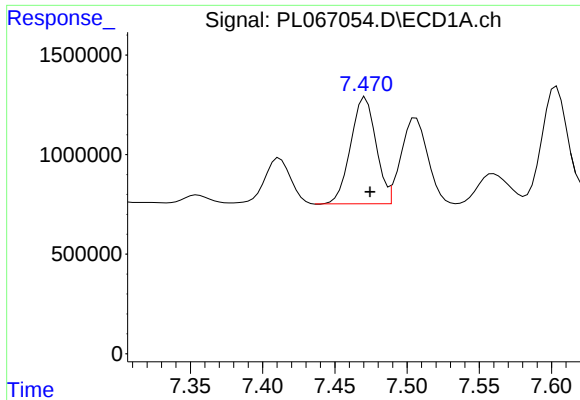


#12 4,4'-DDE

R.T.: 7.471 min
Delta R.T.: -0.003 min
Response: 6531866
Conc: 12.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
18-B3(0-2)


Manual Integrations
APPROVED

Ankita
6/4/2021 2:09:04 PM

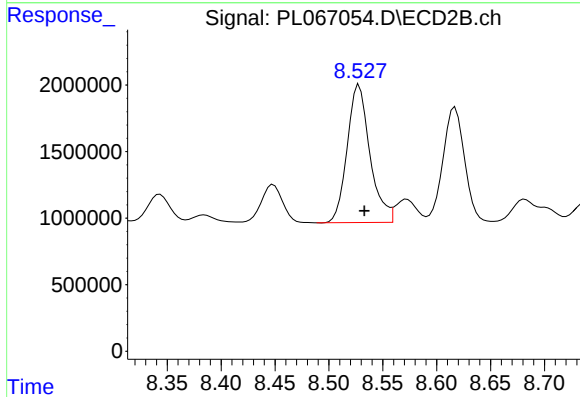


#12 4,4'-DDE

R.T.: 8.528 min
Delta R.T.: -0.005 min
Response: 15243678
Conc: 23.32 ng/ml

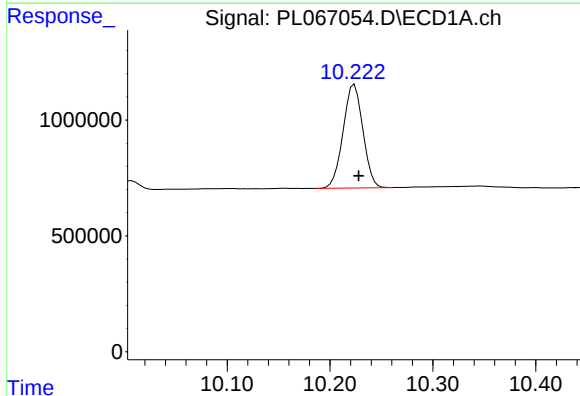

#28 Decachlorobiphenyl

R.T.: 10.224 min
Delta R.T.: -0.004 min
Response: 5975645
Conc: 9.24 ng/ml

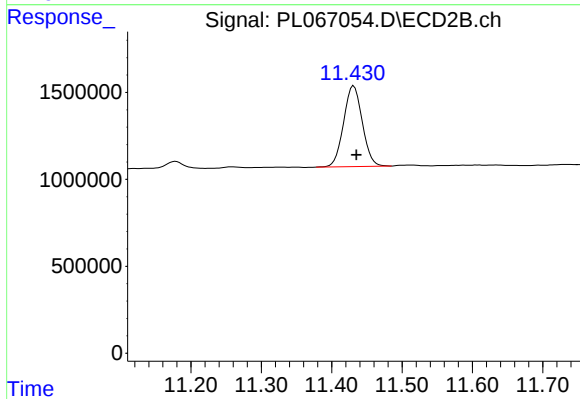

#28 Decachlorobiphenyl

R.T.: 11.431 min
Delta R.T.: -0.004 min
Response: 8586050
Conc: 10.29 ng/ml