

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060324\
 Data File : PL089892.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2024 10:41
 Operator : AR\AJ
 Sample : PB161235BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB161235BL

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 06/05/2024
 Supervised By :Ankita Jodhani 06/05/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 23:11:59 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052424.M
 Quant Title : GC Extractables
 QLast Update : Fri May 24 14:57:01 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.555	2.792	40457969	27549346	19.323	19.214
2) SA Decachlor...	9.069	7.944	25971924	26113519	17.663m	17.573

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060324\
Data File : PL089892.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2024 10:41
Operator : AR\AJ
Sample : PB161235BL
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PB161235BL


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 06/05/2024
Supervised By : Ankita Jodhani 06/05/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 23:11:59 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052424.M
Quant Title : GC Extractables
QLast Update : Fri May 24 14:57:01 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

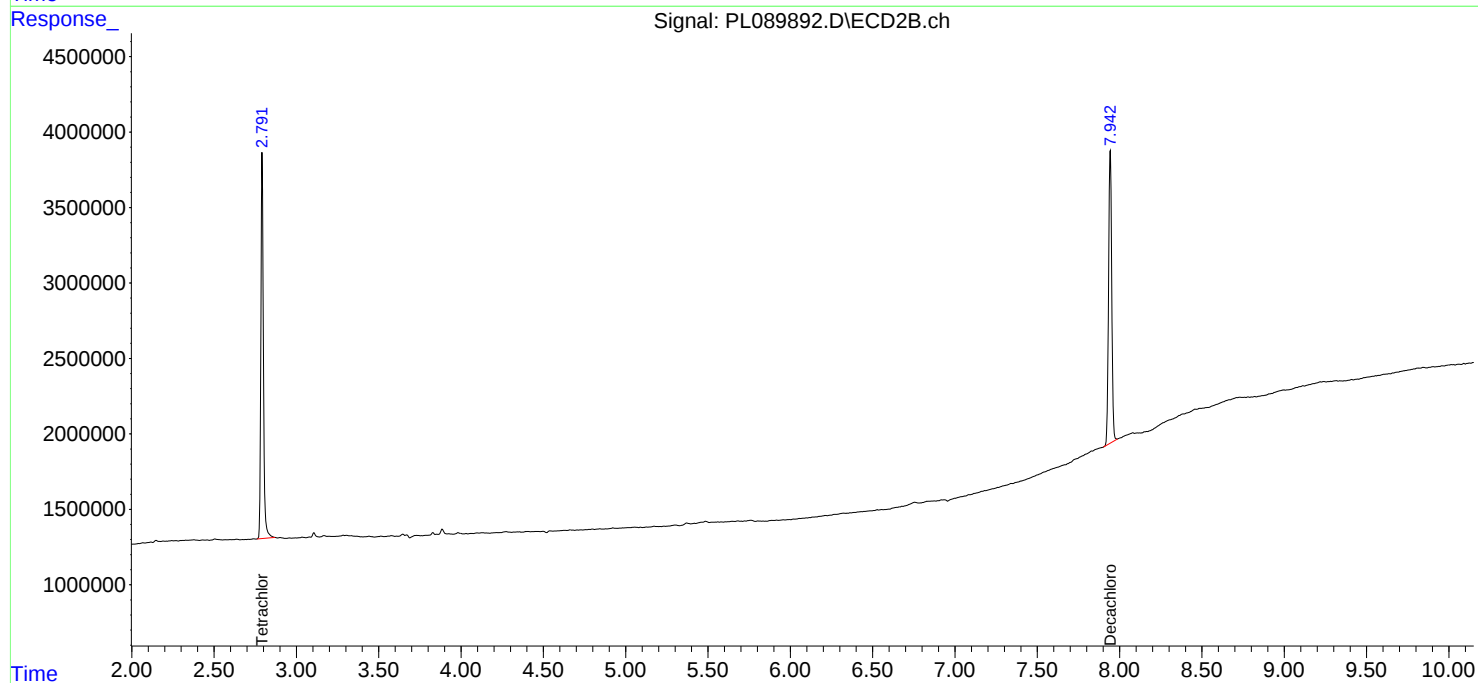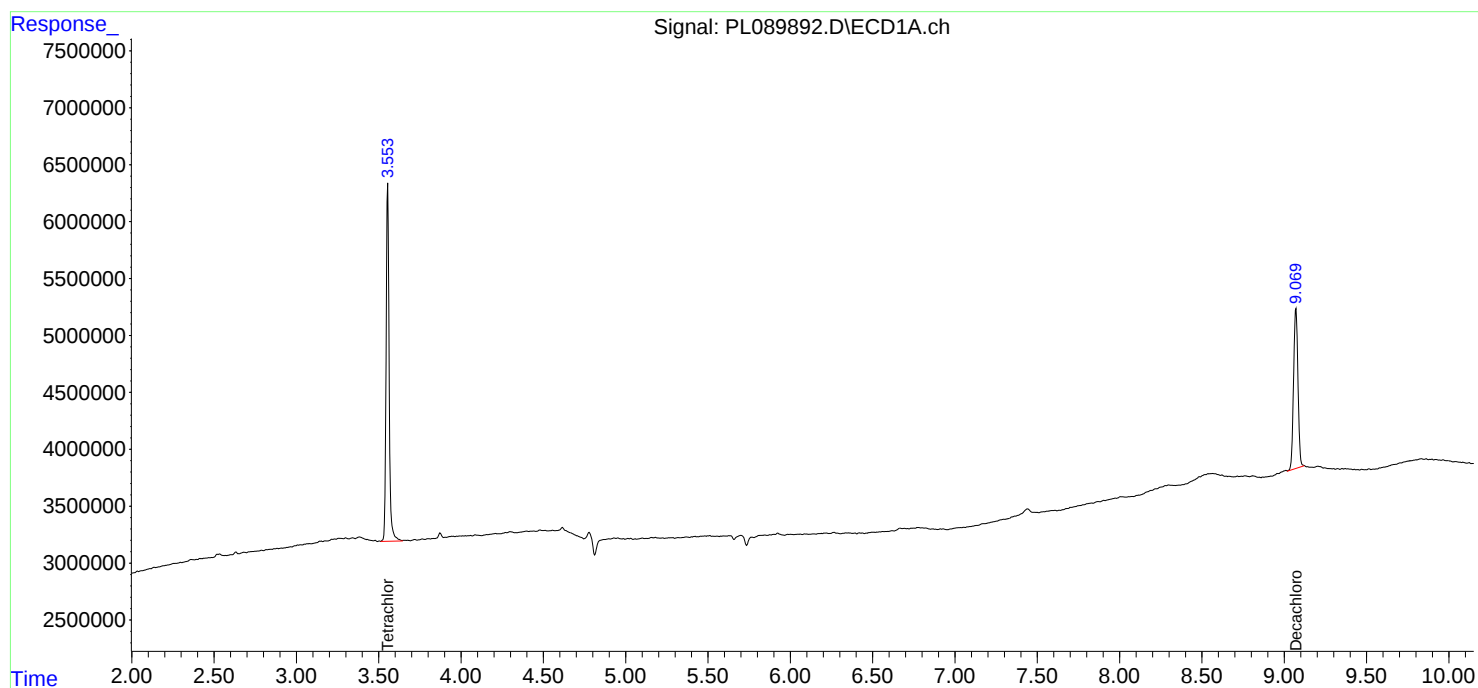

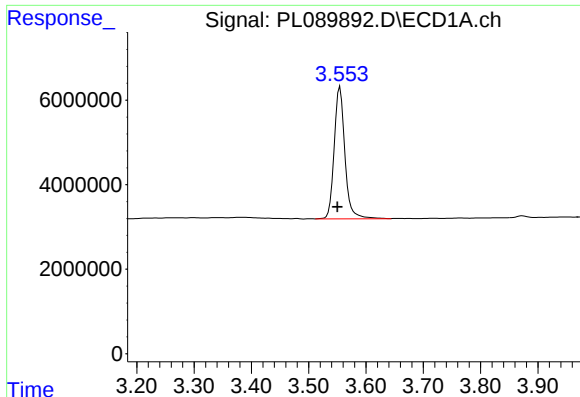


#1 Tetrachloro-m-xylene

R.T.: 3.555 min
Delta R.T.: 0.005 min
Response: 40457969
Conc: 19.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB161235BL


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/05/2024
Supervised By :Ankita Jodhani 06/05/2024

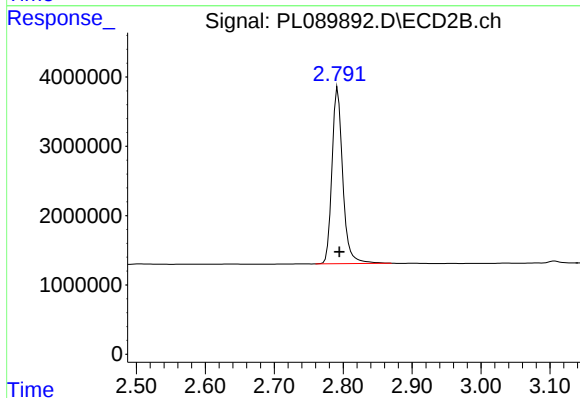


#1 Tetrachloro-m-xylene

R.T.: 2.792 min
Delta R.T.: -0.002 min
Response: 27549346
Conc: 19.21 ng/ml

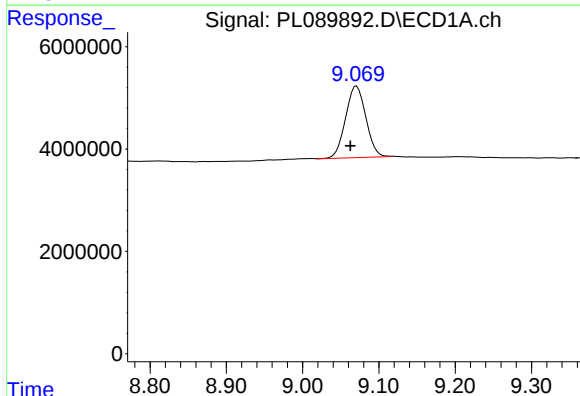

#28 Decachlorobiphenyl

R.T.: 9.069 min
Delta R.T.: 0.007 min
Response: 25971924
Conc: 17.66 ng/ml m

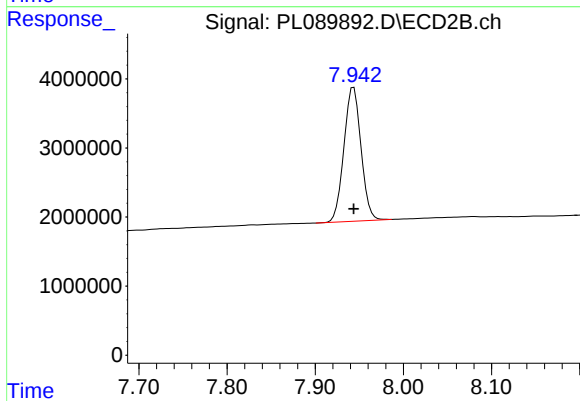

#28 Decachlorobiphenyl

R.T.: 7.944 min
Delta R.T.: 0.000 min
Response: 26113519
Conc: 17.57 ng/ml