

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060325\
 Data File : PL095887.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2025 14:42
 Operator : AR\AJ
 Sample : Q2176-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-25

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 01:36:10 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052125.M
 Quant Title : GC Extractables
 QLast Update : Thu May 22 06:29:30 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.572	2.886	95251635	77616934	30.188	19.831 #
28)	SA Decachlor...	9.099	8.060	34605078	64097333	14.686	14.653
Target Compounds							
9)	A Endosulfan I	0.000	5.258f	0	6213077	N.D.	1.304 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060325\
Data File : PL095887.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2025 14:42
Operator : AR\AJ
Sample : Q2176-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-25

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 01:36:10 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052125.M
Quant Title : GC Extractables
QLast Update : Thu May 22 06:29:30 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

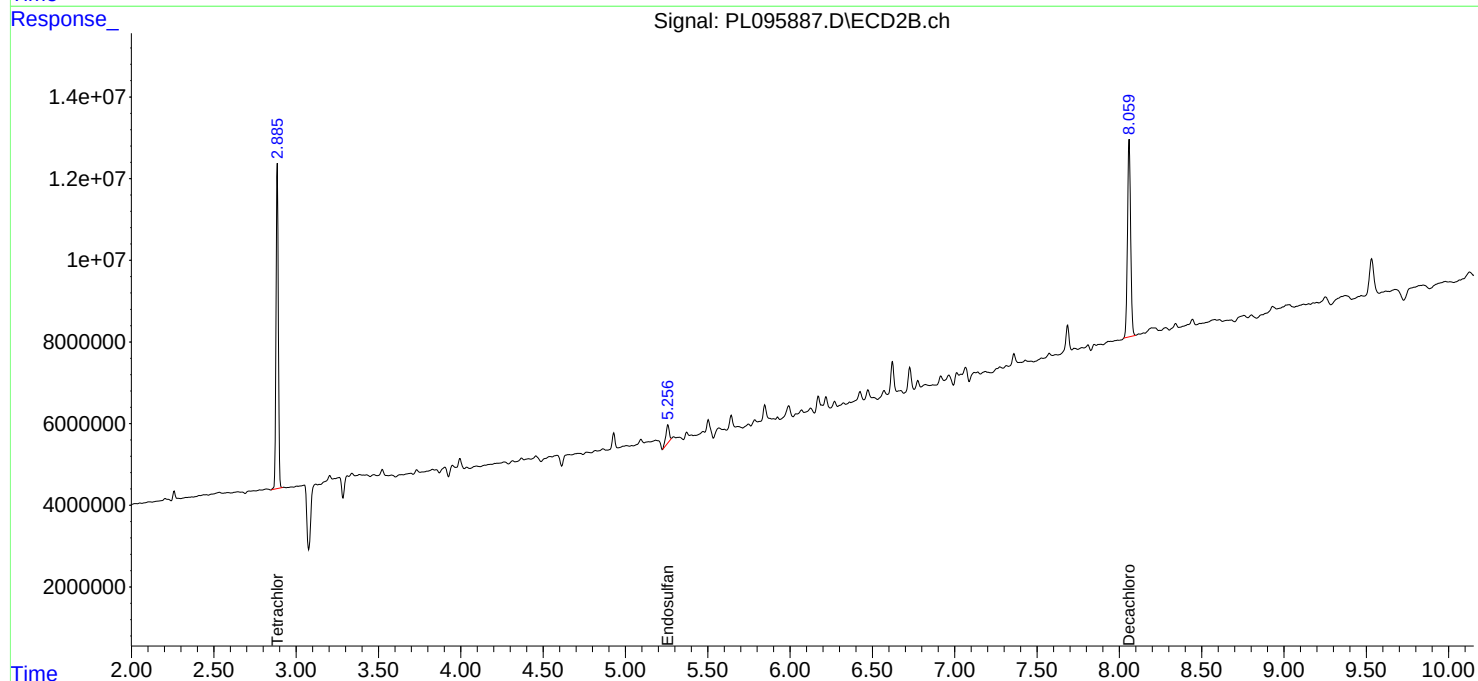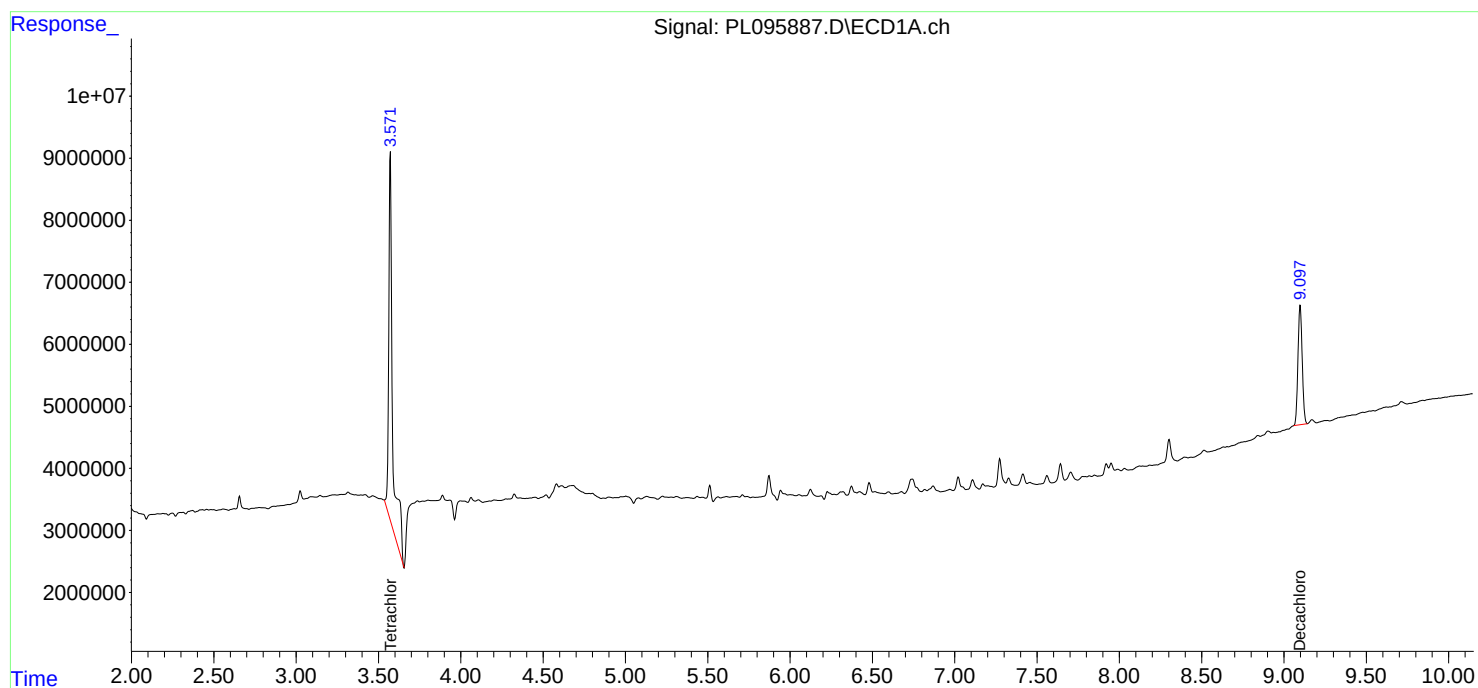


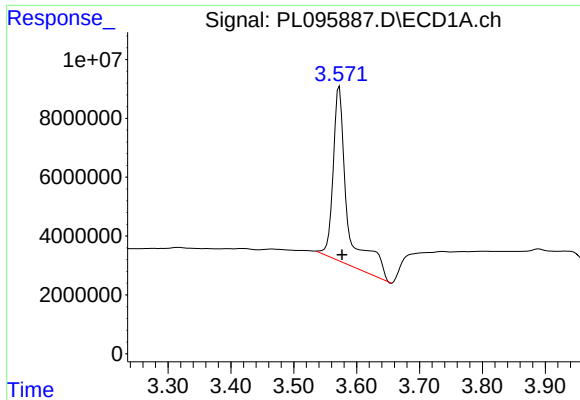

#1 Tetrachloro-m-xylene


R.T.: 3.572 min
Delta R.T.: -0.005 min
Response: 95251635
Conc: 30.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-25

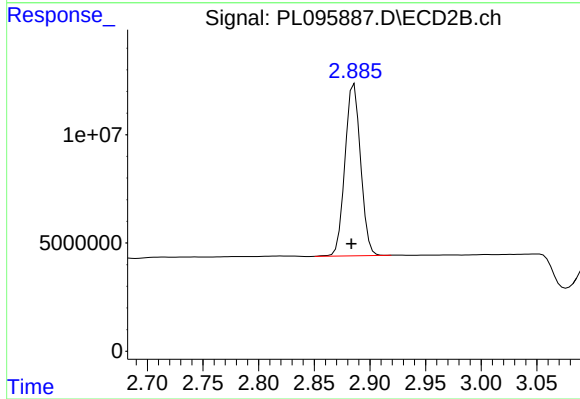


#1 Tetrachloro-m-xylene

R.T.: 2.886 min
Delta R.T.: 0.002 min
Response: 77616934
Conc: 19.83 ng/ml

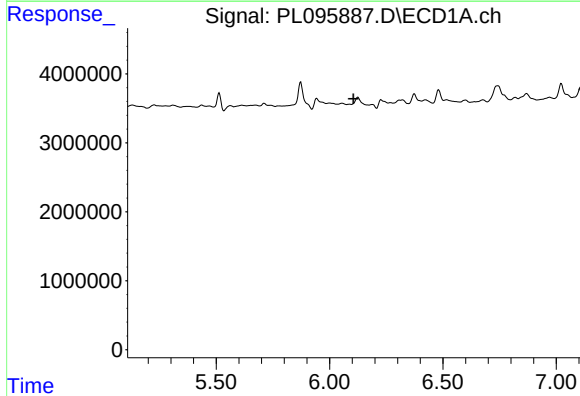


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.106 min
Response: 0
Conc: N.D.

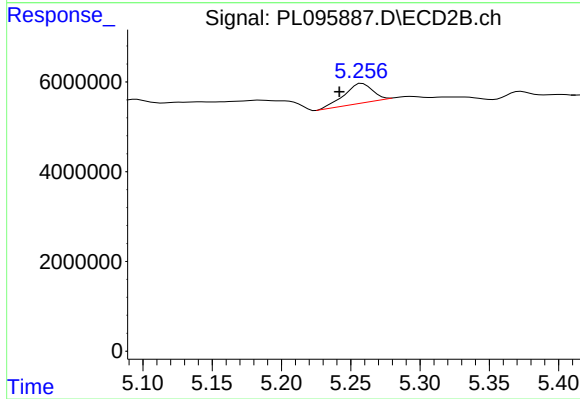

#9 Endosulfan I


R.T.: 5.258 min
Delta R.T.: 0.017 min
Response: 6213077
Conc: 1.30 ng/ml

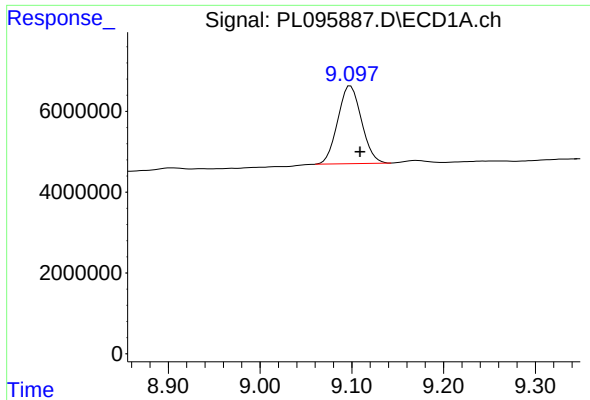

#28 Decachlorobiphenyl

R.T.: 9.099 min
Delta R.T.: -0.010 min
Response: 34605078
Conc: 14.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-25

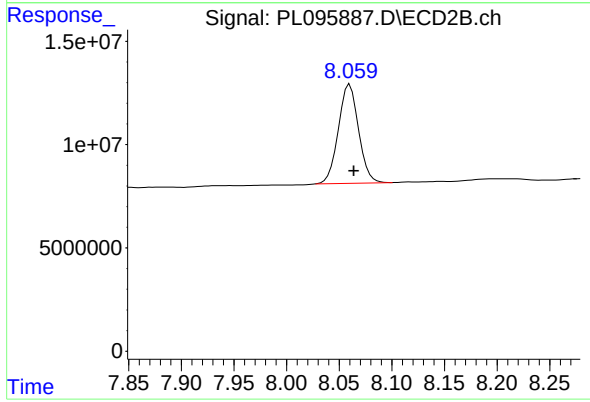

#28 Decachlorobiphenyl

R.T.: 8.060 min
Delta R.T.: -0.004 min
Response: 64097333
Conc: 14.65 ng/ml