

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060325\
 Data File : PL095890.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2025 15:22
 Operator : AR\AJ
 Sample : Q2176-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-26

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 01:36:50 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052125.M
 Quant Title : GC Extractables
 QLast Update : Thu May 22 06:29:30 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.573	2.886	38810193	49555817	12.300	12.661
28)	SA Decachlor...	9.100	8.059	26384854	36482705	11.197	8.340 #
Target Compounds							
4)	MA Heptachlor	4.979f	0.000	15641196	0	4.132	N.D. #
9)	A Endosulfan I	0.000	5.254	0	13613648	N.D.	2.857 #
10)	B gamma-Chl...	5.971	5.121	28271221	28328647	7.264	5.393 #
11)	B alpha-Chl...	6.056	5.184	51228252	48066727	12.975	9.239 #
12)	B 4,4'-DDE	6.225	5.371	7061202	21811564	1.925	4.068 #
15)	B Endosulfa...	0.000	6.079	0	5935818	N.D.	1.249 #
23)	Chlordane-1	4.738	3.904	7167551	17944757	40.232	92.033 #
24)	Chlordane-2	0.000	4.487	0	20081084	N.D.	90.150 #
25)	Chlordane-3	5.971	5.121	28271221	28328647	38.255	42.994
26)	Chlordane-4	6.056	5.184	51228252	48066727	56.997	84.193 #
27)	Chlordane-5	0.000	6.079	0	5935818	N.D.	23.284 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060325\
Data File : PL095890.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2025 15:22
Operator : AR\AJ
Sample : Q2176-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-26

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 01:36:50 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052125.M
Quant Title : GC Extractables
QLast Update : Thu May 22 06:29:30 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

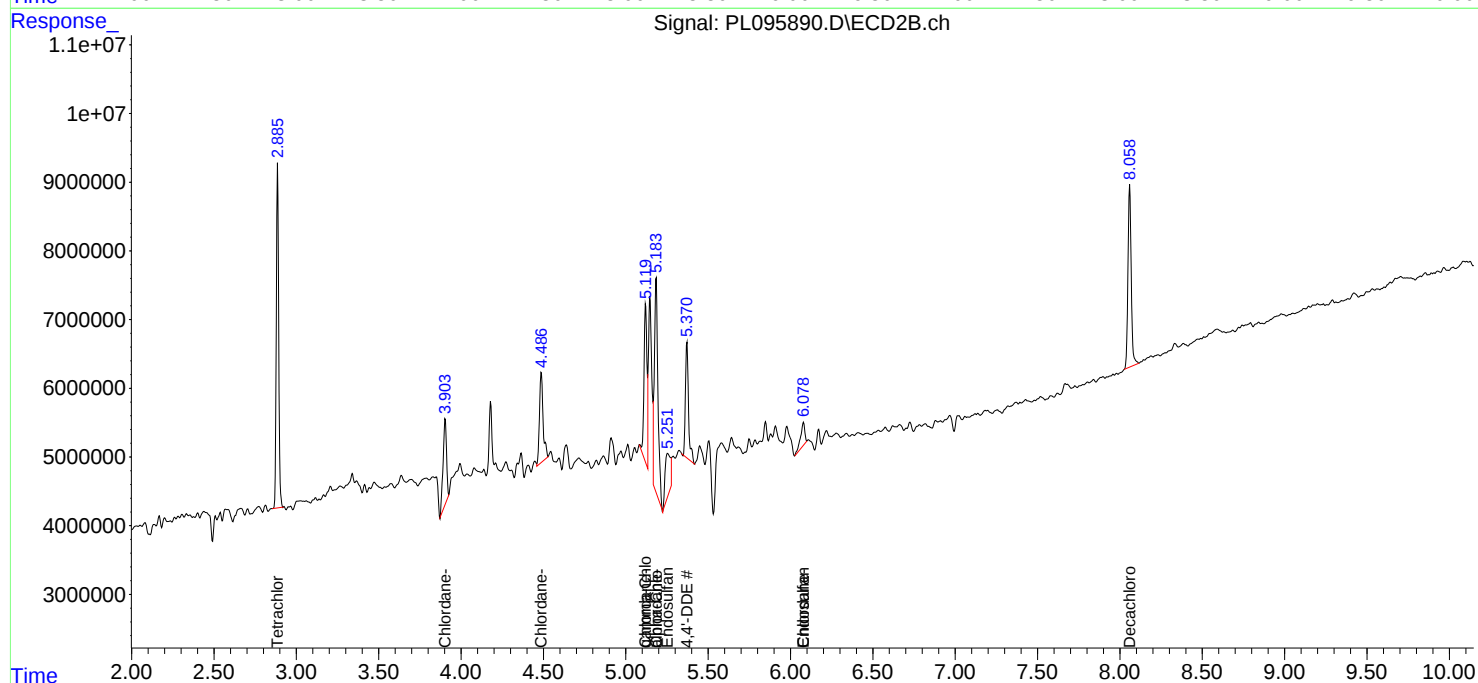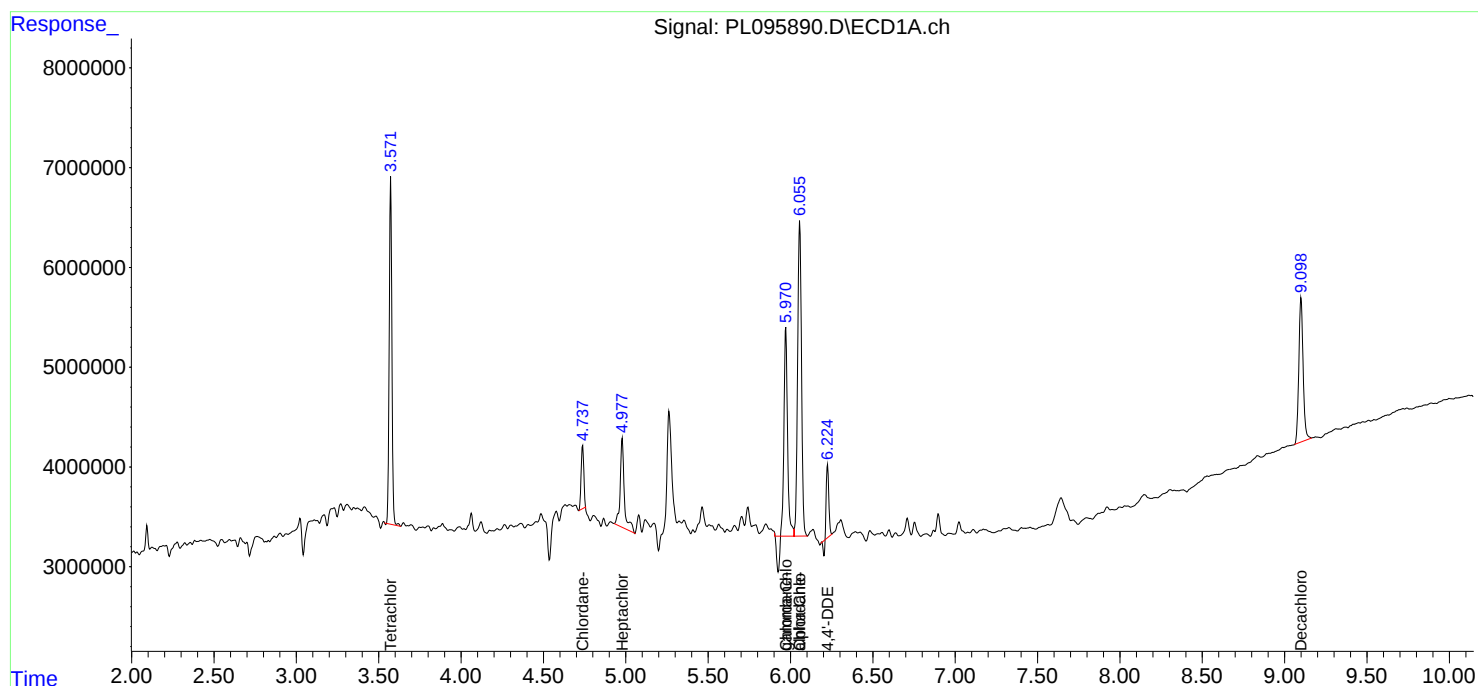


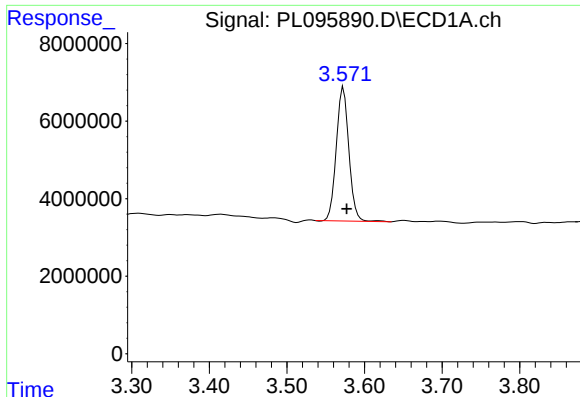

#1 Tetrachloro-m-xylene


R.T.: 3.573 min
Delta R.T.: -0.004 min
Response: 38810193
Conc: 12.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-26

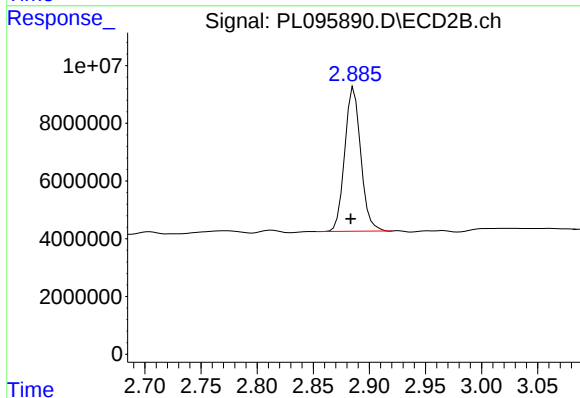


#1 Tetrachloro-m-xylene

R.T.: 2.886 min
Delta R.T.: 0.003 min
Response: 49555817
Conc: 12.66 ng/ml

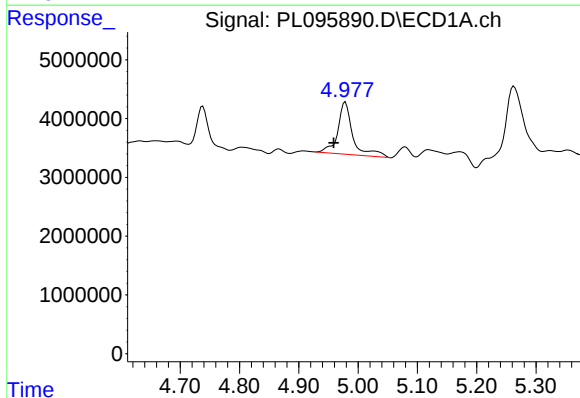


#4 Heptachlor

R.T.: 4.979 min
Delta R.T.: 0.020 min
Response: 15641196
Conc: 4.13 ng/ml

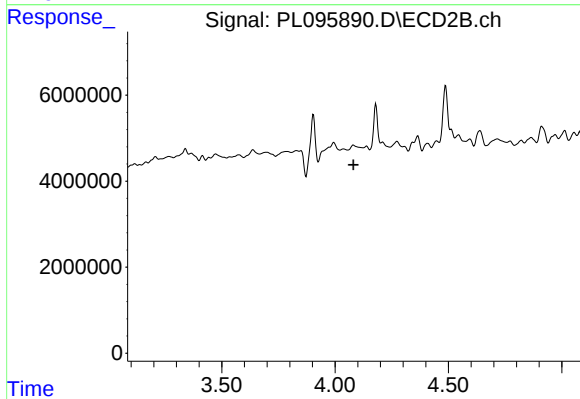

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.081 min
Response: 0
Conc: N.D.

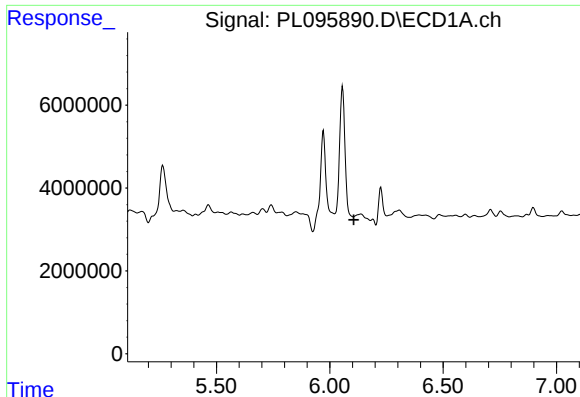

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.106 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-26

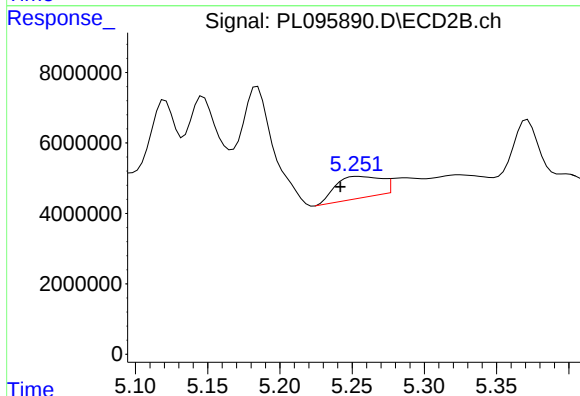


#9 Endosulfan I

R.T.: 5.254 min
Delta R.T.: 0.012 min
Response: 13613648
Conc: 2.86 ng/ml

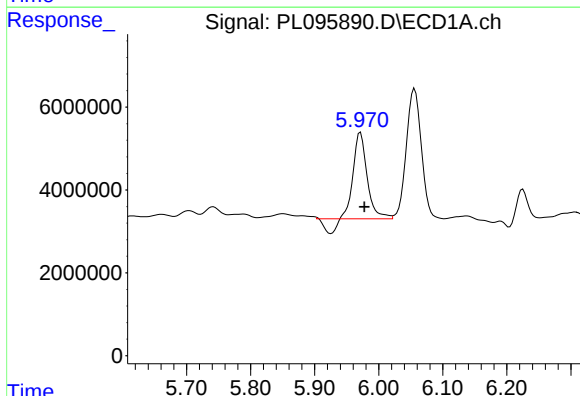


#10 gamma-Chlordane

R.T.: 5.971 min
Delta R.T.: -0.006 min
Response: 28271221
Conc: 7.26 ng/ml

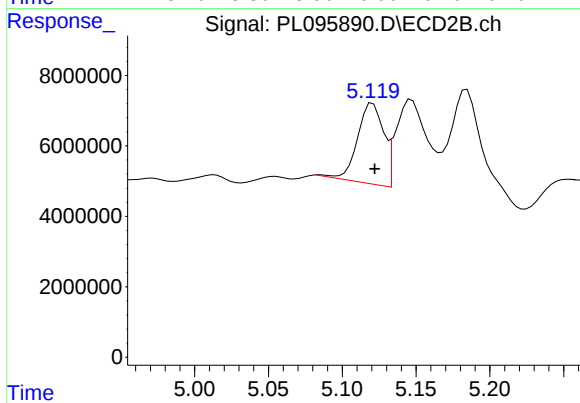

#10 gamma-Chlordane


R.T.: 5.121 min
Delta R.T.: -0.001 min
Response: 28328647
Conc: 5.39 ng/ml

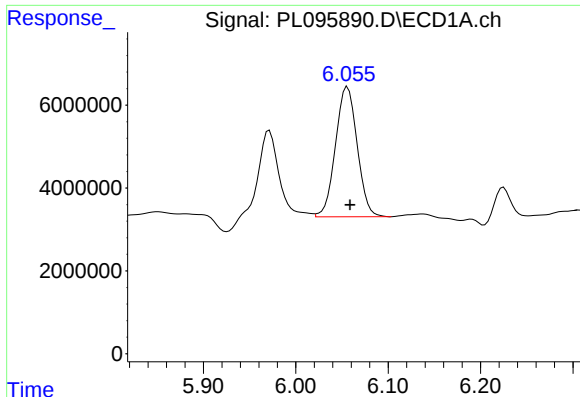

#11 alpha-Chlordane


R.T.: 6.056 min
Delta R.T.: -0.003 min
Response: 51228252
Conc: 12.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-26

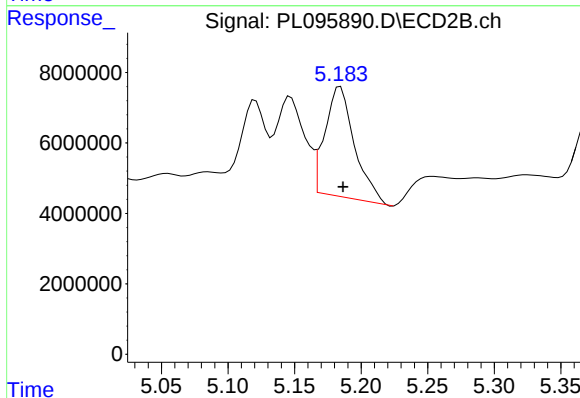


#11 alpha-Chlordane

R.T.: 5.184 min
Delta R.T.: -0.002 min
Response: 48066727
Conc: 9.24 ng/ml

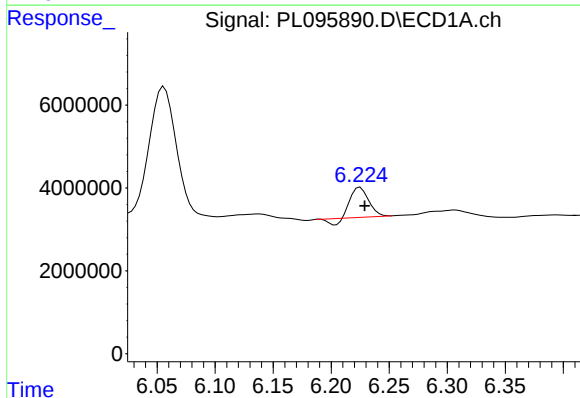


#12 4,4'-DDE

R.T.: 6.225 min
Delta R.T.: -0.004 min
Response: 7061202
Conc: 1.93 ng/ml

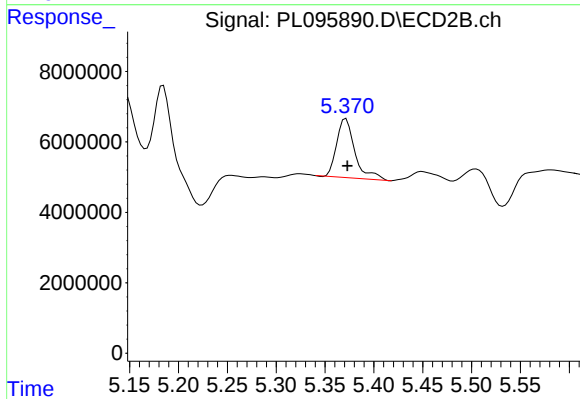

#12 4,4'-DDE


R.T.: 5.371 min
Delta R.T.: -0.002 min
Response: 21811564
Conc: 4.07 ng/ml

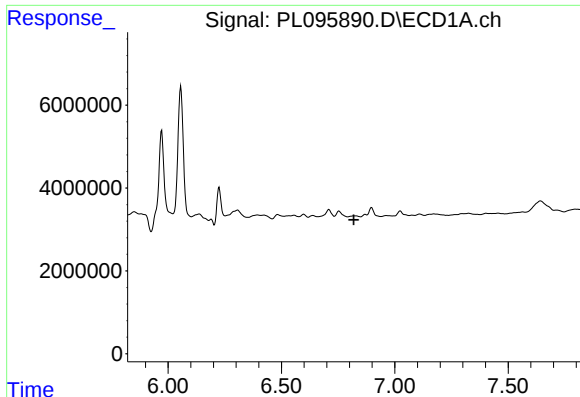

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.820 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-26

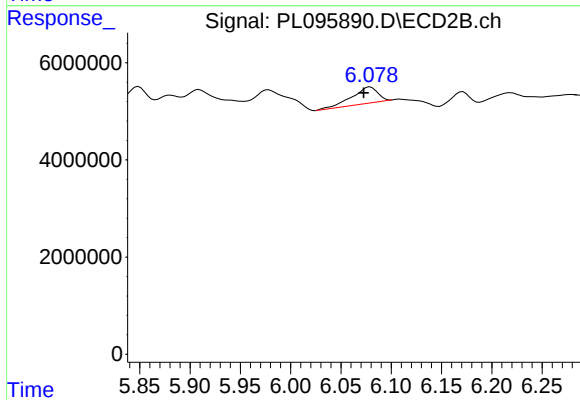


#15 Endosulfan II

R.T.: 6.079 min
Delta R.T.: 0.006 min
Response: 5935818
Conc: 1.25 ng/ml

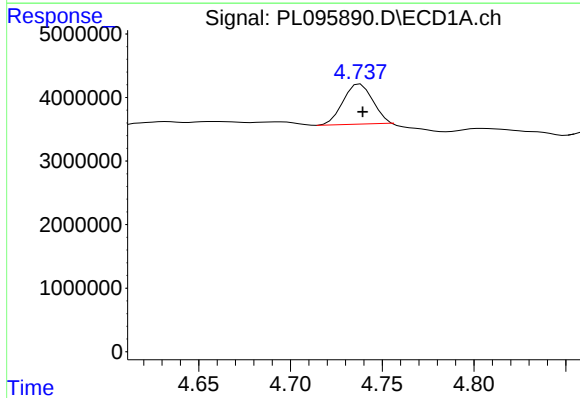


#23 Chlordane-1

R.T.: 4.738 min
Delta R.T.: -0.001 min
Response: 7167551
Conc: 40.23 ng/ml

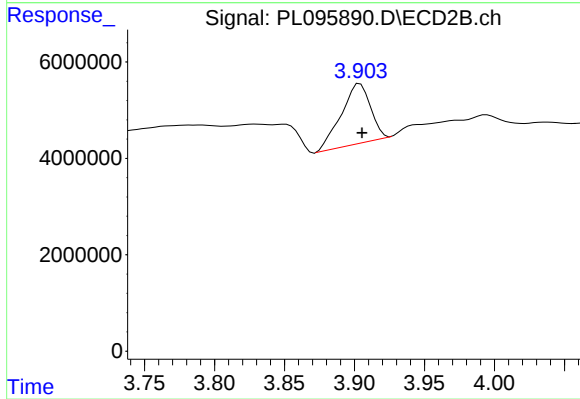

#23 Chlordane-1


R.T.: 3.904 min
Delta R.T.: -0.002 min
Response: 17944757
Conc: 92.03 ng/ml

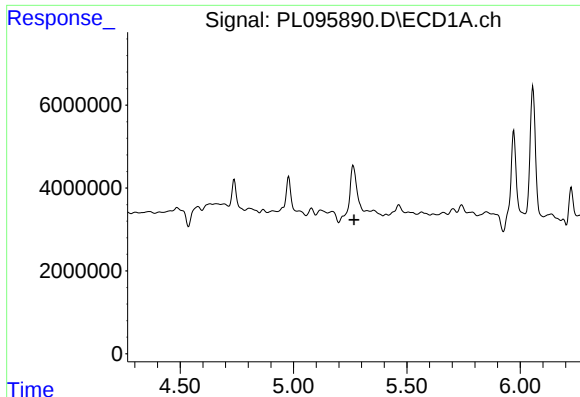

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.267 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-26

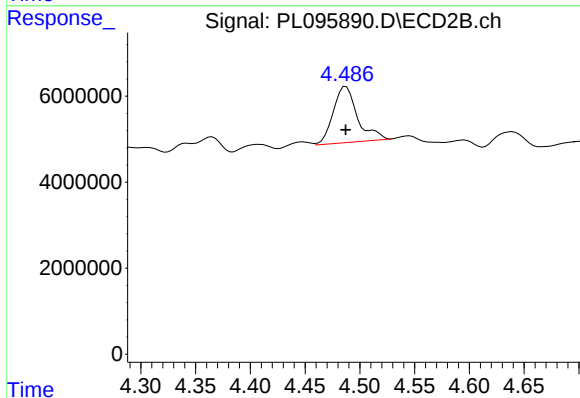


#24 Chlordane-2

R.T.: 4.487 min
Delta R.T.: 0.000 min
Response: 20081084
Conc: 90.15 ng/ml

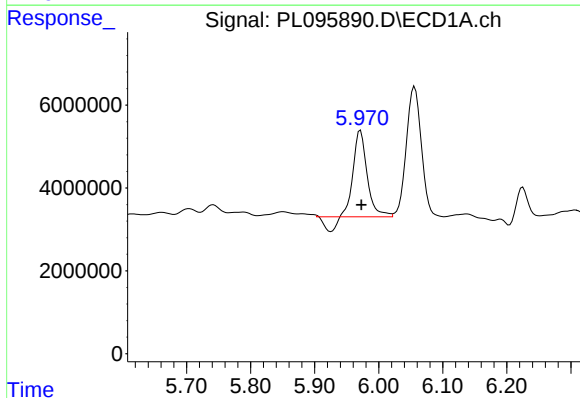


#25 Chlordane-3

R.T.: 5.971 min
Delta R.T.: -0.001 min
Response: 28271221
Conc: 38.25 ng/ml

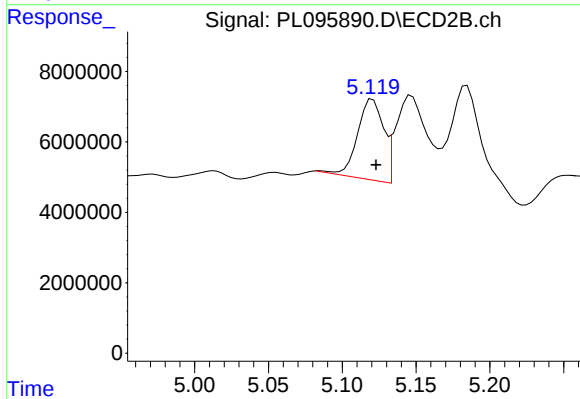

#25 Chlordane-3


R.T.: 5.121 min
Delta R.T.: -0.002 min
Response: 28328647
Conc: 42.99 ng/ml

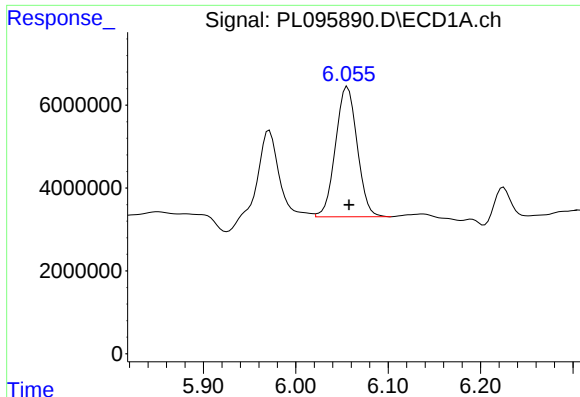

#26 Chlordane-4


R.T.: 6.056 min
Delta R.T.: -0.002 min
Response: 51228252
Conc: 57.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-26

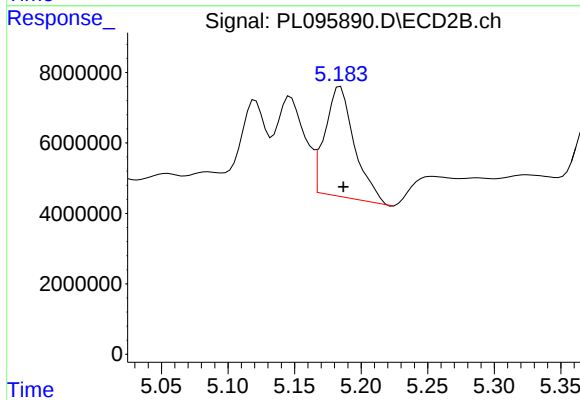


#26 Chlordane-4

R.T.: 5.184 min
Delta R.T.: -0.002 min
Response: 48066727
Conc: 84.19 ng/ml

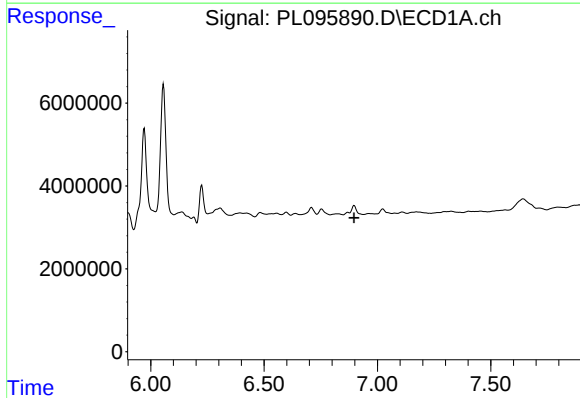


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.897 min
Response: 0
Conc: N.D.

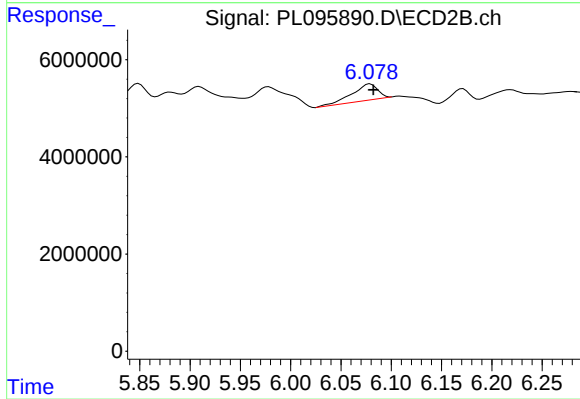

#27 Chlordane-5


R.T.: 6.079 min
Delta R.T.: -0.003 min
Response: 5935818
Conc: 23.28 ng/ml

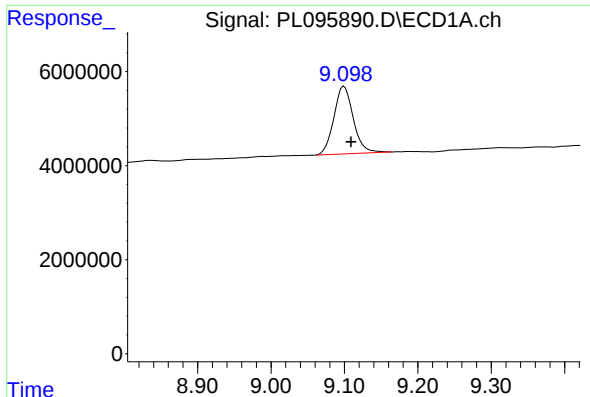

#28 Decachlorobiphenyl

R.T.: 9.100 min
Delta R.T.: -0.009 min
Response: 26384854
Conc: 11.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-26

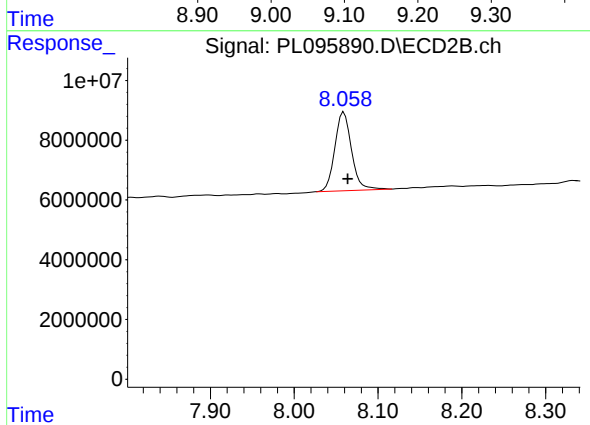

#28 Decachlorobiphenyl

R.T.: 8.059 min
Delta R.T.: -0.004 min
Response: 36482705
Conc: 8.34 ng/ml