

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL060325\  
 Data File : PL095910.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 03 Jun 2025 19:59  
 Operator : AR\AJ  
 Sample : Q217707  
 Misc :  
 ALS Vial : 29 Sample Multiplier: 1

Instrument :  
 ECD\_L  
 ClientSampleId :  
 B-202-SB01

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Jun 04 03:40:51 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL052125.M  
 Quant Title : GC Extractables  
 QLast Update : Thu May 22 06:29:30 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

|                             | Compound        | RT#1   | RT#2   | Resp#1   | Resp#2   | ng/ml  | ng/ml    |
|-----------------------------|-----------------|--------|--------|----------|----------|--------|----------|
| -----                       |                 |        |        |          |          |        |          |
| System Monitoring Compounds |                 |        |        |          |          |        |          |
| 1)                          | SA Tetrachlo... | 3.572  | 2.885  | 58846542 | 71932684 | 18.650 | 18.379   |
| 28)                         | SA Decachlor... | 9.097  | 8.059  | 43981730 | 84681385 | 18.665 | 19.358   |
| Target Compounds            |                 |        |        |          |          |        |          |
| 9)                          | A Endosulfan I  | 6.123f | 5.259f | 7329364  | 7389752  | 2.000  | 1.551    |
| 10)                         | B gamma-Chl...  | 0.000  | 5.102f | 0        | 6590633  | N.D.   | 1.255 #  |
| 13)                         | MA Dieldrin     | 0.000  | 5.504  | 0        | 8166876  | N.D.   | 1.541 #  |
| 15)                         | B Endosulfa...  | 0.000  | 6.049f | 0        | 4308864  | N.D.   | 0.907 #  |
| 23)                         | Chlordane-1     | 0.000  | 3.903  | 0        | 17669321 | N.D.   | 90.621 # |
| 25)                         | Chlordane-3     | 0.000  | 5.102f | 0        | 6590633  | N.D.   | 10.002 # |
| 27)                         | Chlordane-5     | 0.000  | 6.049f | 0        | 4308864  | N.D.   | 16.902 # |
| -----                       |                 |        |        |          |          |        |          |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL060325\  
Data File : PL095910.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 03 Jun 2025 19:59  
Operator : AR\AJ  
Sample : Q217707  
Misc :  
ALS Vial : 29 Sample Multiplier: 1

Instrument :  
ECD\_L  
ClientSampleId :  
B-202-SB01

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Jun 04 03:40:51 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL052125.M  
Quant Title : GC Extractables  
QLast Update : Thu May 22 06:29:30 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

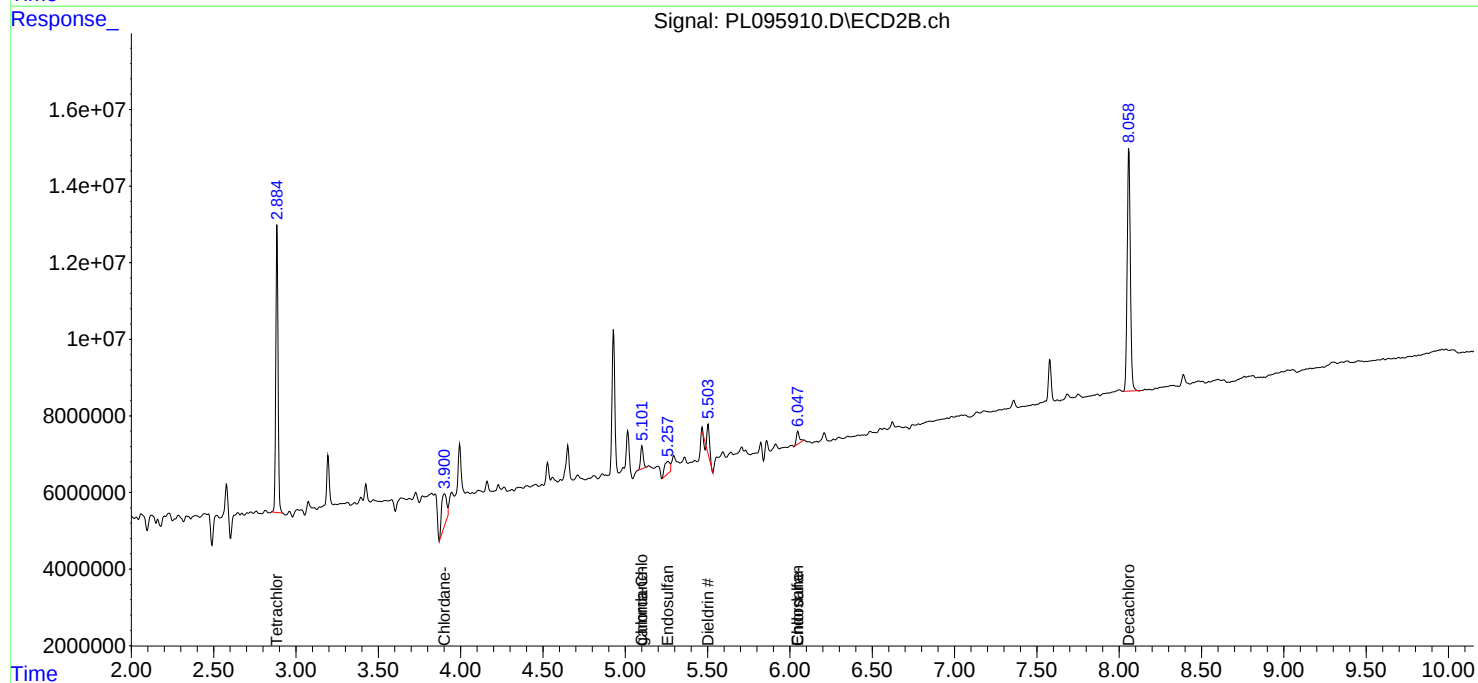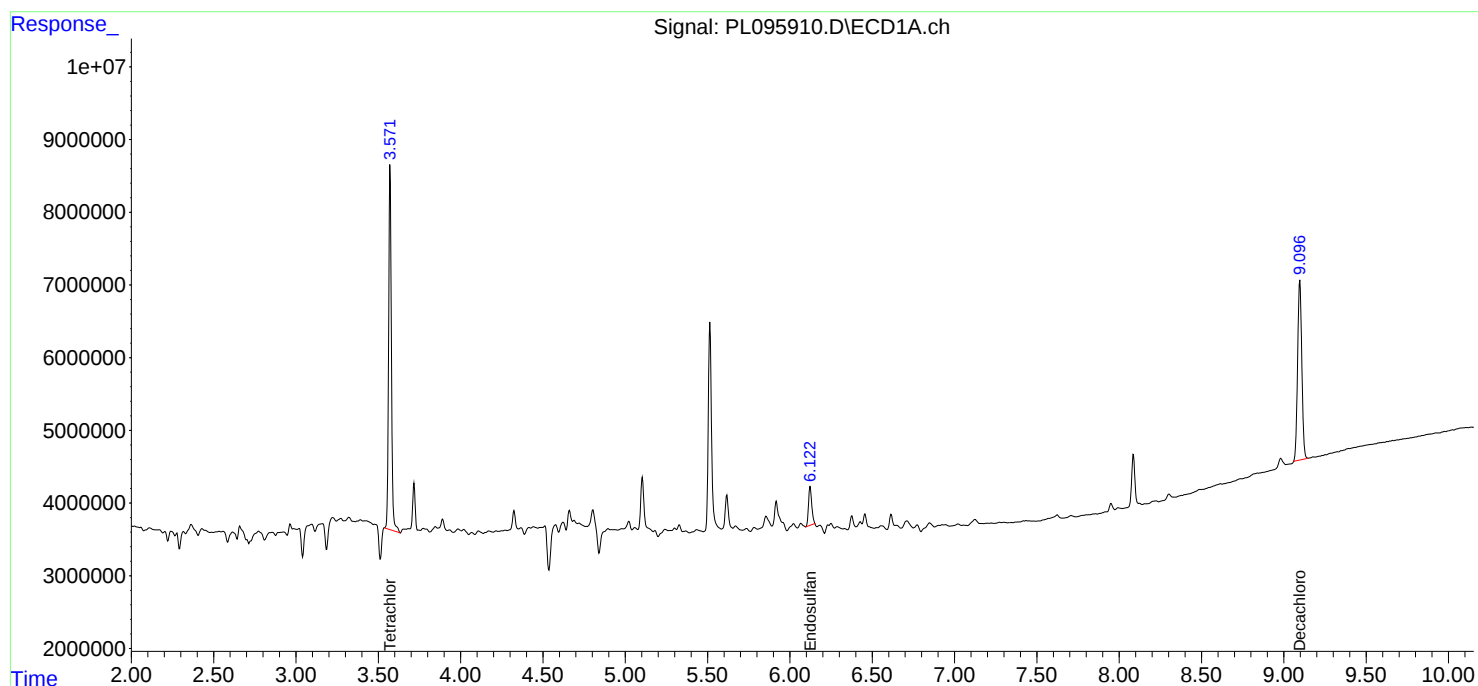


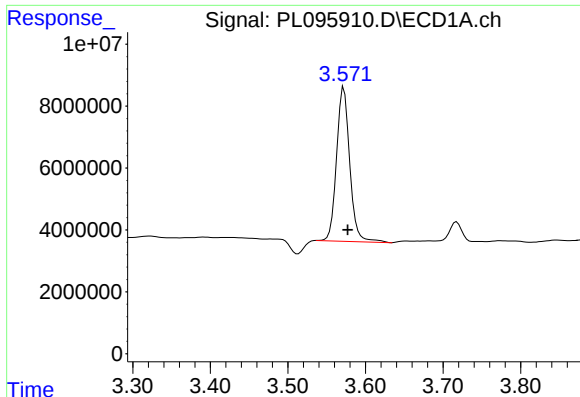

#1 Tetrachloro-m-xylene


R.T.: 3.572 min  
Delta R.T.: -0.005 min  
Response: 58846542  
Conc: 18.65 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :  
B-202-SB01

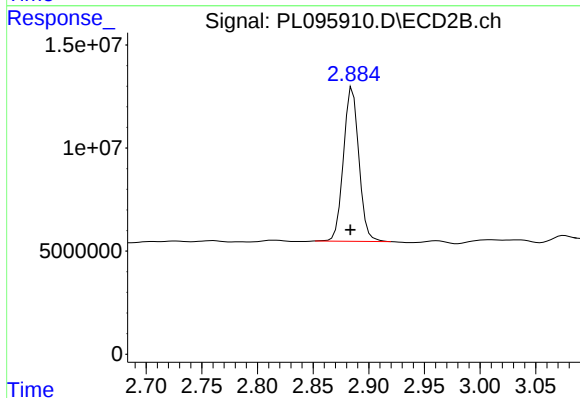


#1 Tetrachloro-m-xylene

R.T.: 2.885 min  
Delta R.T.: 0.002 min  
Response: 71932684  
Conc: 18.38 ng/ml

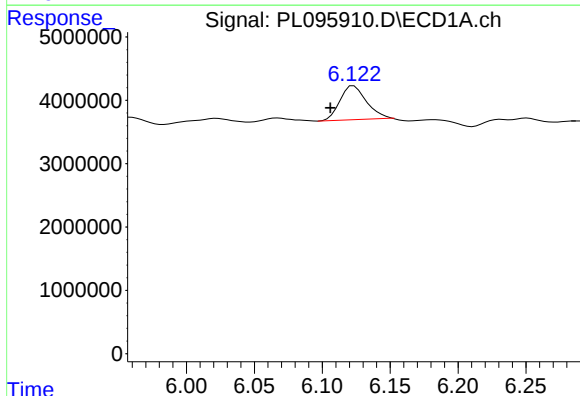


#9 Endosulfan I

R.T.: 6.123 min  
Delta R.T.: 0.017 min  
Response: 7329364  
Conc: 2.00 ng/ml

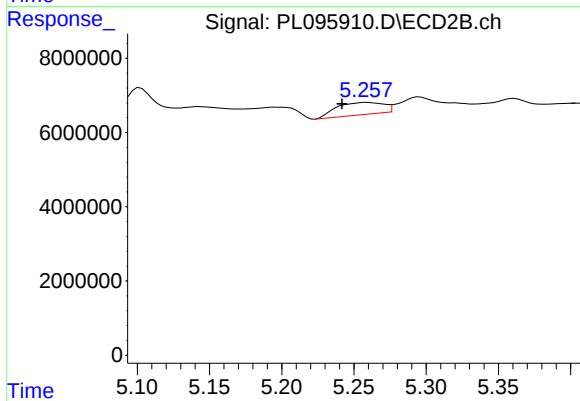

#9 Endosulfan I


R.T.: 5.259 min  
Delta R.T.: 0.017 min  
Response: 7389752  
Conc: 1.55 ng/ml

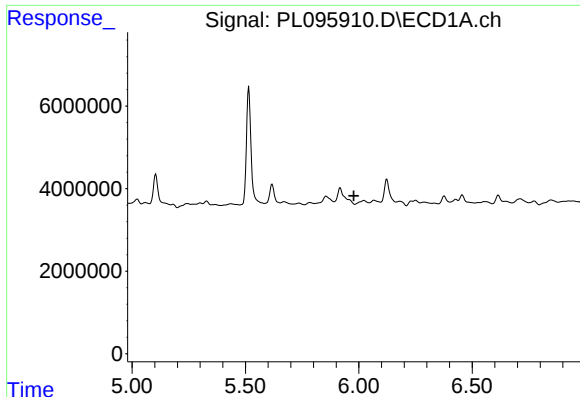

#10 gamma-Chlordane


R.T.: 0.000 min  
Exp R.T.: 5.977 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_L  
ClientSampleId :  
B-202-SB01

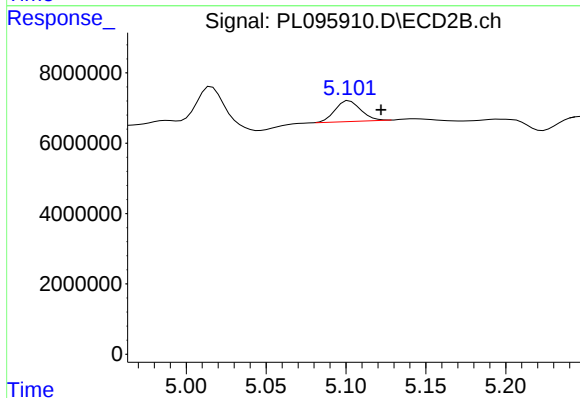


#10 gamma-Chlordane

R.T.: 5.102 min  
Delta R.T.: -0.020 min  
Response: 6590633  
Conc: 1.25 ng/ml

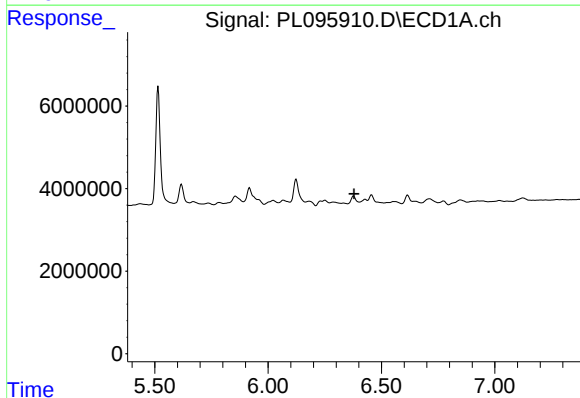


#13 Dieldrin

R.T.: 0.000 min  
Exp R.T.: 6.379 min  
Response: 0  
Conc: N.D.

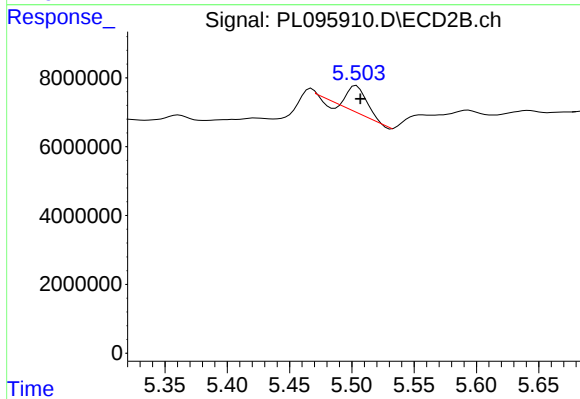

#13 Dieldrin


R.T.: 5.504 min  
Delta R.T.: -0.003 min  
Response: 8166876  
Conc: 1.54 ng/ml

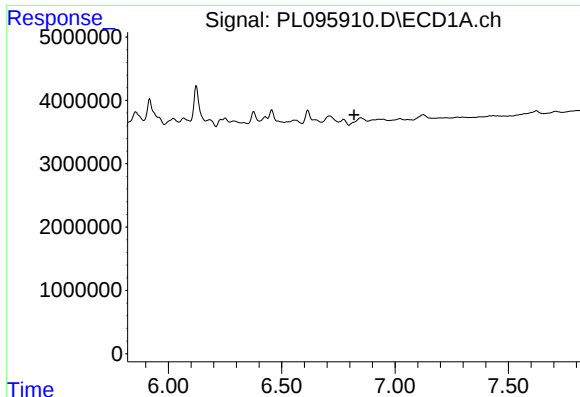

#15 Endosulfan II


R.T.: 0.000 min  
Exp R.T.: 6.820 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_L  
ClientSampleId :  
B-202-SB01

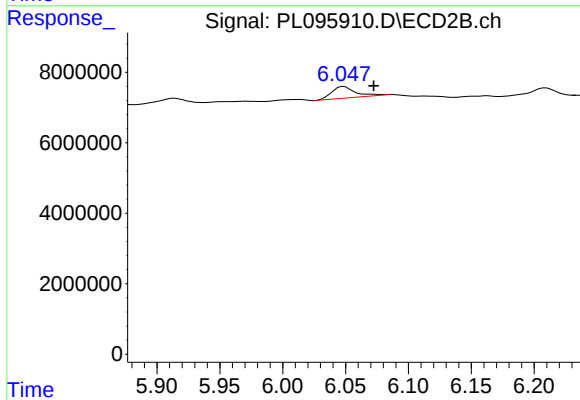


#15 Endosulfan II

R.T.: 6.049 min  
Delta R.T.: -0.024 min  
Response: 4308864  
Conc: 0.91 ng/ml

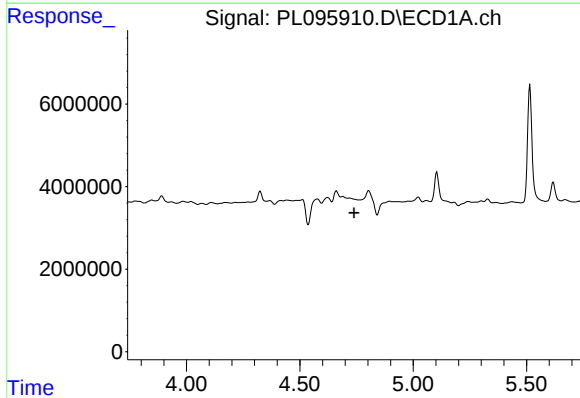


#23 Chlordane-1

R.T.: 0.000 min  
Exp R.T.: 4.739 min  
Response: 0  
Conc: N.D.

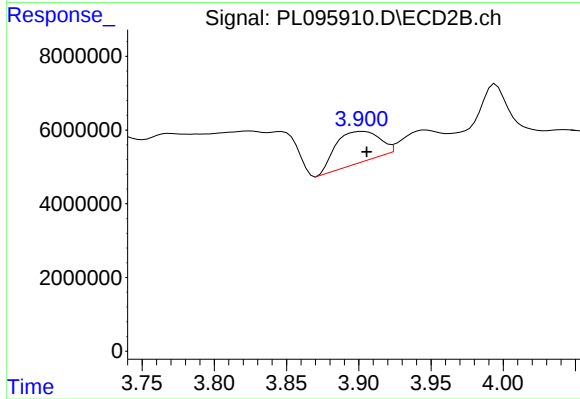

#23 Chlordane-1


R.T.: 3.903 min  
Delta R.T.: -0.003 min  
Response: 17669321  
Conc: 90.62 ng/ml

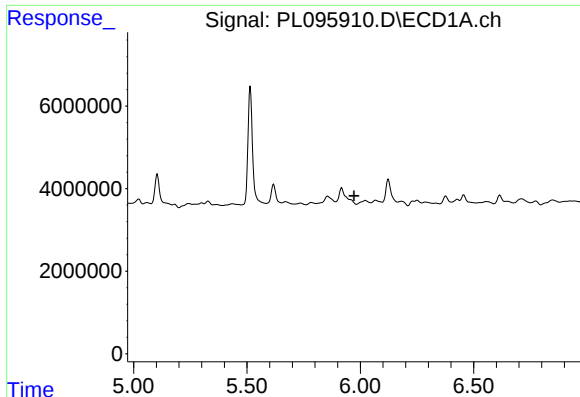

#25 Chlordane-3


R.T.: 0.000 min  
Exp R.T.: 5.973 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_L  
ClientSampleId :  
B-202-SB01

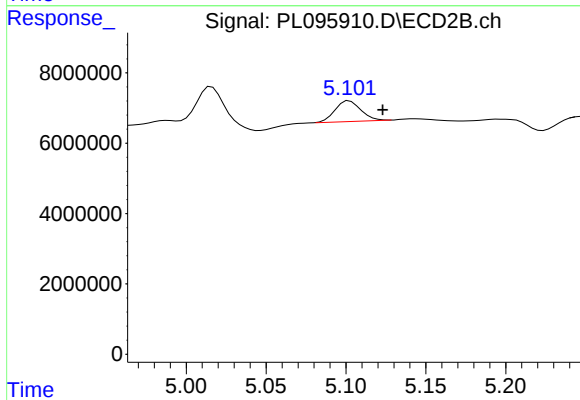


#25 Chlordane-3

R.T.: 5.102 min  
Delta R.T.: -0.021 min  
Response: 6590633  
Conc: 10.00 ng/ml

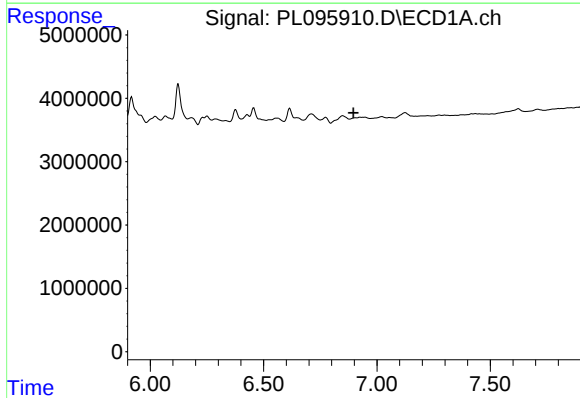


#27 Chlordane-5

R.T.: 0.000 min  
Exp R.T.: 6.897 min  
Response: 0  
Conc: N.D.

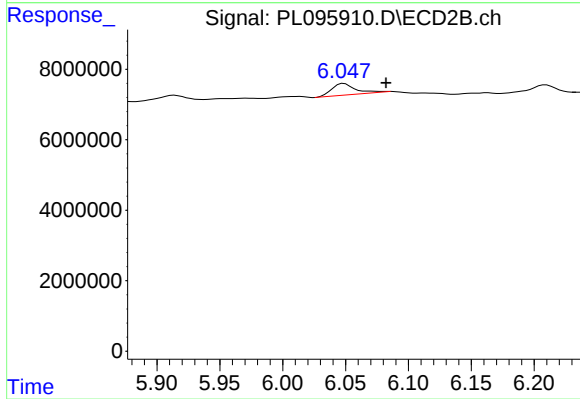

#27 Chlordane-5


R.T.: 6.049 min  
Delta R.T.: -0.034 min  
Response: 4308864  
Conc: 16.90 ng/ml

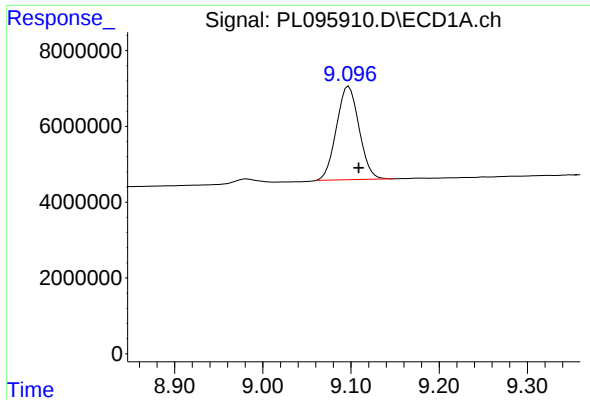

#28 Decachlorobiphenyl

R.T.: 9.097 min  
Delta R.T.: -0.012 min  
Response: 43981730  
Conc: 18.67 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :  
B-202-SB01

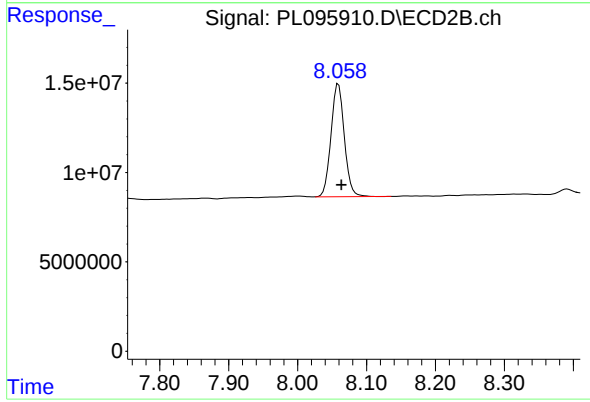

#28 Decachlorobiphenyl

R.T.: 8.059 min  
Delta R.T.: -0.004 min  
Response: 84681385  
Conc: 19.36 ng/ml