

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060325\
 Data File : PL095901.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2025 17:57
 Operator : AR\AJ
 Sample : Q2173-18
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OR-400-CF-402B-COMP-25

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 06/04/2025
 Supervised By :mohammad ahmed 06/05/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 03:39:46 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052125.M
 Quant Title : GC Extractables
 QLast Update : Thu May 22 06:29:30 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.574	2.885	52022624	66607421	16.488	17.018
28) SA Decachlor...	9.099	8.054	37083031	193.8E6	15.738	44.292m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060325\
Data File : PL095901.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2025 17:57
Operator : AR\AJ
Sample : Q2173-18
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
OR-400-CF-402B-COMP-25


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 06/04/2025
Supervised By : mohammad ahmed 06/05/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 03:39:46 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052125.M
Quant Title : GC Extractables
QLast Update : Thu May 22 06:29:30 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

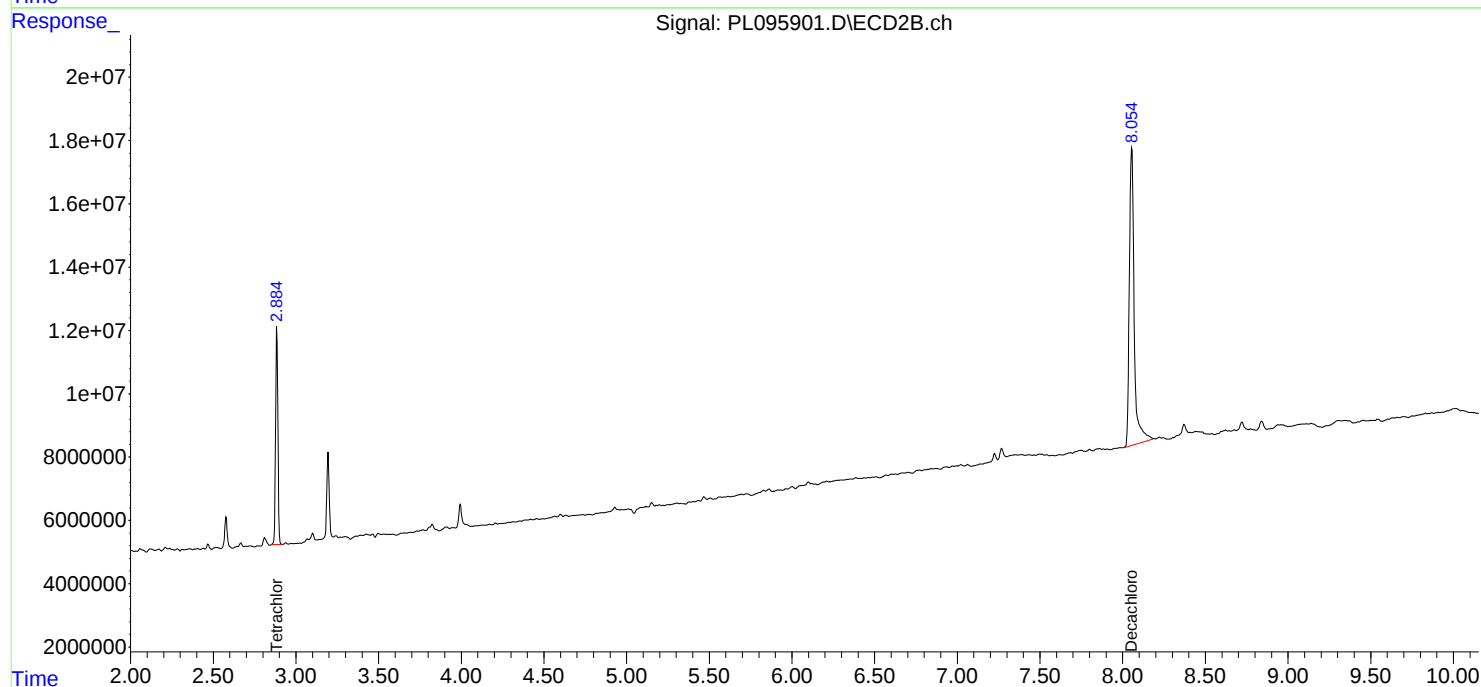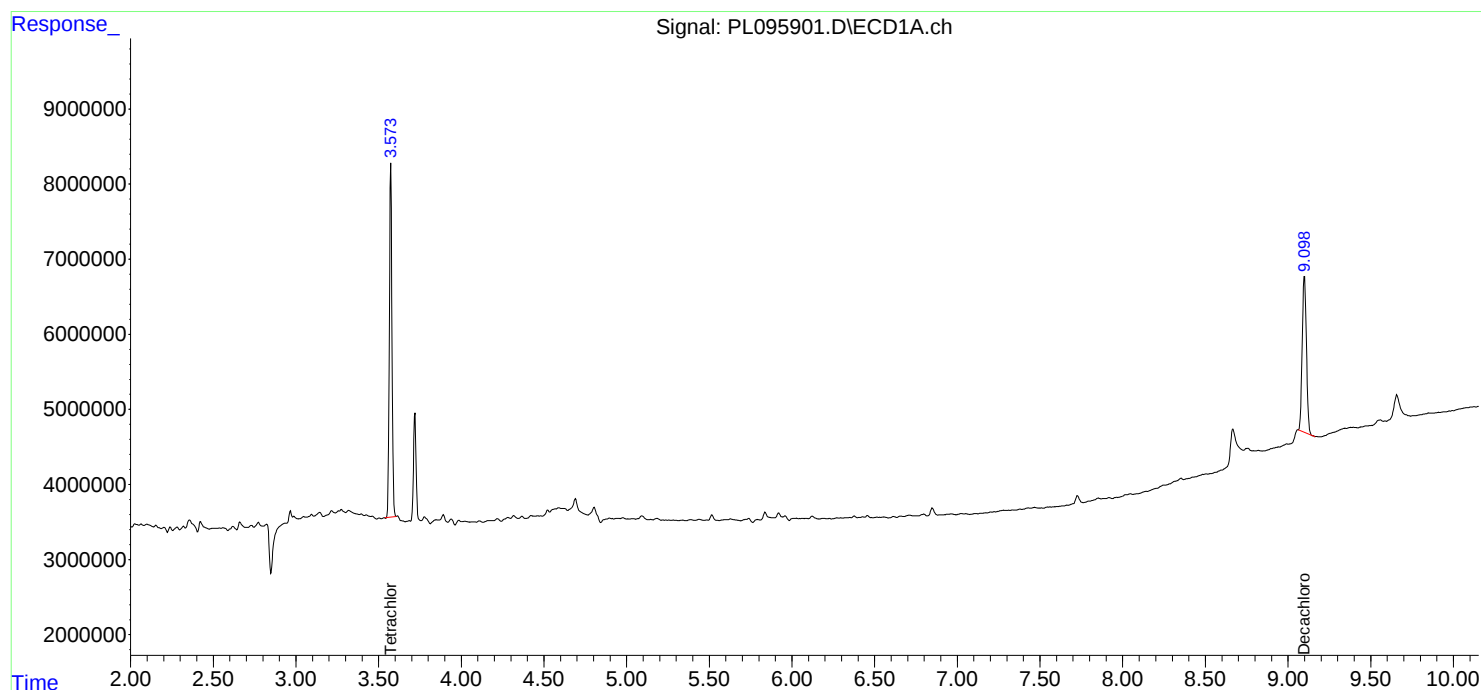

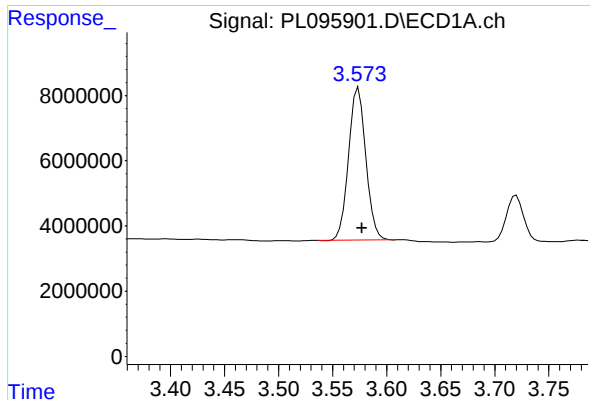


#1 Tetrachloro-m-xylene

R.T.: 3.574 min
Delta R.T.: -0.003 min
Response: 52022624
Conc: 16.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-400-CF-402B-COMP-25


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/04/2025
Supervised By :mohammad ahmed 06/05/2025

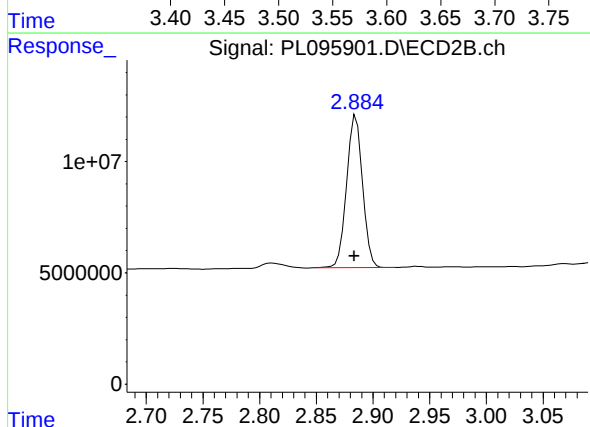


#1 Tetrachloro-m-xylene

R.T.: 2.885 min
Delta R.T.: 0.002 min
Response: 66607421
Conc: 17.02 ng/ml

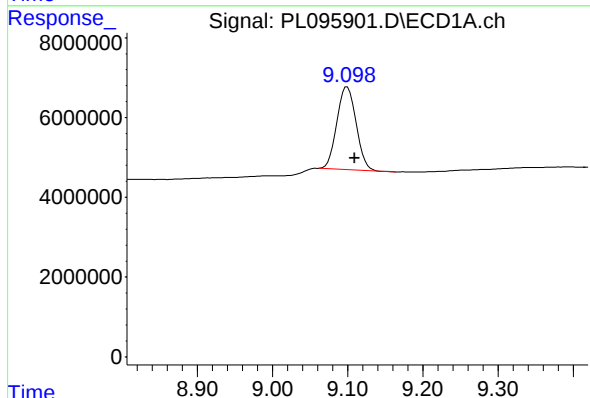

#28 Decachlorobiphenyl

R.T.: 9.099 min
Delta R.T.: -0.010 min
Response: 37083031
Conc: 15.74 ng/ml

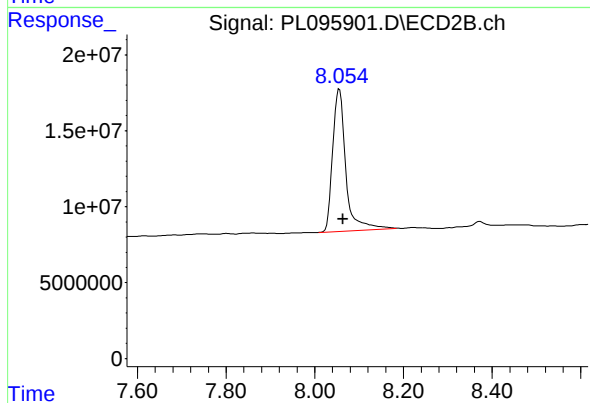

#28 Decachlorobiphenyl

R.T.: 8.054 min
Delta R.T.: -0.010 min
Response: 193754349
Conc: 44.29 ng/ml m