

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060419\
 Data File : PL049243.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jun 2019 08:29
 Operator : SM\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 10:43:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
 Quant Title : GC Extractables
 QLast Update : Fri May 31 01:35:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

6) B	beta-BHC	0.000	4.784	0	1487410	N.D.	0.864 #
8) B	Heptachlo...	0.000	5.798	0	23613603	N.D.	7.224 #
14) MA	Endrin	5.826	0.000	8338575	0	0.578	N.D. #
16) A	4,4'-DDD	0.000	6.759	0	1820854	N.D.	0.692 #
20) A	Methoxychlor	6.706f	0.000	7607502	0	1.186	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060419\
Data File : PL049243.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jun 2019 08:29
Operator : SM\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 10:43:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
Quant Title : GC Extractables
QLast Update : Fri May 31 01:35:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

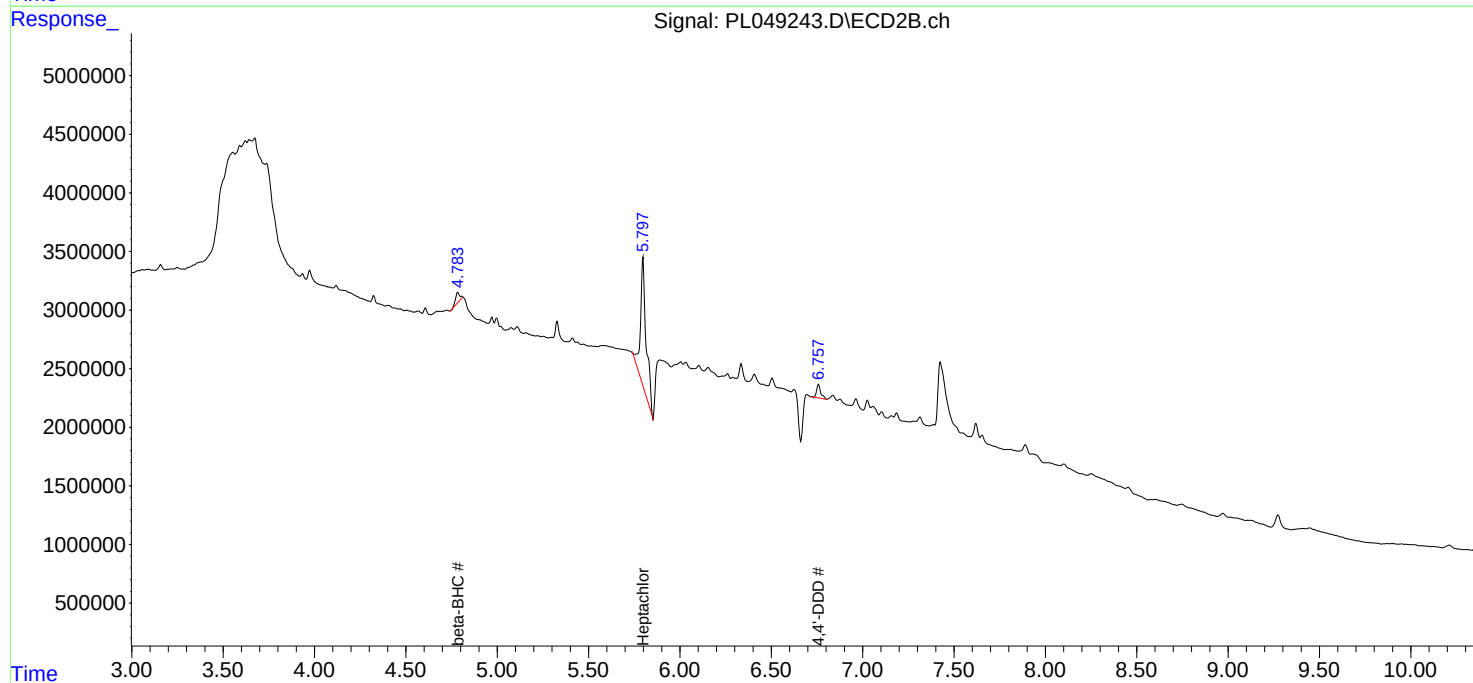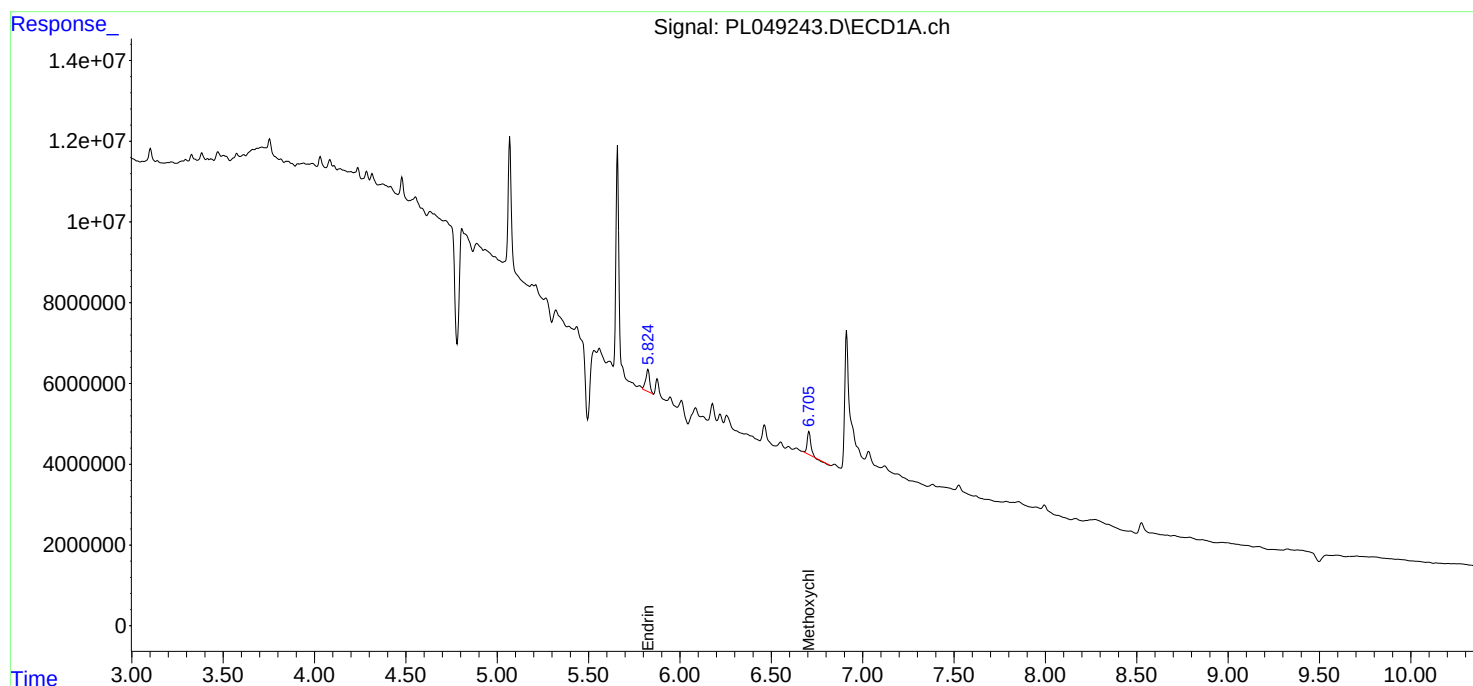


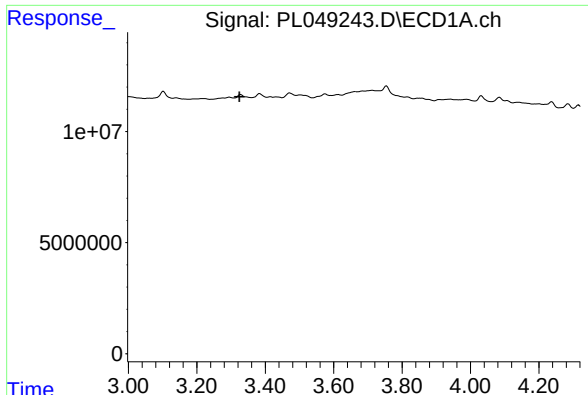

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.324 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

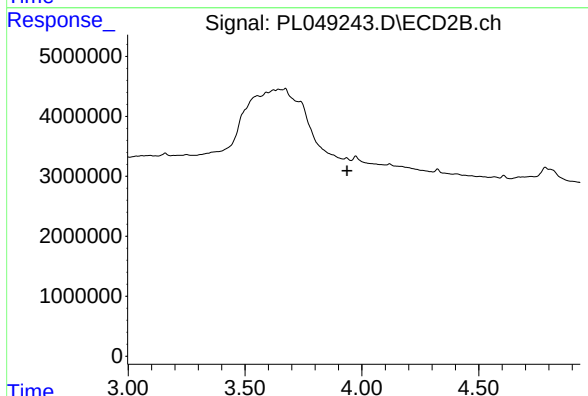


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.936 min
Response: 0
Conc: N.D.

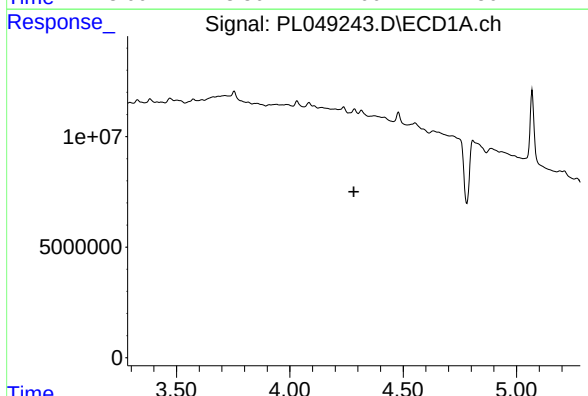


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.282 min
Response: 0
Conc: N.D.

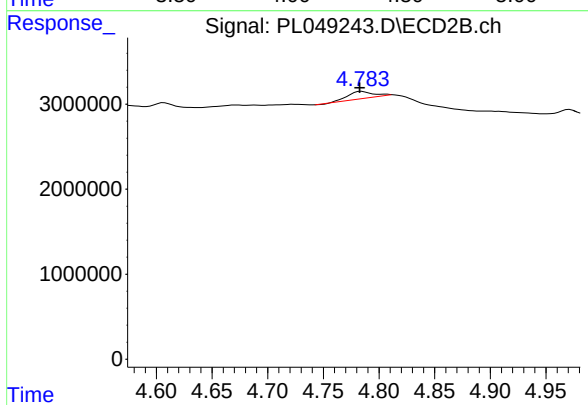

#6 beta-BHC


R.T.: 4.784 min
Delta R.T.: 0.002 min
Response: 1487410
Conc: 0.86 ng/ml

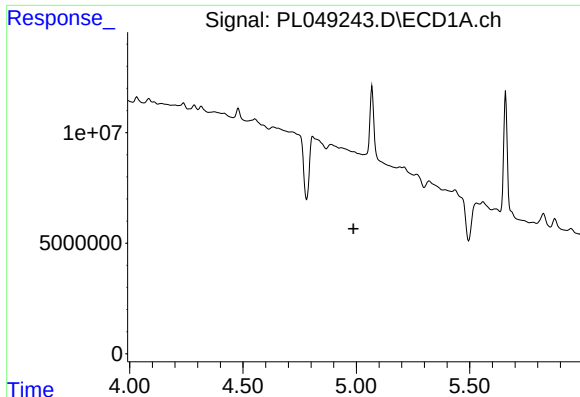

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.988 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

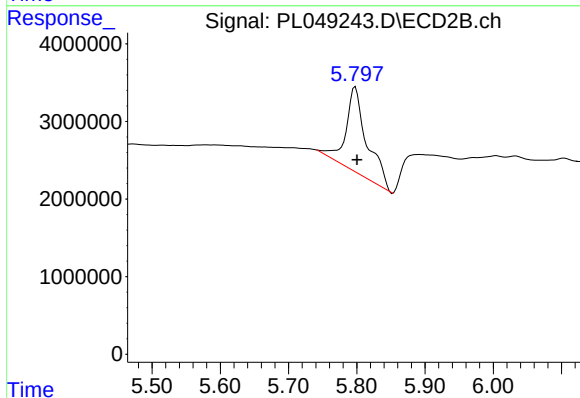


#8 Heptachlor epoxide

R.T.: 5.798 min
Delta R.T.: -0.003 min
Response: 23613603
Conc: 7.22 ng/ml

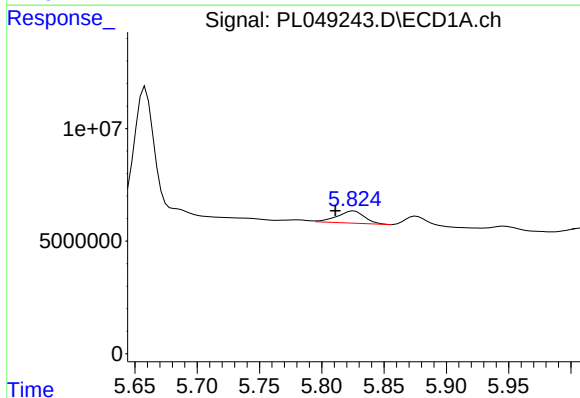


#14 Endrin

R.T.: 5.826 min
Delta R.T.: 0.015 min
Response: 8338575
Conc: 0.58 ng/ml

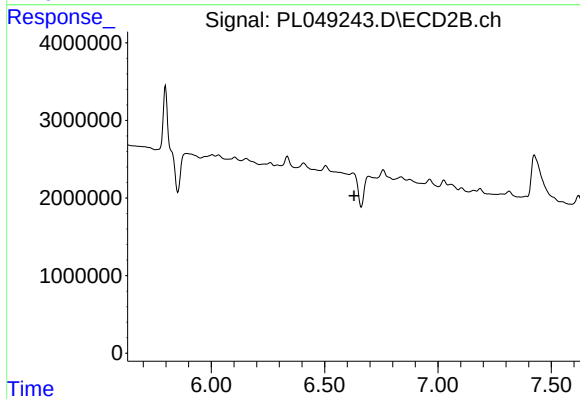

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.630 min
Response: 0
Conc: N.D.

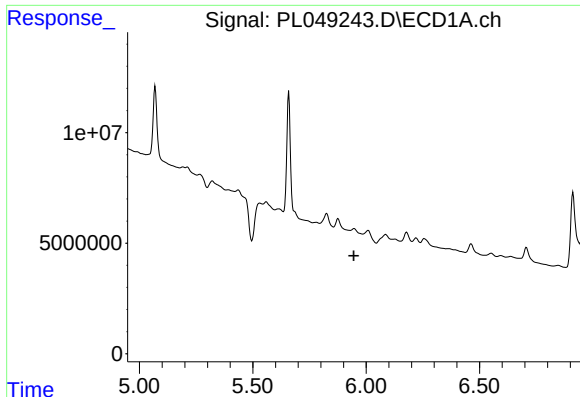

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.945 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

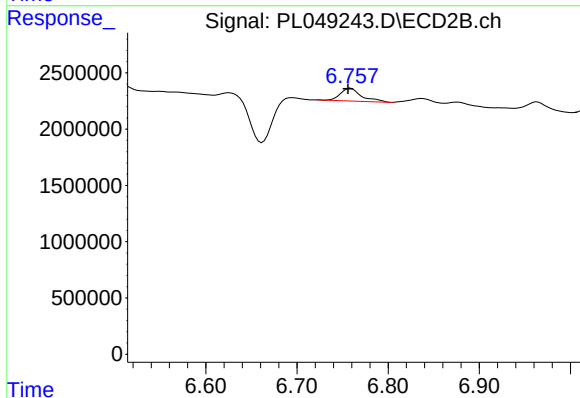


#16 4,4'-DDD

R.T.: 6.759 min
Delta R.T.: 0.003 min
Response: 1820854
Conc: 0.69 ng/ml

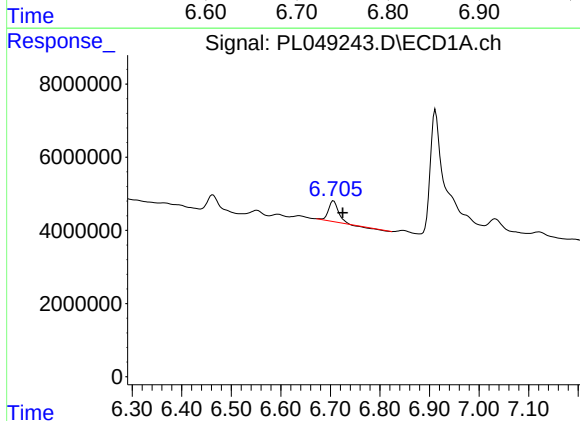


#20 Methoxychlor

R.T.: 6.706 min
Delta R.T.: -0.018 min
Response: 7607502
Conc: 1.19 ng/ml

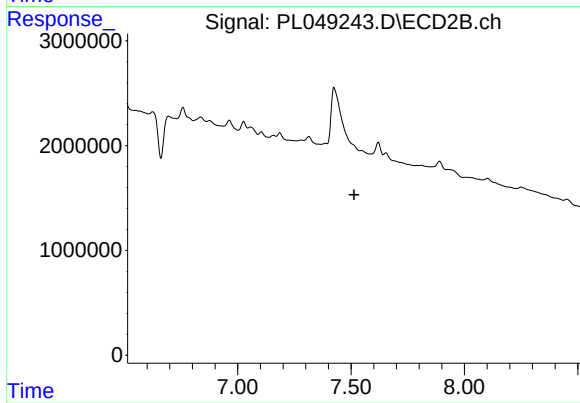

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.514 min
Response: 0
Conc: N.D.

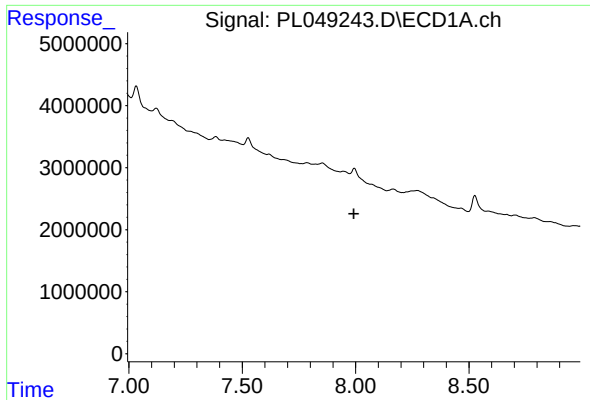

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.992 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

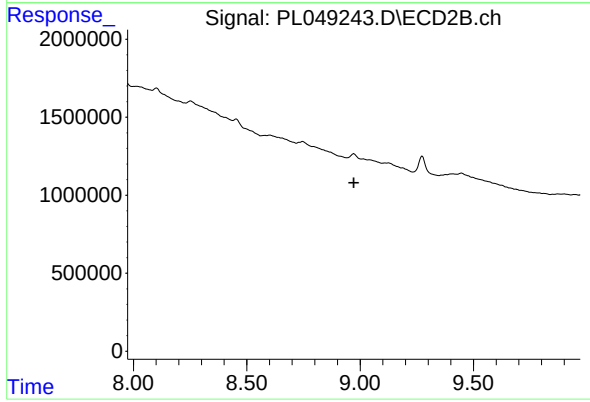

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.972 min
Response: 0
Conc: N.D.