

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060419\
 Data File : PL049264.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jun 2019 15:55
 Operator : SM\AJ
 Sample : K2641-15
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CL-02-053119-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 01:15:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
 Quant Title : GC Extractables
 QLast Update : Fri May 31 01:35:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.323	3.935	187.3E6	51756767	17.001	17.915
28)	SA Decachlor...	7.990	8.970	198.4E6	64388589	15.605	19.280
Target Compounds							
4)	MA Heptachlor	0.000	5.132f	0	4035506	N.D.	1.004 #
8)	B Heptachlo...	0.000	5.796	0	547012	N.D.	0.167 #
10)	B gamma-Chl...	5.210	6.033	16521566	7742190	1.035	2.238 #
11)	B alpha-Chl...	5.264	6.106	47011278	23195236	3.009	6.686 #
12)	B 4,4'-DDE	5.432	6.264	72584326	19012092	4.640	5.792
17)	MA 4,4'-DDT	6.177	7.051	14480962	4714841	1.176	1.682 #
22)	Mirex	0.000	8.132f	0	2262328	N.D.	0.871 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060419\
Data File : PL049264.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jun 2019 15:55
Operator : SM\AJ
Sample : K2641-15
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
CL-02-053119-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 01:15:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
Quant Title : GC Extractables
QLast Update : Fri May 31 01:35:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

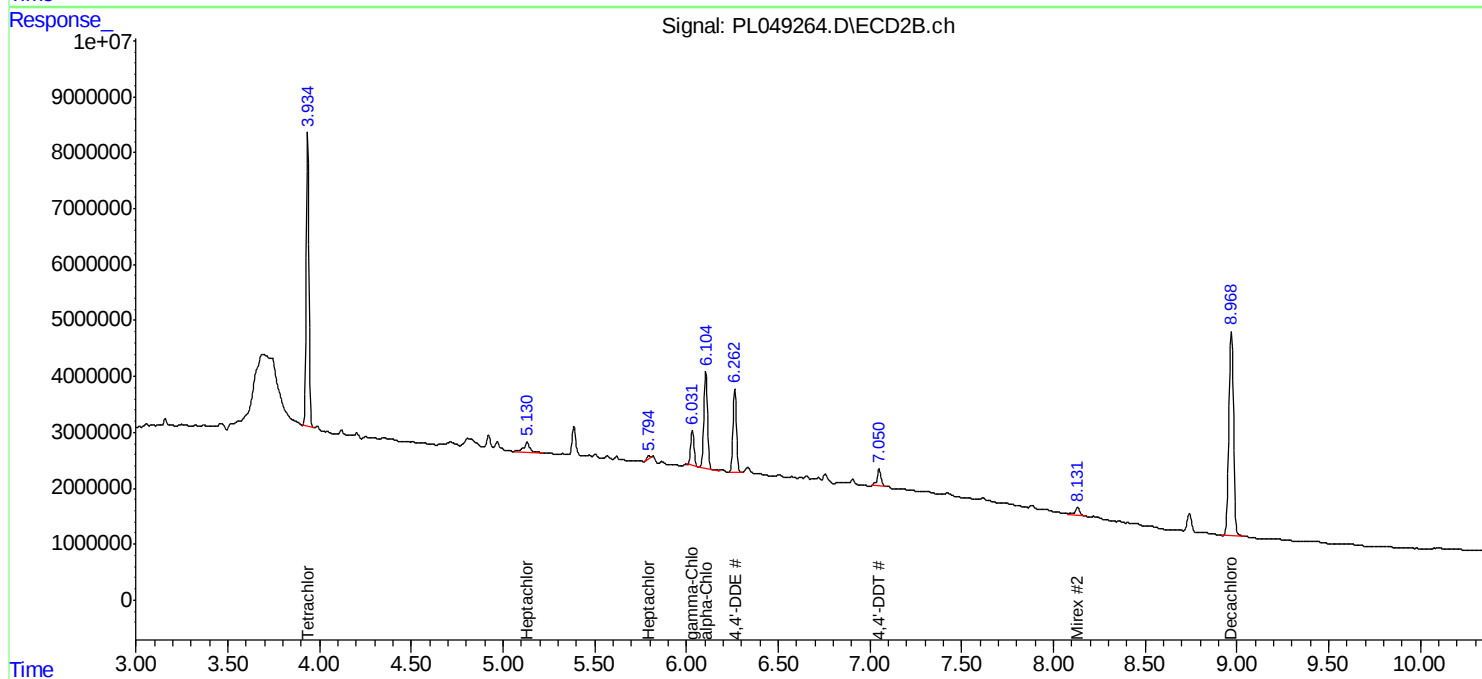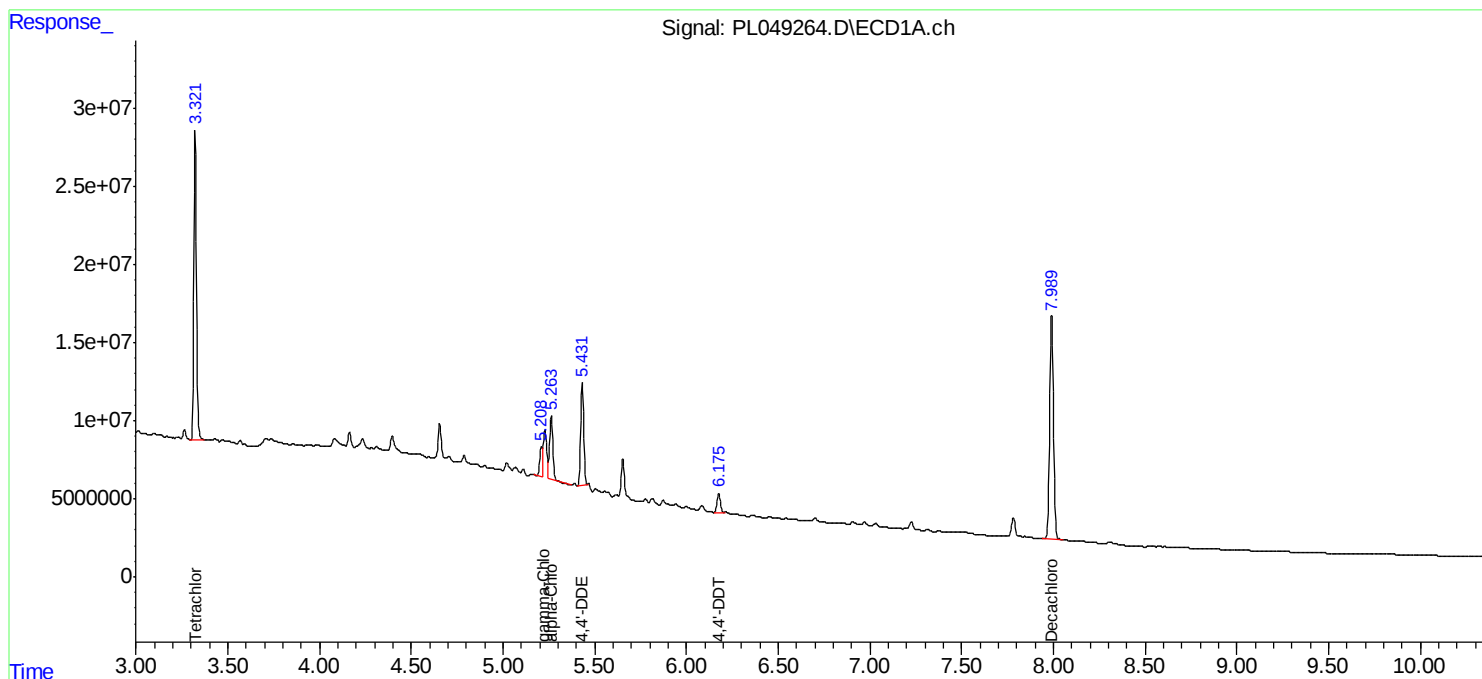


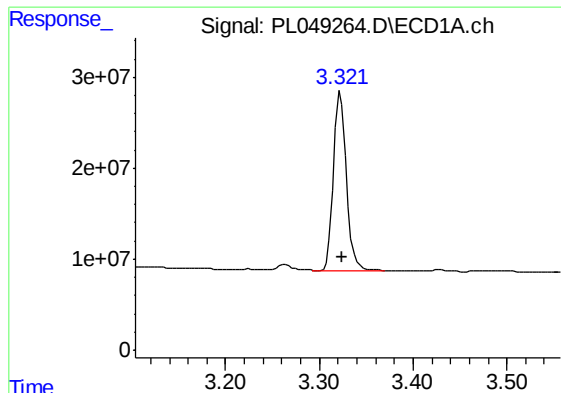

#1 Tetrachloro-m-xylene


R.T.: 3.323 min
Delta R.T.: -0.001 min
Response: 187327718
Conc: 17.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-02-053119-B

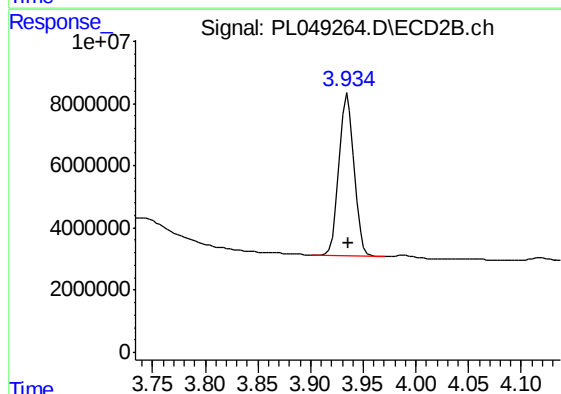


#1 Tetrachloro-m-xylene

R.T.: 3.935 min
Delta R.T.: -0.001 min
Response: 51756767
Conc: 17.91 ng/ml

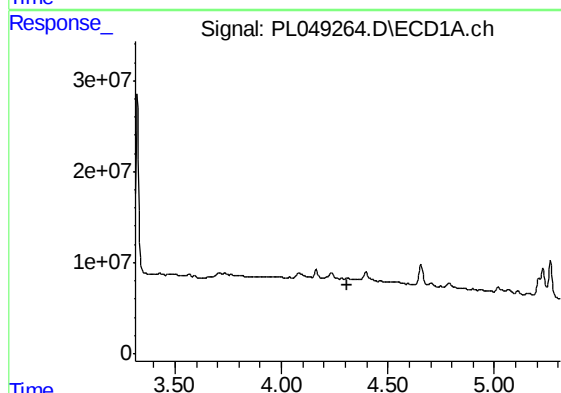


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.312 min
Response: 0
Conc: N.D.

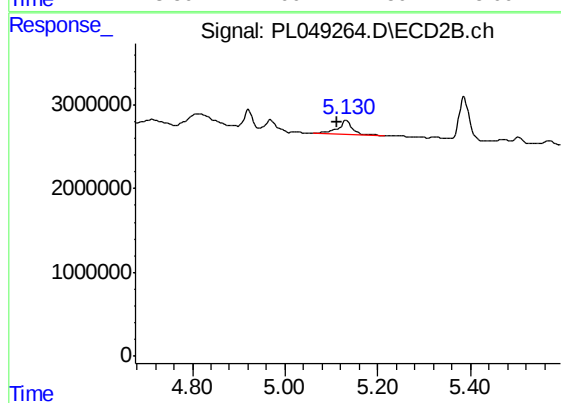

#4 Heptachlor


R.T.: 5.132 min
Delta R.T.: 0.020 min
Response: 4035506
Conc: 1.00 ng/ml

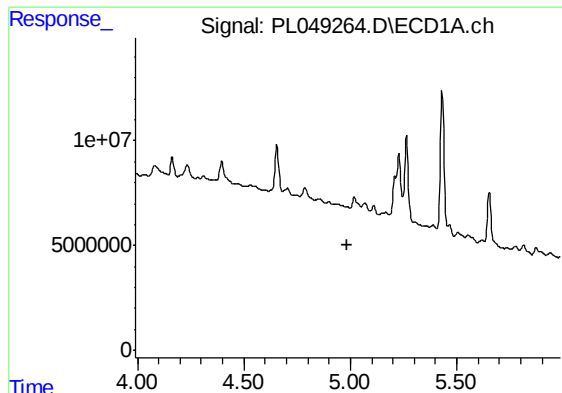

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.988 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
CL-02-053119-B

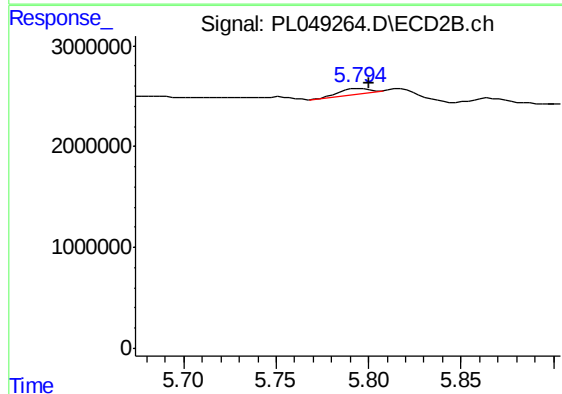


#8 Heptachlor epoxide

R.T.: 5.796 min
Delta R.T.: -0.005 min
Response: 547012
Conc: 0.17 ng/ml

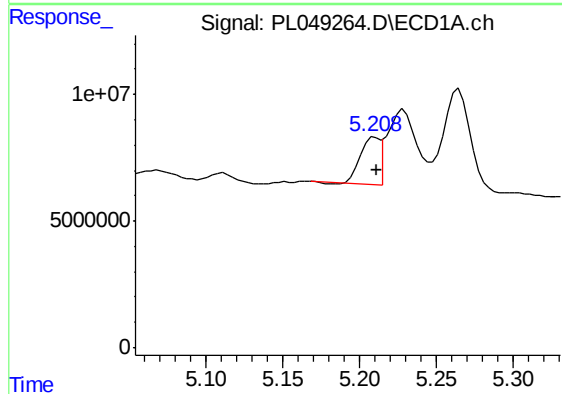


#10 gamma-Chlordane

R.T.: 5.210 min
Delta R.T.: 0.000 min
Response: 16521566
Conc: 1.03 ng/ml

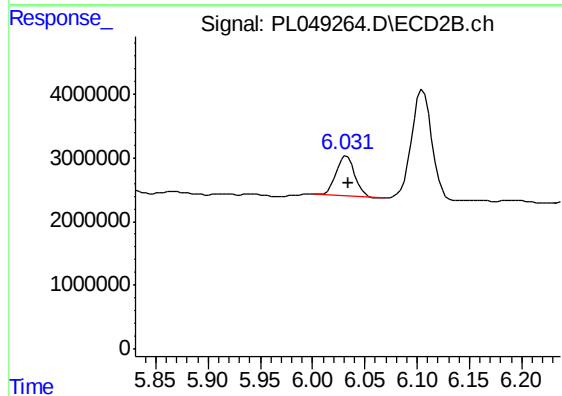

#10 gamma-Chlordane


R.T.: 6.033 min
Delta R.T.: -0.002 min
Response: 7742190
Conc: 2.24 ng/ml

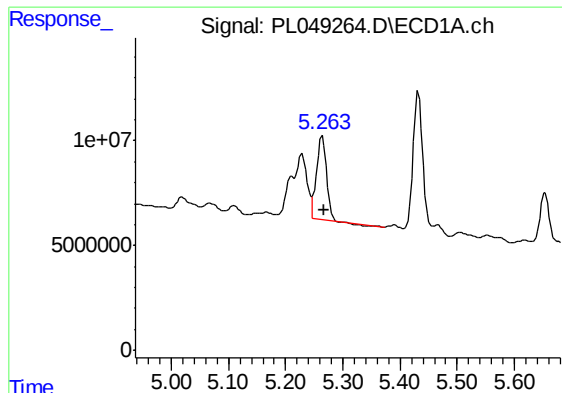

#11 alpha-Chlordane


R.T.: 5.264 min
Delta R.T.: -0.002 min
Response: 47011278
Conc: 3.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-02-053119-B

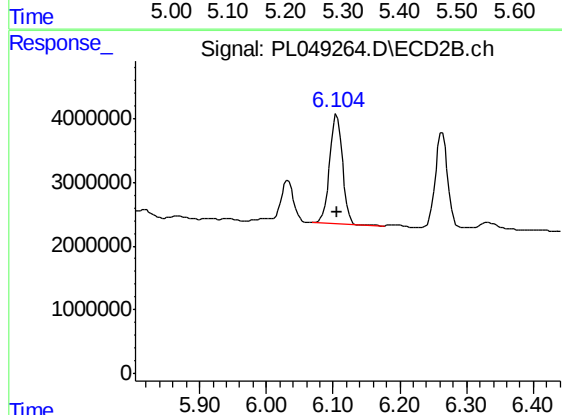


#11 alpha-Chlordane

R.T.: 6.106 min
Delta R.T.: -0.001 min
Response: 23195236
Conc: 6.69 ng/ml

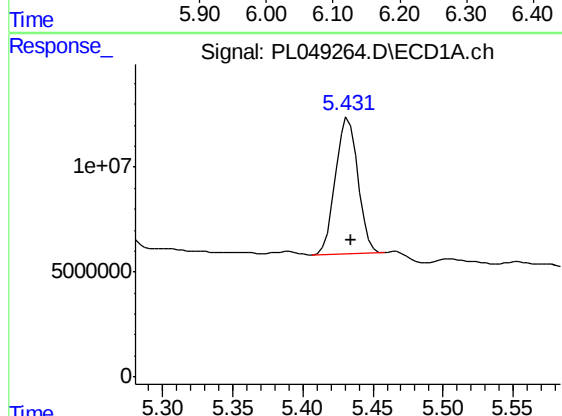


#12 4,4'-DDE

R.T.: 5.432 min
Delta R.T.: -0.002 min
Response: 72584326
Conc: 4.64 ng/ml

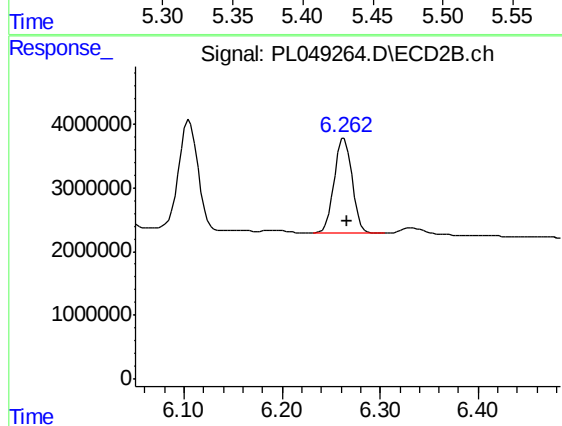

#12 4,4'-DDE


R.T.: 6.264 min
Delta R.T.: -0.003 min
Response: 19012092
Conc: 5.79 ng/ml

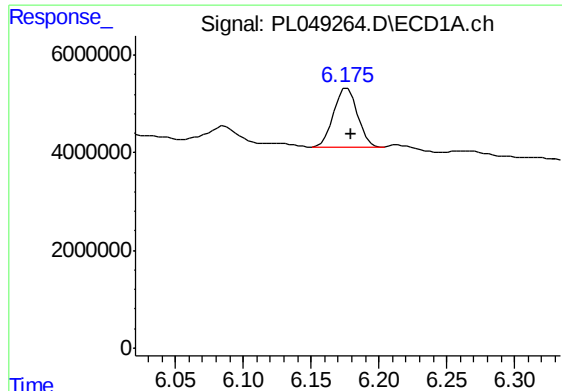

#17 4,4'-DDT


R.T.: 6.177 min
Delta R.T.: -0.003 min
Response: 14480962
Conc: 1.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-02-053119-B

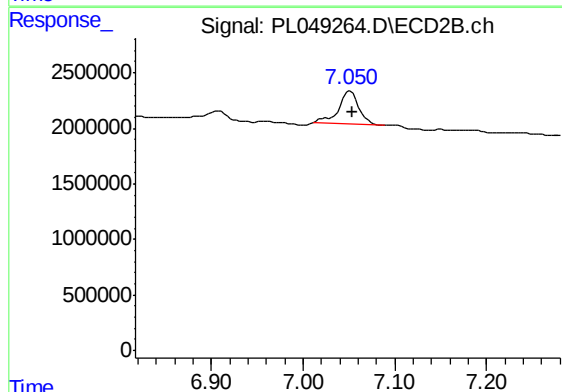


#17 4,4'-DDT

R.T.: 7.051 min
Delta R.T.: -0.002 min
Response: 4714841
Conc: 1.68 ng/ml

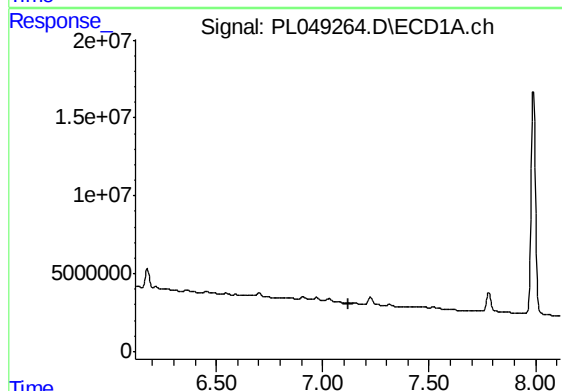


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 7.120 min
Response: 0
Conc: N.D.

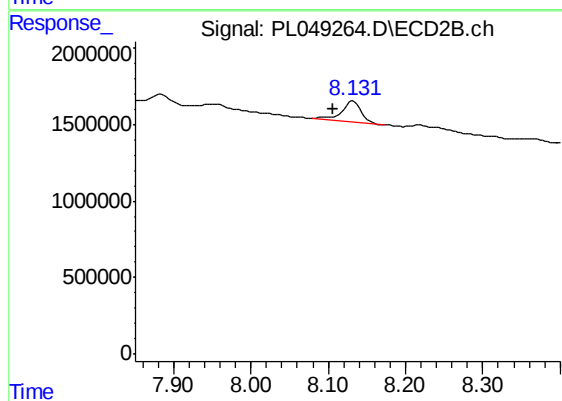

#22 Mirex


R.T.: 8.132 min
Delta R.T.: 0.026 min
Response: 2262328
Conc: 0.87 ng/ml

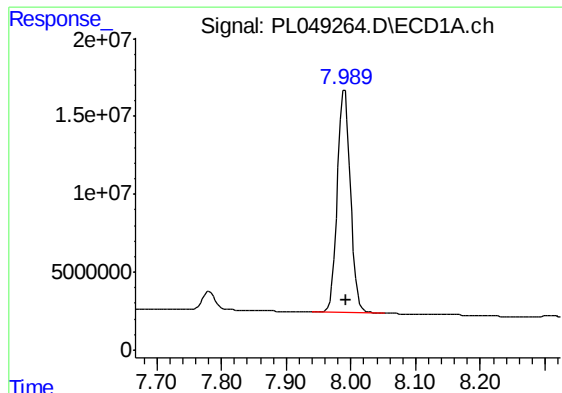

#28 Decachlorobiphenyl

R.T.: 7.990 min
Delta R.T.: -0.002 min
Response: 198420092
Conc: 15.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-02-053119-B

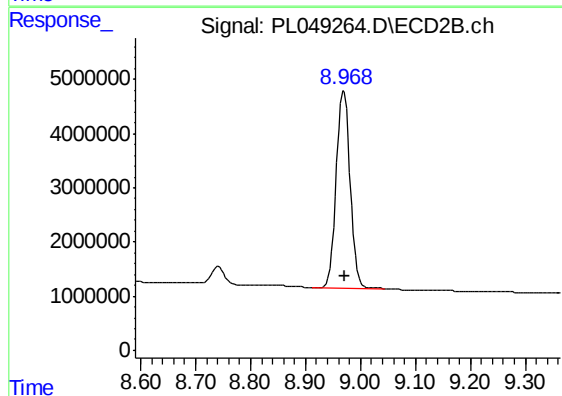

#28 Decachlorobiphenyl

R.T.: 8.970 min
Delta R.T.: -0.002 min
Response: 64388589
Conc: 19.28 ng/ml