

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060419\
 Data File : PL049266.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jun 2019 16:25
 Operator : SM\AJ
 Sample : K3135-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ROLL-OFF-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 01:15:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
 Quant Title : GC Extractables
 QLast Update : Fri May 31 01:35:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.325	3.936	152.6E6	43641455	13.852	15.106
28) SA Decachlor...	7.992	8.971	149.6E6	50609361	11.767	15.154 #
Target Compounds						
10) B gamma-Chl...	5.231f	0.000	26001834	0	1.629	N.D. #
11) B alpha-Chl...	0.000	6.109	0	7150901	N.D.	2.061 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060419\
Data File : PL049266.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jun 2019 16:25
Operator : SM\AJ
Sample : K3135-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ROLL-OFF-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 01:15:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
Quant Title : GC Extractables
QLast Update : Fri May 31 01:35:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

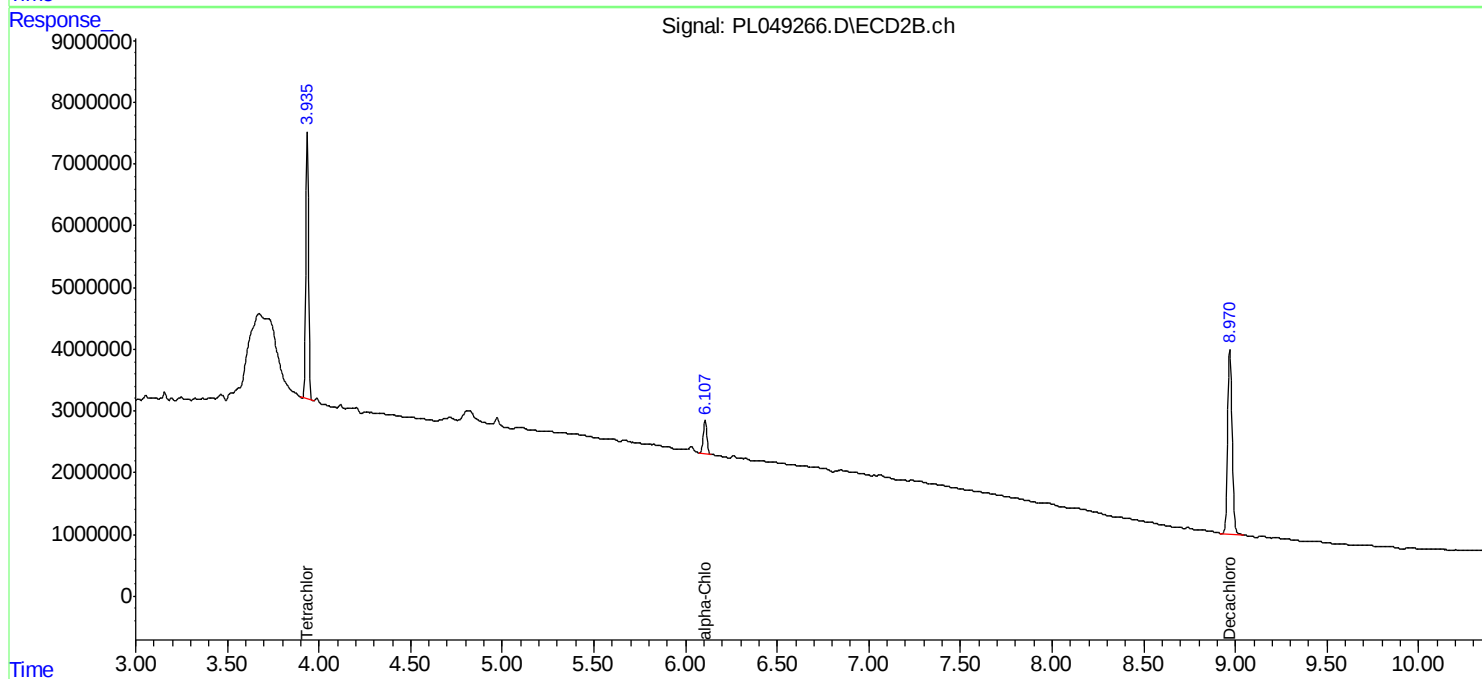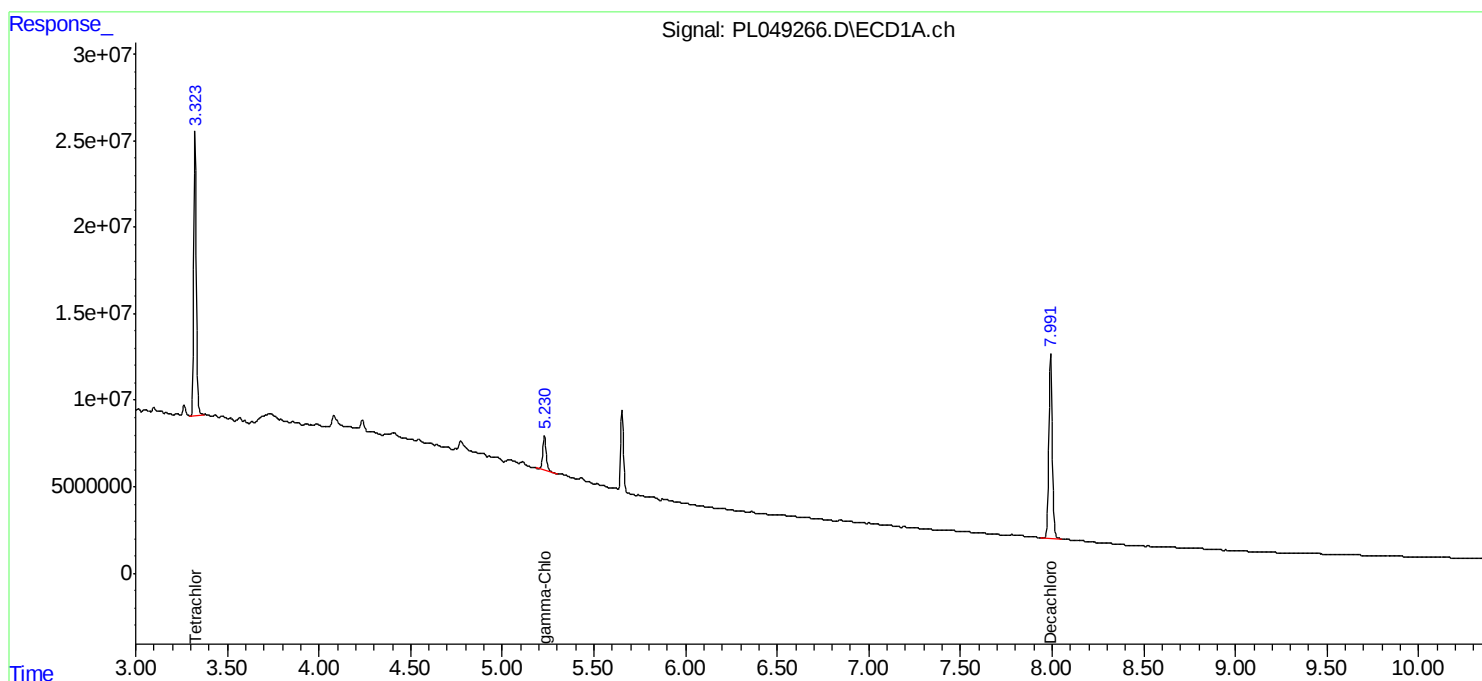


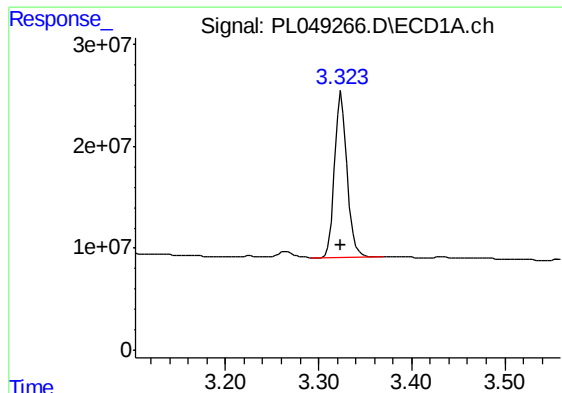

#1 Tetrachloro-m-xylene


R.T.: 3.325 min
Delta R.T.: 0.000 min
Response: 152631516
Conc: 13.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
ROLL-OFF-COMP

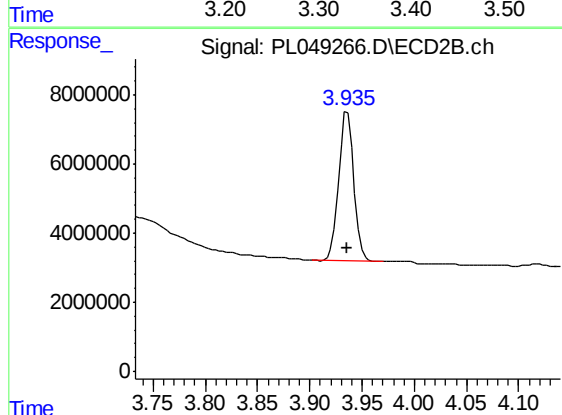


#1 Tetrachloro-m-xylene

R.T.: 3.936 min
Delta R.T.: 0.000 min
Response: 43641455
Conc: 15.11 ng/ml

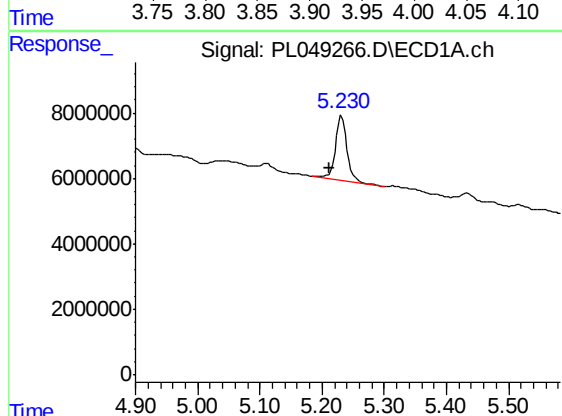


#10 gamma-Chlordane

R.T.: 5.231 min
Delta R.T.: 0.021 min
Response: 26001834
Conc: 1.63 ng/ml

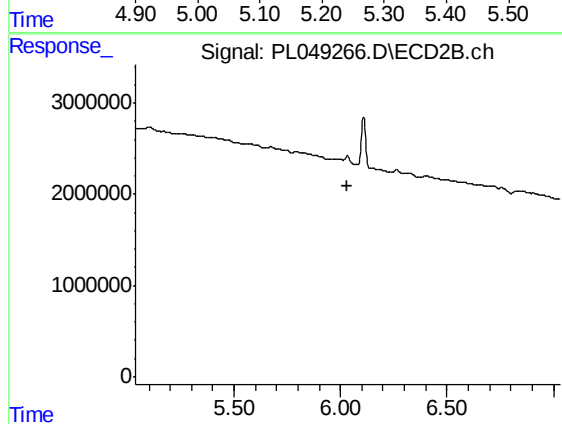

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.035 min
Response: 0
Conc: N.D.

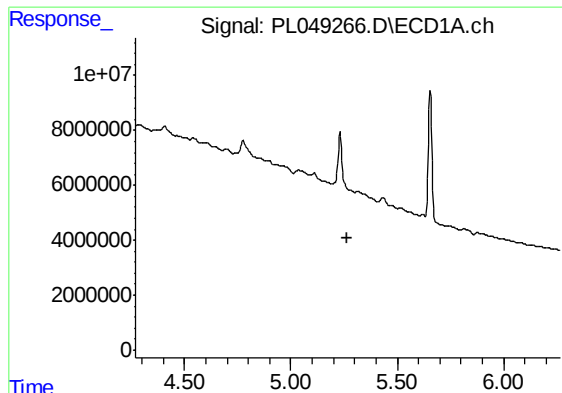

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.267 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
ROLL-OFF-COMP

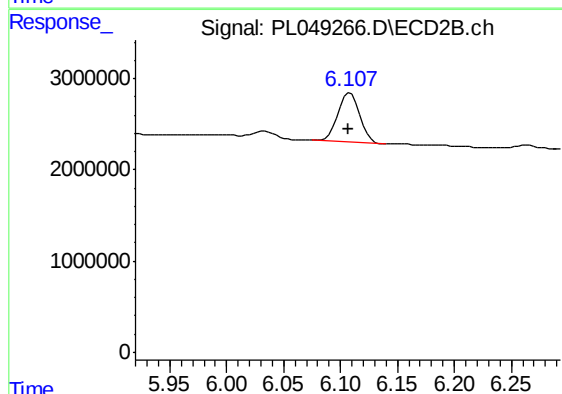


#11 alpha-Chlordane

R.T.: 6.109 min
Delta R.T.: 0.002 min
Response: 7150901
Conc: 2.06 ng/ml

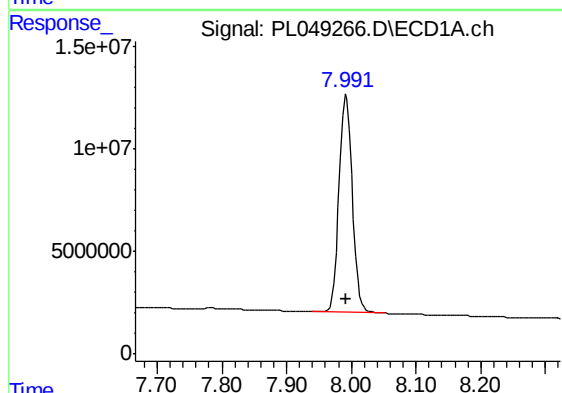

#28 Decachlorobiphenyl

R.T.: 7.992 min
Delta R.T.: 0.000 min
Response: 149621666
Conc: 11.77 ng/ml

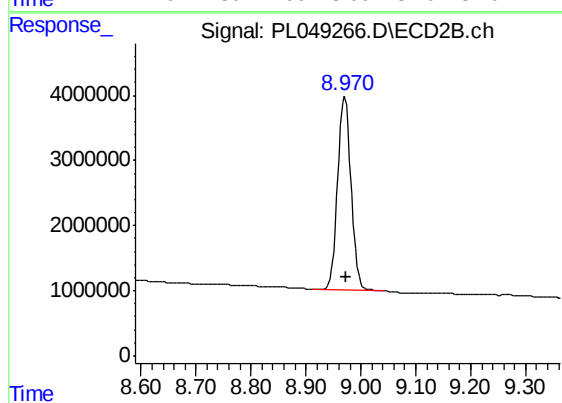

#28 Decachlorobiphenyl

R.T.: 8.971 min
Delta R.T.: -0.001 min
Response: 50609361
Conc: 15.15 ng/ml