

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060420\
 Data File : PL059132.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jun 2020 13:31
 Operator : AJ\MA
 Sample : L2858-01 10X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CHRT27247

Manual Integrations
 APPROVED

mohammad
 6/8/2020 8:27:51 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 14:46:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060320.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 04 08:16:22 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.519	4.072	2346214	3470150	1.359m	1.334
28) SA Decachlor...	8.295	9.181	2087237	3902687	1.269	1.646 #
Target Compounds						
10) B gamma-Chl...	5.464	6.207	686508	726673	0.410m	0.243 #
17) MA 4,4'-DDT	6.455	7.213	1024792	814961	0.812	0.358 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060420\
Data File : PL059132.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jun 2020 13:31
Operator : AJ\MA
Sample : L2858-01 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
CHRT27247


Manual Integrations
APPROVED

mohammad
6/8/2020 8:27:51 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 14:46:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060320.M
Quant Title : GC Extractables
QLast Update : Thu Jun 04 08:16:22 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

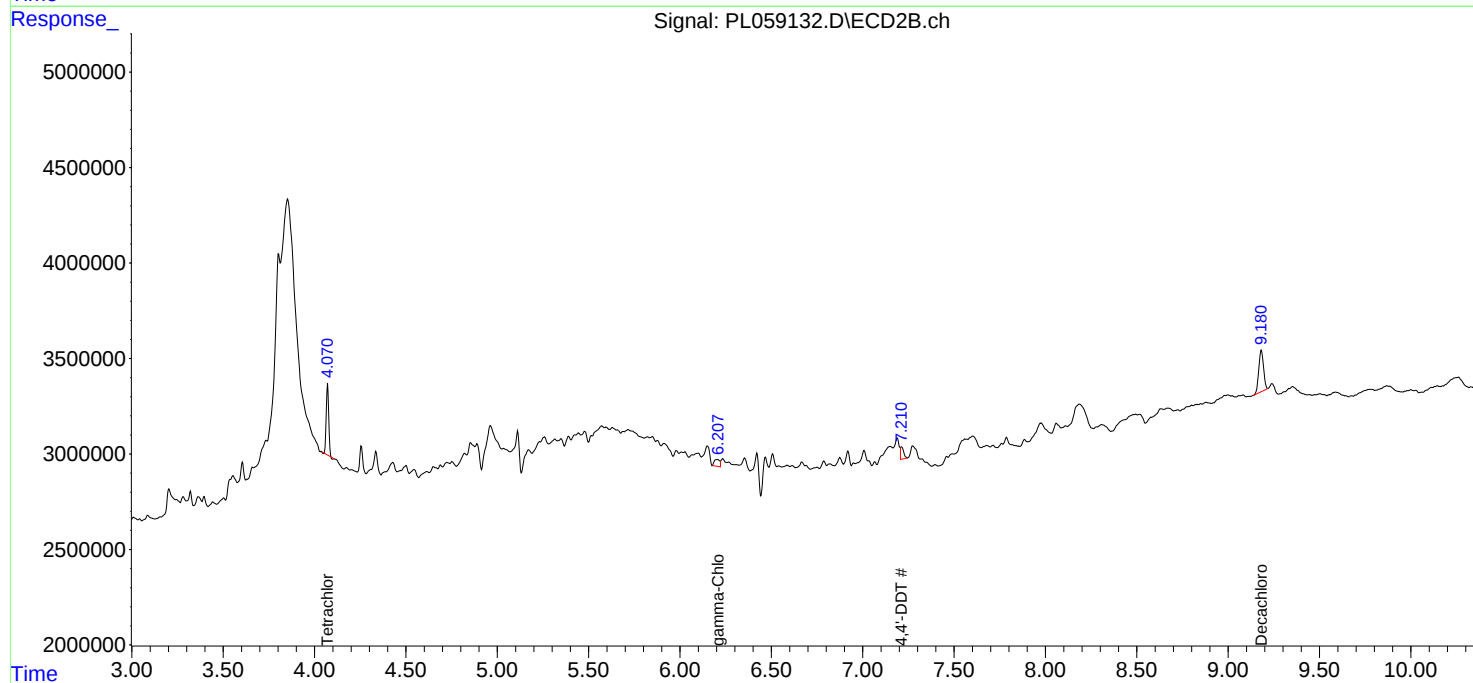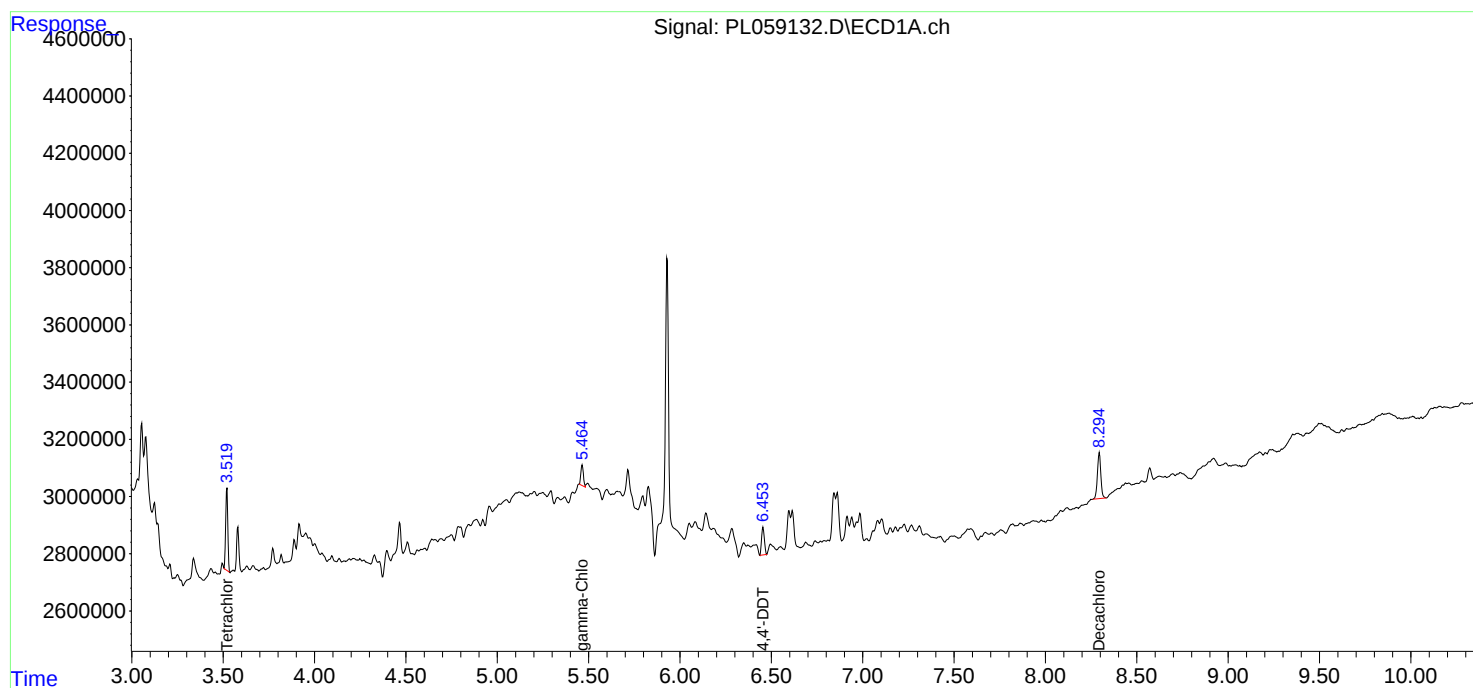

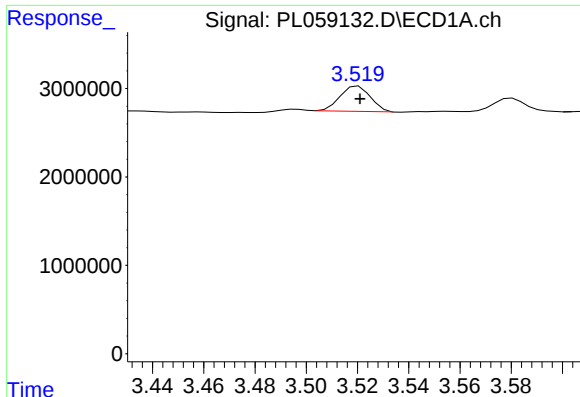


#1 Tetrachloro-m-xylene

R.T.: 3.519 min
Delta R.T.: -0.002 min
Response: 2346214
Conc: 1.36 ng/ml m

Instrument :
ECD_L
ClientSampleId :
CHRT27247


Manual Integrations
APPROVED

mohammad
6/8/2020 8:27:51 AM

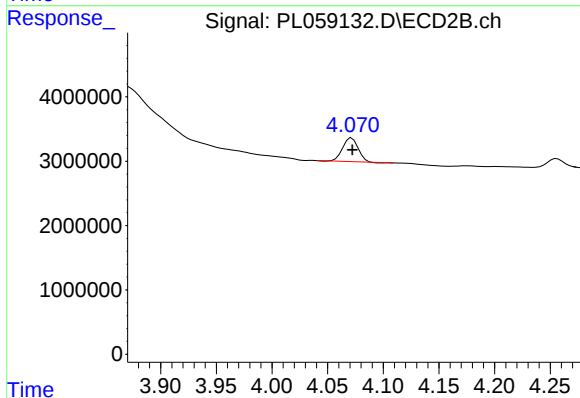


#1 Tetrachloro-m-xylene

R.T.: 4.072 min
Delta R.T.: 0.000 min
Response: 3470150
Conc: 1.33 ng/ml

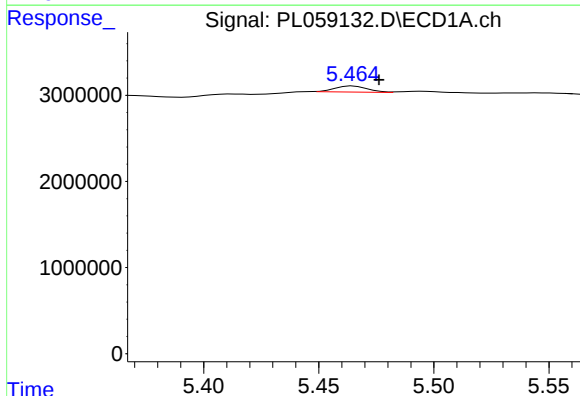


#10 gamma-Chlordane

R.T.: 5.464 min
Delta R.T.: -0.013 min
Response: 686508
Conc: 0.41 ng/ml m

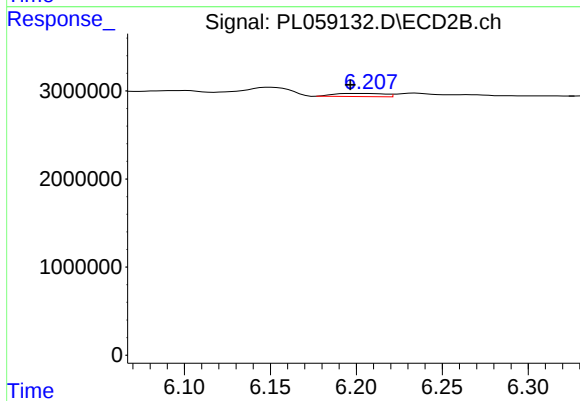

#10 gamma-Chlordane

R.T.: 6.207 min
Delta R.T.: 0.011 min
Response: 726673
Conc: 0.24 ng/ml

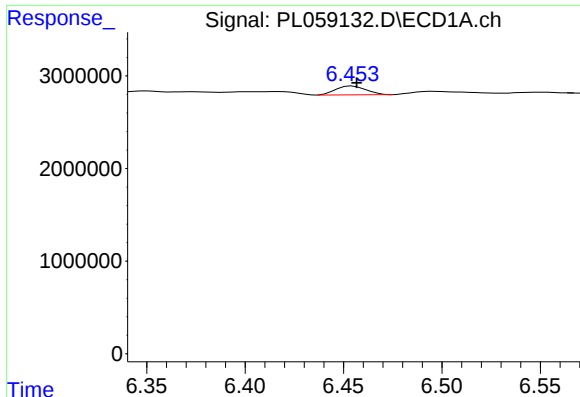


#17 4,4'-DDT

R.T.: 6.455 min
Delta R.T.: -0.002 min
Response: 1024792
Conc: 0.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
CHRT27247


Manual Integrations
APPROVED

mohammad
6/8/2020 8:27:51 AM

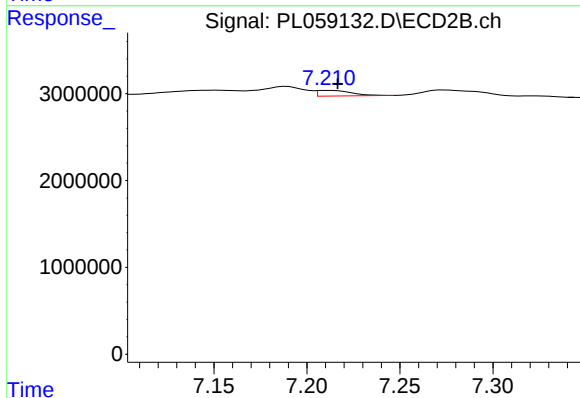


#17 4,4'-DDT

R.T.: 7.213 min
Delta R.T.: -0.004 min
Response: 814961
Conc: 0.36 ng/ml

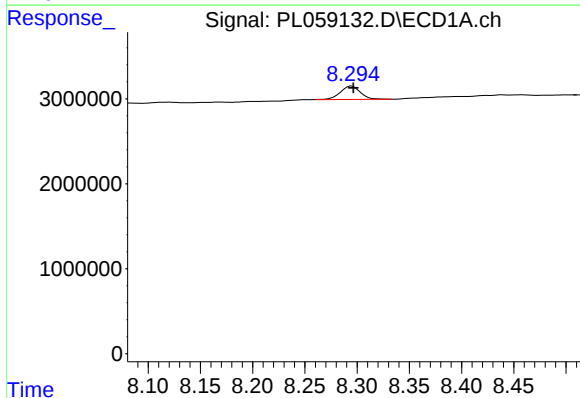

#28 Decachlorobiphenyl

R.T.: 8.295 min
Delta R.T.: -0.002 min
Response: 2087237
Conc: 1.27 ng/ml

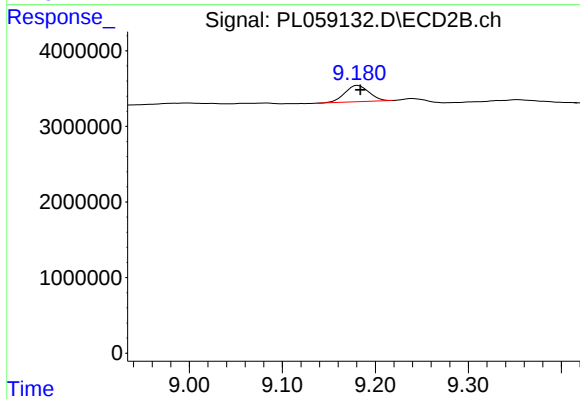

#28 Decachlorobiphenyl

R.T.: 9.181 min
Delta R.T.: -0.003 min
Response: 3902687
Conc: 1.65 ng/ml