

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060422\
 Data File : PL075514.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jun 2022 16:00
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 06 00:19:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060422.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 06 00:15:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.646	4.642	12542877	31207256	20.324	20.317
28)	SA Decachlor...	11.642	10.388	10968287	25251108	21.124	20.790
Target Compounds							
5)	MB Aldrin	7.632f	0.000	1414858	0	1.858	N.D. #
7)	B delta-BHC	0.000	6.405	0	883108	N.D.	0.448 #
10)	B gamma-Chl...	8.383	0.000	351625	0	0.509	N.D. #
11)	B alpha-Chl...	0.000	7.393f	0	491202	N.D.	0.302 #
14)	MA Endrin	0.000	8.071f	0	287890	N.D.	0.213 #
15)	B Endosulfa...	9.306	8.328f	346880	2516349	0.626	1.910 #
17)	MA 4,4'-DDT	0.000	8.489f	0	100796	N.D.	0.079 #
21)	B Endrin ke...	10.187f	0.000	230985	0	0.372	N.D. #
23)	Chlordane-1	0.000	5.984f	0	863746	N.D.	16.754 #
24)	Chlordane-2	7.632	0.000	1414858	0	46.132	N.D. #
25)	Chlordane-3	8.383	0.000	351625	0	3.672	N.D. #
26)	Chlordane-4	0.000	7.393f	0	491202	N.D.	2.873 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060422\
Data File : PL075514.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jun 2022 16:00
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 06 00:19:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060422.M
Quant Title : GC Extractables
QLast Update : Mon Jun 06 00:15:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

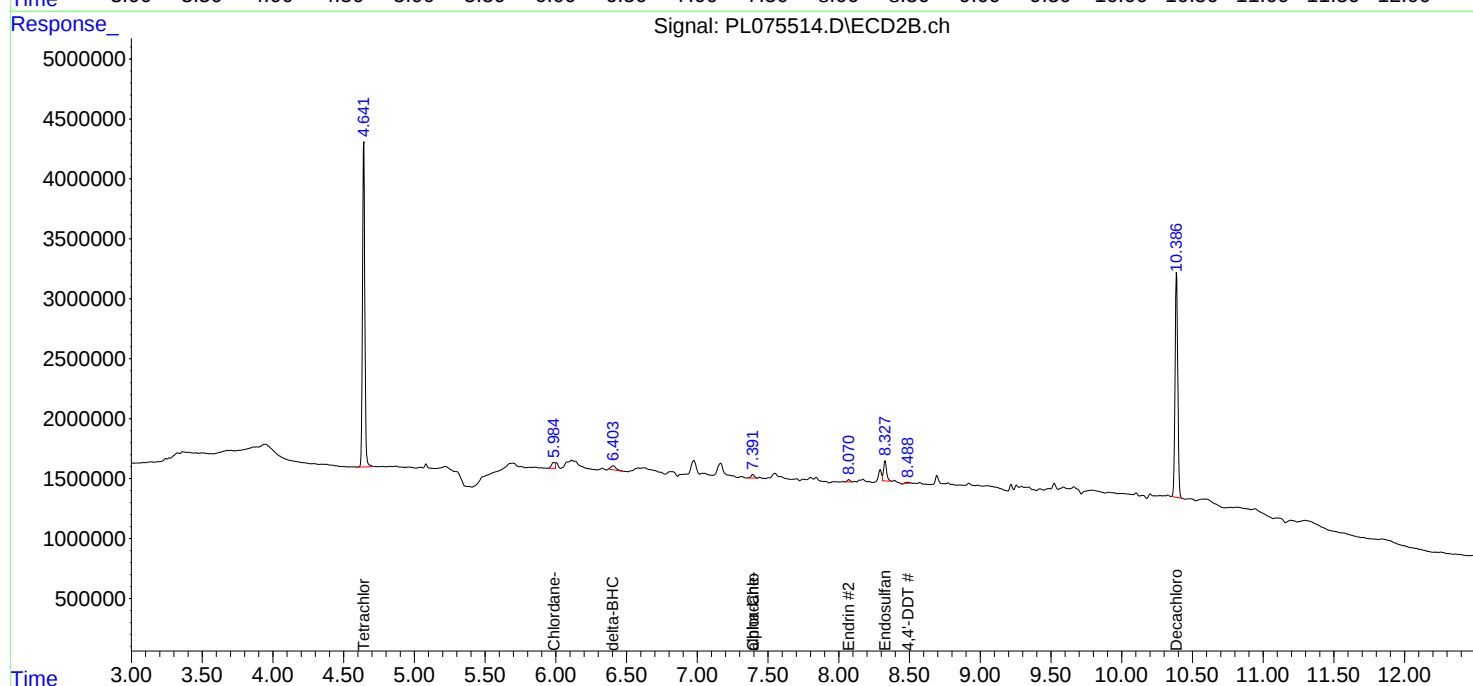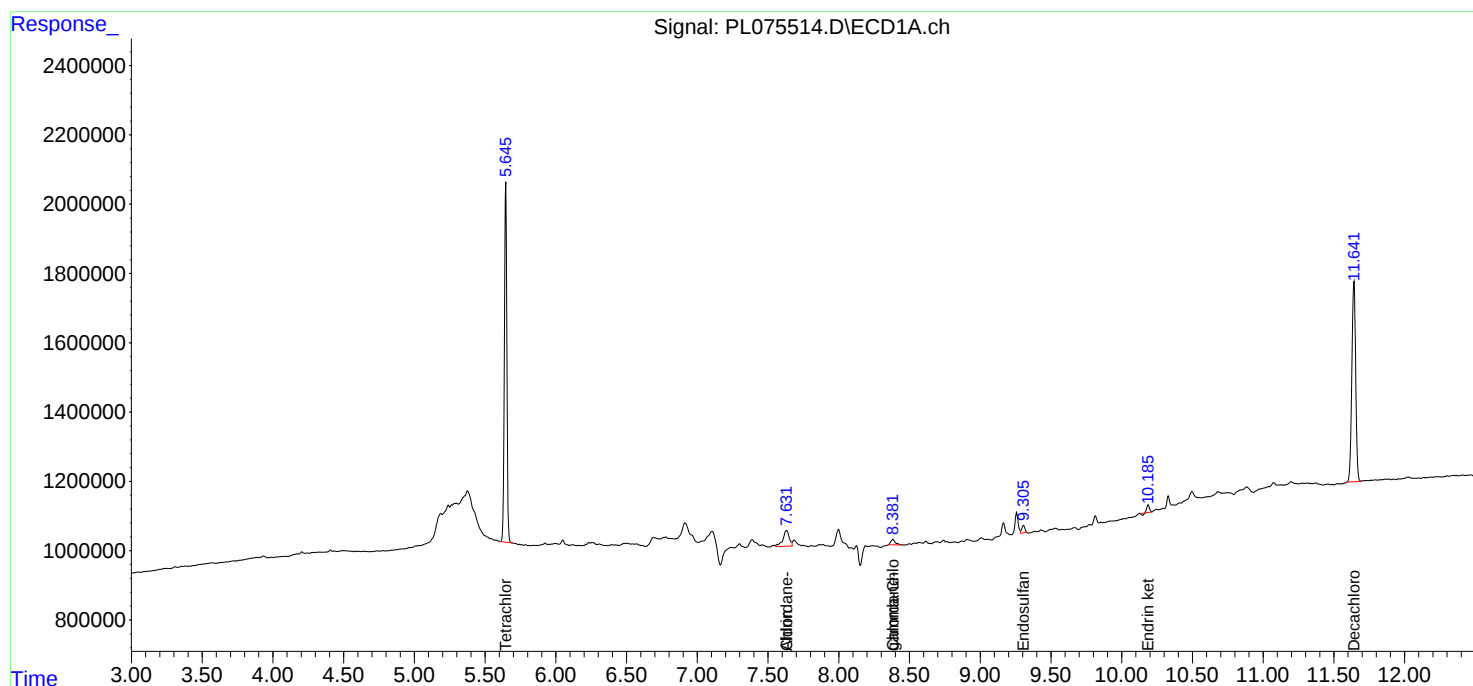


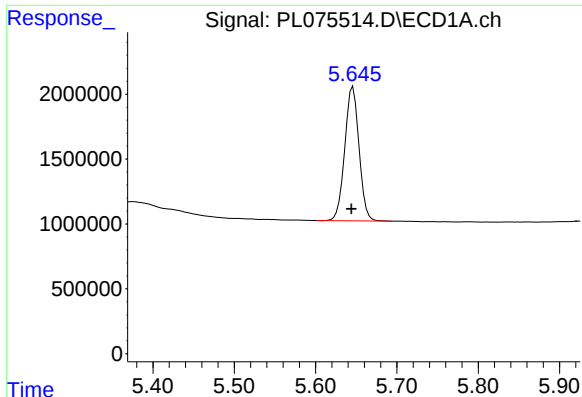

#1 Tetrachloro-m-xylene


R.T.: 5.646 min
Delta R.T.: 0.002 min
Response: 12542877
Conc: 20.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

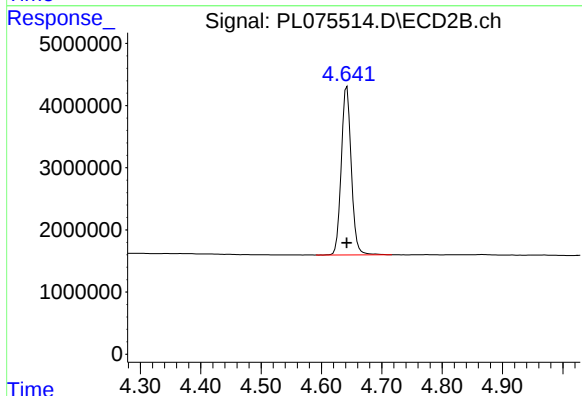


#1 Tetrachloro-m-xylene

R.T.: 4.642 min
Delta R.T.: 0.000 min
Response: 31207256
Conc: 20.32 ng/ml

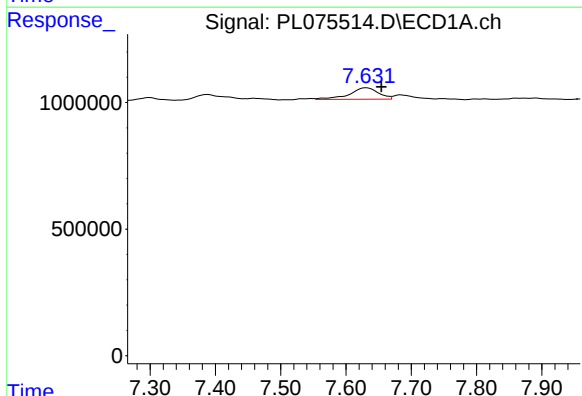


#5 Aldrin

R.T.: 7.632 min
Delta R.T.: -0.023 min
Response: 1414858
Conc: 1.86 ng/ml

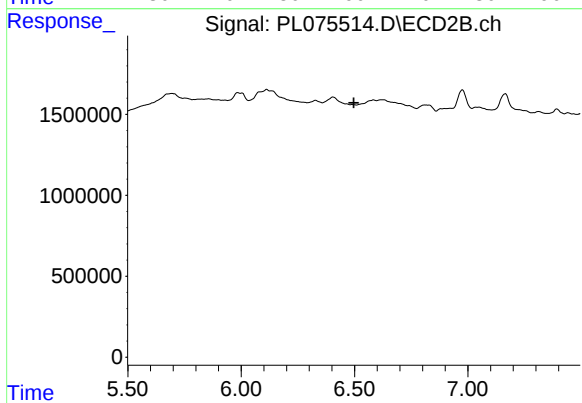

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 6.497 min
Response: 0
Conc: N.D.

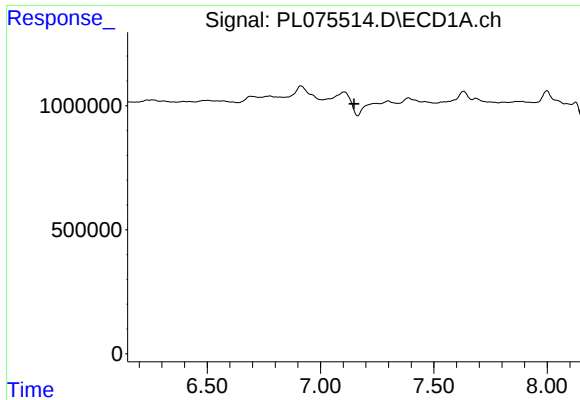

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 7.148 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

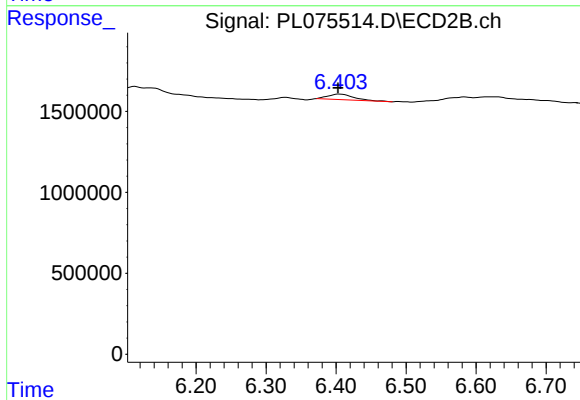


#7 delta-BHC

R.T.: 6.405 min
Delta R.T.: 0.001 min
Response: 883108
Conc: 0.45 ng/ml

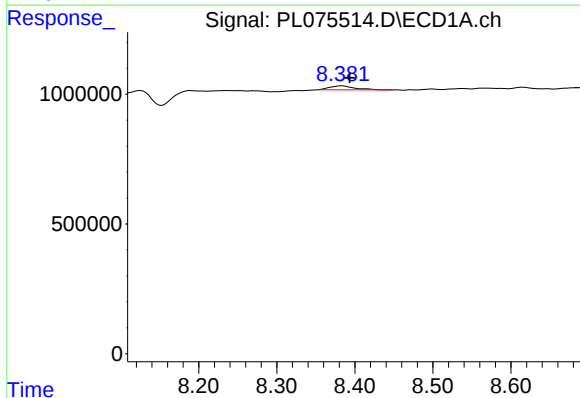


#10 gamma-Chlordane

R.T.: 8.383 min
Delta R.T.: -0.010 min
Response: 351625
Conc: 0.51 ng/ml

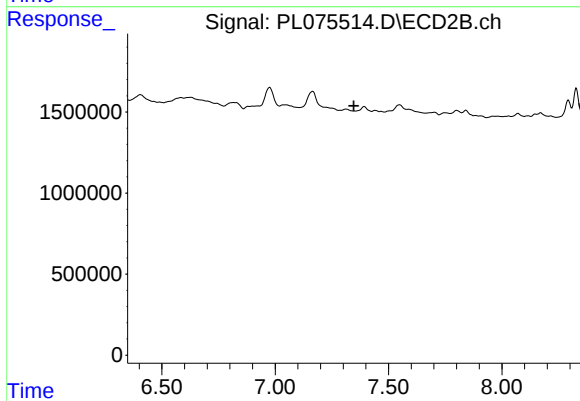

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.347 min
Response: 0
Conc: N.D.

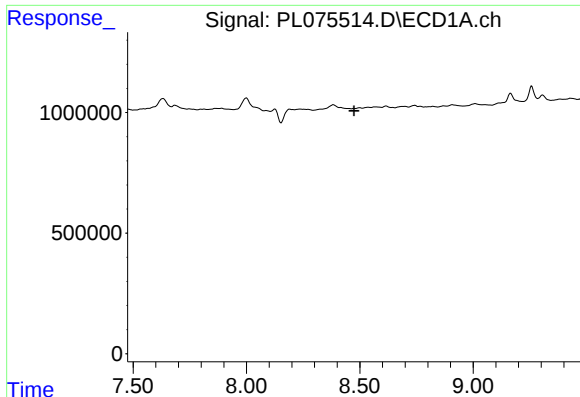

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 8.474 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

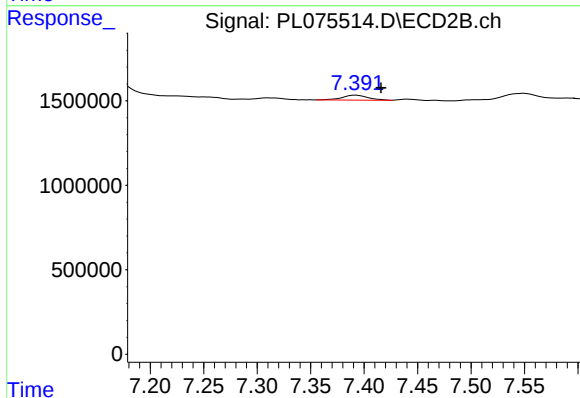


#11 alpha-Chlordane

R.T.: 7.393 min
Delta R.T.: -0.023 min
Response: 491202
Conc: 0.30 ng/ml

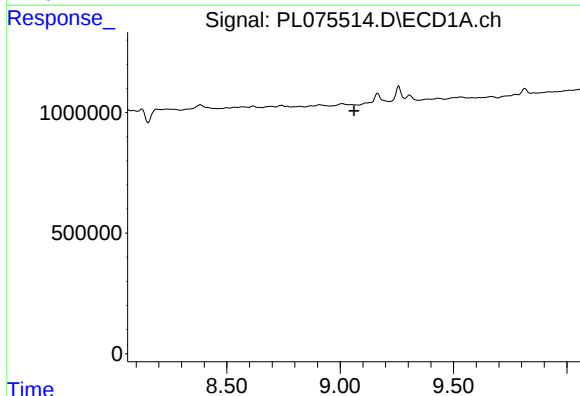


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 9.062 min
Response: 0
Conc: N.D.

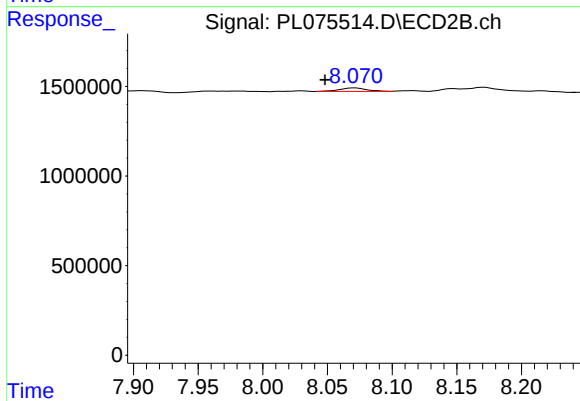

#14 Endrin


R.T.: 8.071 min
Delta R.T.: 0.023 min
Response: 287890
Conc: 0.21 ng/ml

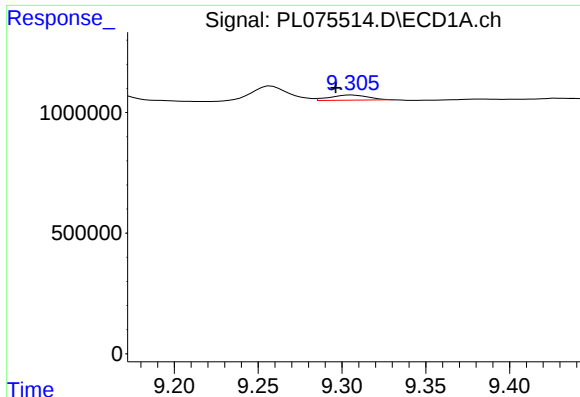

#15 Endosulfan II


R.T.: 9.306 min
Delta R.T.: 0.010 min
Response: 346880
Conc: 0.63 ng/ml

Instrument :
ECD_L
ClientSampleId :

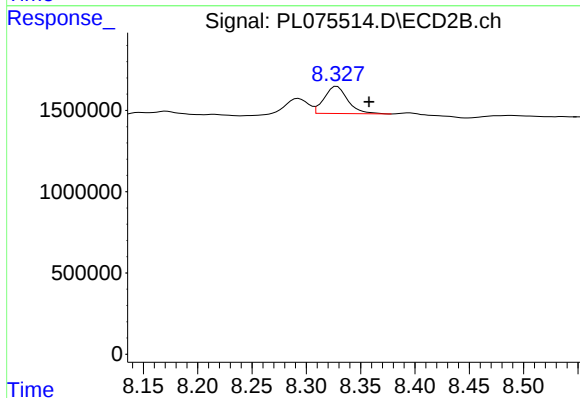


#15 Endosulfan II

R.T.: 8.328 min
Delta R.T.: -0.030 min
Response: 2516349
Conc: 1.91 ng/ml

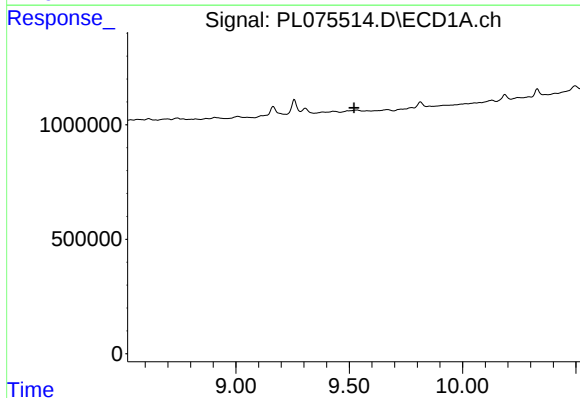


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 9.522 min
Response: 0
Conc: N.D.

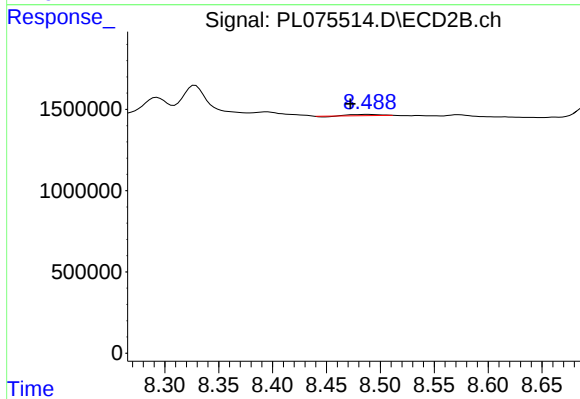

#17 4,4'-DDT


R.T.: 8.489 min
Delta R.T.: 0.017 min
Response: 100796
Conc: 0.08 ng/ml

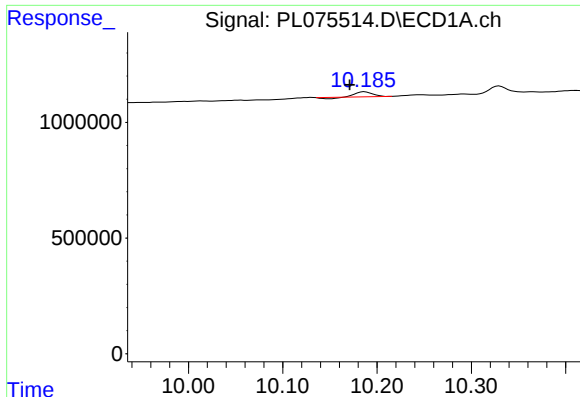

#21 Endrin ketone


R.T.: 10.187 min
Delta R.T.: 0.016 min
Response: 230985
Conc: 0.37 ng/ml

Instrument :
ECD_L
ClientSampleId :

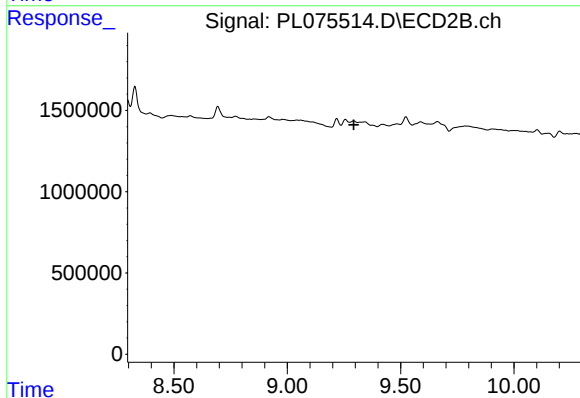


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.294 min
Response: 0
Conc: N.D.

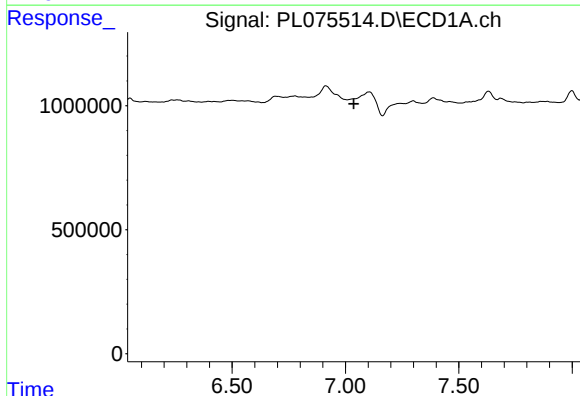


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 7.037 min
Response: 0
Conc: N.D.

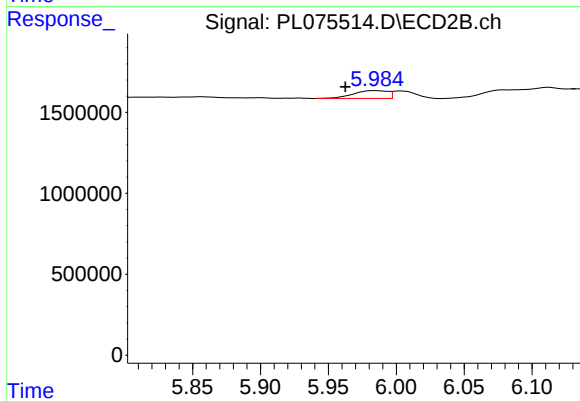

#23 Chlordane-1


R.T.: 5.984 min
Delta R.T.: 0.022 min
Response: 863746
Conc: 16.75 ng/ml

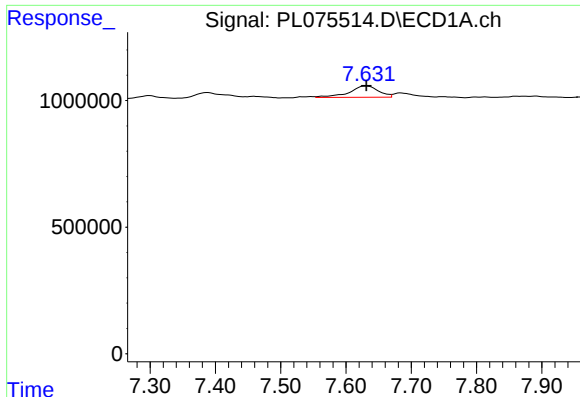

#24 Chlordane-2


R.T.: 7.632 min
Delta R.T.: 0.000 min
Response: 1414858
Conc: 46.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

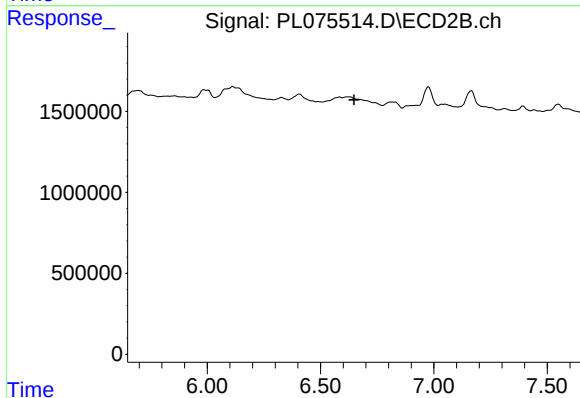


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 6.648 min
Response: 0
Conc: N.D.

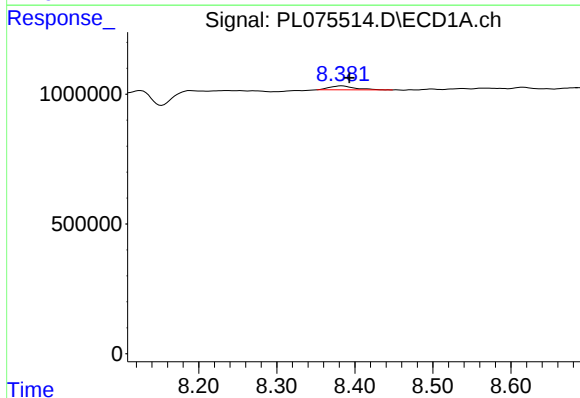


#25 Chlordane-3

R.T.: 8.383 min
Delta R.T.: -0.010 min
Response: 351625
Conc: 3.67 ng/ml

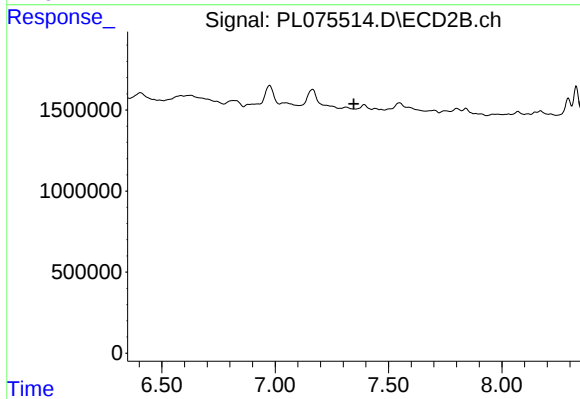

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 7.347 min
Response: 0
Conc: N.D.

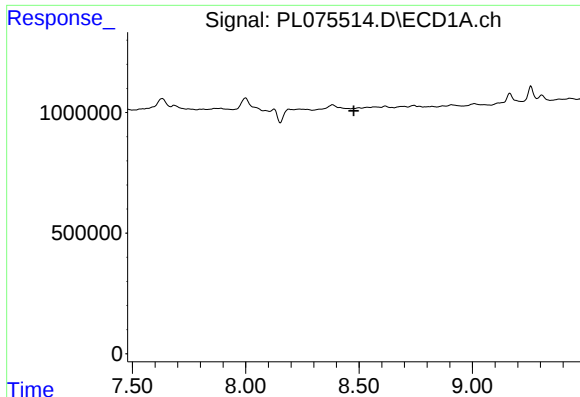

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 8.476 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

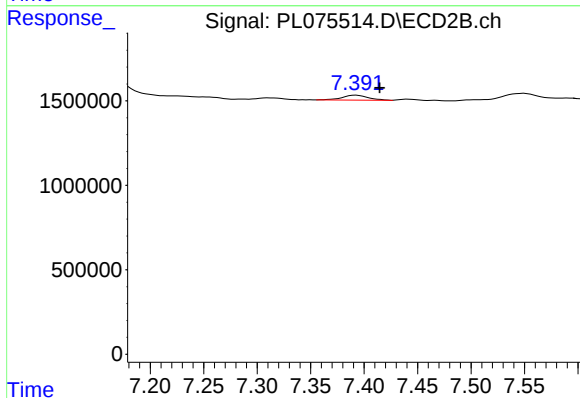


#26 Chlordane-4

R.T.: 7.393 min
Delta R.T.: -0.022 min
Response: 491202
Conc: 2.87 ng/ml

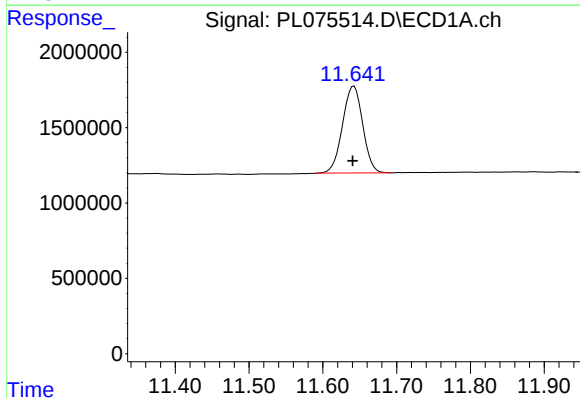

#28 Decachlorobiphenyl

R.T.: 11.642 min
Delta R.T.: 0.002 min
Response: 10968287
Conc: 21.12 ng/ml

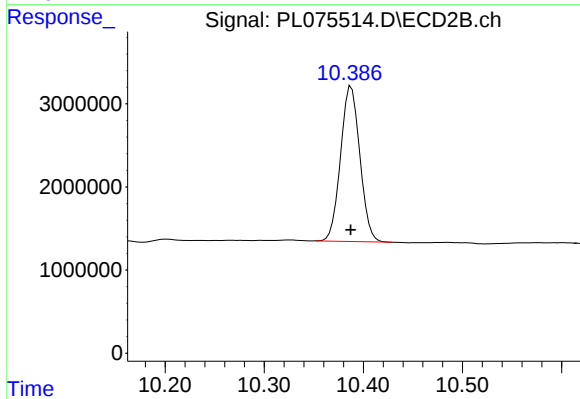

#28 Decachlorobiphenyl

R.T.: 10.388 min
Delta R.T.: 0.000 min
Response: 25251108
Conc: 20.79 ng/ml