

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060422\
 Data File : PL075535.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jun 2022 21:46
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 06 00:20:25 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060422.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 06 00:15:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.643	4.641	12835848	31576579	20.799	20.558
28)	SA Decachlor...	11.638	10.386	11231311	26535817	21.630	21.848
Target Compounds							
5)	MB Aldrin	7.636f	0.000	325725	0	0.428	N.D. #
7)	B delta-BHC	0.000	6.413	0	754207	N.D.	0.383 #
8)	B Heptachlo...	8.125	0.000	605359	0	0.855	N.D. #
11)	B alpha-Chl...	0.000	7.395f	0	345131	N.D.	0.212 #
13)	MA Dieldrin	0.000	7.748	0	494937	N.D.	0.324 #
14)	MA Endrin	0.000	8.069f	0	372067	N.D.	0.275 #
15)	B Endosulfa...	9.304	0.000	210042	0	0.379	N.D. #
21)	B Endrin ke...	10.187f	0.000	258424	0	0.416	N.D. #
24)	Chlordane-2	7.636	0.000	325725	0	10.620	N.D. #
26)	Chlordane-4	0.000	7.395f	0	345131	N.D.	2.019 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060422\
Data File : PL075535.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jun 2022 21:46
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 06 00:20:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060422.M
Quant Title : GC Extractables
QLast Update : Mon Jun 06 00:15:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

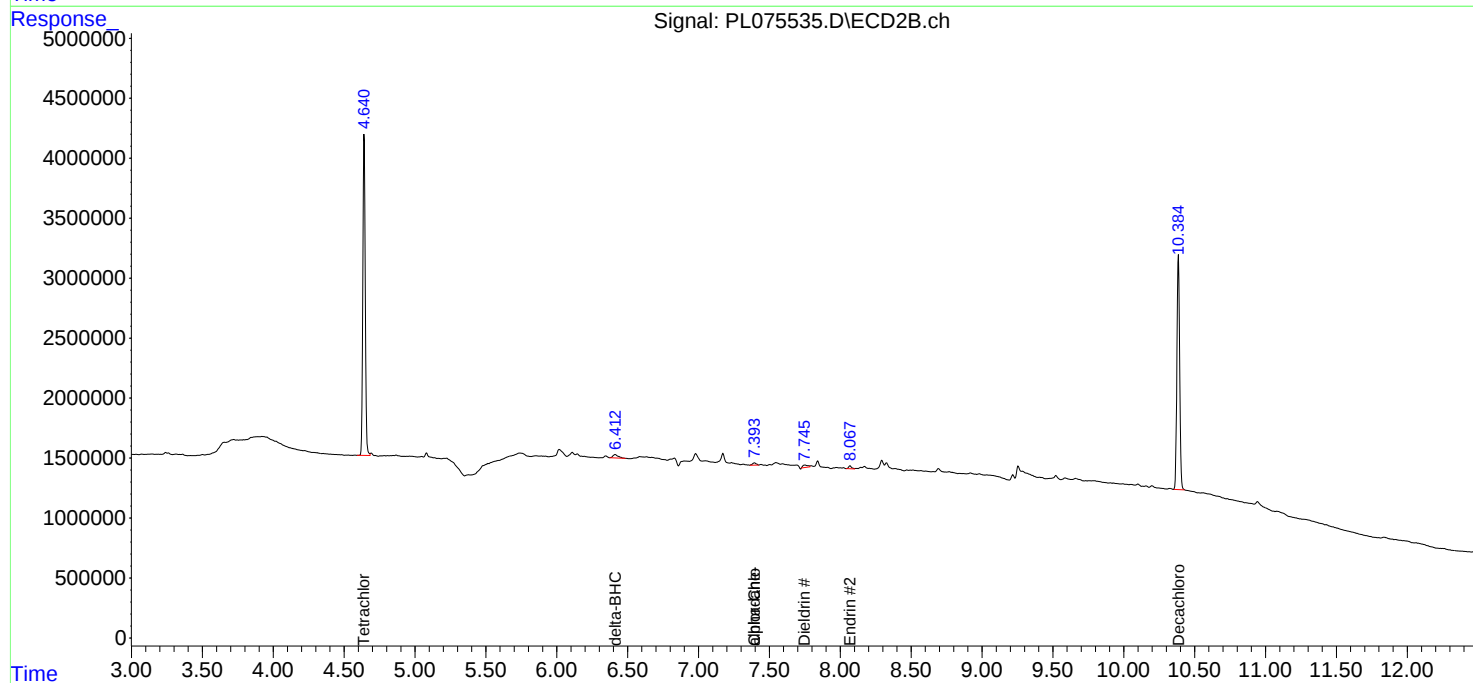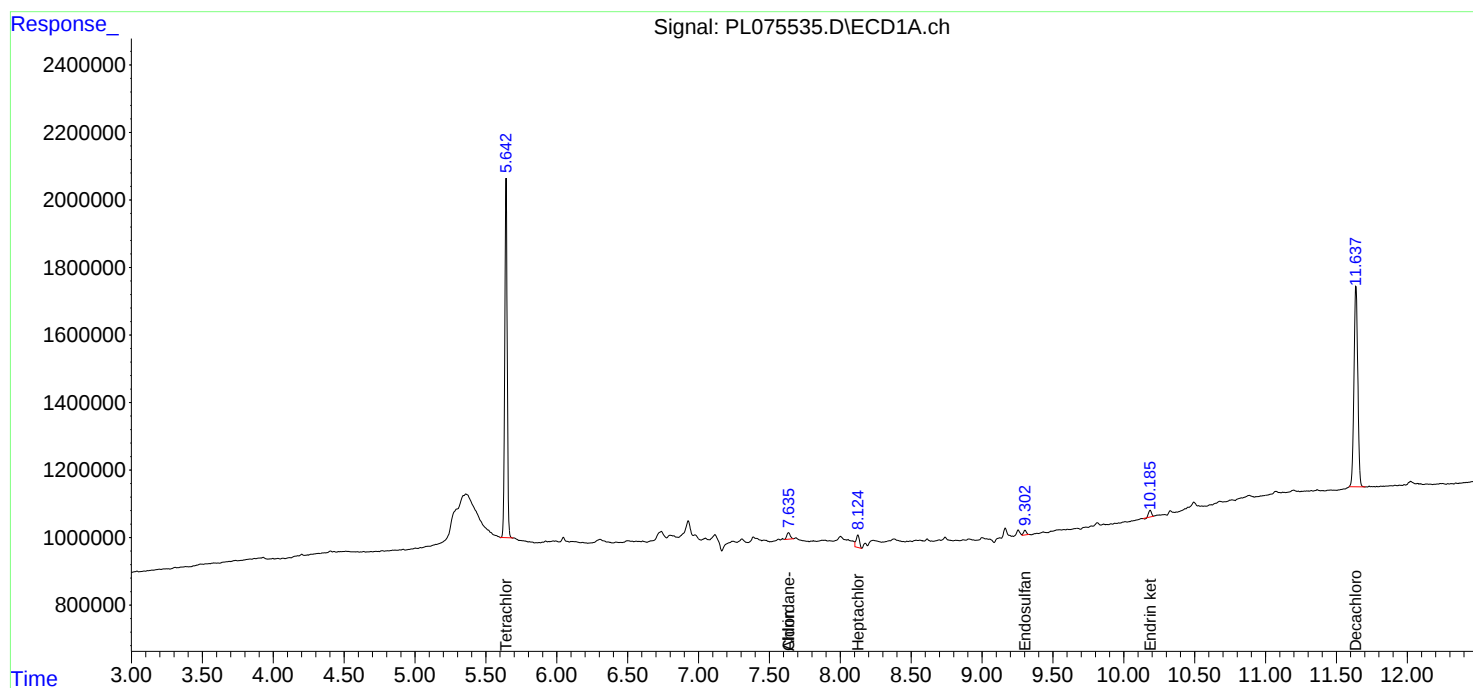


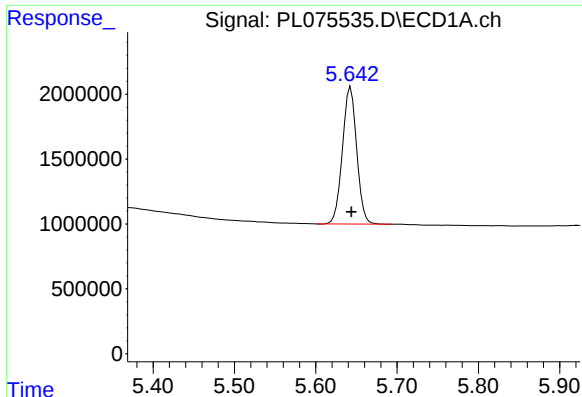

#1 Tetrachloro-m-xylene


R.T.: 5.643 min
Delta R.T.: -0.001 min
Response: 12835848
Conc: 20.80 ng/ml

Instrument :
ECD_L
ClientSampleId :

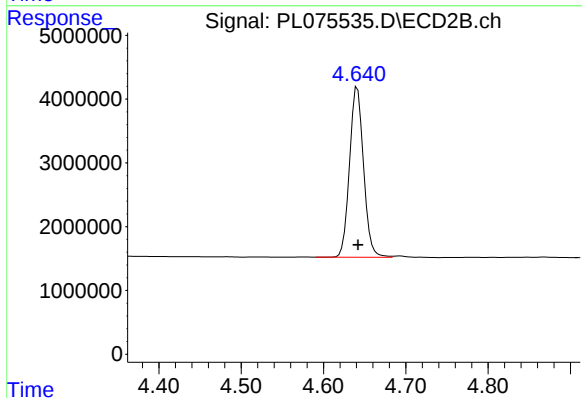


#1 Tetrachloro-m-xylene

R.T.: 4.641 min
Delta R.T.: 0.000 min
Response: 31576579
Conc: 20.56 ng/ml

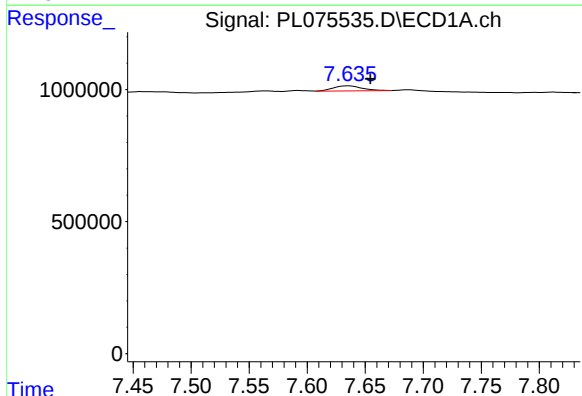


#5 Aldrin

R.T.: 7.636 min
Delta R.T.: -0.019 min
Response: 325725
Conc: 0.43 ng/ml

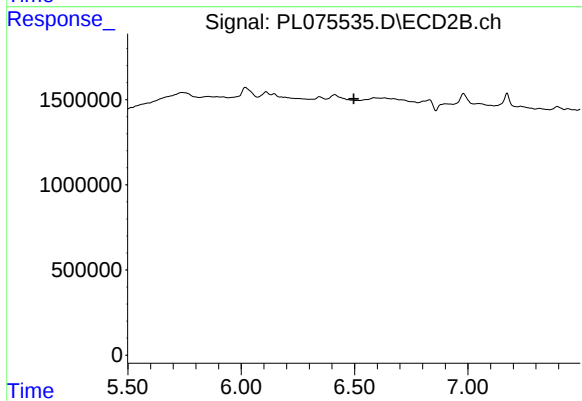

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 6.497 min
Response: 0
Conc: N.D.

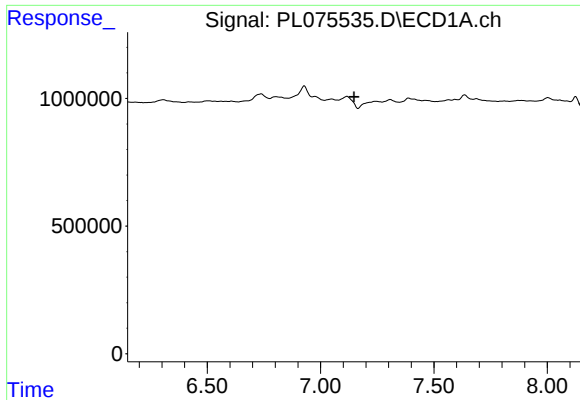

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 7.148 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

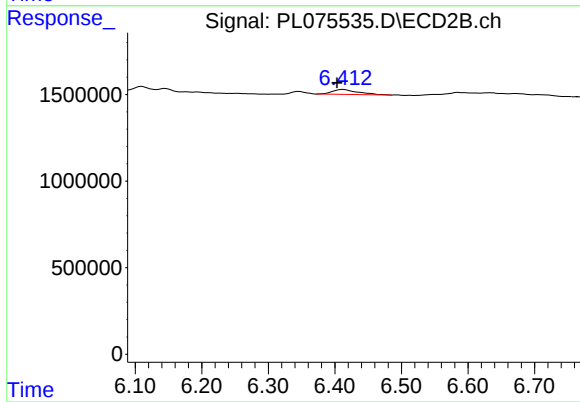


#7 delta-BHC

R.T.: 6.413 min
Delta R.T.: 0.010 min
Response: 754207
Conc: 0.38 ng/ml

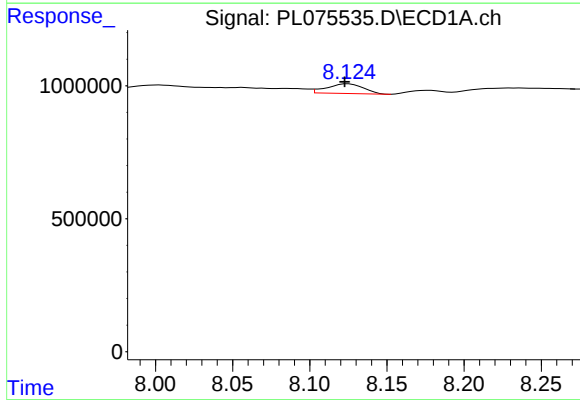


#8 Heptachlor epoxide

R.T.: 8.125 min
Delta R.T.: 0.002 min
Response: 605359
Conc: 0.86 ng/ml

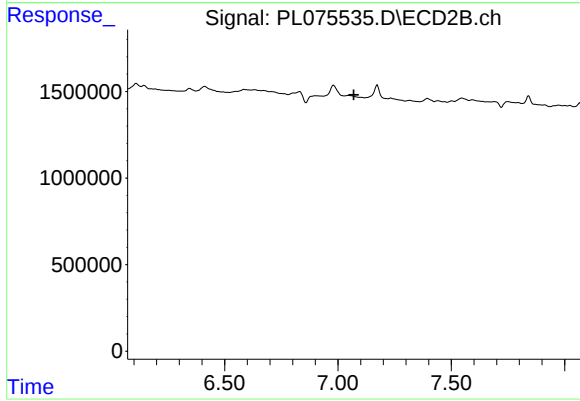

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 7.070 min
Response: 0
Conc: N.D.

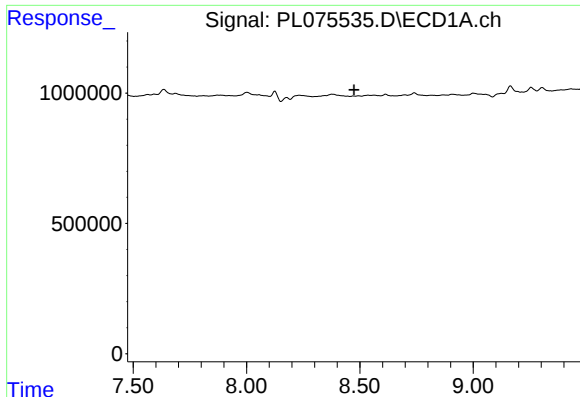

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 8.474 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

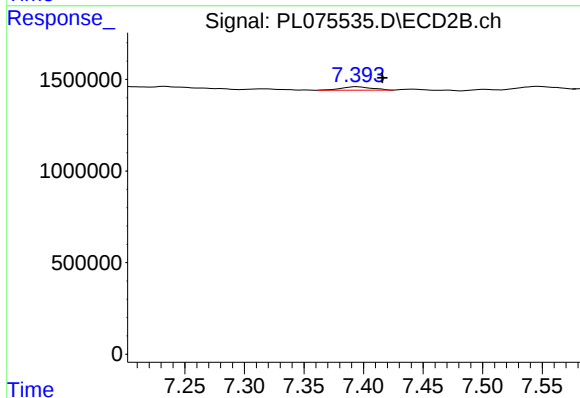


#11 alpha-Chlordane

R.T.: 7.395 min
Delta R.T.: -0.021 min
Response: 345131
Conc: 0.21 ng/ml

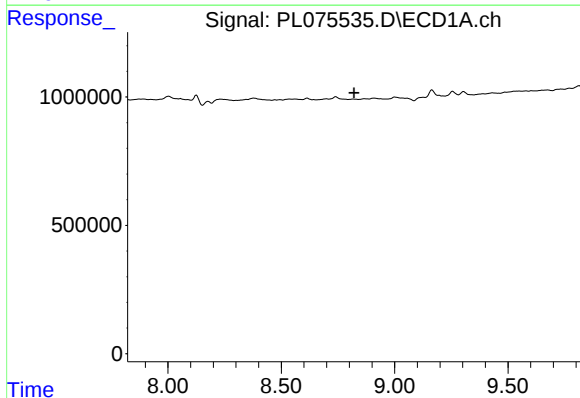


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 8.821 min
Response: 0
Conc: N.D.

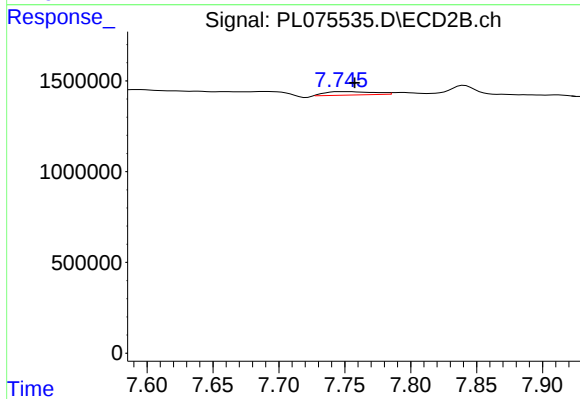

#13 Dieldrin


R.T.: 7.748 min
Delta R.T.: -0.010 min
Response: 494937
Conc: 0.32 ng/ml

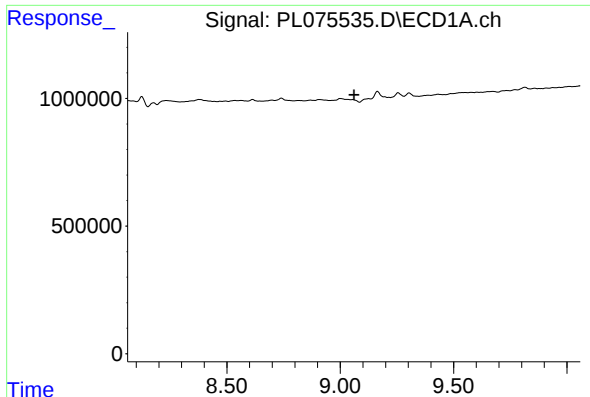

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 9.062 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

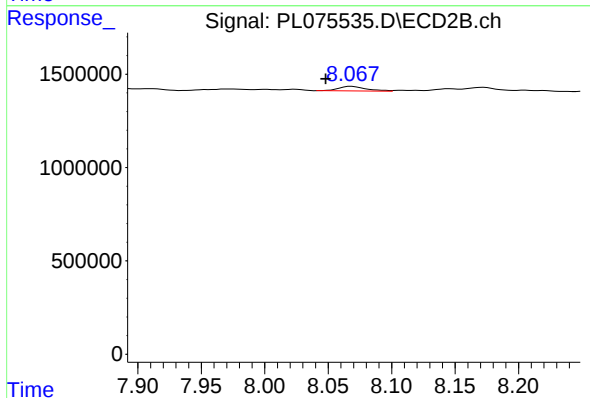


#14 Endrin

R.T.: 8.069 min
Delta R.T.: 0.021 min
Response: 372067
Conc: 0.28 ng/ml

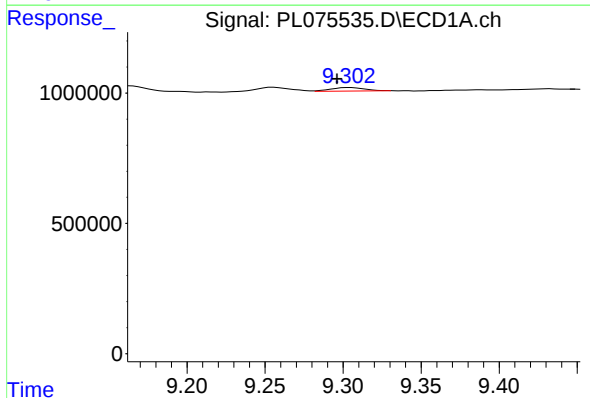


#15 Endosulfan II

R.T.: 9.304 min
Delta R.T.: 0.008 min
Response: 210042
Conc: 0.38 ng/ml

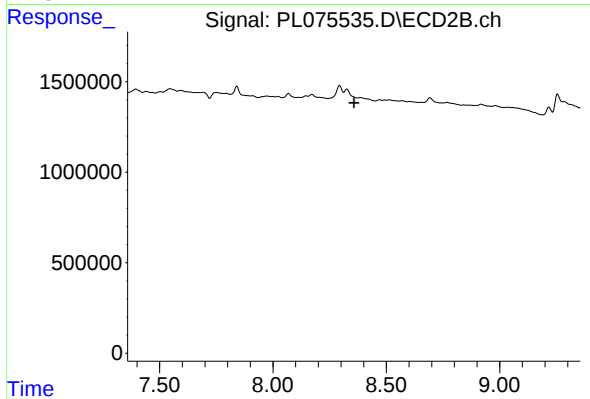

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.358 min
Response: 0
Conc: N.D.

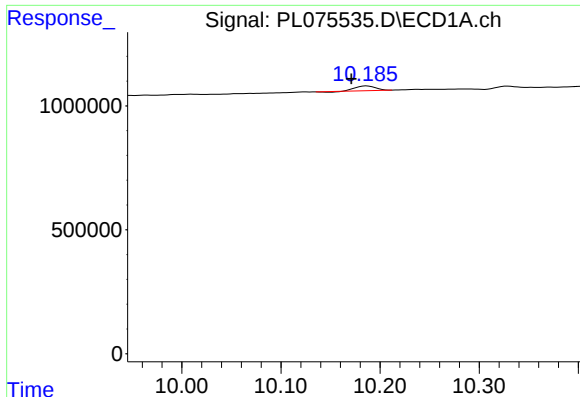

#21 Endrin ketone


R.T.: 10.187 min
Delta R.T.: 0.016 min
Response: 258424
Conc: 0.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

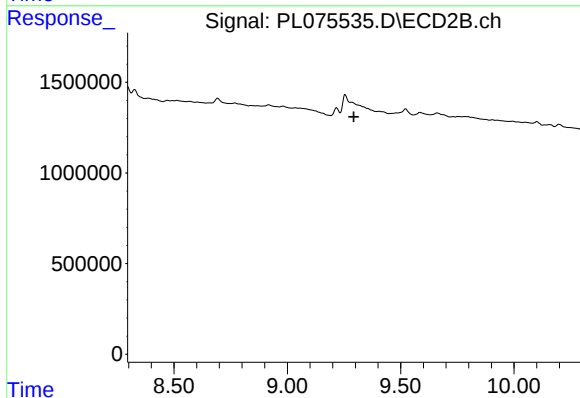


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.294 min
Response: 0
Conc: N.D.

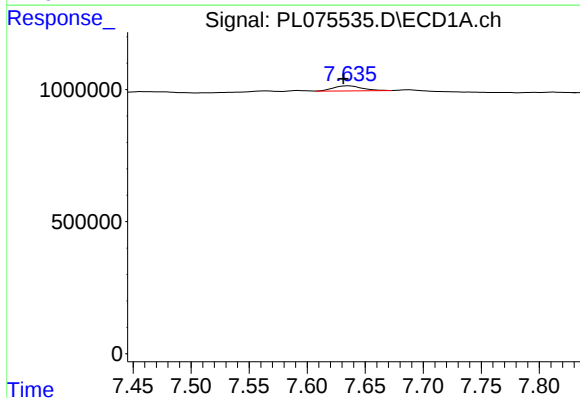


#24 Chlordane-2

R.T.: 7.636 min
Delta R.T.: 0.005 min
Response: 325725
Conc: 10.62 ng/ml

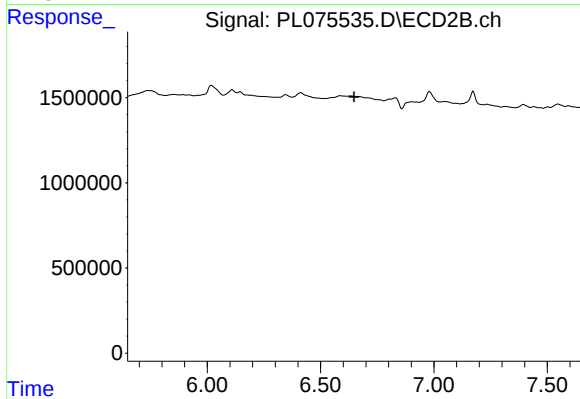

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 6.648 min
Response: 0
Conc: N.D.

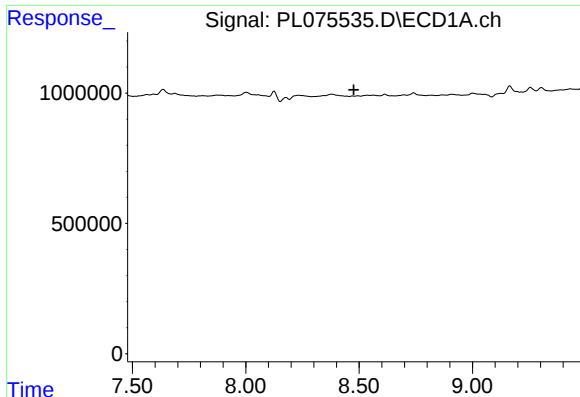

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 8.476 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

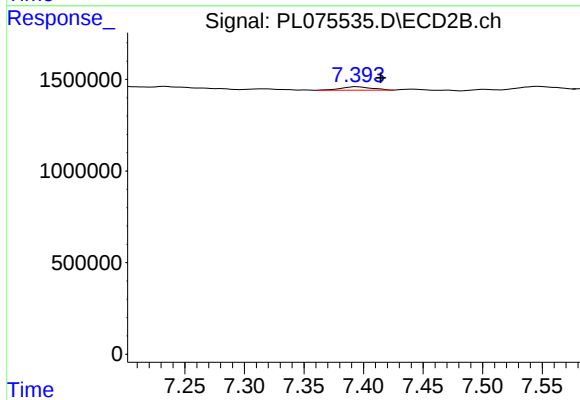


#26 Chlordane-4

R.T.: 7.395 min
Delta R.T.: -0.020 min
Response: 345131
Conc: 2.02 ng/ml

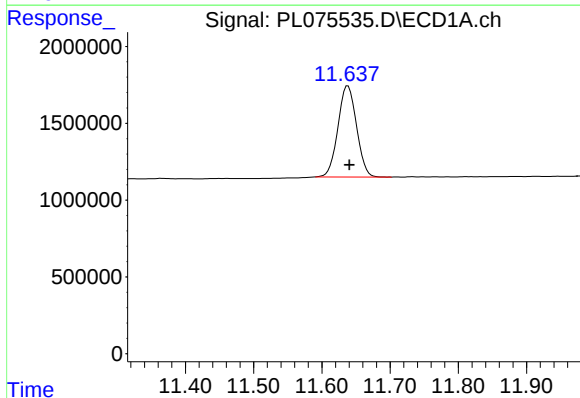

#28 Decachlorobiphenyl

R.T.: 11.638 min
Delta R.T.: -0.002 min
Response: 11231311
Conc: 21.63 ng/ml

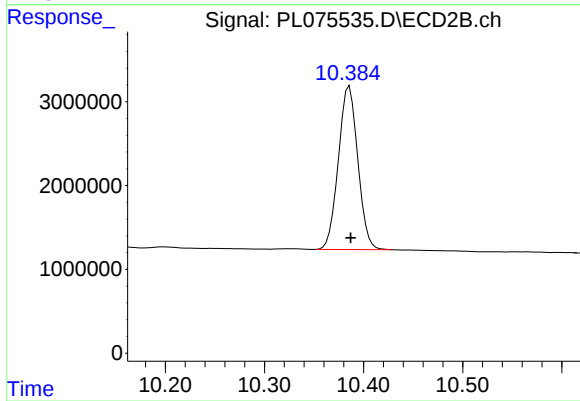

#28 Decachlorobiphenyl

R.T.: 10.386 min
Delta R.T.: -0.002 min
Response: 26535817
Conc: 21.85 ng/ml