

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060422\
 Data File : PL075549.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jun 2022 01:37
 Operator : AR\AJ
 Sample : PB145069BL
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 06 00:24:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060422.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 06 00:15:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.644	4.642	11864672	28223794	19.225	18.375
28)	SA Decachlor...	11.640	10.386	11138061	25497368	21.451	20.993
Target Compounds							
5)	MB Aldrin	7.634f	0.000	240078	0	0.315	N.D. #
7)	B delta-BHC	0.000	6.413	0	417395	N.D.	0.212 #
8)	B Heptachlo...	8.126	0.000	1448609	0	2.046	N.D. #
11)	B alpha-Chl...	0.000	7.396f	0	283763	N.D.	0.174 #
13)	MA Dieldrin	0.000	7.752	0	1497122	N.D.	0.979 #
14)	MA Endrin	0.000	8.070f	0	748434	N.D.	0.554 #
15)	B Endosulfa...	9.306	0.000	166494	0	0.301	N.D. #
17)	MA 4,4'-DDT	0.000	8.467	0	138700	N.D.	0.108 #
21)	B Endrin ke...	10.187f	0.000	249246	0	0.402	N.D. #
24)	Chlordane-2	7.634	0.000	240078	0	7.828	N.D. #
26)	Chlordane-4	0.000	7.396f	0	283763	N.D.	1.660 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060422\
Data File : PL075549.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jun 2022 01:37
Operator : AR\AJ
Sample : PB145069BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 06 00:24:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060422.M
Quant Title : GC Extractables
QLast Update : Mon Jun 06 00:15:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

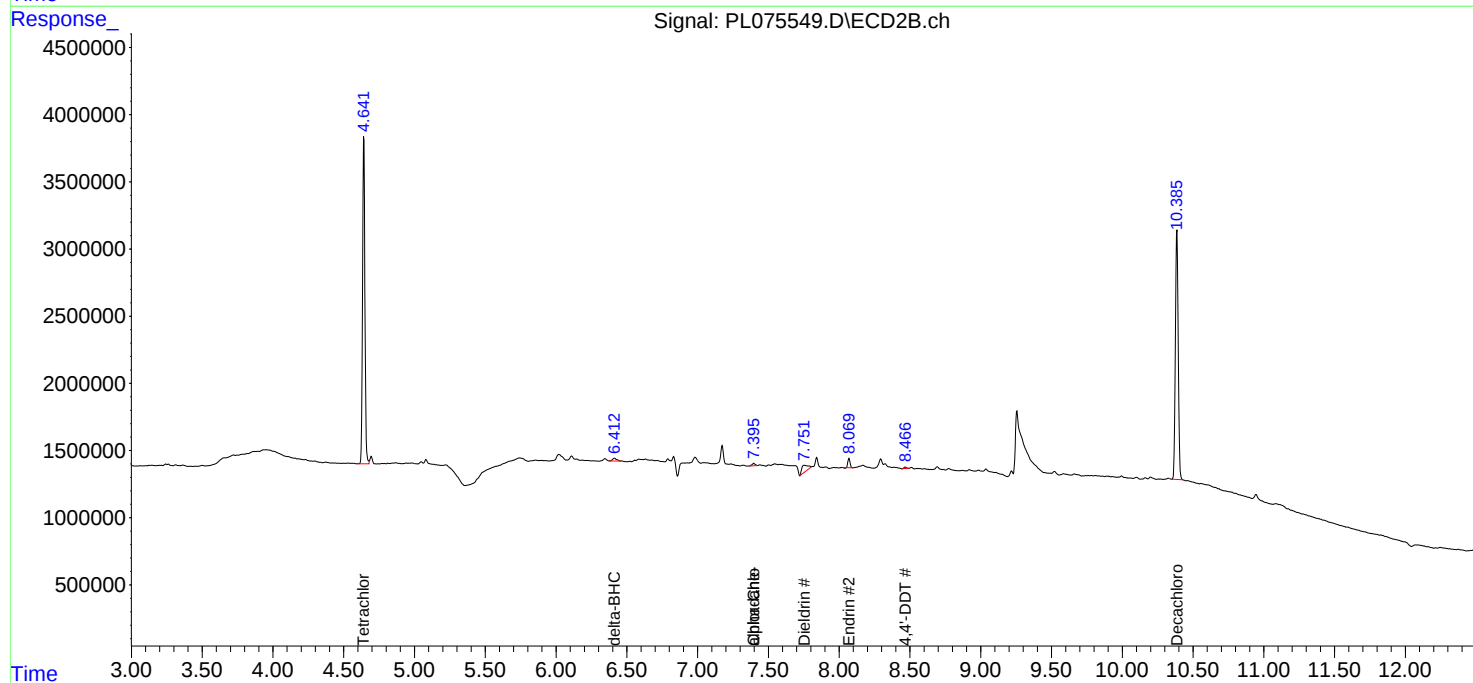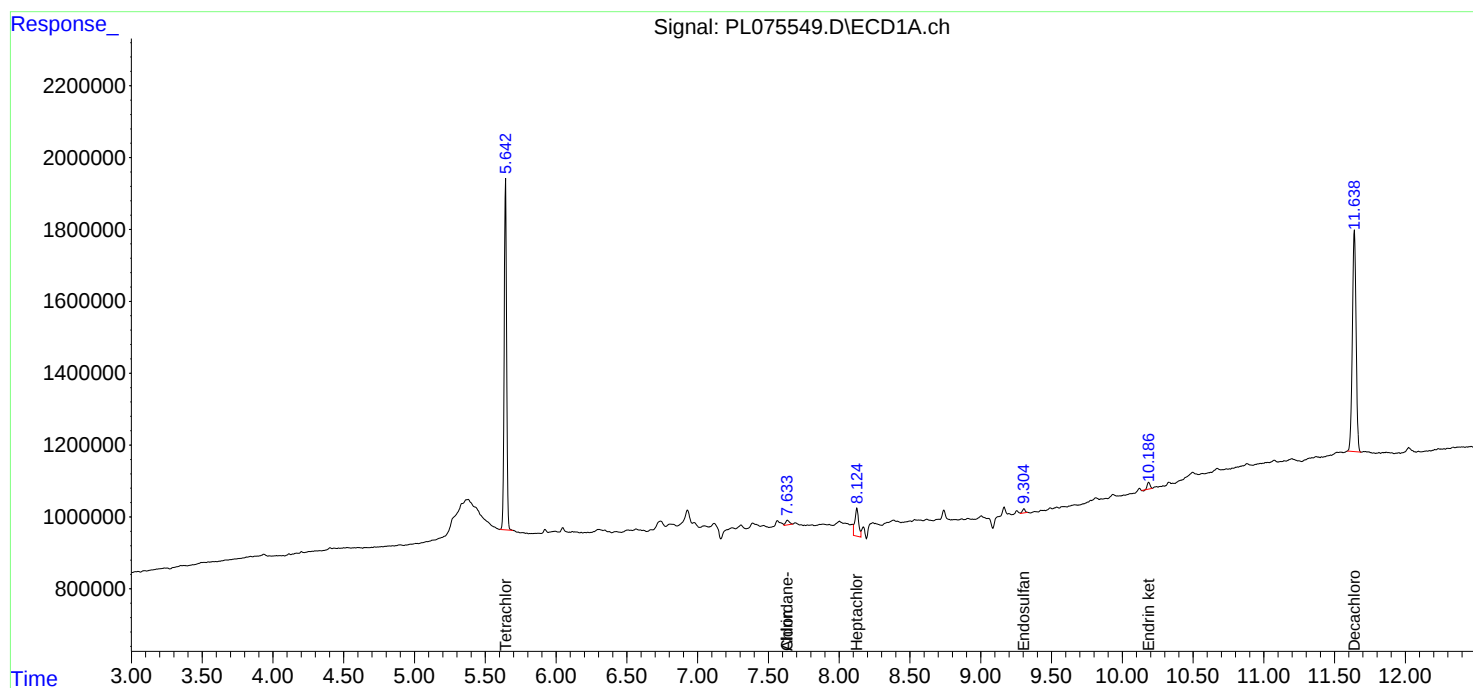


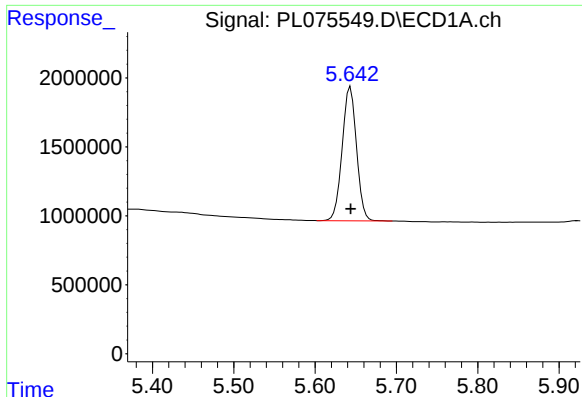

#1 Tetrachloro-m-xylene


R.T.: 5.644 min
Delta R.T.: 0.000 min
Response: 11864672
Conc: 19.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

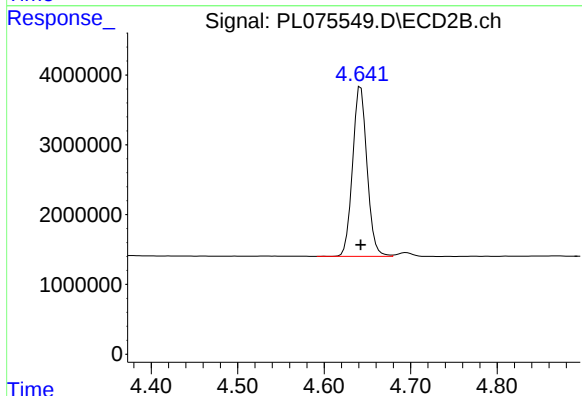


#1 Tetrachloro-m-xylene

R.T.: 4.642 min
Delta R.T.: 0.000 min
Response: 28223794
Conc: 18.38 ng/ml

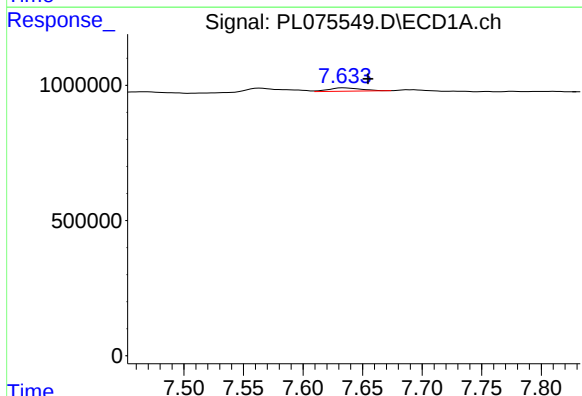


#5 Aldrin

R.T.: 7.634 min
Delta R.T.: -0.020 min
Response: 240078
Conc: 0.32 ng/ml

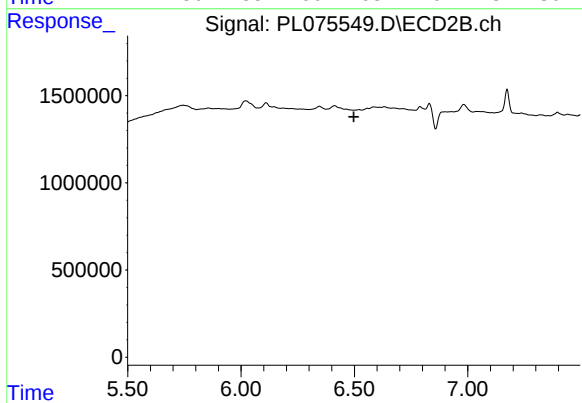

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 6.497 min
Response: 0
Conc: N.D.

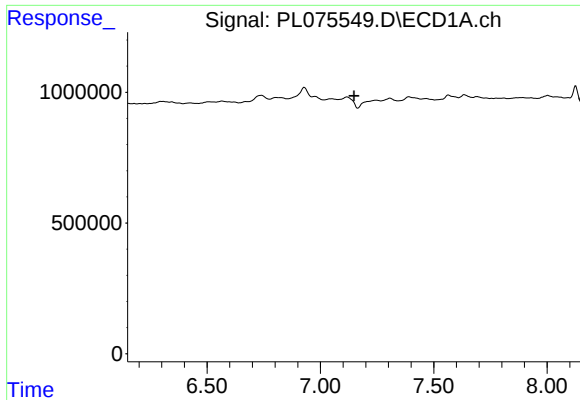

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 7.148 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

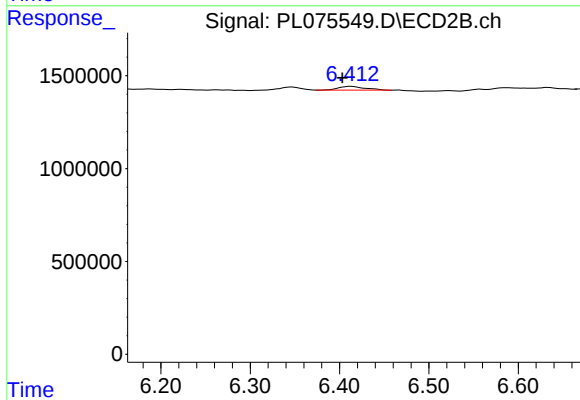


#7 delta-BHC

R.T.: 6.413 min
Delta R.T.: 0.010 min
Response: 417395
Conc: 0.21 ng/ml

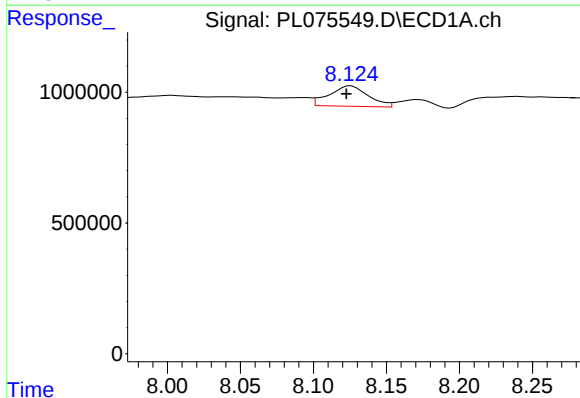


#8 Heptachlor epoxide

R.T.: 8.126 min
Delta R.T.: 0.003 min
Response: 1448609
Conc: 2.05 ng/ml

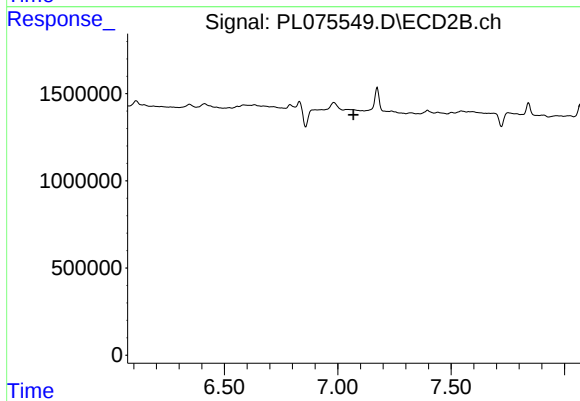

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 7.070 min
Response: 0
Conc: N.D.

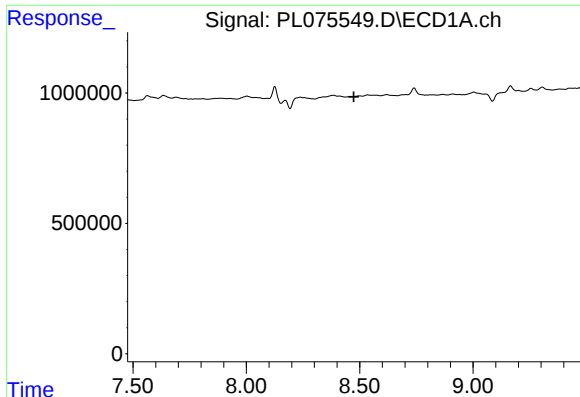

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 8.474 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

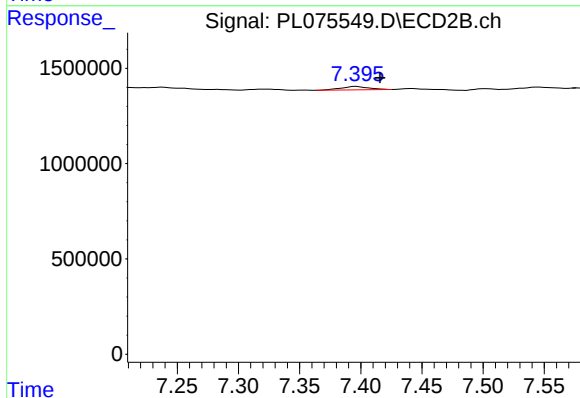


#11 alpha-Chlordane

R.T.: 7.396 min
Delta R.T.: -0.019 min
Response: 283763
Conc: 0.17 ng/ml

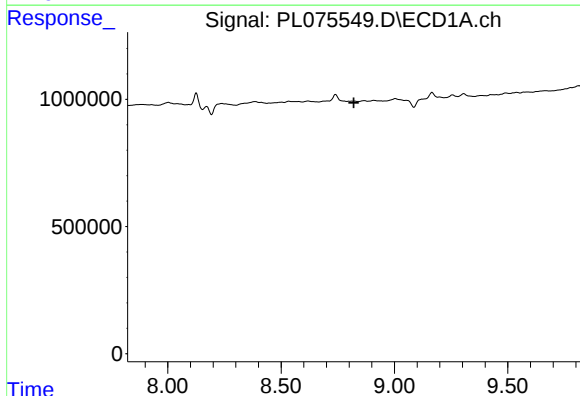


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 8.821 min
Response: 0
Conc: N.D.

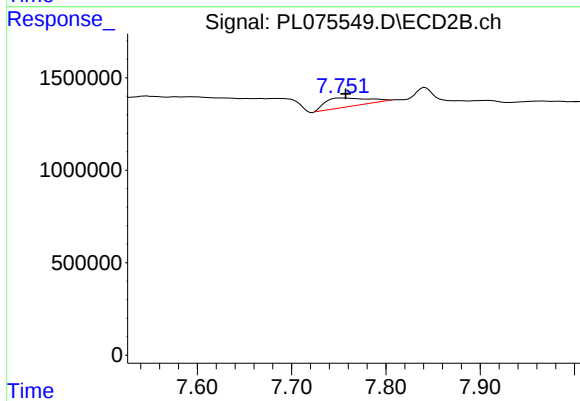

#13 Dieldrin


R.T.: 7.752 min
Delta R.T.: -0.005 min
Response: 1497122
Conc: 0.98 ng/ml

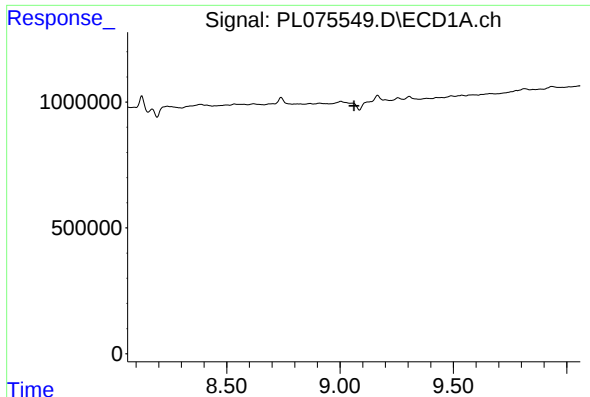

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 9.062 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

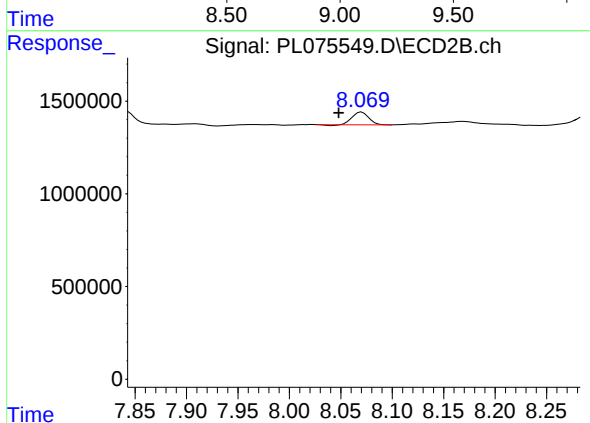


#14 Endrin

R.T.: 8.070 min
Delta R.T.: 0.022 min
Response: 748434
Conc: 0.55 ng/ml

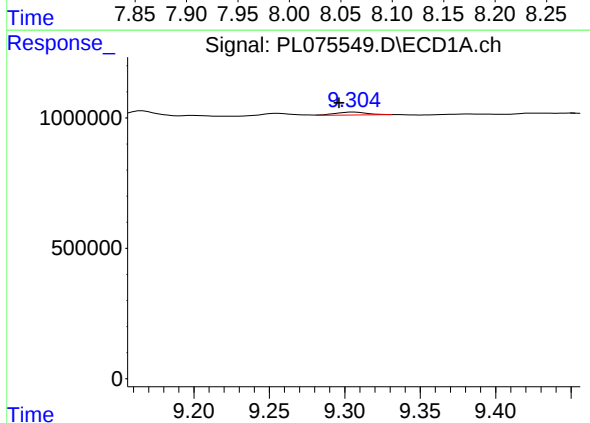


#15 Endosulfan II

R.T.: 9.306 min
Delta R.T.: 0.010 min
Response: 166494
Conc: 0.30 ng/ml

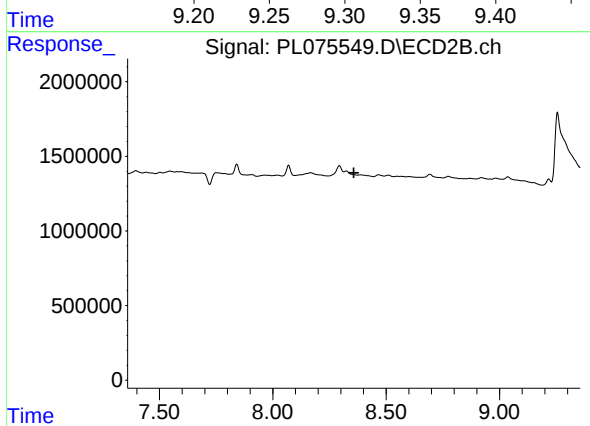

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.358 min
Response: 0
Conc: N.D.

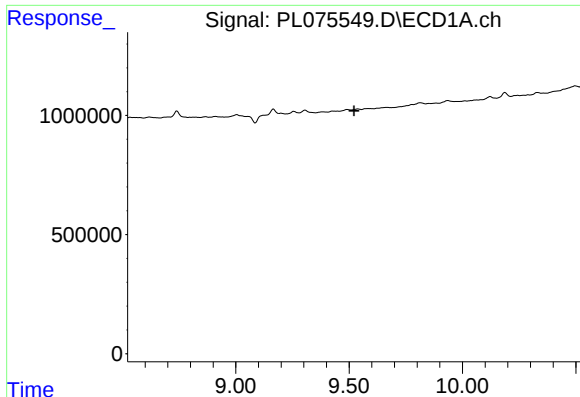

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 9.522 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

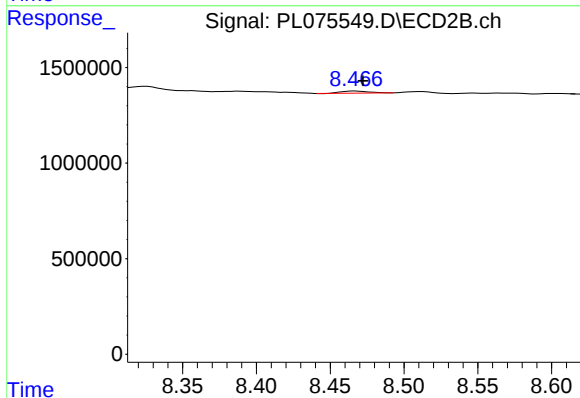


#17 4,4'-DDT

R.T.: 8.467 min
Delta R.T.: -0.005 min
Response: 138700
Conc: 0.11 ng/ml

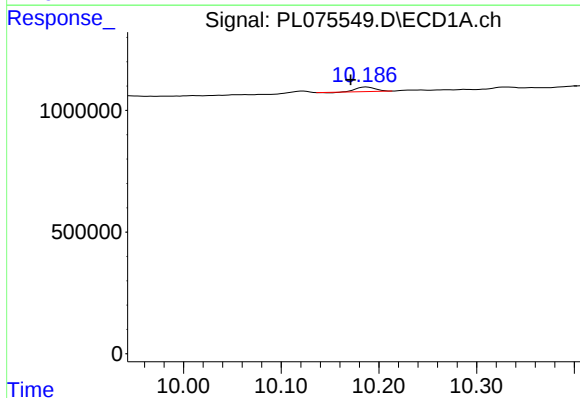


#21 Endrin ketone

R.T.: 10.187 min
Delta R.T.: 0.016 min
Response: 249246
Conc: 0.40 ng/ml

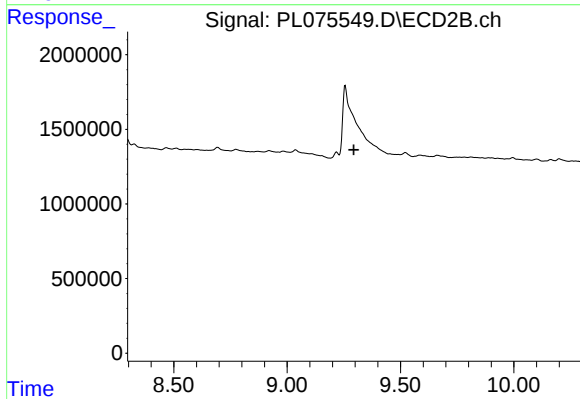

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.294 min
Response: 0
Conc: N.D.

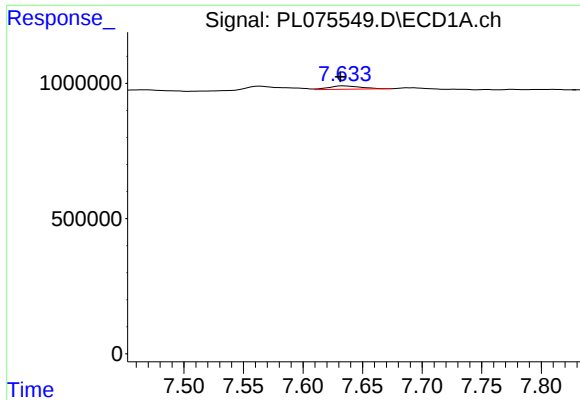

#24 Chlordane-2


R.T.: 7.634 min
Delta R.T.: 0.003 min
Response: 240078
Conc: 7.83 ng/ml

Instrument :
ECD_L
ClientSampleId :

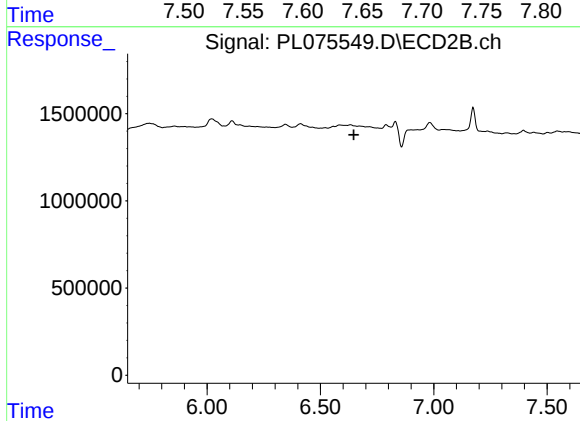


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 6.648 min
Response: 0
Conc: N.D.

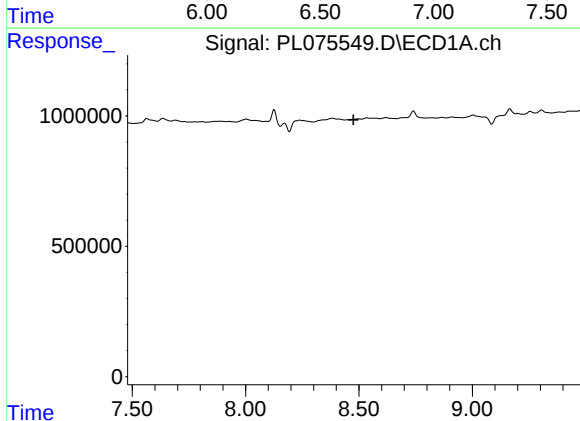


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 8.476 min
Response: 0
Conc: N.D.

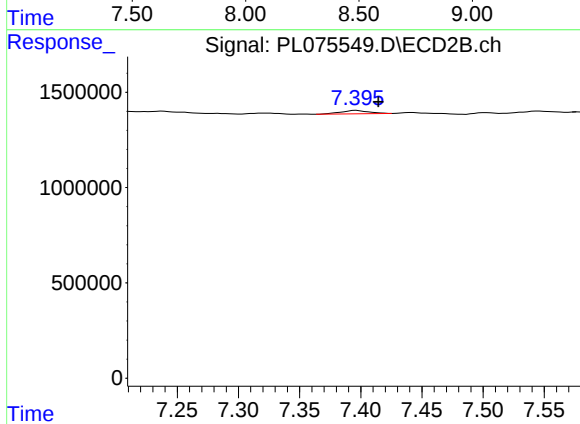

#26 Chlordane-4


R.T.: 7.396 min
Delta R.T.: -0.018 min
Response: 283763
Conc: 1.66 ng/ml

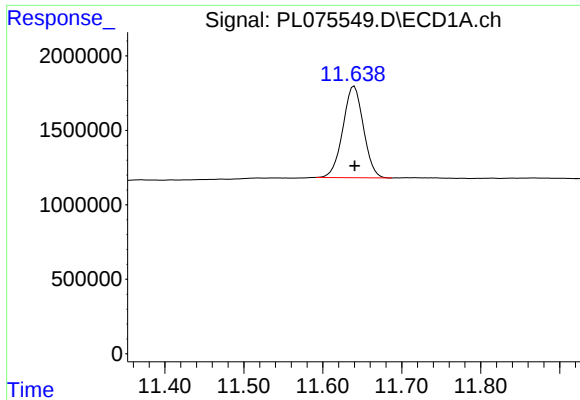

#28 Decachlorobiphenyl

R.T.: 11.640 min
Delta R.T.: 0.000 min
Response: 11138061
Conc: 21.45 ng/ml

Instrument :
ECD_L
ClientSampleId :

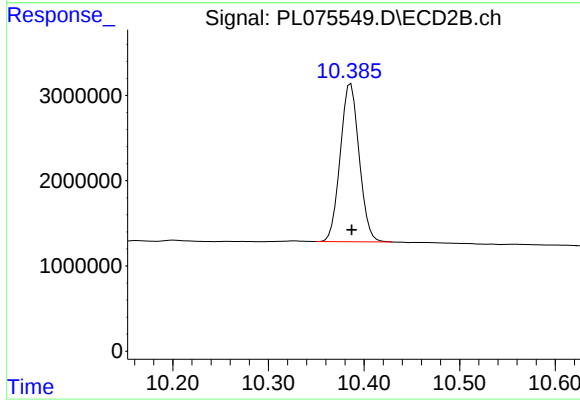

#28 Decachlorobiphenyl

R.T.: 10.386 min
Delta R.T.: -0.001 min
Response: 25497368
Conc: 20.99 ng/ml