

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060422\
 Data File : PL075552.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jun 2022 02:27
 Operator : AR\AJ
 Sample : PB145113BL
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 06 00:25:07 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060422.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 06 00:15:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.643	4.642	12306799	29110874	19.942	18.953
28)	SA Decachlor...	11.639	10.387	11644126	26359052	22.426	21.703
Target Compounds							
5)	MB Aldrin	7.635f	0.000	247120	0	0.324	N.D. #
7)	B delta-BHC	0.000	6.411	0	557826	N.D.	0.283 #
11)	B alpha-Chl...	0.000	7.396f	0	315173	N.D.	0.193 #
13)	MA Dieldrin	0.000	7.753	0	383349	N.D.	0.251 #
15)	B Endosulfa...	9.303	0.000	177099	0	0.320	N.D. #
17)	MA 4,4'-DDT	0.000	8.466	0	192968	N.D.	0.151 #
21)	B Endrin ke...	10.187f	0.000	228483	0	0.368	N.D. #
24)	Chlordane-2	7.635	0.000	247120	0	8.057	N.D. #
26)	Chlordane-4	0.000	7.396f	0	315173	N.D.	1.843 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060422\
Data File : PL075552.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jun 2022 02:27
Operator : AR\AJ
Sample : PB145113BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 06 00:25:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060422.M
Quant Title : GC Extractables
QLast Update : Mon Jun 06 00:15:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

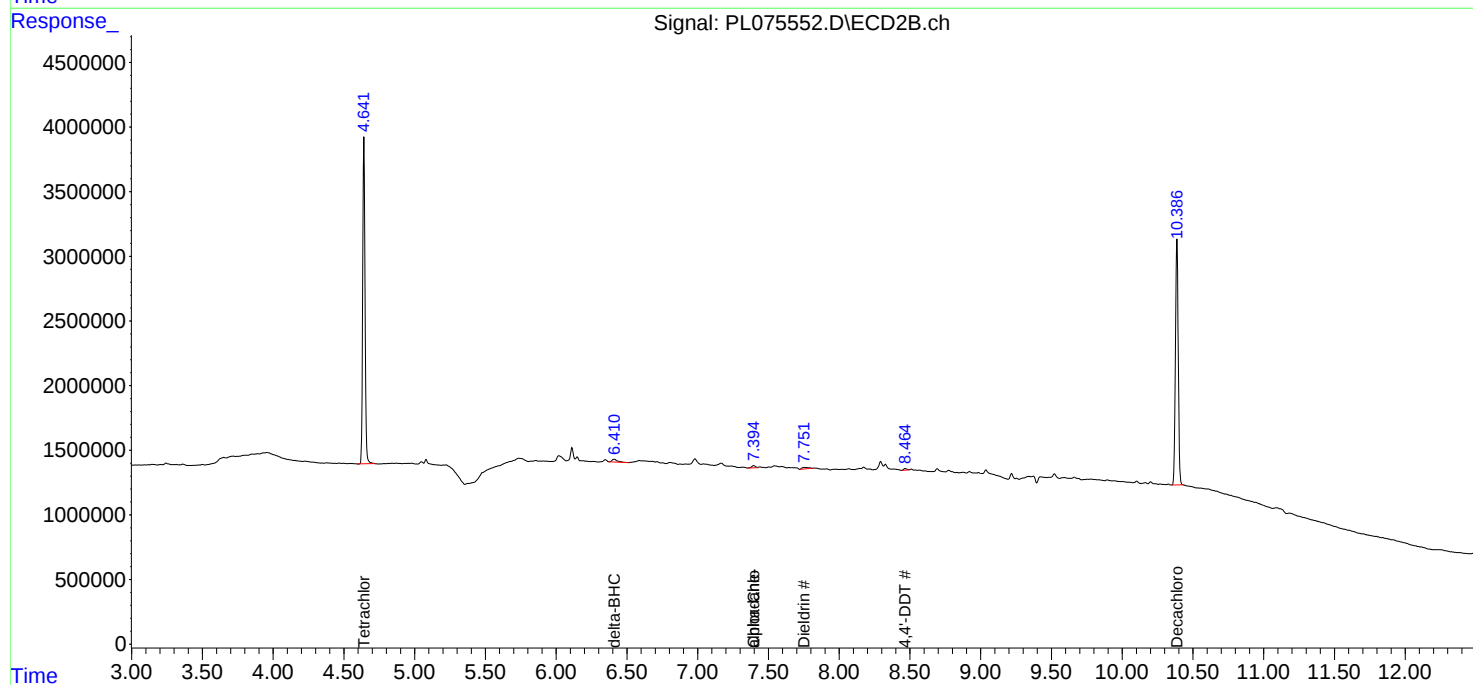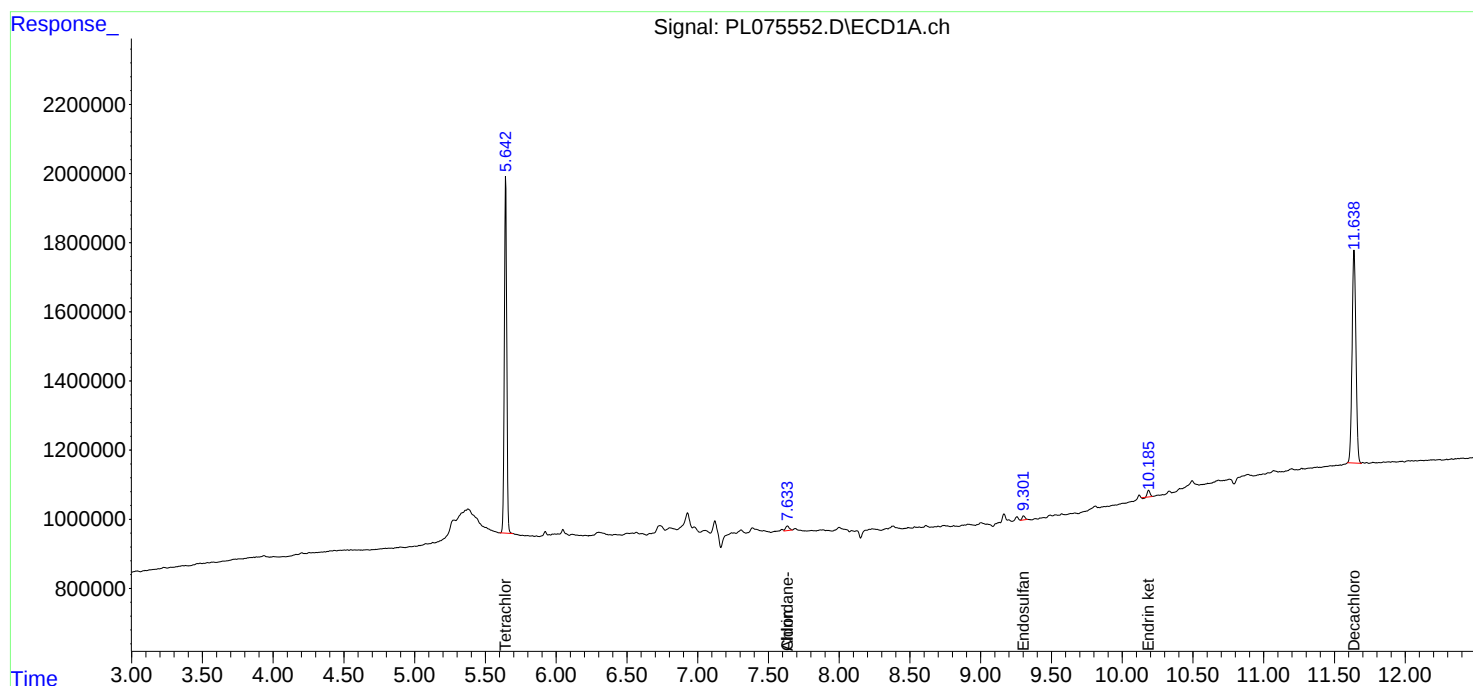


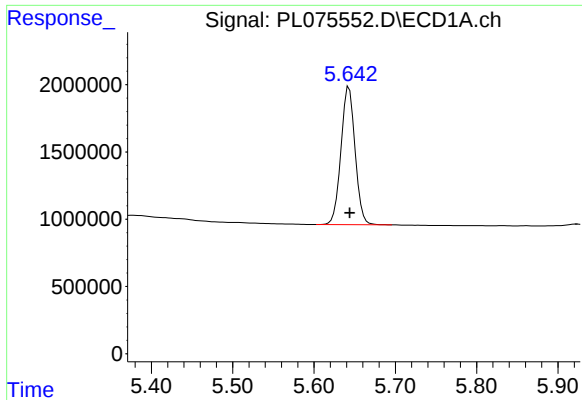

#1 Tetrachloro-m-xylene


R.T.: 5.643 min
Delta R.T.: 0.000 min
Response: 12306799
Conc: 19.94 ng/ml

Instrument :
ECD_L
ClientSampleId :

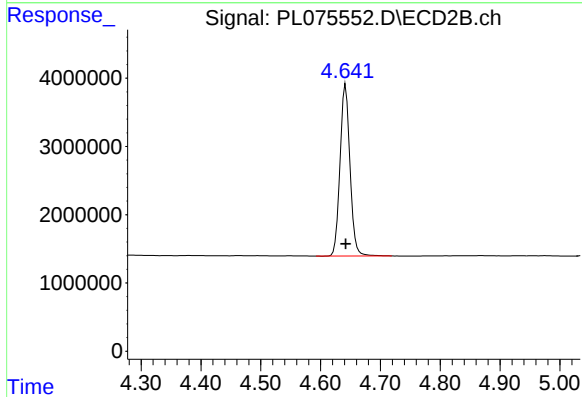


#1 Tetrachloro-m-xylene

R.T.: 4.642 min
Delta R.T.: 0.000 min
Response: 29110874
Conc: 18.95 ng/ml

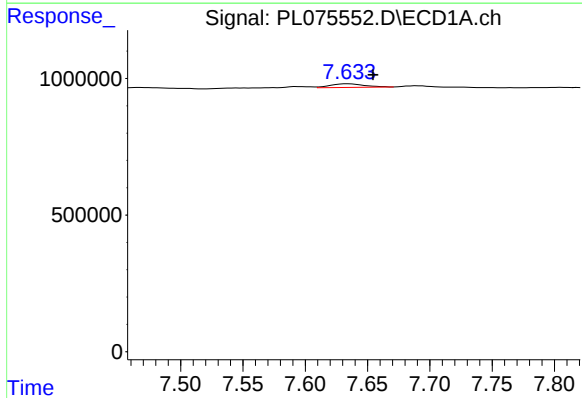


#5 Aldrin

R.T.: 7.635 min
Delta R.T.: -0.020 min
Response: 247120
Conc: 0.32 ng/ml

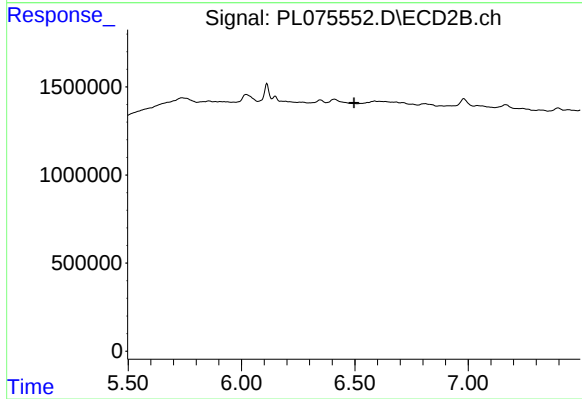

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 6.497 min
Response: 0
Conc: N.D.

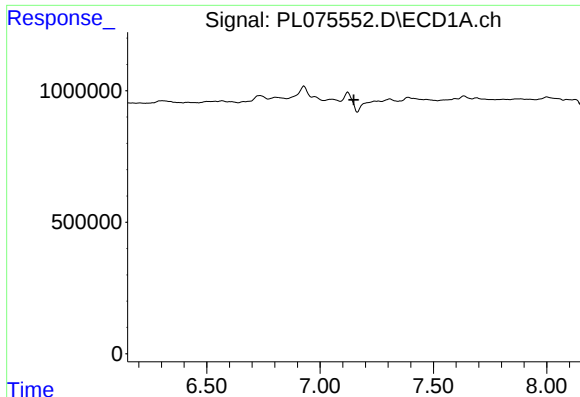

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 7.148 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

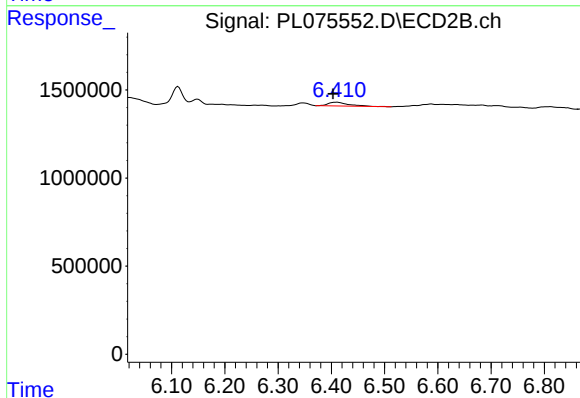


#7 delta-BHC

R.T.: 6.411 min
Delta R.T.: 0.008 min
Response: 557826
Conc: 0.28 ng/ml

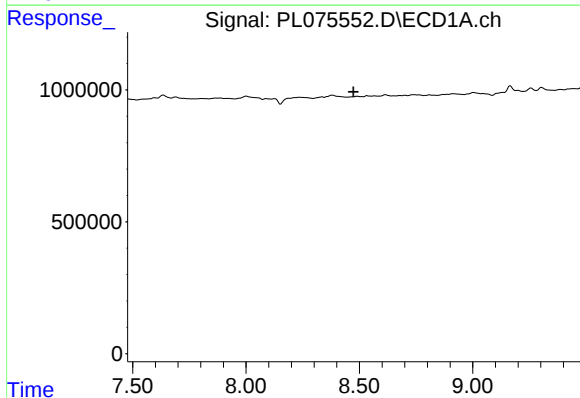


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 8.474 min
Response: 0
Conc: N.D.

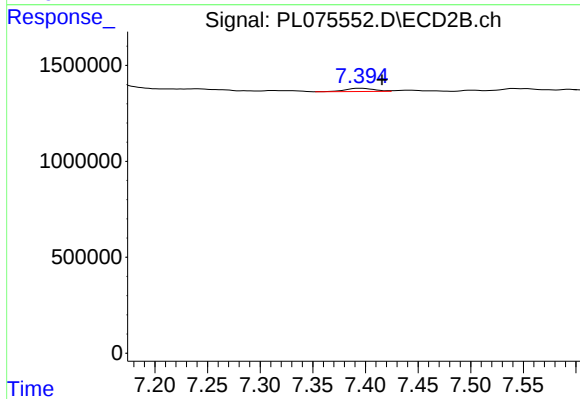

#11 alpha-Chlordane


R.T.: 7.396 min
Delta R.T.: -0.019 min
Response: 315173
Conc: 0.19 ng/ml

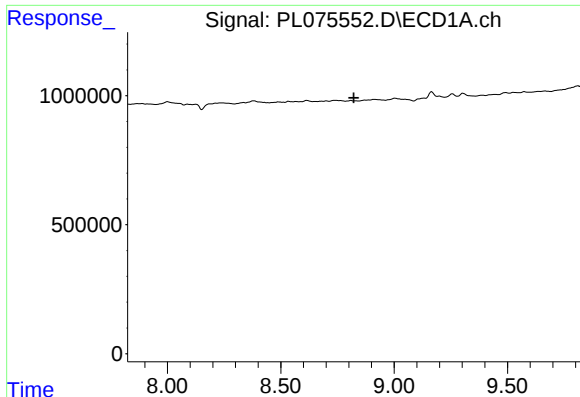

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 8.821 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

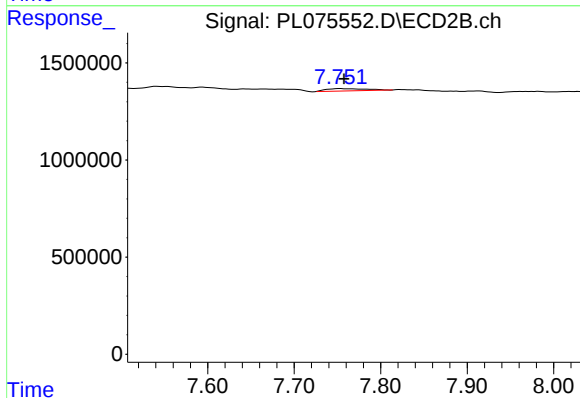


#13 Dieldrin

R.T.: 7.753 min
Delta R.T.: -0.005 min
Response: 383349
Conc: 0.25 ng/ml

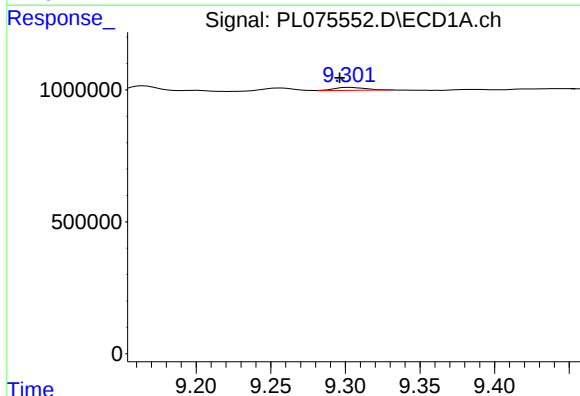


#15 Endosulfan II

R.T.: 9.303 min
Delta R.T.: 0.007 min
Response: 177099
Conc: 0.32 ng/ml

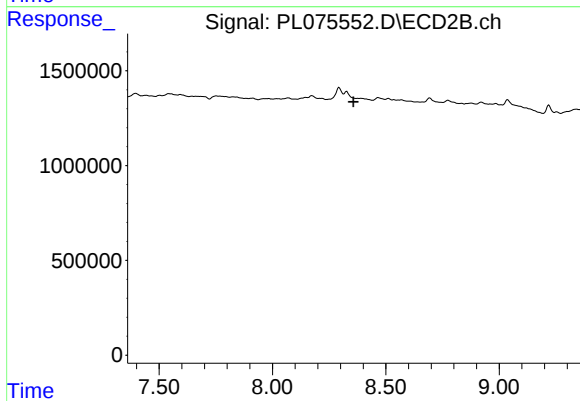

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.358 min
Response: 0
Conc: N.D.

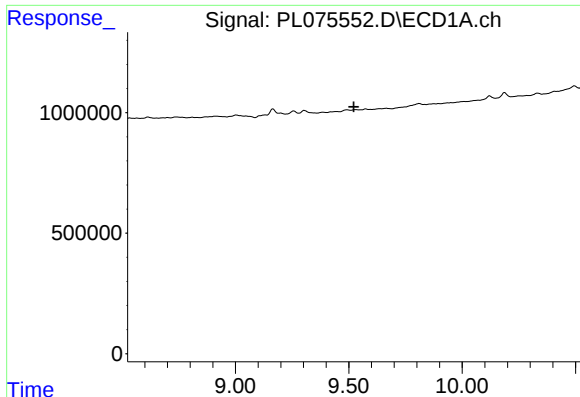

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 9.522 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

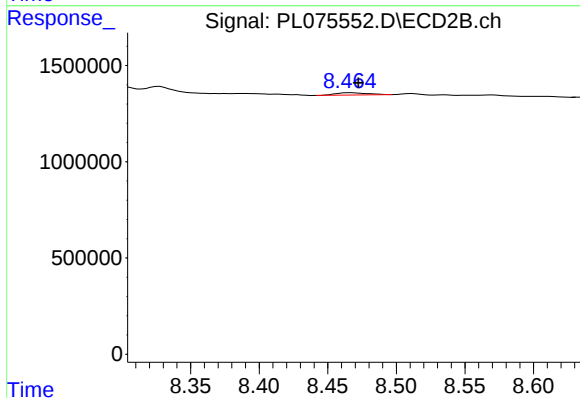


#17 4,4'-DDT

R.T.: 8.466 min
Delta R.T.: -0.006 min
Response: 192968
Conc: 0.15 ng/ml

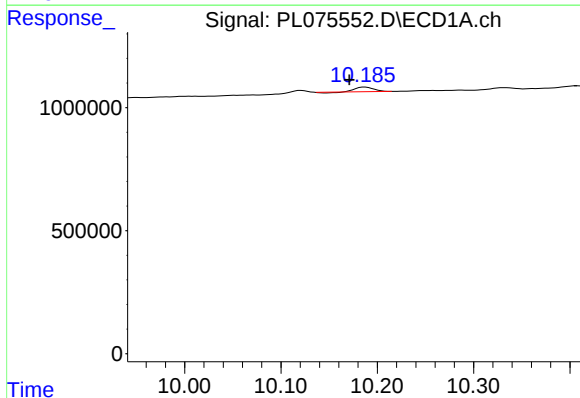


#21 Endrin ketone

R.T.: 10.187 min
Delta R.T.: 0.016 min
Response: 228483
Conc: 0.37 ng/ml

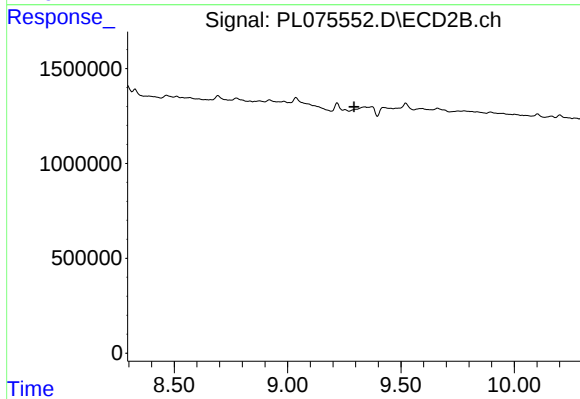

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.294 min
Response: 0
Conc: N.D.

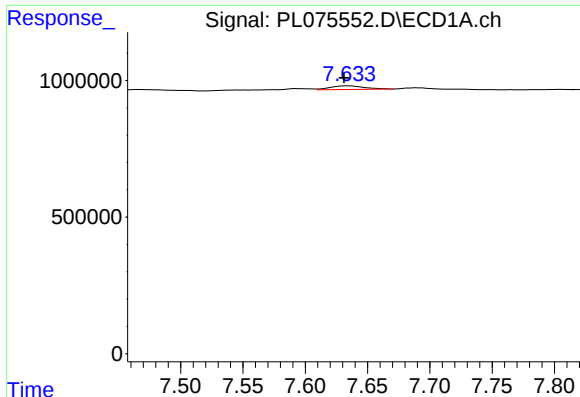

#24 Chlordane-2


R.T.: 7.635 min
Delta R.T.: 0.003 min
Response: 247120
Conc: 8.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

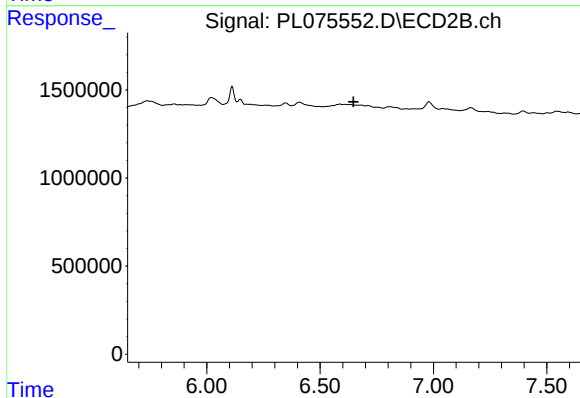


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 6.648 min
Response: 0
Conc: N.D.

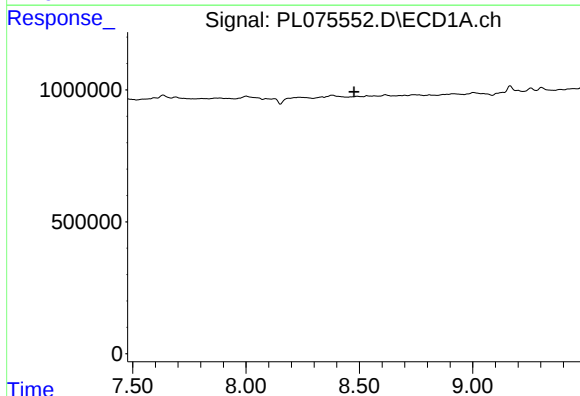


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 8.476 min
Response: 0
Conc: N.D.

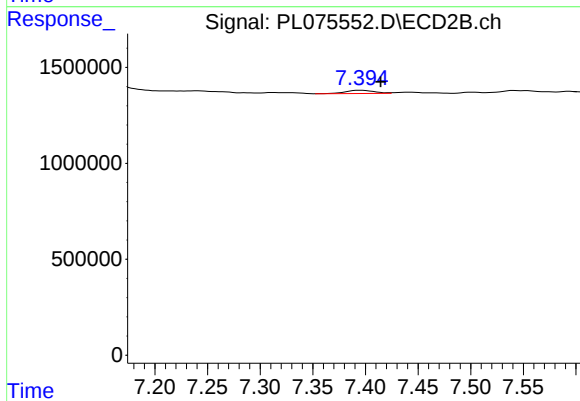

#26 Chlordane-4


R.T.: 7.396 min
Delta R.T.: -0.018 min
Response: 315173
Conc: 1.84 ng/ml

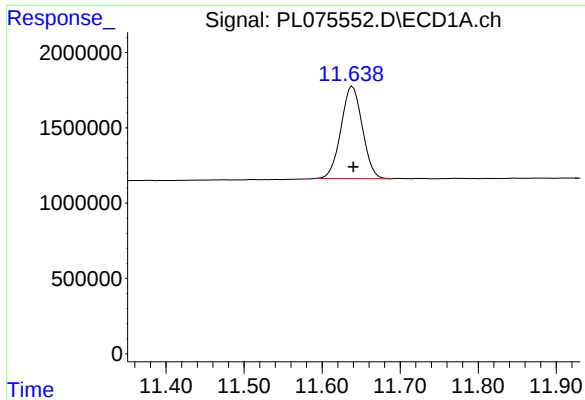

#28 Decachlorobiphenyl

R.T.: 11.639 min
Delta R.T.: -0.001 min
Response: 11644126
Conc: 22.43 ng/ml

Instrument :
ECD_L
ClientSampleId :

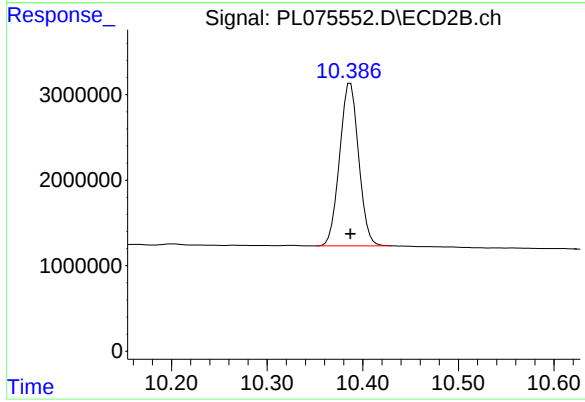

#28 Decachlorobiphenyl

R.T.: 10.387 min
Delta R.T.: 0.000 min
Response: 26359052
Conc: 21.70 ng/ml