

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060422\
 Data File : PL075554.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jun 2022 02:59
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 06 00:25:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060422.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 06 00:15:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.643	4.642	12835492	30510918	20.799	19.864
28)	SA Decachlor...	11.639	10.387	11653136	26376890	22.443	21.717
Target Compounds							
5)	MB Aldrin	7.639f	0.000	267025	0	0.351	N.D. #
7)	B delta-BHC	0.000	6.412	0	549978	N.D.	0.279 #
8)	B Heptachlo...	8.124	0.000	450349	0	0.636	N.D. #
11)	B alpha-Chl...	0.000	7.397f	0	246850	N.D.	0.152 #
13)	MA Dieldrin	0.000	7.755	0	499287	N.D.	0.327 #
14)	MA Endrin	0.000	8.069f	0	187273	N.D.	0.139 #
15)	B Endosulfa...	9.306	0.000	189534	0	0.342	N.D. #
17)	MA 4,4'-DDT	0.000	8.466	0	199477	N.D.	0.156 #
19)	B Endosulfa...	0.000	8.774	0	215470	N.D.	0.164 #
21)	B Endrin ke...	10.186f	0.000	196293	0	0.316	N.D. #
24)	Chlordane-2	7.639	0.000	267025	0	8.706	N.D. #
26)	Chlordane-4	0.000	7.397f	0	246850	N.D.	1.444 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060422\
Data File : PL075554.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jun 2022 02:59
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 06 00:25:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060422.M
Quant Title : GC Extractables
QLast Update : Mon Jun 06 00:15:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

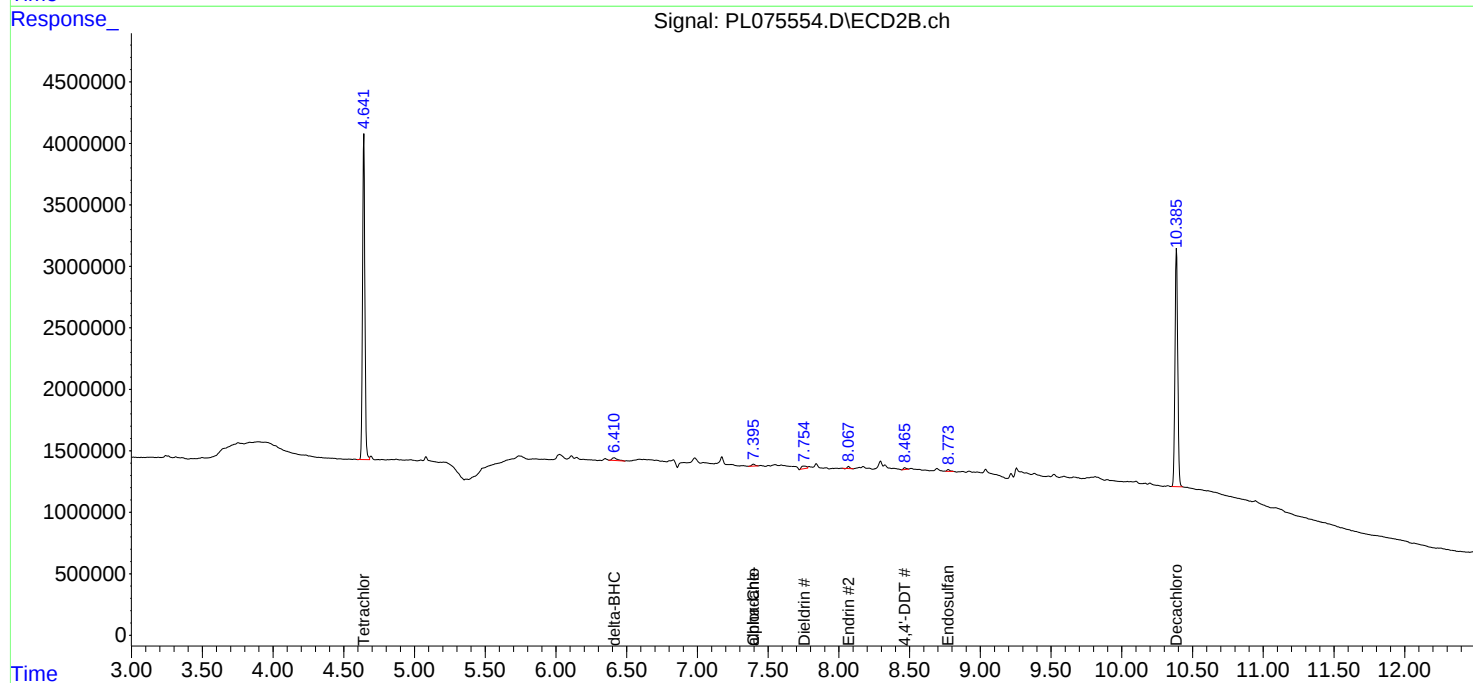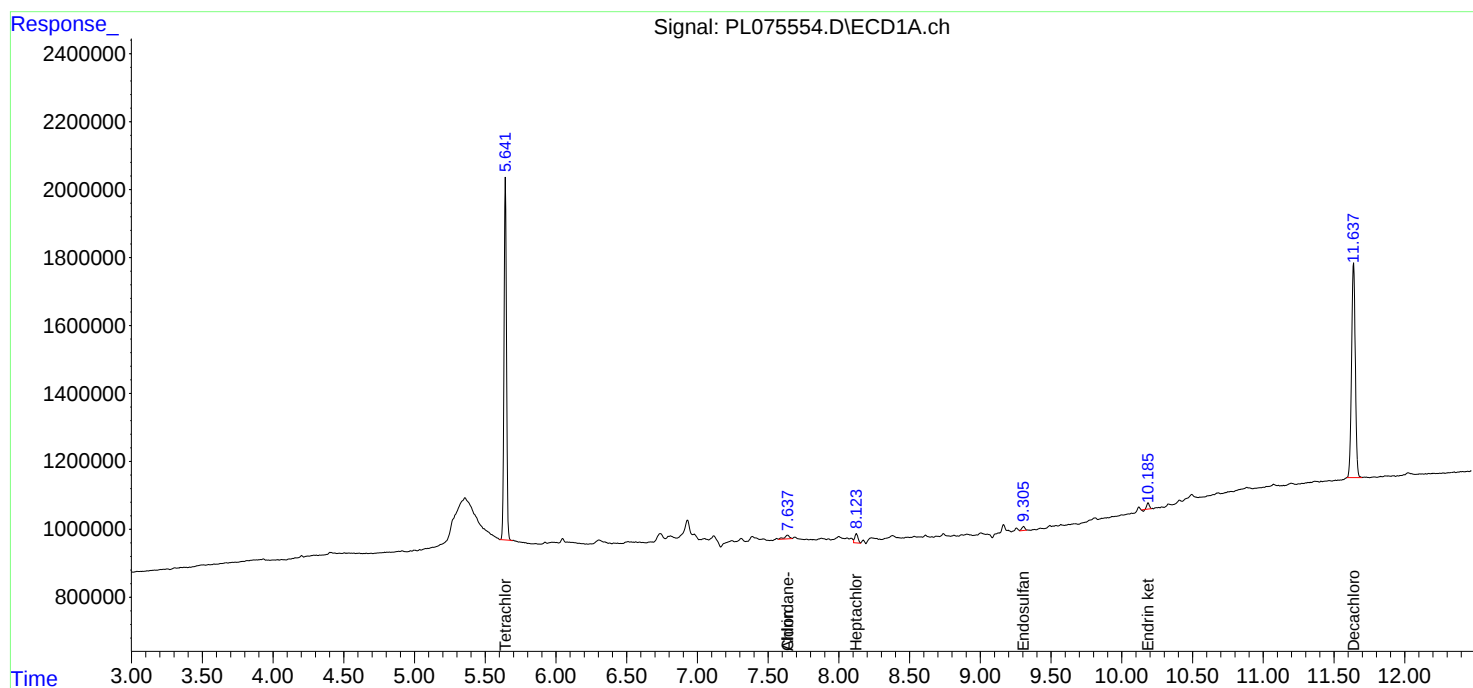


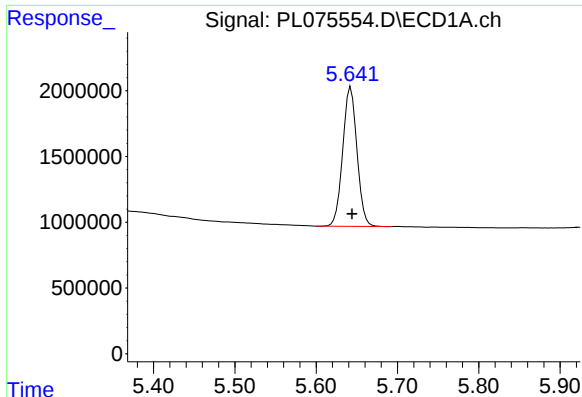

#1 Tetrachloro-m-xylene


R.T.: 5.643 min
Delta R.T.: -0.001 min
Response: 12835492
Conc: 20.80 ng/ml

Instrument :
ECD_L
ClientSampleId :

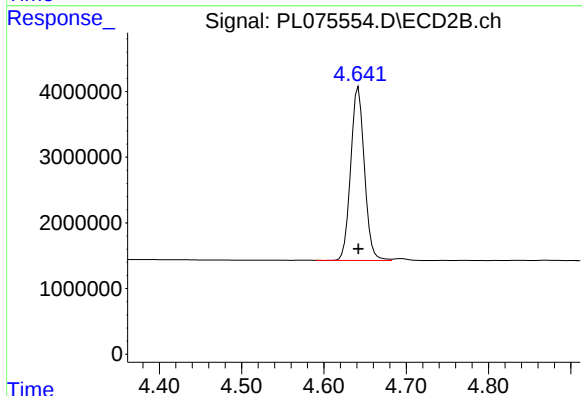


#1 Tetrachloro-m-xylene

R.T.: 4.642 min
Delta R.T.: 0.000 min
Response: 30510918
Conc: 19.86 ng/ml

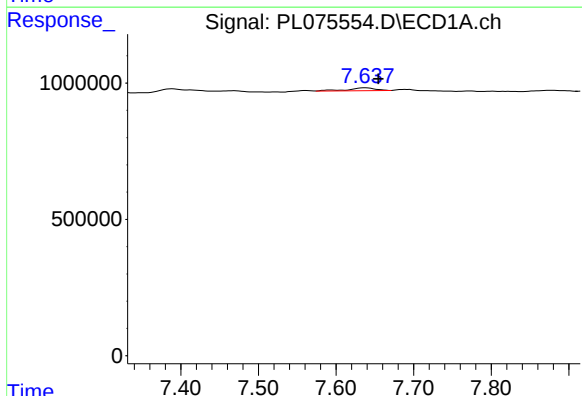


#5 Aldrin

R.T.: 7.639 min
Delta R.T.: -0.016 min
Response: 267025
Conc: 0.35 ng/ml

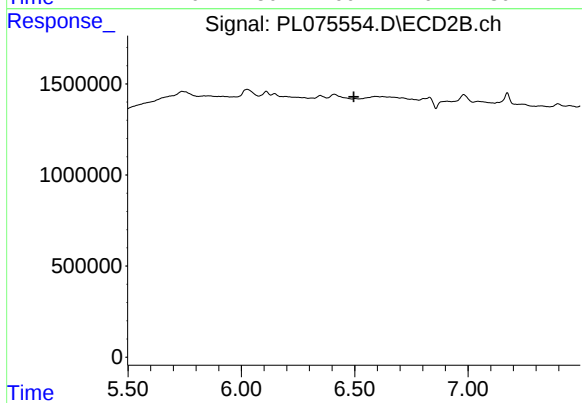

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 6.497 min
Response: 0
Conc: N.D.

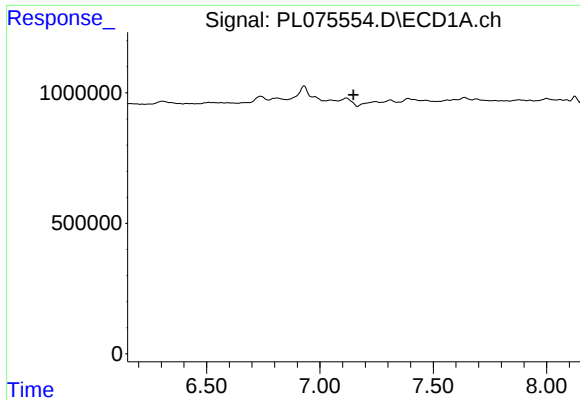

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 7.148 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

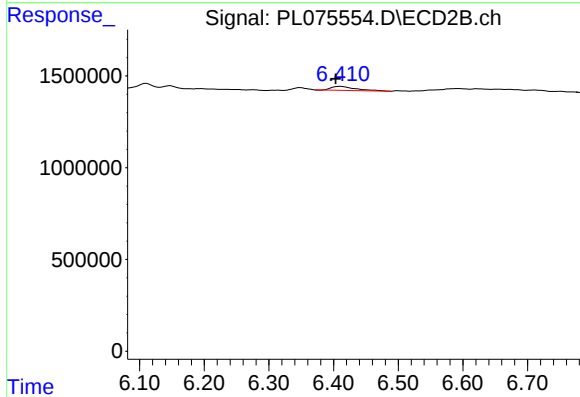


#7 delta-BHC

R.T.: 6.412 min
Delta R.T.: 0.009 min
Response: 549978
Conc: 0.28 ng/ml

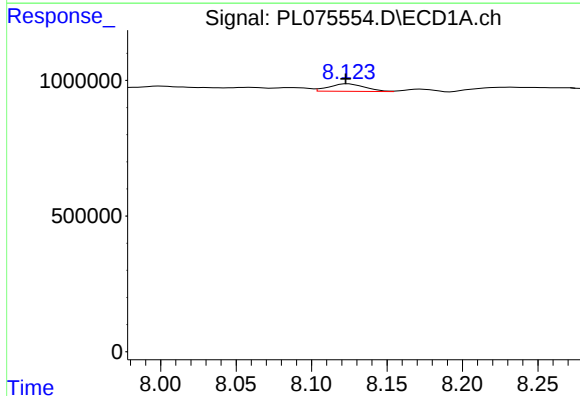


#8 Heptachlor epoxide

R.T.: 8.124 min
Delta R.T.: 0.002 min
Response: 450349
Conc: 0.64 ng/ml

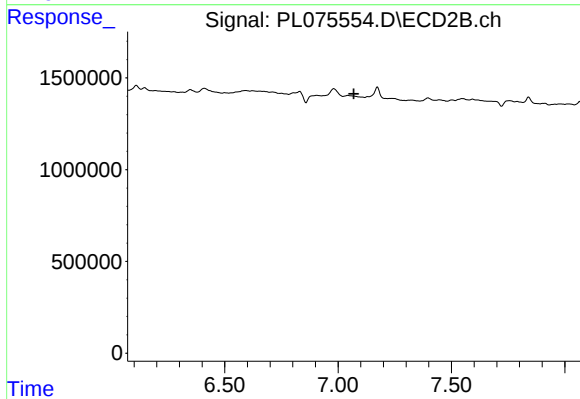

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 7.070 min
Response: 0
Conc: N.D.

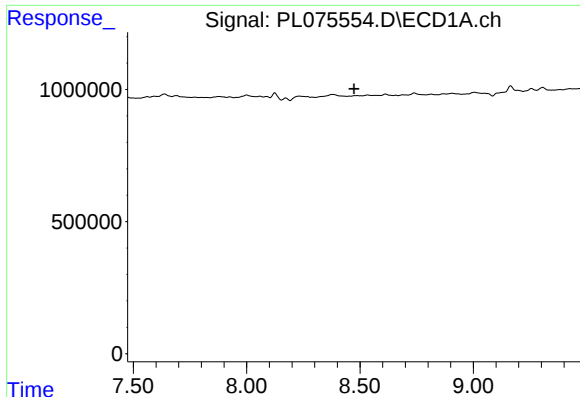

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 8.474 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

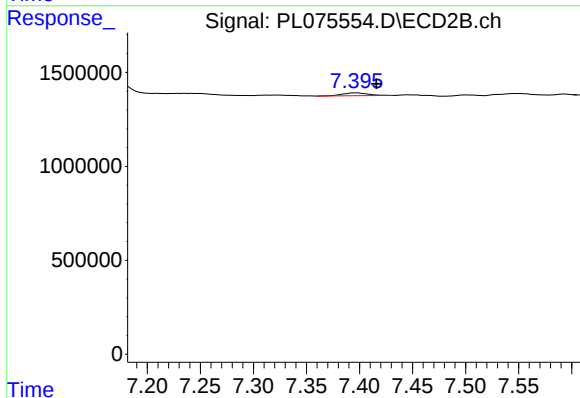


#11 alpha-Chlordane

R.T.: 7.397 min
Delta R.T.: -0.019 min
Response: 246850
Conc: 0.15 ng/ml

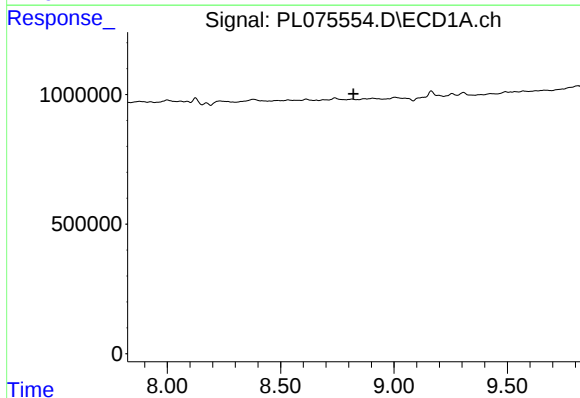


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 8.821 min
Response: 0
Conc: N.D.

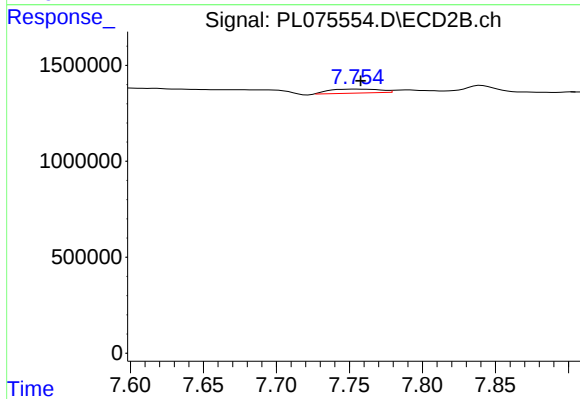

#13 Dieldrin


R.T.: 7.755 min
Delta R.T.: -0.003 min
Response: 499287
Conc: 0.33 ng/ml

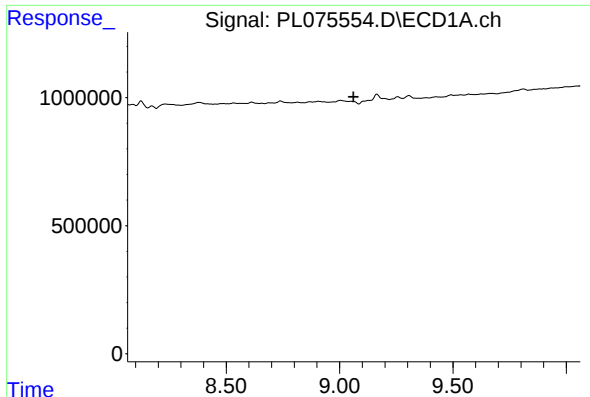

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 9.062 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

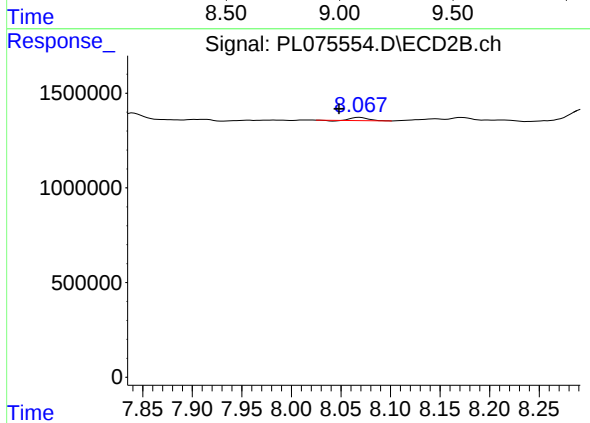


#14 Endrin

R.T.: 8.069 min
Delta R.T.: 0.021 min
Response: 187273
Conc: 0.14 ng/ml

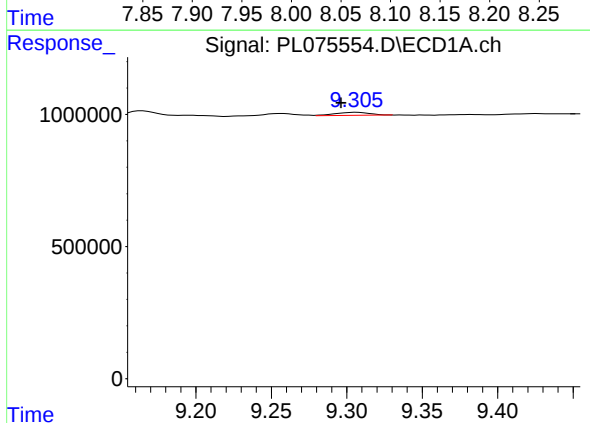


#15 Endosulfan II

R.T.: 9.306 min
Delta R.T.: 0.010 min
Response: 189534
Conc: 0.34 ng/ml

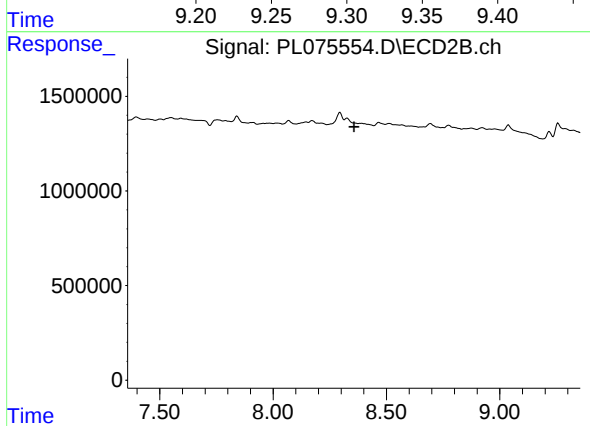

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.358 min
Response: 0
Conc: N.D.

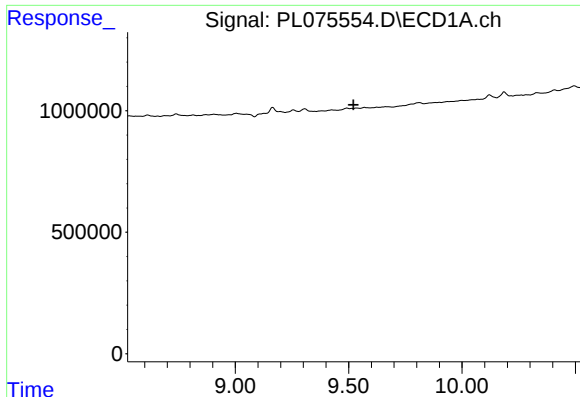

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 9.522 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

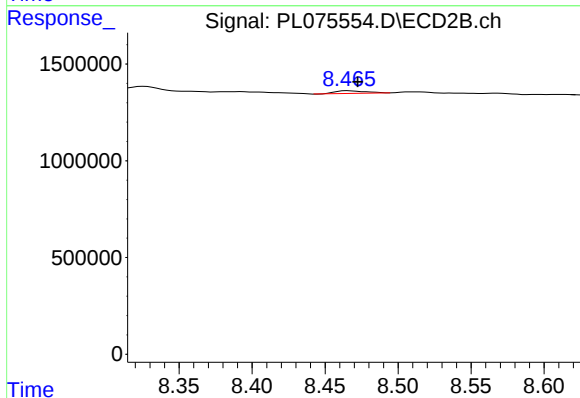


#17 4,4'-DDT

R.T.: 8.466 min
Delta R.T.: -0.006 min
Response: 199477
Conc: 0.16 ng/ml

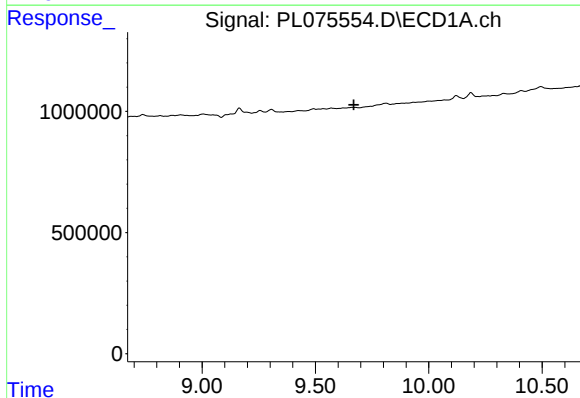


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 9.669 min
Response: 0
Conc: N.D.

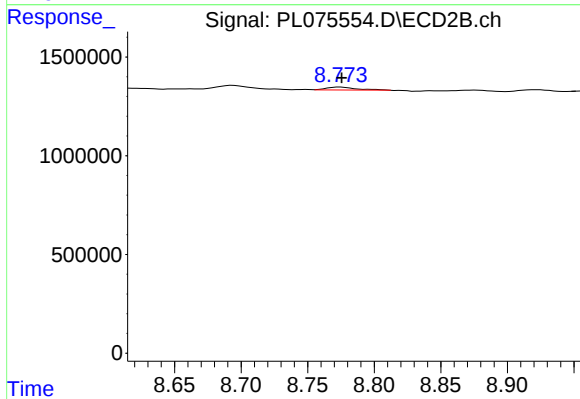

#19 Endosulfan Sulfate


R.T.: 8.774 min
Delta R.T.: -0.001 min
Response: 215470
Conc: 0.16 ng/ml

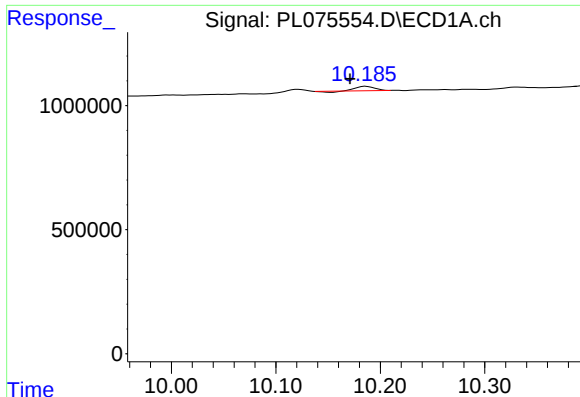

#21 Endrin ketone


R.T.: 10.186 min
Delta R.T.: 0.015 min
Response: 196293
Conc: 0.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

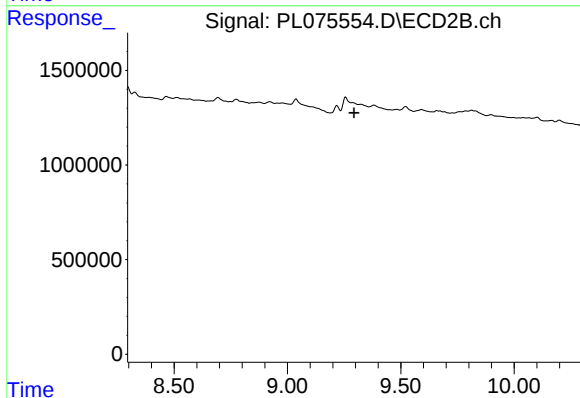


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.294 min
Response: 0
Conc: N.D.

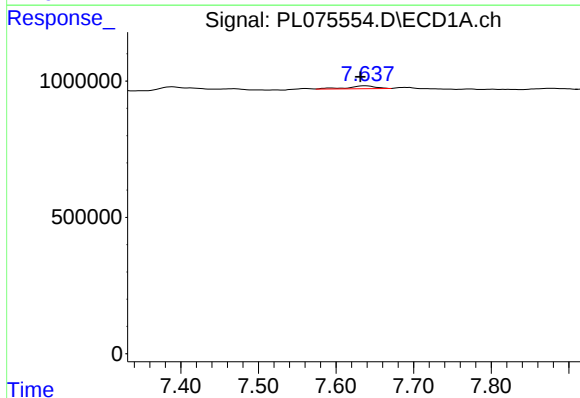


#24 Chlordane-2

R.T.: 7.639 min
Delta R.T.: 0.007 min
Response: 267025
Conc: 8.71 ng/ml

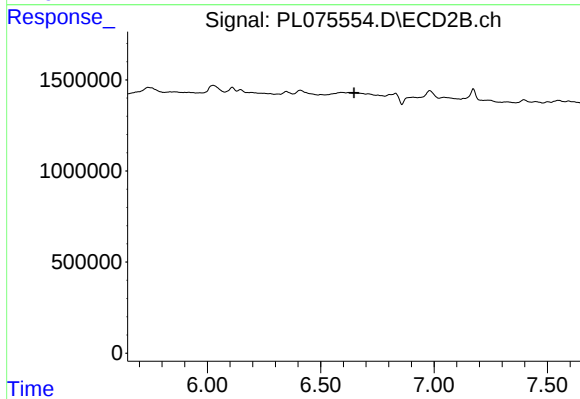

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 6.648 min
Response: 0
Conc: N.D.

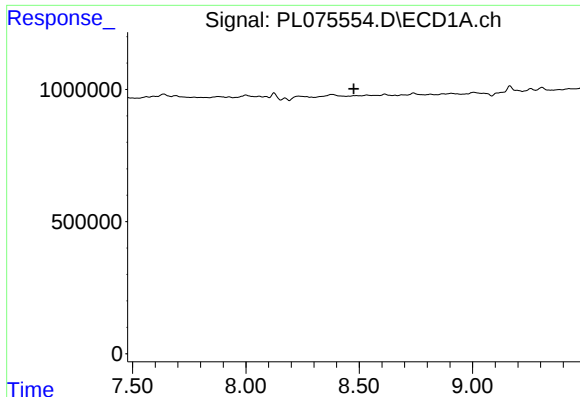

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 8.476 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

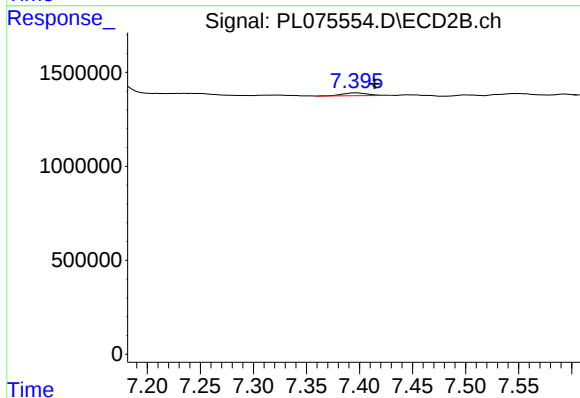


#26 Chlordane-4

R.T.: 7.397 min
Delta R.T.: -0.018 min
Response: 246850
Conc: 1.44 ng/ml

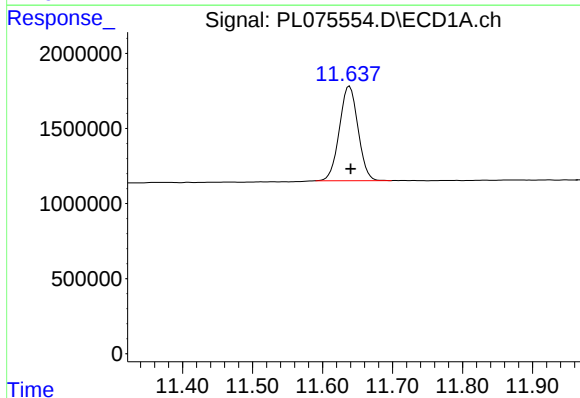

#28 Decachlorobiphenyl

R.T.: 11.639 min
Delta R.T.: -0.002 min
Response: 11653136
Conc: 22.44 ng/ml

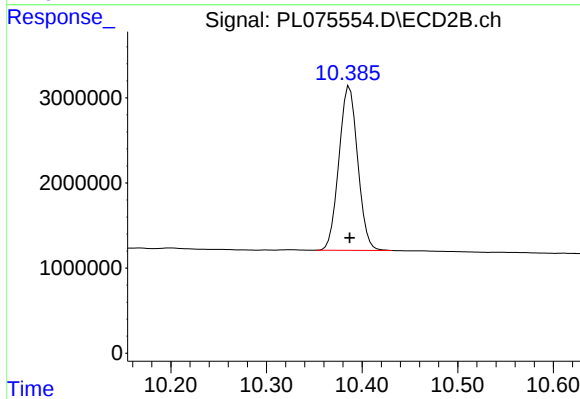

#28 Decachlorobiphenyl

R.T.: 10.387 min
Delta R.T.: 0.000 min
Response: 26376890
Conc: 21.72 ng/ml