

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060422\
 Data File : PL075522.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jun 2022 18:12
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 12:53:02 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060422.M
 Quant Title : GC Extractables
 QLast Update : Sun Jun 05 12:52:55 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.643	4.642	67178170	198.6E6	98.847	98.670
28)	SA Decachlor...	11.640	10.386	51789587	121.1E6	95.760	95.973
Target Compounds							
23)	Chlordane-1	7.037	5.962	23501175	50920826	987.975	981.902
24)	Chlordane-2	7.631	6.648	28151115	58614704	959.481	958.966
25)	Chlordane-3	8.393	7.347	97635983	162.0E6	995.878	992.481
26)	Chlordane-4	8.476	7.414	117.4E6	171.4E6	989.432	990.440
27)	Chlordane-5	9.369	8.126	20973079	42862161	982.461	970.873



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060422\
Data File : PL075522.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jun 2022 18:12
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 12:53:02 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060422.M
Quant Title : GC Extractables
QLast Update : Sun Jun 05 12:52:55 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

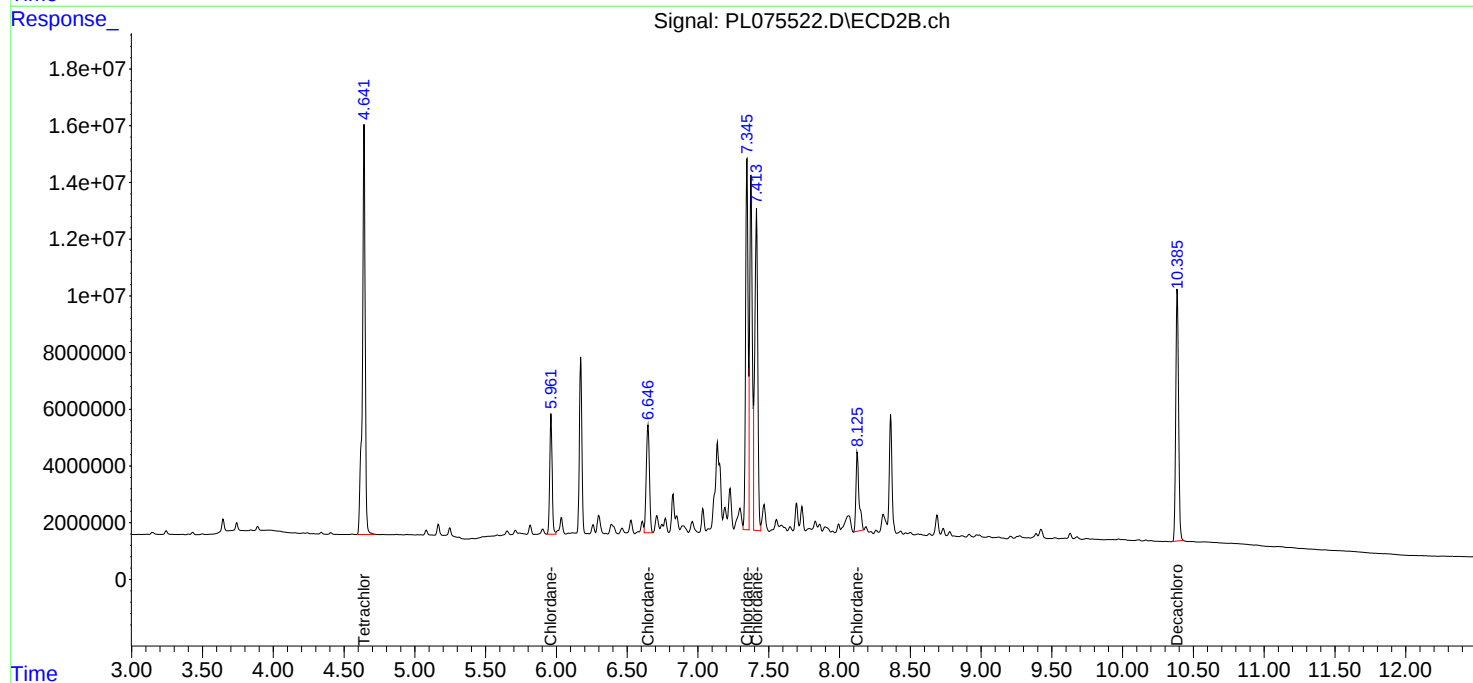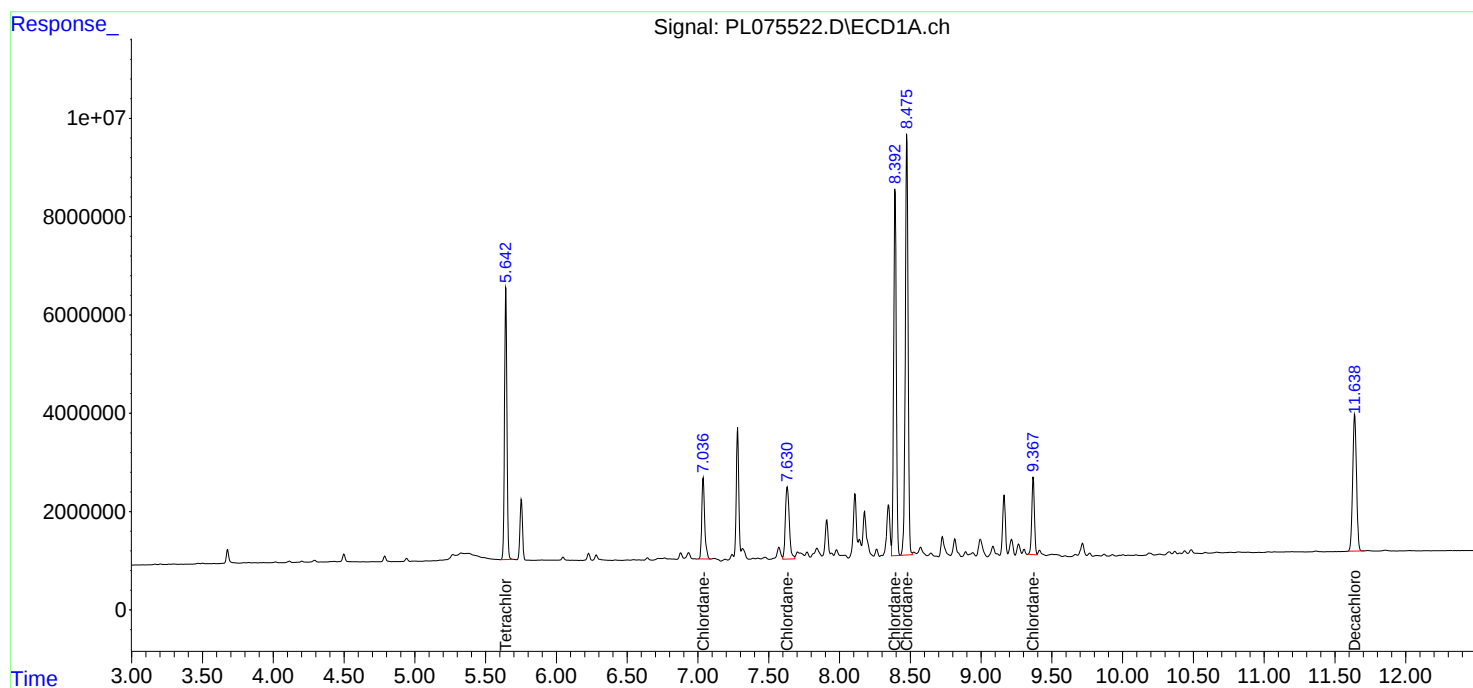


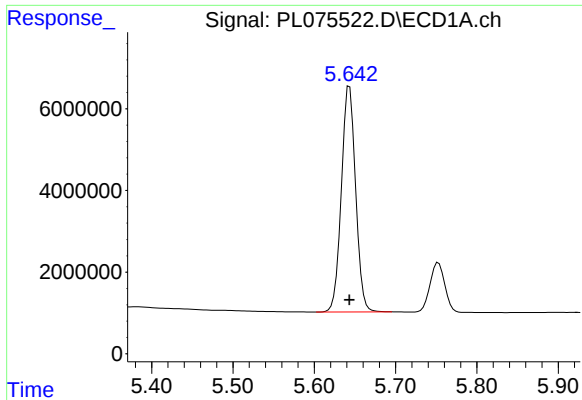

#1 Tetrachloro-m-xylene


R.T.: 5.643 min
Delta R.T.: 0.000 min
Response: 67178170
Conc: 98.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

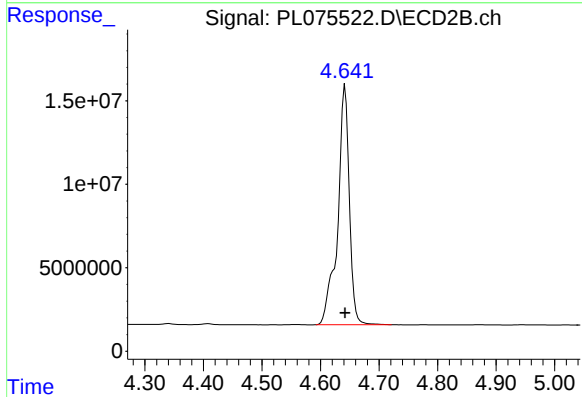


#1 Tetrachloro-m-xylene

R.T.: 4.642 min
Delta R.T.: 0.000 min
Response: 198552380
Conc: 98.67 ng/ml

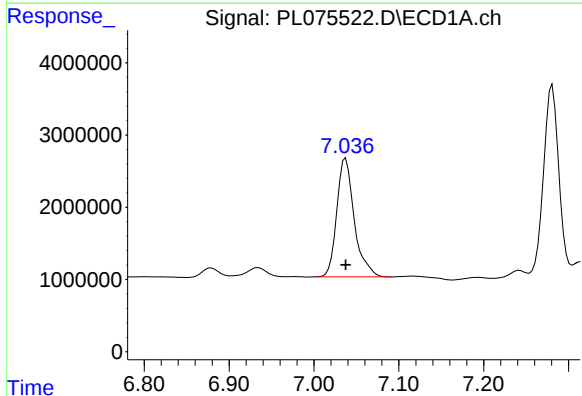


#23 Chlordane-1

R.T.: 7.037 min
Delta R.T.: 0.000 min
Response: 23501175
Conc: 987.97 ng/ml

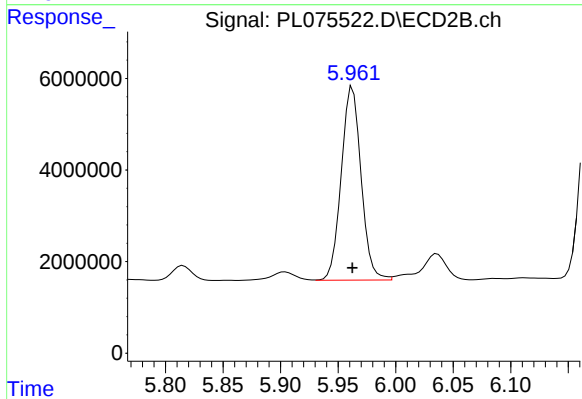

#23 Chlordane-1


R.T.: 5.962 min
Delta R.T.: 0.000 min
Response: 50920826
Conc: 981.90 ng/ml

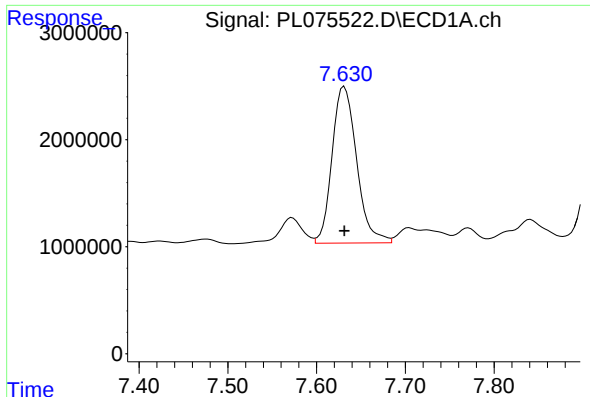

#24 Chlordane-2


R.T.: 7.631 min
Delta R.T.: 0.000 min
Response: 28151115
Conc: 959.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

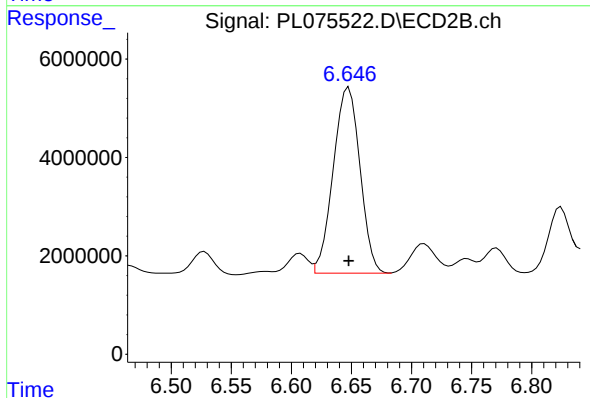


#24 Chlordane-2

R.T.: 6.648 min
Delta R.T.: 0.000 min
Response: 58614704
Conc: 958.97 ng/ml

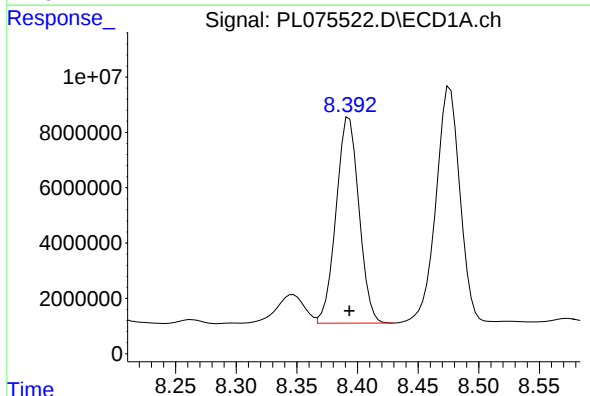


#25 Chlordane-3

R.T.: 8.393 min
Delta R.T.: 0.000 min
Response: 97635983
Conc: 995.88 ng/ml

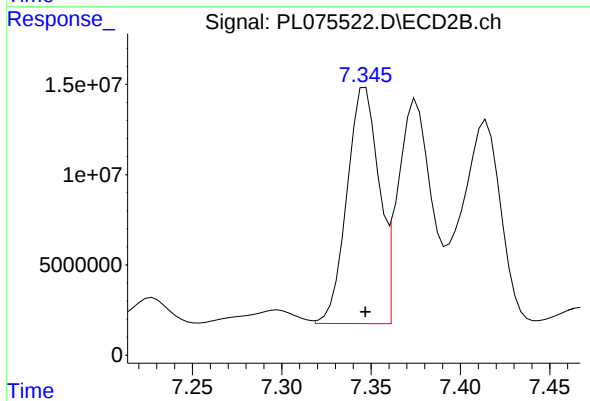

#25 Chlordane-3


R.T.: 7.347 min
Delta R.T.: 0.000 min
Response: 161958330
Conc: 992.48 ng/ml

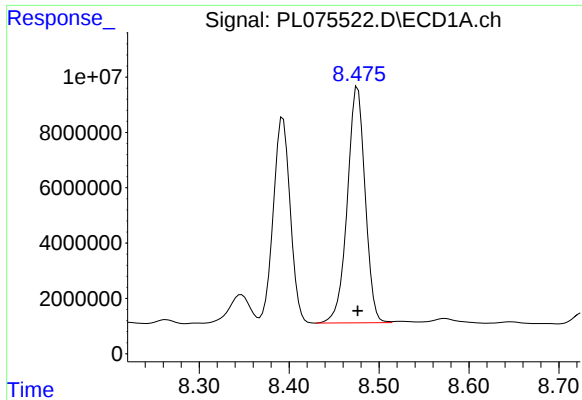

#26 Chlordane-4


R.T.: 8.476 min
Delta R.T.: 0.000 min
Response: 117389058
Conc: 989.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

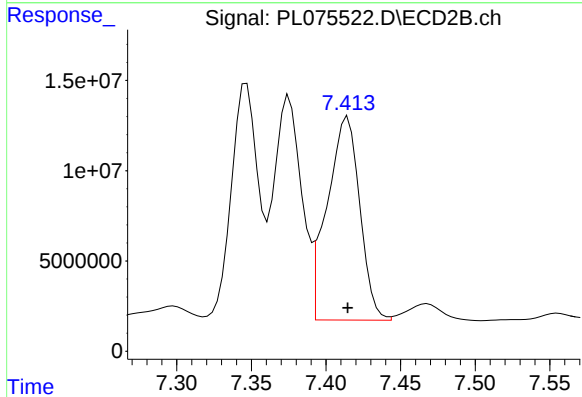


#26 Chlordane-4

R.T.: 7.414 min
Delta R.T.: 0.000 min
Response: 171445757
Conc: 990.44 ng/ml

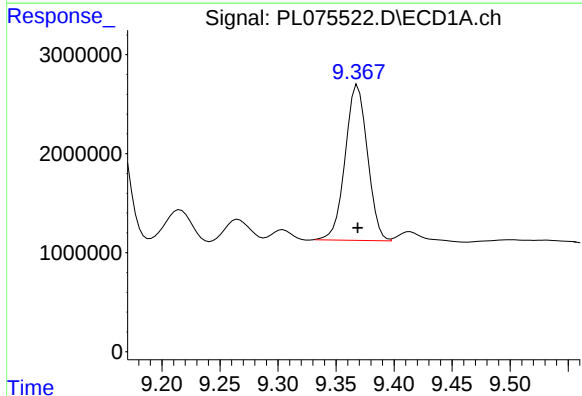


#27 Chlordane-5

R.T.: 9.369 min
Delta R.T.: 0.000 min
Response: 20973079
Conc: 982.46 ng/ml

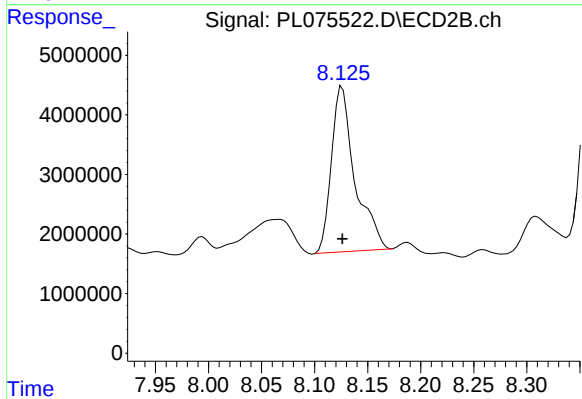

#27 Chlordane-5


R.T.: 8.126 min
Delta R.T.: 0.000 min
Response: 42862161
Conc: 970.87 ng/ml

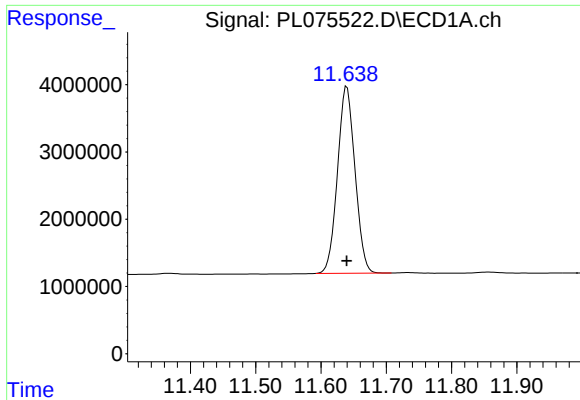

#28 Decachlorobiphenyl

R.T.: 11.640 min
Delta R.T.: 0.000 min
Response: 51789587
Conc: 95.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

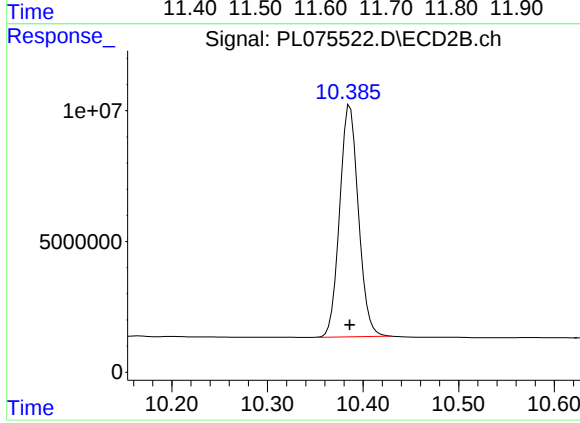

#28 Decachlorobiphenyl

R.T.: 10.386 min
Delta R.T.: 0.000 min
Response: 121098951
Conc: 95.97 ng/ml