

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060422\
 Data File : PL075523.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jun 2022 18:28
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 12:54:51 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060422.M
 Quant Title : GC Extractables
 QLast Update : Sun Jun 05 12:54:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.643	4.642	49598905	147.0E6	73.641	73.693
28)	SA Decachlor...	11.642	10.387	39209353	91362038	73.314	73.250
Target Compounds							
23)	Chlordane-1	7.037	5.963	17405156	37637851	737.701	733.669
24)	Chlordane-2	7.631	6.648	21559457	44220544	739.808	732.102
25)	Chlordane-3	8.394	7.347	71636379	119.0E6	737.011	736.118
26)	Chlordane-4	8.477	7.415	86605928	126.3E6	736.528	736.316
27)	Chlordane-5	9.369	8.126	15493953	31895068	733.689	731.410



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060422\
Data File : PL075523.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jun 2022 18:28
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 12:54:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060422.M
Quant Title : GC Extractables
QLast Update : Sun Jun 05 12:54:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

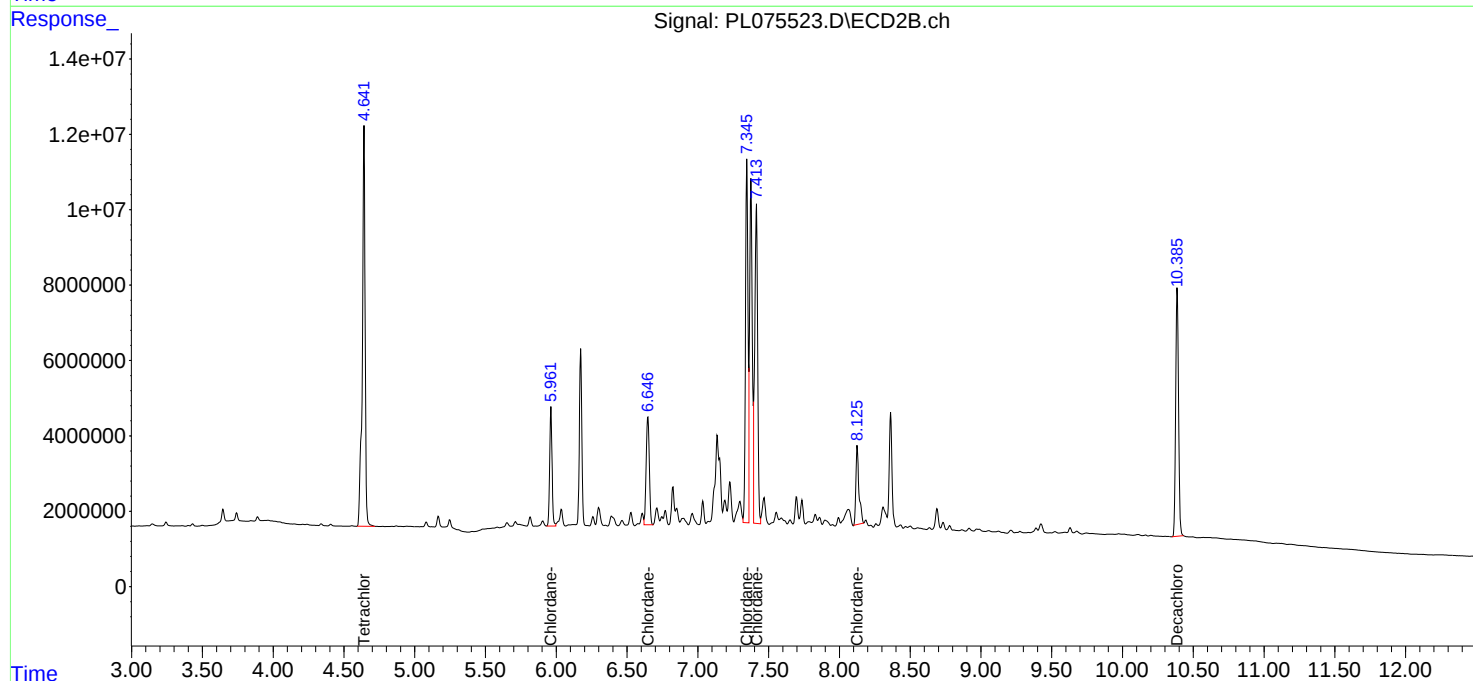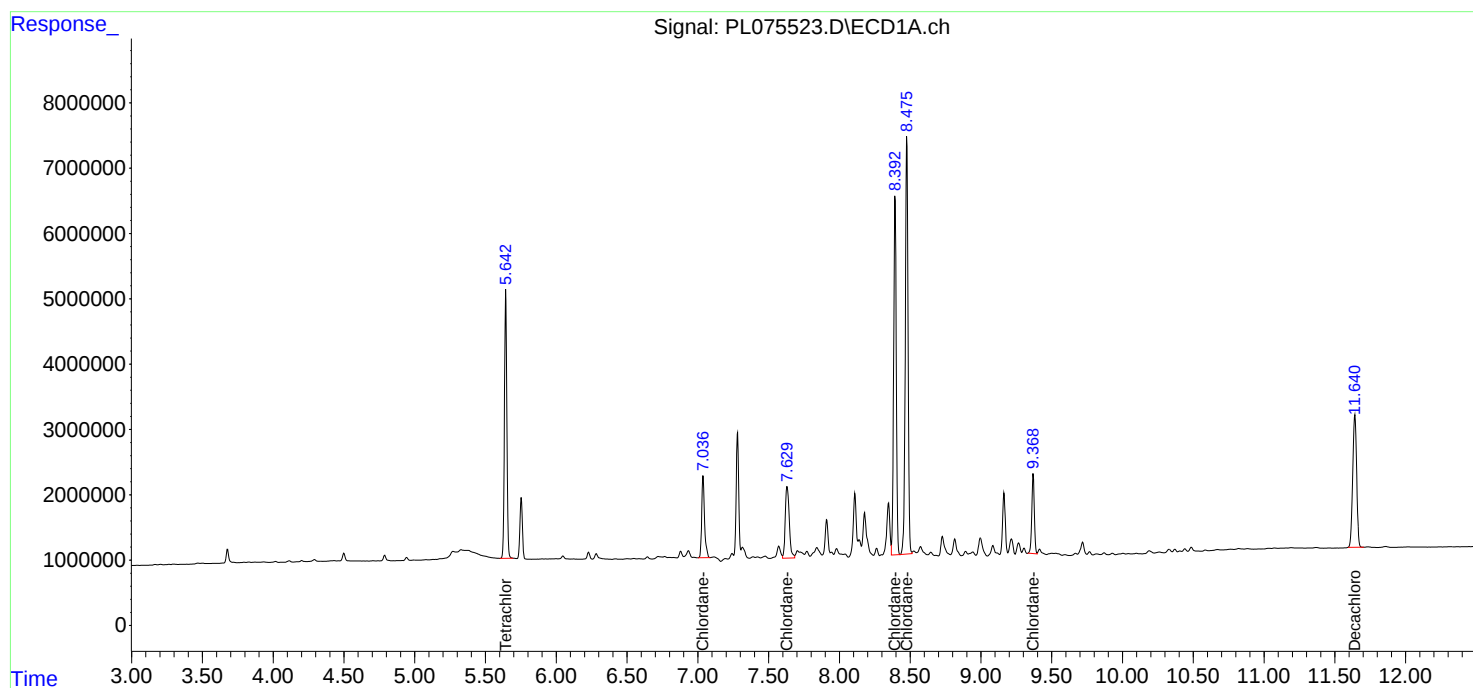


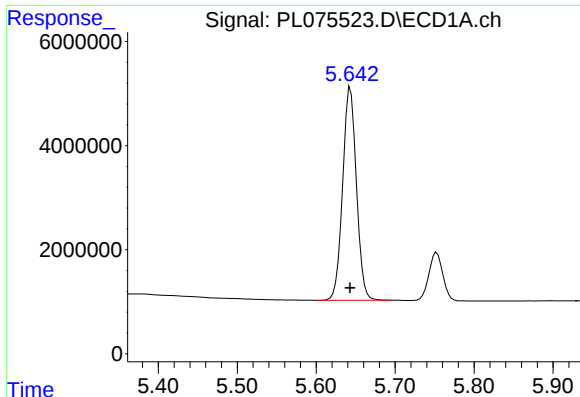

#1 Tetrachloro-m-xylene


R.T.: 5.643 min
Delta R.T.: 0.000 min
Response: 49598905
Conc: 73.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

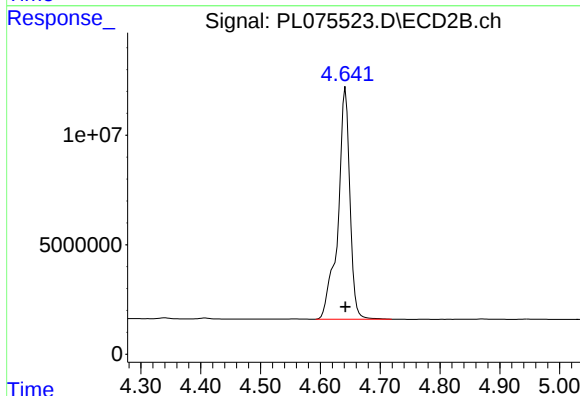


#1 Tetrachloro-m-xylene

R.T.: 4.642 min
Delta R.T.: 0.000 min
Response: 147009893
Conc: 73.69 ng/ml

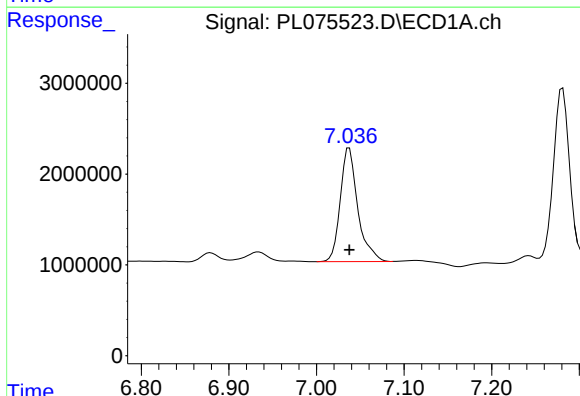


#23 Chlordane-1

R.T.: 7.037 min
Delta R.T.: 0.000 min
Response: 17405156
Conc: 737.70 ng/ml

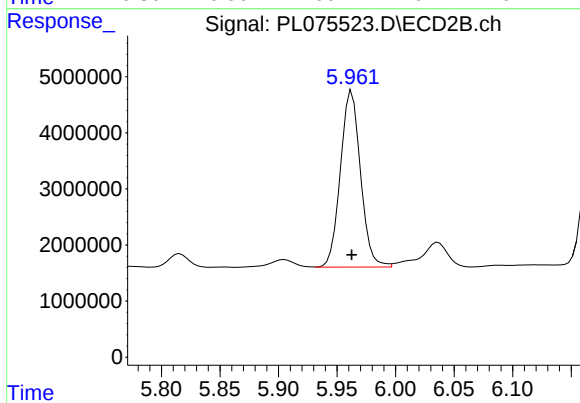

#23 Chlordane-1


R.T.: 5.963 min
Delta R.T.: 0.000 min
Response: 37637851
Conc: 733.67 ng/ml

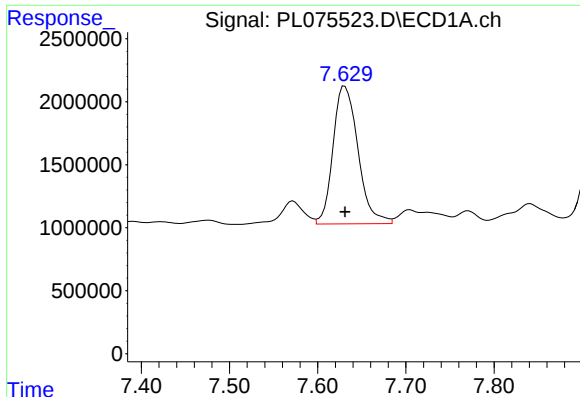

#24 Chlordane-2


R.T.: 7.631 min
Delta R.T.: 0.000 min
Response: 21559457
Conc: 739.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

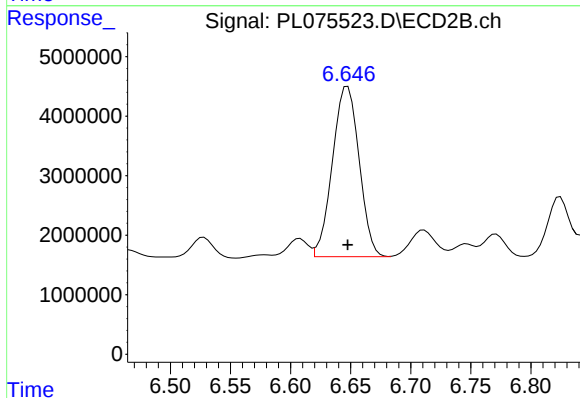


#24 Chlordane-2

R.T.: 6.648 min
Delta R.T.: 0.000 min
Response: 44220544
Conc: 732.10 ng/ml

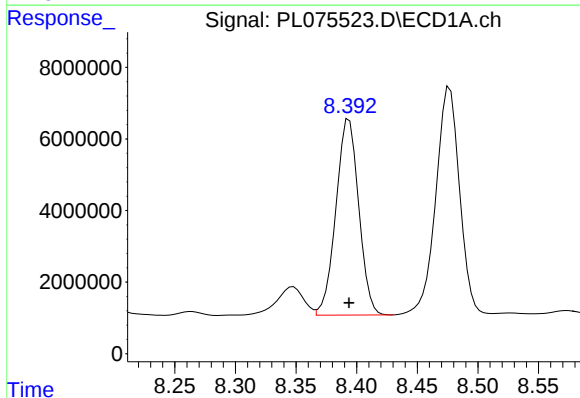


#25 Chlordane-3

R.T.: 8.394 min
Delta R.T.: 0.000 min
Response: 71636379
Conc: 737.01 ng/ml

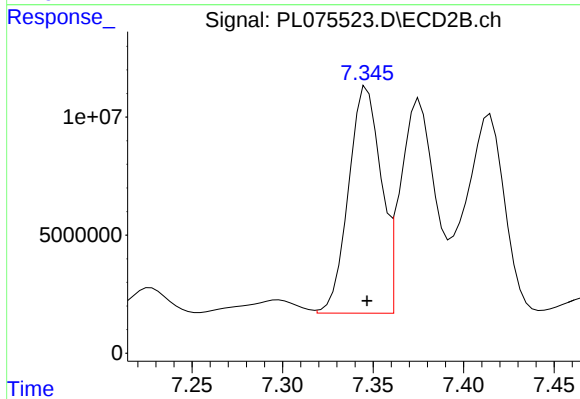

#25 Chlordane-3


R.T.: 7.347 min
Delta R.T.: 0.000 min
Response: 119021986
Conc: 736.12 ng/ml

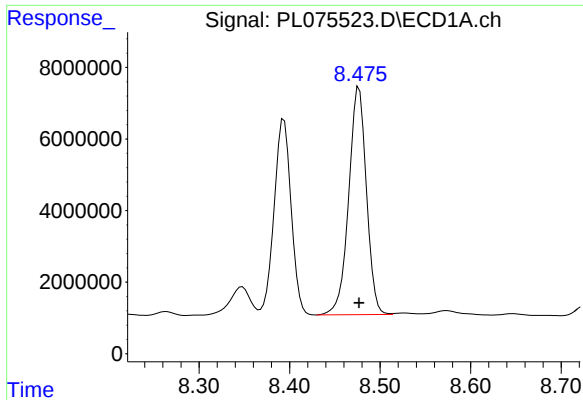

#26 Chlordane-4


R.T.: 8.477 min
Delta R.T.: 0.000 min
Response: 86605928
Conc: 736.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

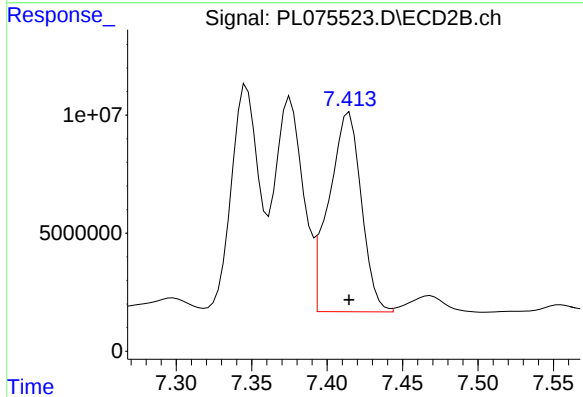


#26 Chlordane-4

R.T.: 7.415 min
Delta R.T.: 0.000 min
Response: 126304548
Conc: 736.32 ng/ml

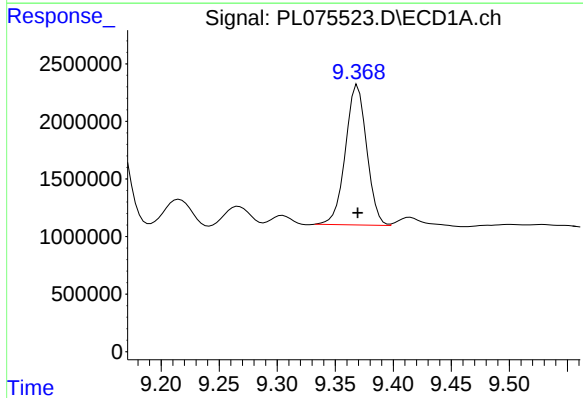


#27 Chlordane-5

R.T.: 9.369 min
Delta R.T.: 0.000 min
Response: 15493953
Conc: 733.69 ng/ml

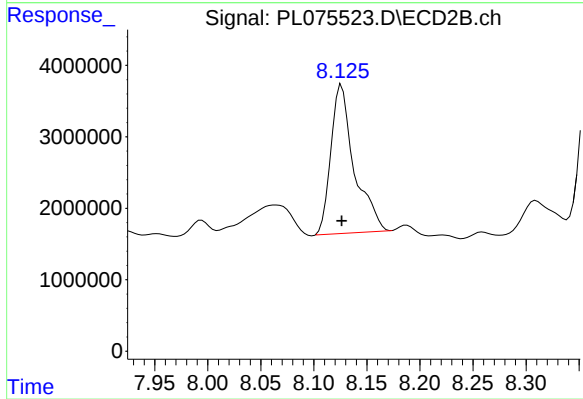

#27 Chlordane-5


R.T.: 8.126 min
Delta R.T.: 0.000 min
Response: 31895068
Conc: 731.41 ng/ml

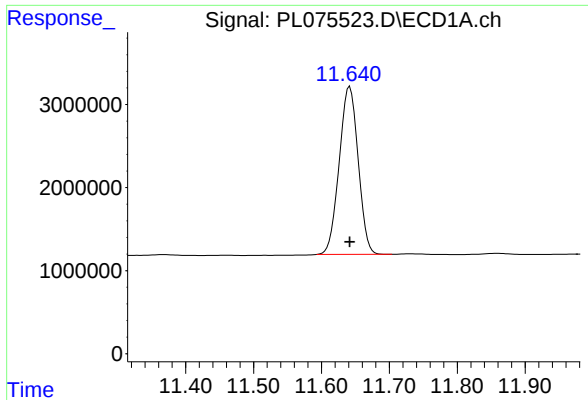

#28 Decachlorobiphenyl

R.T.: 11.642 min
Delta R.T.: 0.000 min
Response: 39209353
Conc: 73.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

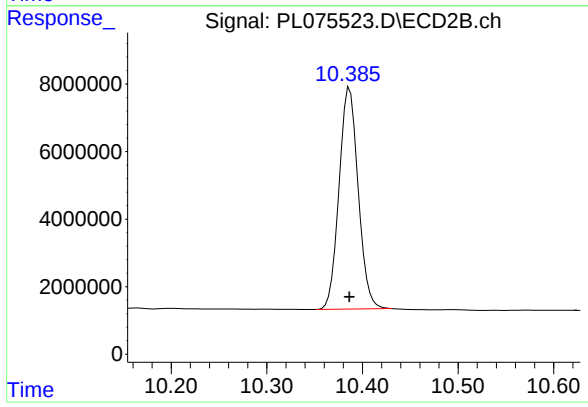

#28 Decachlorobiphenyl

R.T.: 10.387 min
Delta R.T.: 0.000 min
Response: 91362038
Conc: 73.25 ng/ml