

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060422\
 Data File : PL075524.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jun 2022 18:45
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 12:51:14 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060422.M
 Quant Title : GC Extractables
 QLast Update : Sun Jun 05 12:49:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.644	4.642	34372804	102.0E6	50.000	50.000
28)	SA Decachlor...	11.640	10.386	28188025	65630999	50.000	50.000
Target Compounds							
23)	Chlordane-1	7.038	5.963	12036633	26398985	500.000	500.000
24)	Chlordane-2	7.632	6.648	15264396	31815494	500.000	500.000
25)	Chlordane-3	8.393	7.347	49222152	82206084	500.000	500.000
26)	Chlordane-4	8.476	7.414	59948303	87377741	500.000	500.000
27)	Chlordane-5	9.370	8.126	10860953	22716997	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060422\
Data File : PL075524.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jun 2022 18:45
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 12:51:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060422.M
Quant Title : GC Extractables
QLast Update : Sun Jun 05 12:49:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

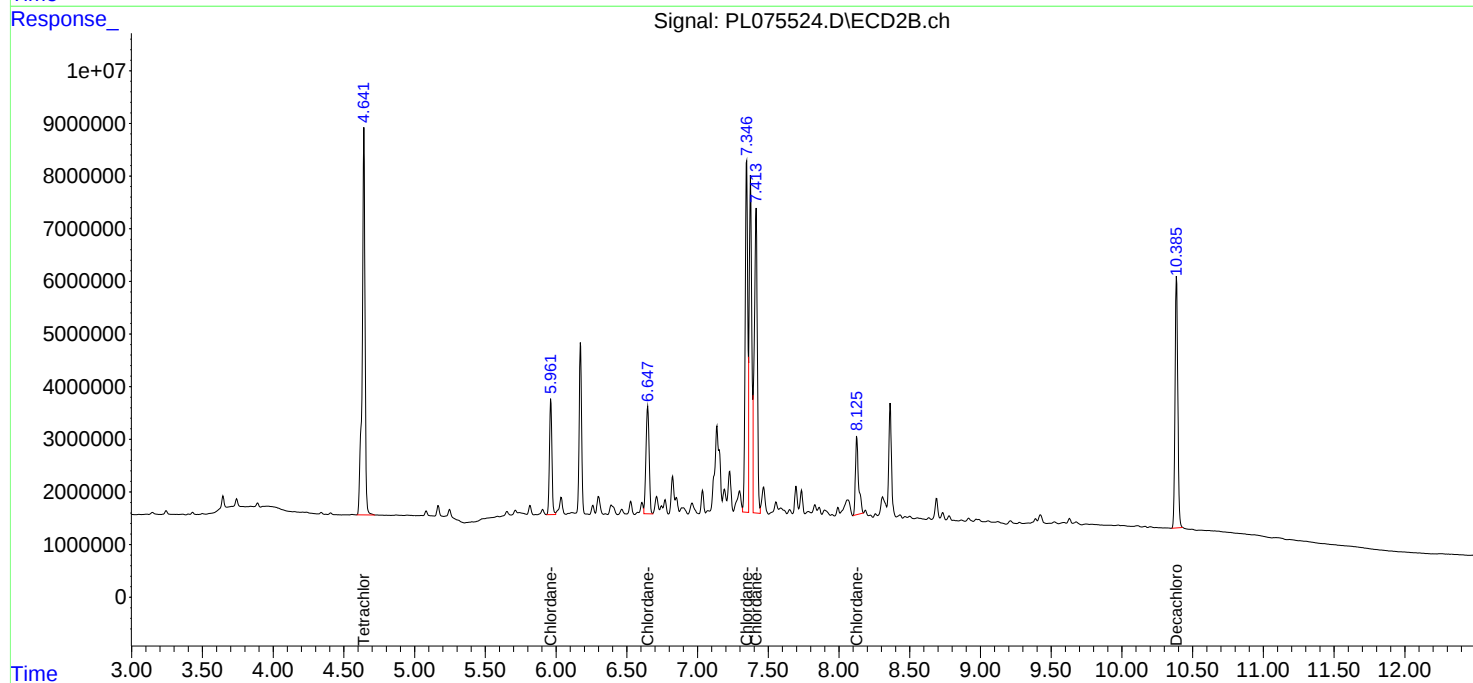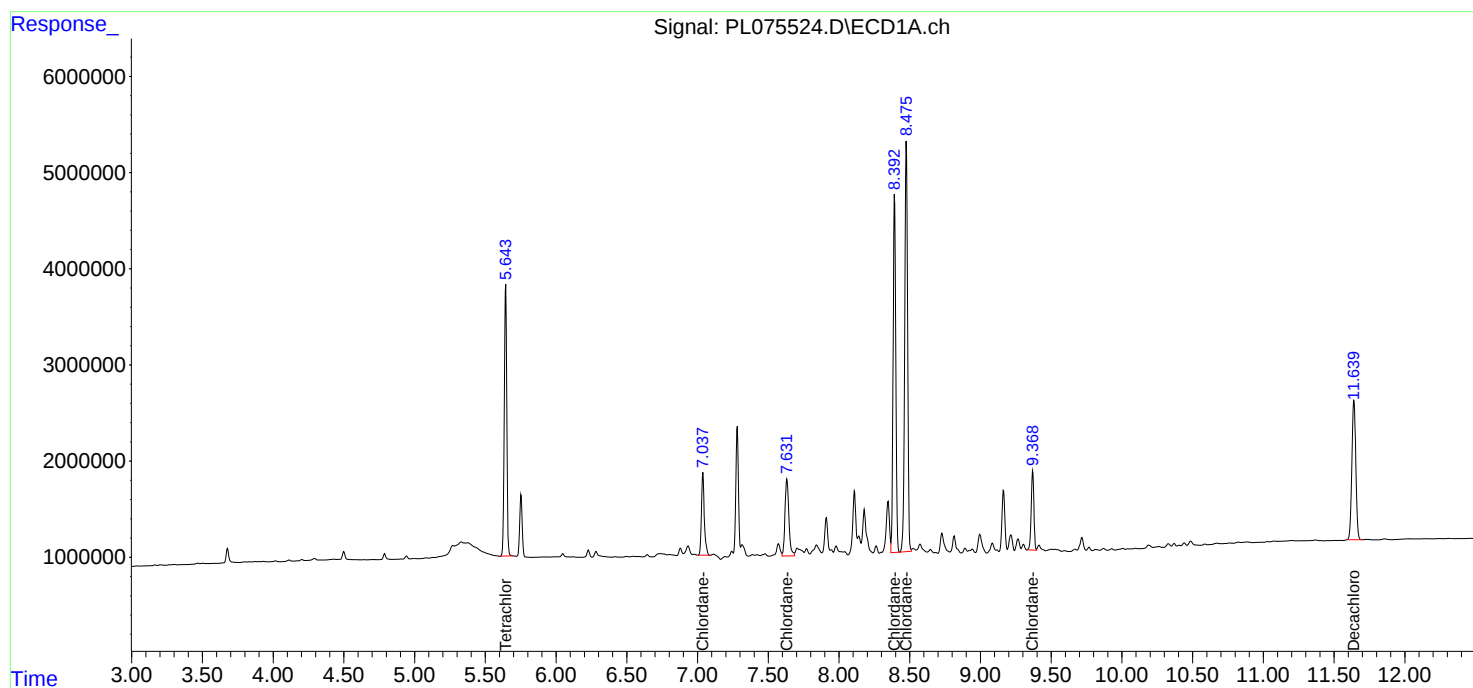


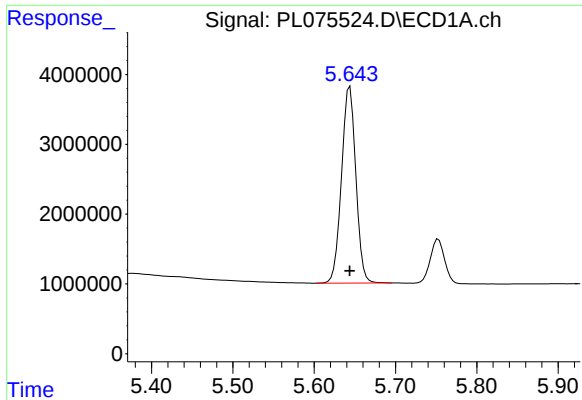

#1 Tetrachloro-m-xylene


R.T.: 5.644 min
Delta R.T.: 0.000 min
Response: 34372804
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

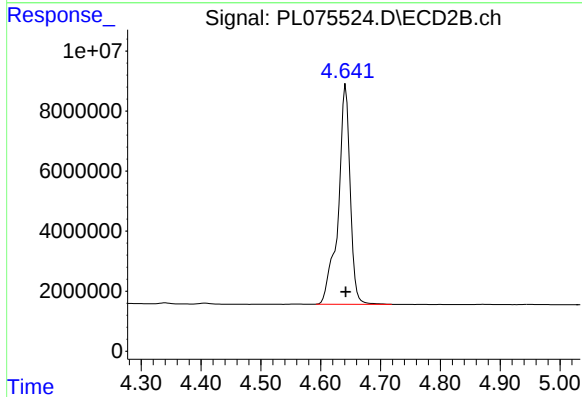


#1 Tetrachloro-m-xylene

R.T.: 4.642 min
Delta R.T.: 0.000 min
Response: 101951630
Conc: 50.00 ng/ml

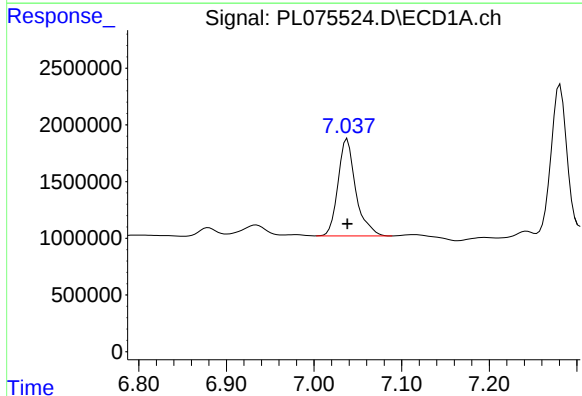


#23 Chlordane-1

R.T.: 7.038 min
Delta R.T.: 0.000 min
Response: 12036633
Conc: 500.00 ng/ml

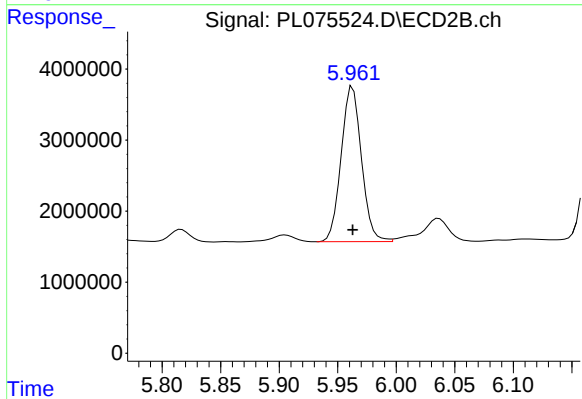

#23 Chlordane-1


R.T.: 5.963 min
Delta R.T.: 0.000 min
Response: 26398985
Conc: 500.00 ng/ml

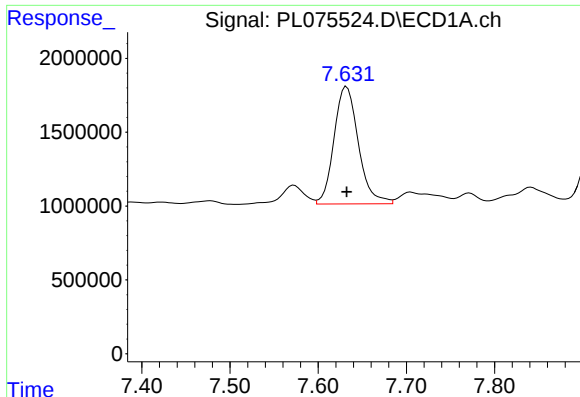

#24 Chlordane-2


R.T.: 7.632 min
Delta R.T.: 0.000 min
Response: 15264396
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

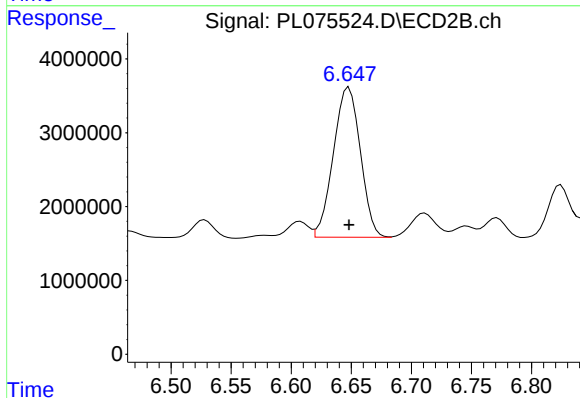


#24 Chlordane-2

R.T.: 6.648 min
Delta R.T.: 0.000 min
Response: 31815494
Conc: 500.00 ng/ml

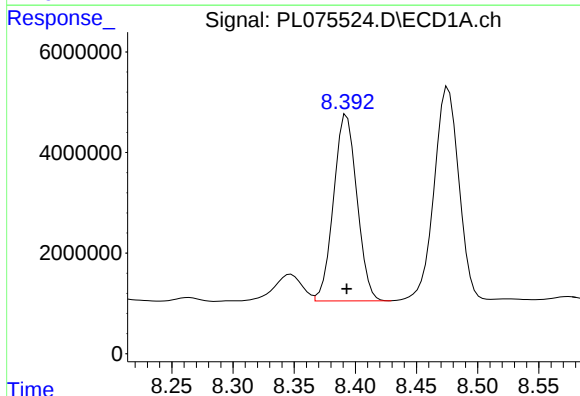


#25 Chlordane-3

R.T.: 8.393 min
Delta R.T.: 0.000 min
Response: 49222152
Conc: 500.00 ng/ml

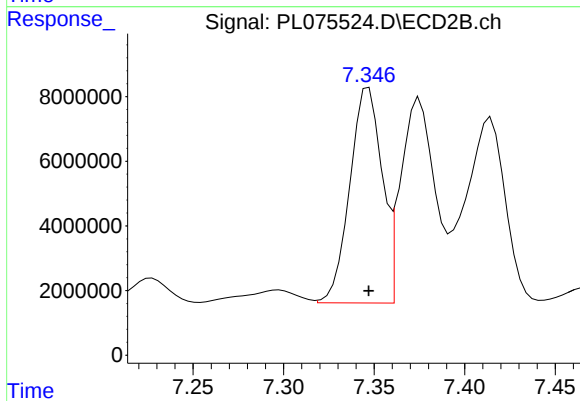

#25 Chlordane-3


R.T.: 7.347 min
Delta R.T.: 0.000 min
Response: 82206084
Conc: 500.00 ng/ml

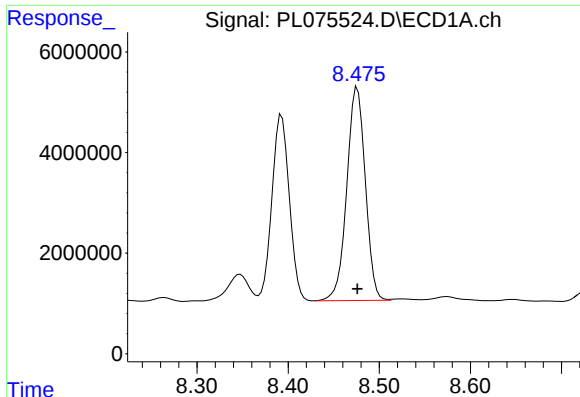

#26 Chlordane-4


R.T.: 8.476 min
Delta R.T.: 0.000 min
Response: 59948303
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

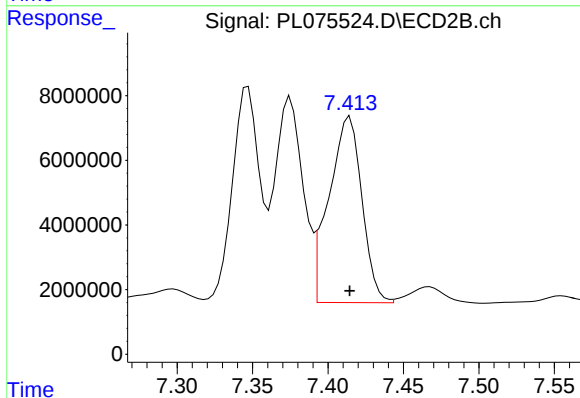


#26 Chlordane-4

R.T.: 7.414 min
Delta R.T.: 0.000 min
Response: 87377741
Conc: 500.00 ng/ml

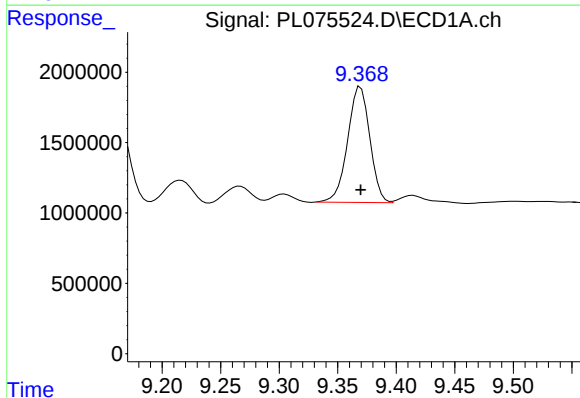


#27 Chlordane-5

R.T.: 9.370 min
Delta R.T.: 0.000 min
Response: 10860953
Conc: 500.00 ng/ml

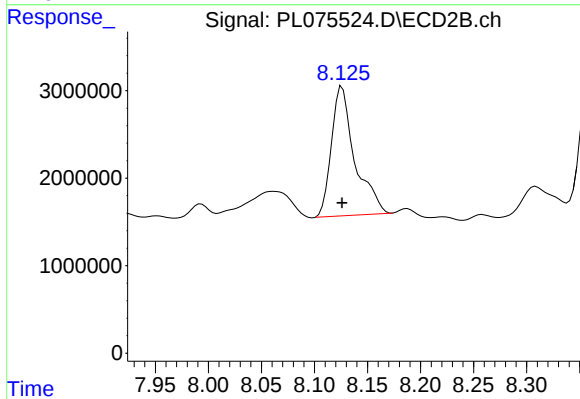

#27 Chlordane-5


R.T.: 8.126 min
Delta R.T.: 0.000 min
Response: 22716997
Conc: 500.00 ng/ml

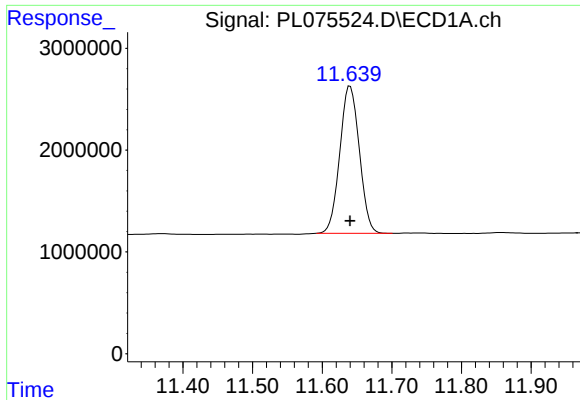

#28 Decachlorobiphenyl

R.T.: 11.640 min
Delta R.T.: 0.000 min
Response: 28188025
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

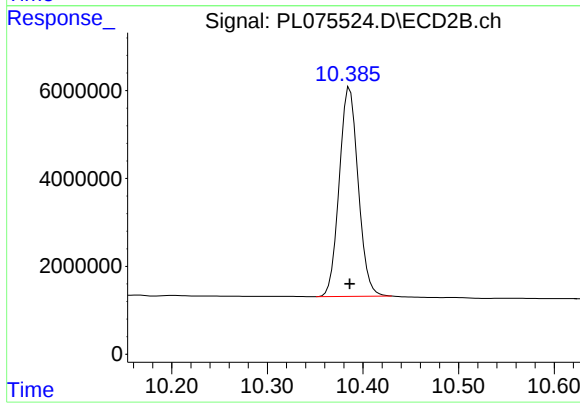

#28 Decachlorobiphenyl

R.T.: 10.386 min
Delta R.T.: 0.000 min
Response: 65630999
Conc: 50.00 ng/ml