

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060422\
 Data File : PL075525.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jun 2022 19:01
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 12:56:30 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060422.M
 Quant Title : GC Extractables
 QLast Update : Sun Jun 05 12:56:21 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.643	4.642	16066763	47958968	24.131	24.274
28)	SA Decachlor...	11.639	10.386	14019058	32952119	25.899	26.050
Target Compounds							
23)	Chlordane-1	7.038	5.962	5562089	12675905	239.153	247.811
24)	Chlordane-2	7.631	6.648	7738634	16028464	261.484	261.348
25)	Chlordane-3	8.393	7.346	22956256	38584873	239.489	241.379
26)	Chlordane-4	8.475	7.414	28198087	40949504	242.276	241.446
27)	Chlordane-5	9.369	8.126	5034325	11217069	241.192	255.381



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060422\
Data File : PL075525.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jun 2022 19:01
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 12:56:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060422.M
Quant Title : GC Extractables
QLast Update : Sun Jun 05 12:56:21 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

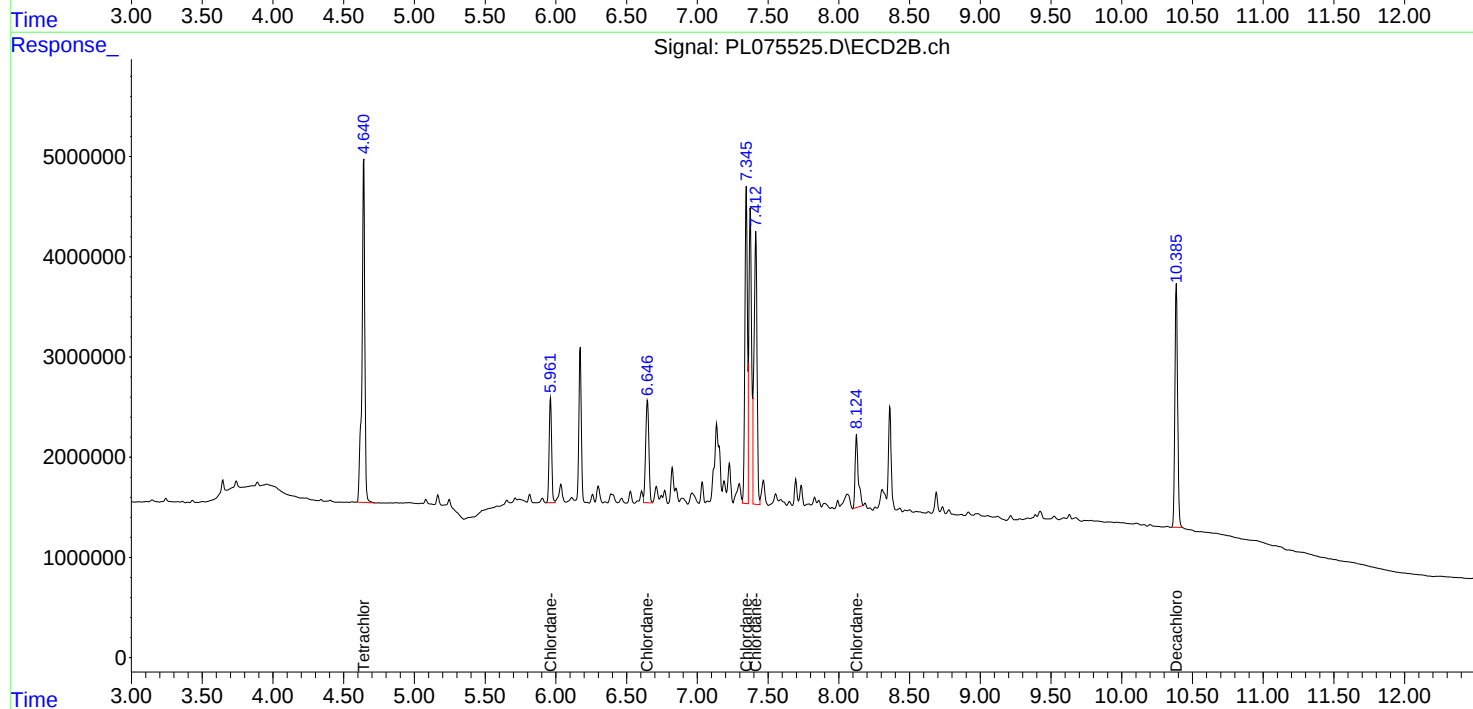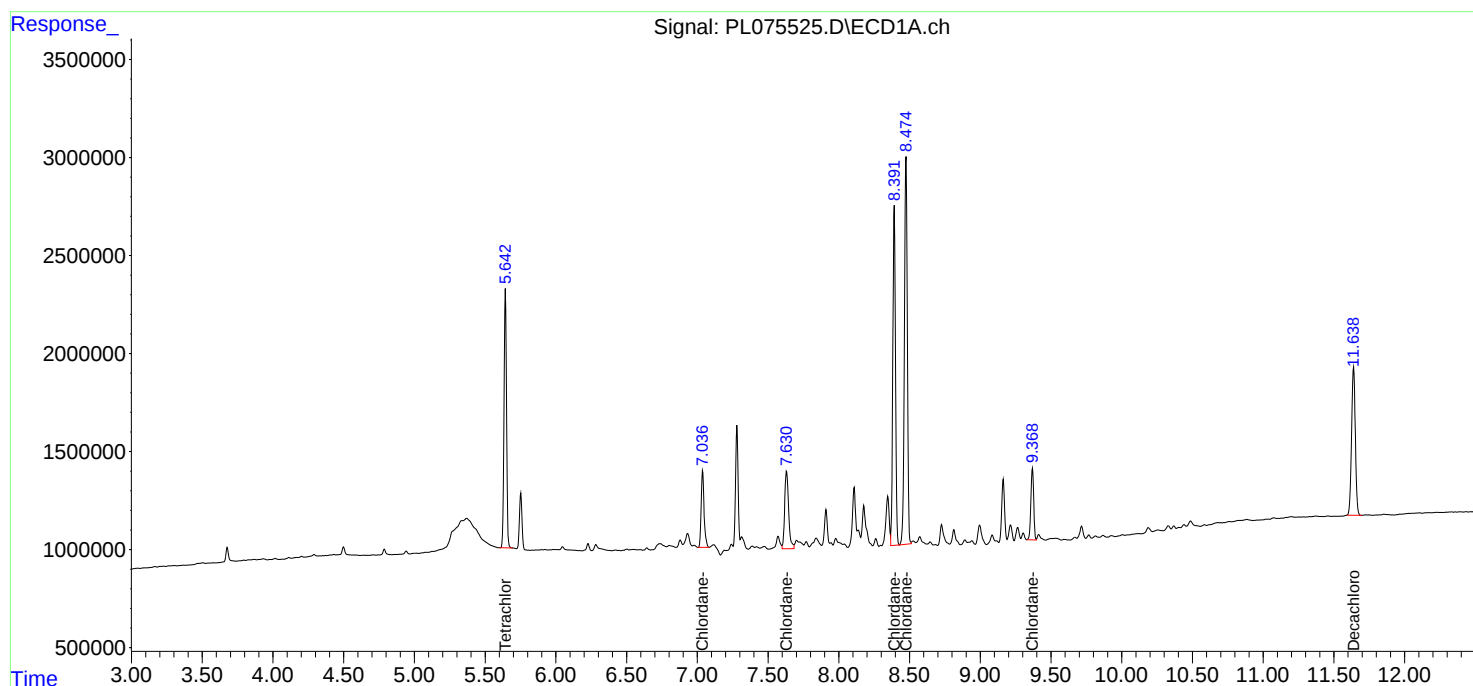


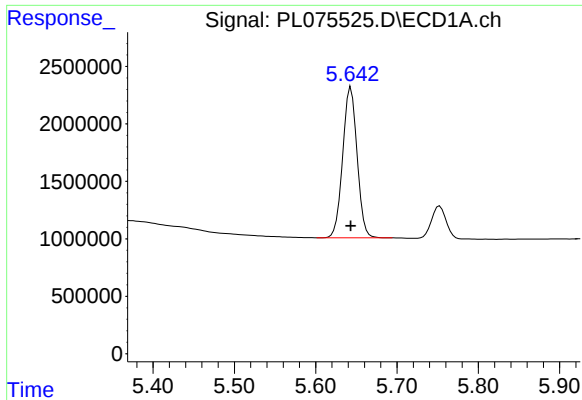

#1 Tetrachloro-m-xylene


R.T.: 5.643 min
Delta R.T.: 0.000 min
Response: 16066763
Conc: 24.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

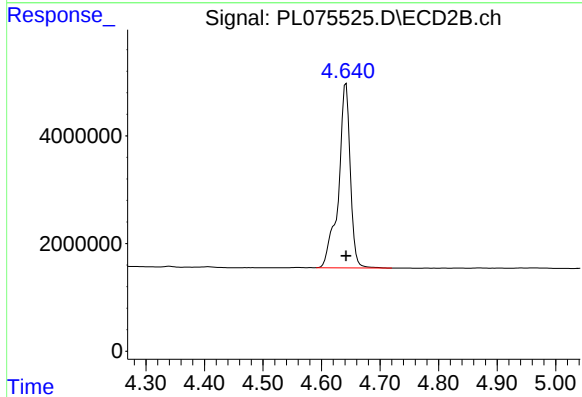


#1 Tetrachloro-m-xylene

R.T.: 4.642 min
Delta R.T.: 0.000 min
Response: 47958968
Conc: 24.27 ng/ml

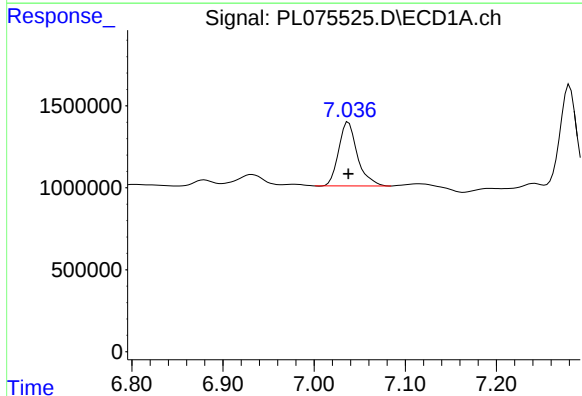


#23 Chlordane-1

R.T.: 7.038 min
Delta R.T.: 0.000 min
Response: 5562089
Conc: 239.15 ng/ml

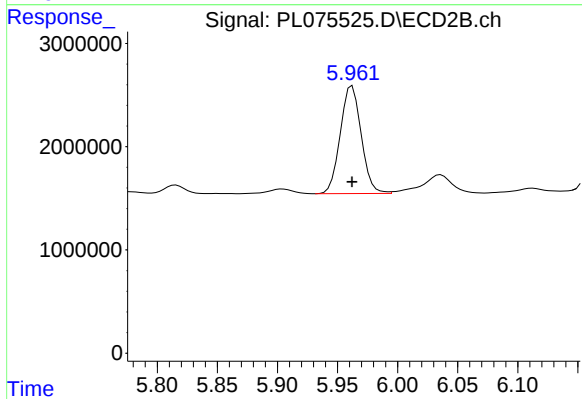

#23 Chlordane-1


R.T.: 5.962 min
Delta R.T.: 0.000 min
Response: 12675905
Conc: 247.81 ng/ml

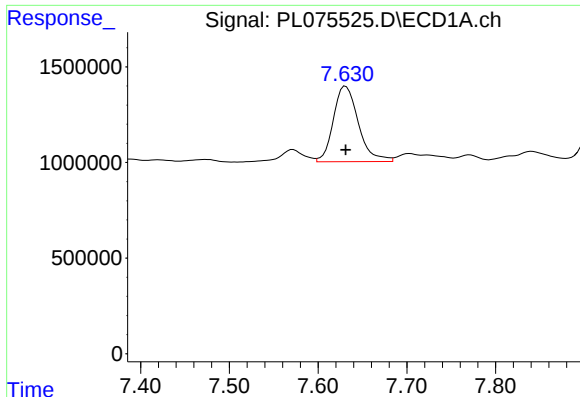

#24 Chlordane-2


R.T.: 7.631 min
Delta R.T.: 0.000 min
Response: 7738634
Conc: 261.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

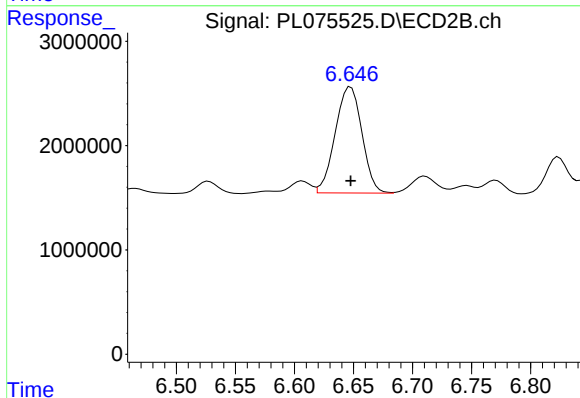


#24 Chlordane-2

R.T.: 6.648 min
Delta R.T.: 0.000 min
Response: 16028464
Conc: 261.35 ng/ml

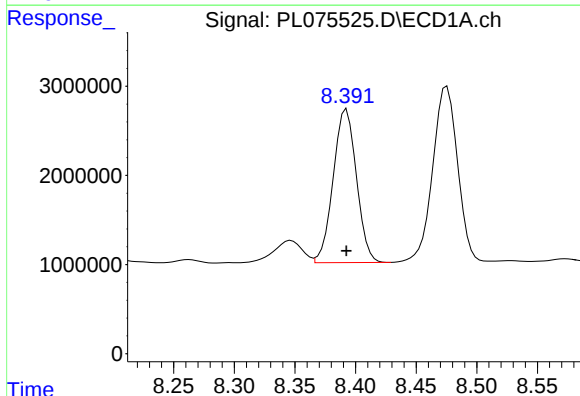


#25 Chlordane-3

R.T.: 8.393 min
Delta R.T.: 0.000 min
Response: 22956256
Conc: 239.49 ng/ml

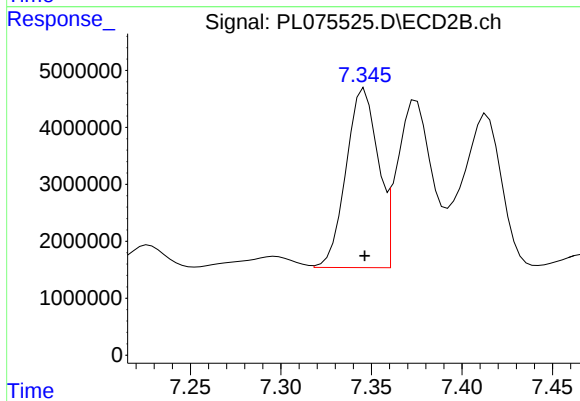

#25 Chlordane-3


R.T.: 7.346 min
Delta R.T.: 0.000 min
Response: 38584873
Conc: 241.38 ng/ml

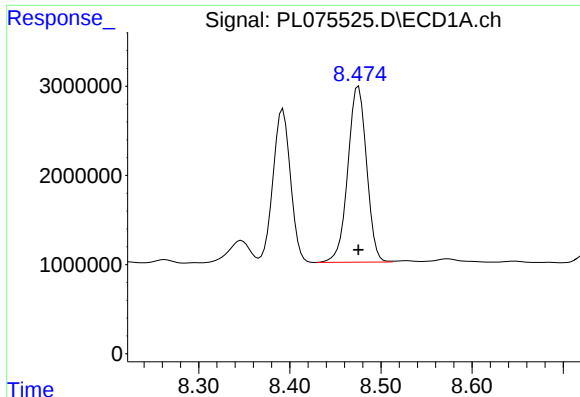

#26 Chlordane-4


R.T.: 8.475 min
Delta R.T.: 0.000 min
Response: 28198087
Conc: 242.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

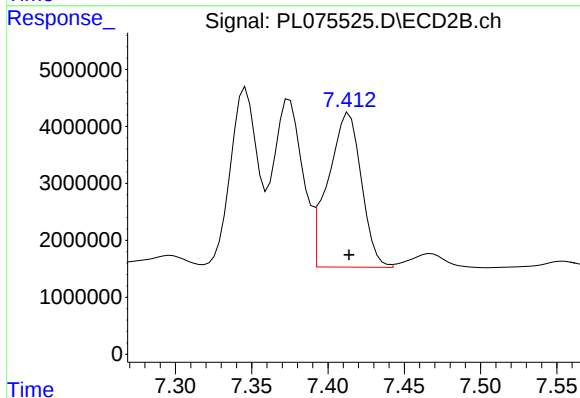


#26 Chlordane-4

R.T.: 7.414 min
Delta R.T.: 0.000 min
Response: 40949504
Conc: 241.45 ng/ml

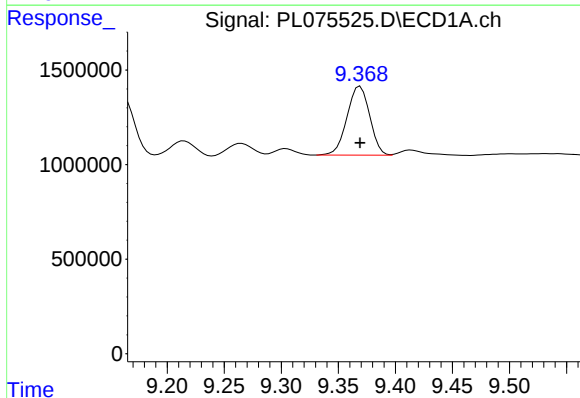


#27 Chlordane-5

R.T.: 9.369 min
Delta R.T.: 0.000 min
Response: 5034325
Conc: 241.19 ng/ml

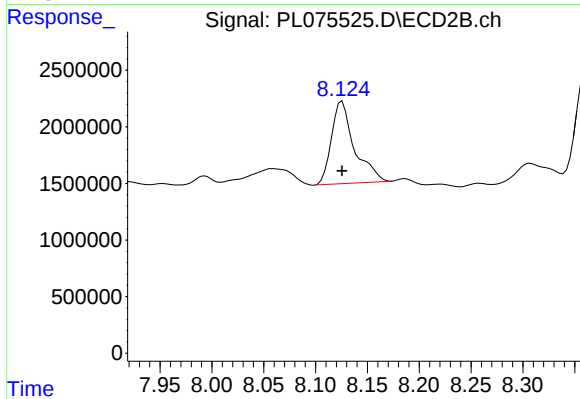

#27 Chlordane-5


R.T.: 8.126 min
Delta R.T.: 0.000 min
Response: 11217069
Conc: 255.38 ng/ml

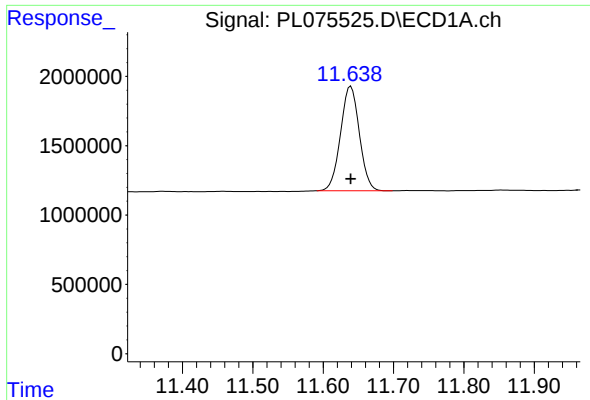

#28 Decachlorobiphenyl

R.T.: 11.639 min
Delta R.T.: 0.000 min
Response: 14019058
Conc: 25.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

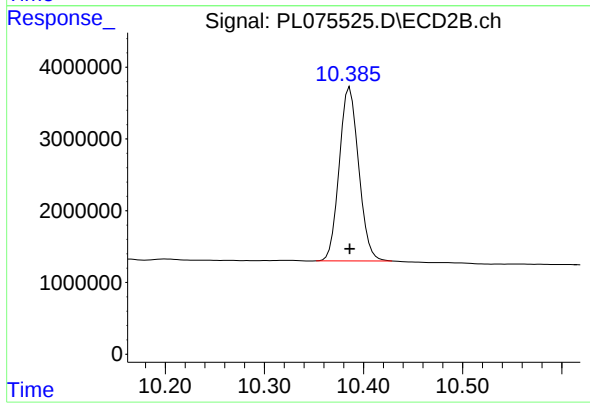

#28 Decachlorobiphenyl

R.T.: 10.386 min
Delta R.T.: 0.000 min
Response: 32952119
Conc: 26.05 ng/ml