

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060424\
 Data File : PL089963.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jun 2024 20:38
 Operator : AR\AJ
 Sample : P2591-09
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BH5T2

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/05/2024
 Supervised By : Ankita Jodhani 06/05/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 05:27:21 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060424CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 04 15:06:25 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.546	2.791	15280323	10847978	7.922m	7.990
2) SA Decachlor...	9.040	7.935	38081680	21288460	28.864m	15.354 #
Target Compounds						
9) A Endosulfan I	6.107	5.148	45541632	119.3E6	22.284m	79.412m#
13) MA Dieldrin	6.368	5.381	70446372	53097762	33.467	32.049m
16) A 4,4'-DDD	6.696	5.808	27481847	19007247	18.053m	15.071
17) MA 4,4'-DDT	7.025	6.057	5382758	8395341	3.476m	6.221m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060424\
Data File : PL089963.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jun 2024 20:38
Operator : AR\AJ
Sample : P2591-09
Misc :
ALS Vial : 34 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 05:27:21 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060424CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jun 04 15:06:25 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

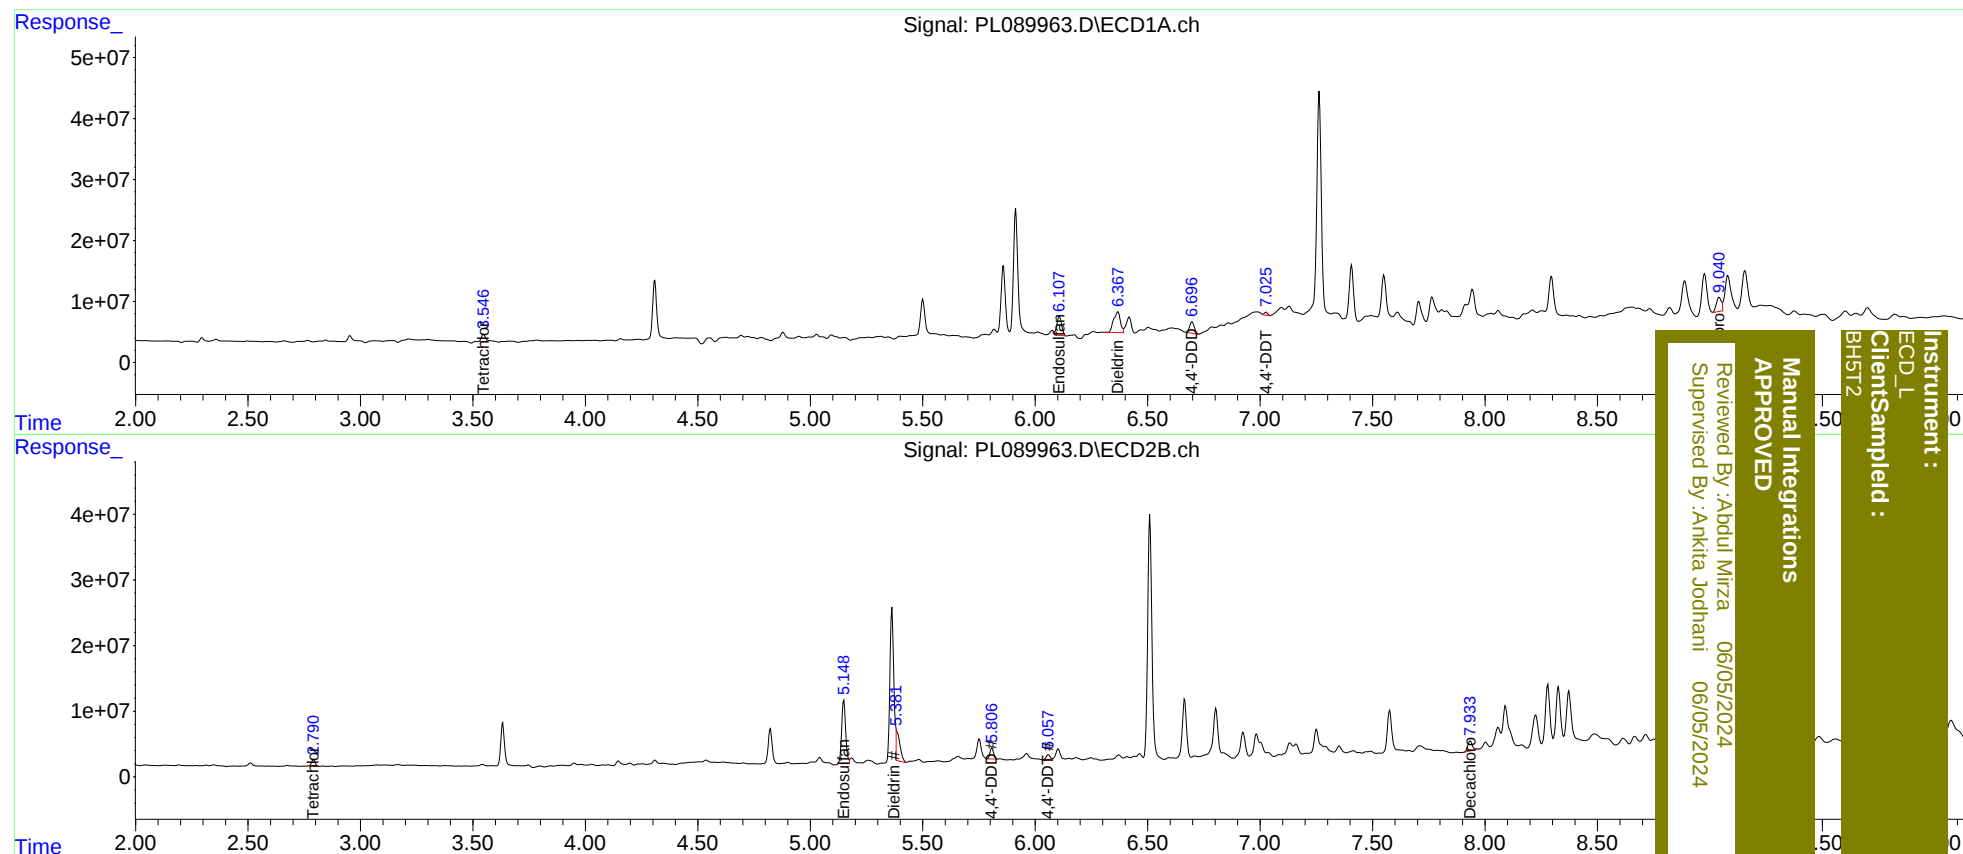

Reviewed By: Abdul Mirza 06/05/2024
Supervised By: Ankita Jodhani 06/05/2024

Manual Integrations
APPROVED

Instrument :
ECD_L
ClientSampled :
BHST2