

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060424\
 Data File : PL089930.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jun 2024 10:06
 Operator : AR\AJ
 Sample : RESC030
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RESC220

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 15:09:04 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060424CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 04 15:06:25 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.549	2.794	39606200	27420702	20.535	20.198
2)	SA Decachlor...	9.064	7.942	53368043	55062115	40.450	39.713
Target Compounds							
2)	A alpha-BHC	4.004	3.298	29331662	17769513	10.469	9.423
3)	MA gamma-BHC...	4.338	3.629	27746943	17235223	10.570	9.566
4)	MA Heptachlor	4.927	3.971	26056747	17751113	10.514	9.856
5)	MB Aldrin	5.268	4.252	26982913	17174918	11.067	10.013
6)	B beta-BHC	4.533	3.927	13925116	9257212	10.768	10.141
7)	B delta-BHC	4.780	4.158	27699684	17406133	10.367	9.486
8)	B Heptachlo...	5.694	4.755	25228670	16787592	10.741	9.982
9)	A Endosulfan I	6.080	5.125	22373311	15092726	10.948	10.050
10)	B trans-Chl...	5.950	5.005	23546914	16472209	10.818	9.931
11)	B cis-Chlor...	6.030	5.069	24125732	16940200	10.792	9.849
12)	B 4,4'-DDE	6.201	5.258	40506540	28922807	21.470	18.887
13)	MA Dieldrin	6.355	5.390	44300502	31764042	21.046	19.172
14)	MA Endrin	6.584	5.665	36308921	28613618	20.578	19.258
15)	B Endosulfa...	6.803	5.959	38184519	29110895	21.135	19.904
16)	A 4,4'-DDD	6.718	5.812	31012949	23833036	20.373	18.897
17)	MA 4,4'-DDT	7.032	6.063	32464006	25395438	20.967	18.817
18)	B Endrin al...	6.933	6.138	27844875	21752328	22.041	20.700
19)	B Endosulfa...	7.167	6.361	36204052	28673286	21.636	19.907
20)	A Methoxychlor	7.507	6.639	79101601	76626470	103.158	100.740
21)	B Endrin ke...	7.652	6.867	39480857	32770003	21.874	20.420

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060424\
Data File : PL089930.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jun 2024 10:06
Operator : AR\AJ
Sample : RESC030
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 15:09:04 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060424CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jun 04 15:06:25 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

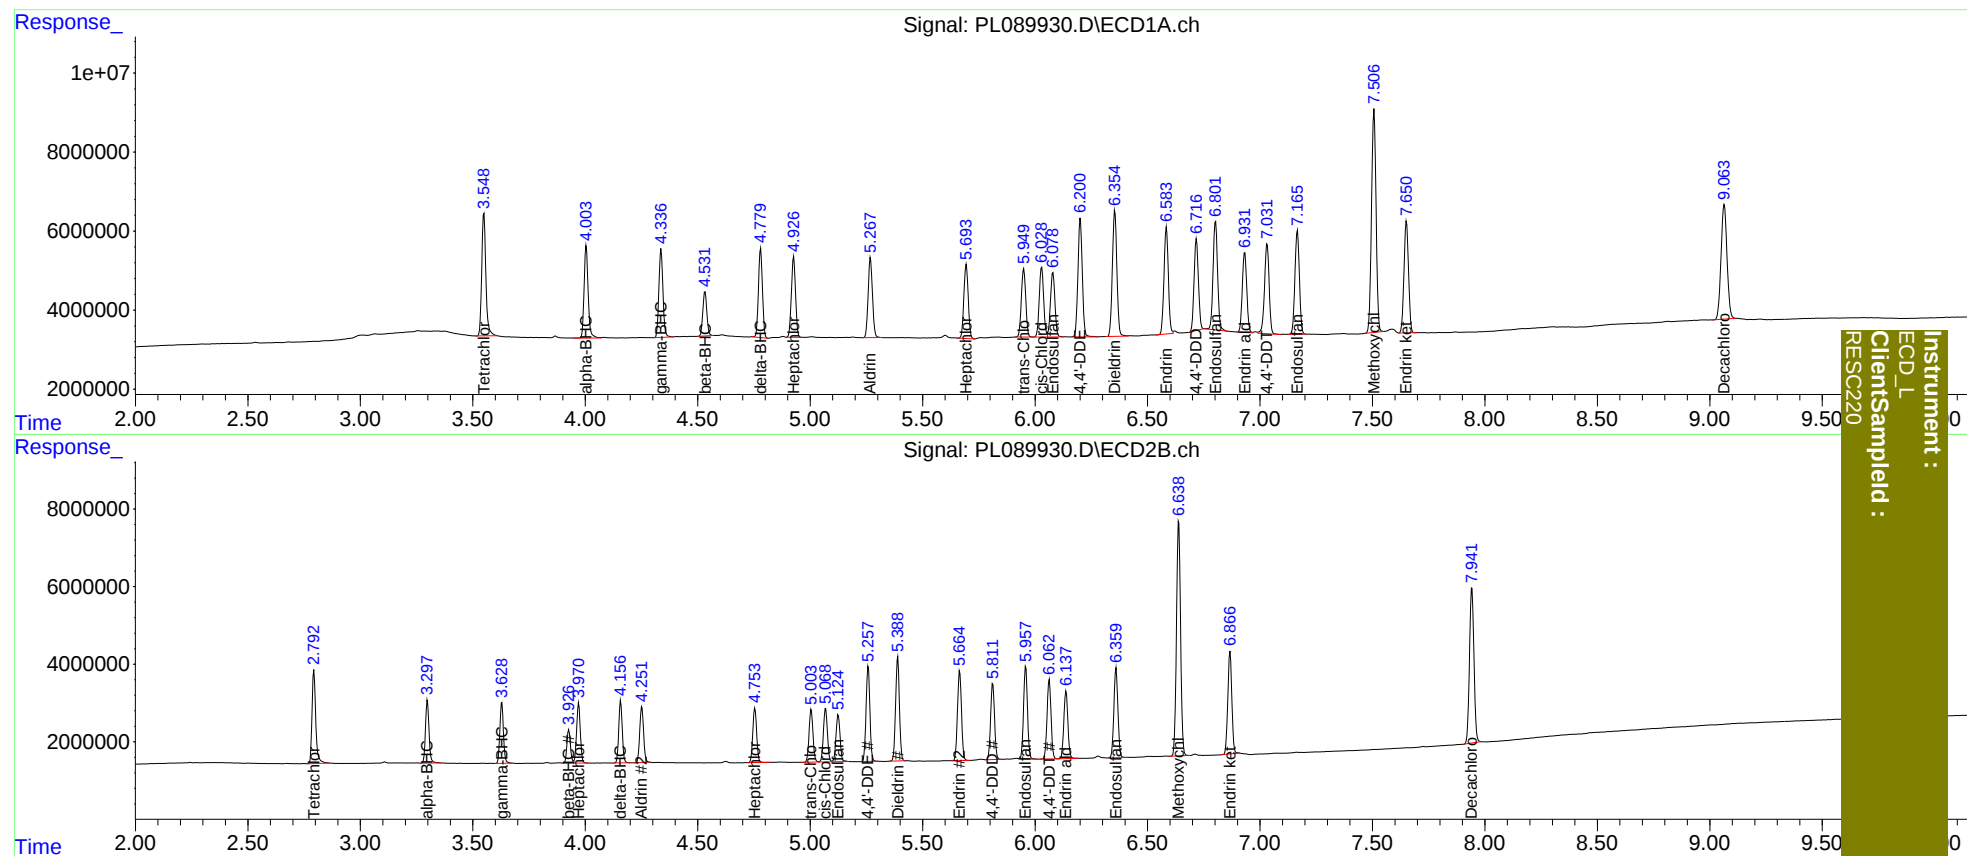

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060424\
Data File : PL089930.D
Acq On : 04 Jun 2024 10:06
Operator : AR\AJ
Sample : RESC030
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
RESC220

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060424CLP.M
Title : GC Extractables
Last Update : Tue Jun 04 15:06:25 2024
Integrator: ChemStation

RT#1	RT#2	Resolution
3.549	4.004	100.00%
4.004	4.338	100.00%
4.338	4.533	100.00%
4.533	4.780	100.00%
4.780	4.927	100.00%
4.927	5.268	100.00%
5.268	5.694	100.00%
5.694	5.950	100.00%
5.950	6.030	100.00%
6.030	6.080	95.08%
6.080	6.201	100.00%
6.201	6.355	100.00%
6.355	6.584	100.00%
6.584	6.718	100.00%
6.718	6.803	100.00%
6.803	6.933	100.00%
6.933	7.032	100.00%
7.032	7.167	100.00%
7.167	7.507	100.00%
7.507	7.652	100.00%
7.652	9.064	100.00%

Signal #2


2.794	3.298	100.00%
3.298	3.629	100.00%
3.629	3.927	100.00%
3.927	3.971	96.84%
3.971	4.158	100.00%
4.158	4.252	100.00%
4.252	4.755	100.00%
4.755	5.005	100.00%
5.005	5.069	100.00%
5.069	5.125	99.70%
5.125	5.258	100.00%
5.258	5.390	100.00%
5.390	5.665	100.00%
5.665	5.812	100.00%
5.812	5.959	100.00%
5.959	6.063	100.00%
6.063	6.138	100.00%
6.138	6.361	100.00%
6.361	6.639	100.00%
6.639	6.867	100.00%
6.867	7.943	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060424\
Data File : PL089930.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jun 2024 10:06
Operator : AR\AJ
Sample : RESC030
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
RESC220

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 15:09:04 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060424CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jun 04 15:06:25 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

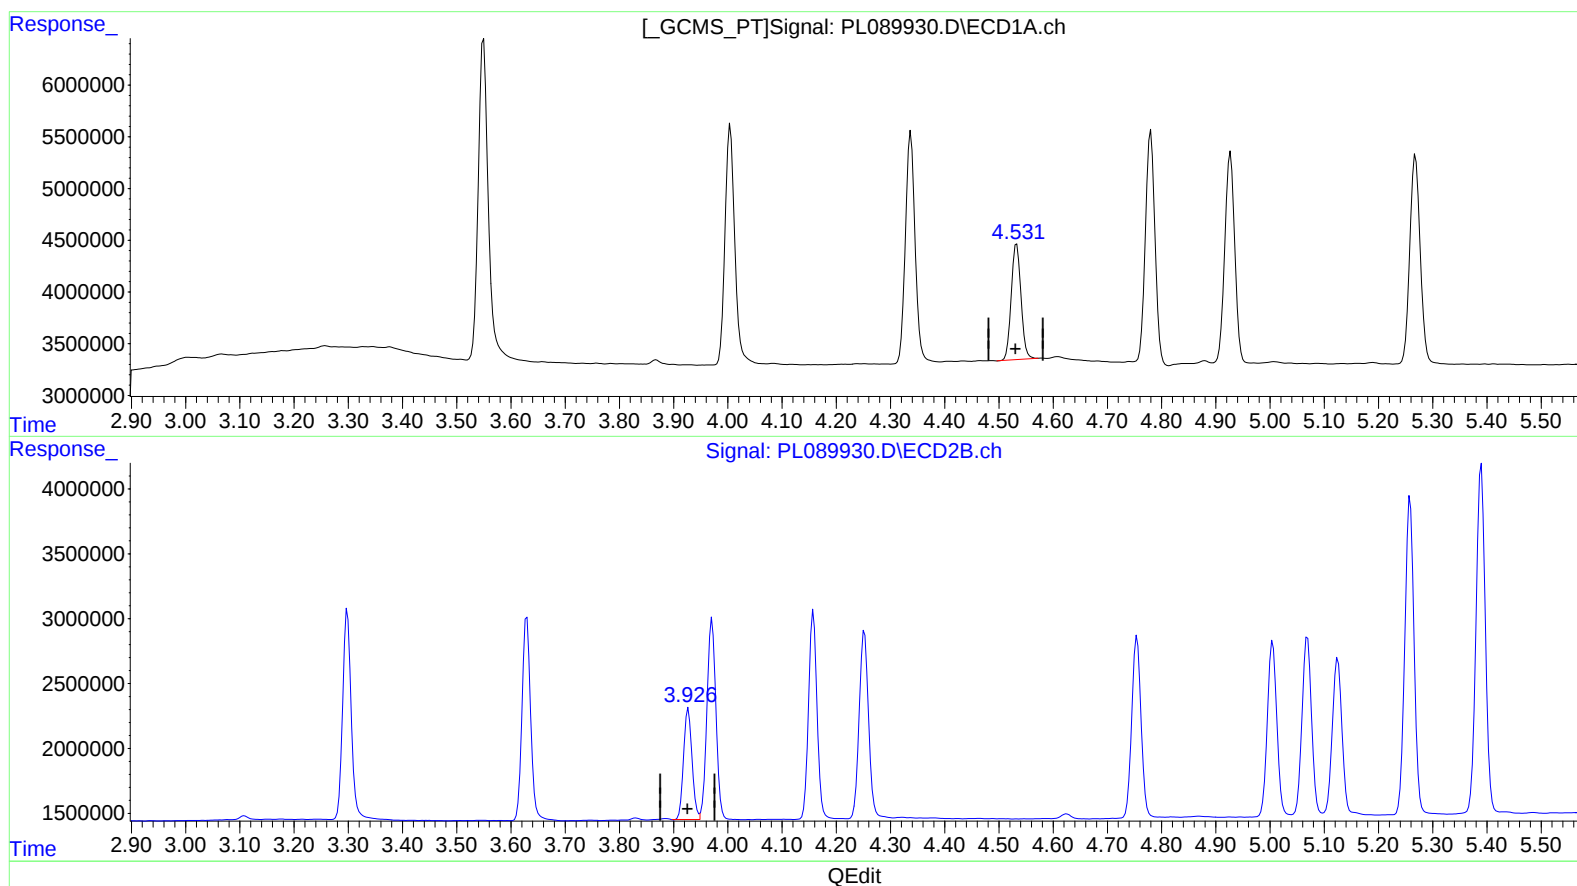

(6) beta-BHC (B)

4.533min 10.768 ng/ml

response 13925116

(6) beta-BHC #2 (B)

3.927min 10.141 ng/ml


response 9257212

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060424\
Data File : PL089930.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jun 2024 10:06
Operator : AR\AJ
Sample : RESC030
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
RESC220

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 15:09:04 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060424CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jun 04 15:06:25 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

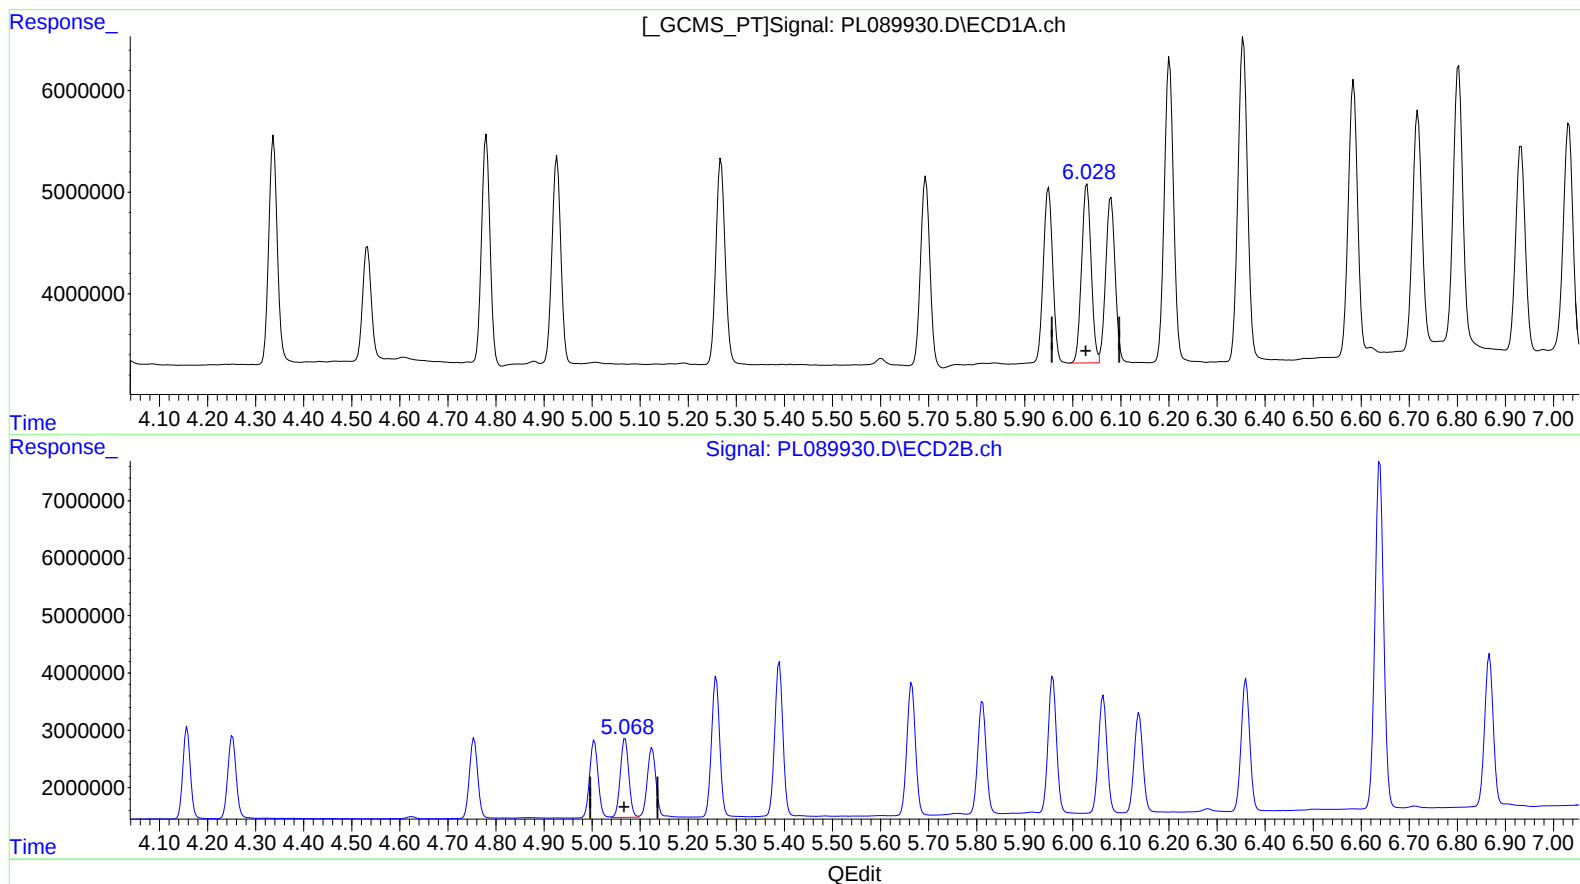

(11) cis-Chlordane (B)

6.030min 10.792 ng/ml

response 24125732

(11) cis-Chlordane #2 (B)

5.069min 9.849 ng/ml

response 16940200