

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060424\
 Data File : PL089962.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jun 2024 20:11
 Operator : AR\AJ
 Sample : P2591-08
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BH5T1

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/05/2024
 Supervised By : Ankita Jodhani 06/05/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 05:27:06 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060424CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 04 15:06:25 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.546	2.790	14026984	10890401	7.273m	8.022m
2)	SA Decachlor...	9.040	7.936	17267590	13430156	13.088m	9.686 #
Target Compounds							
9)	A Endosulfan I	6.107	5.148	32935612	57813780	16.116m	38.497m#
13)	MA Dieldrin	6.368	5.384	43850237	24674860	20.832	14.893m#
16)	A 4,4'-DDD	6.696	5.806	16767292	12345618	11.015m	9.789m
17)	MA 4,4'-DDT	7.025	6.057	3604416	3965832	2.328m	2.939m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060424\
Data File : PL089962.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jun 2024 20:11
Operator : AR\AJ
Sample : P2591-08
Misc :
ALS Vial : 33 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 05:27:06 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060424CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jun 04 15:06:25 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

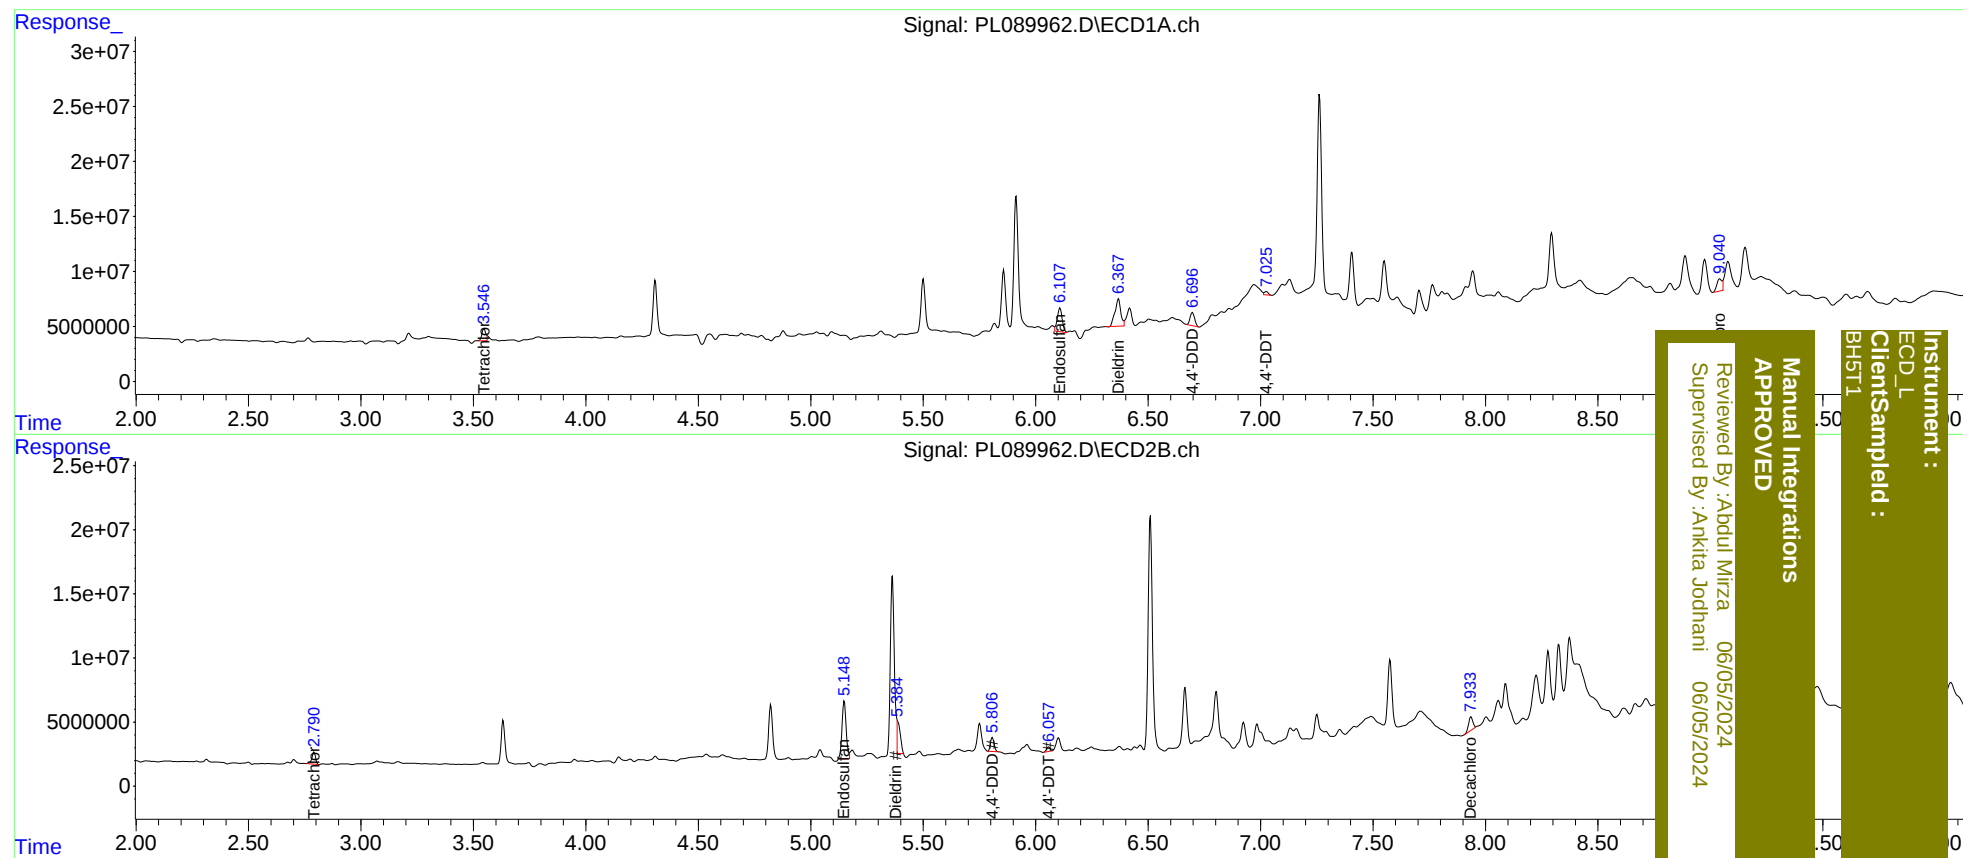

Reviewed By: Abdul Mirza 06/05/2024
Supervised By: Ankita Jodhani 06/05/2024

Manual Integrations
APPROVED

Instrument :
ECD_L
ClientSampled :
BH5T1