

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060425\
 Data File : PL095922.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jun 2025 16:24
 Operator : AR\AJ
 Sample : Q2182-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 01:43:01 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052125.M
 Quant Title : GC Extractables
 QLast Update : Thu May 22 06:29:30 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.572	2.885	37369750	45438253	11.844	11.609
28)	SA Decachlor...	9.099	8.059	22331946	33943092	9.477	7.759
Target Compounds							
9)	A Endosulfan I	6.128f	5.256	1967102	9852215	0.537	2.068 #
10)	B gamma-Chl...	5.968	0.000	2489701	0	0.640	N.D. #
23)	Chlordane-1	0.000	3.897	0	14177745	N.D.	72.713 #
24)	Chlordane-2	0.000	4.512f	0	8163566	N.D.	36.649 #
25)	Chlordane-3	5.968	0.000	2489701	0	3.369	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060425\
Data File : PL095922.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jun 2025 16:24
Operator : AR\AJ
Sample : Q2182-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 01:43:01 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052125.M
Quant Title : GC Extractables
QLast Update : Thu May 22 06:29:30 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

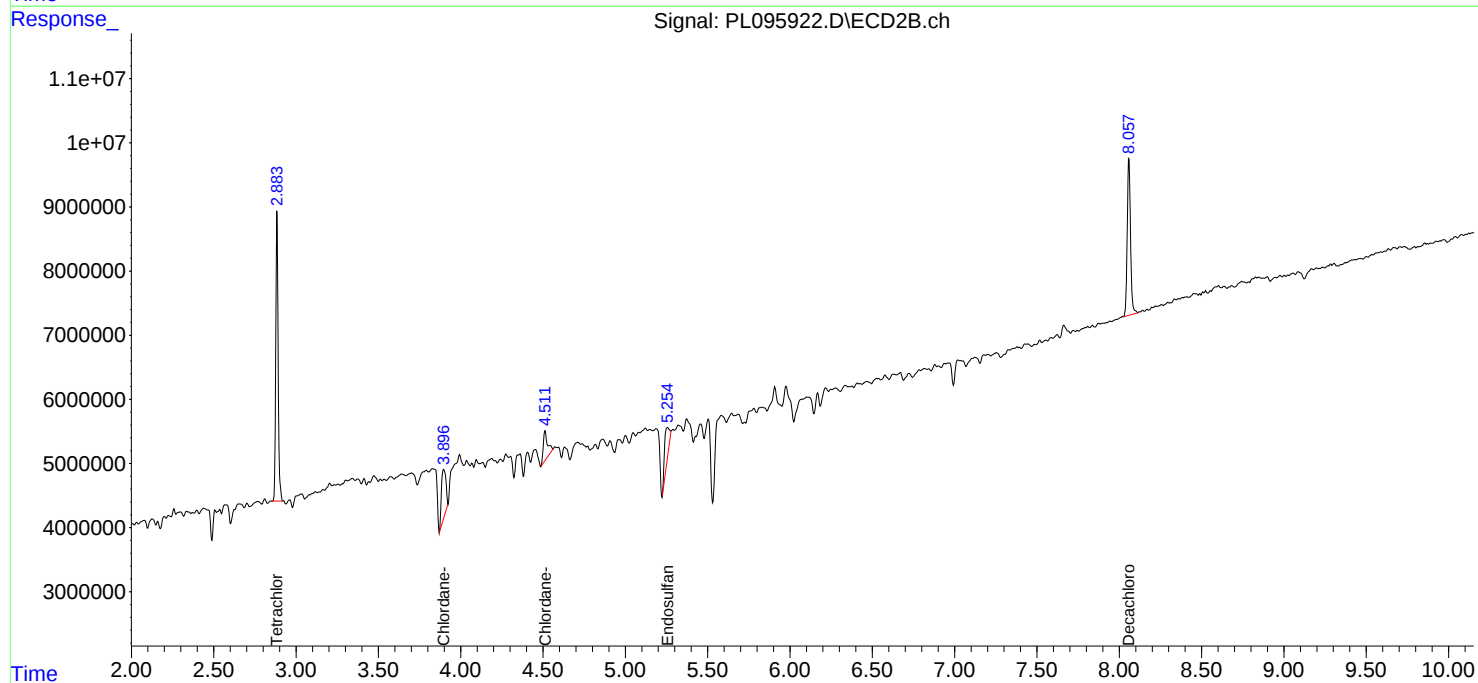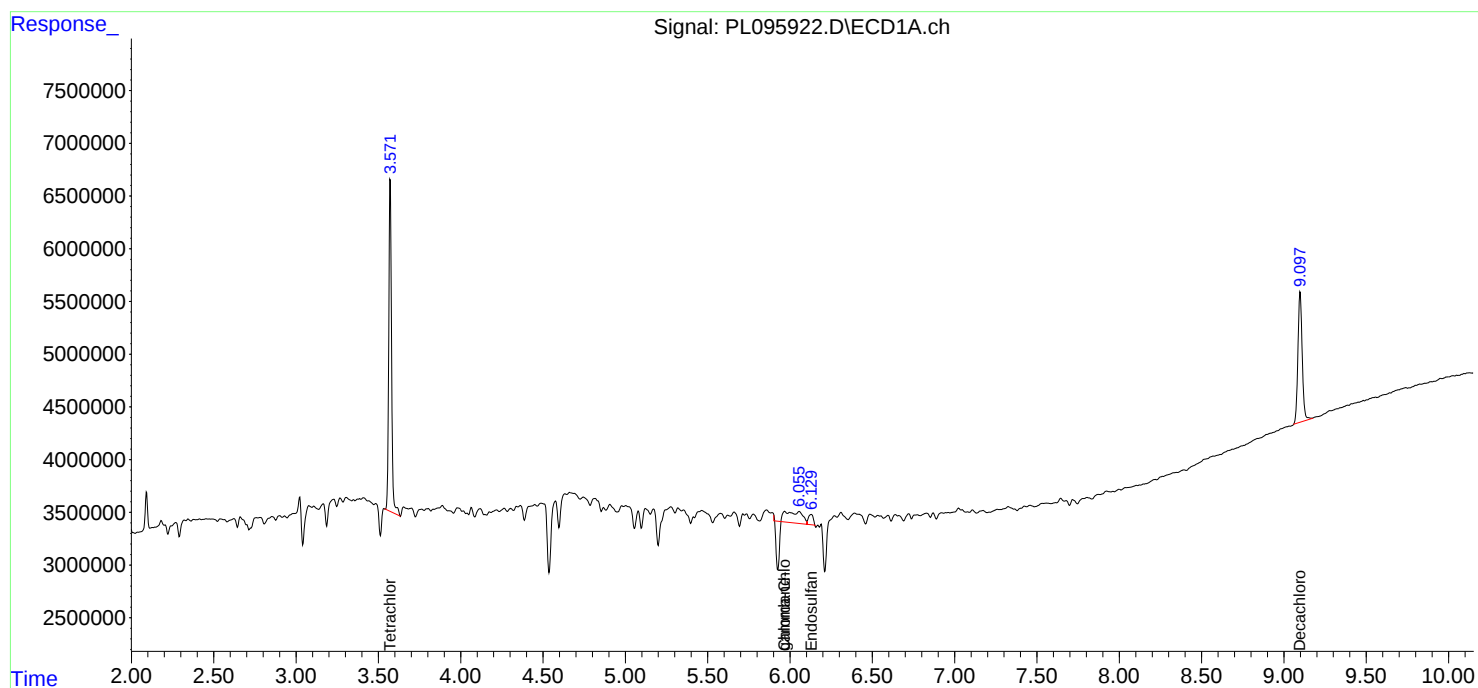


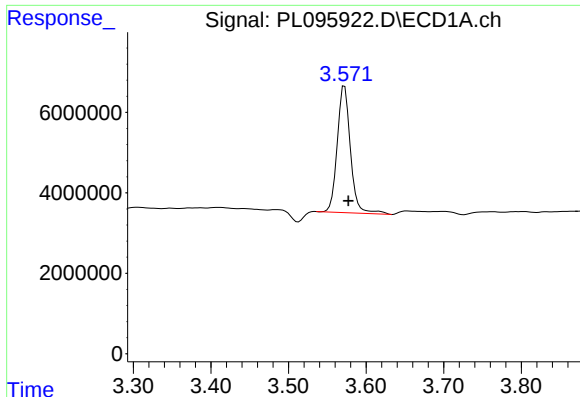

#1 Tetrachloro-m-xylene


R.T.: 3.572 min
Delta R.T.: -0.005 min
Response: 37369750
Conc: 11.84 ng/ml

Instrument :
ECD_L
ClientSampleId :

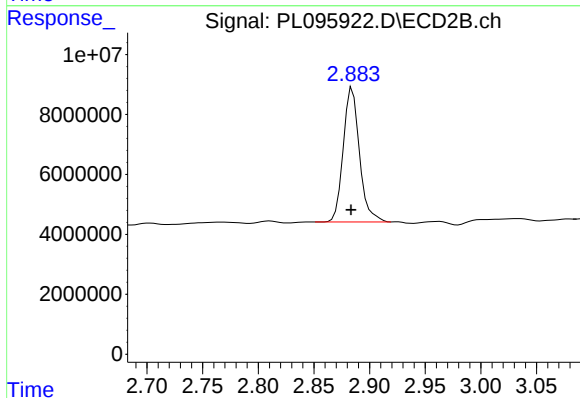


#1 Tetrachloro-m-xylene

R.T.: 2.885 min
Delta R.T.: 0.001 min
Response: 45438253
Conc: 11.61 ng/ml

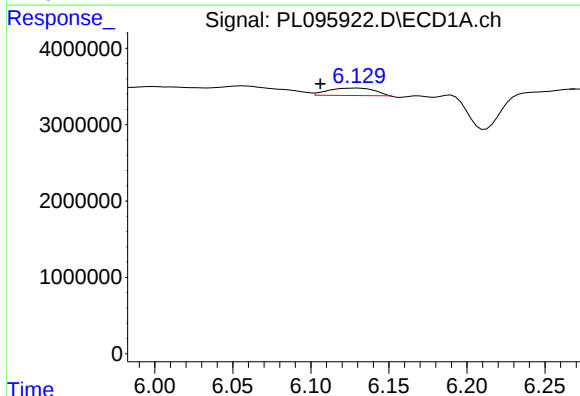


#9 Endosulfan I

R.T.: 6.128 min
Delta R.T.: 0.022 min
Response: 1967102
Conc: 0.54 ng/ml

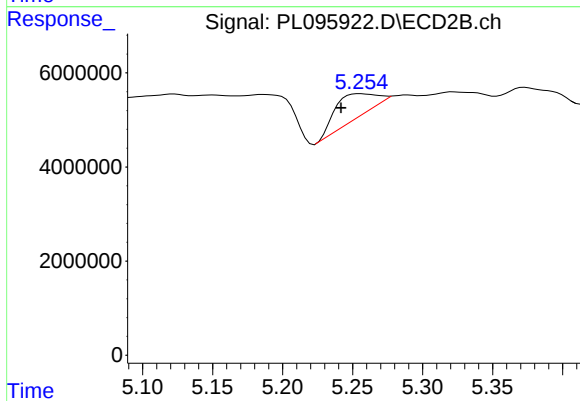

#9 Endosulfan I


R.T.: 5.256 min
Delta R.T.: 0.014 min
Response: 9852215
Conc: 2.07 ng/ml

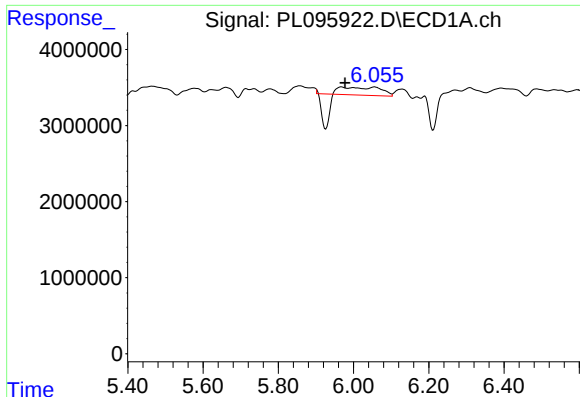

#10 gamma-Chlordane


R.T.: 5.968 min
Delta R.T.: -0.010 min
Response: 2489701
Conc: 0.64 ng/ml

Instrument :
ECD_L
ClientSampleId :

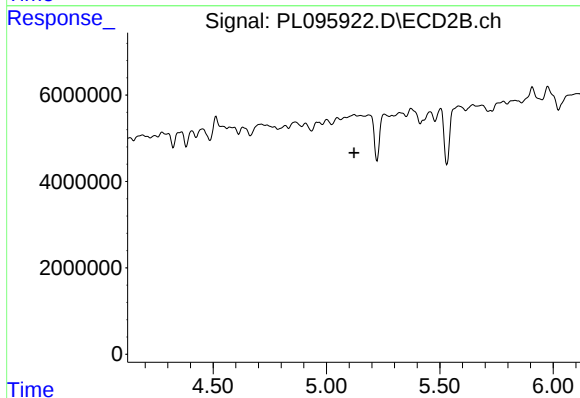


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.122 min
Response: 0
Conc: N.D.

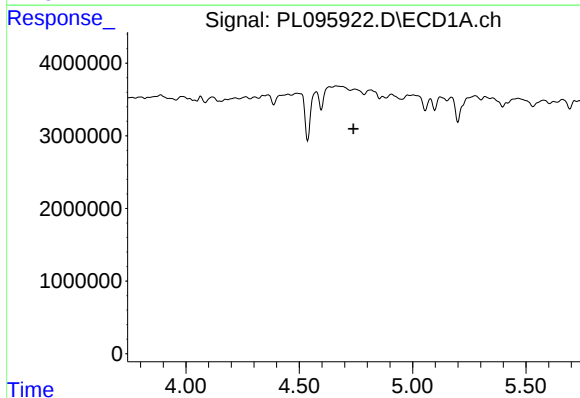


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.739 min
Response: 0
Conc: N.D.

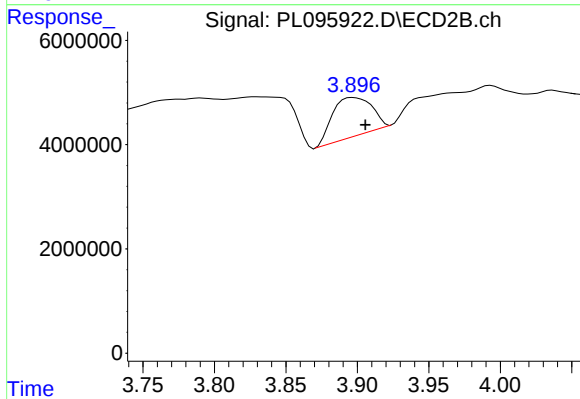

#23 Chlordane-1


R.T.: 3.897 min
Delta R.T.: -0.009 min
Response: 14177745
Conc: 72.71 ng/ml

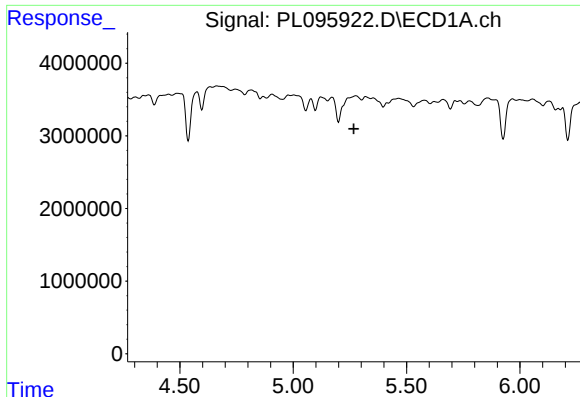

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.267 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

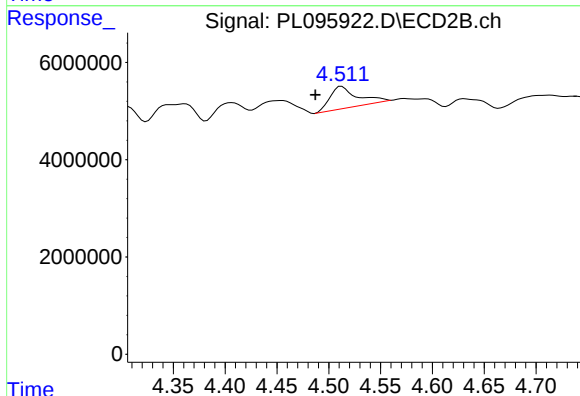


#24 Chlordane-2

R.T.: 4.512 min
Delta R.T.: 0.025 min
Response: 8163566
Conc: 36.65 ng/ml

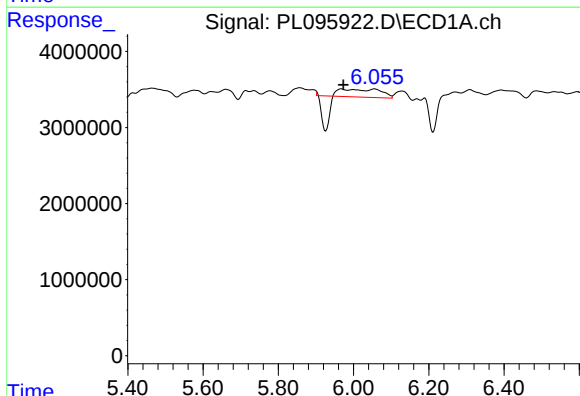


#25 Chlordane-3

R.T.: 5.968 min
Delta R.T.: -0.005 min
Response: 2489701
Conc: 3.37 ng/ml

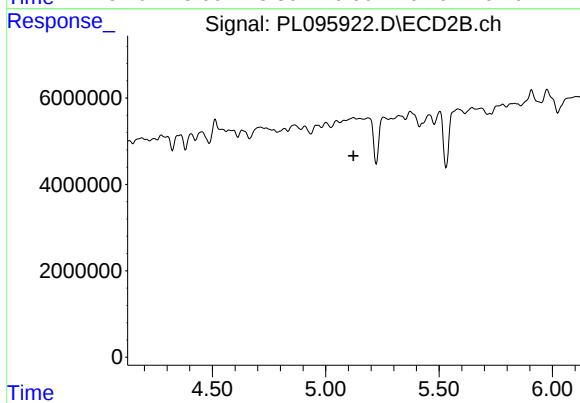

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.123 min
Response: 0
Conc: N.D.

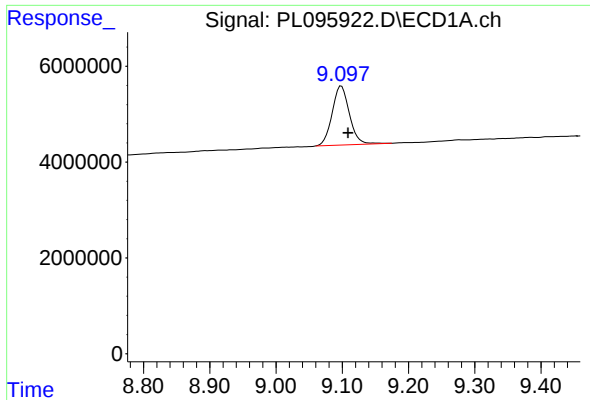

#28 Decachlorobiphenyl

R.T.: 9.099 min
Delta R.T.: -0.010 min
Response: 22331946
Conc: 9.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

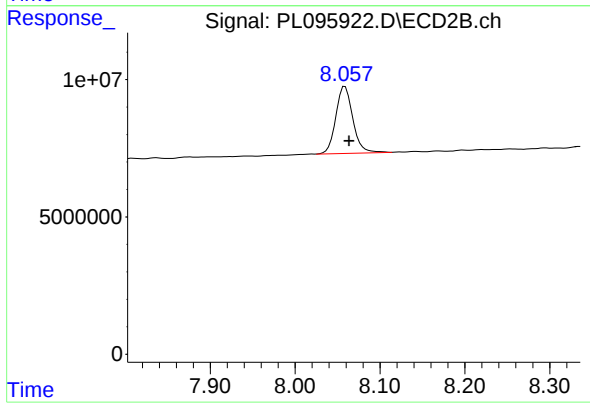

#28 Decachlorobiphenyl

R.T.: 8.059 min
Delta R.T.: -0.005 min
Response: 33943092
Conc: 7.76 ng/ml