

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060425\
 Data File : PL095922.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jun 2025 16:24
 Operator : AR\AJ
 Sample : Q2182-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OR-03-06022025

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/05/2025
 Supervised By : mohammad ahmed 06/06/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 01:43:01 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052125.M
 Quant Title : GC Extractables
 QLast Update : Thu May 22 06:29:30 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.571	2.885	35624463	45438253	11.290m	11.609
28) SA Decachlor...	9.099	8.059	22331946	33943092	9.477	7.759

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060425\
Data File : PL095922.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jun 2025 16:24
Operator : AR\AJ
Sample : Q2182-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
OR-03-06022025


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 06/05/2025
Supervised By : mohammad ahmed 06/06/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 01:43:01 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052125.M
Quant Title : GC Extractables
QLast Update : Thu May 22 06:29:30 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

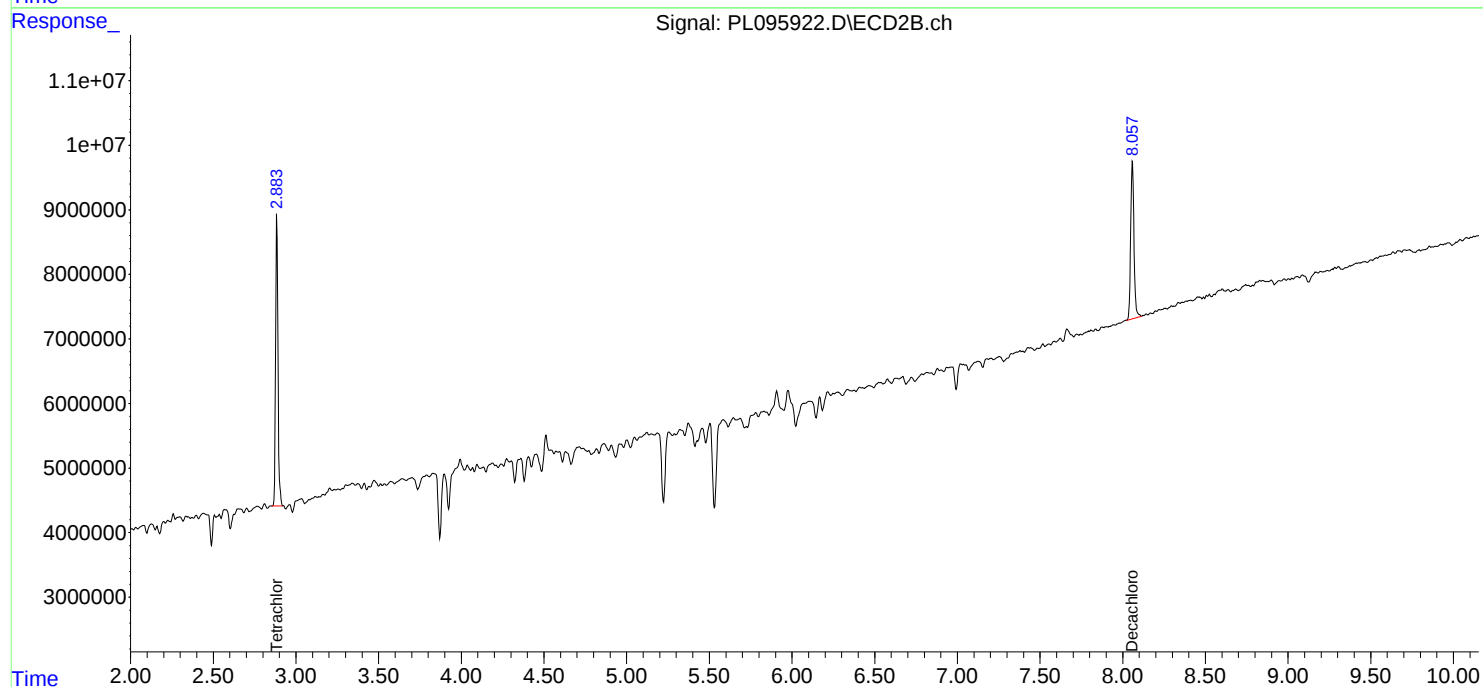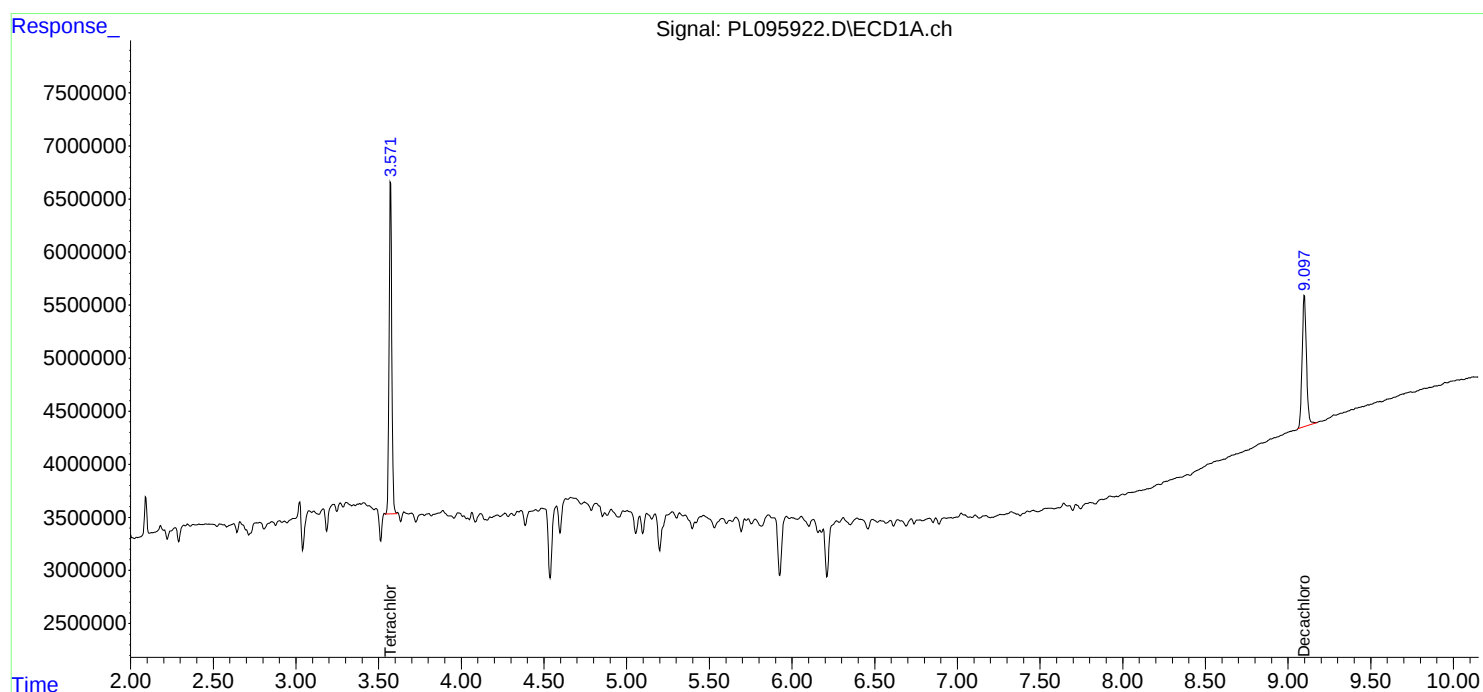

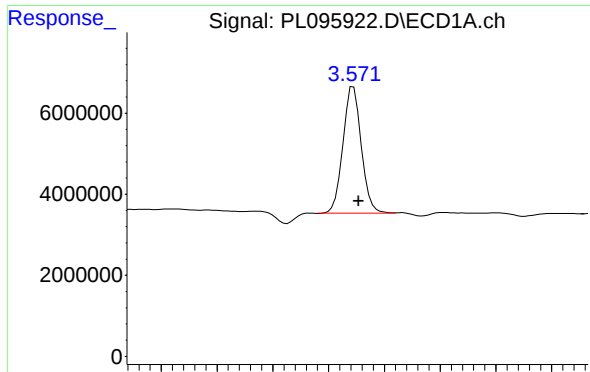


#1 Tetrachloro-m-xylene

R.T.: 3.571 min
Delta R.T.: -0.006 min
Response: 35624463
Conc: 11.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-03-06022025


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/05/2025
Supervised By :mohammad ahmed 06/06/2025

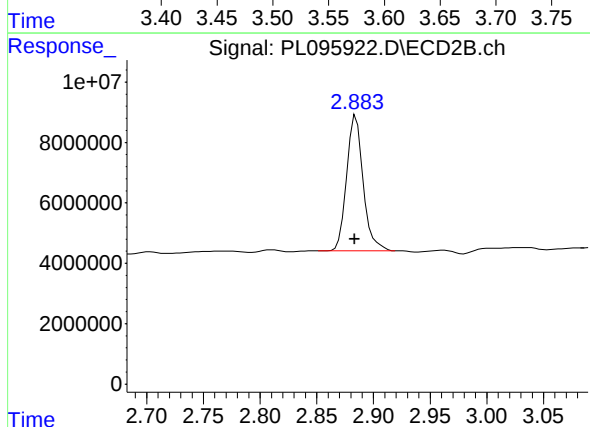


#1 Tetrachloro-m-xylene

R.T.: 2.885 min
Delta R.T.: 0.001 min
Response: 45438253
Conc: 11.61 ng/ml

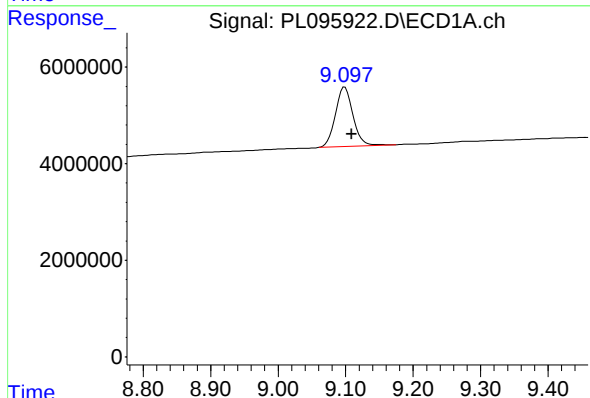

#28 Decachlorobiphenyl

R.T.: 9.099 min
Delta R.T.: -0.010 min
Response: 22331946
Conc: 9.48 ng/ml

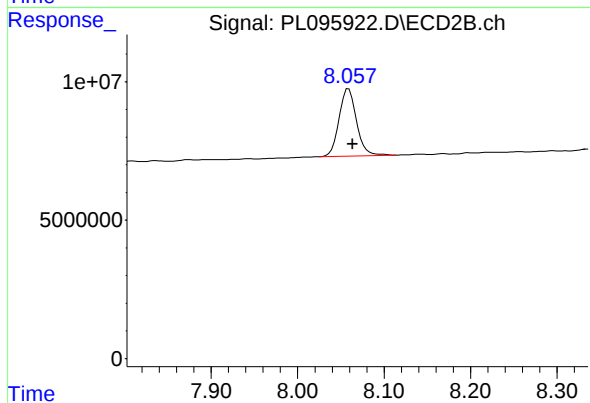

#28 Decachlorobiphenyl

R.T.: 8.059 min
Delta R.T.: -0.005 min
Response: 33943092
Conc: 7.76 ng/ml