

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060519\
 Data File : PL049307.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jun 2019 15:25
 Operator : SM\AJ
 Sample : PB120326BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB120326BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 06 00:59:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
 Quant Title : GC Extractables
 QLast Update : Fri May 31 01:35:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

14) MA	Endrin	5.821	0.000	20922906	0	1.451	N.D.	#
--------	--------	-------	-------	----------	---	-------	------	---



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060519\
Data File : PL049307.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jun 2019 15:25
Operator : SM\AJ
Sample : PB120326BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB120326BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 06 00:59:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
Quant Title : GC Extractables
QLast Update : Fri May 31 01:35:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

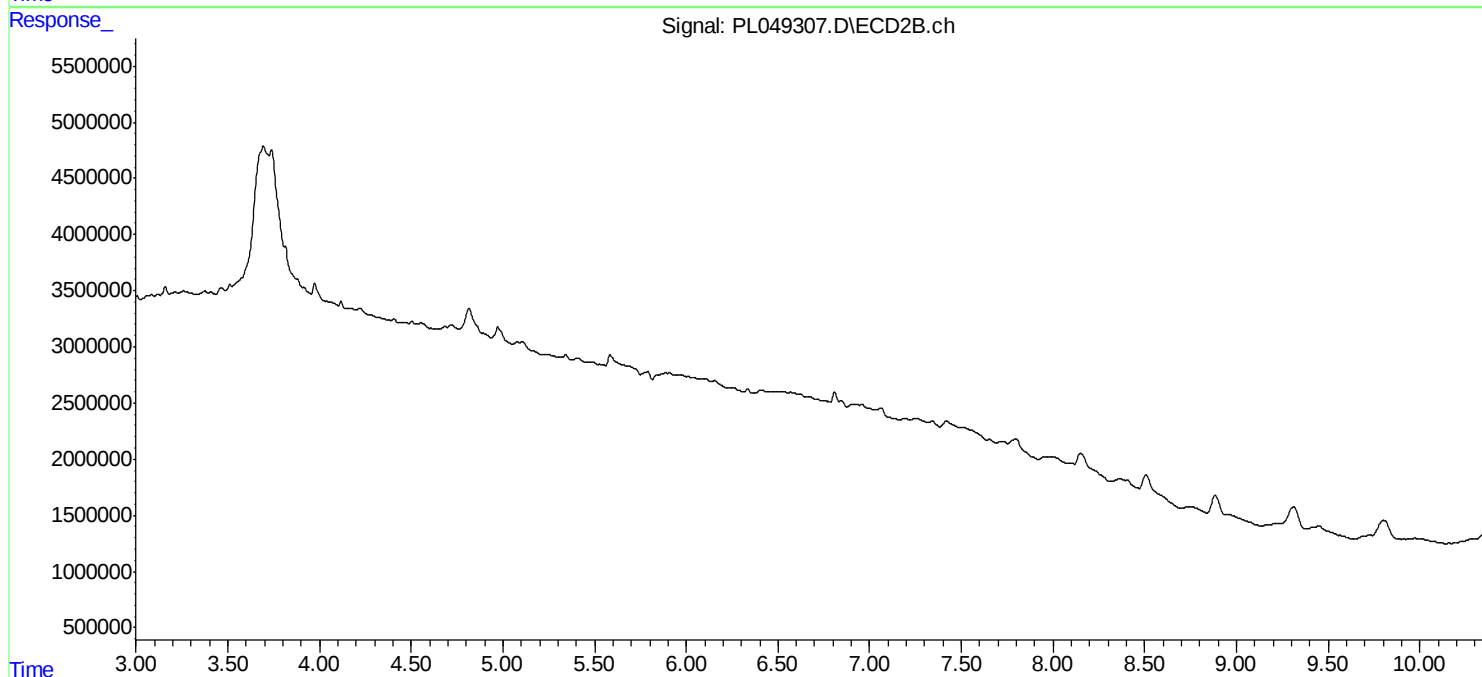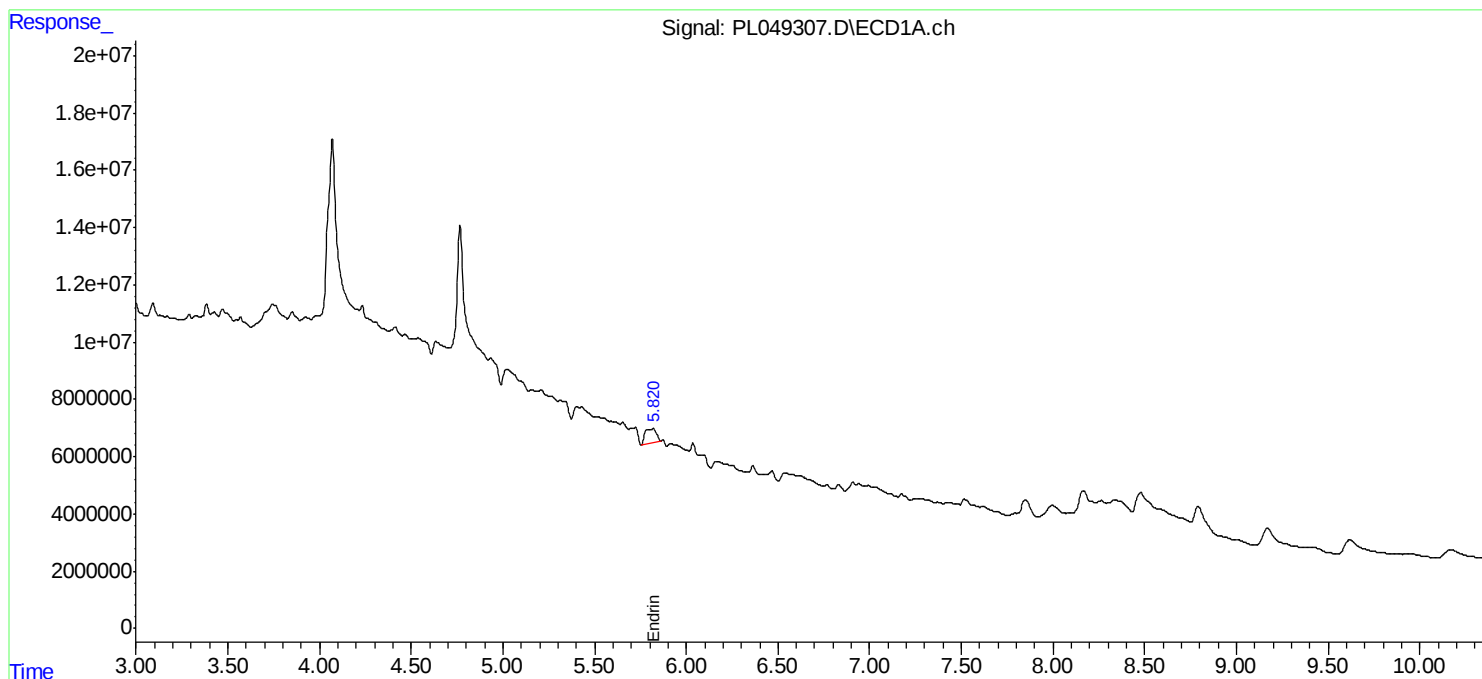


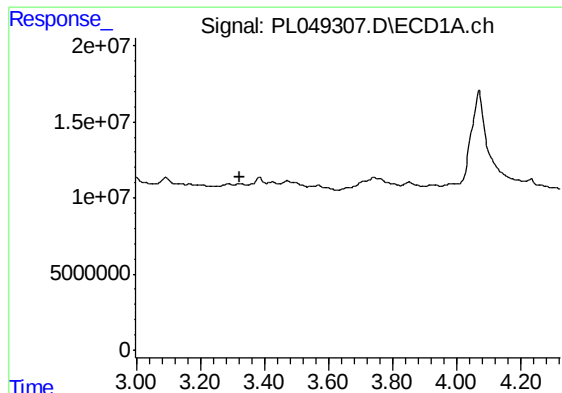

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.324 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB120326BL

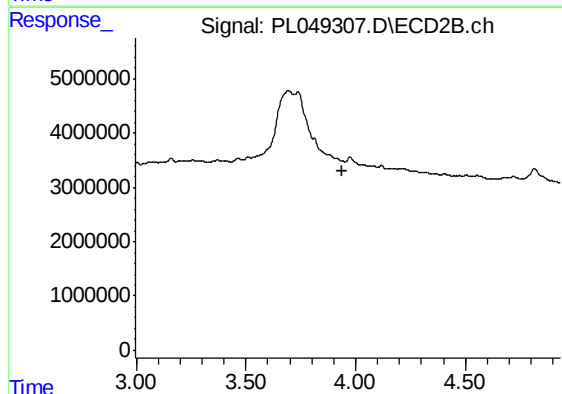


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.936 min
Response: 0
Conc: N.D.

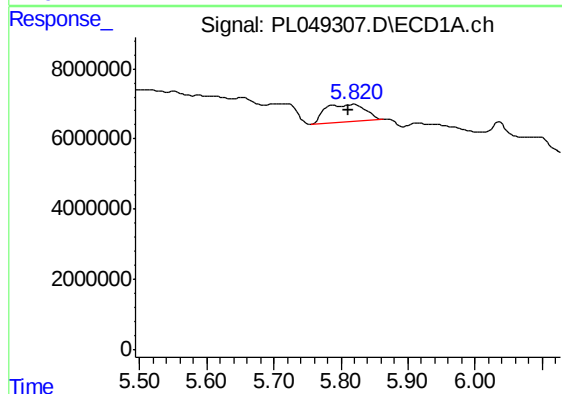


#14 Endrin

R.T.: 5.821 min
Delta R.T.: 0.010 min
Response: 20922906
Conc: 1.45 ng/ml

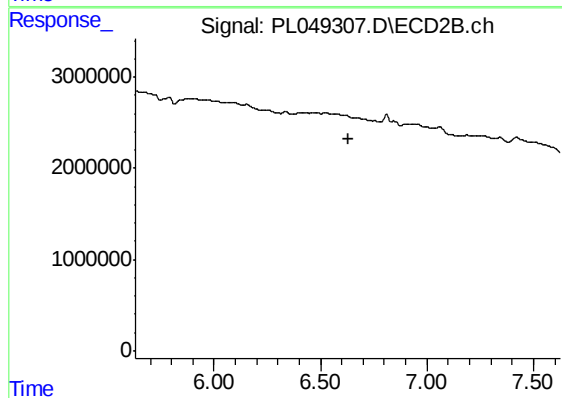

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.630 min
Response: 0
Conc: N.D.

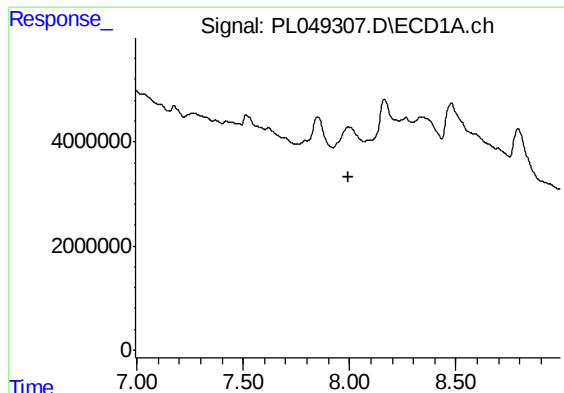

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.992 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB120326BL

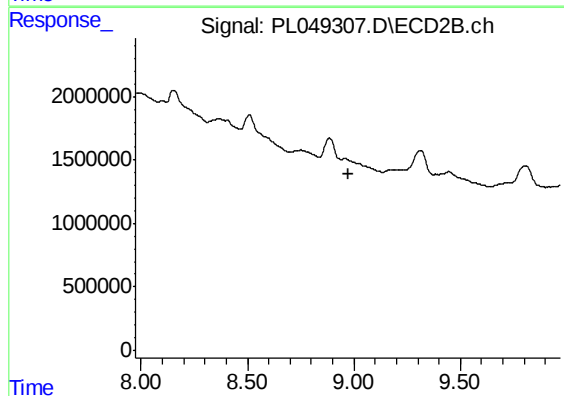

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.972 min
Response: 0
Conc: N.D.