

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060519\
 Data File : PL049327.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jun 2019 20:54
 Operator : SM\AJ
 Sample : K3183-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SP-COMP-1

Manual Integrations
 APPROVED

Ankita
 6/6/2019 11:05:57 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 06 01:04:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
 Quant Title : GC Extractables
 QLast Update : Fri May 31 01:35:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.325	3.937	197.5E6	50405976	17.922	17.447
28)	SA Decachlor...	7.993	8.975	179.1E6	52291592	14.085	15.658
Target Compounds							
12)	B 4,4'-DDE	5.433	6.265	56265001	13092552	3.597m	3.988
16)	A 4,4'-DDD	5.942	6.756	11149223	7726194	0.937m	2.937 #
17)	MA 4,4'-DDT	6.179	7.054	36013704	8318490	2.925	2.967

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060519\
Data File : PL049327.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jun 2019 20:54
Operator : SM\AJ
Sample : K3183-01
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SP-COMP-1


Manual Integrations
APPROVED

Ankita
6/6/2019 11:05:57 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 06 01:04:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
Quant Title : GC Extractables
QLast Update : Fri May 31 01:35:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

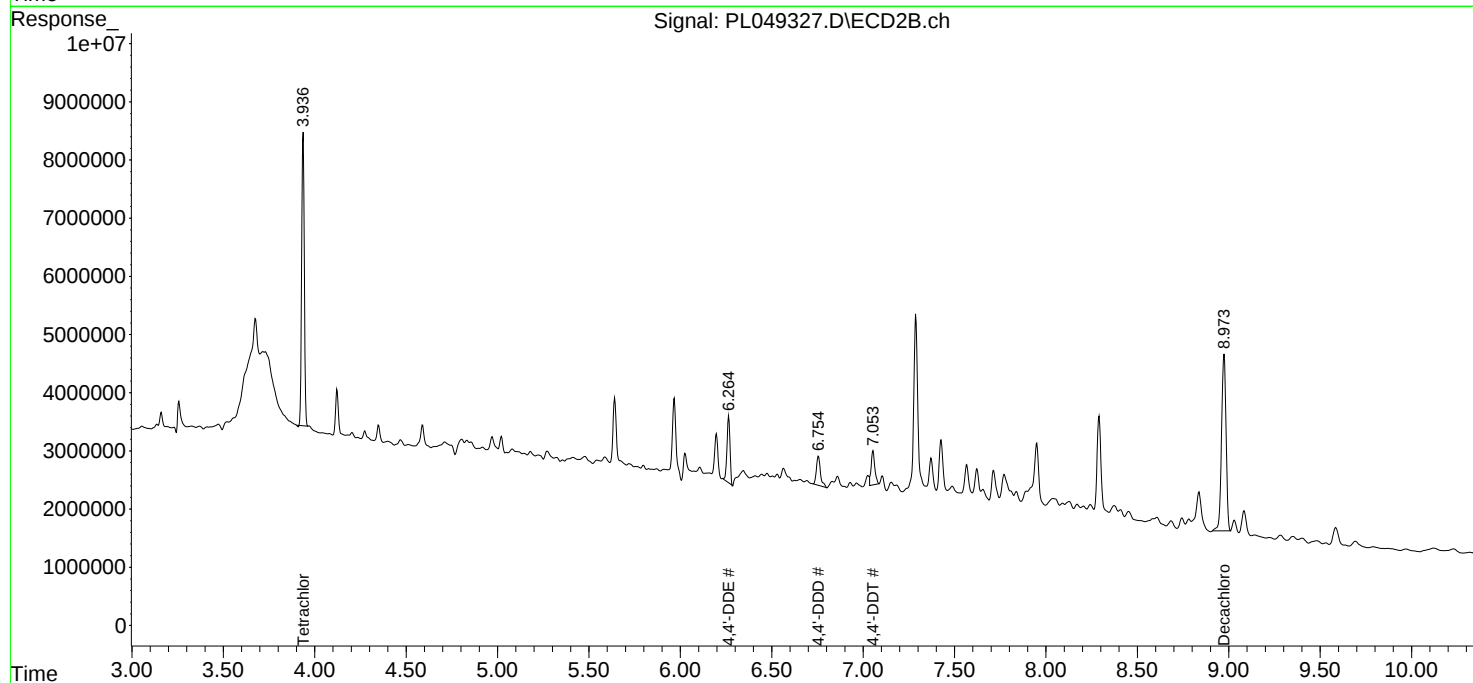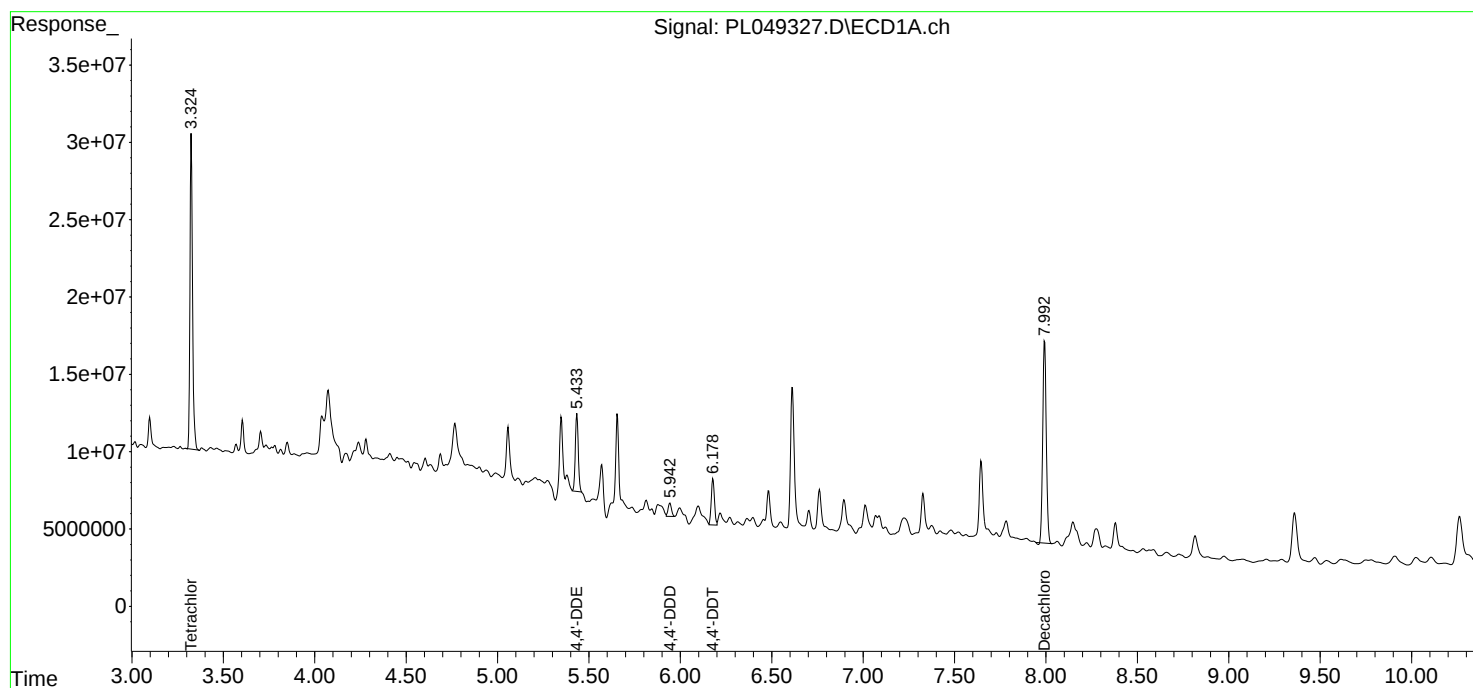

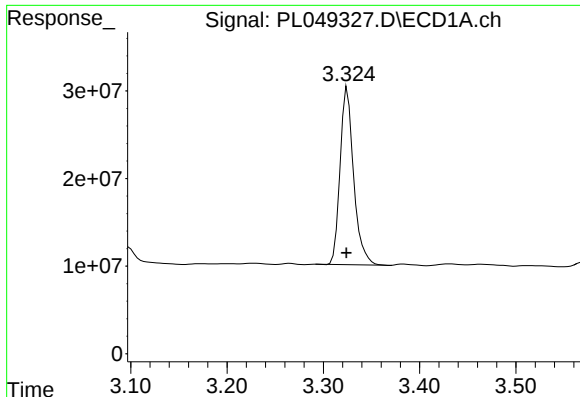


#1 Tetrachloro-m-xylene

R.T.: 3.325 min
Delta R.T.: 0.001 min
Response: 197477444
Conc: 17.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
SP-COMP-1


Manual Integrations
APPROVED

Ankita
6/6/2019 11:05:57 AM

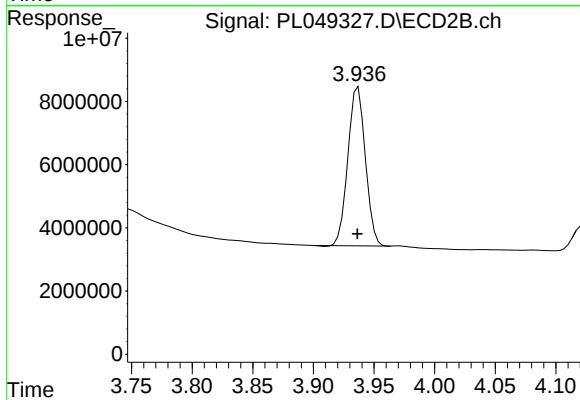


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: 0.000 min
Response: 50405976
Conc: 17.45 ng/ml

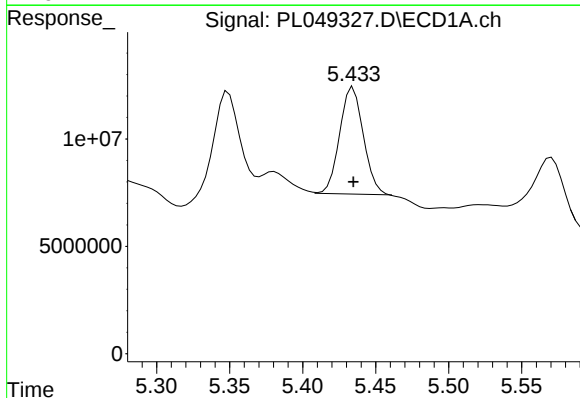


#12 4,4'-DDE

R.T.: 5.433 min
Delta R.T.: -0.002 min
Response: 56265001
Conc: 3.60 ng/ml m

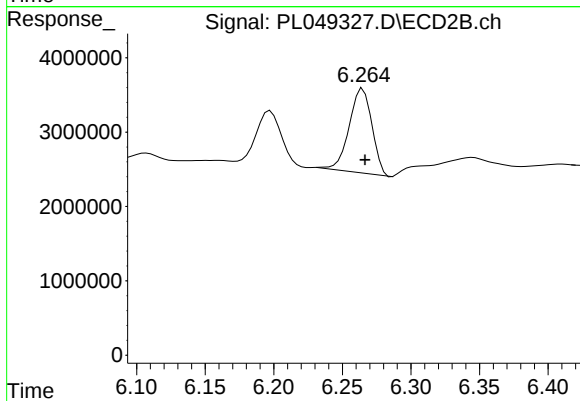

#12 4,4'-DDE

R.T.: 6.265 min
Delta R.T.: -0.002 min
Response: 13092552
Conc: 3.99 ng/ml

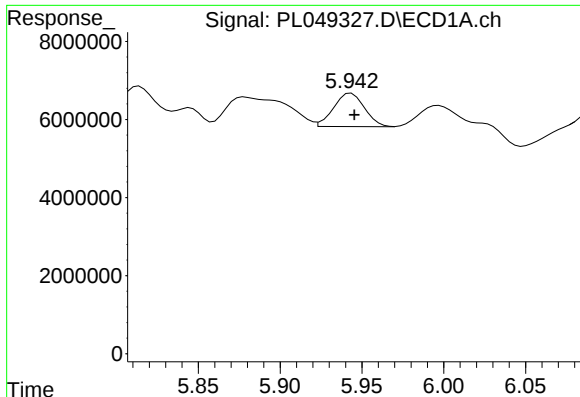


#16 4,4'-DDD

R.T.: 5.942 min
Delta R.T.: -0.003 min
Response: 11149223
Conc: 0.94 ng/ml m

Instrument :
ECD_L
ClientSampleId :
SP-COMP-1


Manual Integrations
APPROVED

Ankita
6/6/2019 11:05:57 AM

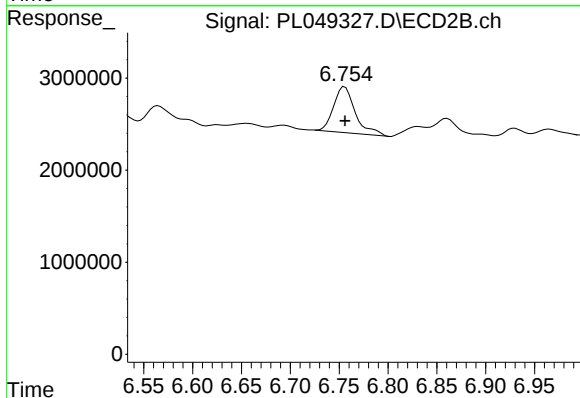


#16 4,4'-DDD

R.T.: 6.756 min
Delta R.T.: 0.000 min
Response: 7726194
Conc: 2.94 ng/ml

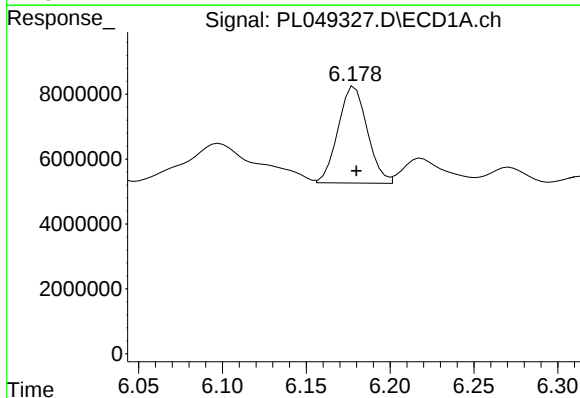


#17 4,4'-DDT

R.T.: 6.179 min
Delta R.T.: -0.001 min
Response: 36013704
Conc: 2.92 ng/ml

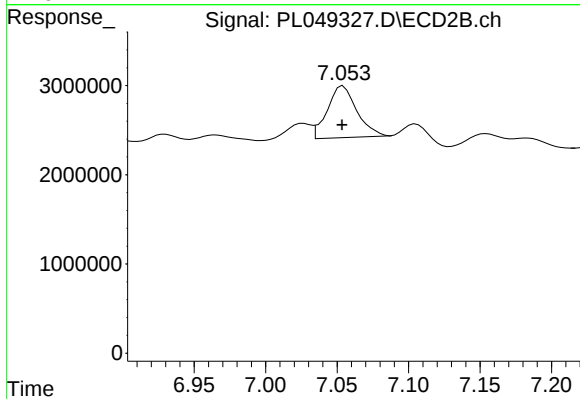

#17 4,4'-DDT

R.T.: 7.054 min
Delta R.T.: 0.000 min
Response: 8318490
Conc: 2.97 ng/ml

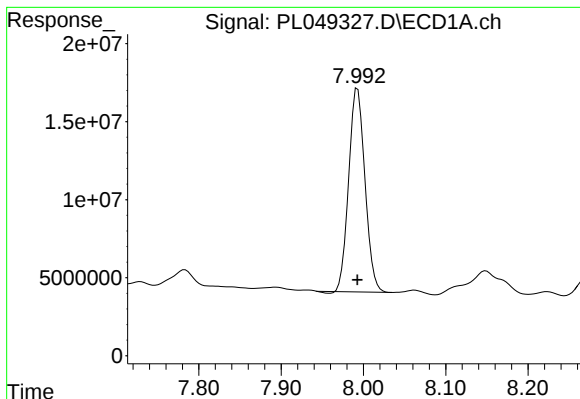

#28 Decachlorobiphenyl

R.T.: 7.993 min

Delta R.T.: 0.000 min


Response: 179091024

Conc: 14.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
SP-COMP-1

Manual Integrations
APPROVED

Ankita
6/6/2019 11:05:57 AM

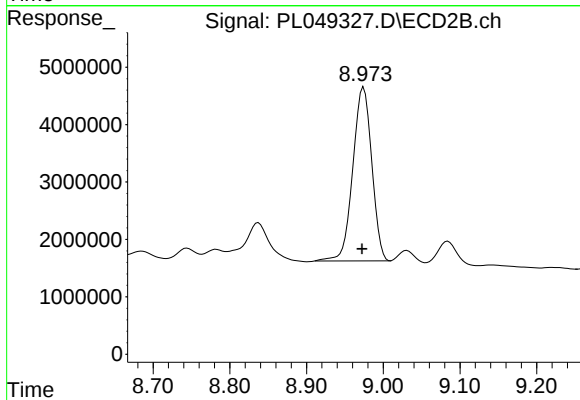

#28 Decachlorobiphenyl

R.T.: 8.975 min

Delta R.T.: 0.002 min

Response: 52291592

Conc: 15.66 ng/ml