

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060519\
 Data File : PL049330.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jun 2019 21:40
 Operator : SM\AJ
 Sample : K3183-03
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SP-COMP-2

Manual Integrations
 APPROVED

Ankita
 6/6/2019 11:06:02 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 06 01:05:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
 Quant Title : GC Extractables
 QLast Update : Fri May 31 01:35:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.325	3.937	94500273	25267587	8.576	8.746
28) SA Decachlor...	7.993	8.974	91762886	25687372	7.217	7.692
Target Compounds						
12) B 4,4'-DDE	5.433	6.266	15258426	2955303	0.975m	0.900
17) MA 4,4'-DDT	6.178	7.056	6910504	1464651	0.561	0.522m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060519\
Data File : PL049330.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jun 2019 21:40
Operator : SM\AJ
Sample : K3183-03
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SP-COMP-2


Manual Integrations
APPROVED

Ankita
6/6/2019 11:06:02 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 06 01:05:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
Quant Title : GC Extractables
QLast Update : Fri May 31 01:35:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

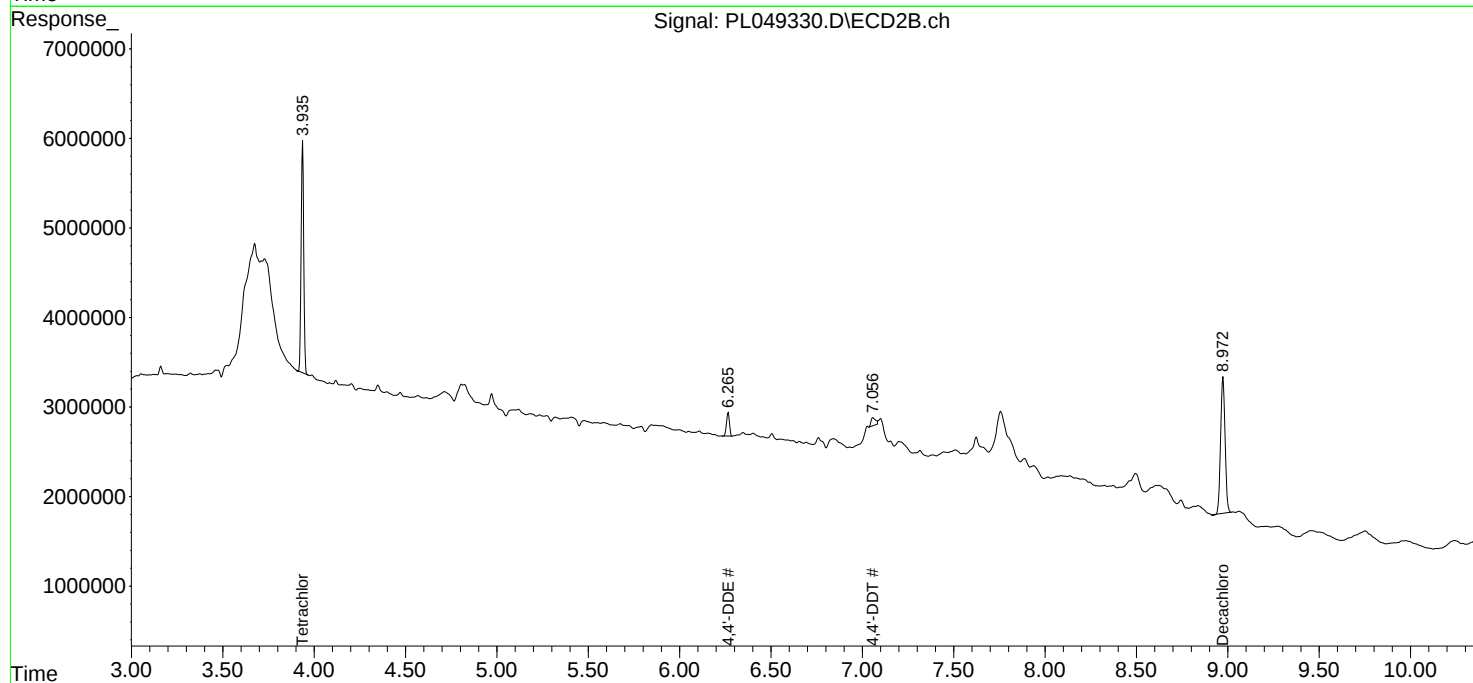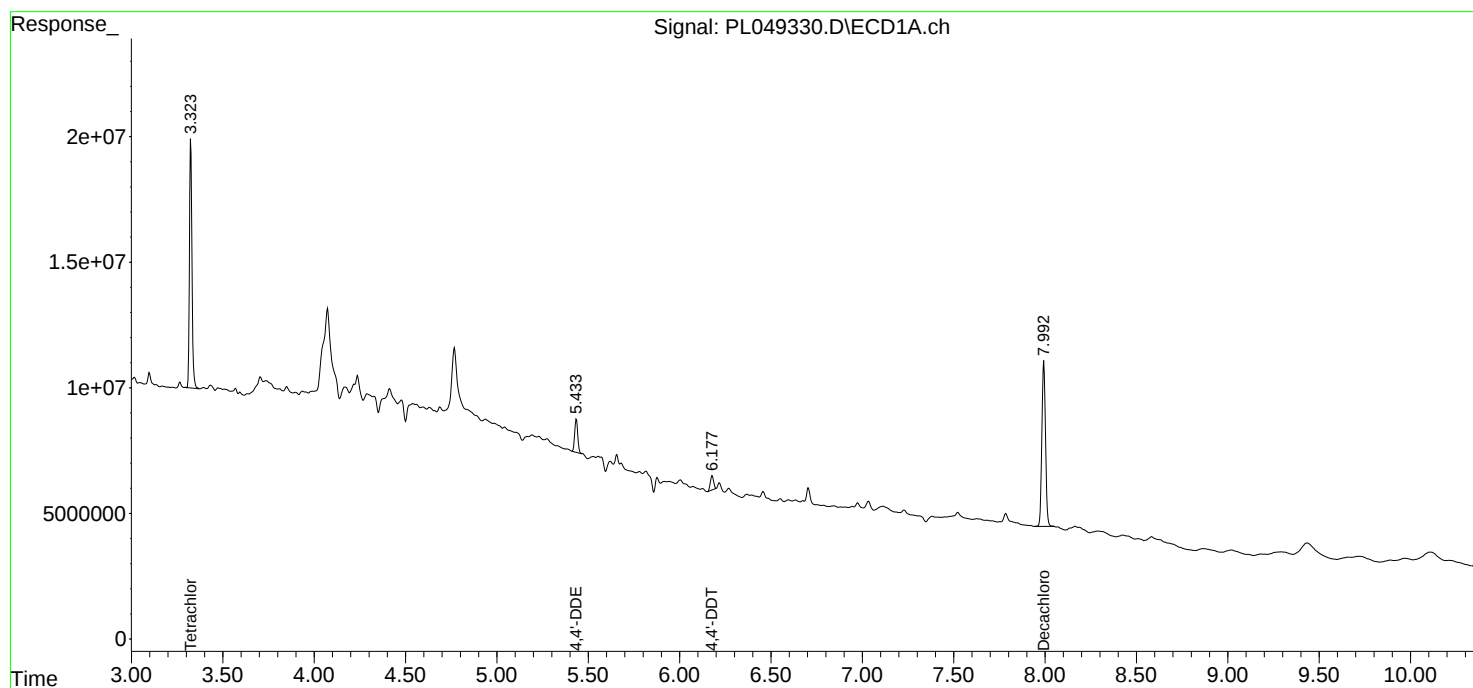

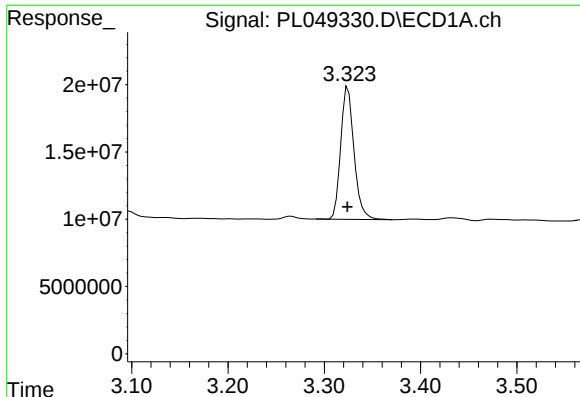


#1 Tetrachloro-m-xylene

R.T.: 3.325 min
Delta R.T.: 0.000 min
Response: 94500273
Conc: 8.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
SP-COMP-2


Manual Integrations
APPROVED

Ankita
6/6/2019 11:06:02 AM

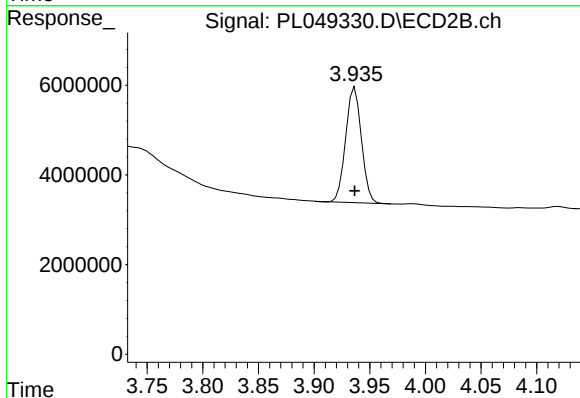


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: 0.000 min
Response: 25267587
Conc: 8.75 ng/ml

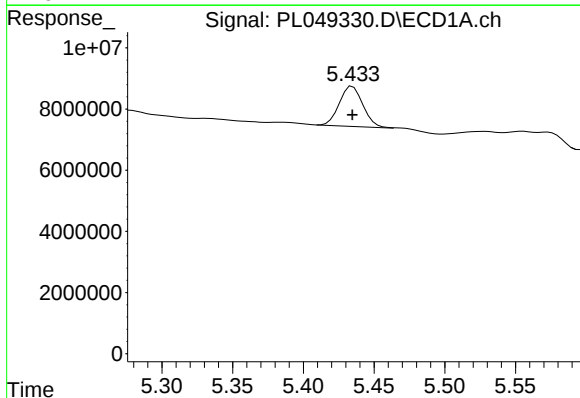


#12 4,4'-DDE

R.T.: 5.433 min
Delta R.T.: -0.001 min
Response: 15258426
Conc: 0.98 ng/ml m

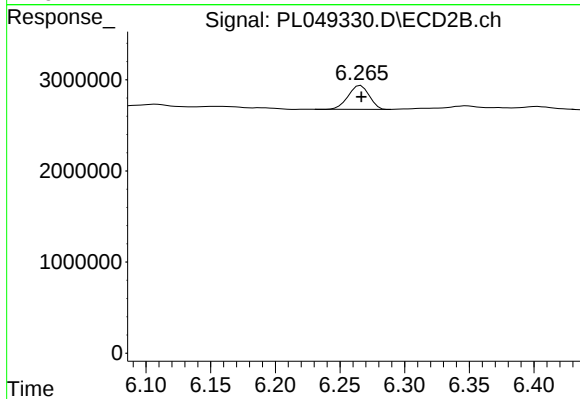

#12 4,4'-DDE

R.T.: 6.266 min
Delta R.T.: 0.000 min
Response: 2955303
Conc: 0.90 ng/ml

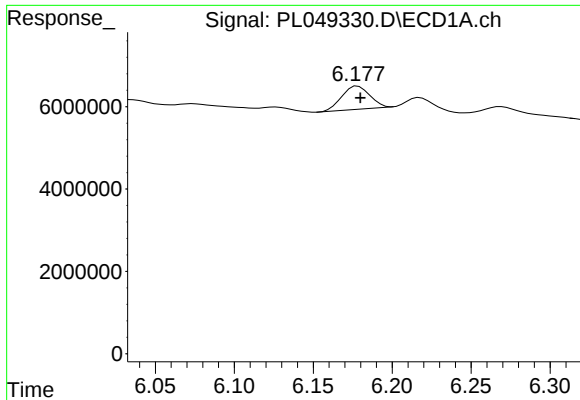


#17 4,4'-DDT

R.T.: 6.178 min
Delta R.T.: -0.002 min
Response: 6910504
Conc: 0.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
SP-COMP-2


Manual Integrations
APPROVED

Ankita
6/6/2019 11:06:02 AM

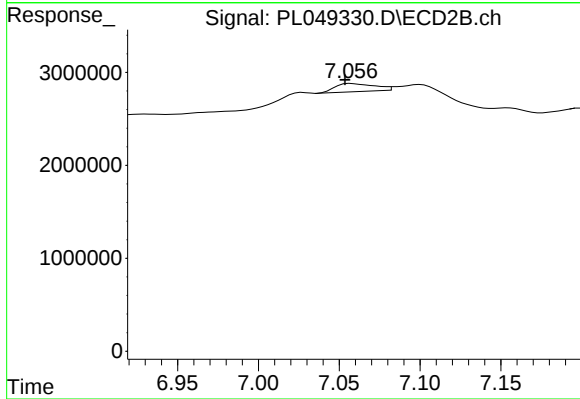


#17 4,4'-DDT

R.T.: 7.056 min
Delta R.T.: 0.002 min
Response: 1464651
Conc: 0.52 ng/ml m

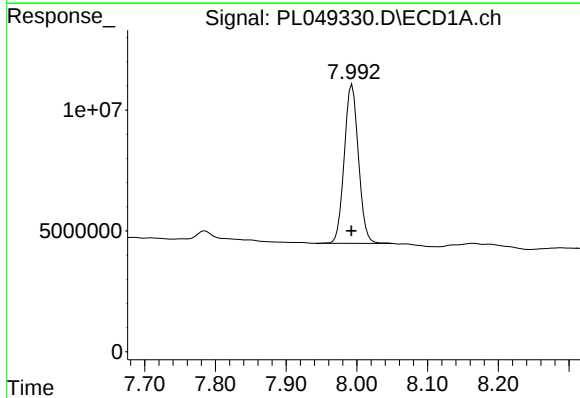

#28 Decachlorobiphenyl

R.T.: 7.993 min
Delta R.T.: 0.000 min
Response: 91762886
Conc: 7.22 ng/ml

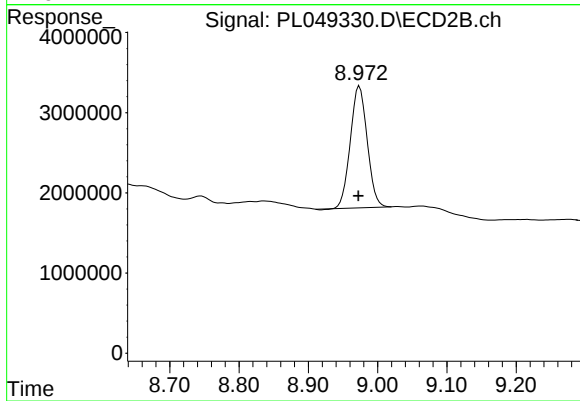

#28 Decachlorobiphenyl

R.T.: 8.974 min
Delta R.T.: 0.002 min
Response: 25687372
Conc: 7.69 ng/ml