

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060520\
 Data File : PL059142.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jun 2020 13:29
 Operator : AJ\MA
 Sample : PB129338BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 15:06:11 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060320.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 04 08:16:22 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.528	4.072	34972892	40121998	20.253	15.420
28)	SA Decachlor...	8.303	9.184	34119129	49036408	20.749	20.686
Target Compounds							
8)	B Heptachlo...	0.000	5.947	0	318289	N.D.	0.115 #
11)	B alpha-Chl...	0.000	6.277	0	2671966	N.D.	0.879 #
13)	MA Dieldrin	0.000	6.579	0	197053	N.D.	0.067 #
14)	MA Endrin	0.000	6.803	0	2050118	N.D.	0.823 #
15)	B Endosulfa...	0.000	6.994	0	5935453	N.D.	2.279 #
16)	A 4,4'-DDD	6.218	6.932f	2663532	117207	2.015	0.050 #
17)	MA 4,4'-DDT	6.465	7.211	534674	1162592	0.424	0.511
21)	B Endrin ke...	7.249	0.000	713032	0	0.411	N.D. #
22)	Mirex	7.431	0.000	2524318	0	1.829	N.D. #
26)	Chlordane-4	0.000	6.277	0	2671966	N.D.	5.872 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060520\
Data File : PL059142.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jun 2020 13:29
Operator : AJ\MA
Sample : PB129338BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 15:06:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060320.M
Quant Title : GC Extractables
QLast Update : Thu Jun 04 08:16:22 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

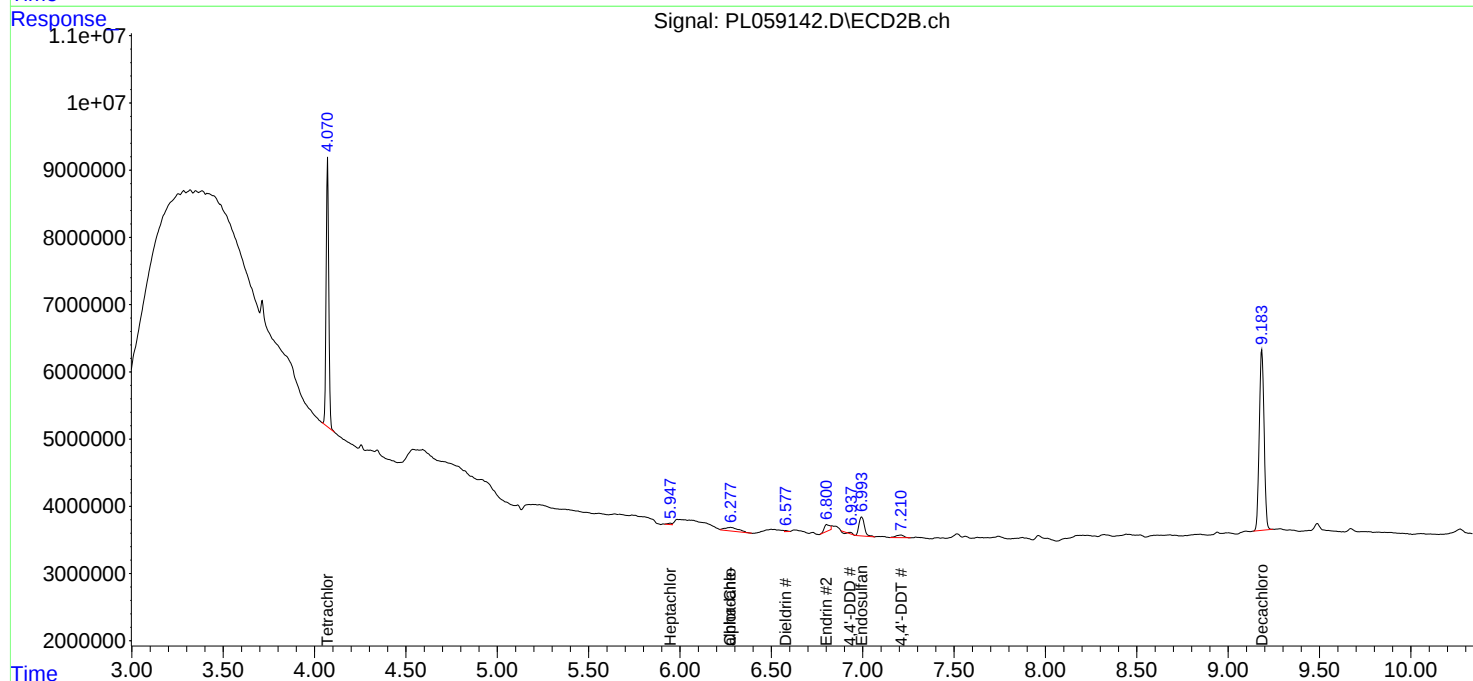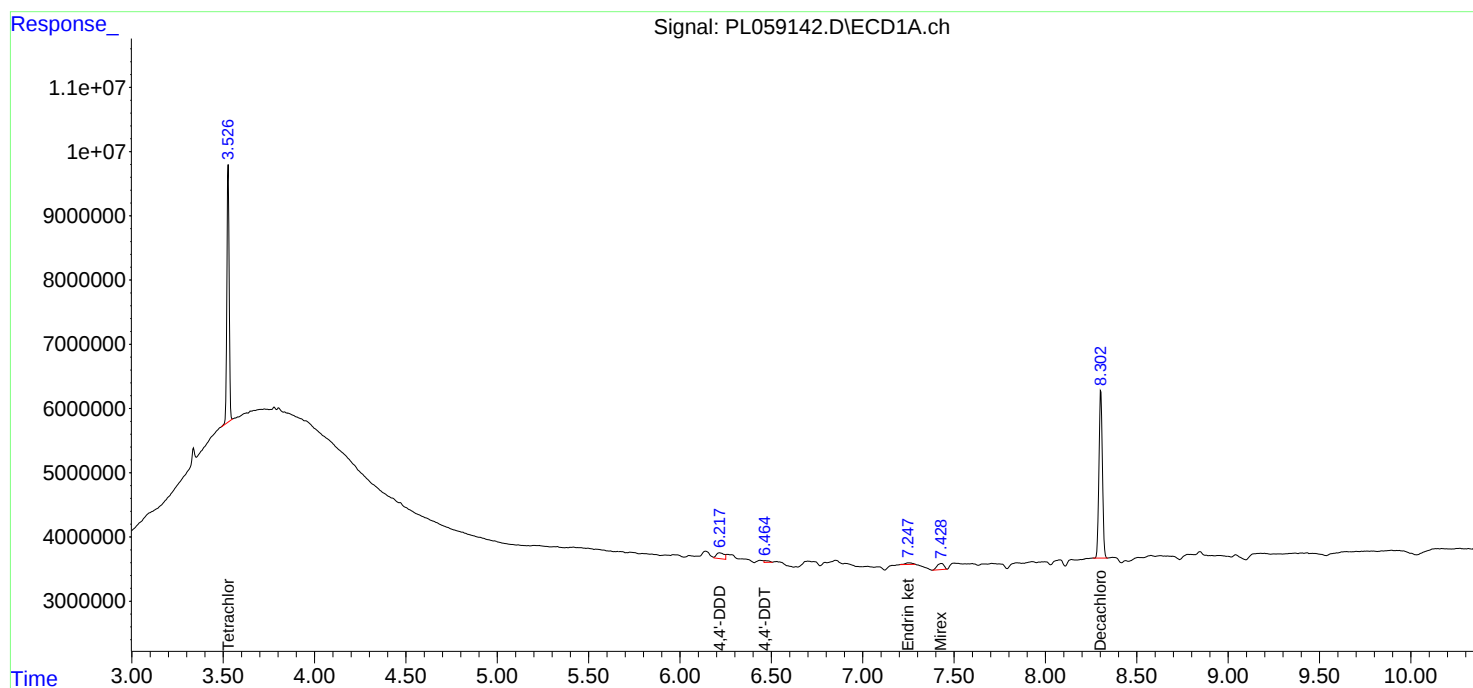


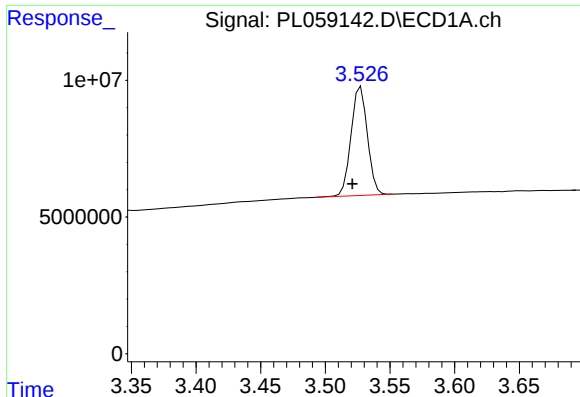

#1 Tetrachloro-m-xylene


R.T.: 3.528 min
Delta R.T.: 0.007 min
Response: 34972892
Conc: 20.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

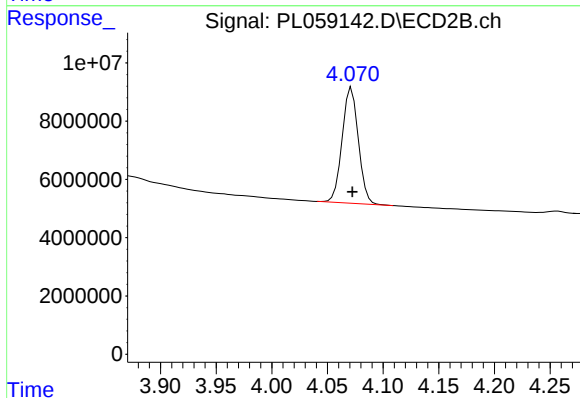


#1 Tetrachloro-m-xylene

R.T.: 4.072 min
Delta R.T.: 0.000 min
Response: 40121998
Conc: 15.42 ng/ml

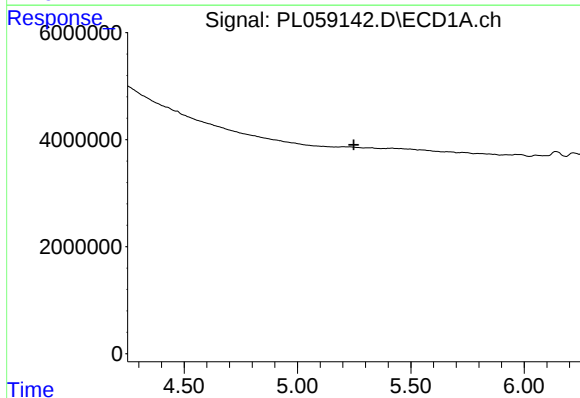


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.248 min
Response: 0
Conc: N.D.

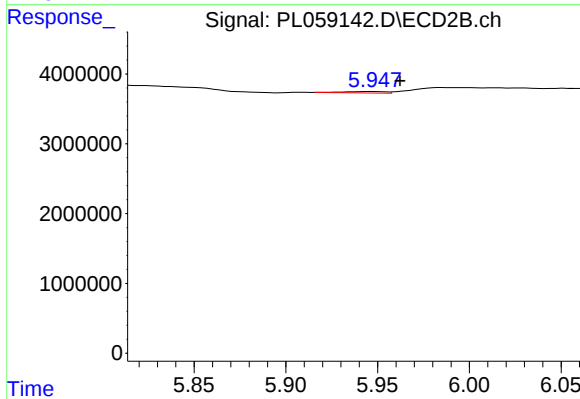

#8 Heptachlor epoxide


R.T.: 5.947 min
Delta R.T.: -0.015 min
Response: 318289
Conc: 0.11 ng/ml

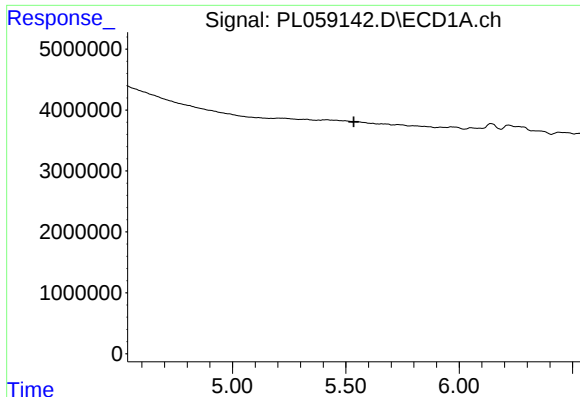

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.535 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

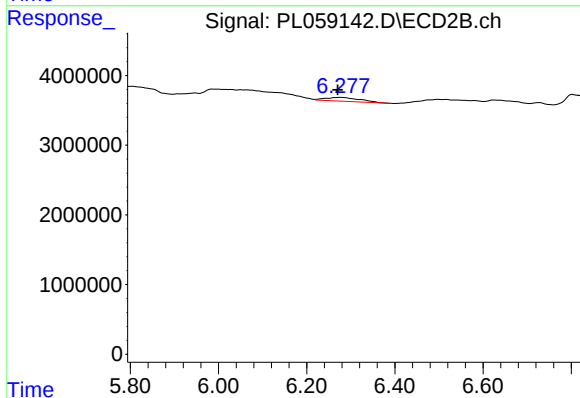


#11 alpha-Chlordane

R.T.: 6.277 min
Delta R.T.: 0.006 min
Response: 2671966
Conc: 0.88 ng/ml

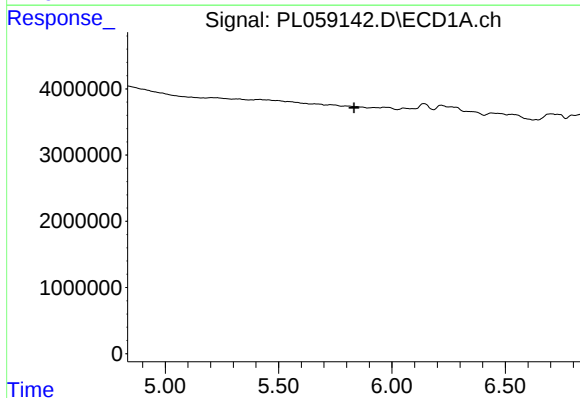


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 5.833 min
Response: 0
Conc: N.D.

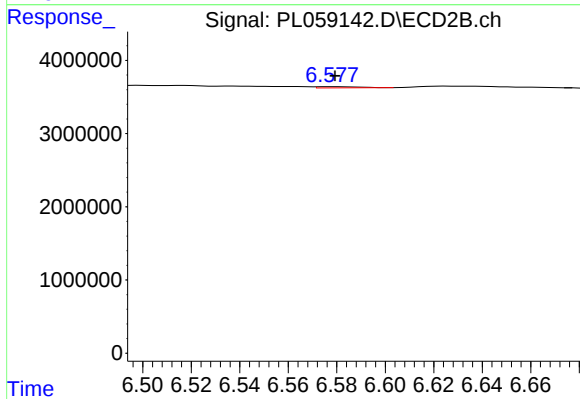

#13 Dieldrin


R.T.: 6.579 min
Delta R.T.: 0.000 min
Response: 197053
Conc: 0.07 ng/ml

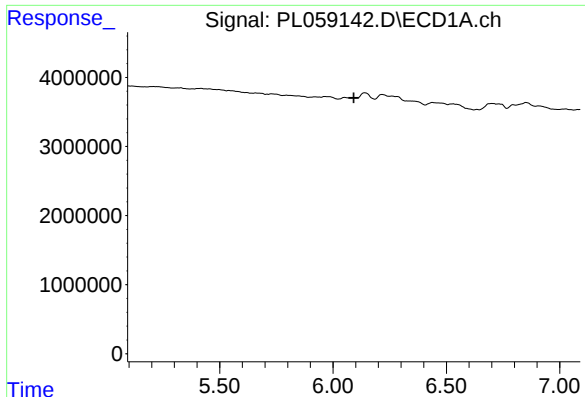

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.091 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

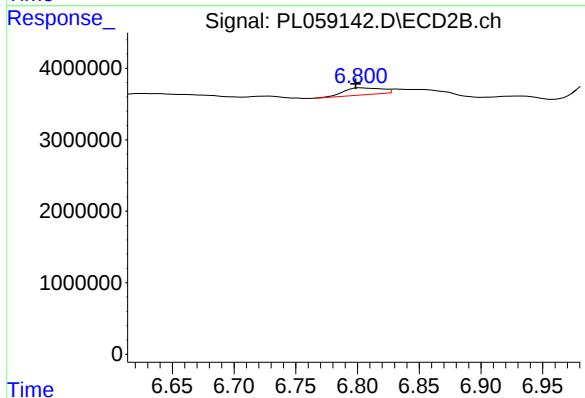


#14 Endrin

R.T.: 6.803 min
Delta R.T.: 0.004 min
Response: 2050118
Conc: 0.82 ng/ml

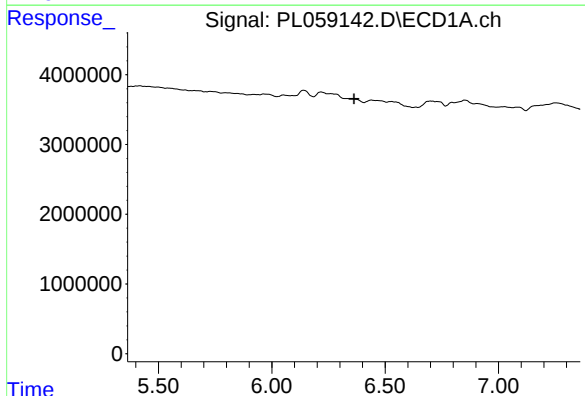


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.363 min
Response: 0
Conc: N.D.

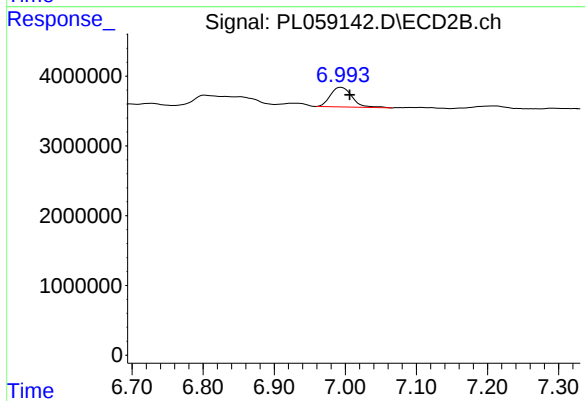

#15 Endosulfan II


R.T.: 6.994 min
Delta R.T.: -0.012 min
Response: 5935453
Conc: 2.28 ng/ml

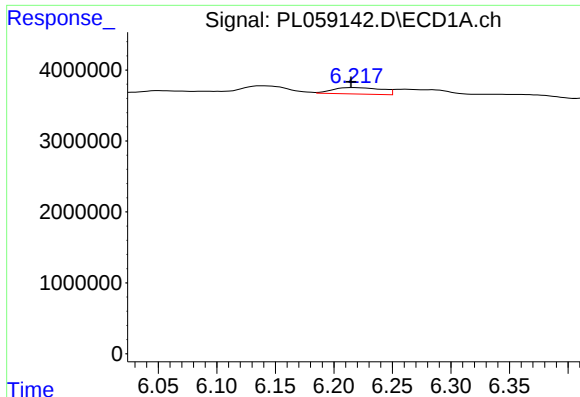

#16 4,4'-DDD


R.T.: 6.218 min
Delta R.T.: 0.003 min
Response: 2663532
Conc: 2.01 ng/ml

Instrument :
ECD_L
ClientSampleId :

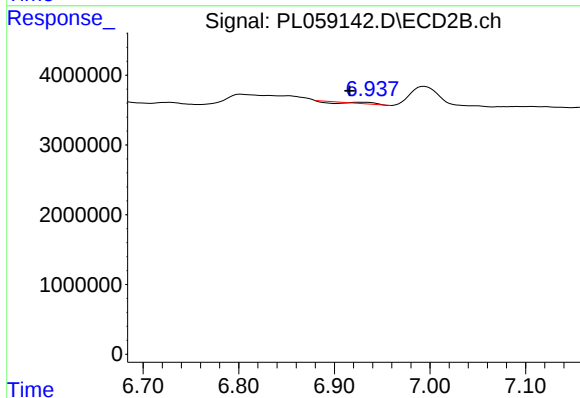


#16 4,4'-DDD

R.T.: 6.932 min
Delta R.T.: 0.016 min
Response: 117207
Conc: 0.05 ng/ml

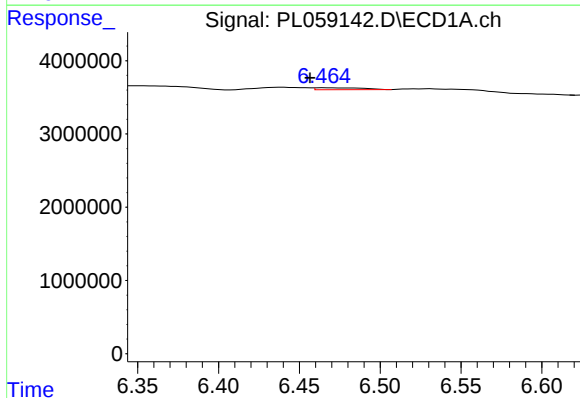


#17 4,4'-DDT

R.T.: 6.465 min
Delta R.T.: 0.008 min
Response: 534674
Conc: 0.42 ng/ml

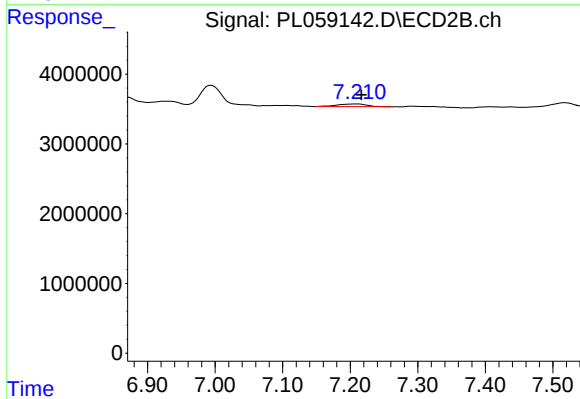

#17 4,4'-DDT


R.T.: 7.211 min
Delta R.T.: -0.006 min
Response: 1162592
Conc: 0.51 ng/ml

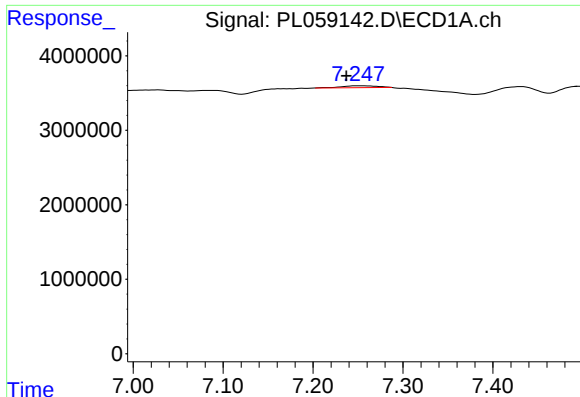

#21 Endrin ketone


R.T.: 7.249 min
Delta R.T.: 0.012 min
Response: 713032
Conc: 0.41 ng/ml

Instrument :
ECD_L
ClientSampleId :

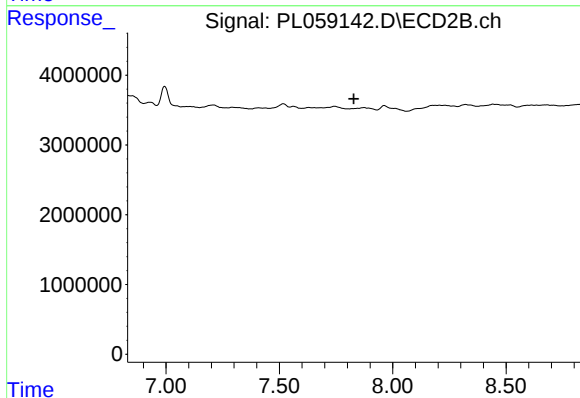


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.828 min
Response: 0
Conc: N.D.

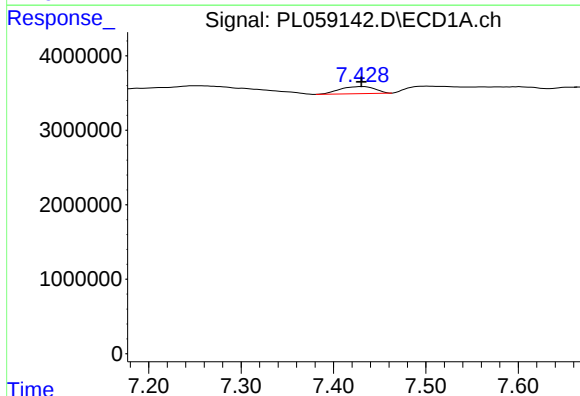


#22 Mirex

R.T.: 7.431 min
Delta R.T.: 0.000 min
Response: 2524318
Conc: 1.83 ng/ml

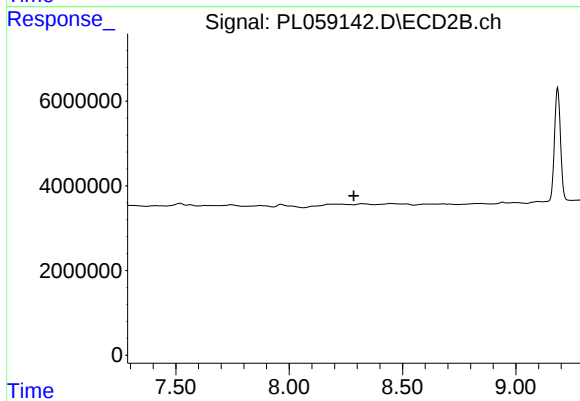

#22 Mirex


R.T.: 0.000 min
Exp R.T. : 8.285 min
Response: 0
Conc: N.D.

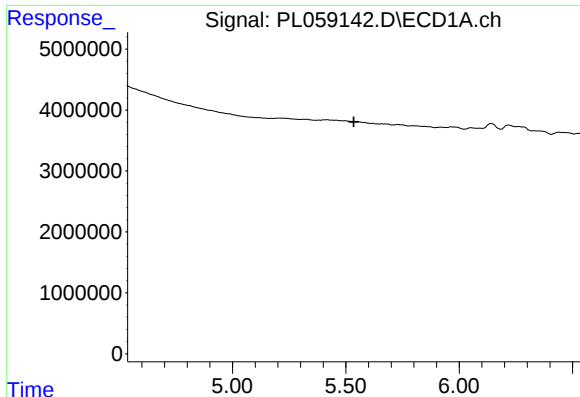

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.535 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

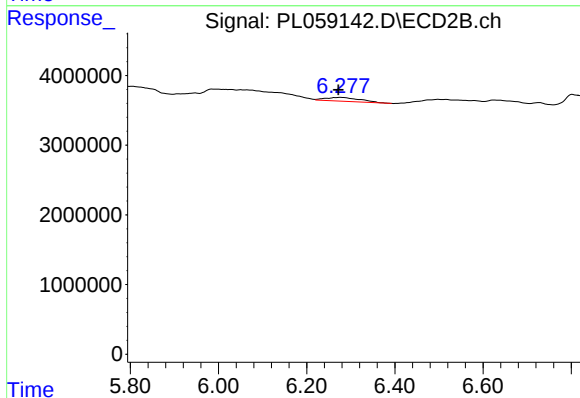


#26 Chlordane-4

R.T.: 6.277 min
Delta R.T.: 0.005 min
Response: 2671966
Conc: 5.87 ng/ml

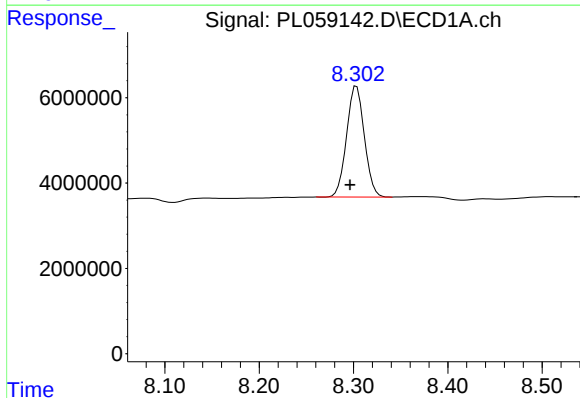

#28 Decachlorobiphenyl

R.T.: 8.303 min
Delta R.T.: 0.007 min
Response: 34119129
Conc: 20.75 ng/ml

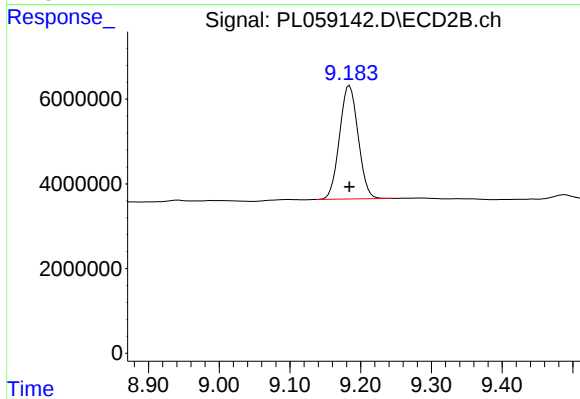

#28 Decachlorobiphenyl

R.T.: 9.184 min
Delta R.T.: 0.000 min
Response: 49036408
Conc: 20.69 ng/ml