

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060521\
 Data File : PL067105.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jun 2021 14:46
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 INDA501

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 04:57:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060521CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 07 04:55:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.016	4.899	40010141	70865510	75.961	78.947
27)	SA Decachlor...	9.234	10.437	86818054	127.6E6	136.766	138.926
Target Compounds							
2)	A alpha-BHC	4.582	5.389	66425896	101.7E6	83.466	90.580
3)	MA gamma-BHC...	4.928	5.732	57480536	96111908	80.543	88.048
4)	MA Heptachlor	5.279	6.313	54173596	85417348	78.342	79.761
9)	A Endosulfan I	6.431	7.469	47247886	68289131	76.771	80.854
13)	MA Dieldrin	6.694	7.745	107.5E6	153.6E6	160.106	170.252
14)	MA Endrin	6.964	7.975	95172464	121.9E6	155.336	166.876
16)	A 4,4'-DDD	7.119	8.107	86012695	119.1E6	160.837	170.833
17)	MA 4,4'-DDT	7.367	8.417	89665087	119.0E6	163.686	169.408
20)	A Methoxychlor	7.937	8.890	219.6E6	303.3E6	693.272	747.201


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060521\
Data File : PL067105.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jun 2021 14:46
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
INDA501

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 04:57:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060521CLP.M
Quant Title : GC Extractables
QLast Update : Mon Jun 07 04:55:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

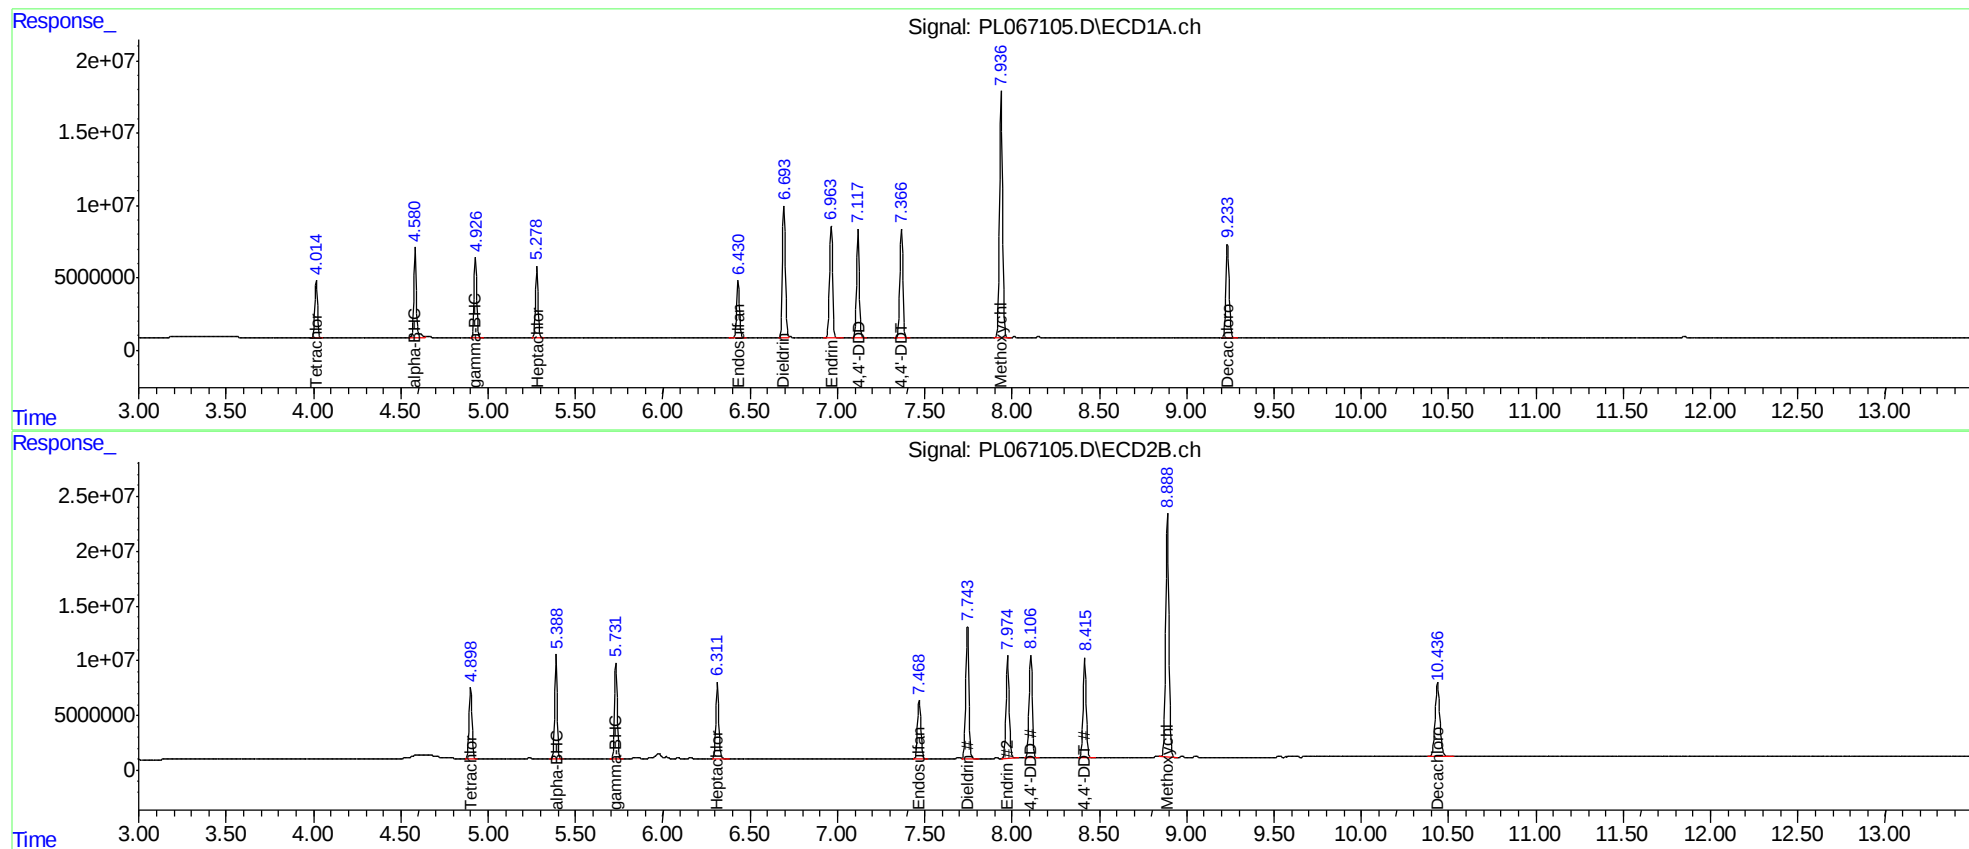


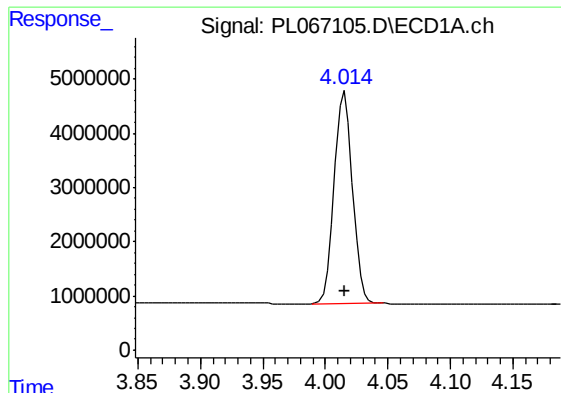

#1 Tetrachloro-m-xylene


R.T.: 4.016 min
Delta R.T.: 0.000 min
Response: 40010141
Conc: 75.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA501

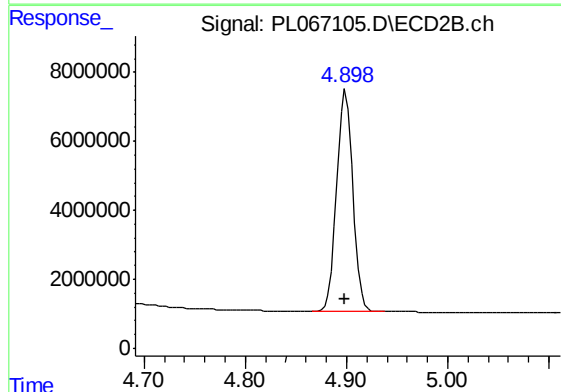


#1 Tetrachloro-m-xylene

R.T.: 4.899 min
Delta R.T.: 0.000 min
Response: 70865510
Conc: 78.95 ng/ml

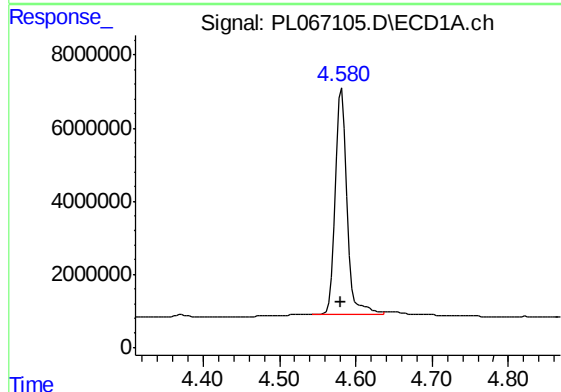


#2 alpha-BHC

R.T.: 4.582 min
Delta R.T.: 0.000 min
Response: 66425896
Conc: 83.47 ng/ml

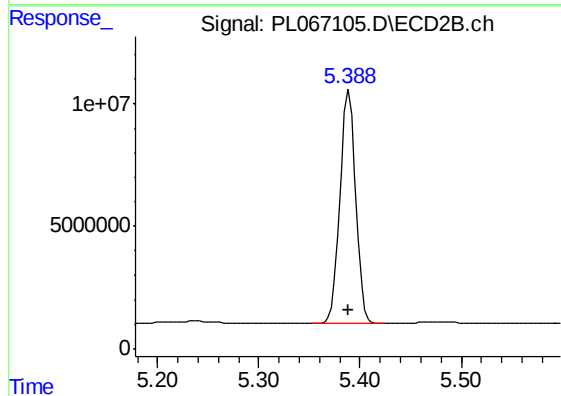

#2 alpha-BHC


R.T.: 5.389 min
Delta R.T.: 0.001 min
Response: 101676840
Conc: 90.58 ng/ml

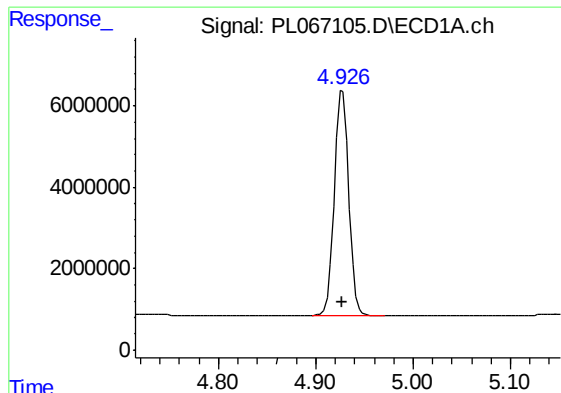

#3 gamma-BHC (Lindane)


R.T.: 4.928 min
Delta R.T.: 0.000 min
Response: 57480536
Conc: 80.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA501

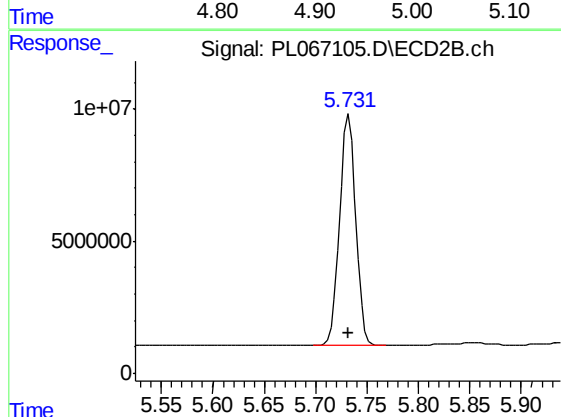


#3 gamma-BHC (Lindane)

R.T.: 5.732 min
Delta R.T.: 0.001 min
Response: 96111908
Conc: 88.05 ng/ml

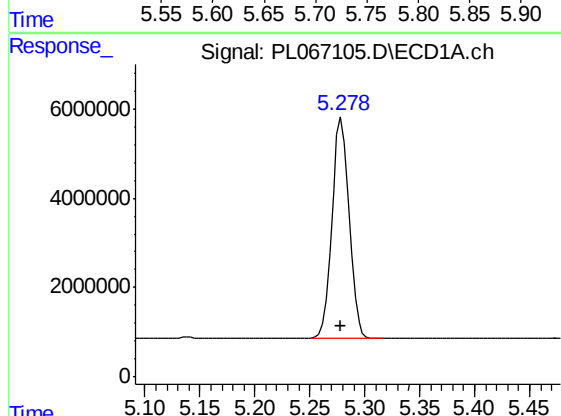


#4 Heptachlor

R.T.: 5.279 min
Delta R.T.: 0.000 min
Response: 54173596
Conc: 78.34 ng/ml

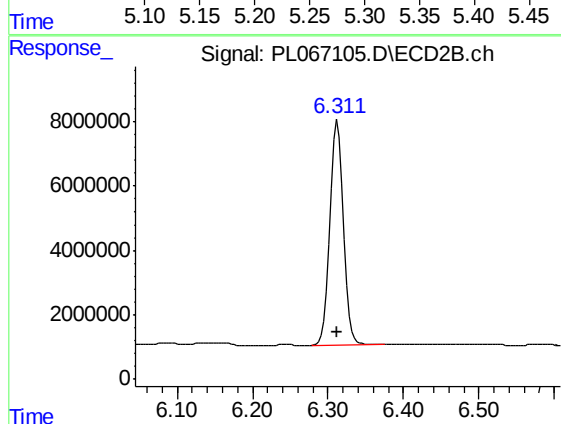

#4 Heptachlor


R.T.: 6.313 min
Delta R.T.: 0.001 min
Response: 85417348
Conc: 79.76 ng/ml

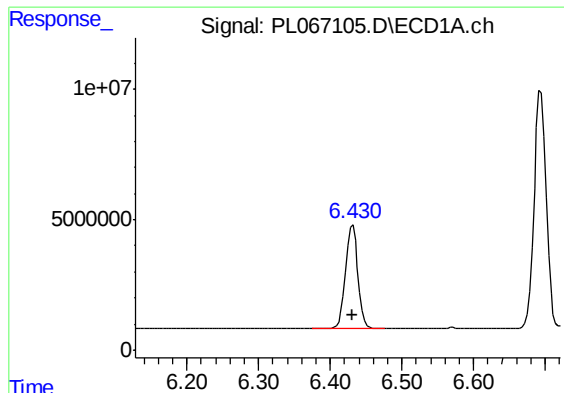

#9 Endosulfan I


R.T.: 6.431 min
Delta R.T.: 0.000 min
Response: 47247886
Conc: 76.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA501

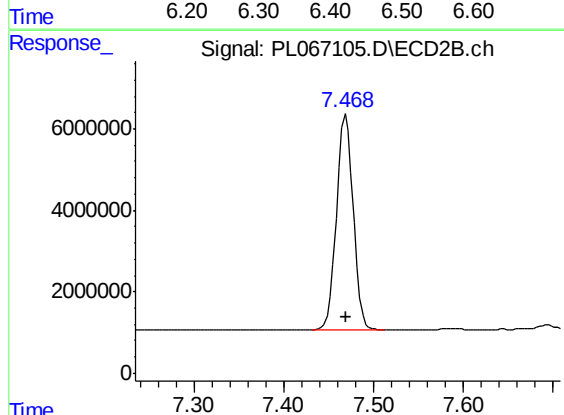


#9 Endosulfan I

R.T.: 7.469 min
Delta R.T.: 0.000 min
Response: 68289131
Conc: 80.85 ng/ml

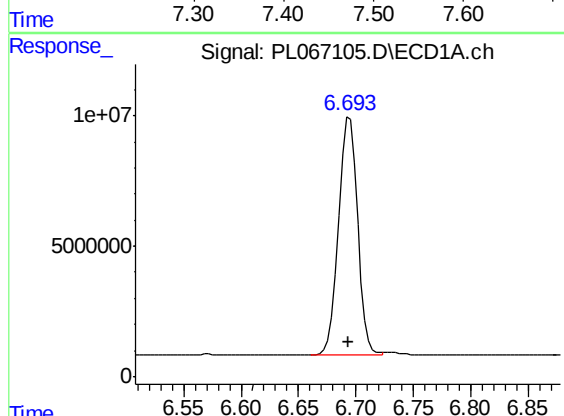


#13 Dieldrin

R.T.: 6.694 min
Delta R.T.: 0.000 min
Response: 107514743
Conc: 160.11 ng/ml

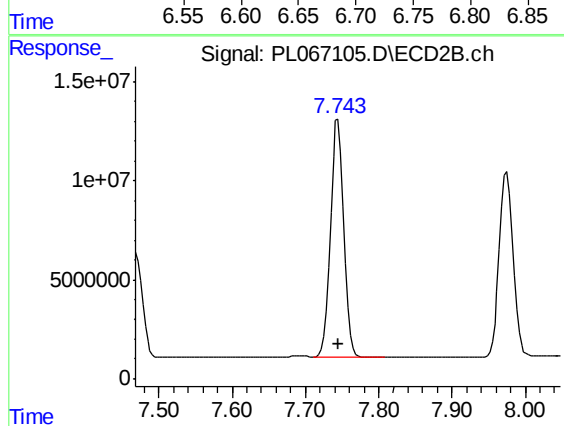

#13 Dieldrin


R.T.: 7.745 min
Delta R.T.: 0.000 min
Response: 153622582
Conc: 170.25 ng/ml

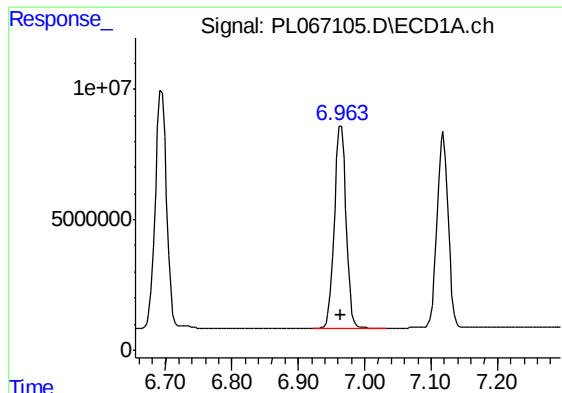

#14 Endrin


R.T.: 6.964 min
Delta R.T.: 0.000 min
Response: 95172464
Conc: 155.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA501

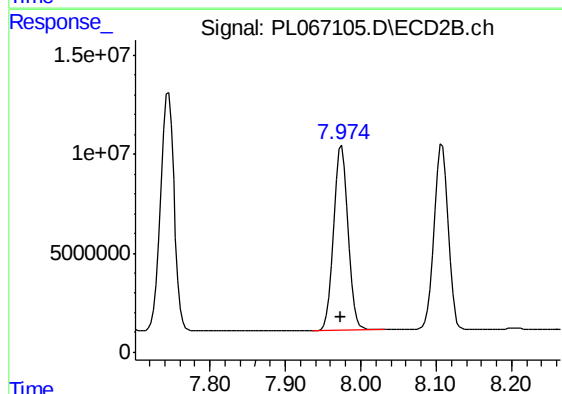


#14 Endrin

R.T.: 7.975 min
Delta R.T.: 0.000 min
Response: 121926575
Conc: 166.88 ng/ml

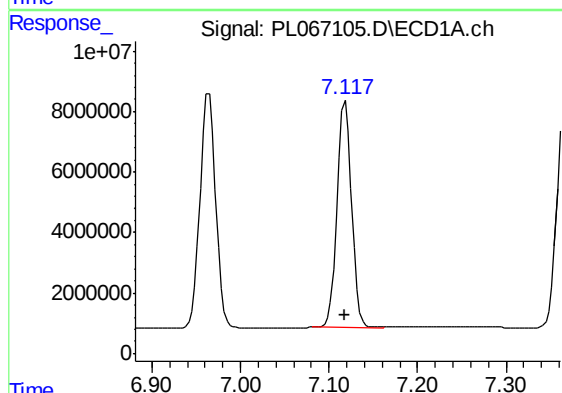


#16 4,4'-DDD

R.T.: 7.119 min
Delta R.T.: 0.000 min
Response: 86012695
Conc: 160.84 ng/ml

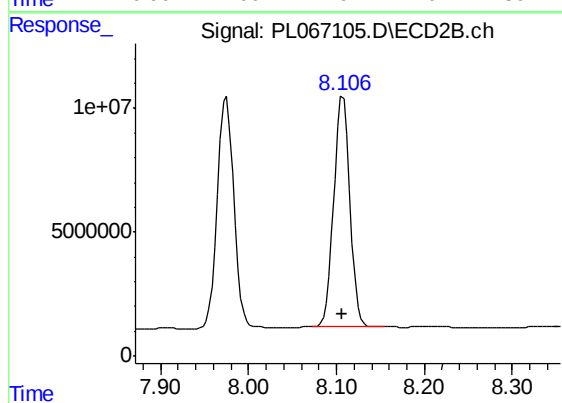

#16 4,4'-DDD


R.T.: 8.107 min
Delta R.T.: 0.001 min
Response: 119064791
Conc: 170.83 ng/ml

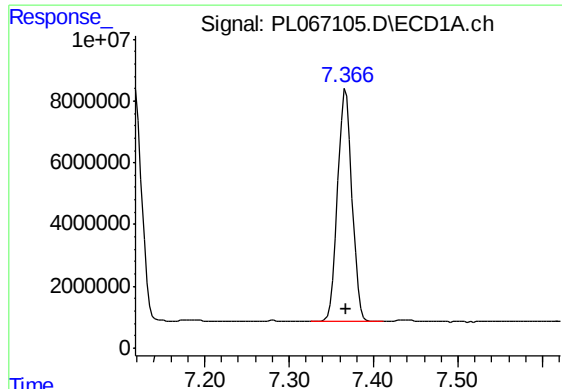

#17 4,4'-DDT


R.T.: 7.367 min
Delta R.T.: 0.000 min
Response: 89665087
Conc: 163.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA501

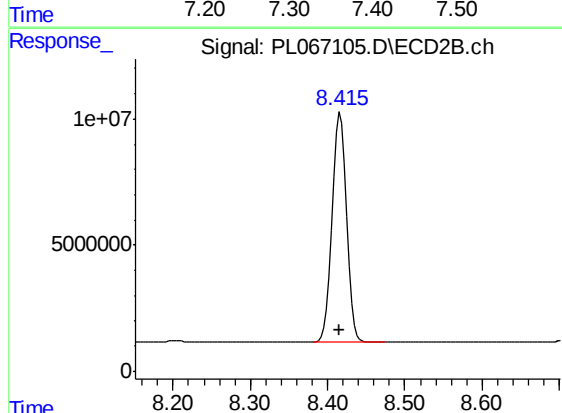


#17 4,4'-DDT

R.T.: 8.417 min
Delta R.T.: 0.001 min
Response: 119026828
Conc: 169.41 ng/ml

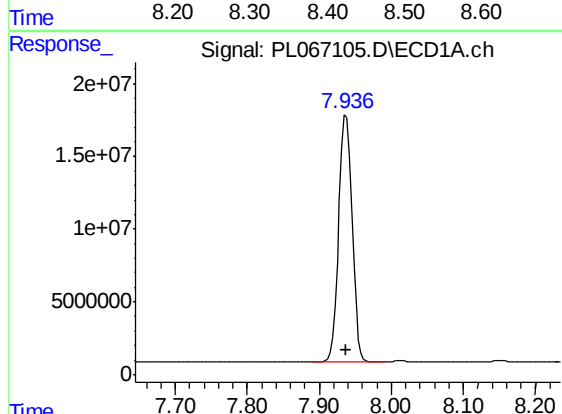


#20 Methoxychlor

R.T.: 7.937 min
Delta R.T.: 0.001 min
Response: 219586991
Conc: 693.27 ng/ml

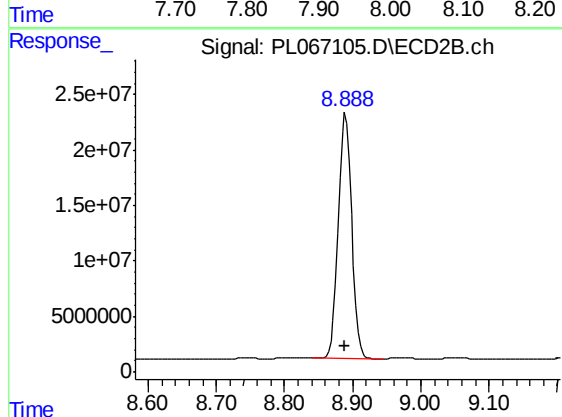

#20 Methoxychlor


R.T.: 8.890 min
Delta R.T.: 0.000 min
Response: 303303841
Conc: 747.20 ng/ml

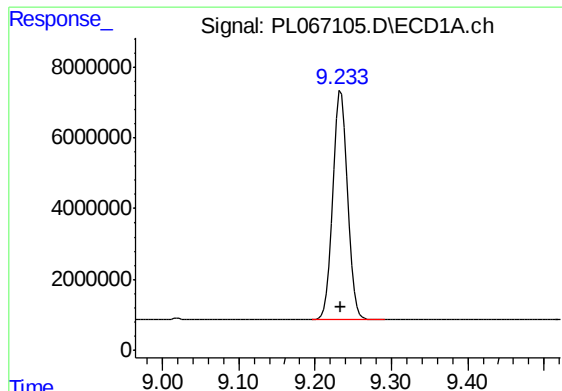

#27 Decachlorobiphenyl

R.T.: 9.234 min
Delta R.T.: 0.000 min
Response: 86818054
Conc: 136.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA501

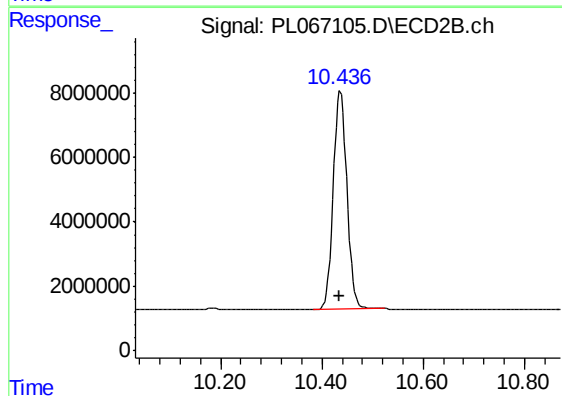

#27 Decachlorobiphenyl

R.T.: 10.437 min
Delta R.T.: 0.002 min
Response: 127616454
Conc: 138.93 ng/ml