

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060621\
 Data File : PL067120.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jun 2021 19:59
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 07:23:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060521CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 07 05:11:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.062f	0.000	608971	0	1.169	N.D. #
Target Compounds							
7)	B delta-BHC	0.000	6.159f	0	524308	N.D.	0.581
8)	B Heptachlo...	6.009f	7.083	1420569	10485784	2.252	12.489 #
9)	A Endosulfan I	6.468	0.000	270913	0	0.440	N.D. #
14)	MA Endrin	6.986	0.000	1813492	0	2.992	N.D. #
15)	B Endosulfa...	7.282	8.193	-142688	751125	N.D.	1.023
16)	A 4,4'-DDD	0.000	8.051f	0	3841441	N.D.	5.588
17)	MA 4,4'-DDT	7.360	0.000	602760	0	1.118	N.D. #
19)	B Endosulfa...	0.000	8.563	0	615921	N.D.	0.838
20)	A Methoxychlor	0.000	8.826f	0	1000314	N.D.	2.486
21)	B Endrin ke...	8.119	0.000	21523387	0	33.040	N.D. #
23)	Toxaphene-2	6.774	0.000	4858086	0	1337.043	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060621\
Data File : PL067120.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jun 2021 19:59
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 07:23:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060521CLP.M
Quant Title : GC Extractables
QLast Update : Mon Jun 07 05:11:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

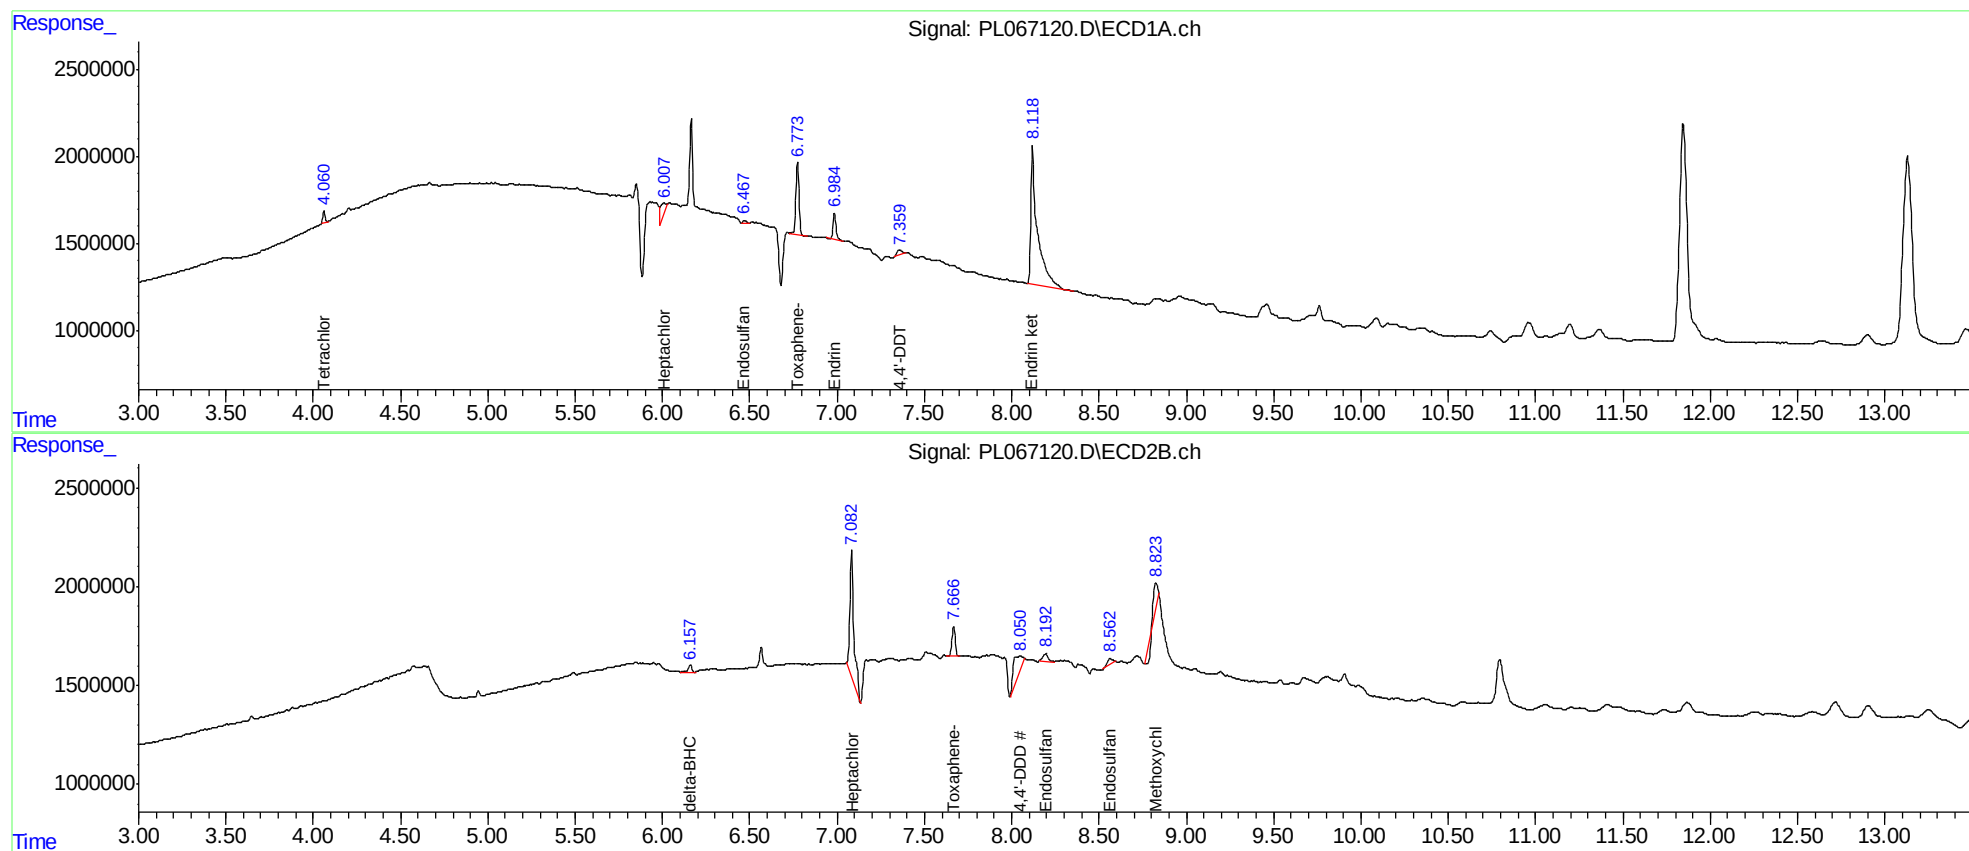


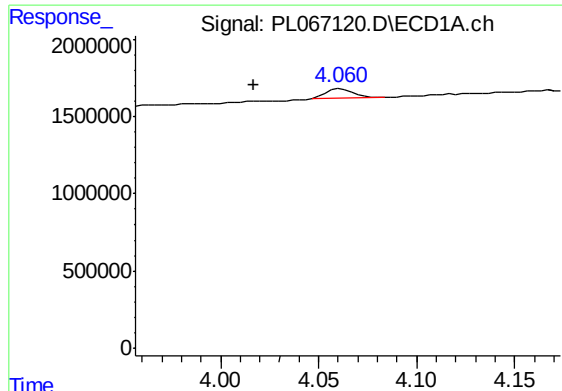

#1 Tetrachloro-m-xylene


R.T.: 4.062 min
Delta R.T.: 0.045 min
Response: 608971
Conc: 1.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

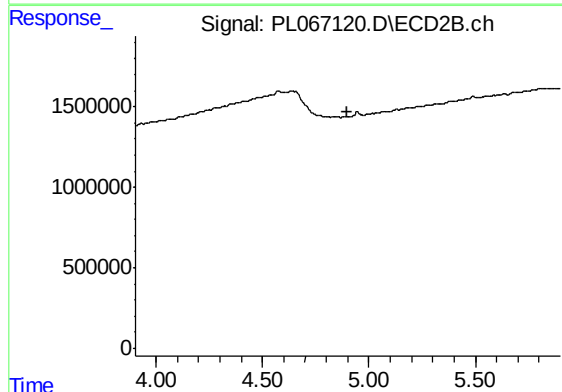


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.901 min
Response: 0
Conc: N.D.

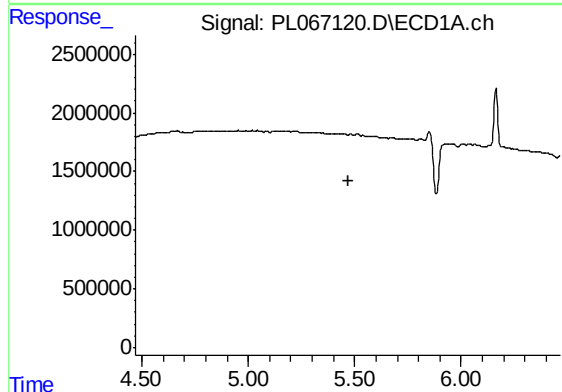


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 5.468 min
Response: 0
Conc: N.D.

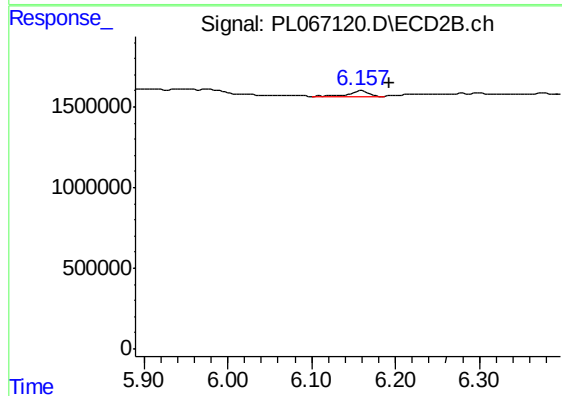

#7 delta-BHC


R.T.: 6.159 min
Delta R.T.: -0.034 min
Response: 524308
Conc: 0.58 ng/ml

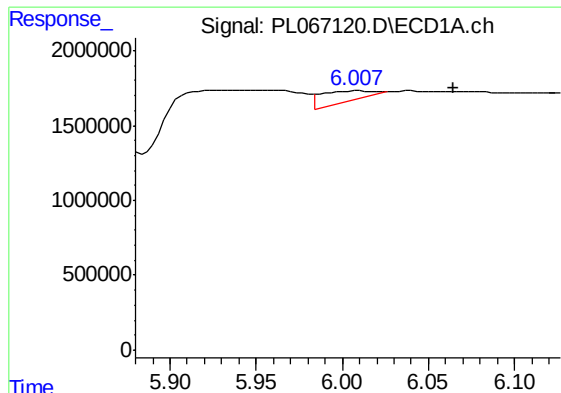

#8 Heptachlor epoxide


R.T.: 6.009 min
Delta R.T.: -0.056 min
Response: 1420569
Conc: 2.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

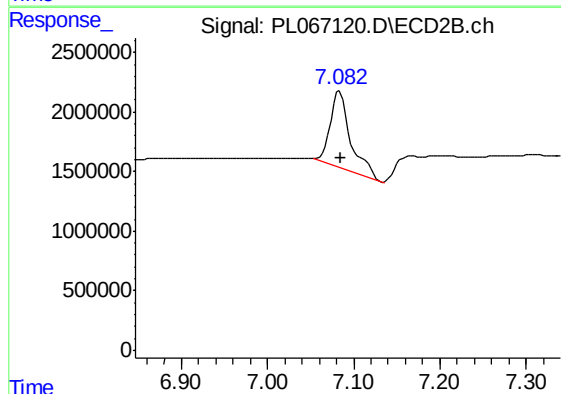


#8 Heptachlor epoxide

R.T.: 7.083 min
Delta R.T.: -0.001 min
Response: 10485784
Conc: 12.49 ng/ml

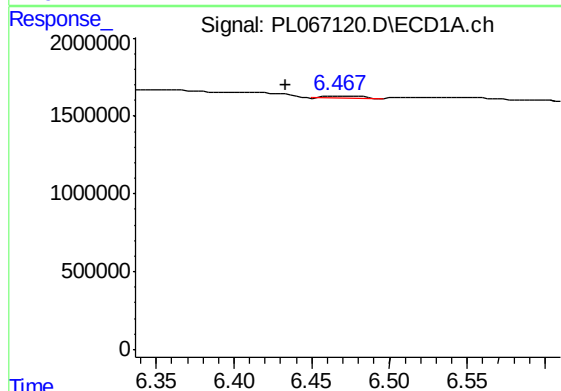


#9 Endosulfan I

R.T.: 6.468 min
Delta R.T.: 0.034 min
Response: 270913
Conc: 0.44 ng/ml

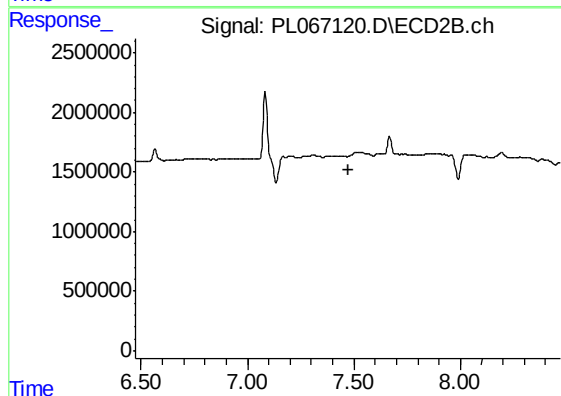

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 7.472 min
Response: 0
Conc: N.D.

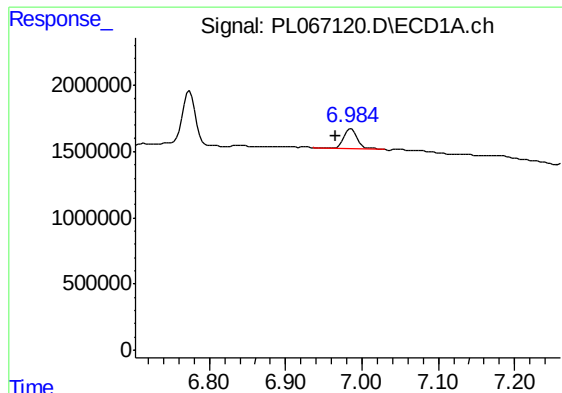

#14 Endrin


R.T.: 6.986 min
Delta R.T.: 0.019 min
Response: 1813492
Conc: 2.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

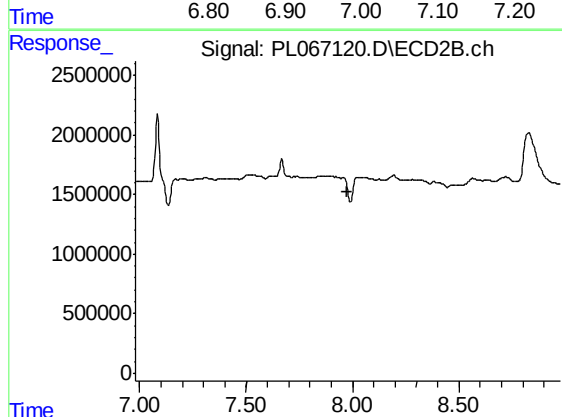


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 7.978 min
Response: 0
Conc: N.D.

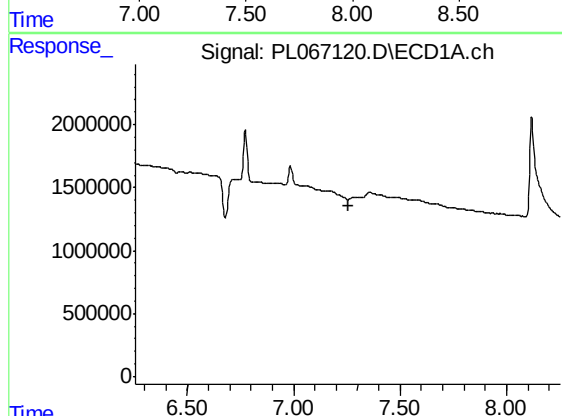


#15 Endosulfan II

R.T.: 7.282 min
Delta R.T.: 0.027 min
Response: -142688
Conc: N.D.

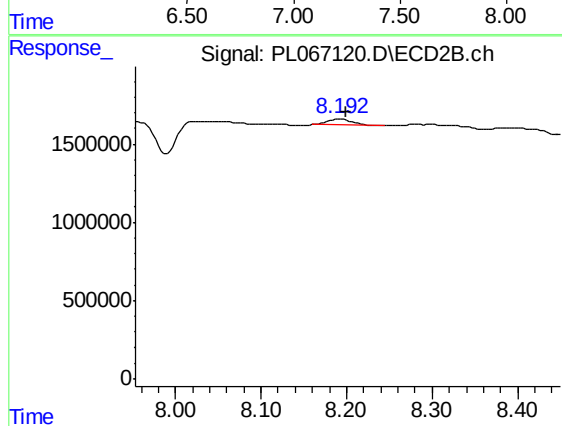

#15 Endosulfan II


R.T.: 8.193 min
Delta R.T.: -0.006 min
Response: 751125
Conc: 1.02 ng/ml

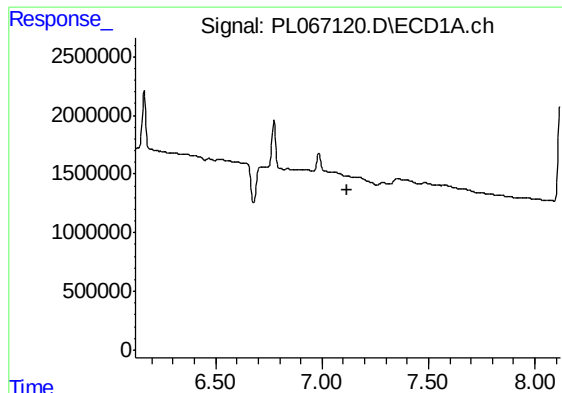

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 7.121 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

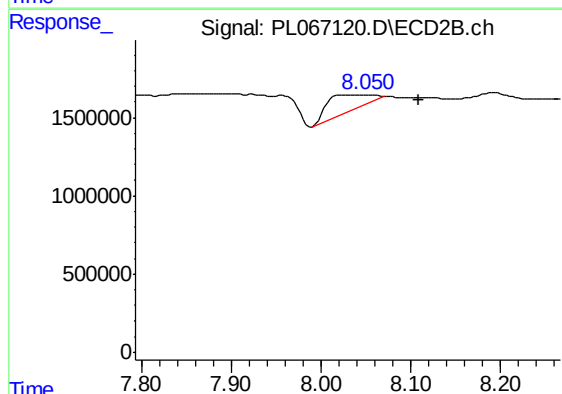


#16 4,4'-DDD

R.T.: 8.051 min
Delta R.T.: -0.059 min
Response: 3841441
Conc: 5.59 ng/ml

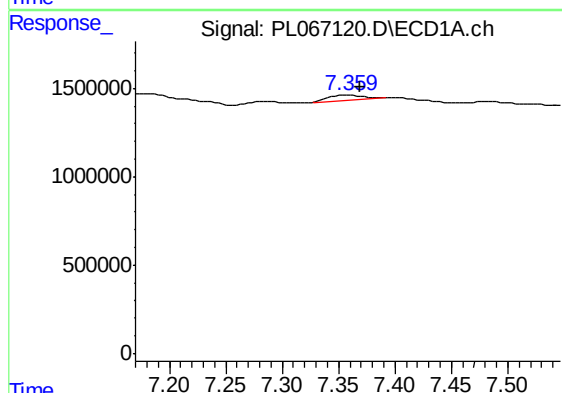


#17 4,4'-DDT

R.T.: 7.360 min
Delta R.T.: -0.009 min
Response: 602760
Conc: 1.12 ng/ml

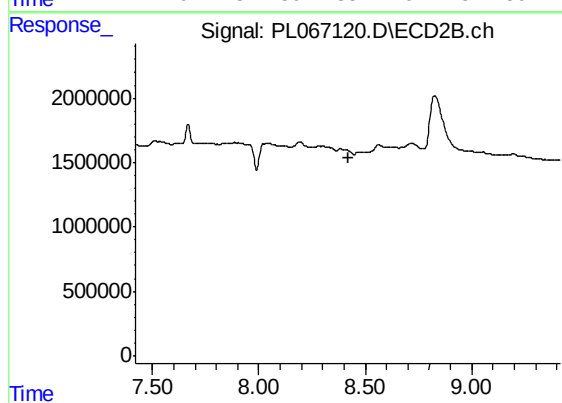

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 8.419 min
Response: 0
Conc: N.D.

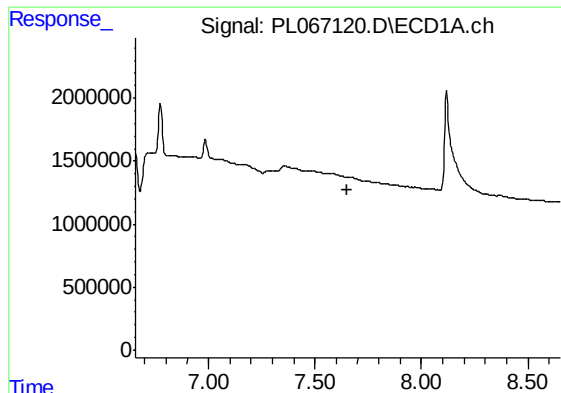

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.654 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

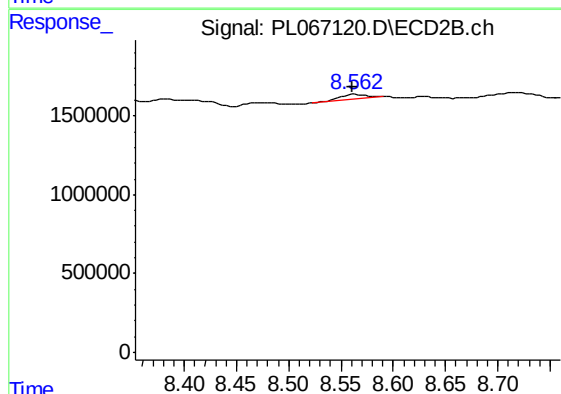


#19 Endosulfan Sulfate

R.T.: 8.563 min
Delta R.T.: 0.003 min
Response: 615921
Conc: 0.84 ng/ml

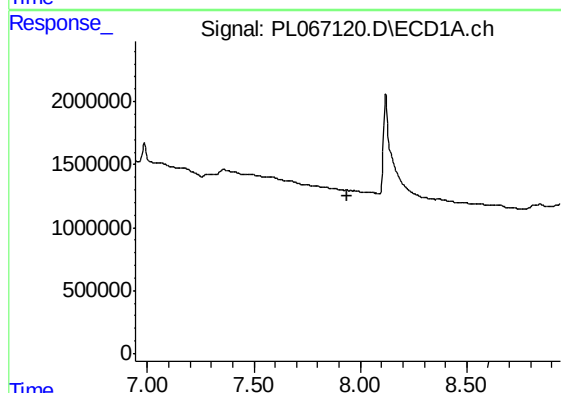


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.940 min
Response: 0
Conc: N.D.

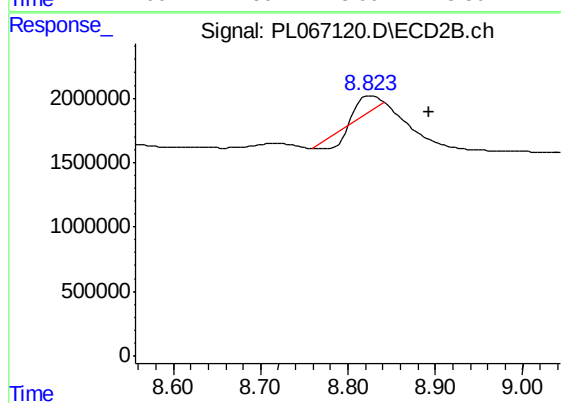

#20 Methoxychlor


R.T.: 8.826 min
Delta R.T.: -0.067 min
Response: 1000314
Conc: 2.49 ng/ml

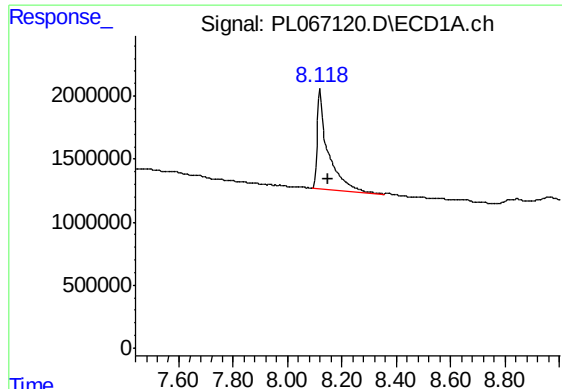

#21 Endrin ketone


R.T.: 8.119 min
Delta R.T.: -0.032 min
Response: 21523387
Conc: 33.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

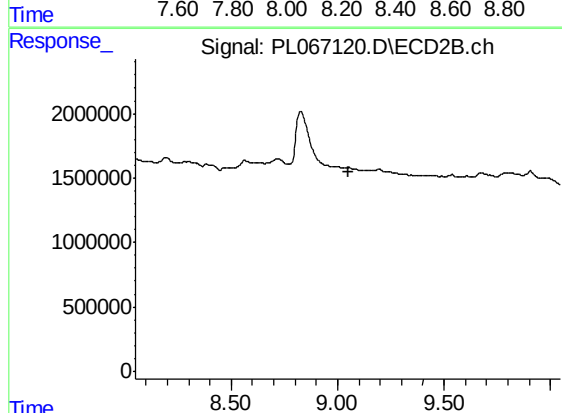


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.050 min
Response: 0
Conc: N.D.

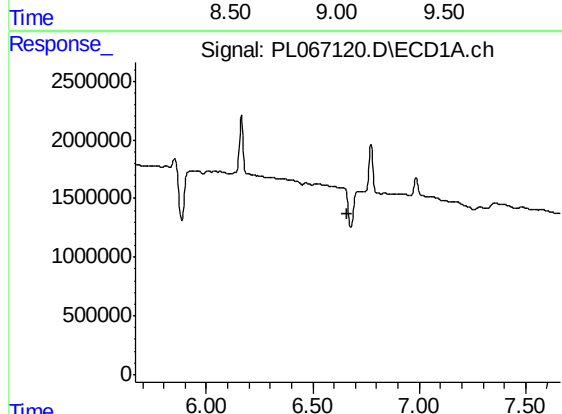


#22 Toxaphene-1

R.T.: 6.714 min
Delta R.T.: 0.049 min
Response: -1508567
Conc: N.D.

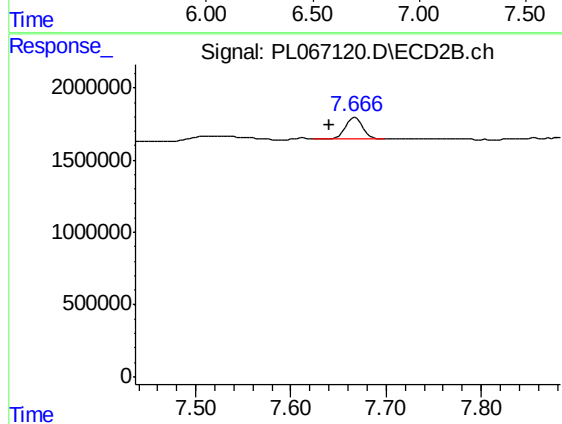

#22 Toxaphene-1


R.T.: 7.668 min
Delta R.T.: 0.027 min
Response: 1814148
Conc: 427.81 ng/ml

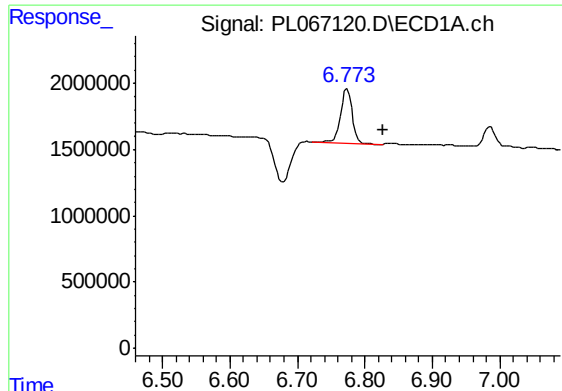

#23 Toxaphene-2


R.T.: 6.774 min
Delta R.T.: -0.052 min
Response: 4858086
Conc: 1337.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

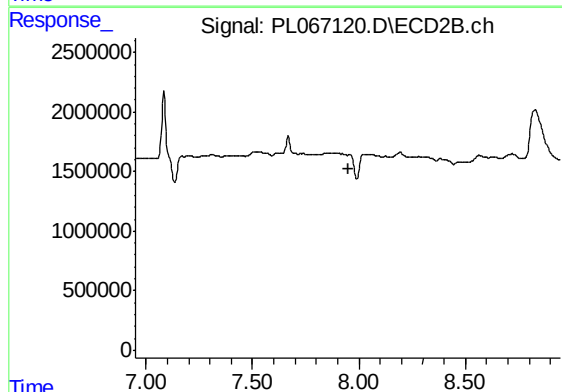


#23 Toxaphene-2

R.T.: 0.000 min
Exp R.T. : 7.950 min
Response: 0
Conc: N.D.

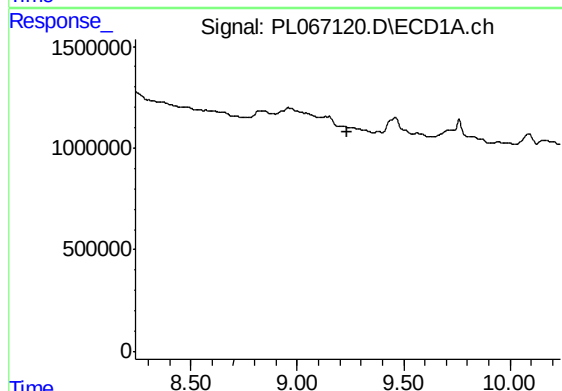

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.237 min
Response: 0
Conc: N.D.

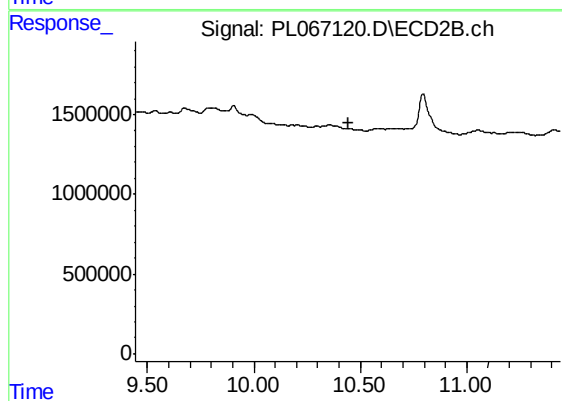

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.442 min
Response: 0
Conc: N.D.