

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060523\
 Data File : PL083221.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jun 2023 16:18
 Operator : AR\AJ
 Sample : PEM
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 21:13:13 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051923.M
 Quant Title : GC Extractables
 QLast Update : Sat May 20 04:58:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.316	2.635	51646515	45845398	17.573	17.659
28)	SA Decachlor...	8.737	7.740	39075350	42522370	18.631	17.101
Target Compounds							
2)	A alpha-BHC	3.765	3.131	35967616	29334748	8.102	7.861
3)	MA gamma-BHC...	4.094	3.457	35531178	27328682	8.576	8.199
5)	MB Aldrin	0.000	4.087f	0	261306	N.D.	0.080 #
6)	B beta-BHC	4.298	3.759	17997797	14379556	9.559	10.055
7)	B delta-BHC	0.000	3.981	0	112045	N.D.	0.034 #
8)	B Heptachlo...	5.437	0.000	601099	0	0.188	N.D. #
9)	A Endosulfan I	5.834	4.940	58154	46316	0.019	0.017
10)	B gamma-Chl...	5.706	4.822	576032	550963	0.181	0.183
11)	B alpha-Chl...	5.773	4.853f	162618	84916	0.051	0.028 #
12)	B 4,4'-DDE	0.000	5.070	0	153800	N.D.	0.063 #
13)	MA Dieldrin	6.091	5.193	216858	116174	0.072	0.041 #
14)	MA Endrin	6.318	5.471	108.7E6	99997748	40.441	39.416
16)	A 4,4'-DDD	6.463	5.622	3413631	3000216	1.571	1.560
17)	MA 4,4'-DDT	6.774	5.870	210.9E6	192.9E6	84.244	86.485
18)	B Endrin al...	6.671	5.948	2860882	2867920	1.423	1.450
19)	B Endosulfa...	0.000	6.167	0	338539	N.D.	0.138 #
20)	A Methoxychlor	7.255	6.449	278.2E6	261.8E6	210.346	205.875
21)	B Endrin ke...	7.385	6.674	4600030	5711085	1.803	2.112
25)	Chlordane-3	5.706f	4.822	576032	550963	1.388	2.067 #
26)	Chlordane-4	5.773	4.853f	162618	84916	0.321	0.301
27)	Chlordane-5	0.000	5.785	0	253845	N.D.	2.613 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060523\
Data File : PL083221.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jun 2023 16:18
Operator : AR\AJ
Sample : PEM
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 21:13:13 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051923.M
Quant Title : GC Extractables
QLast Update : Sat May 20 04:58:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

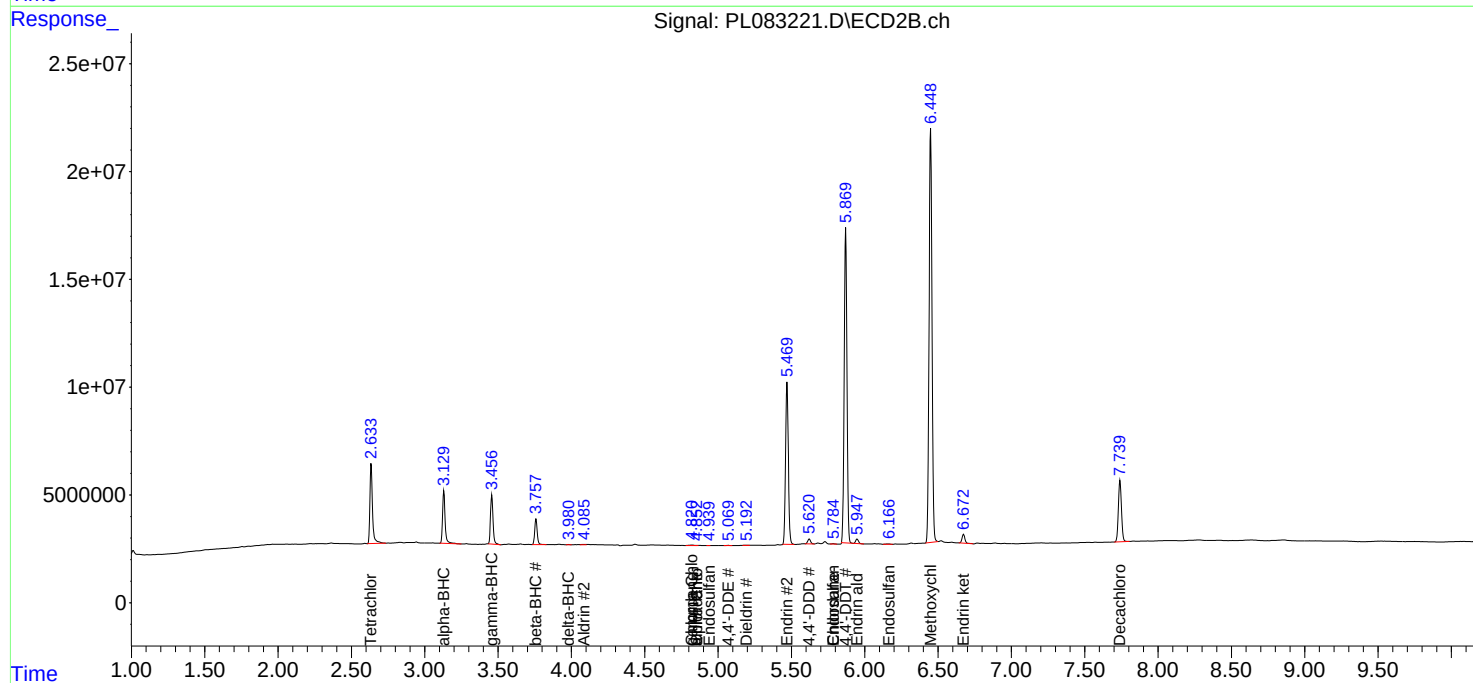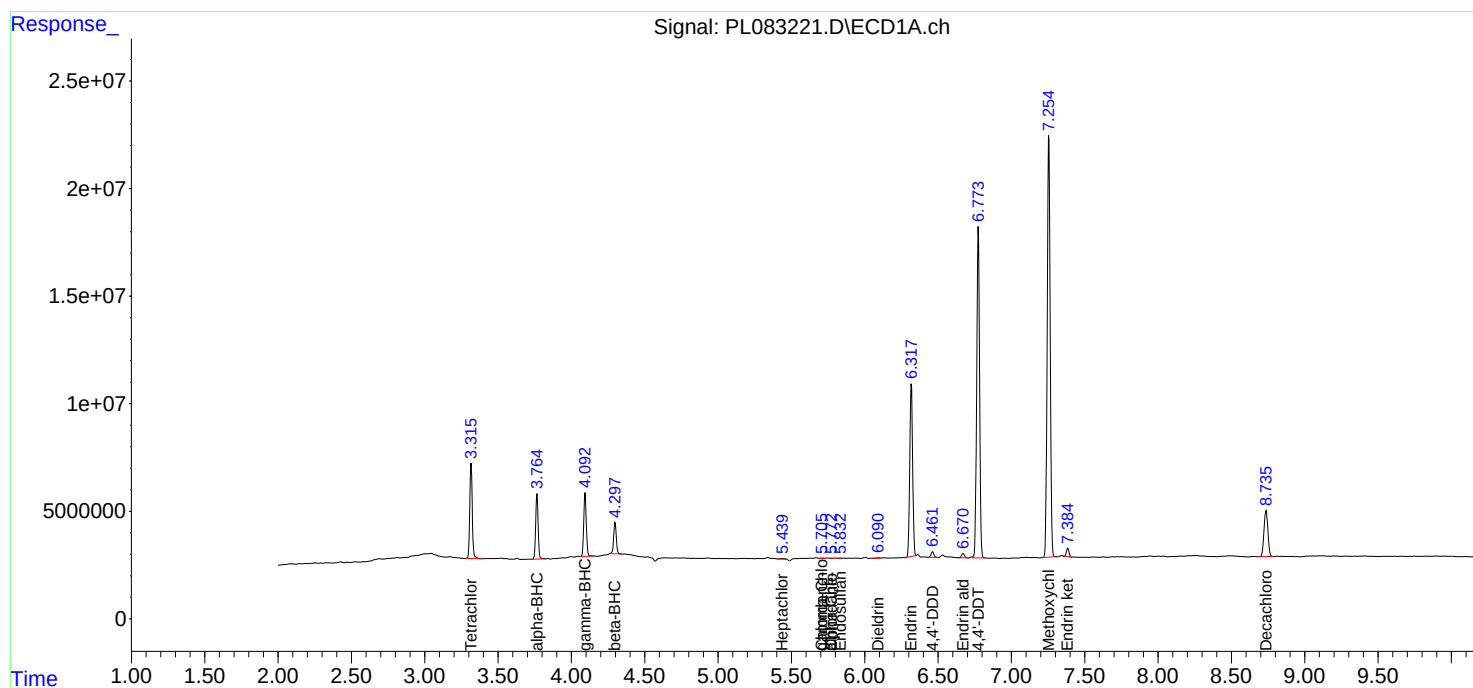


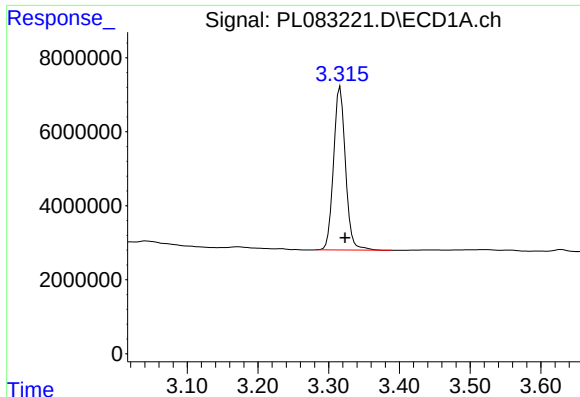

#1 Tetrachloro-m-xylene


R.T.: 3.316 min
Delta R.T.: -0.007 min
Response: 51646515
Conc: 17.57 ng/ml

Instrument :
ECD_L
ClientSampleId :

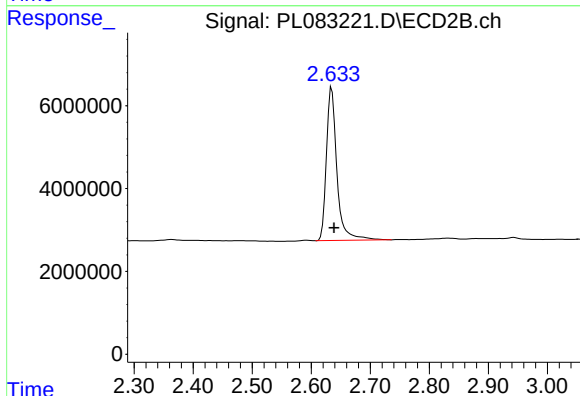


#1 Tetrachloro-m-xylene

R.T.: 2.635 min
Delta R.T.: -0.004 min
Response: 45845398
Conc: 17.66 ng/ml

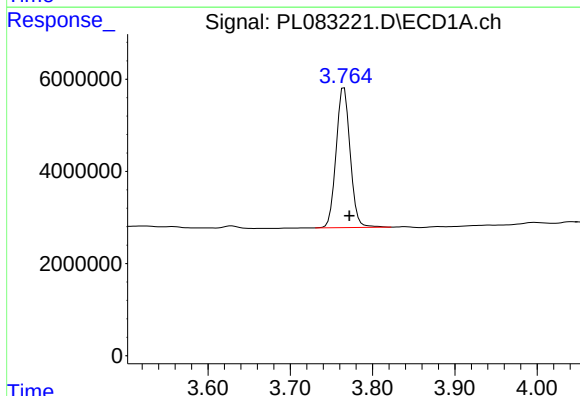


#2 alpha-BHC

R.T.: 3.765 min
Delta R.T.: -0.007 min
Response: 35967616
Conc: 8.10 ng/ml

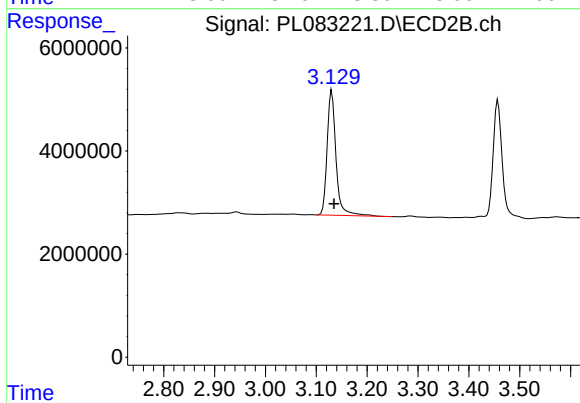

#2 alpha-BHC


R.T.: 3.131 min
Delta R.T.: -0.005 min
Response: 29334748
Conc: 7.86 ng/ml

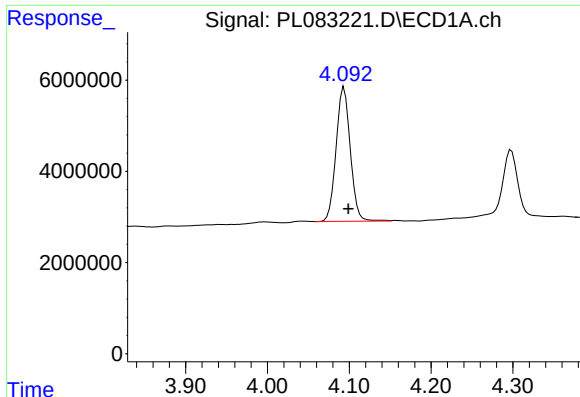

#3 gamma-BHC (Lindane)


R.T.: 4.094 min
Delta R.T.: -0.005 min
Response: 35531178
Conc: 8.58 ng/ml

Instrument :
ECD_L
ClientSampleId :

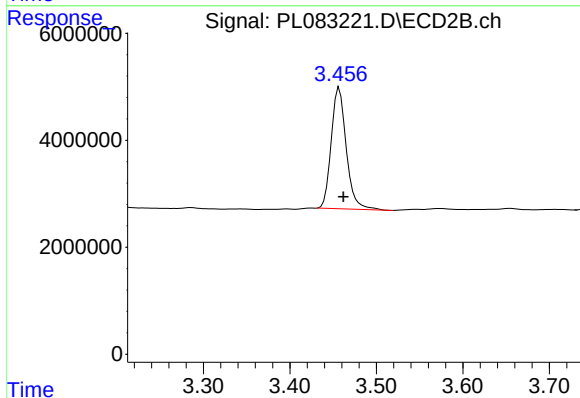


#3 gamma-BHC (Lindane)

R.T.: 3.457 min
Delta R.T.: -0.005 min
Response: 27328682
Conc: 8.20 ng/ml

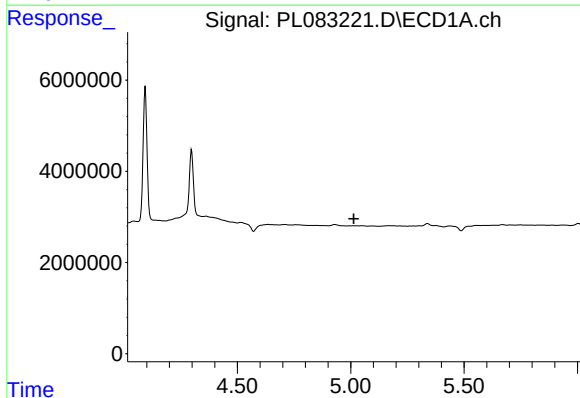


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.014 min
Response: 0
Conc: N.D.

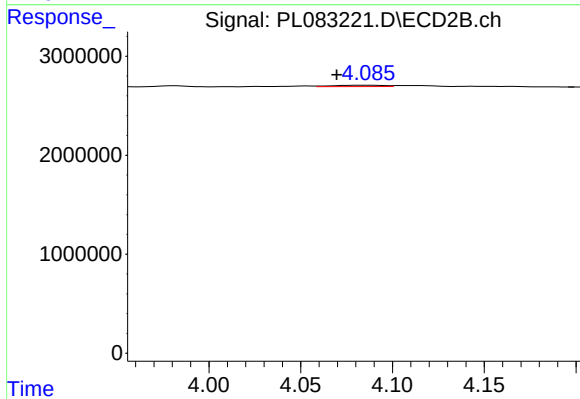

#5 Aldrin


R.T.: 4.087 min
Delta R.T.: 0.017 min
Response: 261306
Conc: 0.08 ng/ml

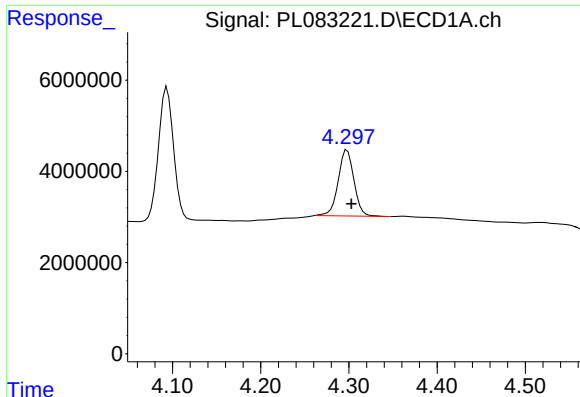

#6 beta-BHC


R.T.: 4.298 min
Delta R.T.: -0.005 min
Response: 17997797
Conc: 9.56 ng/ml

Instrument :
ECD_L
ClientSampleId :

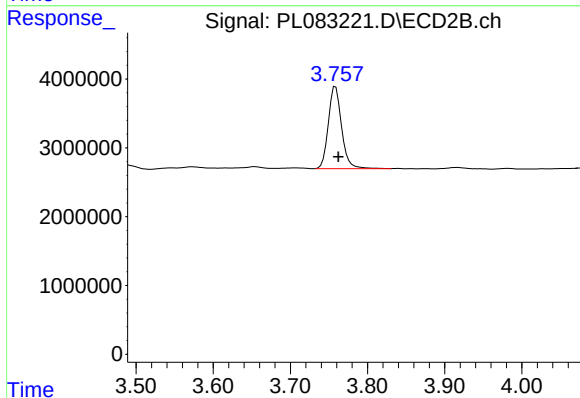


#6 beta-BHC

R.T.: 3.759 min
Delta R.T.: -0.004 min
Response: 14379556
Conc: 10.06 ng/ml

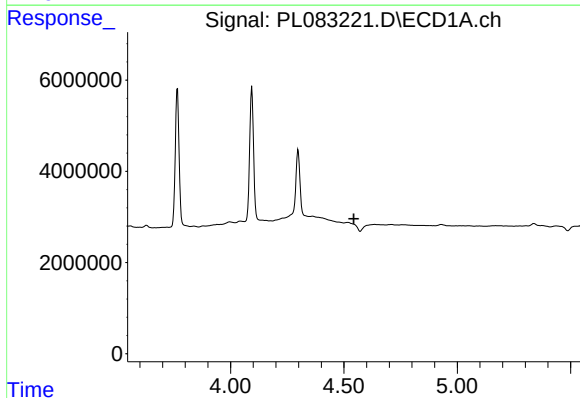


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.544 min
Response: 0
Conc: N.D.

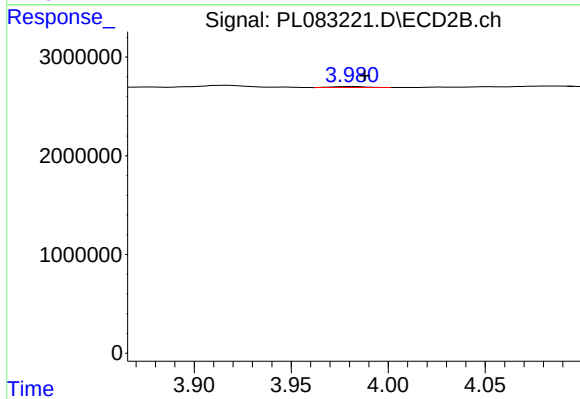

#7 delta-BHC


R.T.: 3.981 min
Delta R.T.: -0.007 min
Response: 112045
Conc: 0.03 ng/ml

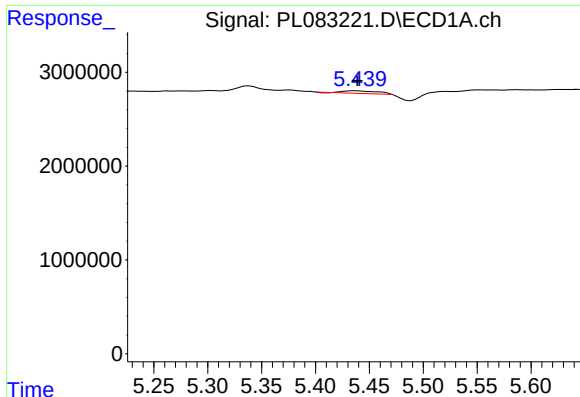

#8 Heptachlor epoxide


R.T.: 5.437 min
Delta R.T.: -0.002 min
Response: 601099
Conc: 0.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

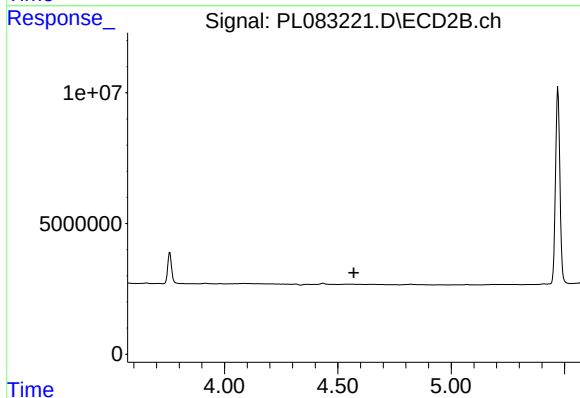


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.570 min
Response: 0
Conc: N.D.

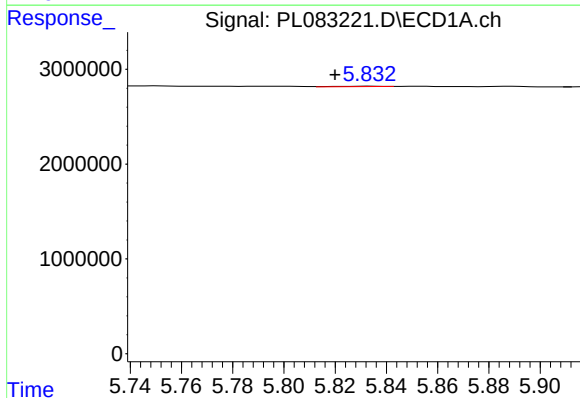


#9 Endosulfan I

R.T.: 5.834 min
Delta R.T.: 0.014 min
Response: 58154
Conc: 0.02 ng/ml

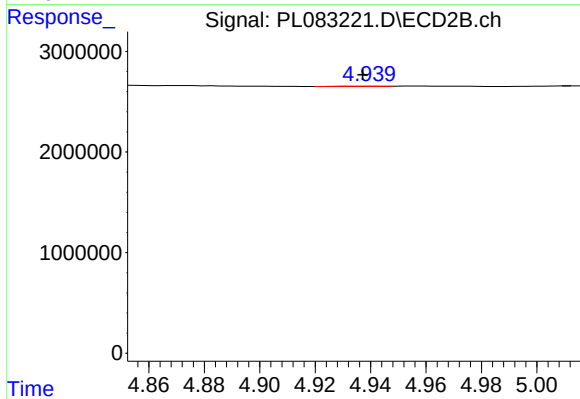

#9 Endosulfan I


R.T.: 4.940 min
Delta R.T.: 0.003 min
Response: 46316
Conc: 0.02 ng/ml

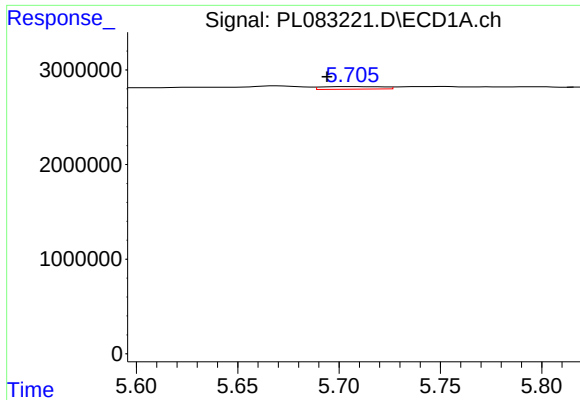

#10 gamma-Chlordane


R.T.: 5.706 min
Delta R.T.: 0.012 min
Response: 576032
Conc: 0.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

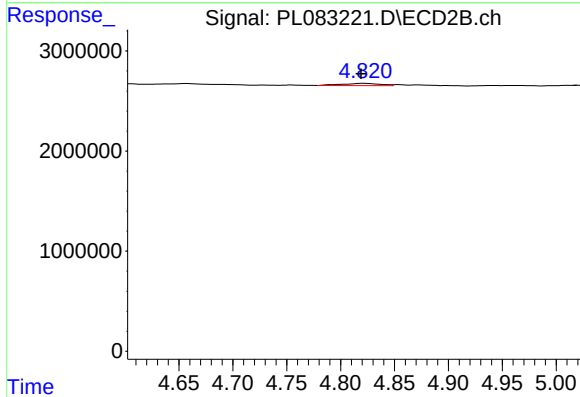


#10 gamma-Chlordane

R.T.: 4.822 min
Delta R.T.: 0.003 min
Response: 550963
Conc: 0.18 ng/ml

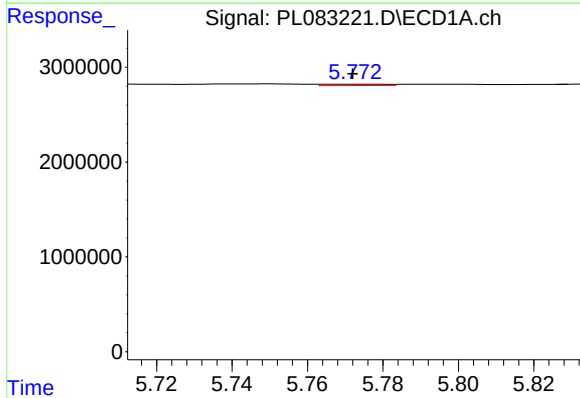


#11 alpha-Chlordane

R.T.: 5.773 min
Delta R.T.: 0.001 min
Response: 162618
Conc: 0.05 ng/ml

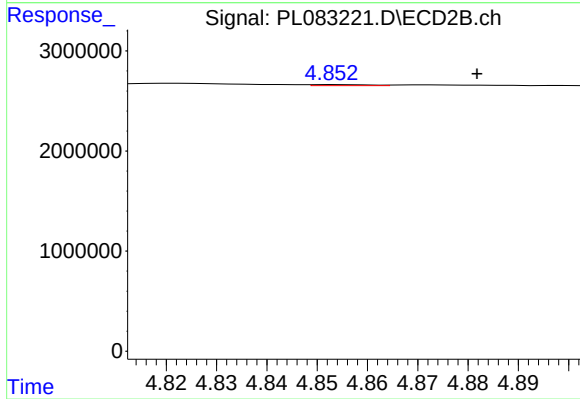

#11 alpha-Chlordane


R.T.: 4.853 min
Delta R.T.: -0.029 min
Response: 84916
Conc: 0.03 ng/ml

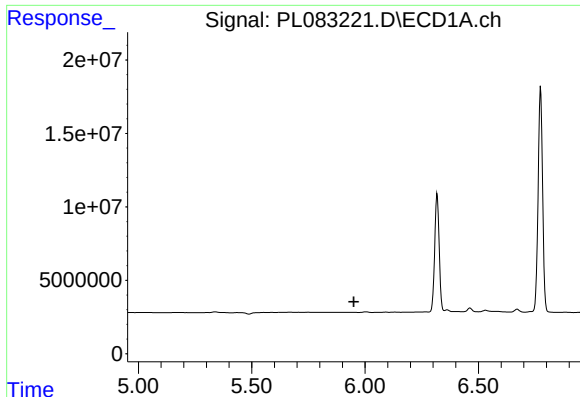

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 5.951 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

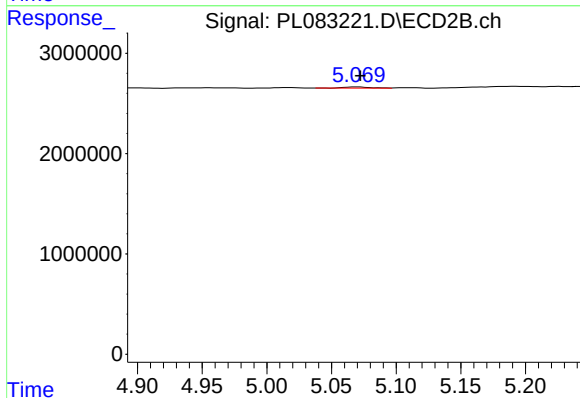


#12 4,4'-DDE

R.T.: 5.070 min
Delta R.T.: -0.002 min
Response: 153800
Conc: 0.06 ng/ml

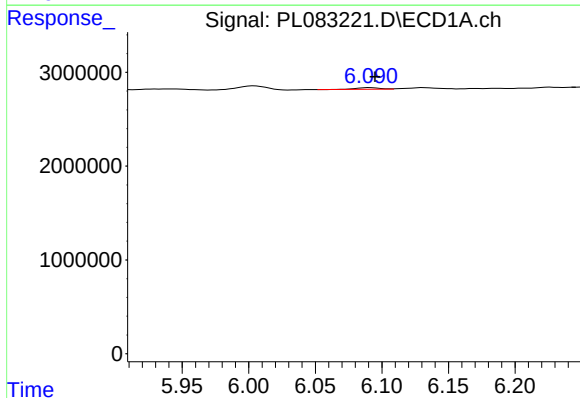


#13 Dieldrin

R.T.: 6.091 min
Delta R.T.: -0.004 min
Response: 216858
Conc: 0.07 ng/ml

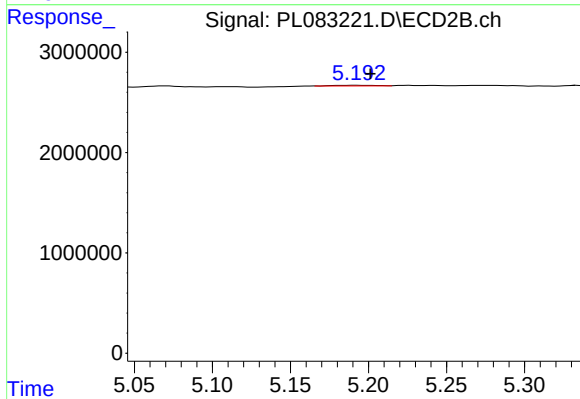

#13 Dieldrin


R.T.: 5.193 min
Delta R.T.: -0.008 min
Response: 116174
Conc: 0.04 ng/ml

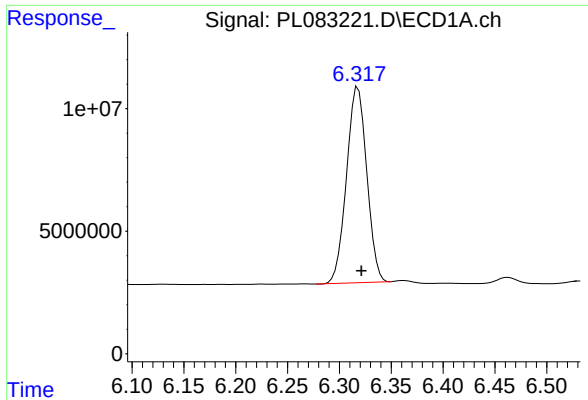

#14 Endrin


R.T.: 6.318 min
Delta R.T.: -0.003 min
Response: 108673918
Conc: 40.44 ng/ml

Instrument :
ECD_L
ClientSampleId :

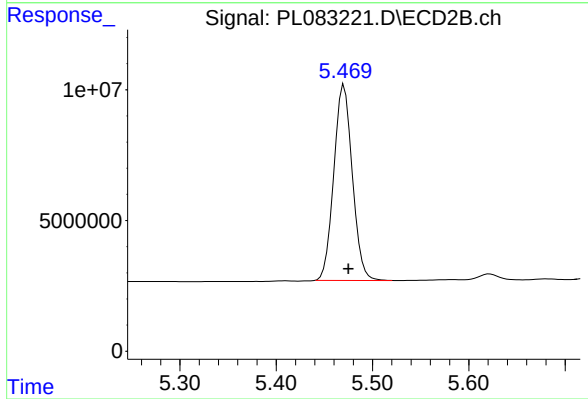


#14 Endrin

R.T.: 5.471 min
Delta R.T.: -0.004 min
Response: 99997748
Conc: 39.42 ng/ml

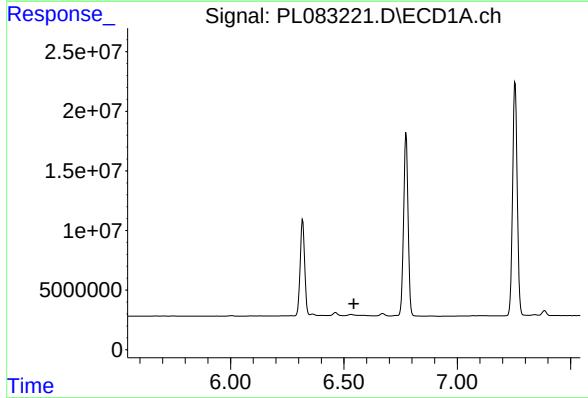


#15 Endosulfan II

R.T.: 6.532 min
Delta R.T.: -0.011 min
Response: 1595950
Conc: N.D.

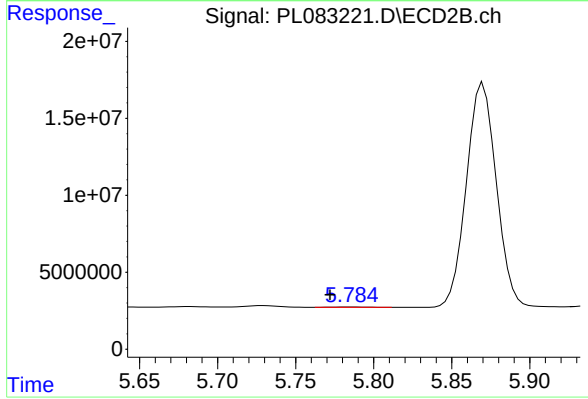

#15 Endosulfan II


R.T.: 5.785 min
Delta R.T.: 0.013 min
Response: 253845
Conc: 0.10 ng/ml

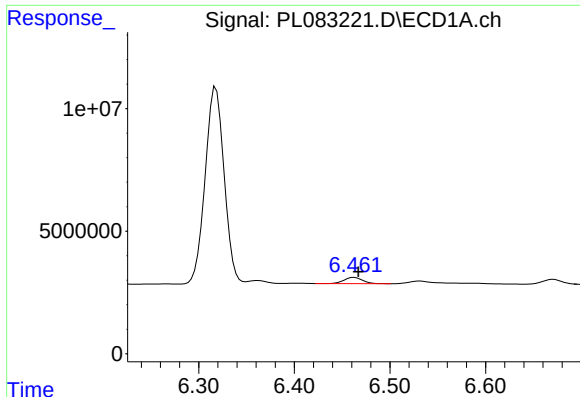

#16 4,4'-DDD


R.T.: 6.463 min
Delta R.T.: -0.004 min
Response: 3413631
Conc: 1.57 ng/ml

Instrument :
ECD_L
ClientSampleId :

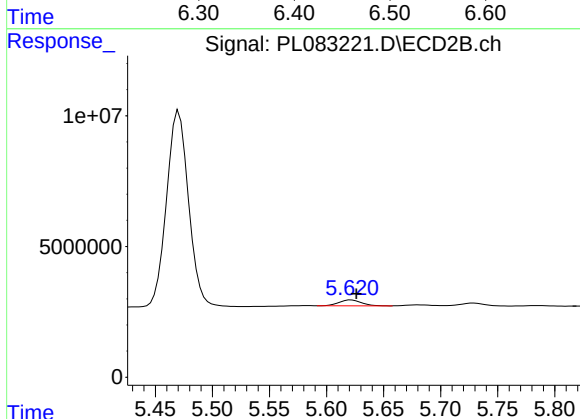


#16 4,4'-DDD

R.T.: 5.622 min
Delta R.T.: -0.005 min
Response: 3000216
Conc: 1.56 ng/ml

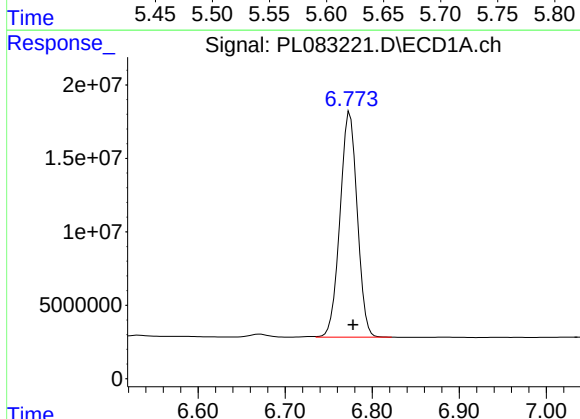


#17 4,4'-DDT

R.T.: 6.774 min
Delta R.T.: -0.004 min
Response: 210876488
Conc: 84.24 ng/ml

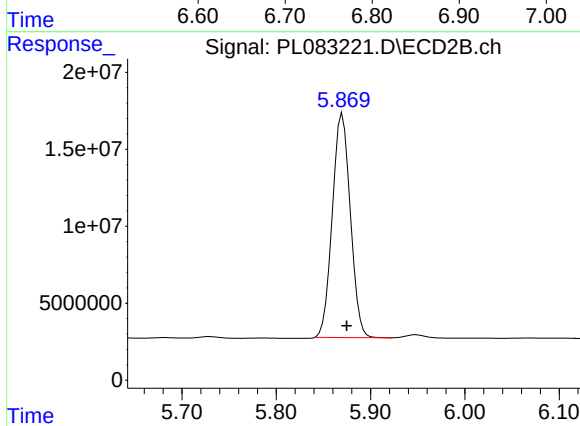

#17 4,4'-DDT


R.T.: 5.870 min
Delta R.T.: -0.005 min
Response: 192949653
Conc: 86.48 ng/ml

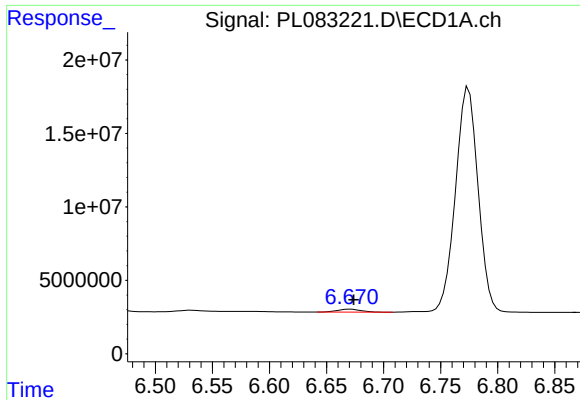

#18 Endrin aldehyde


R.T.: 6.671 min
Delta R.T.: -0.003 min
Response: 2860882
Conc: 1.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

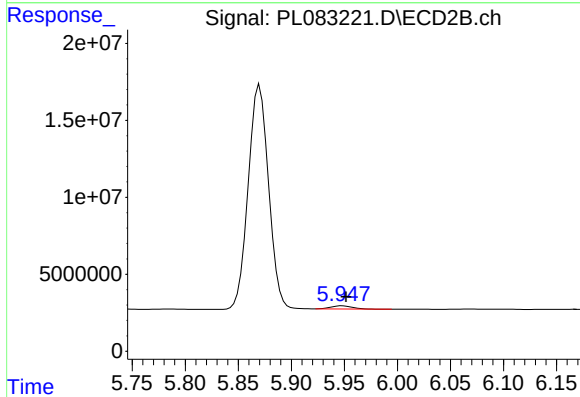


#18 Endrin aldehyde

R.T.: 5.948 min
Delta R.T.: -0.003 min
Response: 2867920
Conc: 1.45 ng/ml

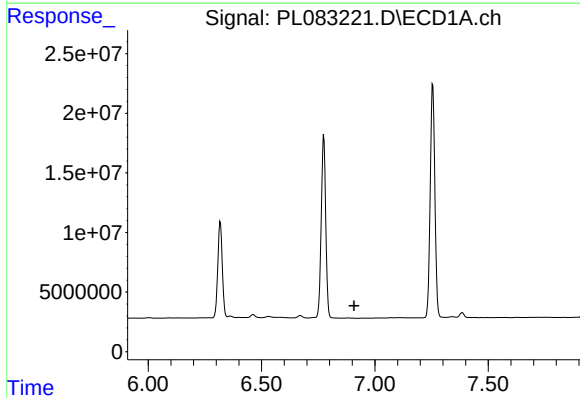


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 6.908 min
Response: 0
Conc: N.D.

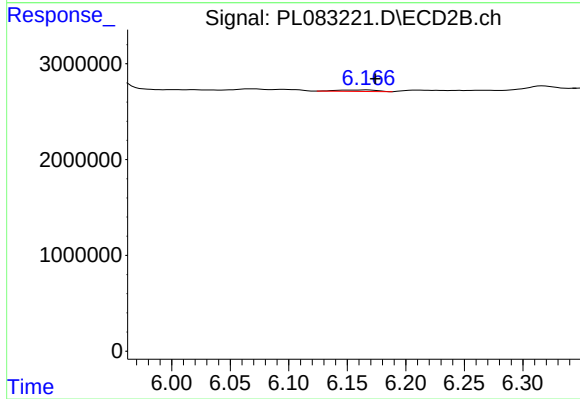

#19 Endosulfan Sulfate


R.T.: 6.167 min
Delta R.T.: -0.007 min
Response: 338539
Conc: 0.14 ng/ml

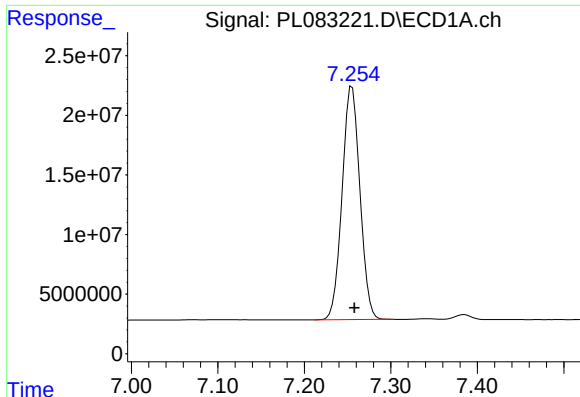

#20 Methoxychlor


R.T.: 7.255 min
Delta R.T.: -0.003 min
Response: 278157904
Conc: 210.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

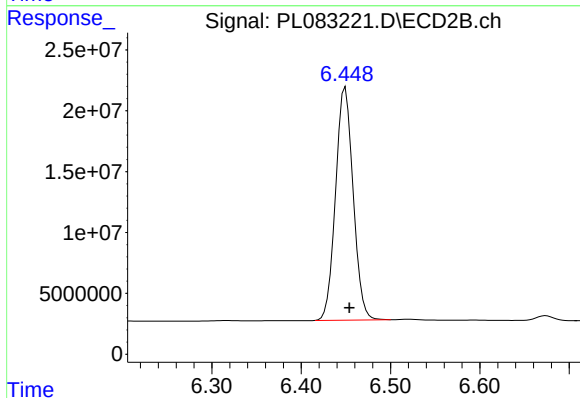


#20 Methoxychlor

R.T.: 6.449 min
Delta R.T.: -0.004 min
Response: 261821165
Conc: 205.88 ng/ml

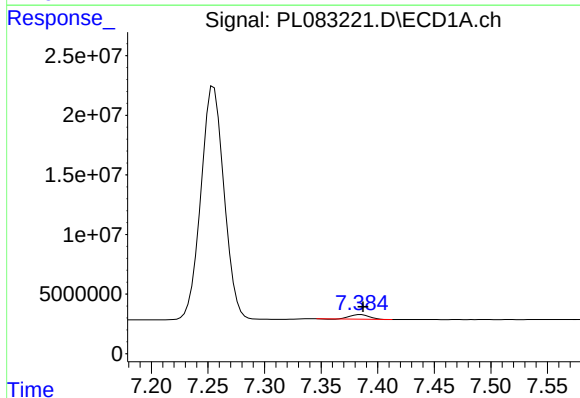


#21 Endrin ketone

R.T.: 7.385 min
Delta R.T.: -0.002 min
Response: 4600030
Conc: 1.80 ng/ml

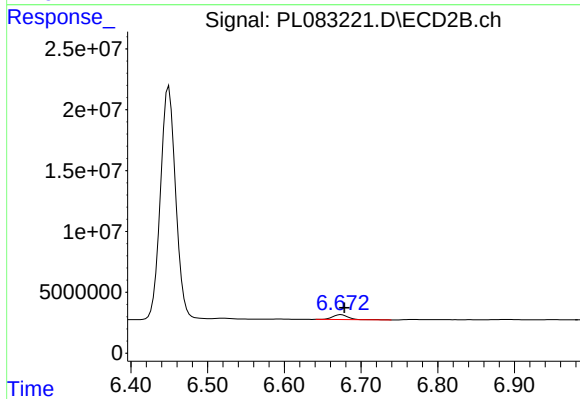

#21 Endrin ketone


R.T.: 6.674 min
Delta R.T.: -0.004 min
Response: 5711085
Conc: 2.11 ng/ml

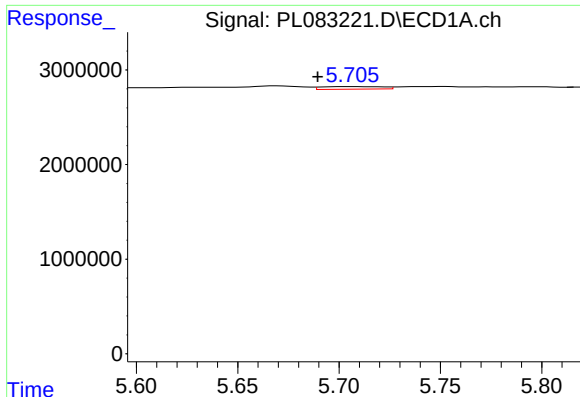

#25 Chlordane-3


R.T.: 5.706 min
Delta R.T.: 0.017 min
Response: 576032
Conc: 1.39 ng/ml

Instrument :
ECD_L
ClientSampleId :

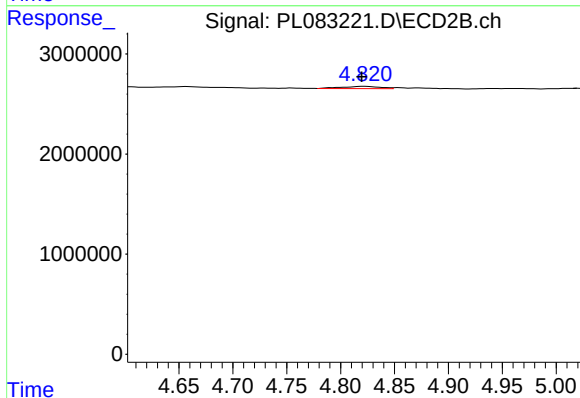


#25 Chlordane-3

R.T.: 4.822 min
Delta R.T.: 0.002 min
Response: 550963
Conc: 2.07 ng/ml

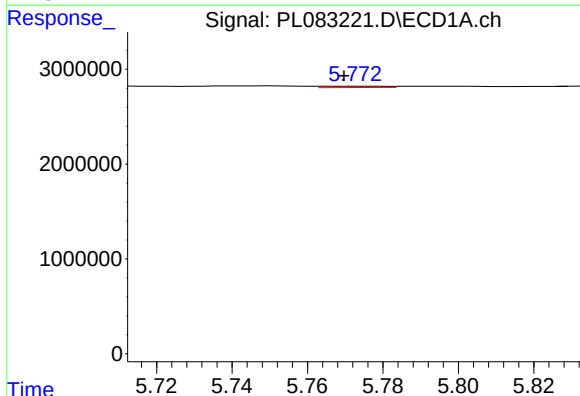


#26 Chlordane-4

R.T.: 5.773 min
Delta R.T.: 0.003 min
Response: 162618
Conc: 0.32 ng/ml

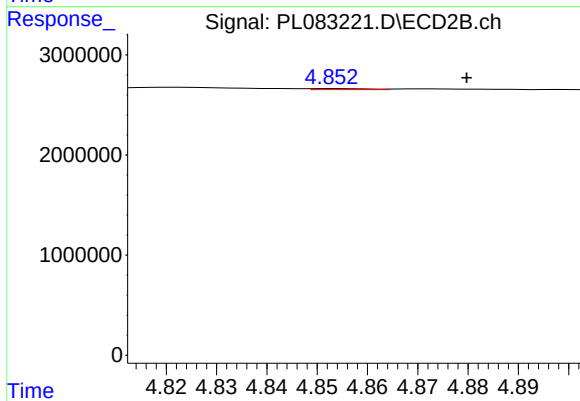

#26 Chlordane-4


R.T.: 4.853 min
Delta R.T.: -0.026 min
Response: 84916
Conc: 0.30 ng/ml

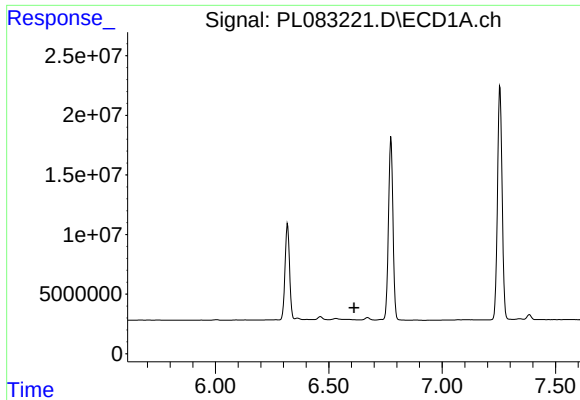

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.612 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

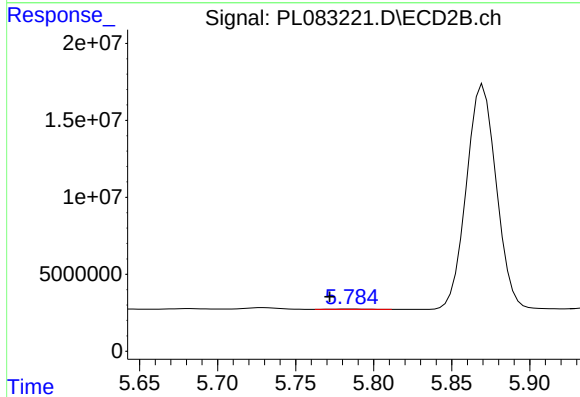


#27 Chlordane-5

R.T.: 5.785 min
Delta R.T.: 0.013 min
Response: 253845
Conc: 2.61 ng/ml

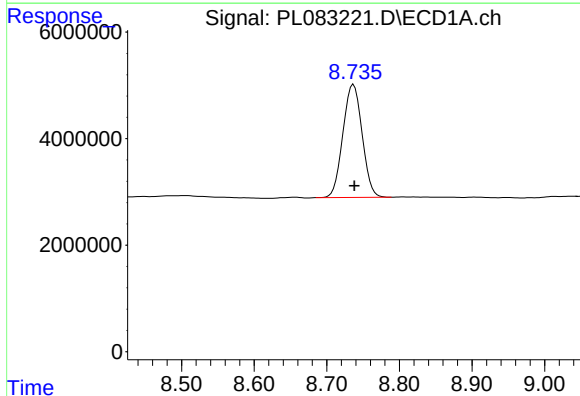

#28 Decachlorobiphenyl

R.T.: 8.737 min
Delta R.T.: -0.001 min
Response: 39075350
Conc: 18.63 ng/ml

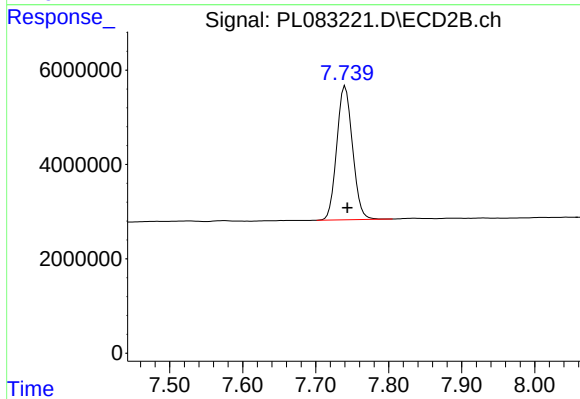

#28 Decachlorobiphenyl

R.T.: 7.740 min
Delta R.T.: -0.003 min
Response: 42522370
Conc: 17.10 ng/ml