

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060525\
 Data File : PL095936.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jun 2025 09:58
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 06 00:48:59 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052125.M
 Quant Title : GC Extractables
 QLast Update : Thu May 22 06:29:30 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
8) B	Heptachlo...	5.714	0.000	6272607	0	1.643	N.D. #
10) B	gamma-Chl...	5.957f	0.000	5637058	0	1.448	N.D. #
13) MA	Dieldrin	0.000	5.522f	0	9702145	N.D.	1.831 #
14) MA	Endrin	0.000	5.783	0	10110607	N.D.	2.074 #
16) A	4,4'-DDD	6.752	0.000	12121320	0	4.136	N.D. #
25)	Chlordane-3	5.957	0.000	5637058	0	7.628	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060525\
Data File : PL095936.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jun 2025 09:58
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 06 00:48:59 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052125.M
Quant Title : GC Extractables
QLast Update : Thu May 22 06:29:30 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

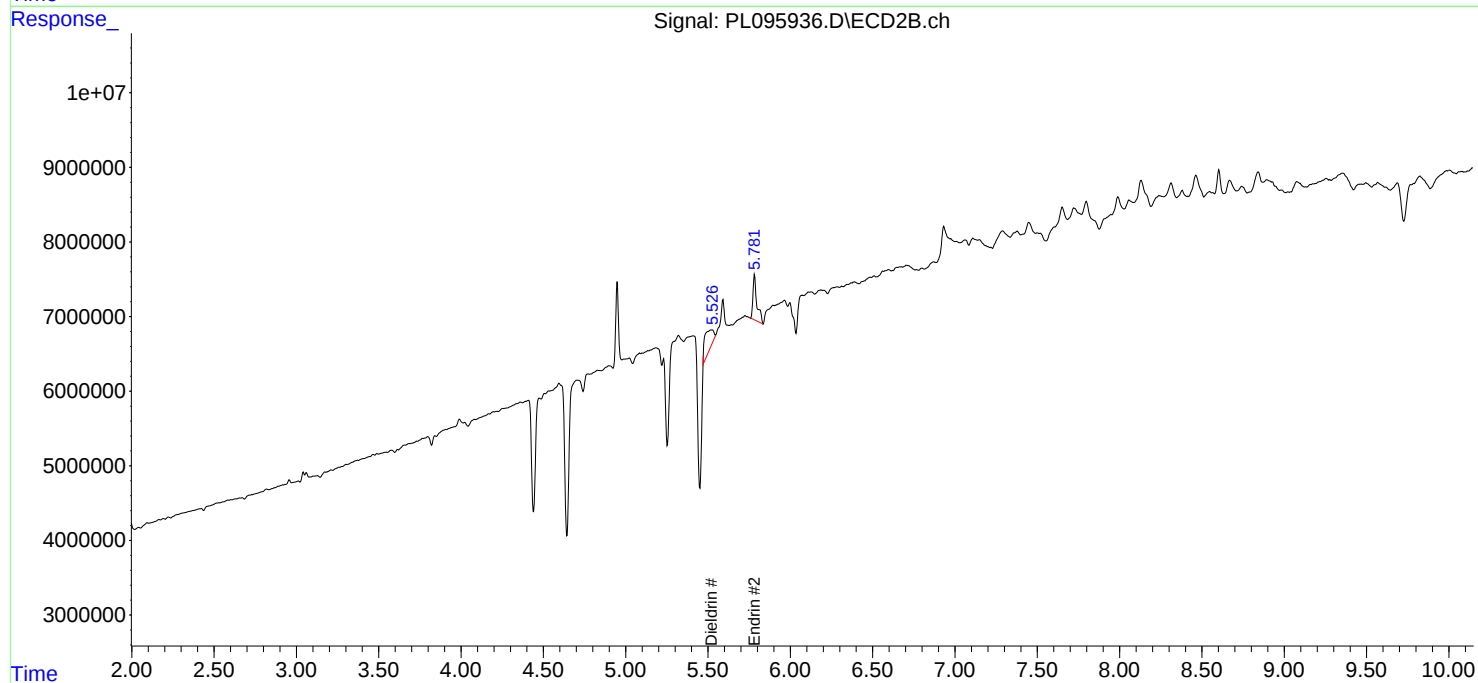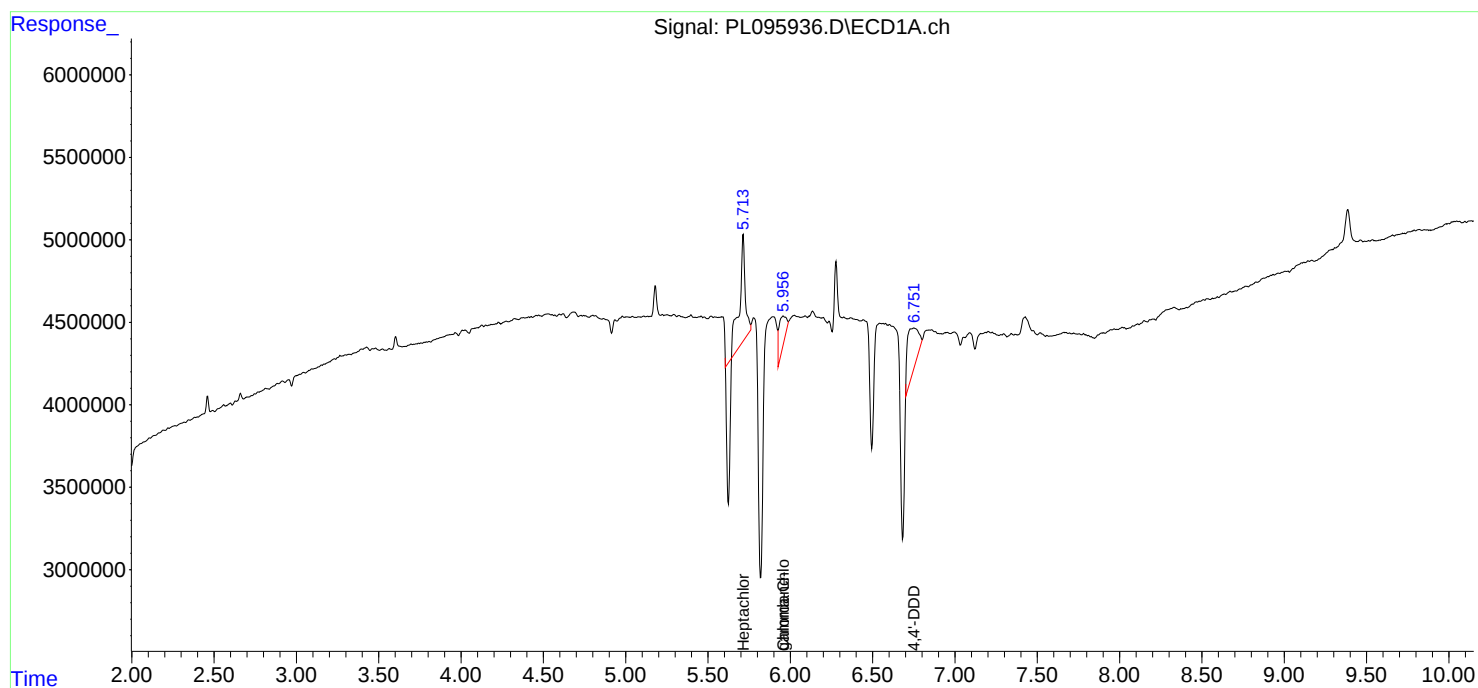


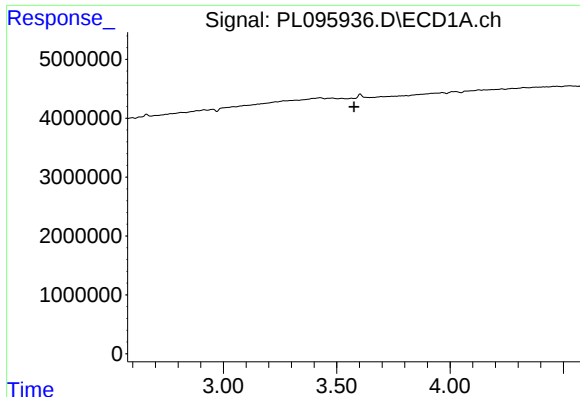

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.577 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

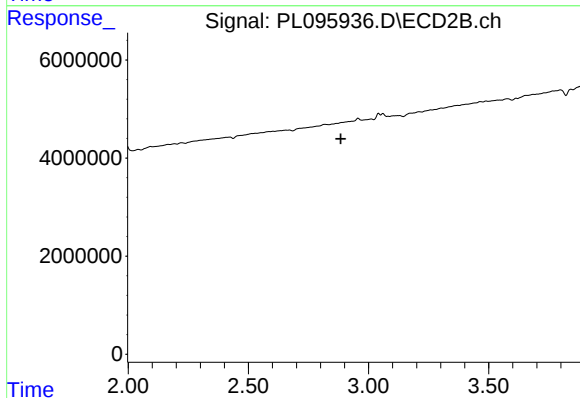


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 2.883 min
Response: 0
Conc: N.D.

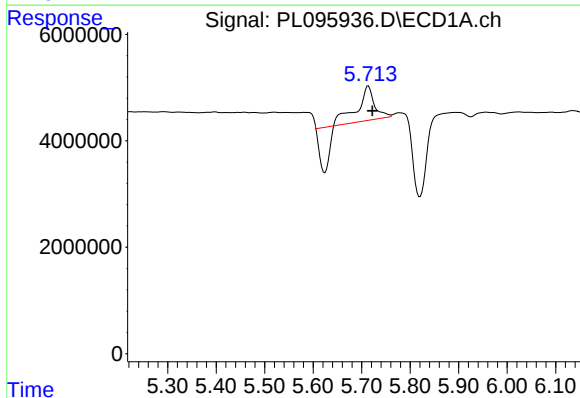


#8 Heptachlor epoxide

R.T.: 5.714 min
Delta R.T.: -0.008 min
Response: 6272607
Conc: 1.64 ng/ml

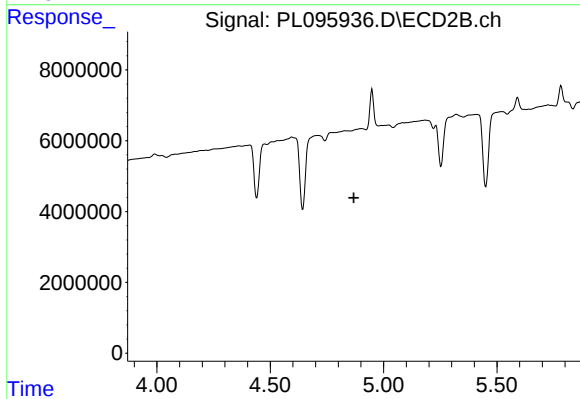

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.869 min
Response: 0
Conc: N.D.

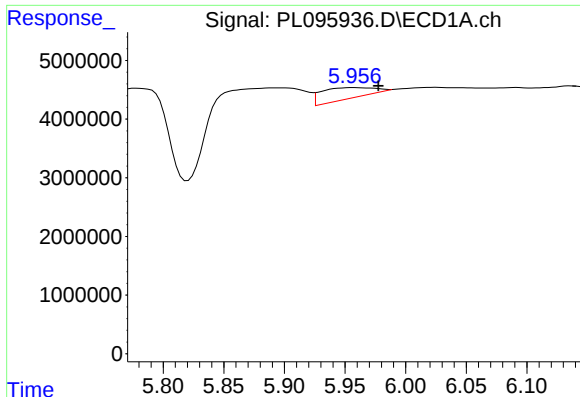

#10 gamma-Chlordane


R.T.: 5.957 min
Delta R.T.: -0.021 min
Response: 5637058
Conc: 1.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

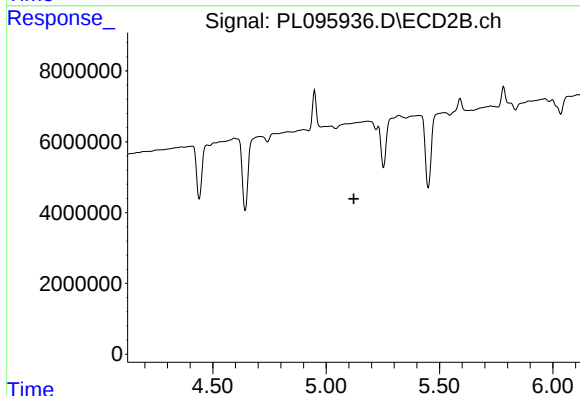


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.122 min
Response: 0
Conc: N.D.

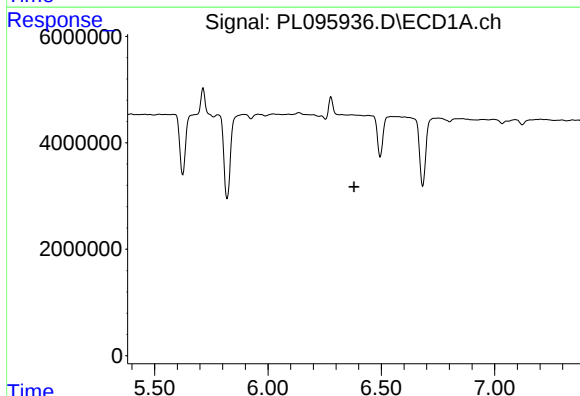


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.379 min
Response: 0
Conc: N.D.

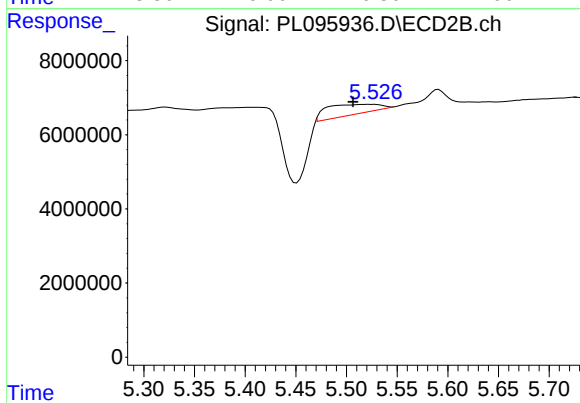

#13 Dieldrin


R.T.: 5.522 min
Delta R.T.: 0.015 min
Response: 9702145
Conc: 1.83 ng/ml

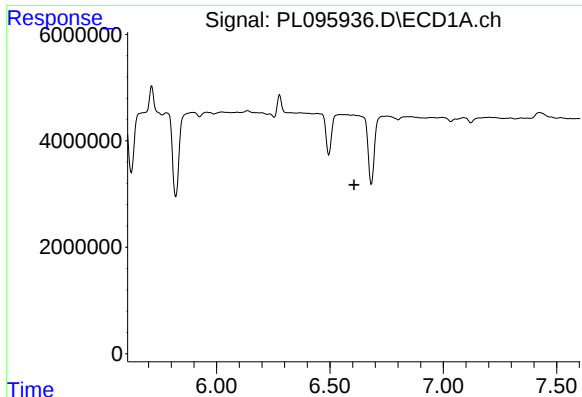

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.607 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

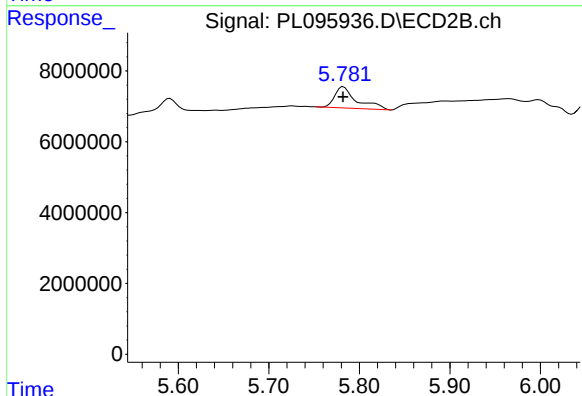


#14 Endrin

R.T.: 5.783 min
Delta R.T.: 0.000 min
Response: 10110607
Conc: 2.07 ng/ml

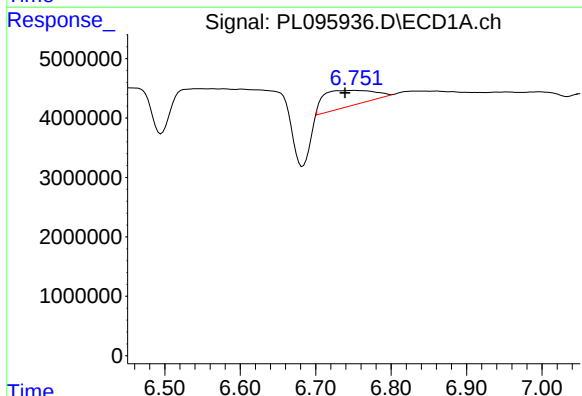


#16 4,4'-DDD

R.T.: 6.752 min
Delta R.T.: 0.013 min
Response: 12121320
Conc: 4.14 ng/ml

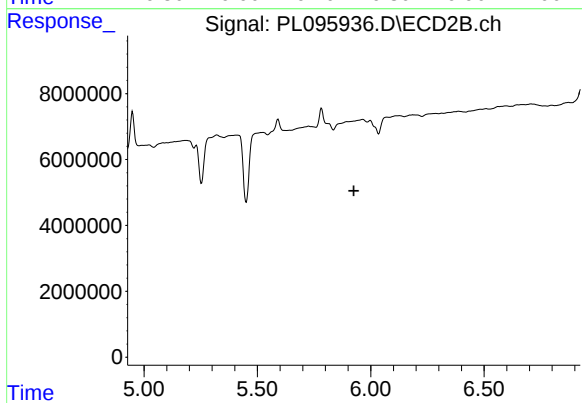

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.926 min
Response: 0
Conc: N.D.

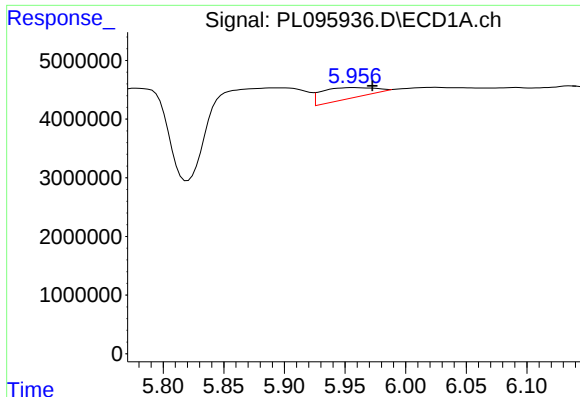

#25 Chlordane-3


R.T.: 5.957 min
Delta R.T.: -0.016 min
Response: 5637058
Conc: 7.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

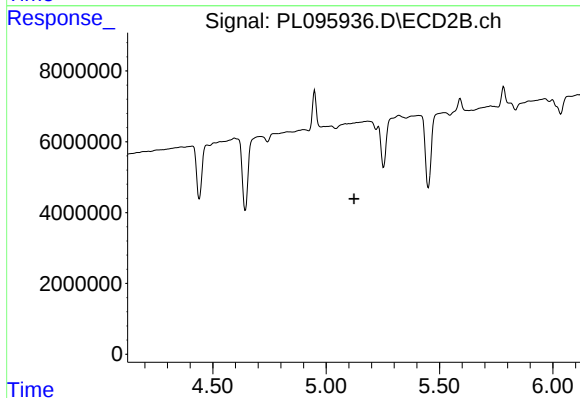


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.123 min
Response: 0
Conc: N.D.

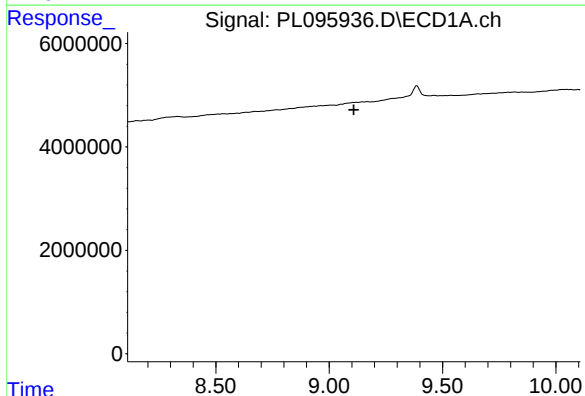

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.109 min
Response: 0
Conc: N.D.

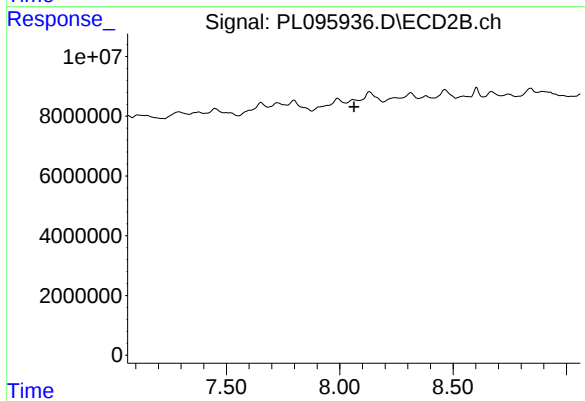

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.064 min
Response: 0
Conc: N.D.