

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060525\
 Data File : PL095955.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jun 2025 16:23
 Operator : AR\AJ
 Sample : Q2208-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BU-703-COMP-06

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 06/06/2025
 Supervised By :mohammad ahmed 06/09/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 06 00:51:29 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052125.M
 Quant Title : GC Extractables
 QLast Update : Thu May 22 06:29:30 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.570	2.885	63820613	81759094	20.227m	20.889
28) SA Decachlor...	9.098	8.059	38780708	73971568	16.458	16.910

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060525\
Data File : PL095955.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jun 2025 16:23
Operator : AR\AJ
Sample : Q2208-01
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
BU-703-COMP-06


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 06/06/2025
Supervised By : mohammad ahmed 06/09/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 06 00:51:29 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052125.M
Quant Title : GC Extractables
QLast Update : Thu May 22 06:29:30 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

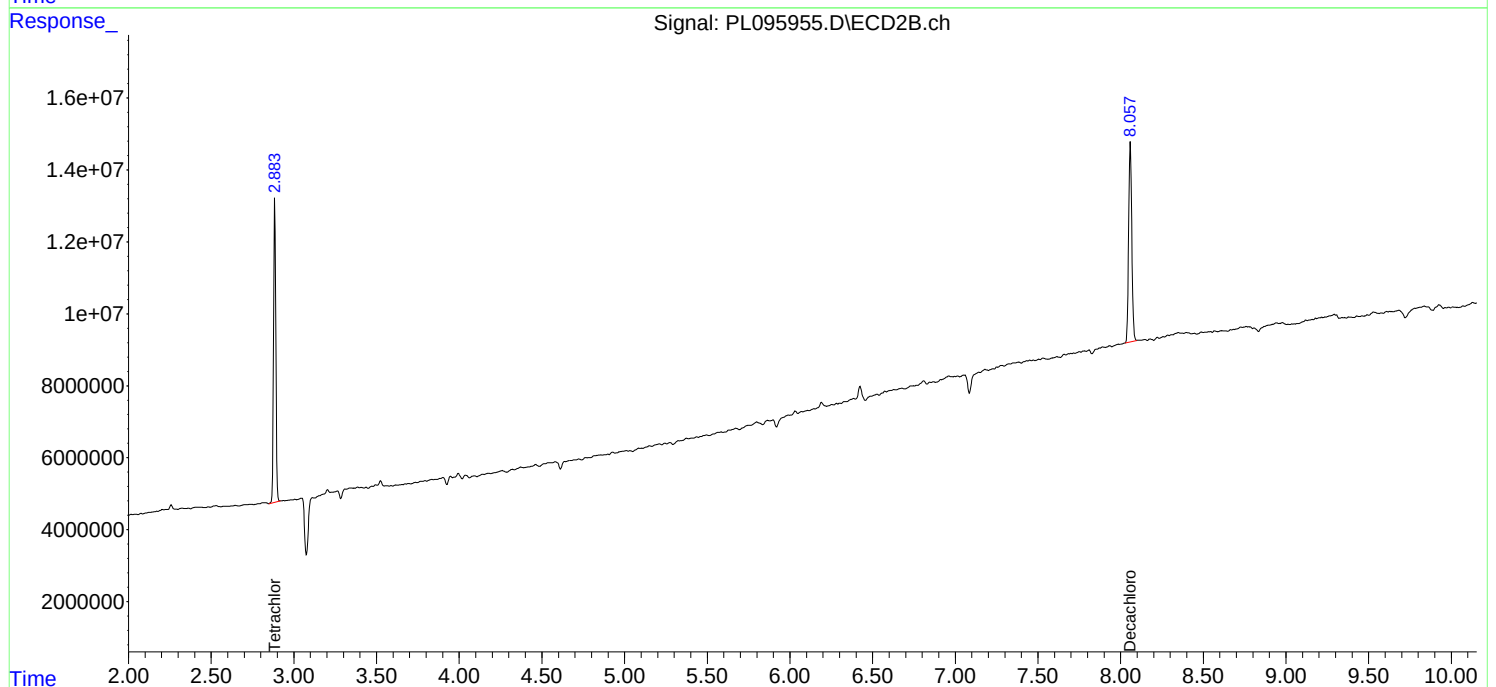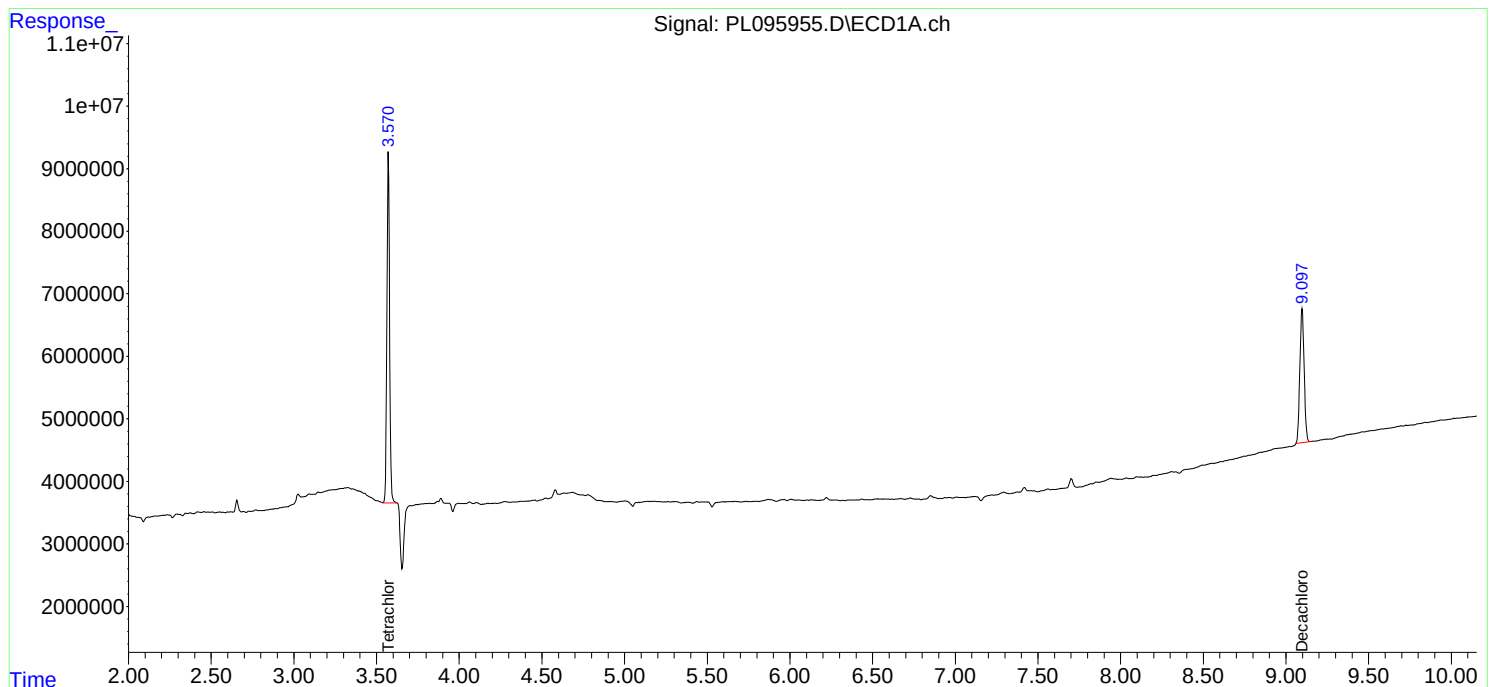

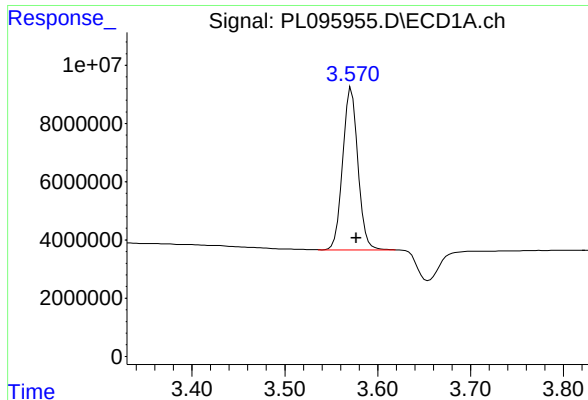


#1 Tetrachloro-m-xylene

R.T.: 3.570 min
Delta R.T.: -0.007 min
Response: 63820613
Conc: 20.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
BU-703-COMP-06


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/06/2025
Supervised By :mohammad ahmed 06/09/2025

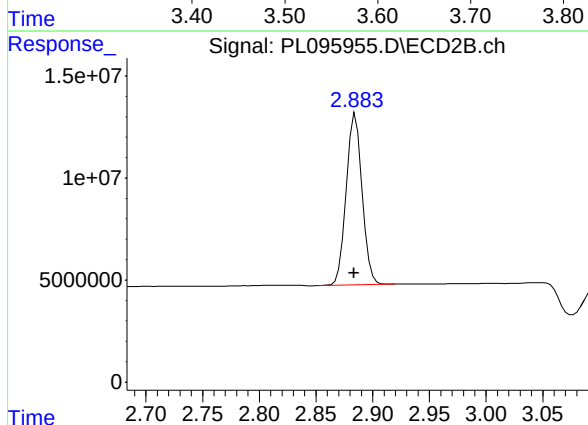


#1 Tetrachloro-m-xylene

R.T.: 2.885 min
Delta R.T.: 0.001 min
Response: 81759094
Conc: 20.89 ng/ml

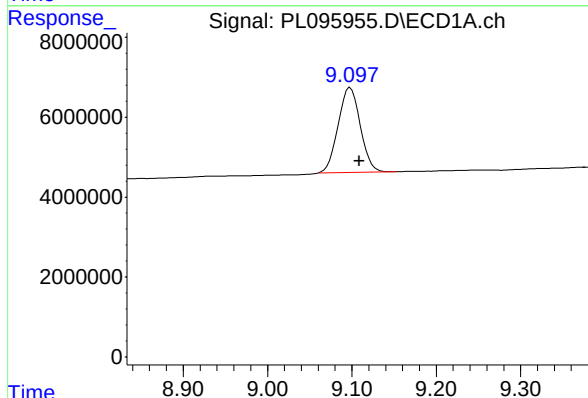

#28 Decachlorobiphenyl

R.T.: 9.098 min
Delta R.T.: -0.011 min
Response: 38780708
Conc: 16.46 ng/ml

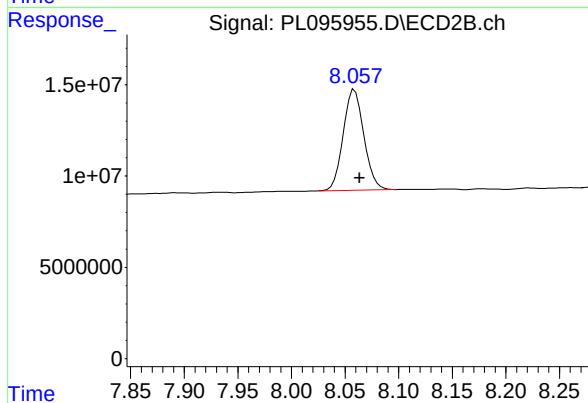

#28 Decachlorobiphenyl

R.T.: 8.059 min
Delta R.T.: -0.005 min
Response: 73971568
Conc: 16.91 ng/ml