

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060621\
 Data File : PL067125.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jun 2021 21:32
 Operator : AR\AJ
 Sample : M2250-02
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MDL-WATER-QT3-2021-06

Manual Integrations
 APPROVED

Ankita
 6/7/2021 4:19:40 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 07:24:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060521CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 07 05:11:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	4.014	4.899	10332643	18054539	19.830	20.526
27)	SA Decachlor...	9.232	10.434	25283667	36352050	39.999	40.005
Target Compounds							
2)	A alpha-BHC	4.583	5.387	974920	990428	1.226m	0.886 #
3)	MA gamma-BHC...	4.926	5.731	894486	979574	1.248	0.903 #
4)	MA Heptachlor	5.278	6.312	750783	1092396	1.089	0.996
5)	MB Aldrin	5.559	6.652	673058	935207	1.035	0.994
6)	B beta-BHC	5.238	5.947	465572	1973190	1.298m	2.737m#
7)	B delta-BHC	5.465	6.190	746213	853784	1.111m	0.946
8)	B Heptachlo...	6.063	7.083	701970	863555	1.113	1.029
9)	A Endosulfan I	6.429	7.467	675382	896819	1.097	1.080
10)	B trans-Chl...	6.315	7.336	686444	958552	1.048	1.060
11)	B cis-Chlor...	6.378	7.413	780980	964199	1.184	1.080
12)	B 4,4'-DDE	6.570	7.585	629181	782799	1.037	0.924
13)	MA Dieldrin	6.691	7.743	669138	840401	1.005m	0.939
14)	MA Endrin	6.961	7.974	623901	630301	1.029m	0.876
15)	B Endosulfa...	7.253	8.199	602036	908929	1.085	1.237
16)	A 4,4'-DDD	7.115	8.104	556430	691360	1.054m	1.006m
17)	MA 4,4'-DDT	7.365	8.415	410197	594697	0.761	0.854
18)	B Endrin al...	7.431	8.328	567185	674953	1.156	1.024
19)	B Endosulfa...	7.652	8.559	660427	794437	1.183	1.080
20)	A Methoxychlor	7.935	8.888	320373	370567	1.026	0.921
21)	B Endrin ke...	8.148	9.048	718432	889797	1.103	1.066

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060621\
Data File : PL067125.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jun 2021 21:32
Operator : AR\AJ
Sample : M2250-02
Misc :
ALS Vial : 34 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 07:24:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060521CLP.M
Quant Title : GC Extractables
QLast Update : Mon Jun 07 05:11:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

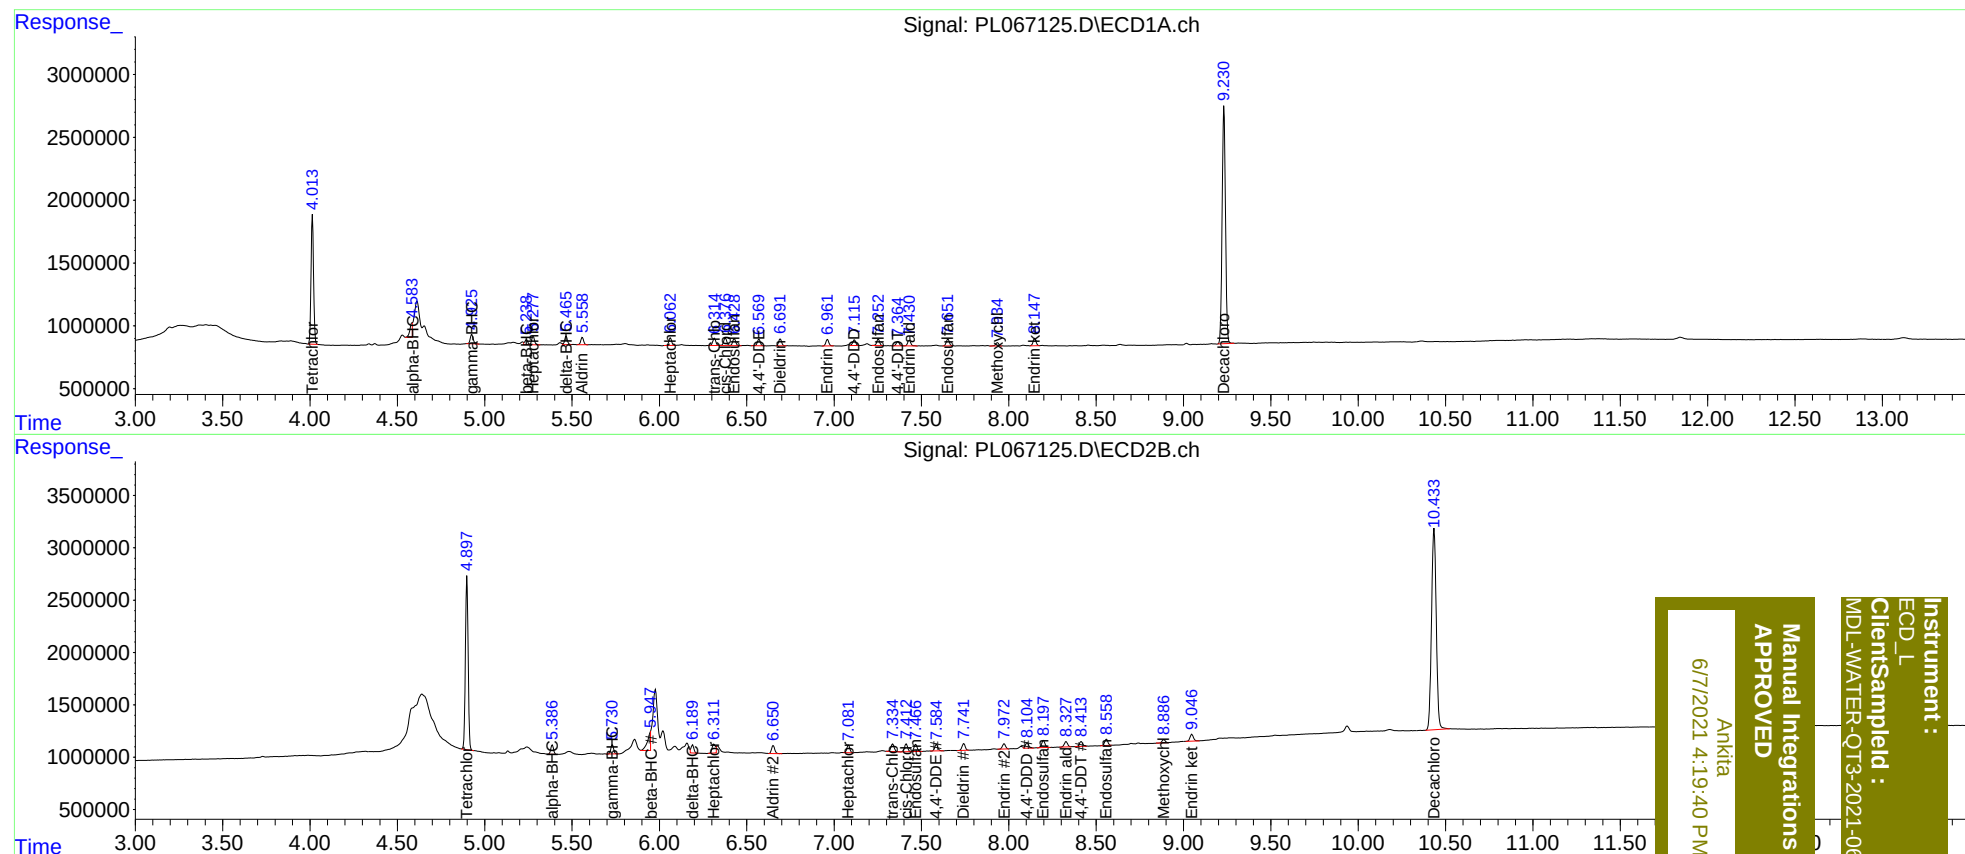

Manual Integrations
APPROVED

Ankita

6/7/2021 4:19:40 PM

Instrument :
ECD_L
Client Sampled :
MDL-WATER-QT3-2021-06