

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060623\
 Data File : PL083242.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jun 2023 13:49
 Operator : AR\AJ
 Sample : 03028-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OR-02-060223

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/07/2023
 Supervised By : Ankita Jodhani 06/07/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 06 20:52:04 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051923.M
 Quant Title : GC Extractables
 QLast Update : Sat May 20 04:58:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.316	2.633	37027713	32708574	12.599	12.599
28)	SA Decachlor...	8.739	7.742	32519152	35887565	15.505	14.433
Target Compounds							
11)	B alpha-Chl...	5.771	4.873	2515908	1090492	0.784m	0.363m#
12)	B 4,4'-DDE	5.949	5.066	1191701	1213261	0.432	0.500m
17)	MA 4,4'-DDT	6.775	5.869	1215941	1589710	0.486	0.713 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060623\
Data File : PL083242.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jun 2023 13:49
Operator : AR\AJ
Sample : 03028-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
OR-02-060223


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 06/07/2023
Supervised By : Ankita Jodhani 06/07/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 06 20:52:04 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051923.M
Quant Title : GC Extractables
QLast Update : Sat May 20 04:58:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

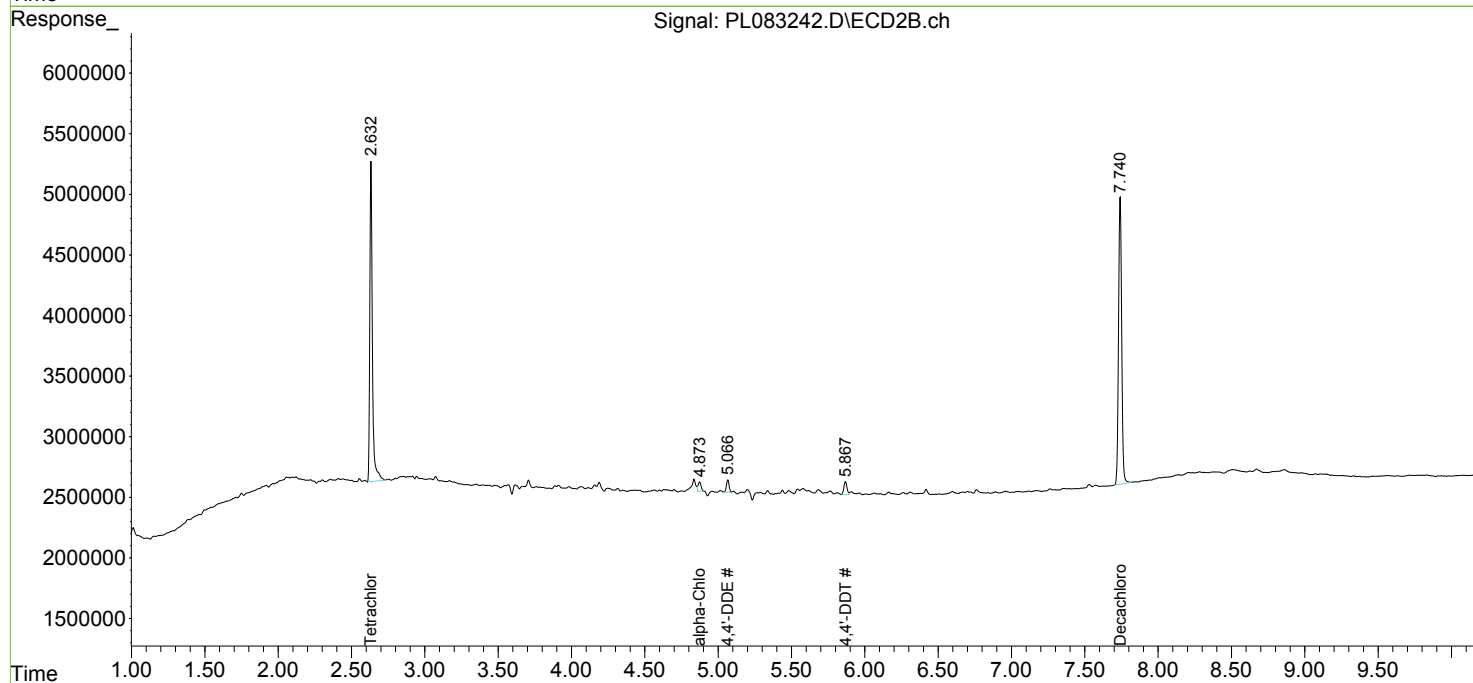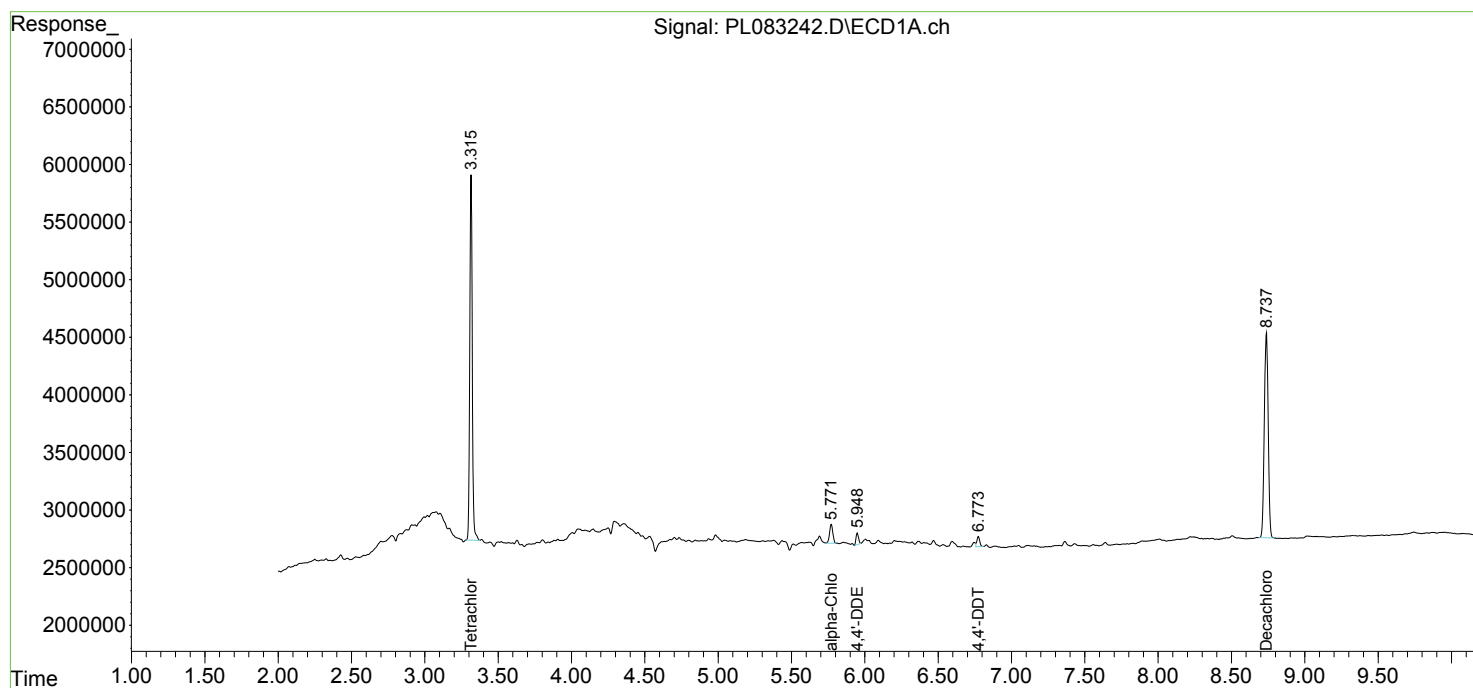

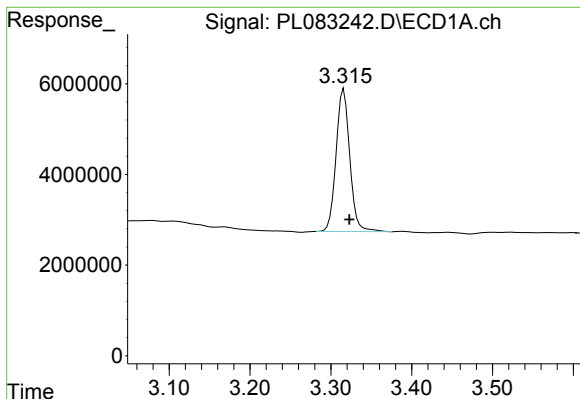


#1 Tetrachloro-m-xylene

R.T.: 3.316 min
Delta R.T.: -0.007 min
Response: 37027713
Conc: 12.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-02-060223


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/07/2023
Supervised By :Ankita Jodhani 06/07/2023

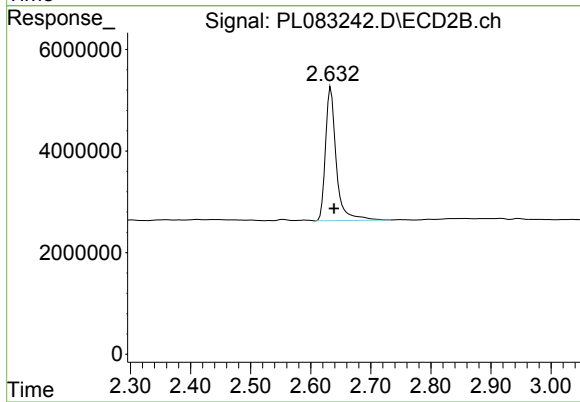


#1 Tetrachloro-m-xylene

R.T.: 2.633 min
Delta R.T.: -0.006 min
Response: 32708574
Conc: 12.60 ng/ml

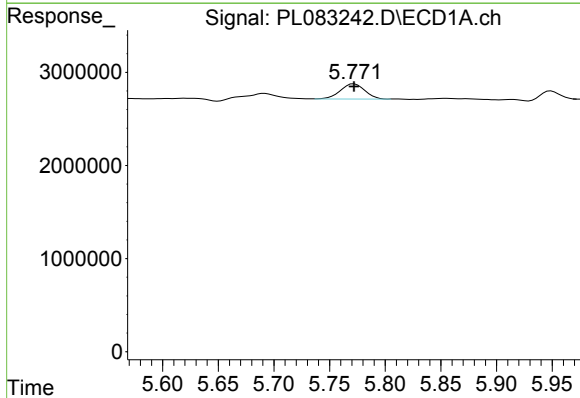


#11 alpha-Chlordane

R.T.: 5.771 min
Delta R.T.: -0.001 min
Response: 2515908
Conc: 0.78 ng/ml m

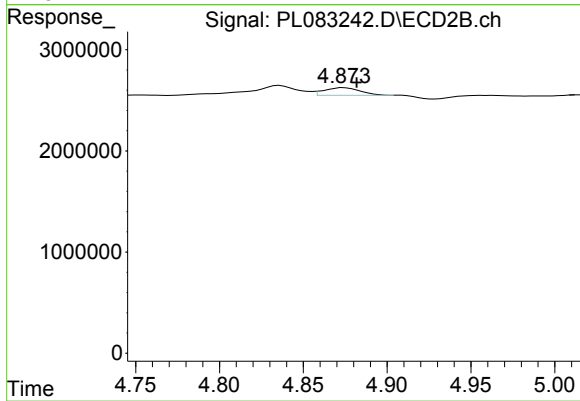

#11 alpha-Chlordane

R.T.: 4.873 min
Delta R.T.: -0.009 min
Response: 1090492
Conc: 0.36 ng/ml m

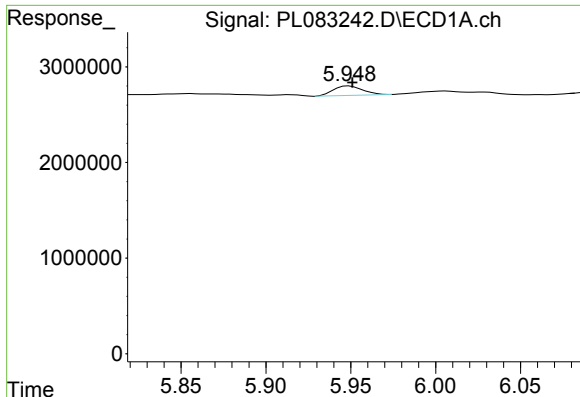


#12 4,4'-DDE

R.T.: 5.949 min
Delta R.T.: -0.002 min
Response: 1191701
Conc: 0.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-02-060223


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/07/2023
Supervised By :Ankita Jodhani 06/07/2023

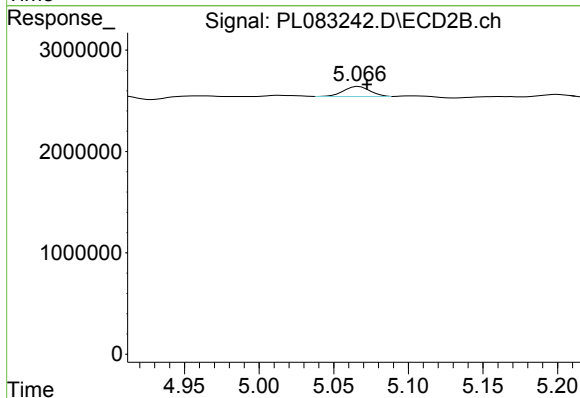


#12 4,4'-DDE

R.T.: 5.066 min
Delta R.T.: -0.007 min
Response: 1213261
Conc: 0.50 ng/ml m

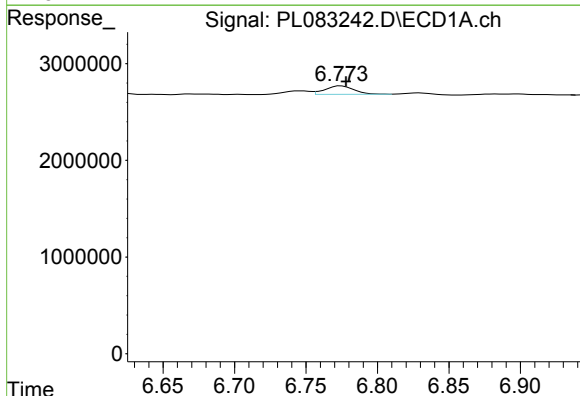


#17 4,4'-DDT

R.T.: 6.775 min
Delta R.T.: -0.003 min
Response: 1215941
Conc: 0.49 ng/ml

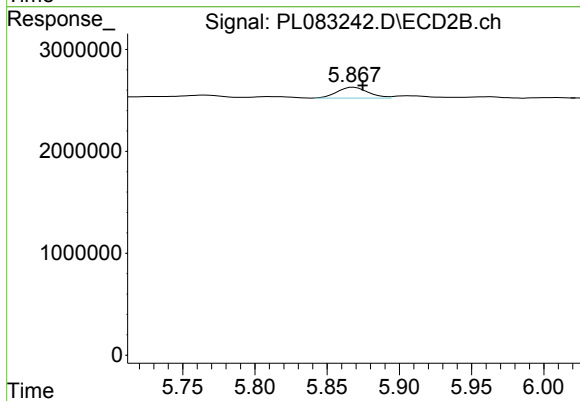

#17 4,4'-DDT

R.T.: 5.869 min
Delta R.T.: -0.006 min
Response: 1589710
Conc: 0.71 ng/ml

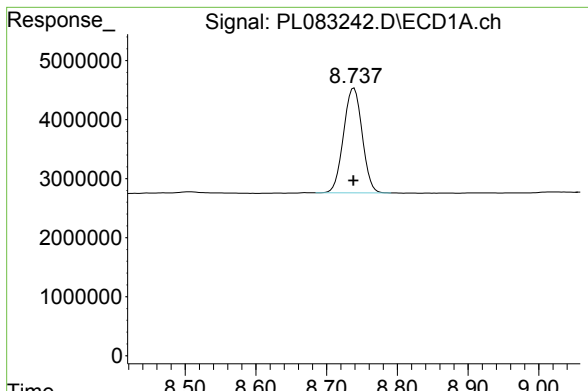


#28 Decachlorobiphenyl

R.T.: 8.739 min
Delta R.T.: 0.000 min
Response: 32519152
Conc: 15.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-02-060223

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/07/2023
Supervised By :Ankita Jodhani 06/07/2023

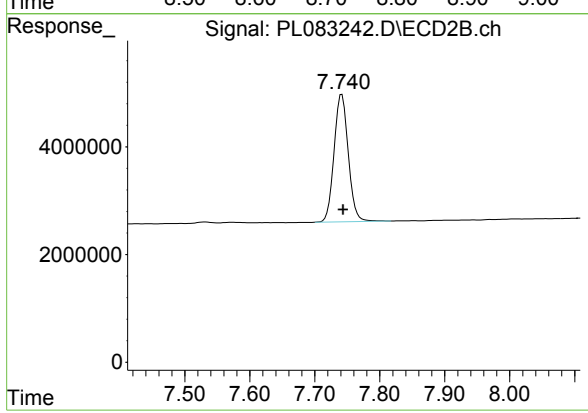

#28 Decachlorobiphenyl

R.T.: 7.742 min
Delta R.T.: -0.002 min
Response: 35887565
Conc: 14.43 ng/ml